

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052822\
 Data File : PL075172.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 May 2022 16:34
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 30 03:00:31 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
 Quant Title : GC Extractables
 QLast Update : Mon May 30 03:00:24 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.651	4.644	64575978	205.8E6	99.509	100.159
28)	SA Decachlor...	11.649	10.395	50865229	132.6E6	93.458	95.831
Target Compounds							
23)	Chlordane-1	7.044	5.967	22805164	54560787	989.447	978.266
24)	Chlordane-2	7.638	6.653	27235979	62769785	963.816	952.558
25)	Chlordane-3	8.399	7.353	92755941	175.8E6	971.654	981.562
26)	Chlordane-4	8.482	7.420	112.0E6	185.9E6	966.082	978.990
27)	Chlordane-5	9.375	8.133	20105822	45795478	959.653	941.198



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052822\
Data File : PL075172.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 May 2022 16:34
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 30 03:00:31 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
Quant Title : GC Extractables
QLast Update : Mon May 30 03:00:24 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

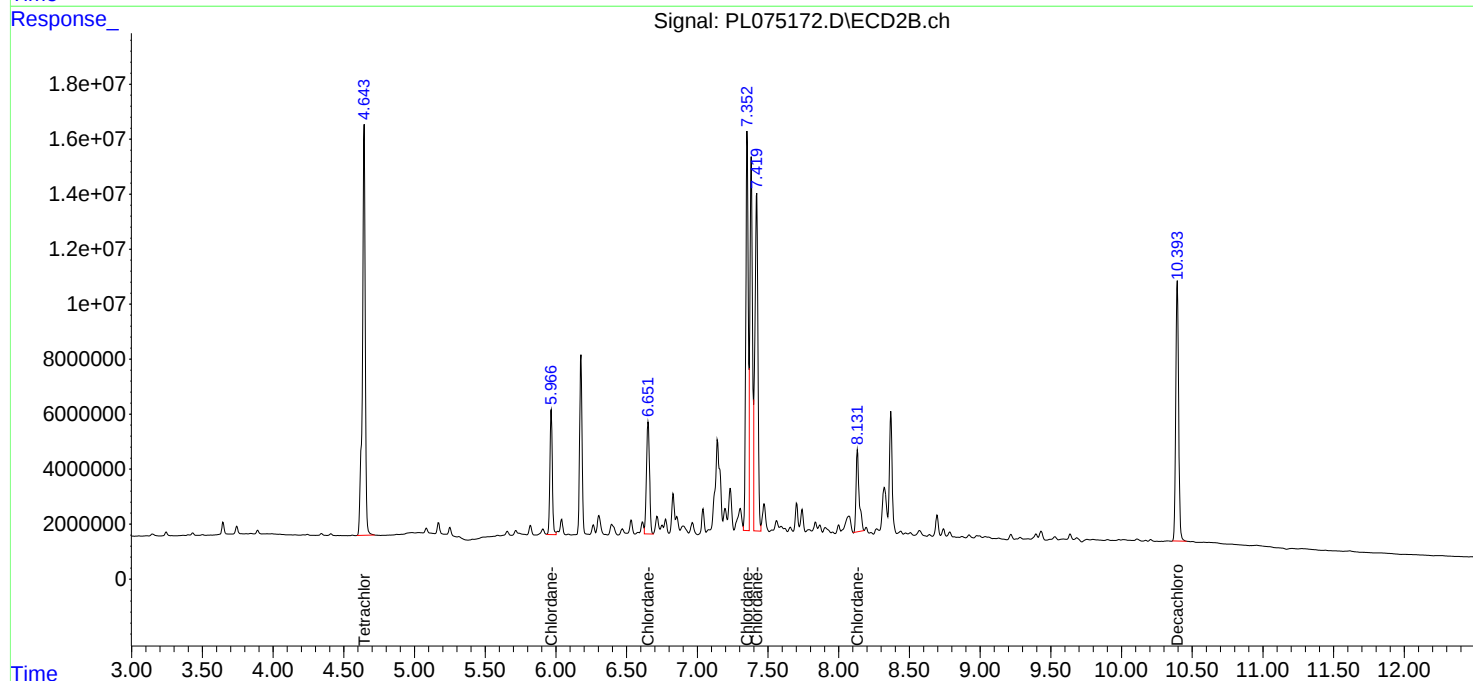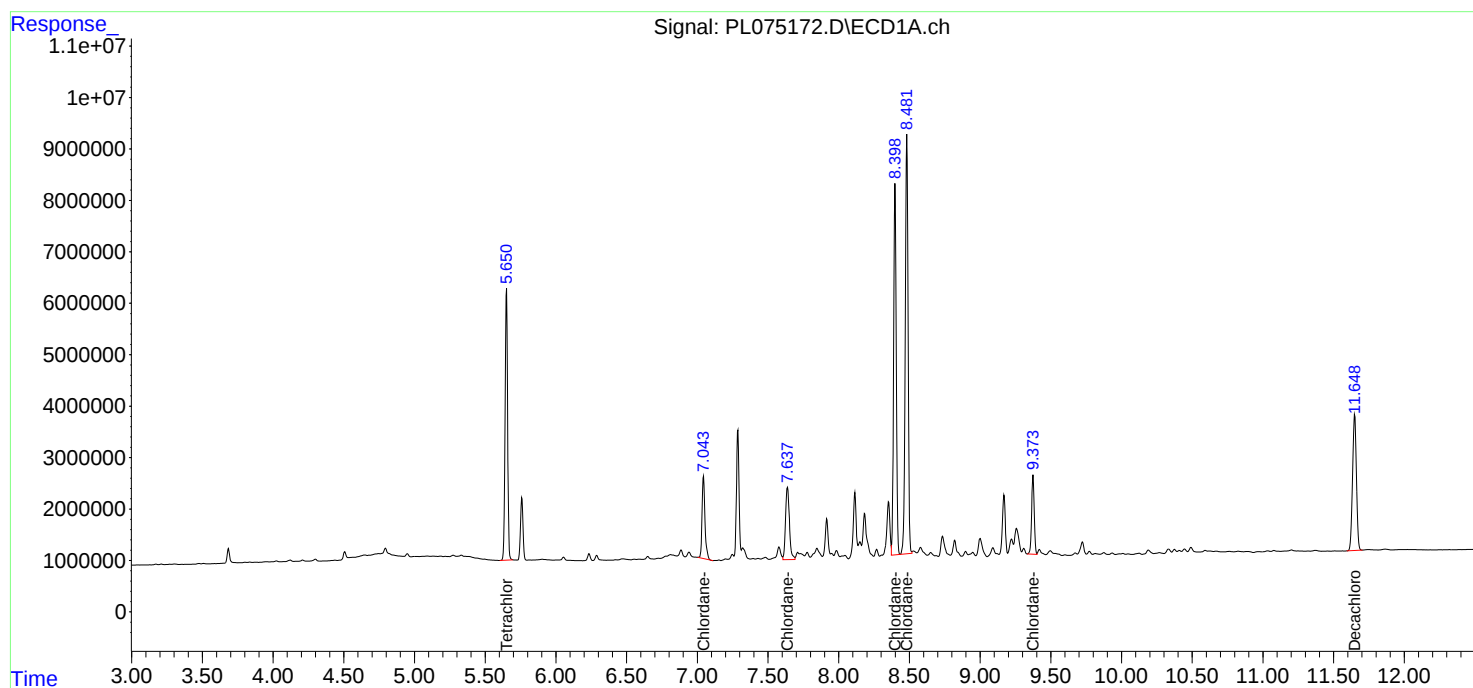


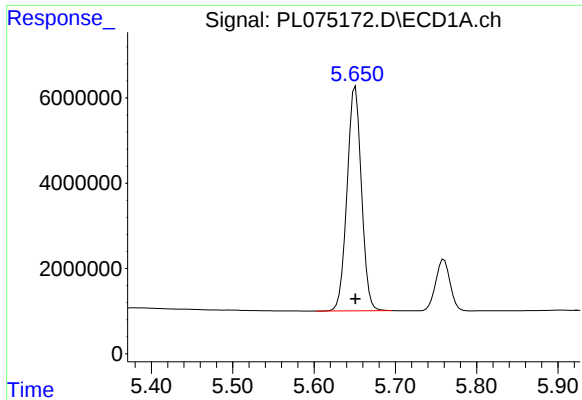

#1 Tetrachloro-m-xylene


R.T.: 5.651 min
Delta R.T.: 0.000 min
Response: 64575978
Conc: 99.51 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

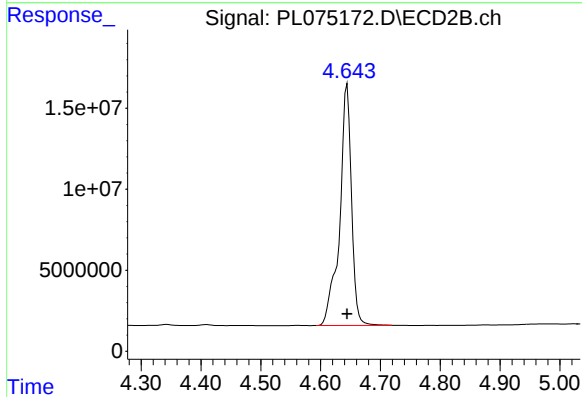


#1 Tetrachloro-m-xylene

R.T.: 4.644 min
Delta R.T.: 0.000 min
Response: 205805732
Conc: 100.16 ng/ml

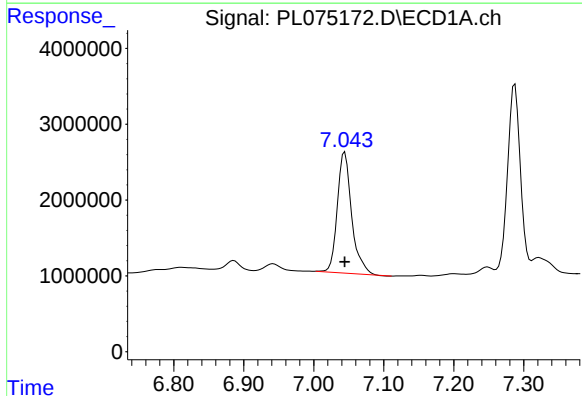


#23 Chlordane-1

R.T.: 7.044 min
Delta R.T.: 0.000 min
Response: 22805164
Conc: 989.45 ng/ml

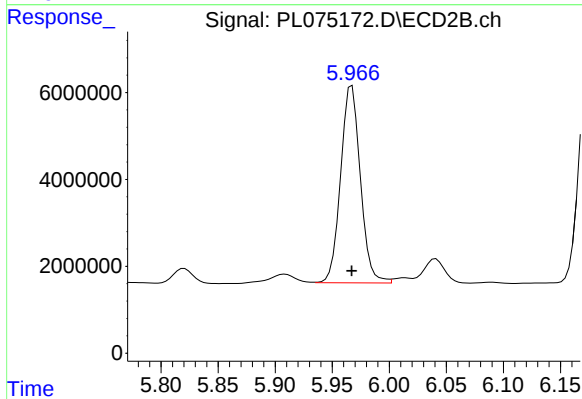

#23 Chlordane-1


R.T.: 5.967 min
Delta R.T.: 0.000 min
Response: 54560787
Conc: 978.27 ng/ml

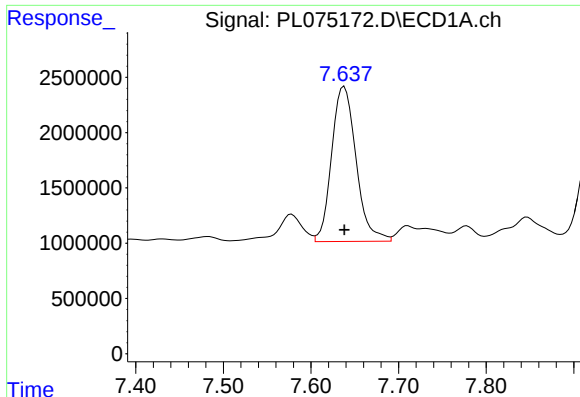

#24 Chlordane-2


R.T.: 7.638 min
Delta R.T.: 0.000 min
Response: 27235979
Conc: 963.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

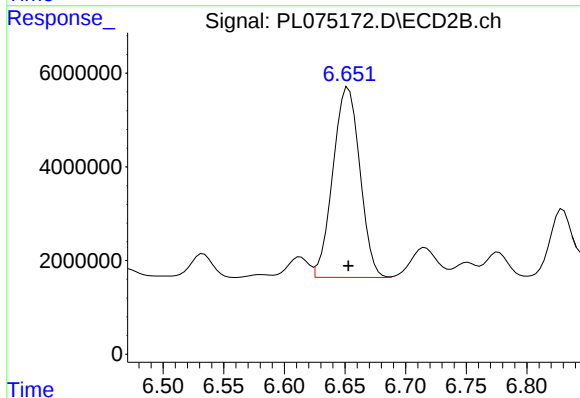


#24 Chlordane-2

R.T.: 6.653 min
Delta R.T.: 0.000 min
Response: 62769785
Conc: 952.56 ng/ml

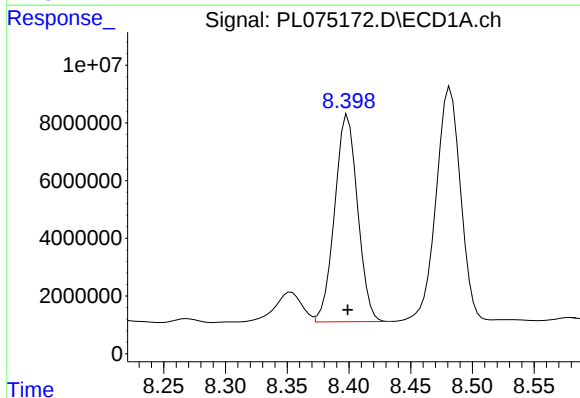


#25 Chlordane-3

R.T.: 8.399 min
Delta R.T.: 0.000 min
Response: 92755941
Conc: 971.65 ng/ml

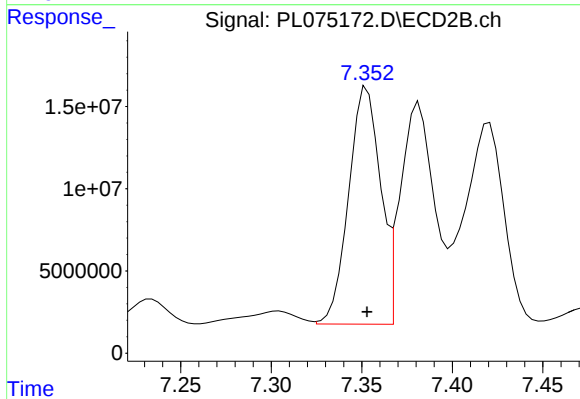

#25 Chlordane-3


R.T.: 7.353 min
Delta R.T.: 0.000 min
Response: 175776962
Conc: 981.56 ng/ml

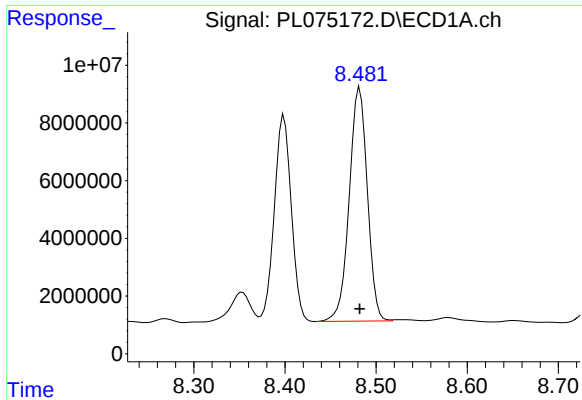

#26 Chlordane-4


R.T.: 8.482 min
Delta R.T.: 0.000 min
Response: 112010043
Conc: 966.08 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

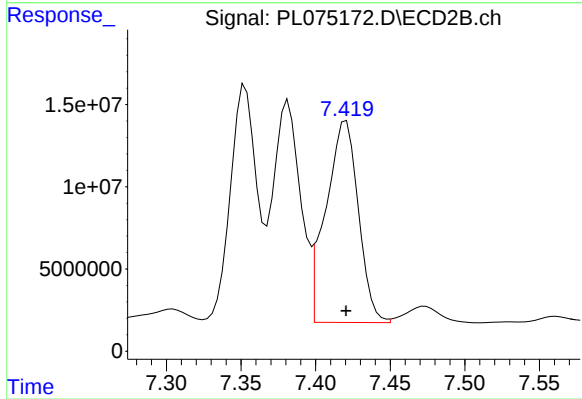


#26 Chlordane-4

R.T.: 7.420 min
Delta R.T.: 0.000 min
Response: 185861338
Conc: 978.99 ng/ml

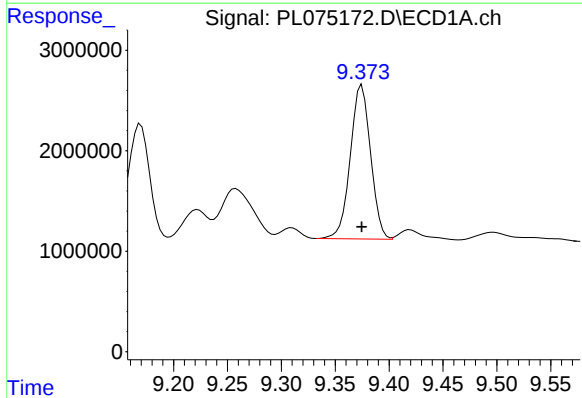


#27 Chlordane-5

R.T.: 9.375 min
Delta R.T.: 0.000 min
Response: 20105822
Conc: 959.65 ng/ml

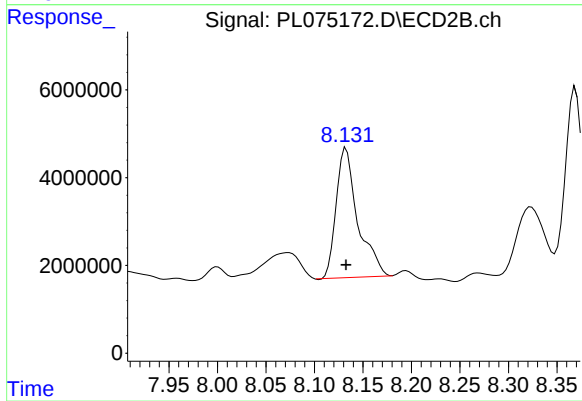

#27 Chlordane-5


R.T.: 8.133 min
Delta R.T.: 0.000 min
Response: 45795478
Conc: 941.20 ng/ml

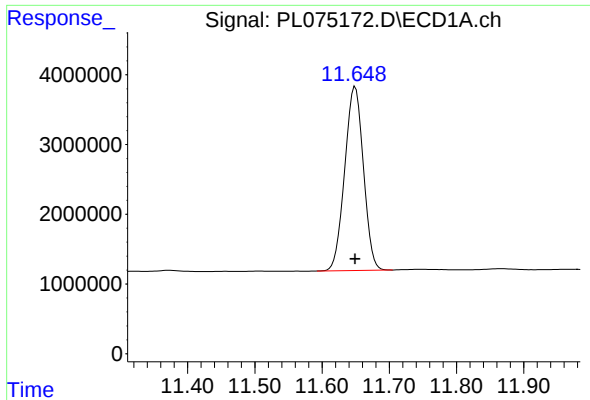

#28 Decachlorobiphenyl

R.T.: 11.649 min
Delta R.T.: 0.000 min
Response: 50865229
Conc: 93.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

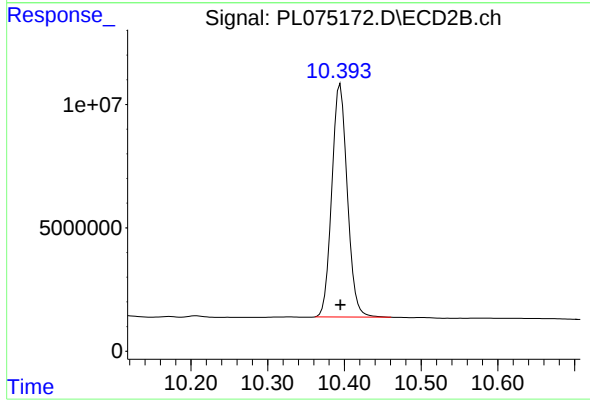

#28 Decachlorobiphenyl

R.T.: 10.395 min
Delta R.T.: 0.000 min
Response: 132641247
Conc: 95.83 ng/ml