

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052822\
 Data File : PL075173.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 May 2022 16:51
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 30 03:05:49 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
 Quant Title : GC Extractables
 QLast Update : Mon May 30 03:05:41 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.642	4.641	47473360	149.8E6	73.760	73.577
28)	SA Decachlor...	11.639	10.390	40522788	101.1E6	74.636	73.704
Target Compounds							
23)	Chlordane-1	7.037	5.963	17109988	40429880	744.883	733.079
24)	Chlordane-2	7.630	6.649	20606546	48019714	736.015	735.678
25)	Chlordane-3	8.392	7.348	70089209	130.8E6	739.400	736.652
26)	Chlordane-4	8.475	7.416	84928745	138.6E6	738.246	736.470
27)	Chlordane-5	9.368	8.128	15461936	35610952	741.957	737.824



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052822\
Data File : PL075173.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 May 2022 16:51
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 30 03:05:49 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
Quant Title : GC Extractables
QLast Update : Mon May 30 03:05:41 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

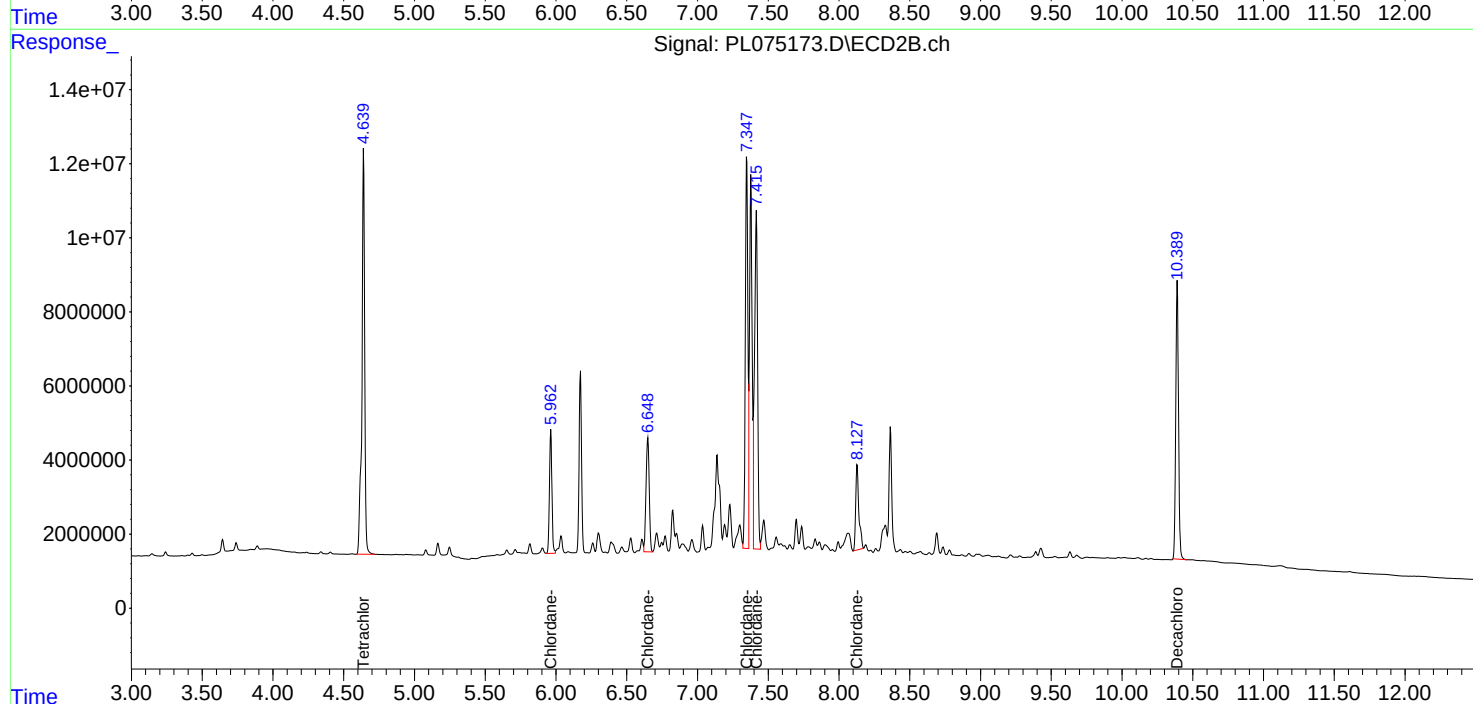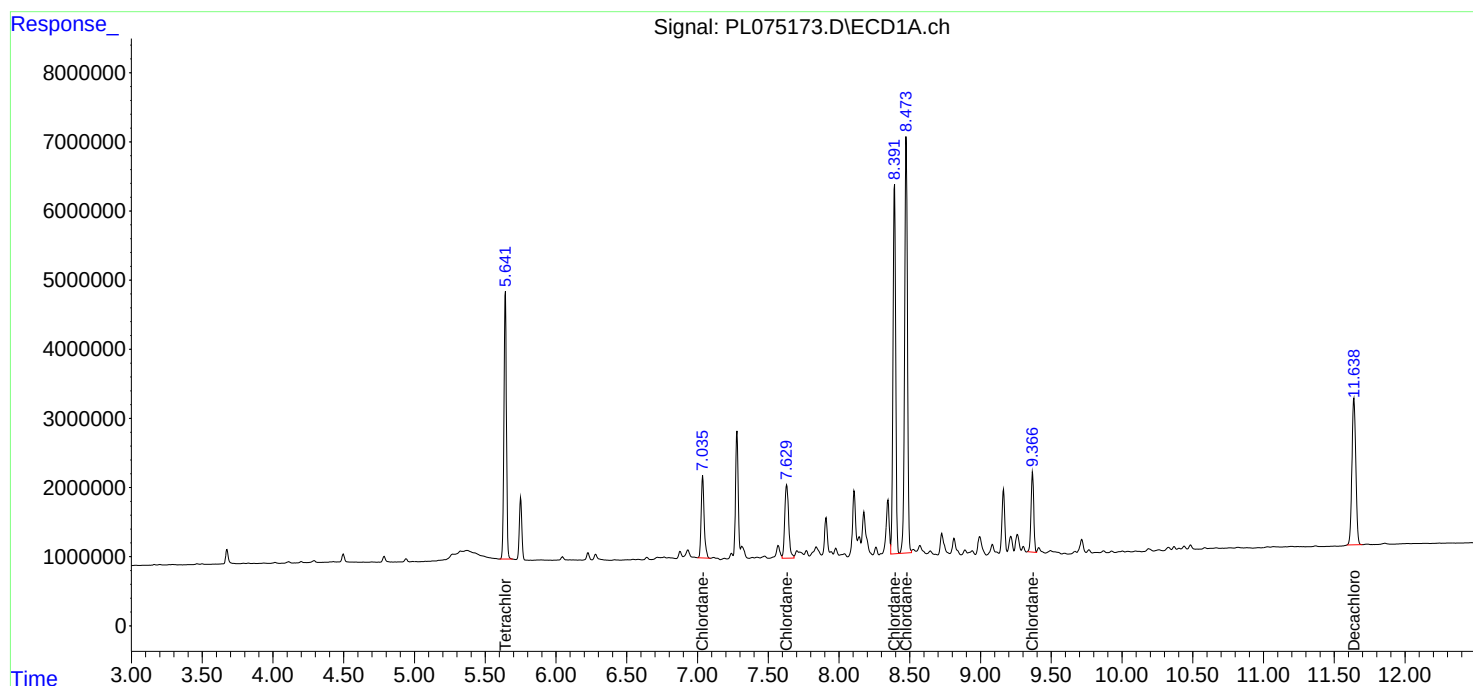


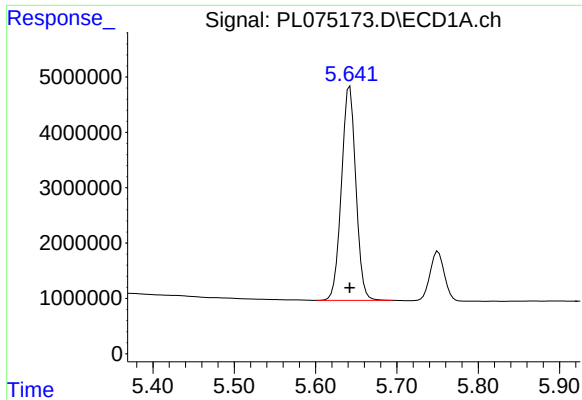

#1 Tetrachloro-m-xylene


R.T.: 5.642 min
Delta R.T.: 0.000 min
Response: 47473360
Conc: 73.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

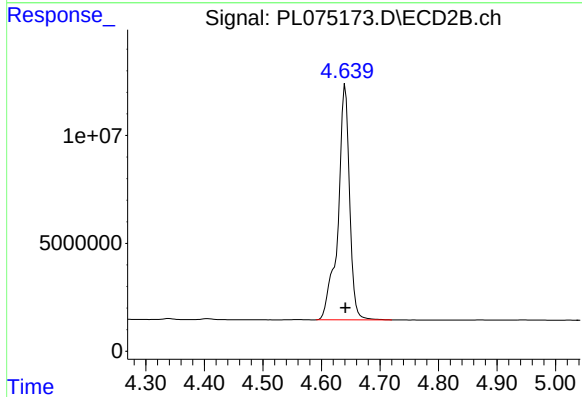


#1 Tetrachloro-m-xylene

R.T.: 4.641 min
Delta R.T.: 0.000 min
Response: 149764789
Conc: 73.58 ng/ml

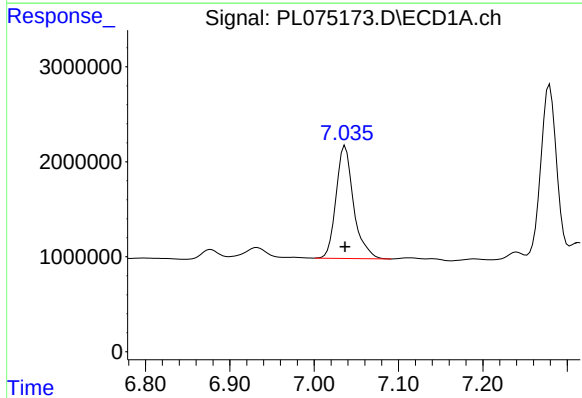


#23 Chlordane-1

R.T.: 7.037 min
Delta R.T.: 0.000 min
Response: 17109988
Conc: 744.88 ng/ml

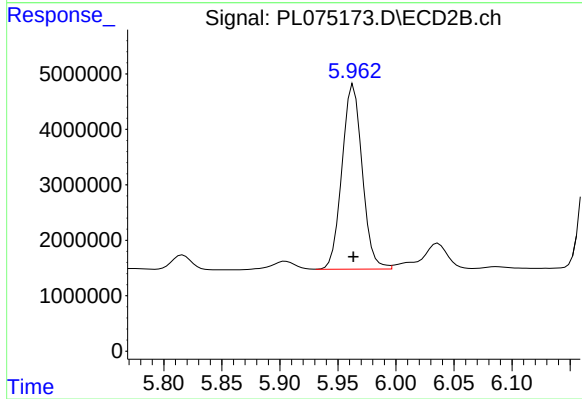

#23 Chlordane-1


R.T.: 5.963 min
Delta R.T.: 0.000 min
Response: 40429880
Conc: 733.08 ng/ml

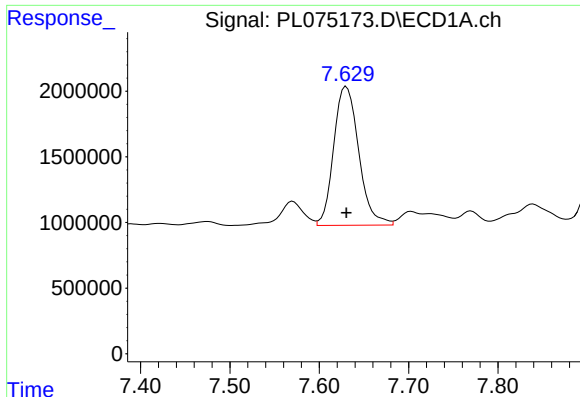

#24 Chlordane-2


R.T.: 7.630 min
Delta R.T.: 0.000 min
Response: 20606546
Conc: 736.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

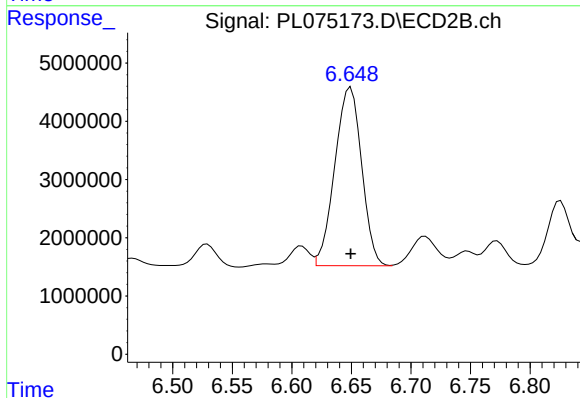


#24 Chlordane-2

R.T.: 6.649 min
Delta R.T.: 0.000 min
Response: 48019714
Conc: 735.68 ng/ml

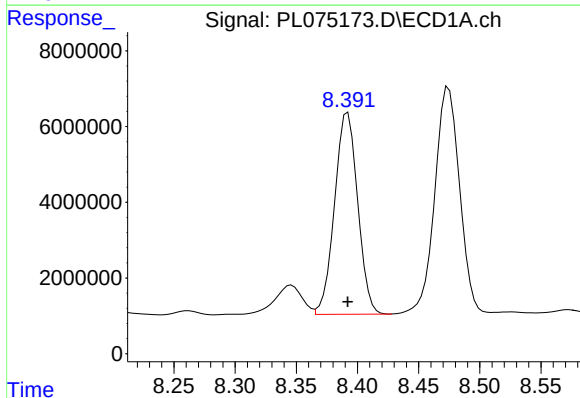


#25 Chlordane-3

R.T.: 8.392 min
Delta R.T.: 0.000 min
Response: 70089209
Conc: 739.40 ng/ml

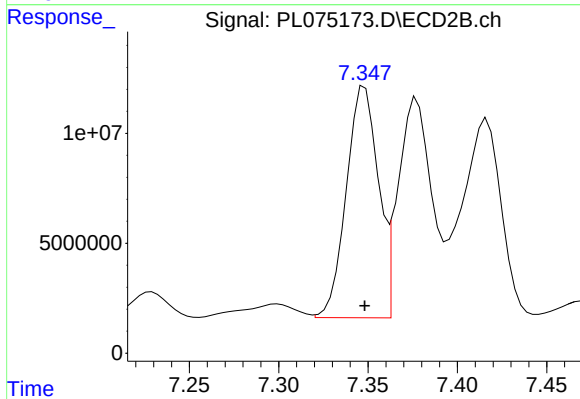

#25 Chlordane-3


R.T.: 7.348 min
Delta R.T.: 0.000 min
Response: 130755325
Conc: 736.65 ng/ml

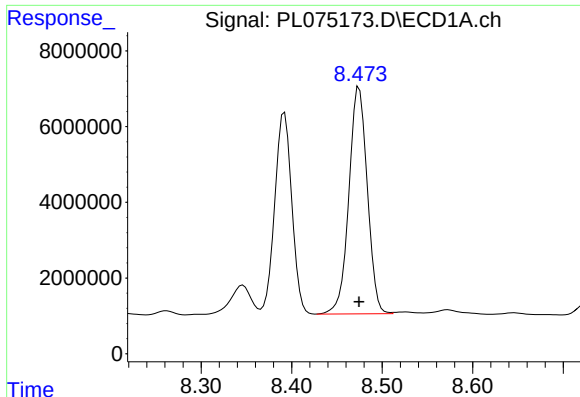

#26 Chlordane-4


R.T.: 8.475 min
Delta R.T.: 0.000 min
Response: 84928745
Conc: 738.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

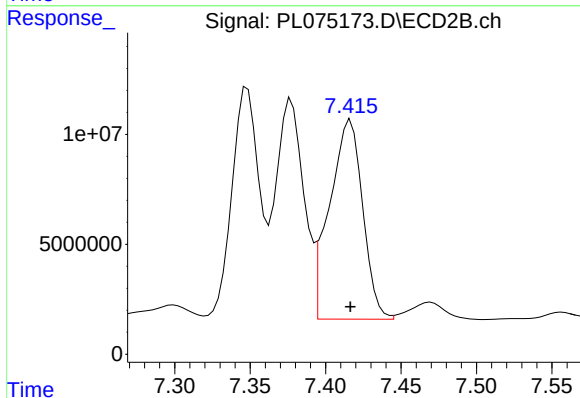


#26 Chlordane-4

R.T.: 7.416 min
Delta R.T.: 0.000 min
Response: 138569110
Conc: 736.47 ng/ml

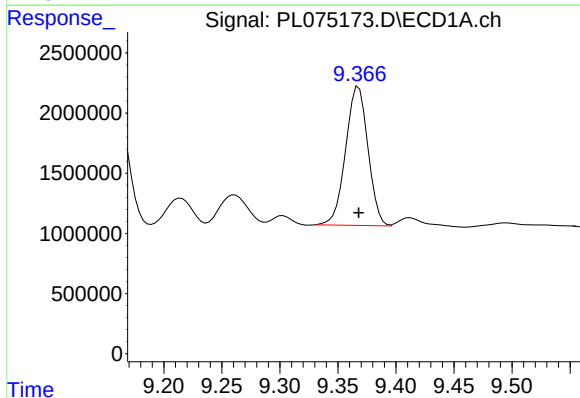


#27 Chlordane-5

R.T.: 9.368 min
Delta R.T.: 0.000 min
Response: 15461936
Conc: 741.96 ng/ml

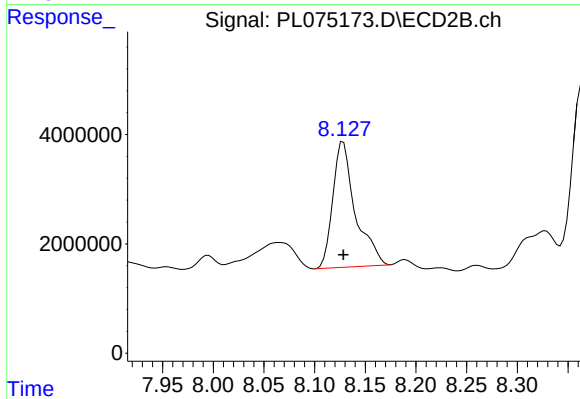

#27 Chlordane-5


R.T.: 8.128 min
Delta R.T.: 0.000 min
Response: 35610952
Conc: 737.82 ng/ml

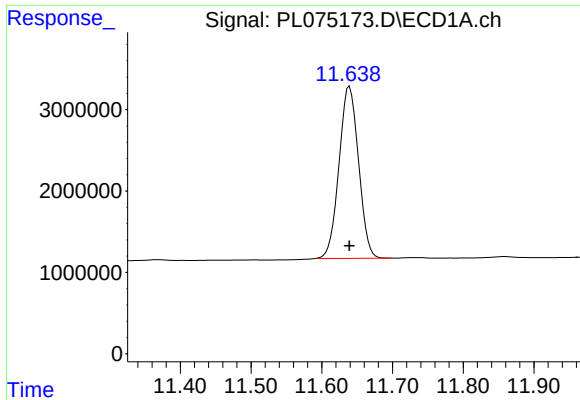

#28 Decachlorobiphenyl

R.T.: 11.639 min
Delta R.T.: 0.000 min
Response: 40522788
Conc: 74.64 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

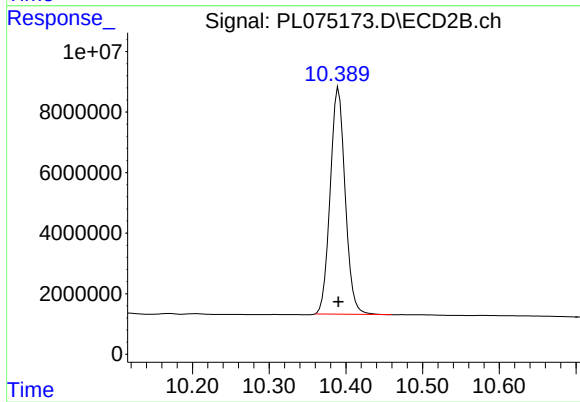

#28 Decachlorobiphenyl

R.T.: 10.390 min
Delta R.T.: 0.000 min
Response: 101140890
Conc: 73.70 ng/ml