

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052822\
 Data File : PL075174.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 May 2022 17:08
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 30 02:57:05 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
 Quant Title : GC Extractables
 QLast Update : Mon May 30 02:55:42 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.641	4.641	32606435	102.6E6	50.000	50.000
28)	SA Decachlor...	11.640	10.391	28993337	72090470	50.000	50.000
Target Compounds							
23)	Chlordane-1	7.036	5.963	11645813	28492544	500.000	500.000
24)	Chlordane-2	7.630	6.649	14640499	34511113	500.000	500.000
25)	Chlordane-3	8.392	7.348	49083977	91190392	500.000	500.000
26)	Chlordane-4	8.476	7.416	59937596	96919410	500.000	500.000
27)	Chlordane-5	9.369	8.129	10898225	25758864	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052822\
Data File : PL075174.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 May 2022 17:08
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 30 02:57:05 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
Quant Title : GC Extractables
QLast Update : Mon May 30 02:55:42 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

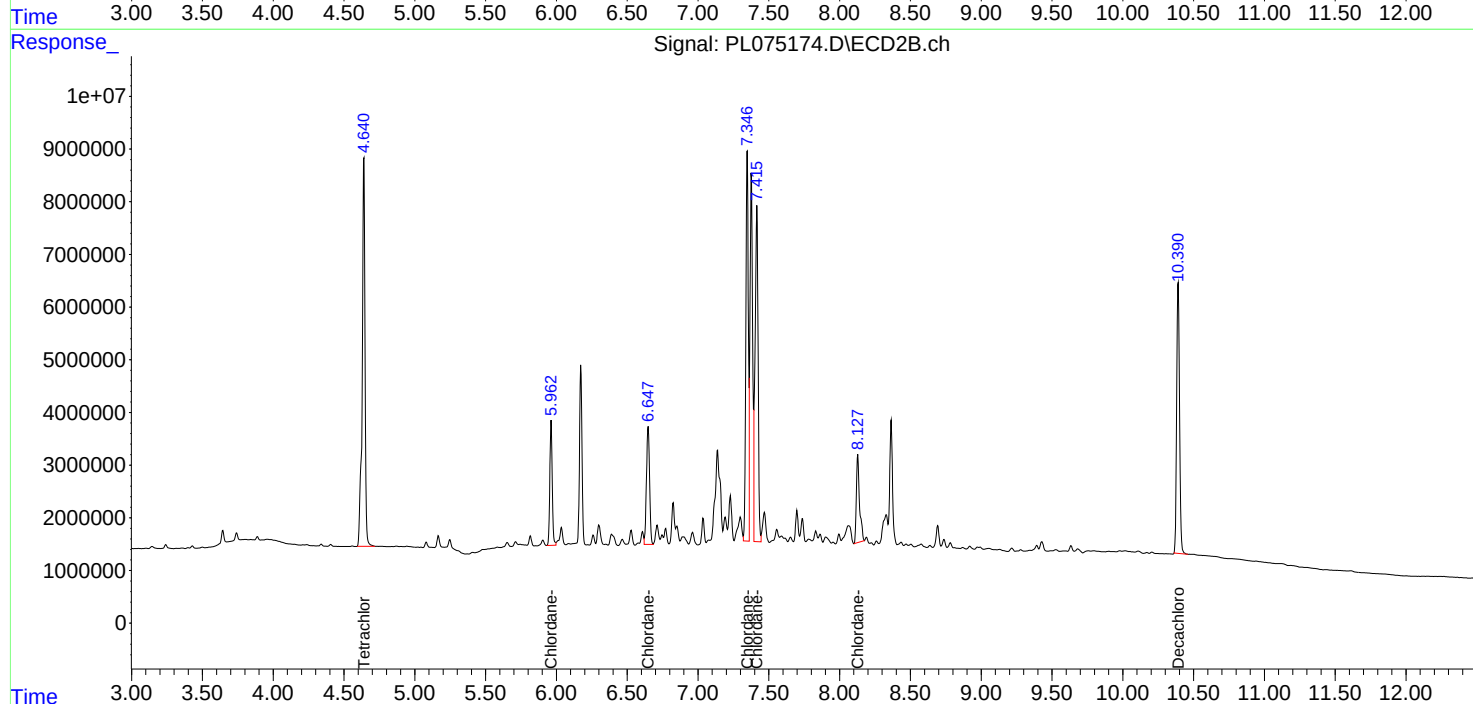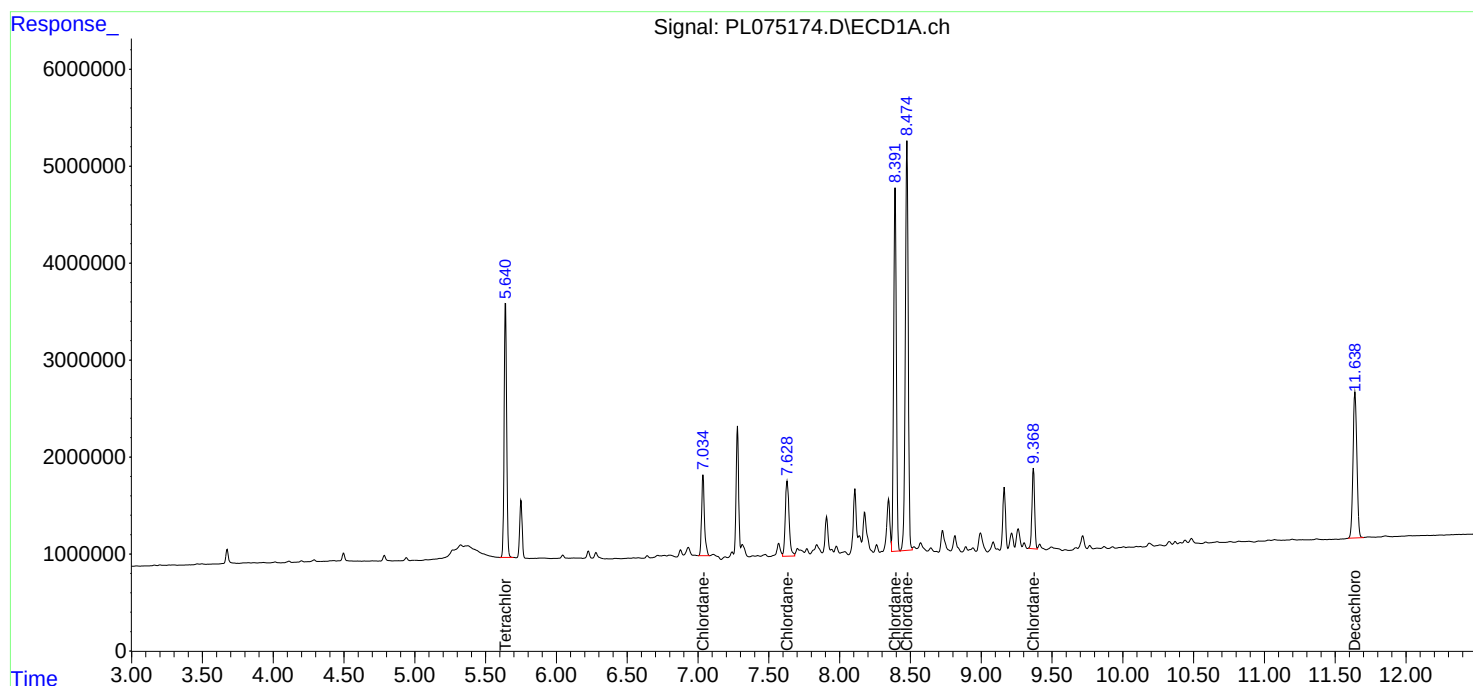


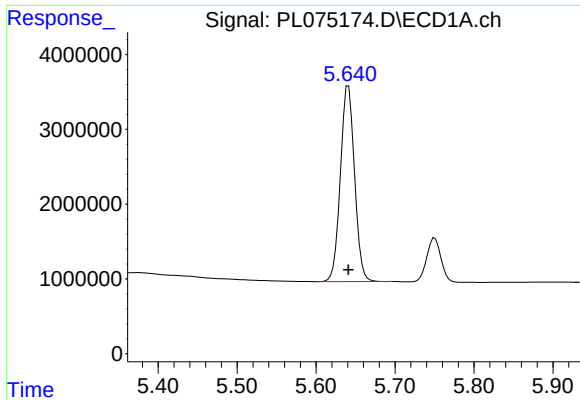

#1 Tetrachloro-m-xylene


R.T.: 5.641 min
Delta R.T.: 0.000 min
Response: 32606435
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

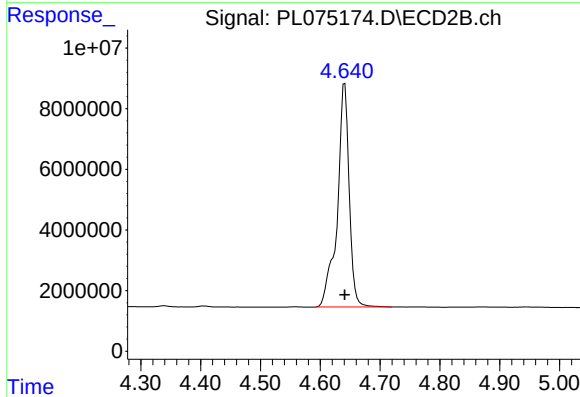


#1 Tetrachloro-m-xylene

R.T.: 4.641 min
Delta R.T.: 0.000 min
Response: 102575933
Conc: 50.00 ng/ml

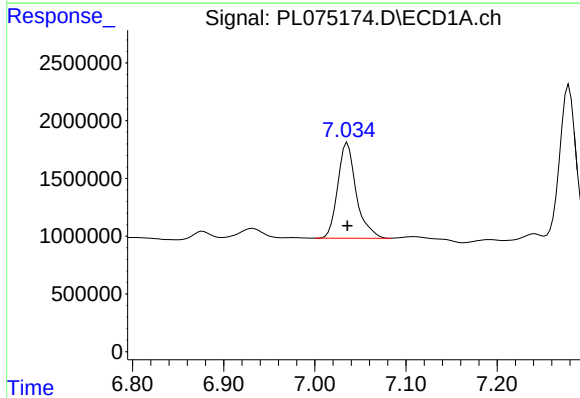


#23 Chlordane-1

R.T.: 7.036 min
Delta R.T.: 0.000 min
Response: 11645813
Conc: 500.00 ng/ml

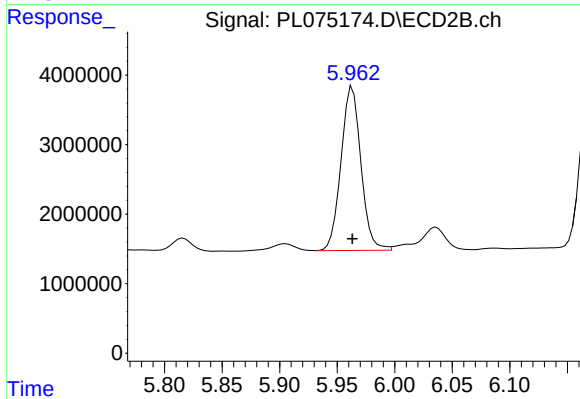

#23 Chlordane-1


R.T.: 5.963 min
Delta R.T.: 0.000 min
Response: 28492544
Conc: 500.00 ng/ml

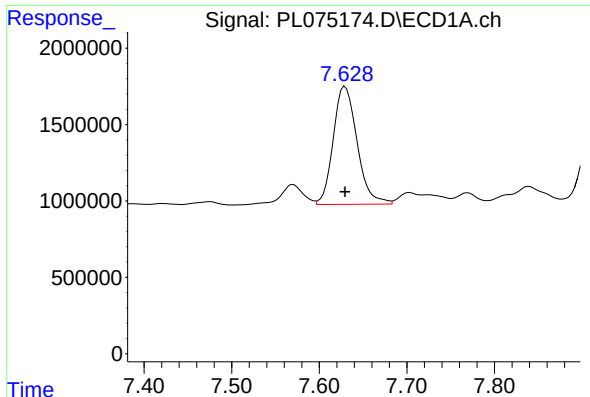

#24 Chlordane-2


R.T.: 7.630 min
Delta R.T.: 0.000 min
Response: 14640499
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

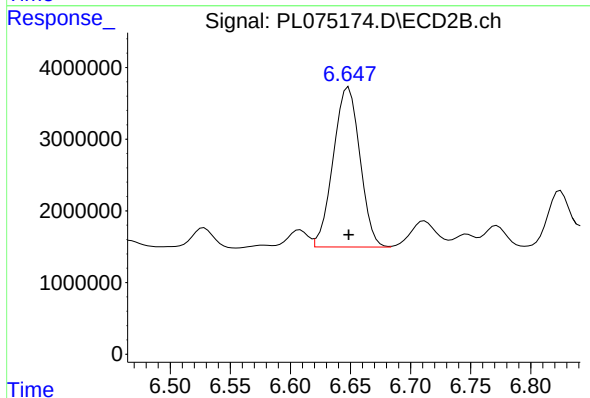


#24 Chlordane-2

R.T.: 6.649 min
Delta R.T.: 0.000 min
Response: 34511113
Conc: 500.00 ng/ml

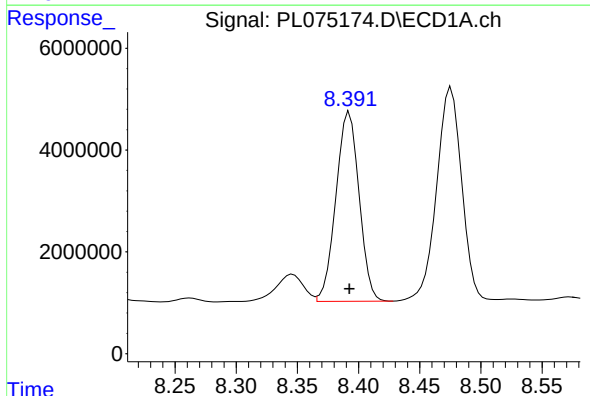


#25 Chlordane-3

R.T.: 8.392 min
Delta R.T.: 0.000 min
Response: 49083977
Conc: 500.00 ng/ml

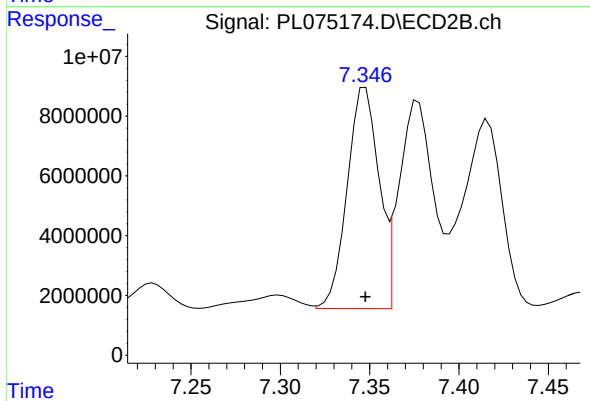

#25 Chlordane-3


R.T.: 7.348 min
Delta R.T.: 0.000 min
Response: 91190392
Conc: 500.00 ng/ml

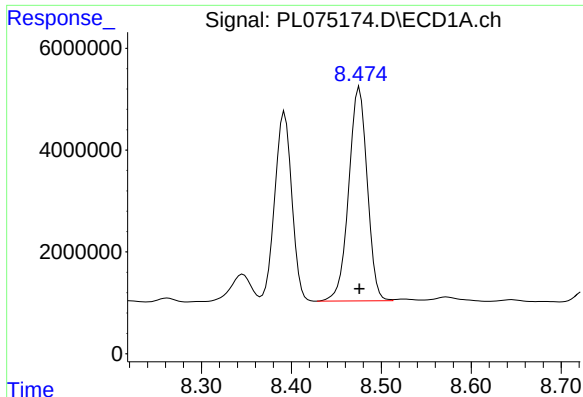

#26 Chlordane-4


R.T.: 8.476 min
Delta R.T.: 0.000 min
Response: 59937596
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

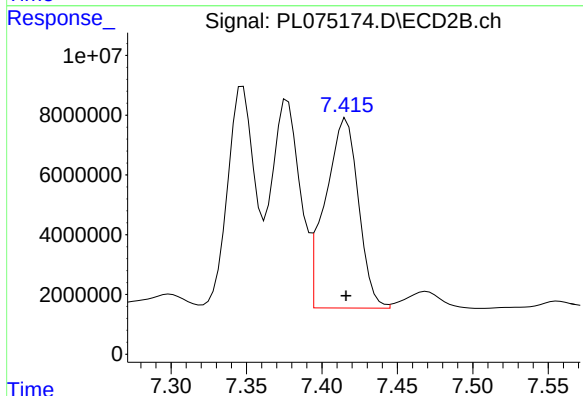


#26 Chlordane-4

R.T.: 7.416 min
Delta R.T.: 0.000 min
Response: 96919410
Conc: 500.00 ng/ml

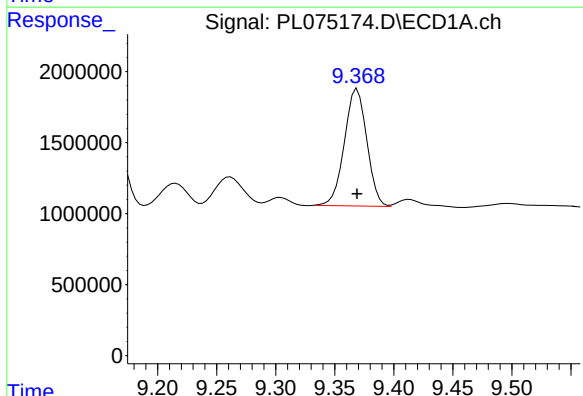


#27 Chlordane-5

R.T.: 9.369 min
Delta R.T.: 0.000 min
Response: 10898225
Conc: 500.00 ng/ml

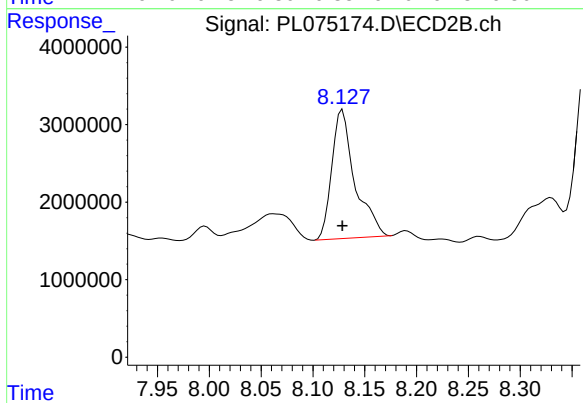

#27 Chlordane-5


R.T.: 8.129 min
Delta R.T.: 0.000 min
Response: 25758864
Conc: 500.00 ng/ml

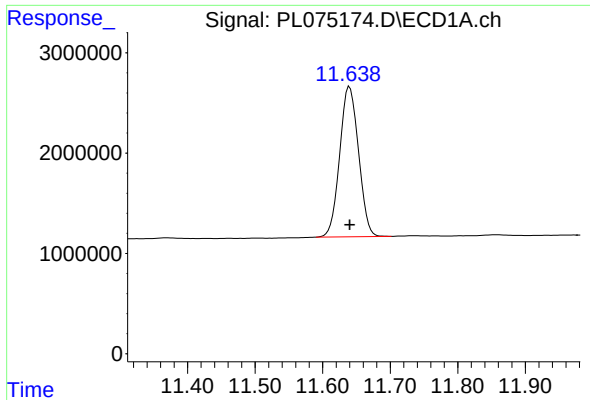

#28 Decachlorobiphenyl

R.T.: 11.640 min
Delta R.T.: 0.000 min
Response: 28993337
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

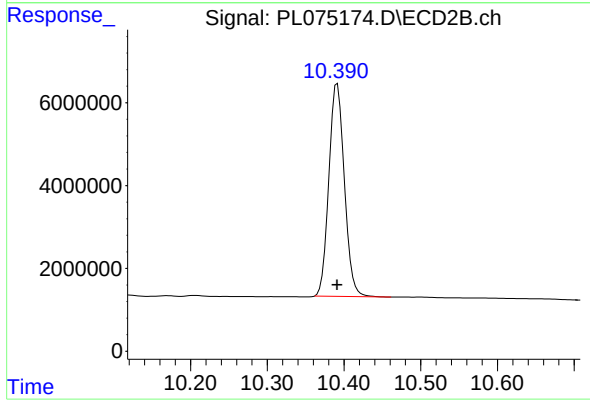

#28 Decachlorobiphenyl

R.T.: 10.391 min
Delta R.T.: 0.000 min
Response: 72090470
Conc: 50.00 ng/ml