

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052822\
 Data File : PL075175.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 May 2022 17:24
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 30 03:07:20 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
 Quant Title : GC Extractables
 QLast Update : Mon May 30 03:07:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.641	4.641	15587870	49648947	24.410	24.541
28)	SA Decachlor...	11.641	10.393	14485126	37770782	26.238	26.847
Target Compounds							
23)	Chlordane-1	7.036	5.963	5560346	13832540	244.005	250.609
24)	Chlordane-2	7.629	6.649	7207024	17608711	255.522	264.541
25)	Chlordane-3	8.392	7.348	22890572	43426401	243.557	245.971
26)	Chlordane-4	8.475	7.416	28245194	46236490	246.627	246.790
27)	Chlordane-5	9.369	8.129	5045923	12875676	244.054	262.371


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052822\
Data File : PL075175.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 May 2022 17:24
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 30 03:07:20 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
Quant Title : GC Extractables
QLast Update : Mon May 30 03:07:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

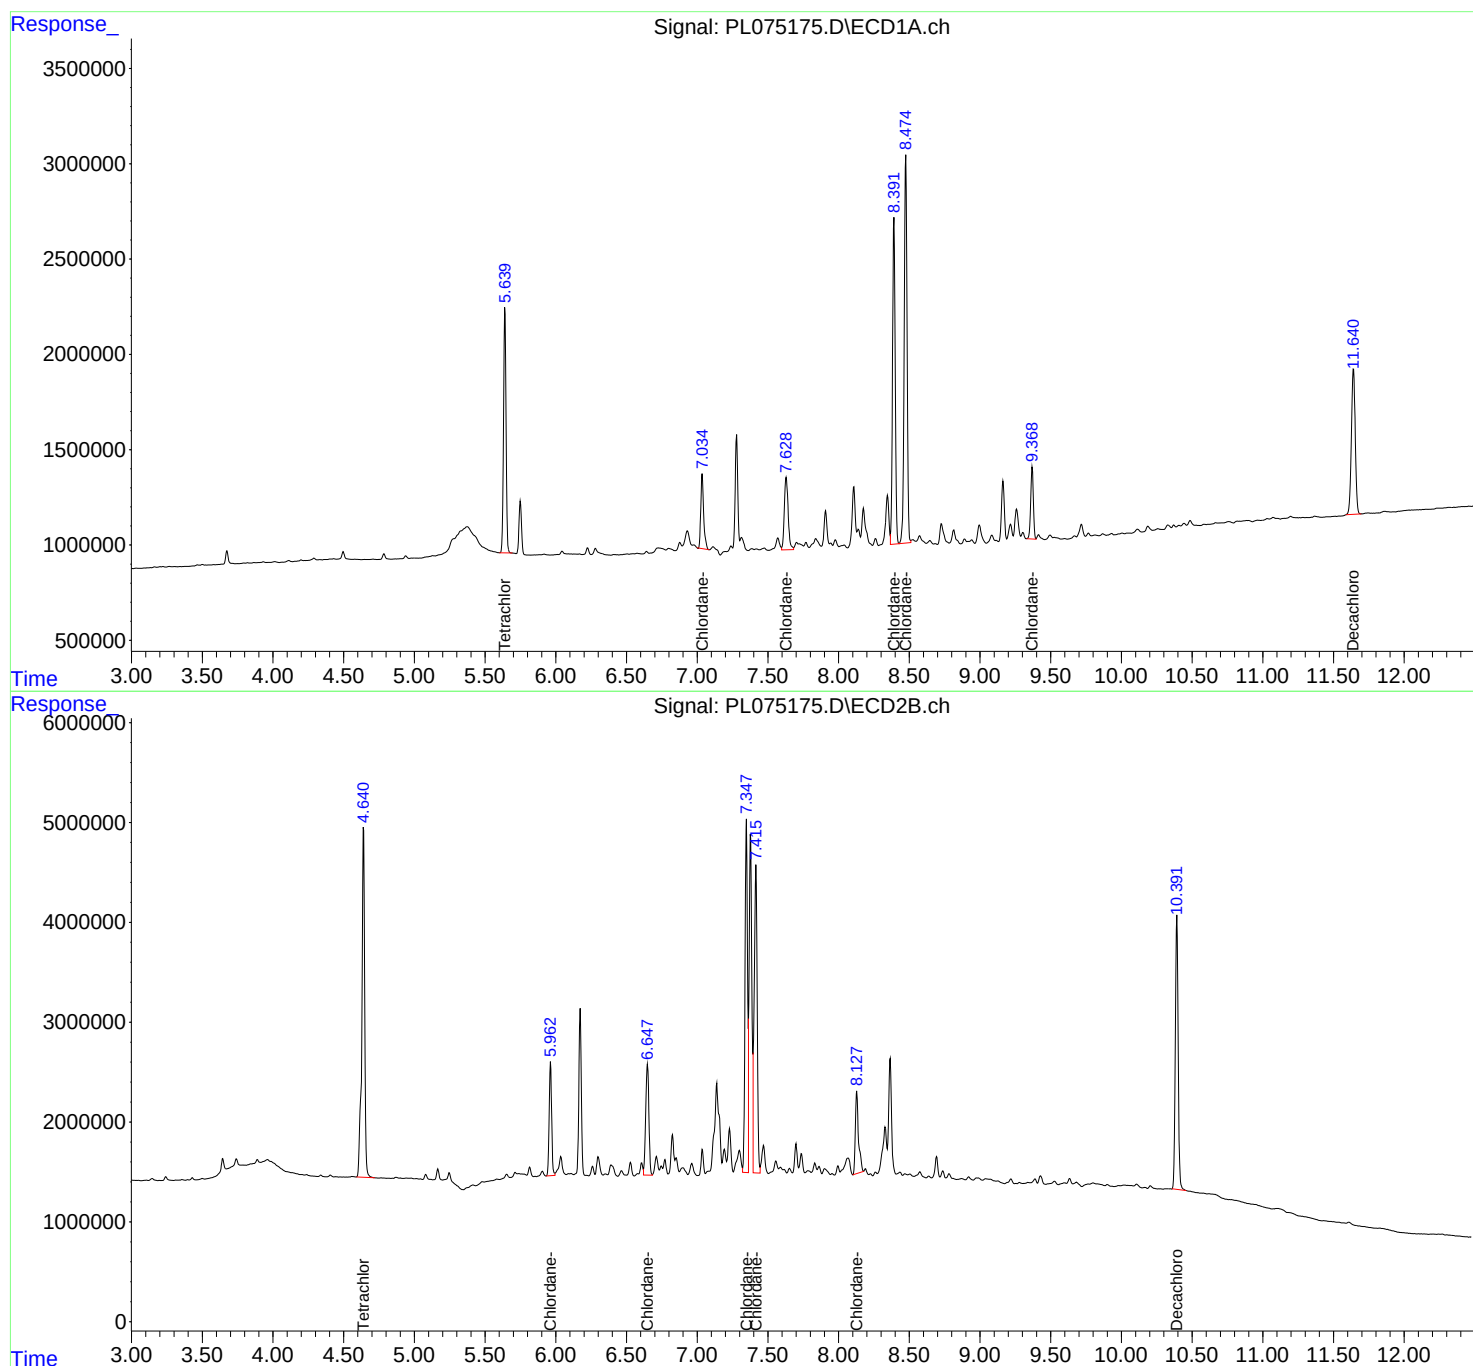


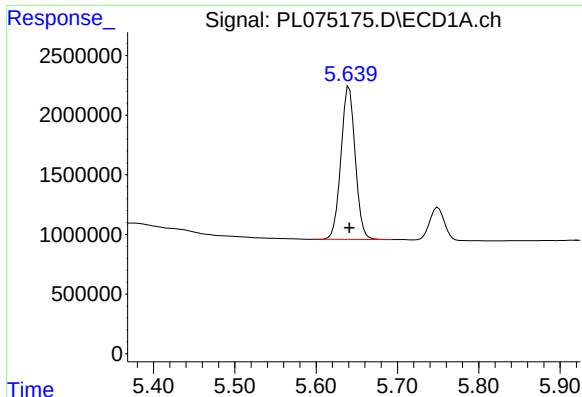

#1 Tetrachloro-m-xylene


R.T.: 5.641 min
Delta R.T.: 0.000 min
Response: 15587870
Conc: 24.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

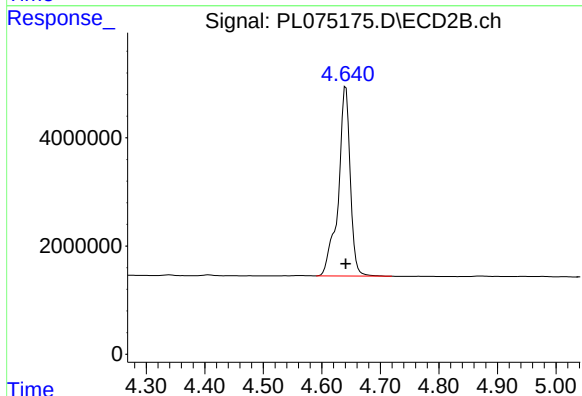


#1 Tetrachloro-m-xylene

R.T.: 4.641 min
Delta R.T.: 0.000 min
Response: 49648947
Conc: 24.54 ng/ml

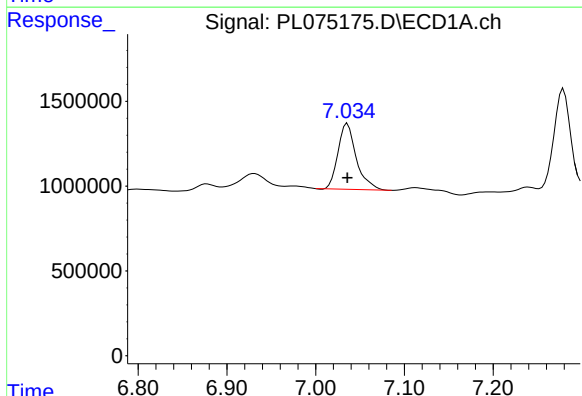


#23 Chlordane-1

R.T.: 7.036 min
Delta R.T.: 0.000 min
Response: 5560346
Conc: 244.00 ng/ml

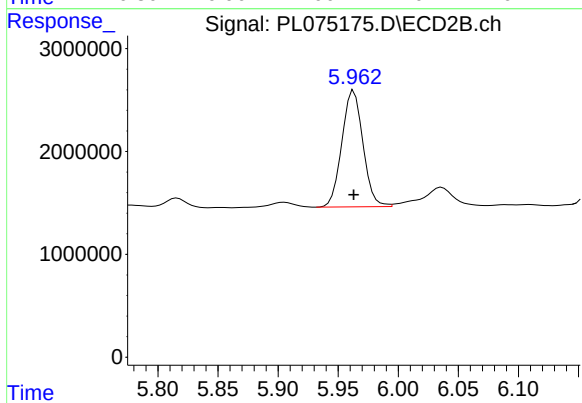

#23 Chlordane-1


R.T.: 5.963 min
Delta R.T.: 0.000 min
Response: 13832540
Conc: 250.61 ng/ml

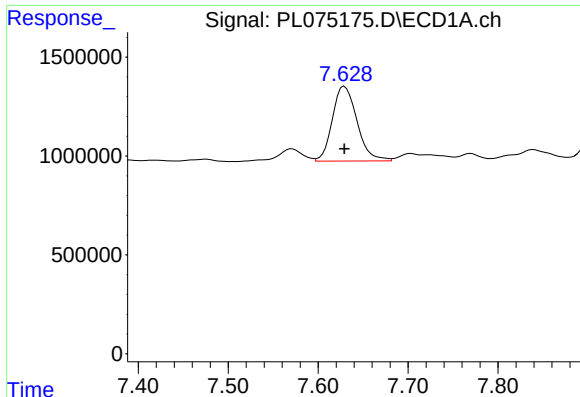

#24 Chlordane-2


R.T.: 7.629 min
Delta R.T.: 0.000 min
Response: 7207024
Conc: 255.52 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

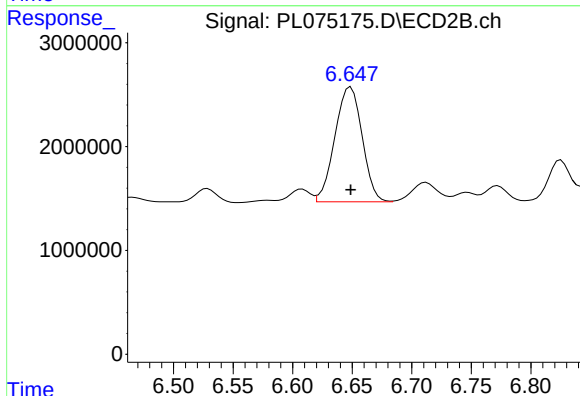


#24 Chlordane-2

R.T.: 6.649 min
Delta R.T.: 0.000 min
Response: 17608711
Conc: 264.54 ng/ml

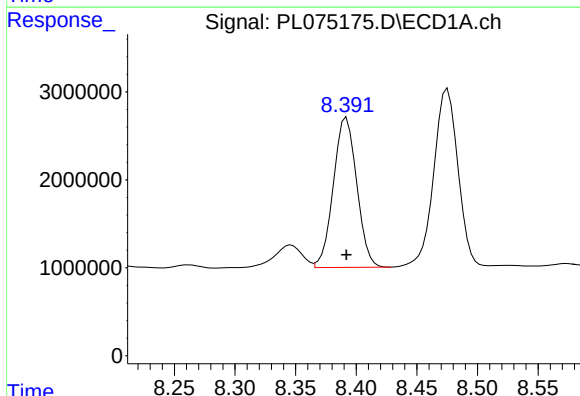


#25 Chlordane-3

R.T.: 8.392 min
Delta R.T.: 0.000 min
Response: 22890572
Conc: 243.56 ng/ml

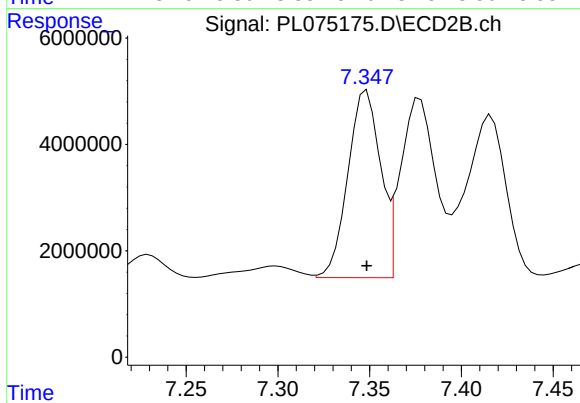

#25 Chlordane-3


R.T.: 7.348 min
Delta R.T.: 0.000 min
Response: 43426401
Conc: 245.97 ng/ml

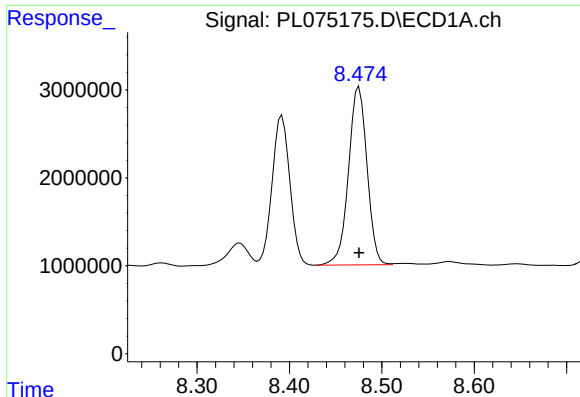

#26 Chlordane-4


R.T.: 8.475 min
Delta R.T.: 0.000 min
Response: 28245194
Conc: 246.63 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

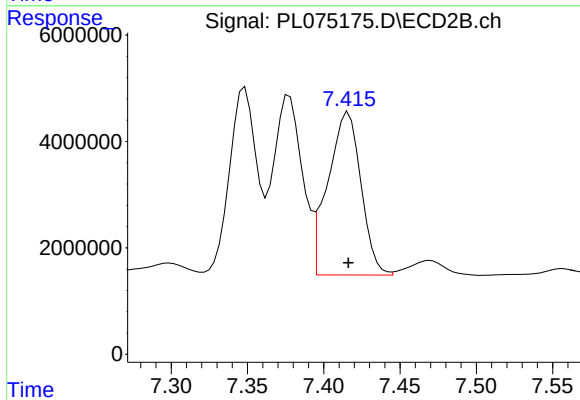


#26 Chlordane-4

R.T.: 7.416 min
Delta R.T.: 0.000 min
Response: 46236490
Conc: 246.79 ng/ml

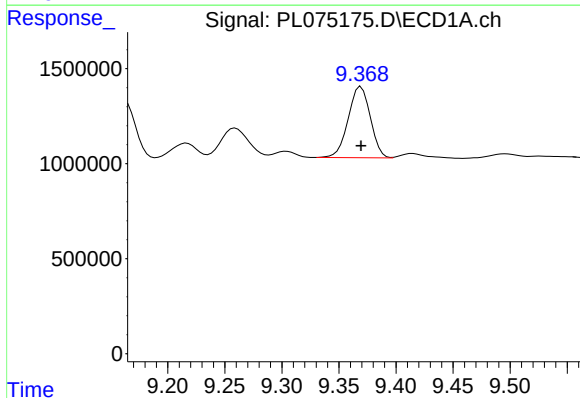


#27 Chlordane-5

R.T.: 9.369 min
Delta R.T.: 0.000 min
Response: 5045923
Conc: 244.05 ng/ml

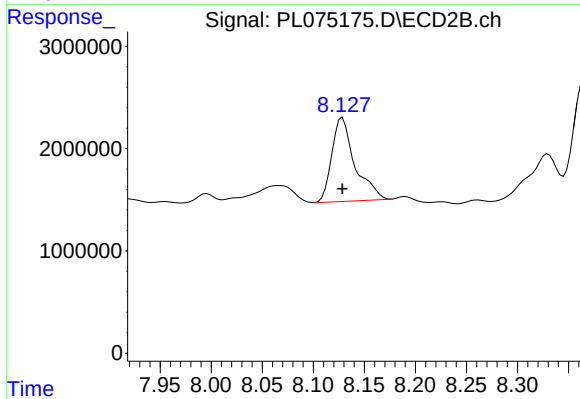

#27 Chlordane-5


R.T.: 8.129 min
Delta R.T.: 0.000 min
Response: 12875676
Conc: 262.37 ng/ml

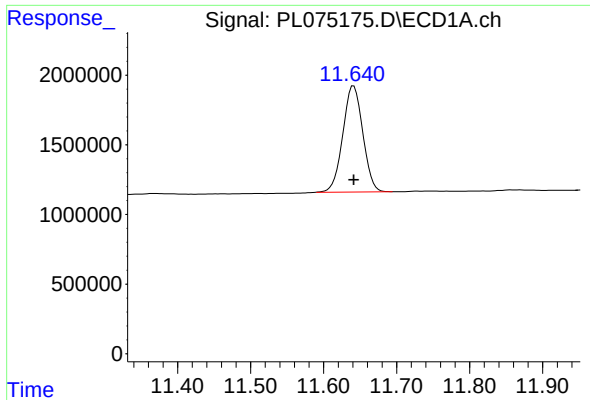

#28 Decachlorobiphenyl

R.T.: 11.641 min
Delta R.T.: 0.000 min
Response: 14485126
Conc: 26.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

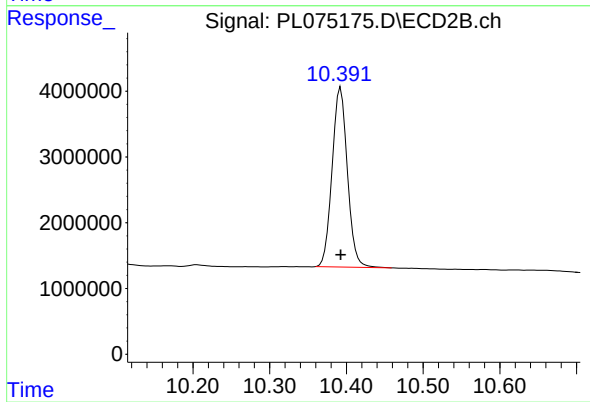

#28 Decachlorobiphenyl

R.T.: 10.393 min
Delta R.T.: 0.000 min
Response: 37770782
Conc: 26.85 ng/ml