

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052822\
 Data File : PL075199.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 May 2022 01:10
 Operator : AR\AJ
 Sample : N3026-01
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 N48967

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 05/31/2022
 Supervised By : Ankita Jodhani 05/31/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 31 03:01:20 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
 Quant Title : GC Extractables
 QLast Update : Tue May 31 02:52:42 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.641	4.641	11700762	30561940	19.908	19.292
2) SA Decachlor...	11.641	10.391	7026464	16219388	13.105	11.819
Target Compounds						
13) MA Dieldrin	8.821	7.759	197659	530786	0.312	0.306m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052822\
Data File : PL075199.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 May 2022 01:10
Operator : AR\AJ
Sample : N3026-01
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
N48967


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 05/31/2022
Supervised By : Ankita Jodhani 05/31/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 31 03:01:20 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
Quant Title : GC Extractables
QLast Update : Tue May 31 02:52:42 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

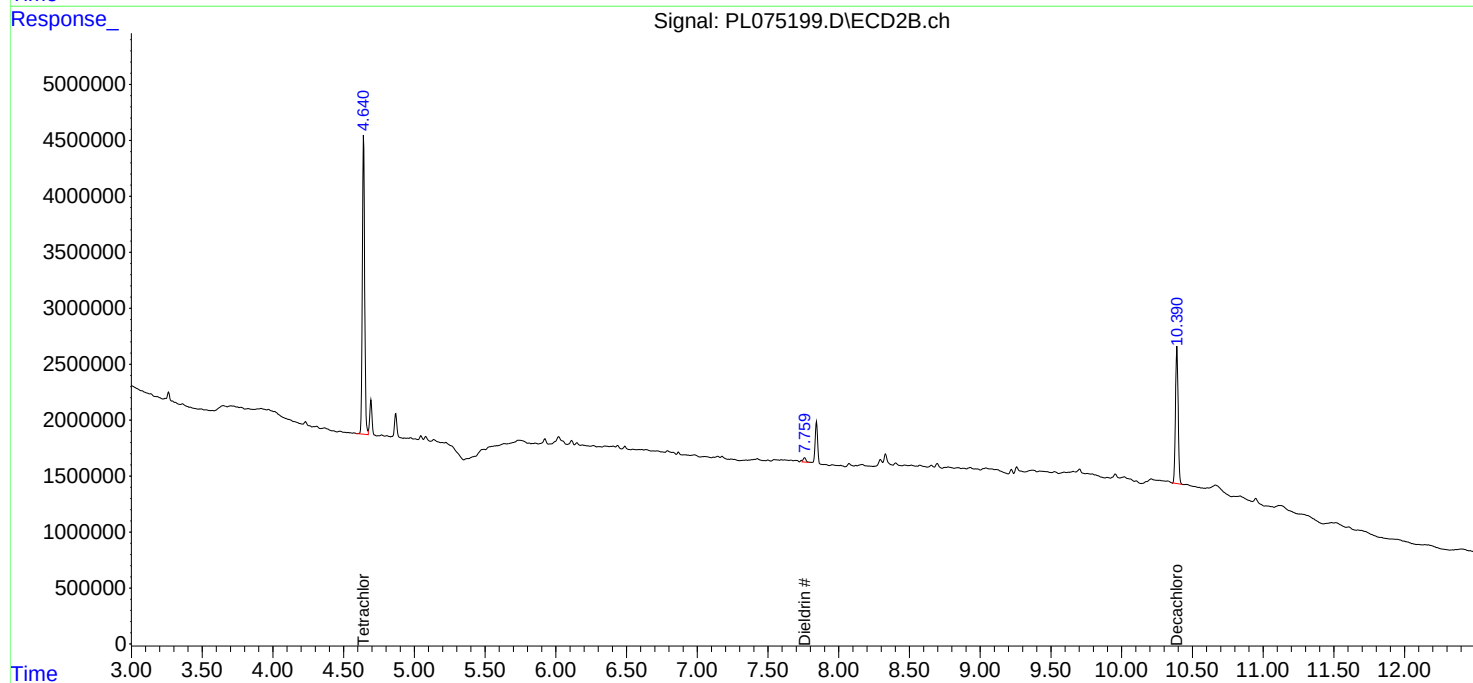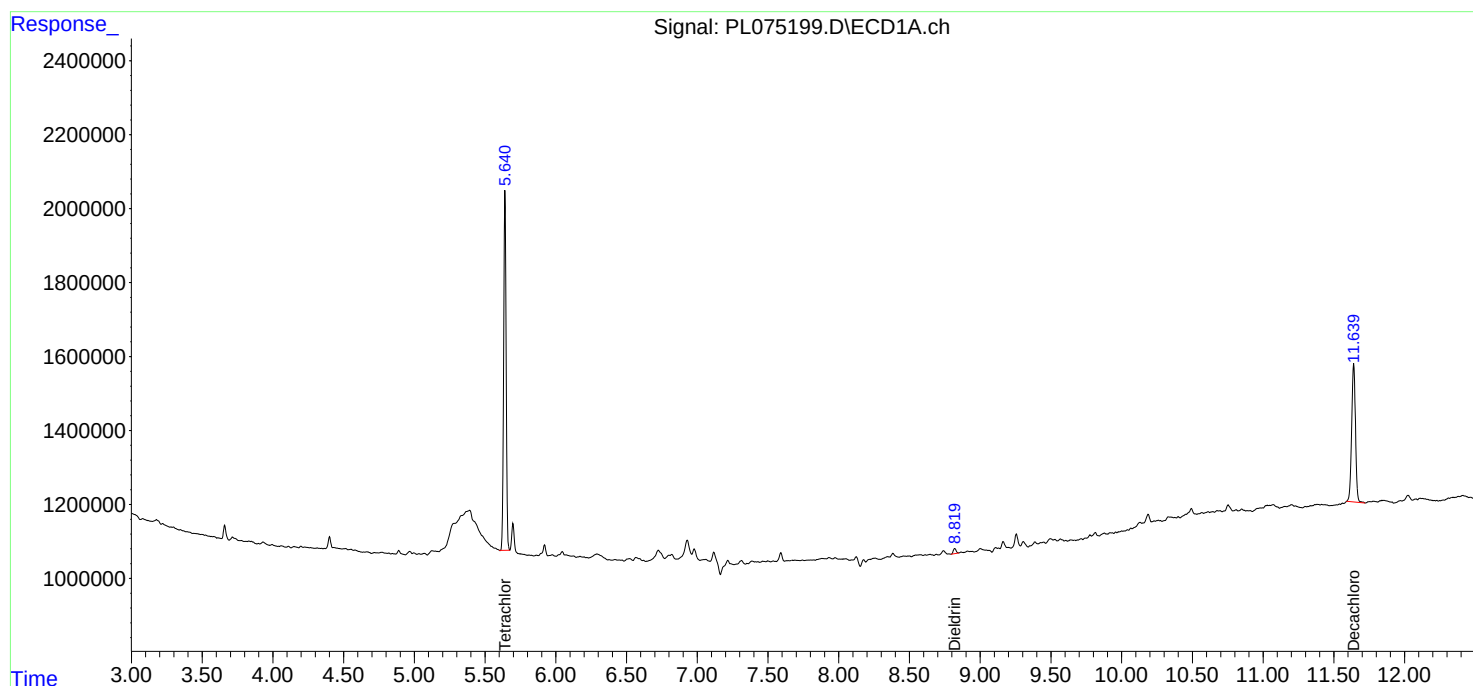

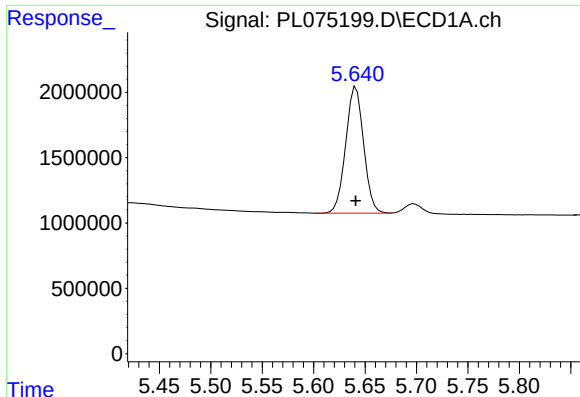


#1 Tetrachloro-m-xylene

R.T.: 5.641 min
Delta R.T.: 0.000 min
Response: 11700762
Conc: 19.91 ng/ml

Instrument :
ECD_L
ClientSampleId :
N48967


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/31/2022
Supervised By :Ankita Jodhani 05/31/2022

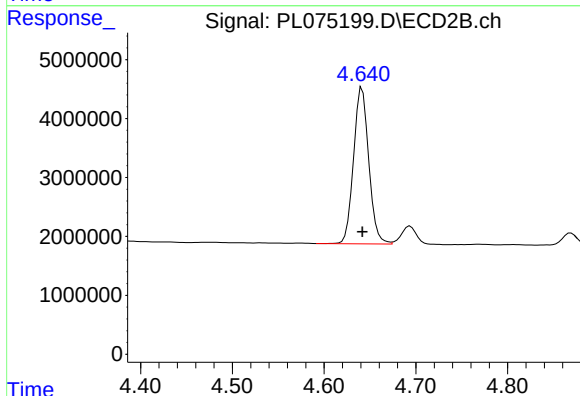


#1 Tetrachloro-m-xylene

R.T.: 4.641 min
Delta R.T.: 0.000 min
Response: 30561940
Conc: 19.29 ng/ml

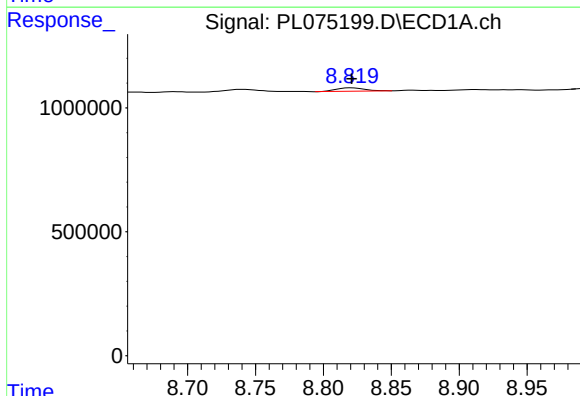


#13 Dieldrin

R.T.: 8.821 min
Delta R.T.: 0.000 min
Response: 197659
Conc: 0.31 ng/ml

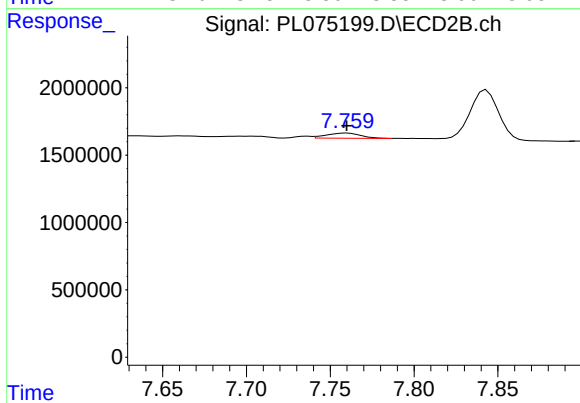

#13 Dieldrin

R.T.: 7.759 min
Delta R.T.: -0.001 min
Response: 530786
Conc: 0.31 ng/ml m

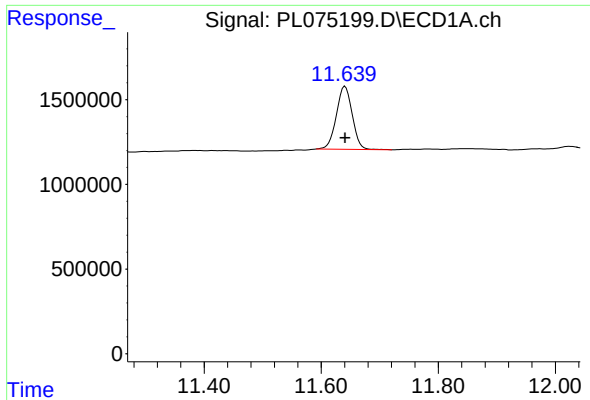


#28 Decachlorobiphenyl

R.T.: 11.641 min
Delta R.T.: 0.000 min
Response: 7026464
Conc: 13.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
N48967

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/31/2022
Supervised By :Ankita Jodhani 05/31/2022

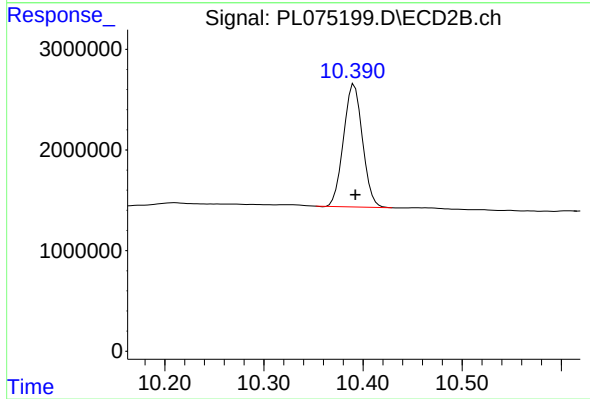

#28 Decachlorobiphenyl

R.T.: 10.391 min
Delta R.T.: -0.001 min
Response: 16219388
Conc: 11.82 ng/ml