

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052919\
 Data File : PL049037.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 May 2019 11:07
 Operator : SM\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 30 01:07:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
 Quant Title : GC Extractables
 QLast Update : Thu May 02 09:36:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
Target Compounds							
8) B	Heptachlo...	5.020f	5.802	7876994	16460281	0.611	5.643 #
13) MA	Dieldrin	5.550	0.000	317.1E6	0	24.355	N.D. #
14) MA	Endrin	0.000	6.644	0	14301231	N.D.	5.485 #
15) B	Endosulfa...	6.068f	0.000	48536482	0	4.206	N.D. #
16) A	4,4'-DDD	5.955	0.000	15171259	0	1.559	N.D. #
17) MA	4,4'-DDT	6.185	0.000	230.3E6	0	22.920	N.D. #
18) B	Endrin al...	6.274f	0.000	230.2E6	0	23.689	N.D. #
20) A	Methoxychlor	6.743	0.000	326.0E6	0	59.881	N.D. #
21) B	Endrin ke...	6.923f	0.000	165.1E6	0	14.165	N.D. #
22)	Mirex	7.114	0.000	23843703	0	2.660	N.D. #
24)	Chlordane-2	4.652	0.000	13120462	0	25.363	N.D. #
27)	Chlordane-5	6.068f	0.000	48536482	0	103.367	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052919\
Data File : PL049037.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 May 2019 11:07
Operator : SM\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 30 01:07:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
Quant Title : GC Extractables
QLast Update : Thu May 02 09:36:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

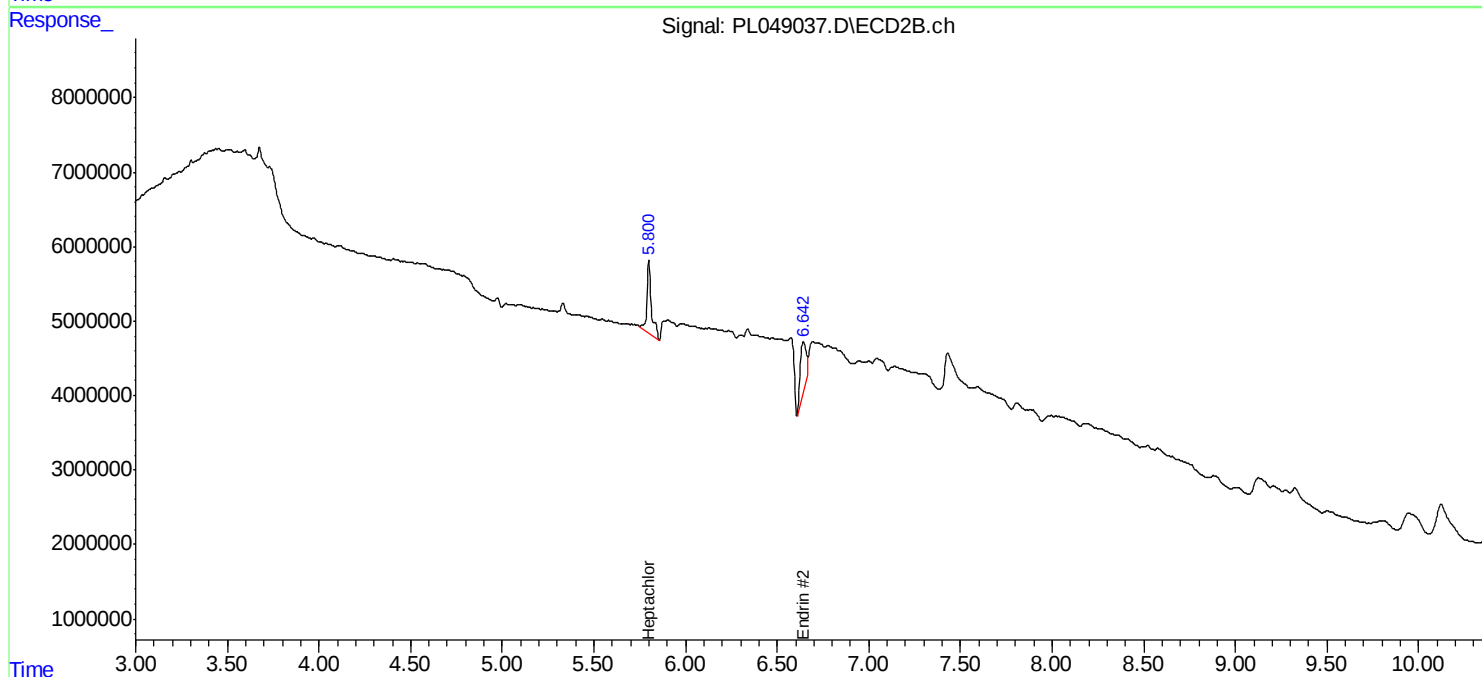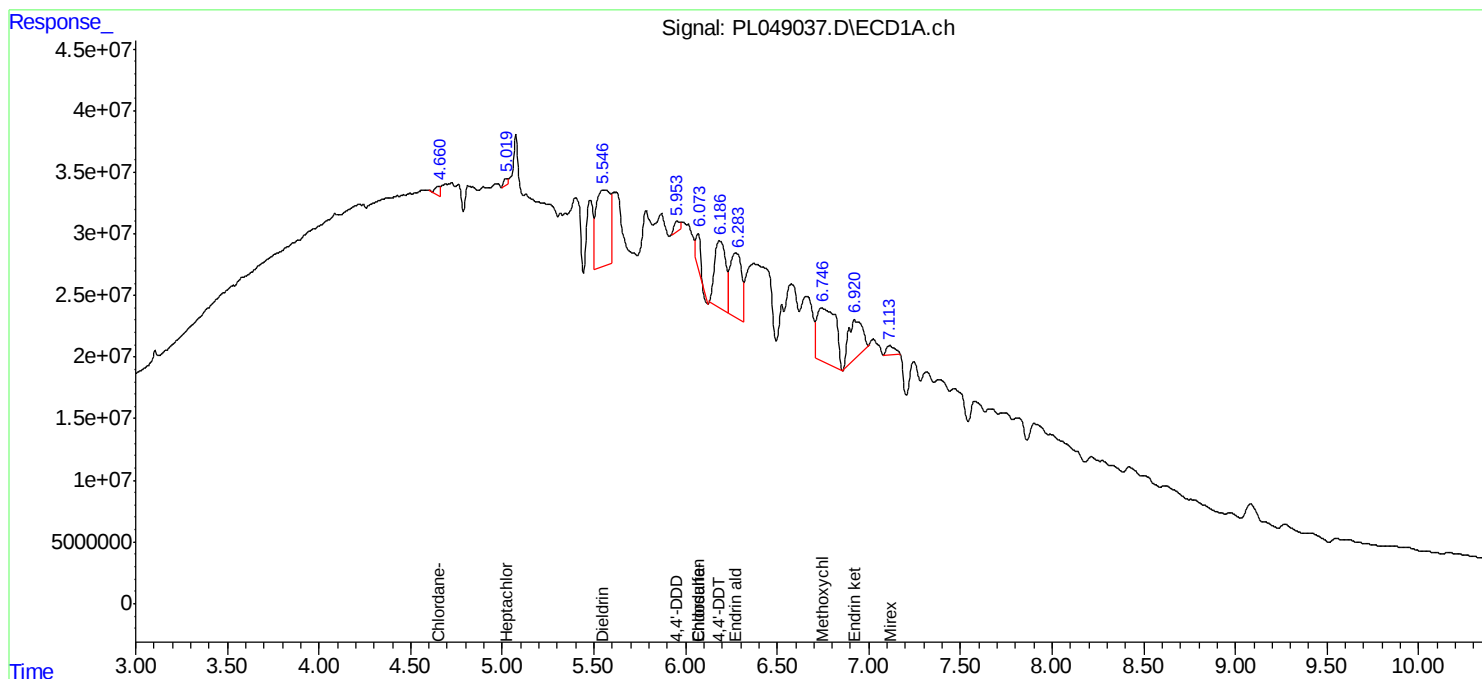


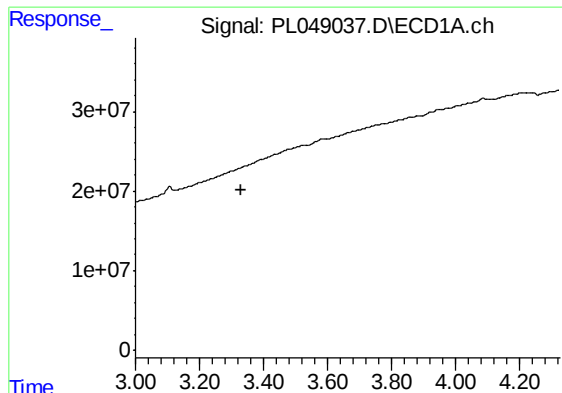

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.328 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

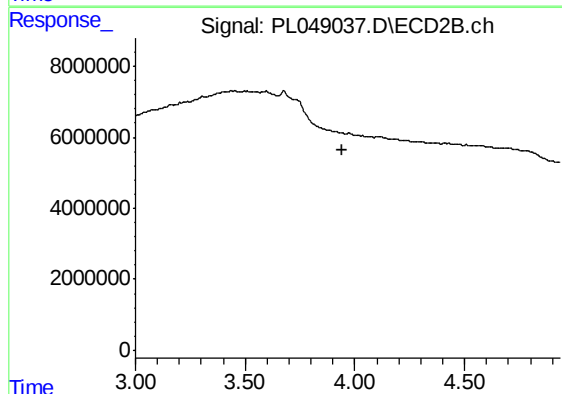


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.940 min
Response: 0
Conc: N.D.

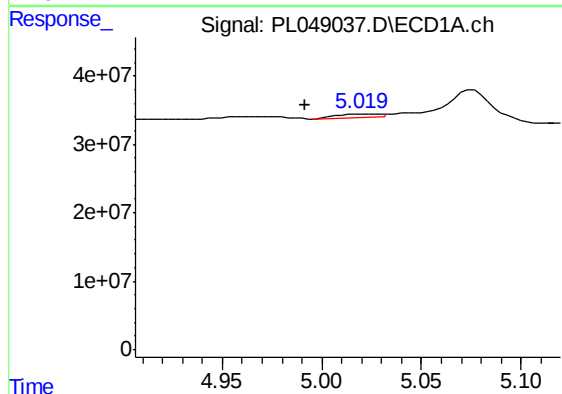


#8 Heptachlor epoxide

R.T.: 5.020 min
Delta R.T.: 0.028 min
Response: 7876994
Conc: 0.61 ng/ml

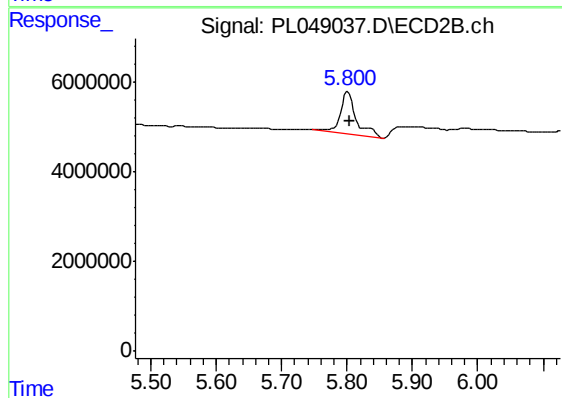

#8 Heptachlor epoxide


R.T.: 5.802 min
Delta R.T.: -0.003 min
Response: 16460281
Conc: 5.64 ng/ml

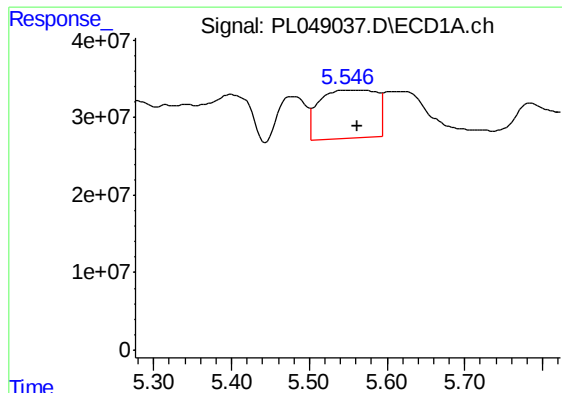

#13 Dieldrin


R.T.: 5.550 min
Delta R.T.: -0.012 min
Response: 317122595
Conc: 24.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

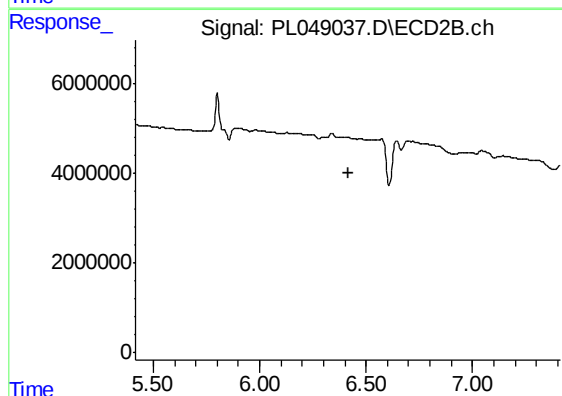


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.416 min
Response: 0
Conc: N.D.

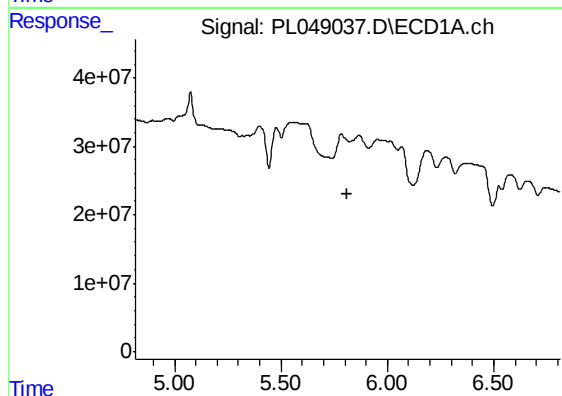


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 5.814 min
Response: 0
Conc: N.D.

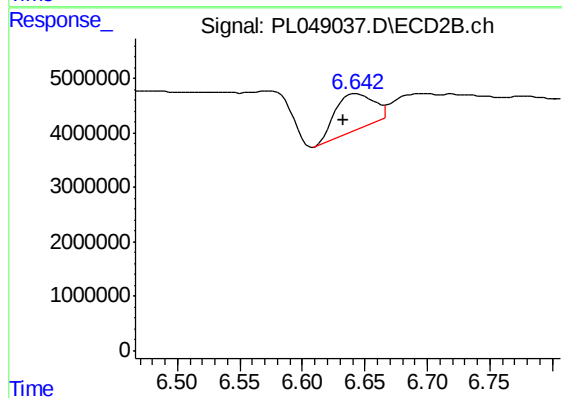

#14 Endrin


R.T.: 6.644 min
Delta R.T.: 0.011 min
Response: 14301231
Conc: 5.48 ng/ml

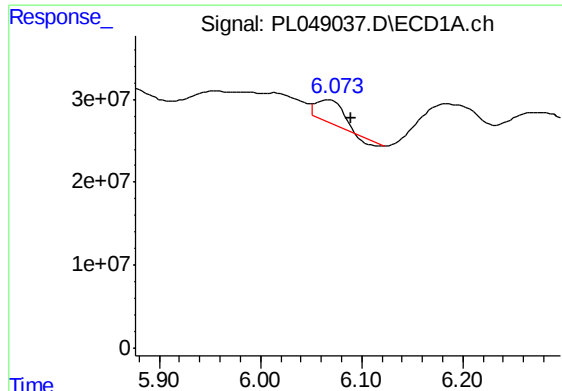

#15 Endosulfan II


R.T.: 6.068 min
Delta R.T.: -0.021 min
Response: 48536482
Conc: 4.21 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

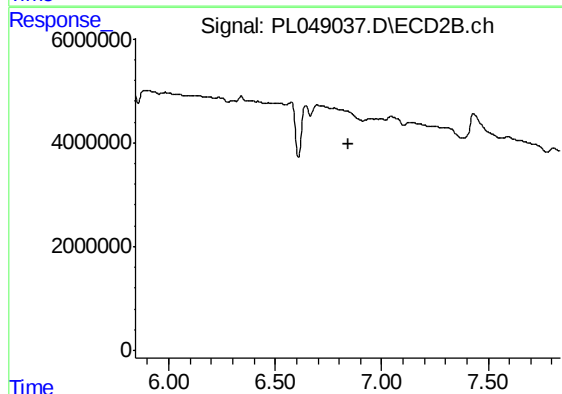


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.843 min
Response: 0
Conc: N.D.

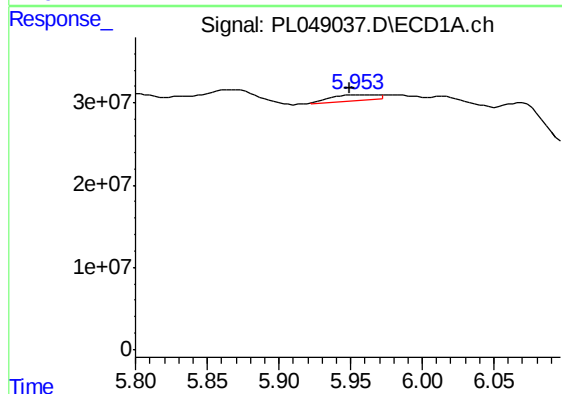


#16 4,4'-DDD

R.T.: 5.955 min
Delta R.T.: 0.006 min
Response: 15171259
Conc: 1.56 ng/ml

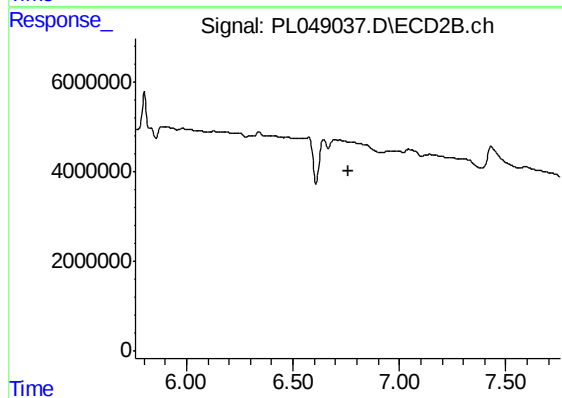

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 6.759 min
Response: 0
Conc: N.D.

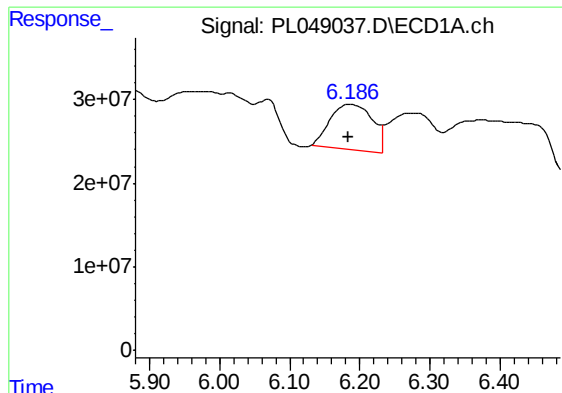

#17 4,4'-DDT


R.T.: 6.185 min
Delta R.T.: 0.001 min
Response: 230264014
Conc: 22.92 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

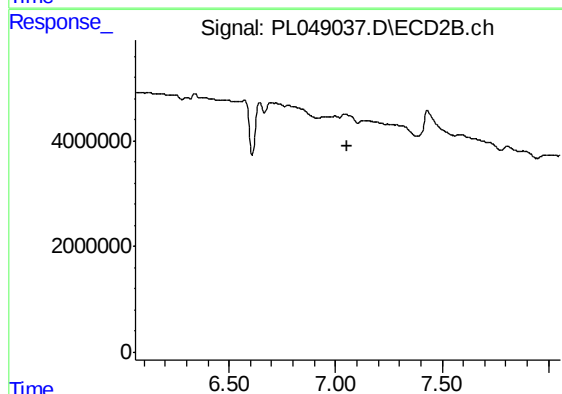


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.057 min
Response: 0
Conc: N.D.

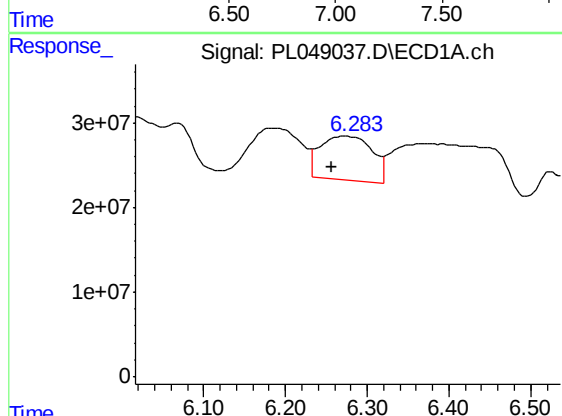


#18 Endrin aldehyde

R.T.: 6.274 min
Delta R.T.: 0.017 min
Response: 230220700
Conc: 23.69 ng/ml

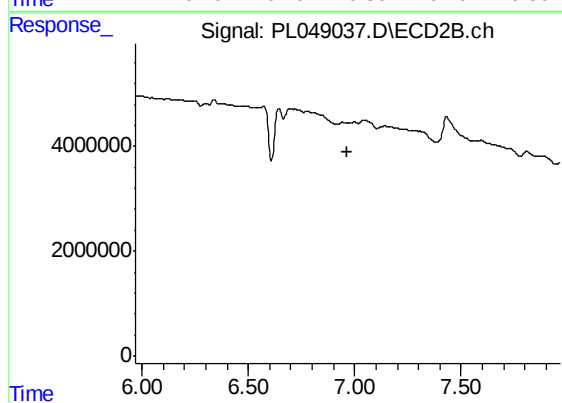

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 6.967 min
Response: 0
Conc: N.D.

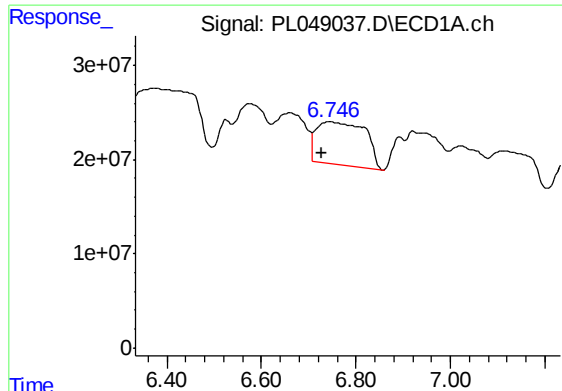

#20 Methoxychlor


R.T.: 6.743 min
Delta R.T.: 0.014 min
Response: 326033900
Conc: 59.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

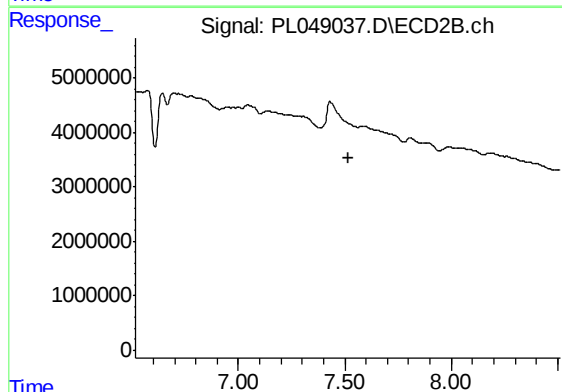


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.516 min
Response: 0
Conc: N.D.

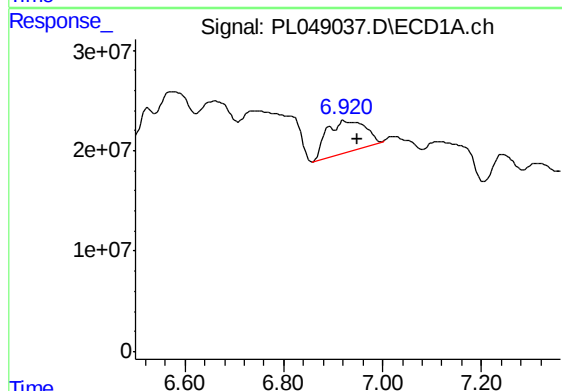


#21 Endrin ketone

R.T.: 6.923 min
Delta R.T.: -0.027 min
Response: 165096319
Conc: 14.17 ng/ml

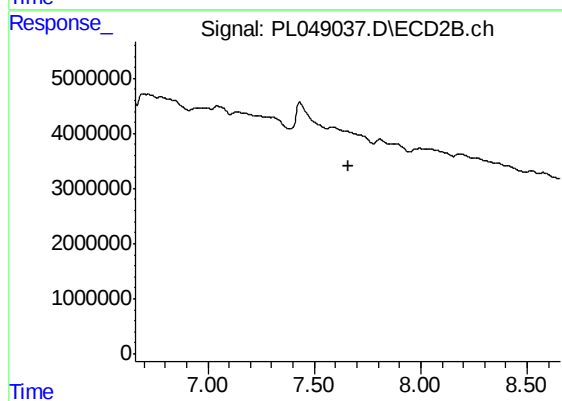

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 7.658 min
Response: 0
Conc: N.D.

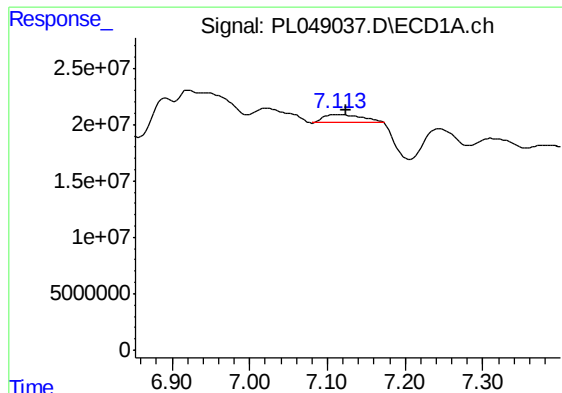

#22 Mirex


R.T.: 7.114 min
Delta R.T.: -0.010 min
Response: 23843703
Conc: 2.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

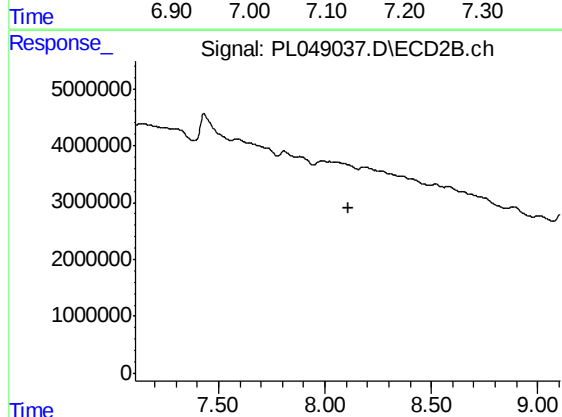


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 8.109 min
Response: 0
Conc: N.D.

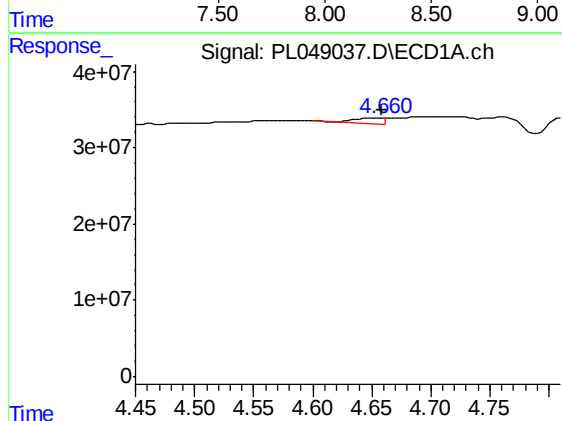


#24 Chlordane-2

R.T.: 4.652 min
Delta R.T.: -0.006 min
Response: 13120462
Conc: 25.36 ng/ml

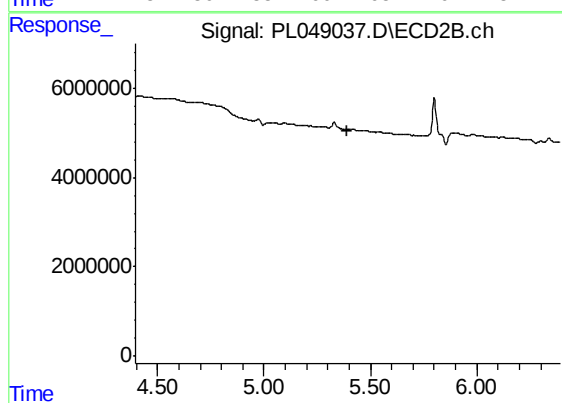

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.394 min
Response: 0
Conc: N.D.

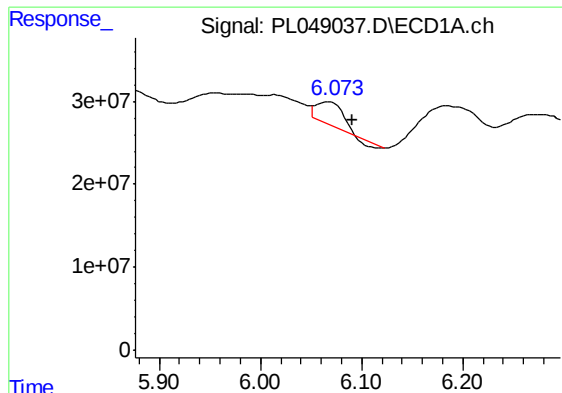

#27 Chlordane-5


R.T.: 6.068 min
Delta R.T.: -0.023 min
Response: 48536482
Conc: 103.37 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

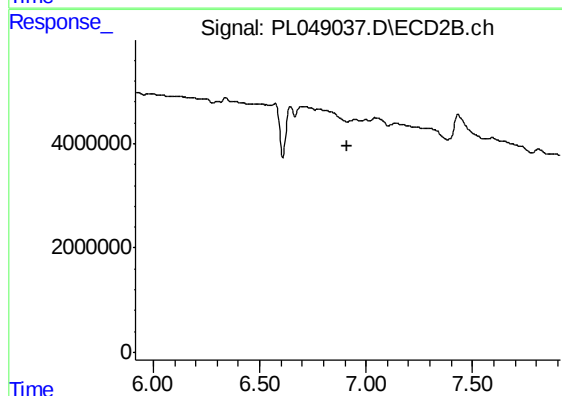


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.913 min
Response: 0
Conc: N.D.

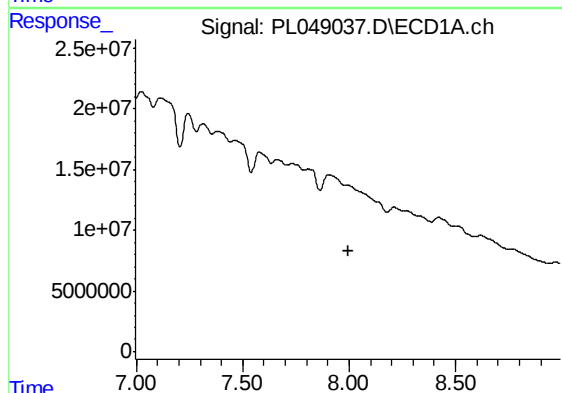

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.996 min
Response: 0
Conc: N.D.

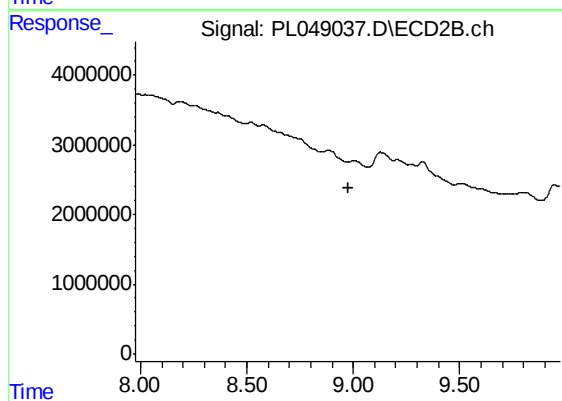

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.975 min
Response: 0
Conc: N.D.