

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052919\
 Data File : PL049045.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 May 2019 14:48
 Operator : SM\AJ
 Sample : K3075-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TEST-PIT-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 30 01:09:14 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
 Quant Title : GC Extractables
 QLast Update : Thu May 02 09:36:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.324	3.937	206.7E6	57397802	21.337	23.043
28)	SA Decachlor...	7.993	8.975	161.4E6	47073325	16.053	17.735
Target Compounds							
19)	B Endosulfa...	6.493f	0.000	22460604	0	2.093	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052919\
Data File : PL049045.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 May 2019 14:48
Operator : SM\AJ
Sample : K3075-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TEST-PIT-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 30 01:09:14 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
Quant Title : GC Extractables
QLast Update : Thu May 02 09:36:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

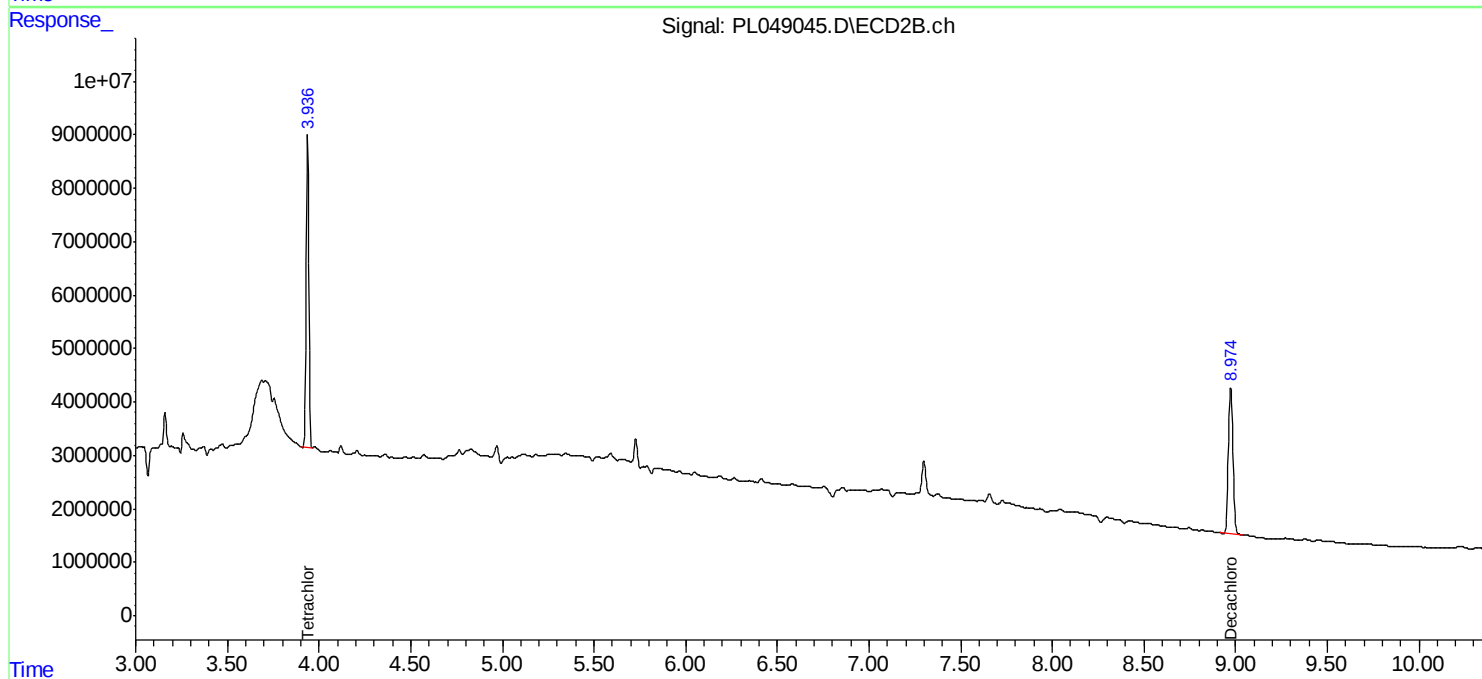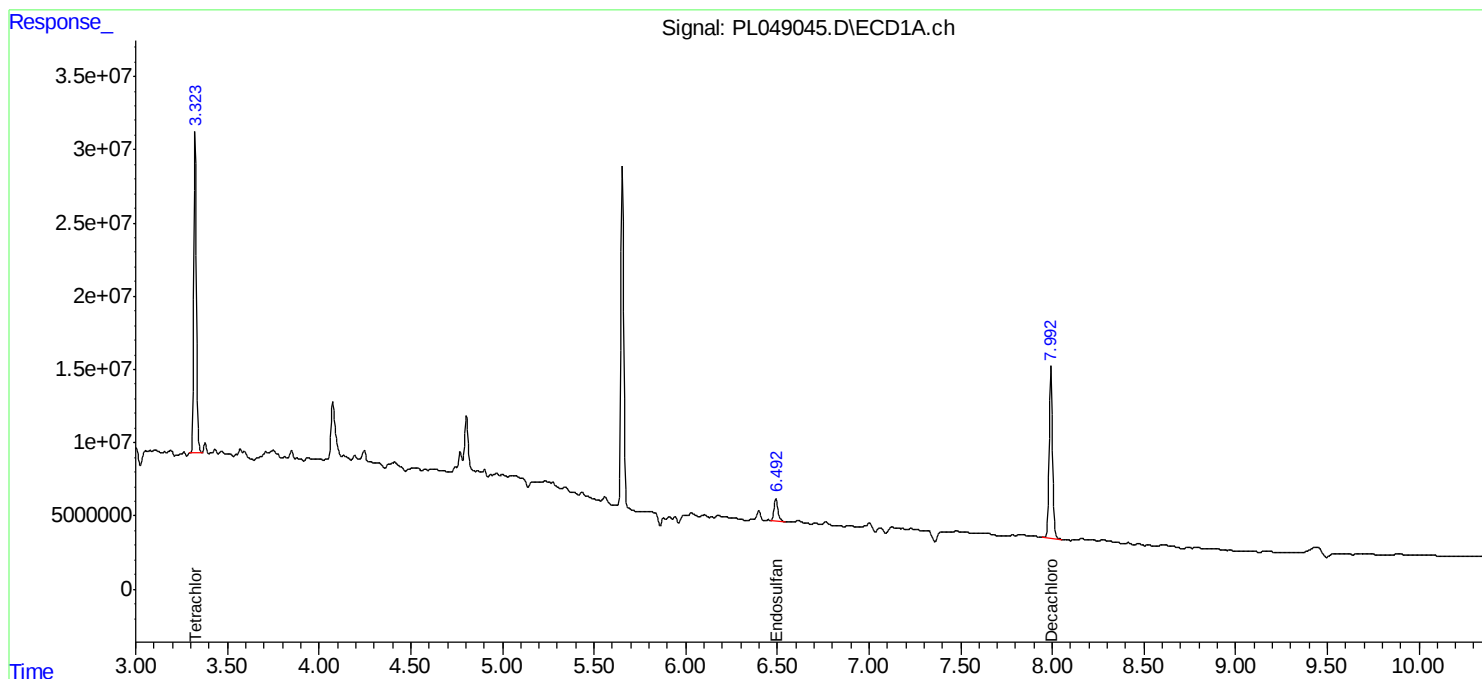


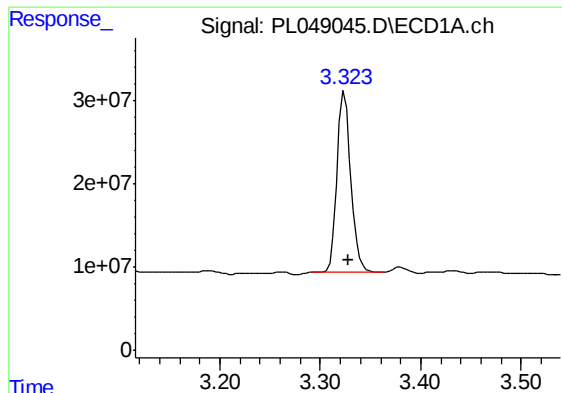

#1 Tetrachloro-m-xylene


R.T.: 3.324 min
Delta R.T.: -0.004 min
Response: 206686535
Conc: 21.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
TEST-PIT-2

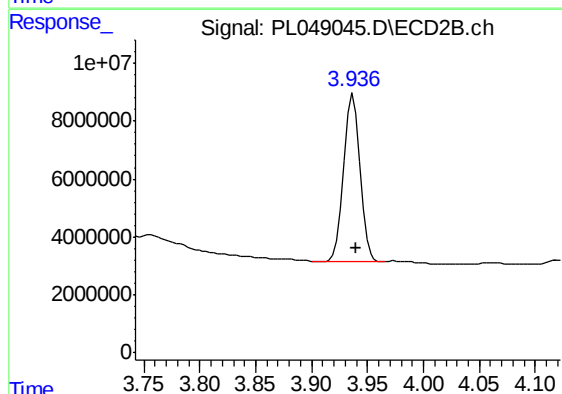


#1 Tetrachloro-m-xylene

R.T.: 3.937 min
Delta R.T.: -0.002 min
Response: 57397802
Conc: 23.04 ng/ml

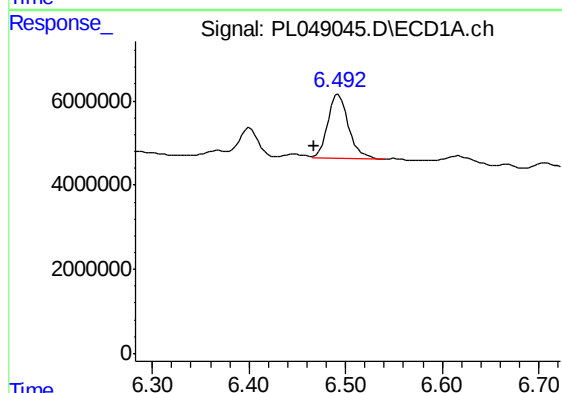


#19 Endosulfan Sulfate

R.T.: 6.493 min
Delta R.T.: 0.025 min
Response: 22460604
Conc: 2.09 ng/ml

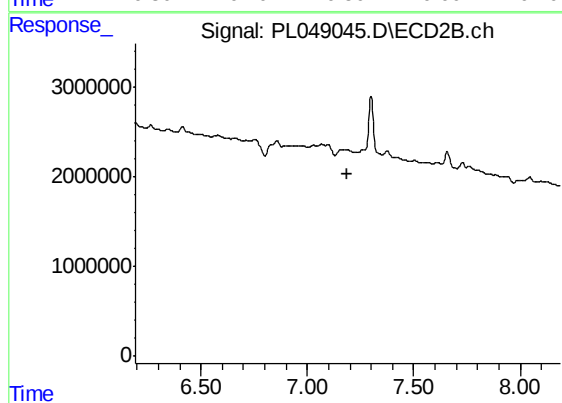

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 7.190 min
Response: 0
Conc: N.D.

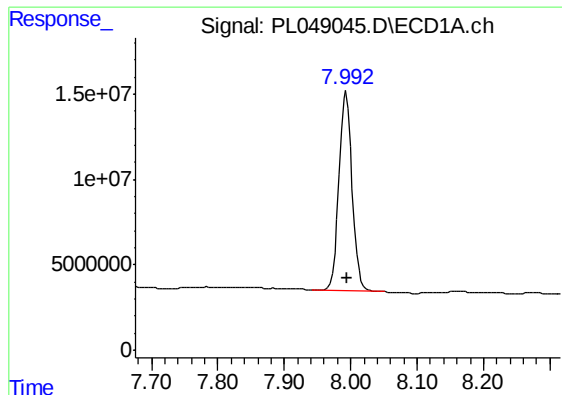

#28 Decachlorobiphenyl

R.T.: 7.993 min
Delta R.T.: -0.003 min
Response: 161404182
Conc: 16.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
TEST-PIT-2

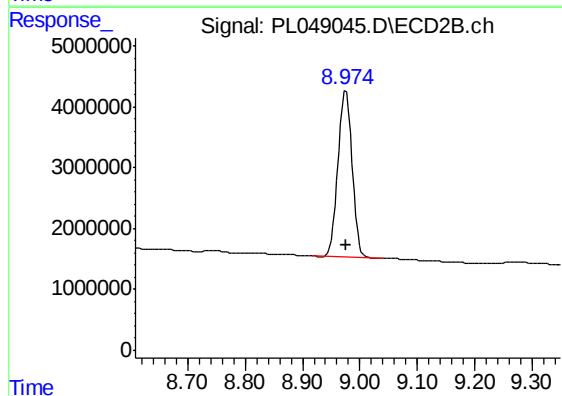

#28 Decachlorobiphenyl

R.T.: 8.975 min
Delta R.T.: 0.000 min
Response: 47073325
Conc: 17.73 ng/ml