

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052919\
 Data File : PL049063.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 May 2019 19:24
 Operator : SM\AJ
 Sample : K3075-01
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TEST-PIT-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 30 01:12:49 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
 Quant Title : GC Extractables
 QLast Update : Thu May 02 09:36:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.324	3.937	187.4E6	50857924	19.343	20.418
28) SA Decachlor...	7.992	8.974	93749244	26822150	9.324	10.105
Target Compounds						
16) A 4,4'-DDD	5.977f	0.000	7189288	0	0.739	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052919\
Data File : PL049063.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 May 2019 19:24
Operator : SM\AJ
Sample : K3075-01
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TEST-PIT-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 30 01:12:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
Quant Title : GC Extractables
QLast Update : Thu May 02 09:36:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

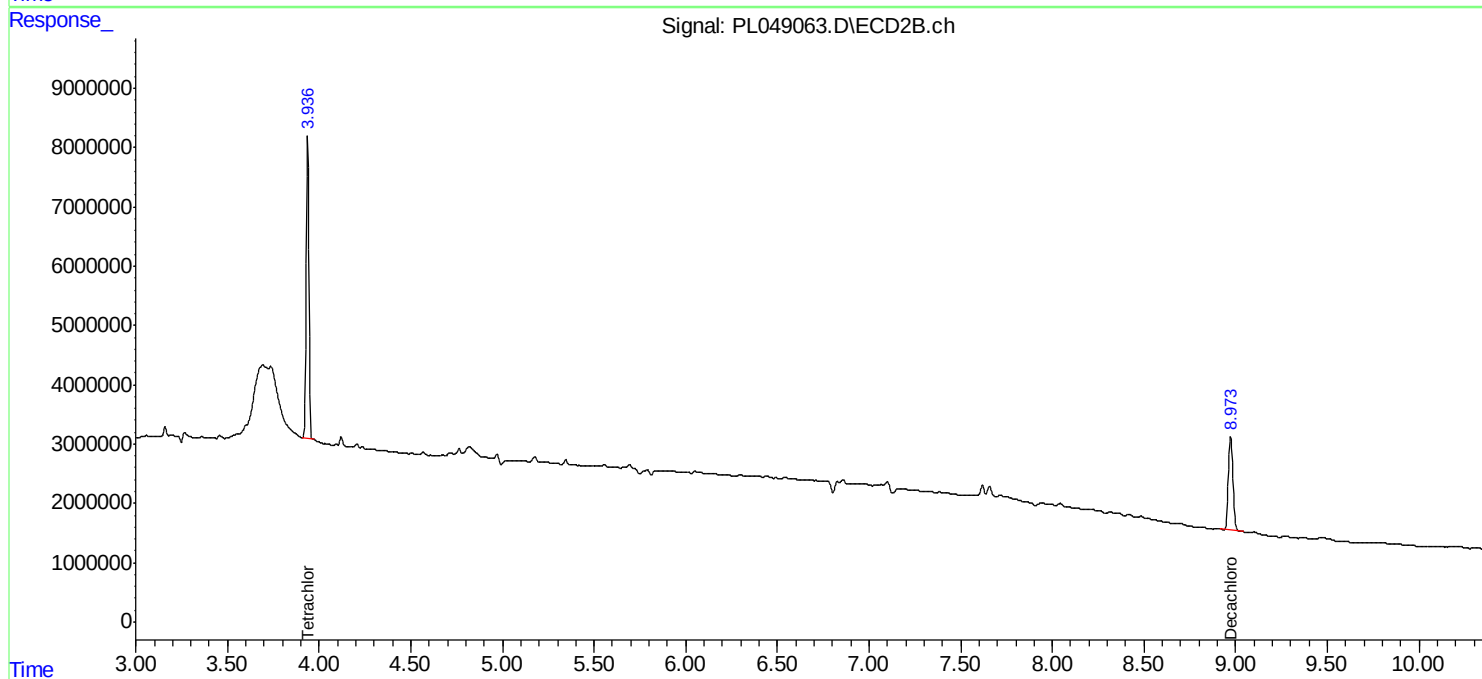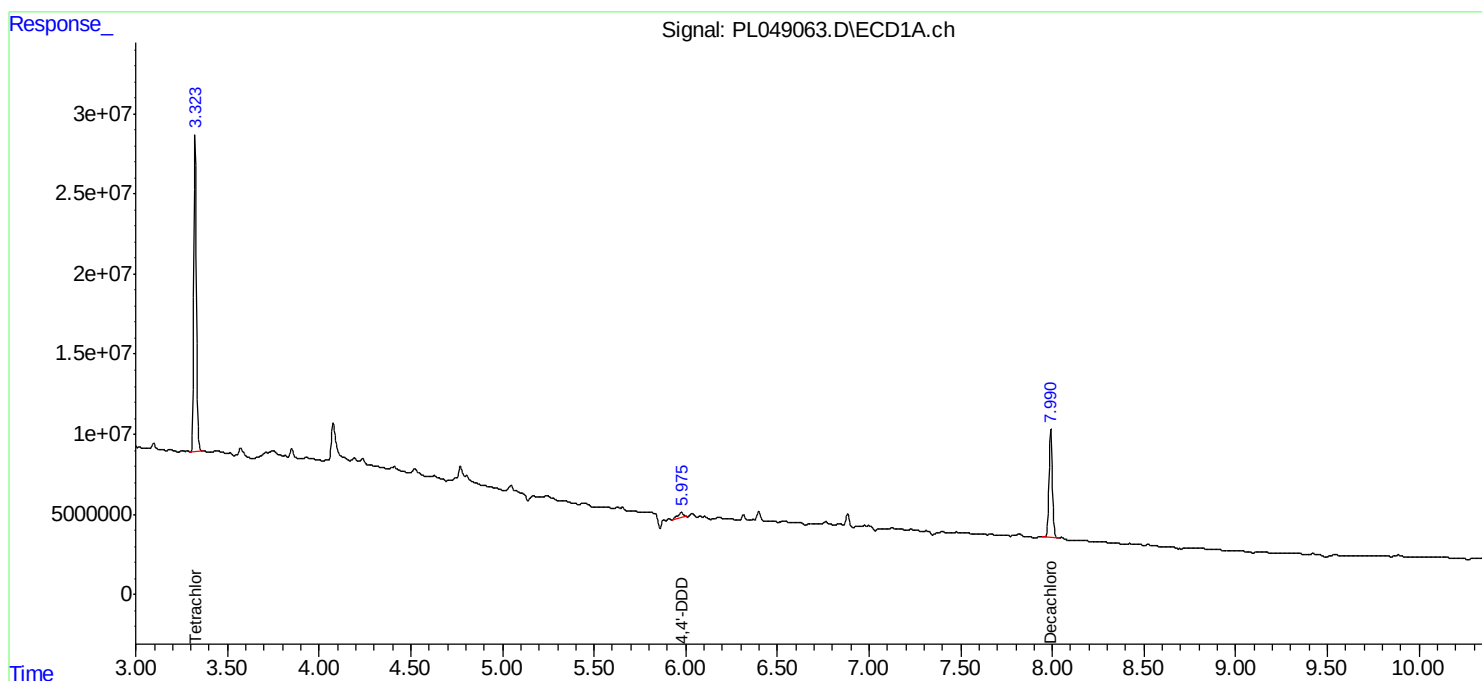


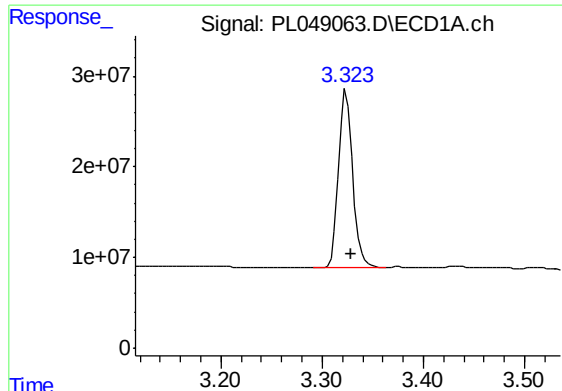

#1 Tetrachloro-m-xylene


R.T.: 3.324 min
Delta R.T.: -0.004 min
Response: 187372058
Conc: 19.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
TEST-PIT-1

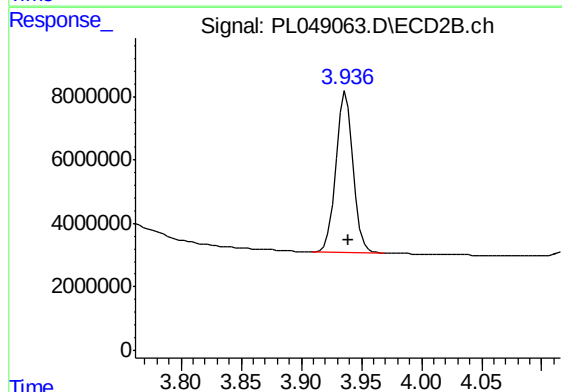


#1 Tetrachloro-m-xylene

R.T.: 3.937 min
Delta R.T.: -0.003 min
Response: 50857924
Conc: 20.42 ng/ml

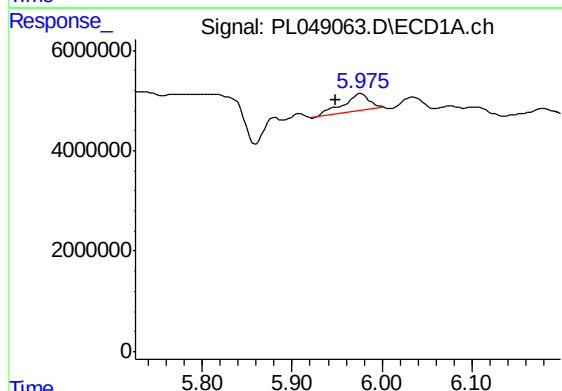


#16 4,4'-DDD

R.T.: 5.977 min
Delta R.T.: 0.027 min
Response: 7189288
Conc: 0.74 ng/ml

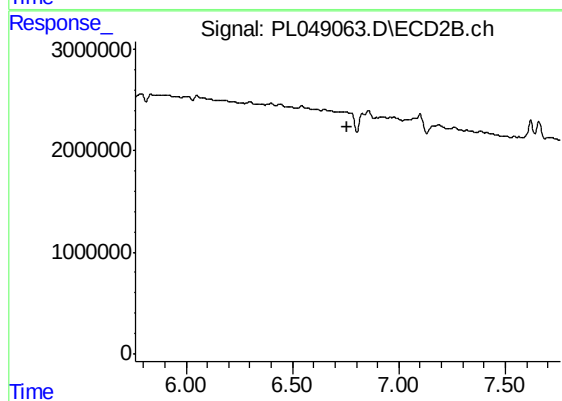

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 6.759 min
Response: 0
Conc: N.D.

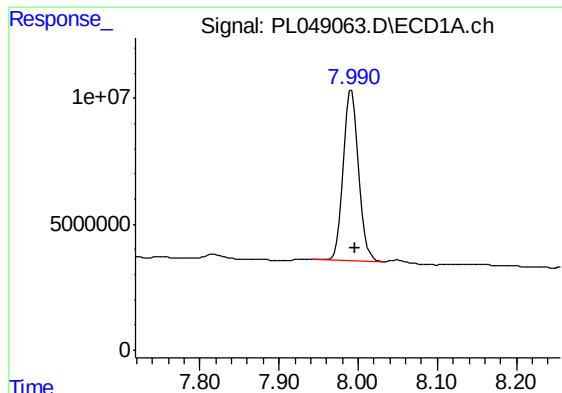

#28 Decachlorobiphenyl

R.T.: 7.992 min
Delta R.T.: -0.004 min
Response: 93749244
Conc: 9.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
TEST-PIT-1

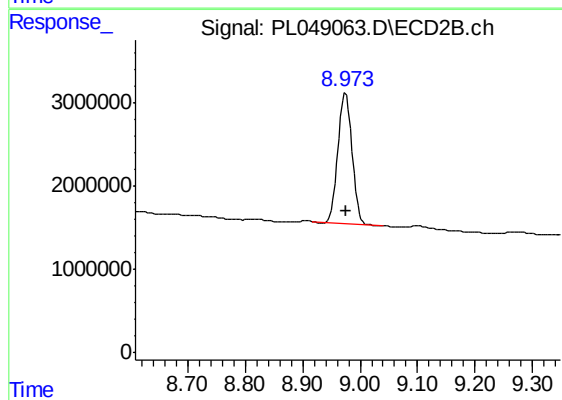

#28 Decachlorobiphenyl

R.T.: 8.974 min
Delta R.T.: 0.000 min
Response: 26822150
Conc: 10.11 ng/ml