

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052919\
 Data File : PL049065.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 May 2019 19:52
 Operator : SM\AJ
 Sample : K3075-07
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TEST-PIT-4

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 30 01:13:09 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
 Quant Title : GC Extractables
 QLast Update : Thu May 02 09:36:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.324	3.937	179.8E6	48566508	18.563	19.498
28)	SA Decachlor...	7.993	8.974	116.7E6	33182592	11.605	12.501
Target Compounds							
15)	B Endosulfa...	0.000	6.861f	0	987983	N.D.	0.366 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052919\
Data File : PL049065.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 May 2019 19:52
Operator : SM\AJ
Sample : K3075-07
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TEST-PIT-4

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 30 01:13:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
Quant Title : GC Extractables
QLast Update : Thu May 02 09:36:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

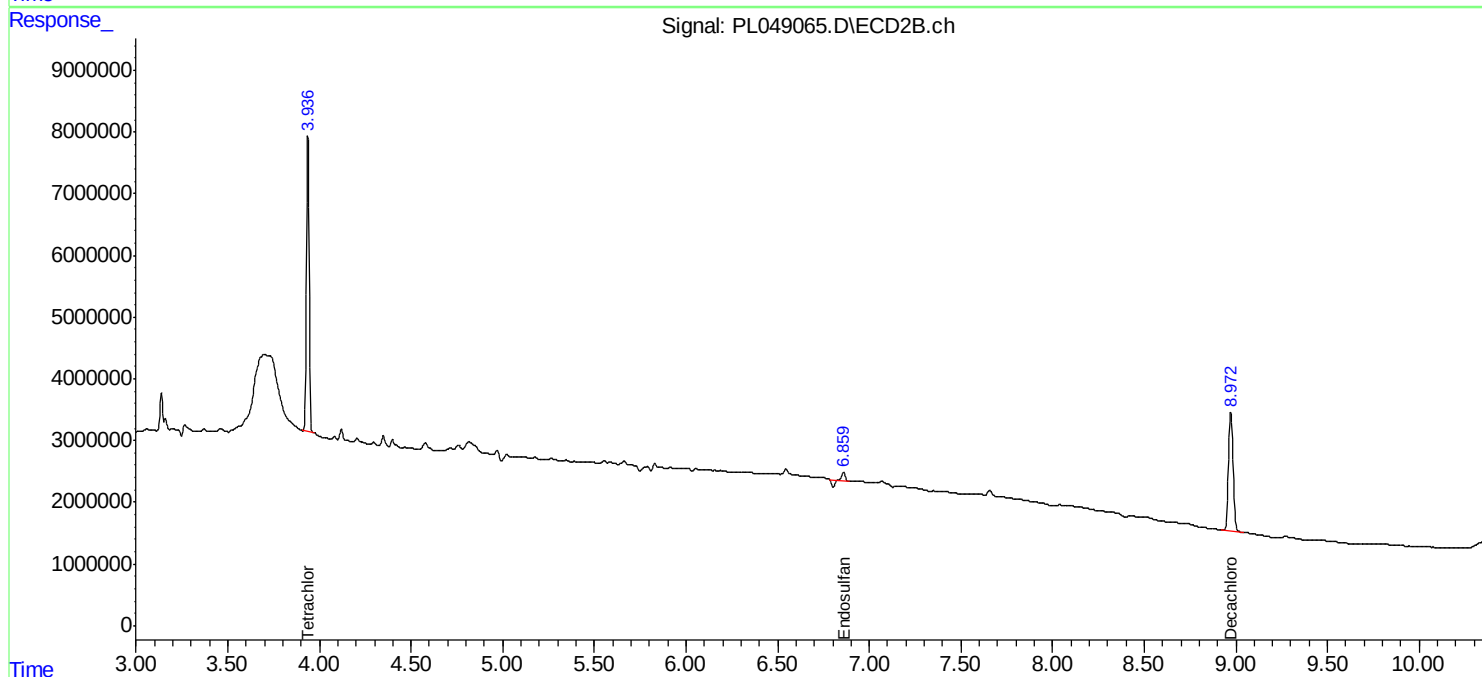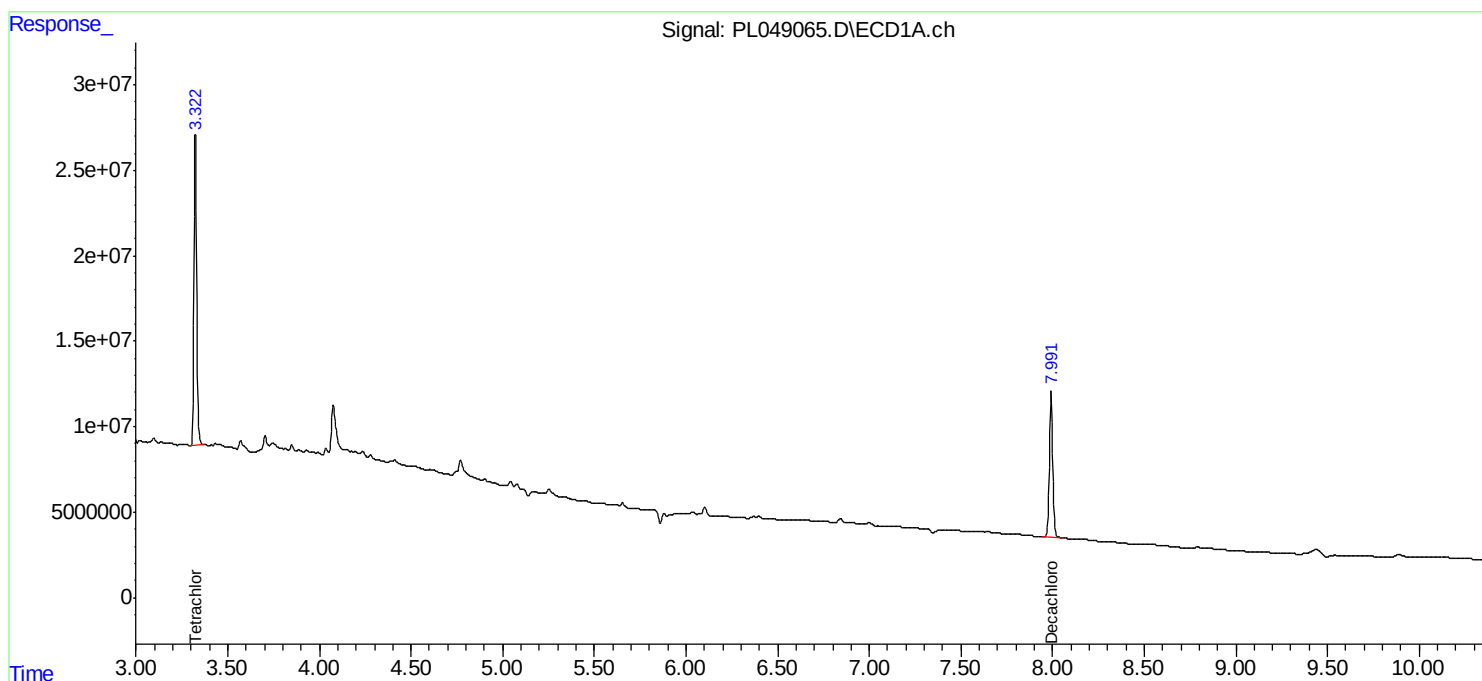


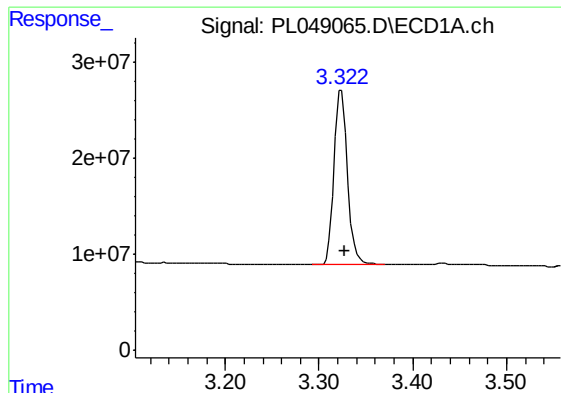

#1 Tetrachloro-m-xylene


R.T.: 3.324 min
Delta R.T.: -0.004 min
Response: 179820949
Conc: 18.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
TEST-PIT-4

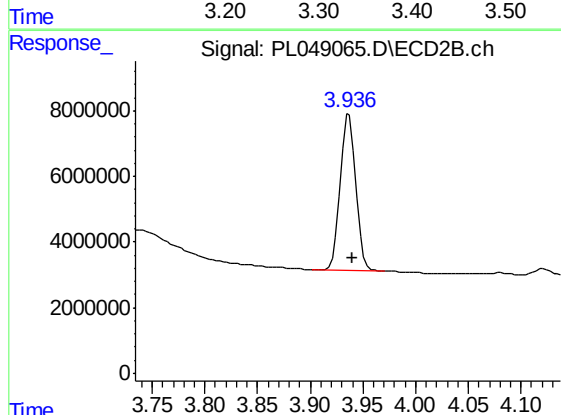


#1 Tetrachloro-m-xylene

R.T.: 3.937 min
Delta R.T.: -0.003 min
Response: 48566508
Conc: 19.50 ng/ml

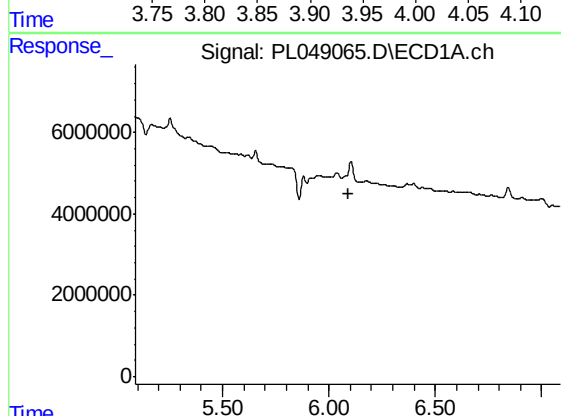


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.089 min
Response: 0
Conc: N.D.

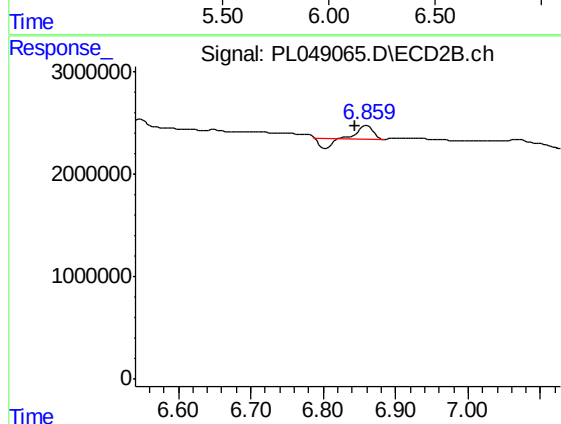

#15 Endosulfan II


R.T.: 6.861 min
Delta R.T.: 0.018 min
Response: 987983
Conc: 0.37 ng/ml

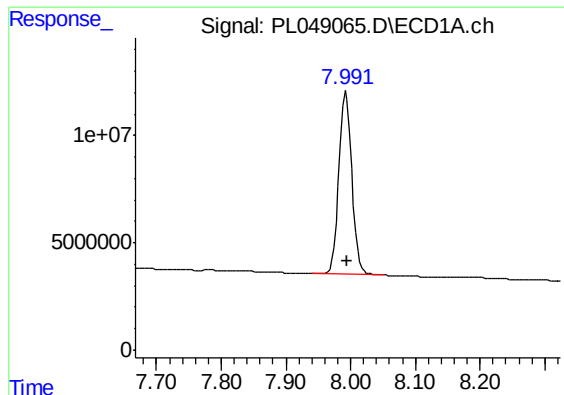

#28 Decachlorobiphenyl

R.T.: 7.993 min
Delta R.T.: -0.003 min
Response: 116673787
Conc: 11.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
TEST-PIT-4

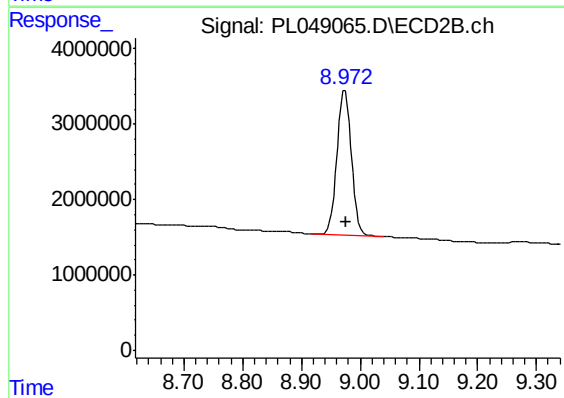

#28 Decachlorobiphenyl

R.T.: 8.974 min
Delta R.T.: -0.001 min
Response: 33182592
Conc: 12.50 ng/ml