

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052919\
 Data File : PL049075.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 May 2019 22:30
 Operator : SM\AJ
 Sample : K3041-13
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 30 01:15:33 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
 Quant Title : GC Extractables
 QLast Update : Thu May 02 09:36:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.325	3.937	166.4E6	51555993	17.177	20.698
28)	SA Decachlor...	7.993	8.974	191.5E6	54831371	19.043	20.658
Target Compounds							
2)	A alpha-BHC	3.763	0.000	59183193	0	3.826	N.D. #
3)	MA gamma-BHC...	4.038	0.000	17705500	0	1.246	N.D. #
5)	MB Aldrin	4.552	0.000	16873390	0	1.231	N.D. #
7)	B delta-BHC	0.000	4.973f	0	5413792	N.D.	1.914 #
9)	A Endosulfan I	5.349f	0.000	6538752	0	0.544	N.D. #
15)	B Endosulfa...	6.074f	0.000	8299621	0	0.719	N.D. #
23)	Chlordane-1	0.000	4.897f	0	10695613	N.D.	87.563 #
27)	Chlordane-5	6.074f	0.000	8299621	0	17.675	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052919\
Data File : PL049075.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 May 2019 22:30
Operator : SM\AJ
Sample : K3041-13
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 30 01:15:33 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
Quant Title : GC Extractables
QLast Update : Thu May 02 09:36:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

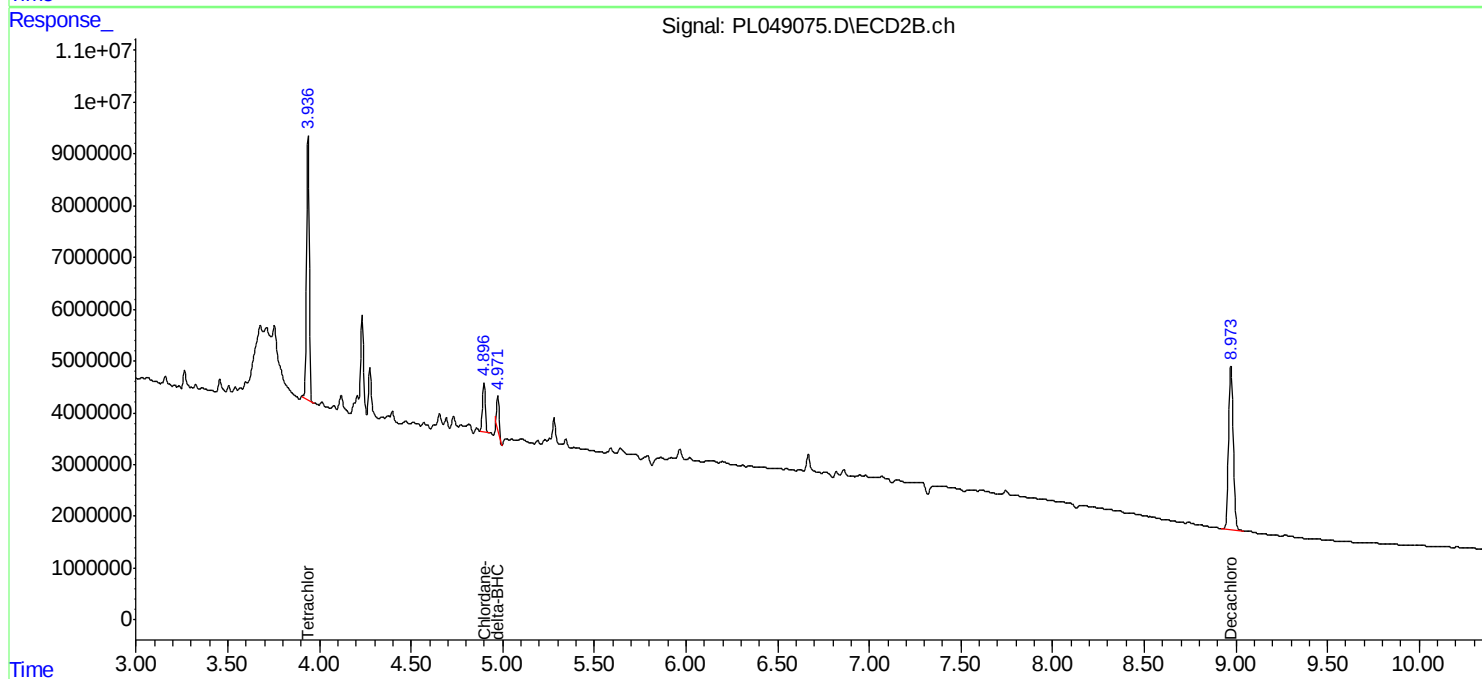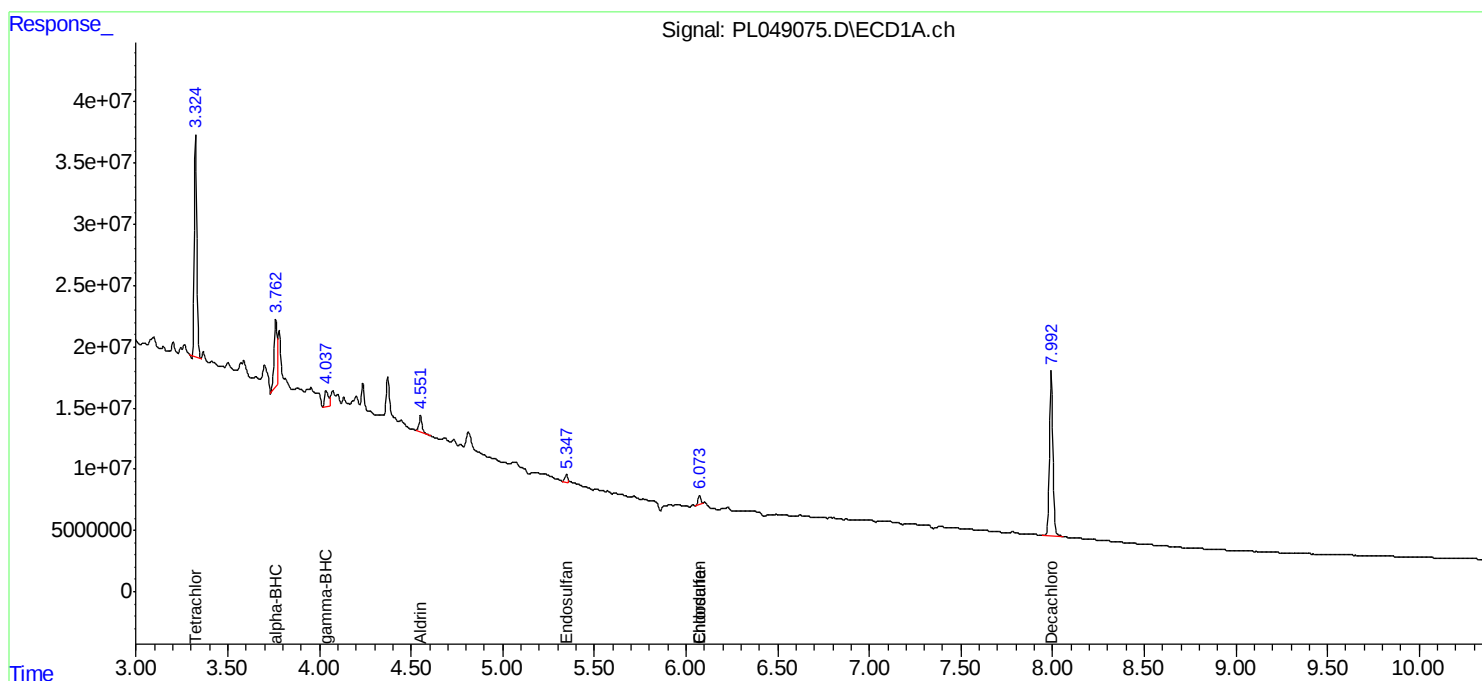


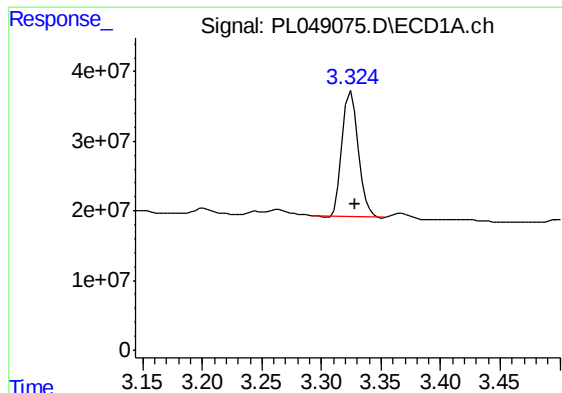

#1 Tetrachloro-m-xylene


R.T.: 3.325 min
Delta R.T.: -0.003 min
Response: 166391620
Conc: 17.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-2

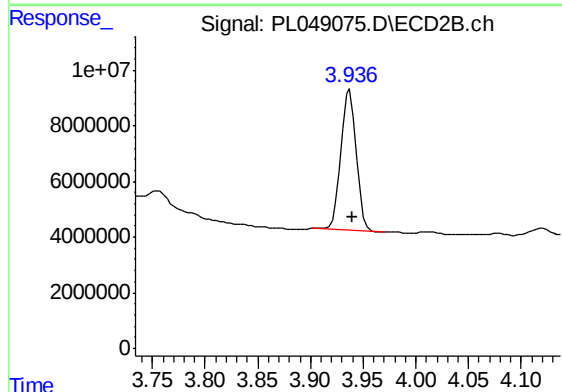


#1 Tetrachloro-m-xylene

R.T.: 3.937 min
Delta R.T.: -0.002 min
Response: 51555993
Conc: 20.70 ng/ml

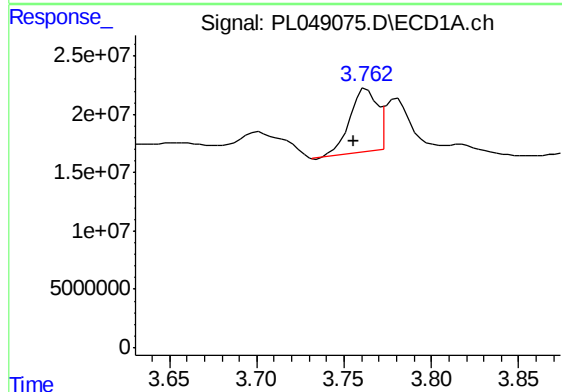


#2 alpha-BHC

R.T.: 3.763 min
Delta R.T.: 0.007 min
Response: 59183193
Conc: 3.83 ng/ml

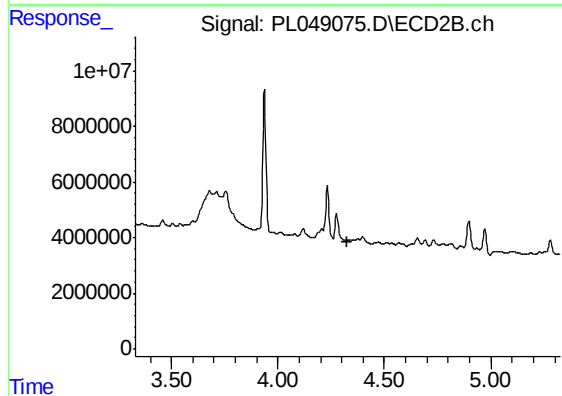

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.328 min
Response: 0
Conc: N.D.

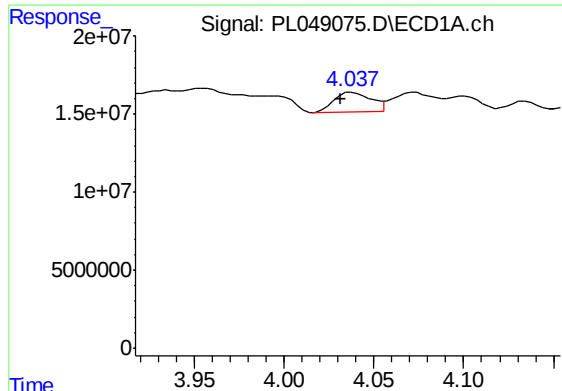

#3 gamma-BHC (Lindane)


R.T.: 4.038 min
Delta R.T.: 0.006 min
Response: 17705500
Conc: 1.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-2

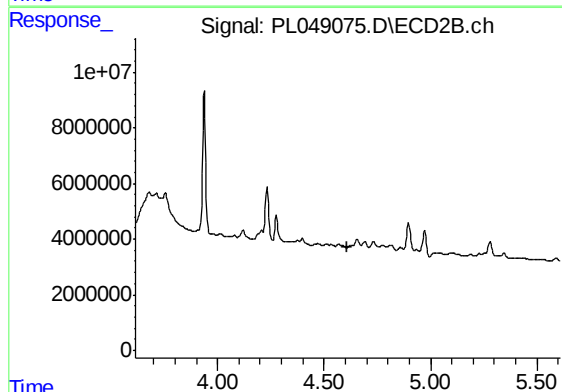


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.612 min
Response: 0
Conc: N.D.

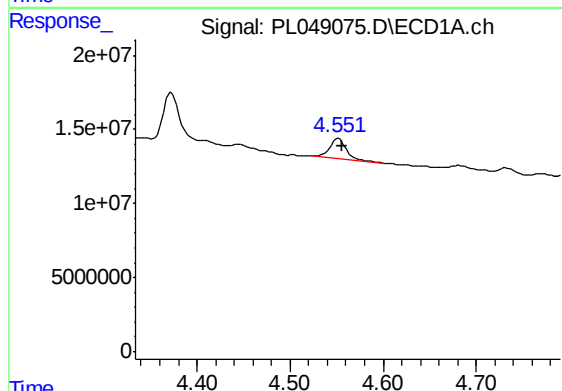


#5 Aldrin

R.T.: 4.552 min
Delta R.T.: -0.003 min
Response: 16873390
Conc: 1.23 ng/ml

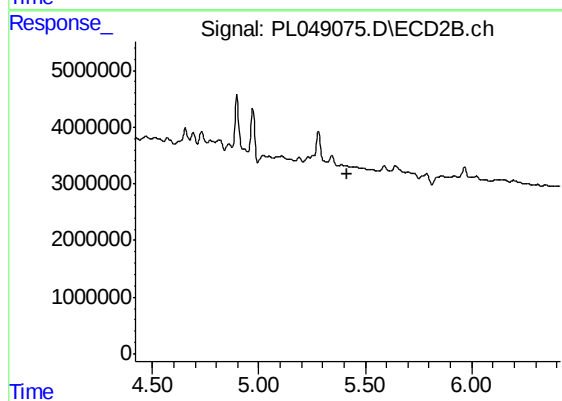

#5 Aldrin


R.T.: 0.000 min
Exp R.T. : 5.418 min
Response: 0
Conc: N.D.

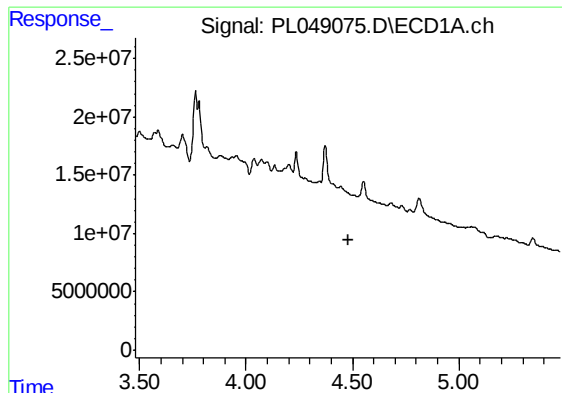

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.479 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-2

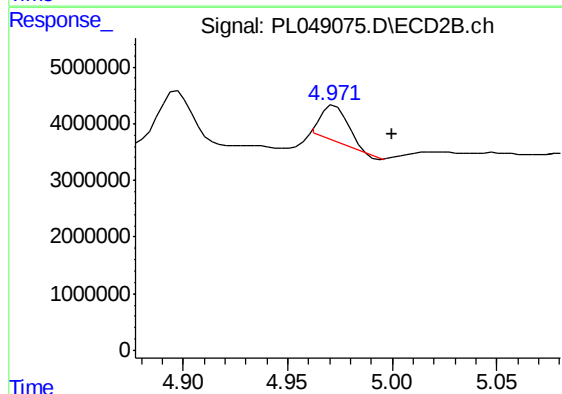


#7 delta-BHC

R.T.: 4.973 min
Delta R.T.: -0.028 min
Response: 5413792
Conc: 1.91 ng/ml

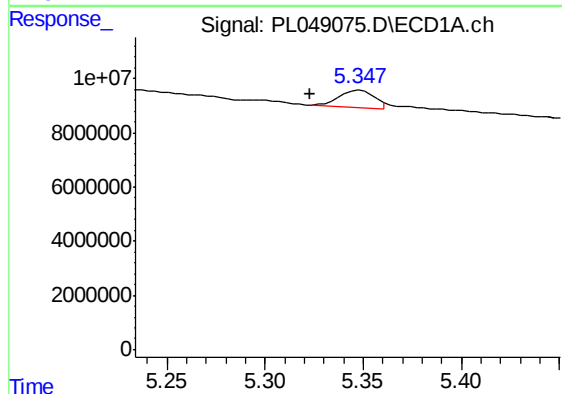


#9 Endosulfan I

R.T.: 5.349 min
Delta R.T.: 0.026 min
Response: 6538752
Conc: 0.54 ng/ml

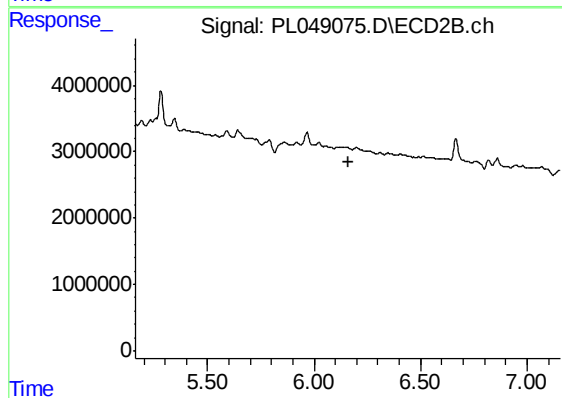

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.159 min
Response: 0
Conc: N.D.

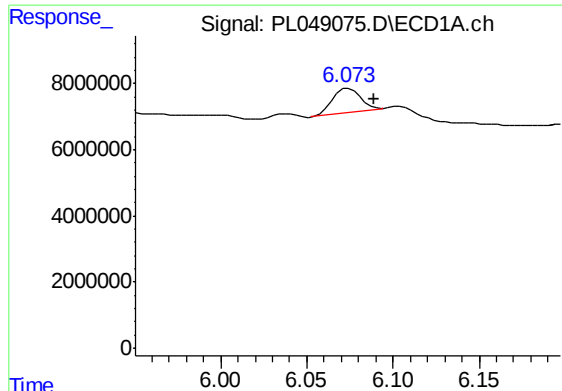

#15 Endosulfan II


R.T.: 6.074 min
Delta R.T.: -0.015 min
Response: 8299621
Conc: 0.72 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-2

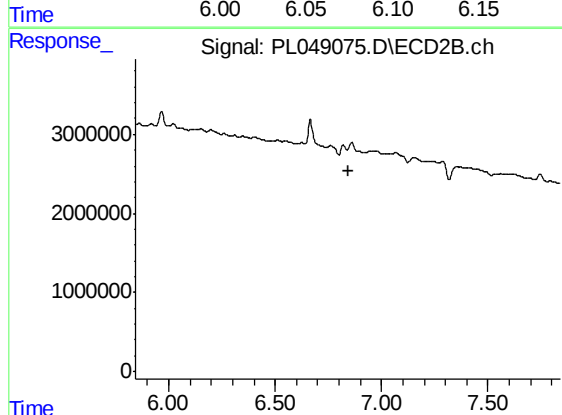


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.843 min
Response: 0
Conc: N.D.

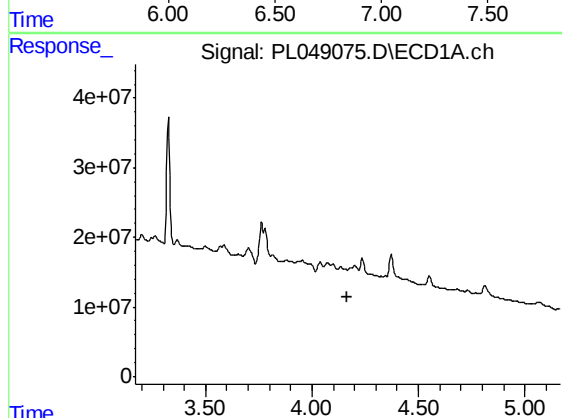


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.168 min
Response: 0
Conc: N.D.

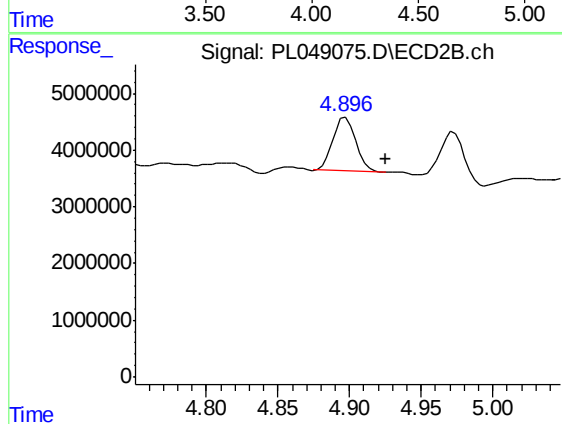

#23 Chlordane-1


R.T.: 4.897 min
Delta R.T.: -0.028 min
Response: 10695613
Conc: 87.56 ng/ml

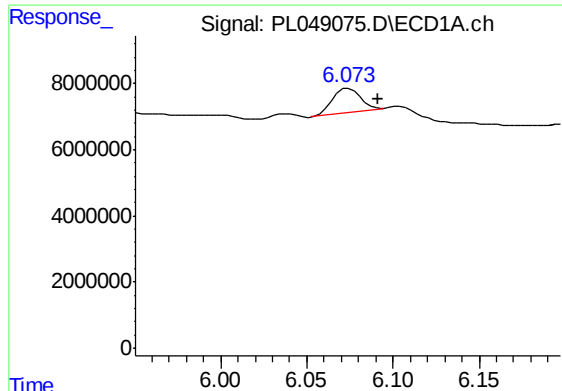

#27 Chlordane-5


R.T.: 6.074 min
Delta R.T.: -0.017 min
Response: 8299621
Conc: 17.68 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-2

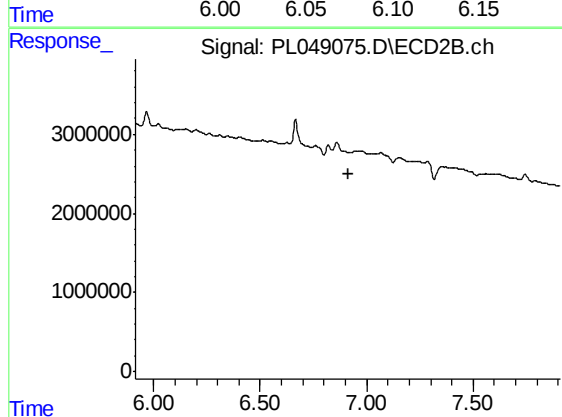


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.913 min
Response: 0
Conc: N.D.

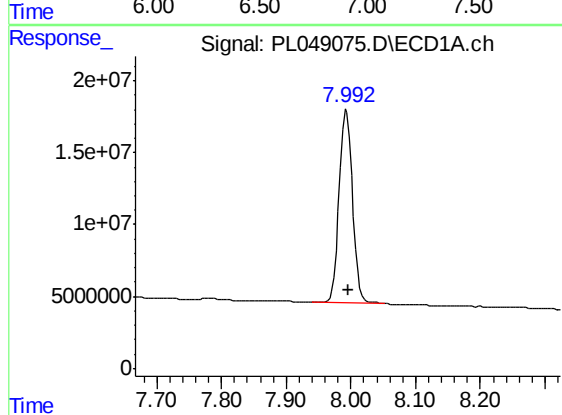

#28 Decachlorobiphenyl

R.T.: 7.993 min
Delta R.T.: -0.003 min
Response: 191461075
Conc: 19.04 ng/ml

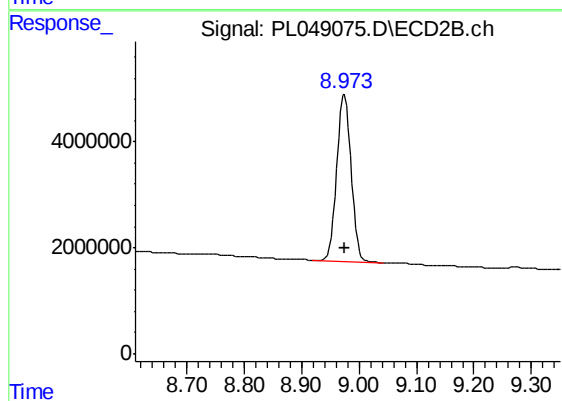

#28 Decachlorobiphenyl

R.T.: 8.974 min
Delta R.T.: 0.000 min
Response: 54831371
Conc: 20.66 ng/ml