

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052920\
 Data File : PL058985.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 May 2020 13:13
 Operator : AJ\MA
 Sample : L2790-07
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 29 15:36:25 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052020.M
 Quant Title : GC Extractables
 QLast Update : Wed May 20 11:27:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.529	4.077	25891298	36658252	14.120	13.535
28)	SA Decachlor...	8.309	9.189	23267513	33203617	13.771	12.595
Target Compounds							
2)	A alpha-BHC	3.986	0.000	1439317	0	0.529	N.D. #
4)	MA Heptachlor	0.000	5.269	0	322973	N.D.	0.084 #
8)	B Heptachlo...	0.000	5.952	0	196970	N.D.	0.060 #
12)	B 4,4'-DDE	0.000	6.429	0	738765	N.D.	0.259 #
15)	B Endosulfa...	0.000	7.013	0	3254009	N.D.	1.161 #
17)	MA 4,4'-DDT	0.000	7.218	0	84262	N.D.	0.035 #
18)	B Endrin al...	0.000	7.134	0	547147	N.D.	0.232 #
23)	Chlordane-1	0.000	5.058f	0	1250079	N.D.	13.033 #
27)	Chlordane-5	0.000	7.078	0	1442151	N.D.	18.203 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052920\
Data File : PL058985.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 May 2020 13:13
Operator : AJ\MA
Sample : L2790-07
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 29 15:36:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052020.M
Quant Title : GC Extractables
QLast Update : Wed May 20 11:27:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

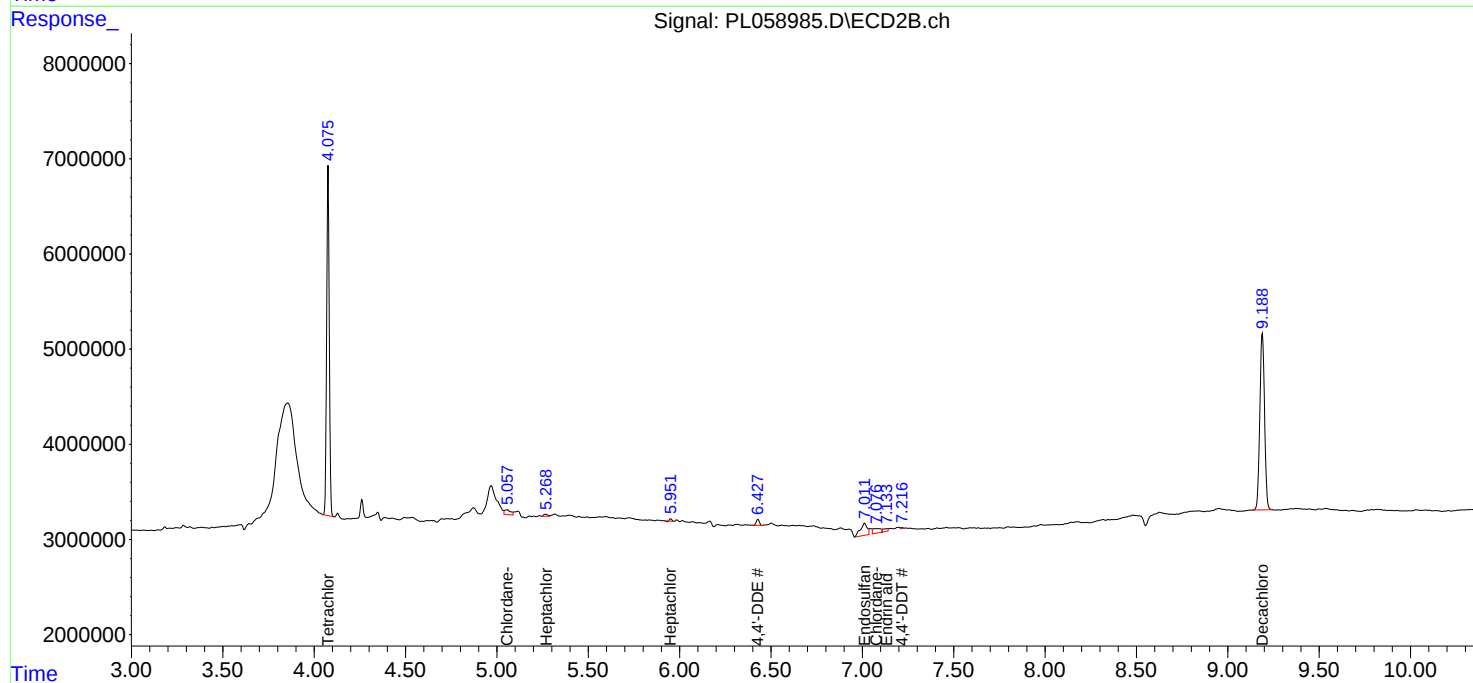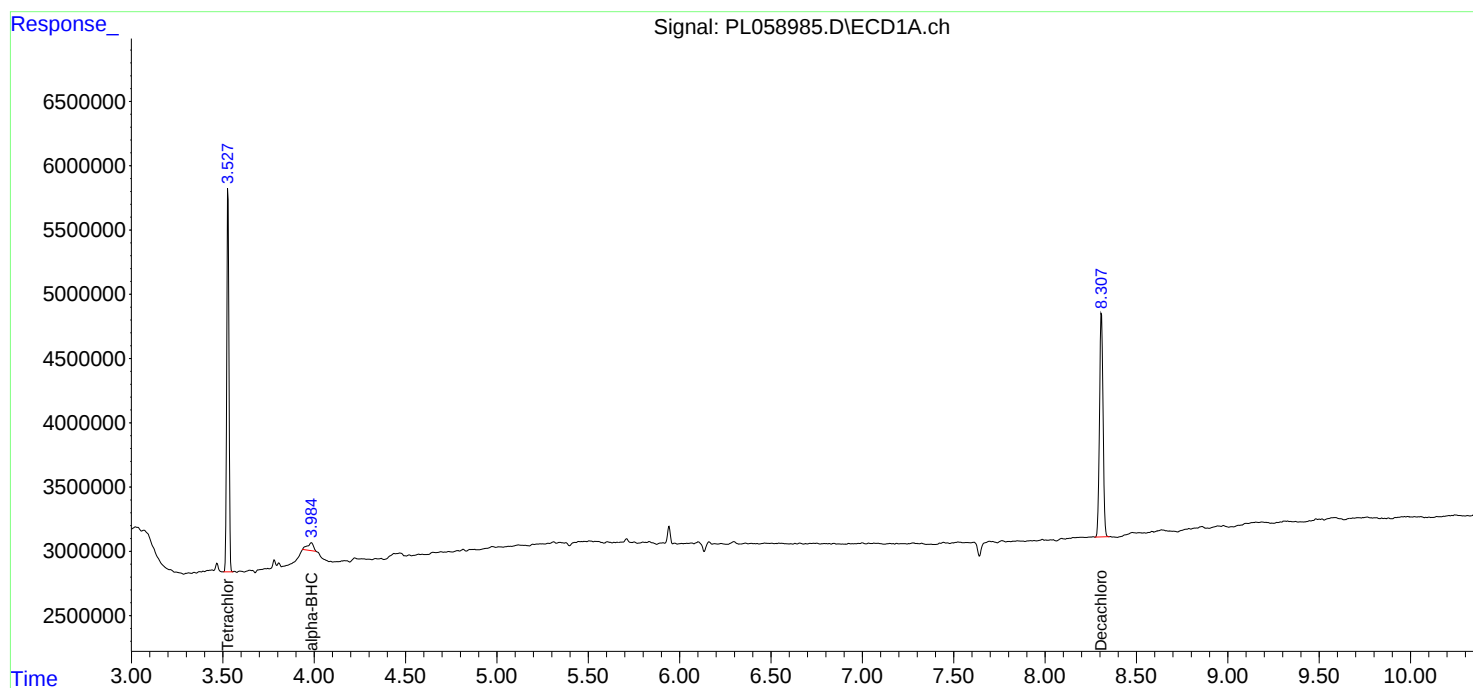


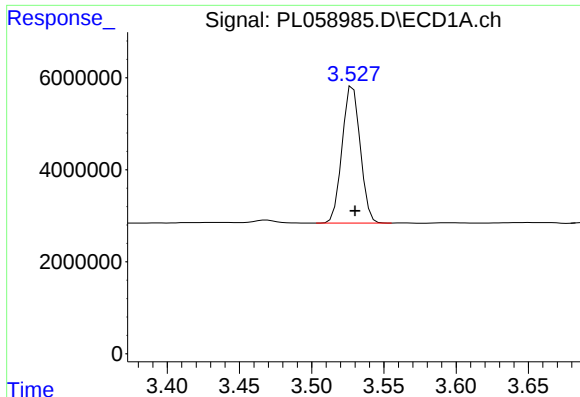

#1 Tetrachloro-m-xylene


R.T.: 3.529 min
Delta R.T.: -0.001 min
Response: 25891298
Conc: 14.12 ng/ml

Instrument :
ECD_L
ClientSampleId :

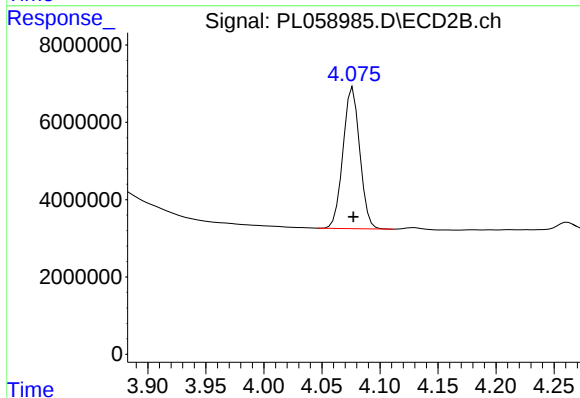


#1 Tetrachloro-m-xylene

R.T.: 4.077 min
Delta R.T.: 0.000 min
Response: 36658252
Conc: 13.53 ng/ml

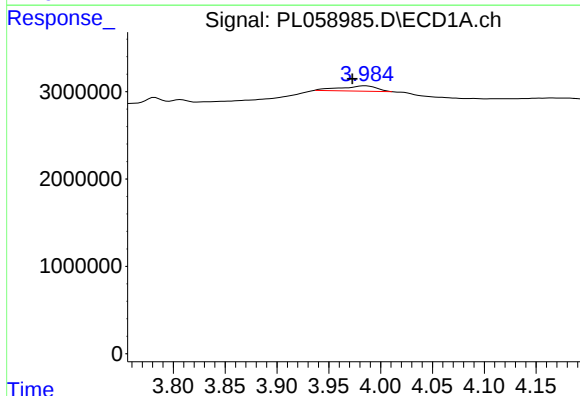


#2 alpha-BHC

R.T.: 3.986 min
Delta R.T.: 0.013 min
Response: 1439317
Conc: 0.53 ng/ml

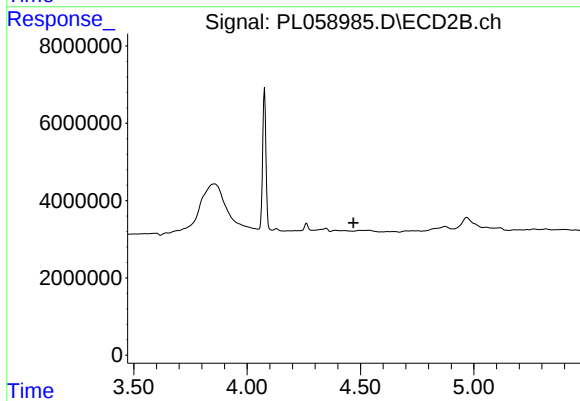

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.469 min
Response: 0
Conc: N.D.

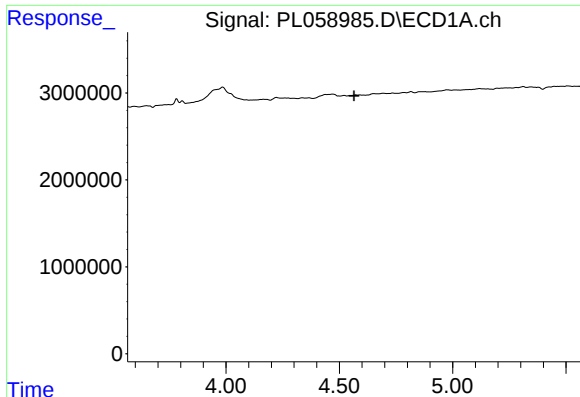

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.566 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

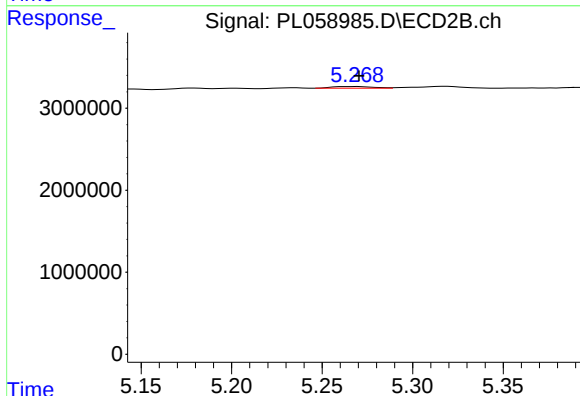


#4 Heptachlor

R.T.: 5.269 min
Delta R.T.: -0.002 min
Response: 322973
Conc: 0.08 ng/ml

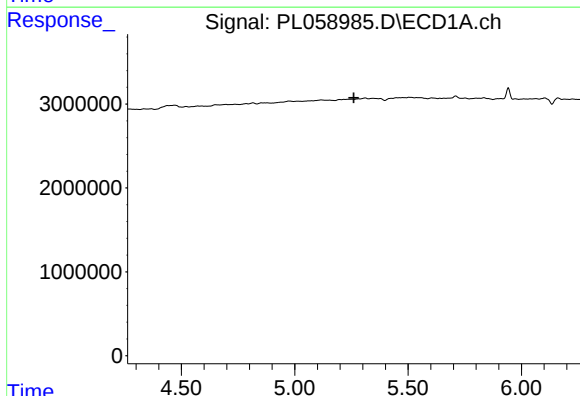


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.261 min
Response: 0
Conc: N.D.

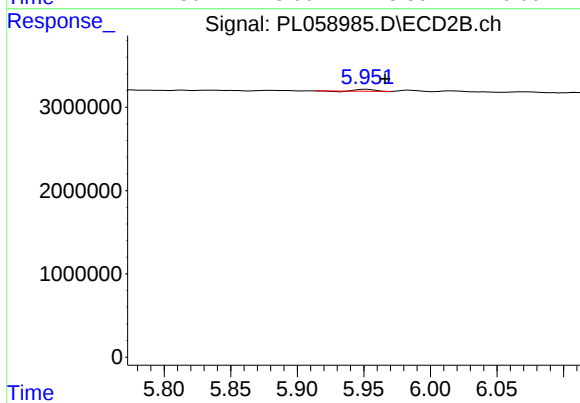

#8 Heptachlor epoxide


R.T.: 5.952 min
Delta R.T.: -0.014 min
Response: 196970
Conc: 0.06 ng/ml

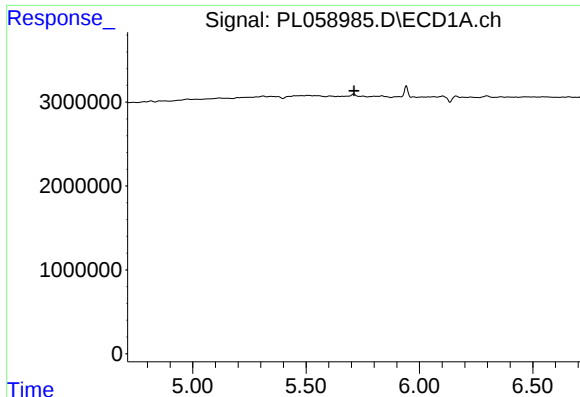

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 5.712 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

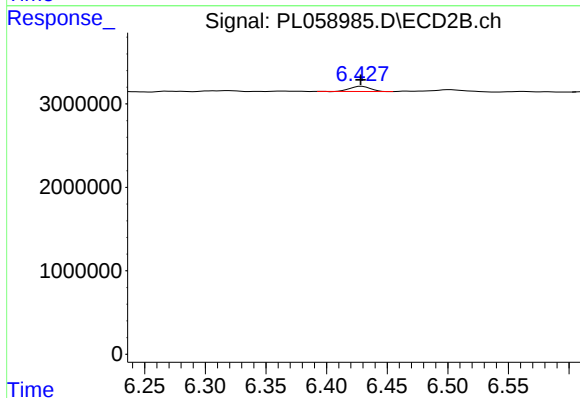


#12 4,4'-DDE

R.T.: 6.429 min
Delta R.T.: 0.000 min
Response: 738765
Conc: 0.26 ng/ml

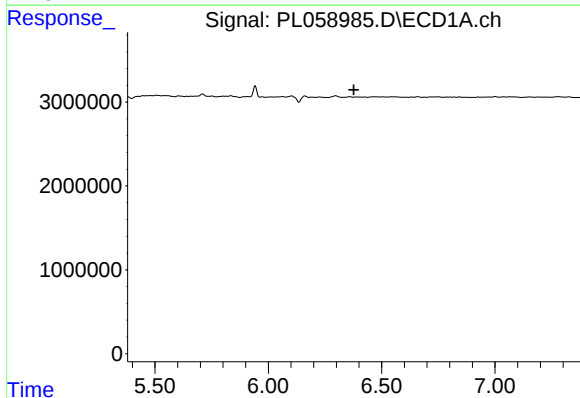


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.377 min
Response: 0
Conc: N.D.

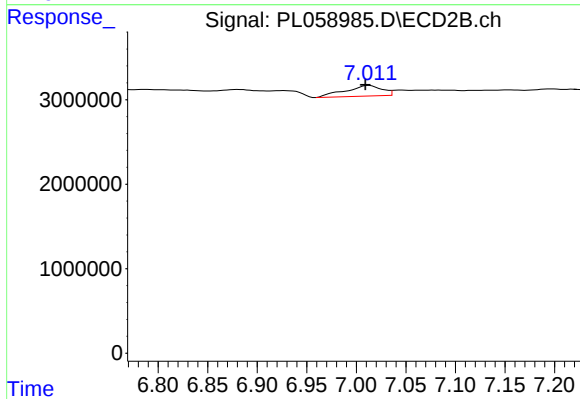

#15 Endosulfan II

R.T.: 7.013 min
Delta R.T.: 0.003 min
Response: 3254009
Conc: 1.16 ng/ml

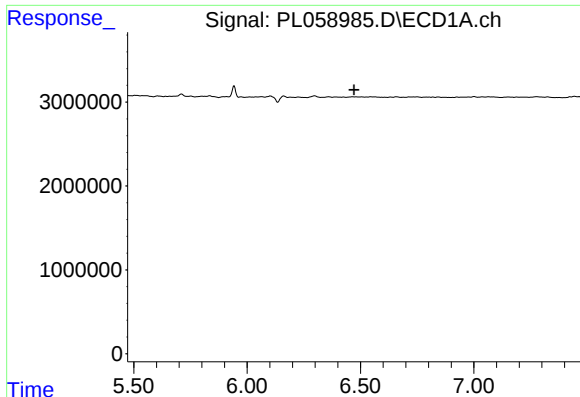

#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 6.471 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

#17 4,4'-DDT


R.T.: 7.218 min
Delta R.T.: 0.000 min
Response: 84262
Conc: 0.04 ng/ml

#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 6.545 min
Response: 0
Conc: N.D.

#18 Endrin aldehyde


R.T.: 7.134 min
Delta R.T.: 0.000 min
Response: 547147
Conc: 0.23 ng/ml

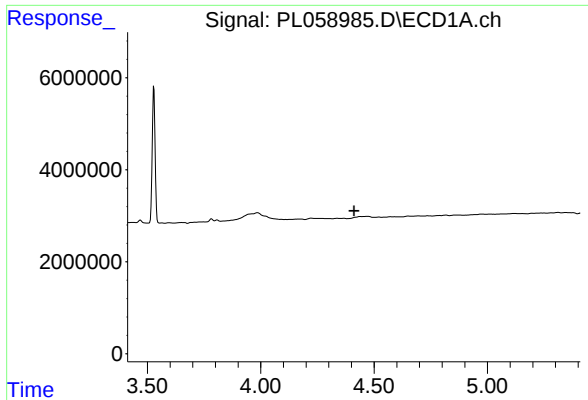

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.412 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

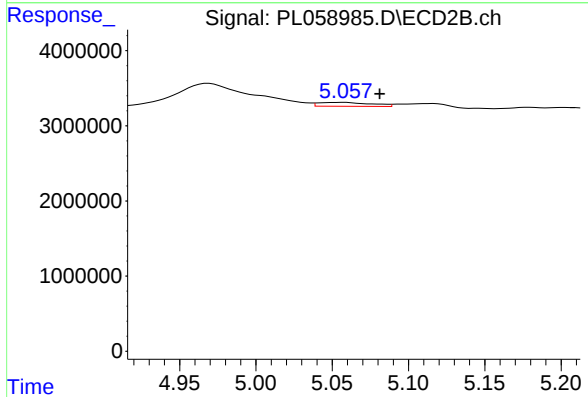


#23 Chlordane-1

R.T.: 5.058 min
Delta R.T.: -0.023 min
Response: 1250079
Conc: 13.03 ng/ml

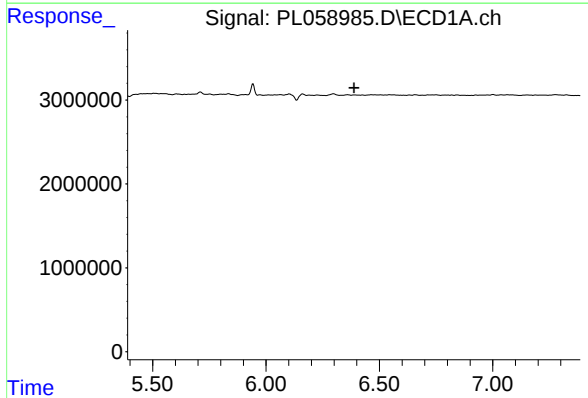


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.389 min
Response: 0
Conc: N.D.

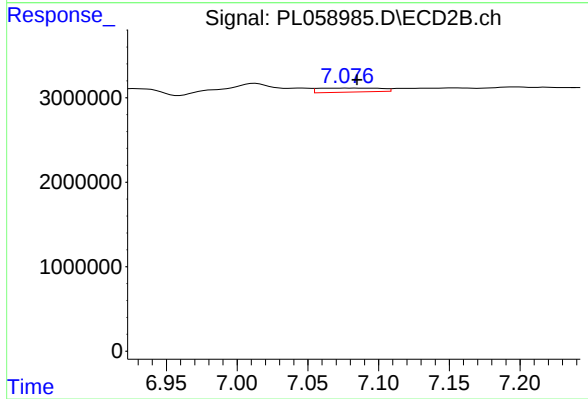

#27 Chlordane-5


R.T.: 7.078 min
Delta R.T.: -0.007 min
Response: 1442151
Conc: 18.20 ng/ml

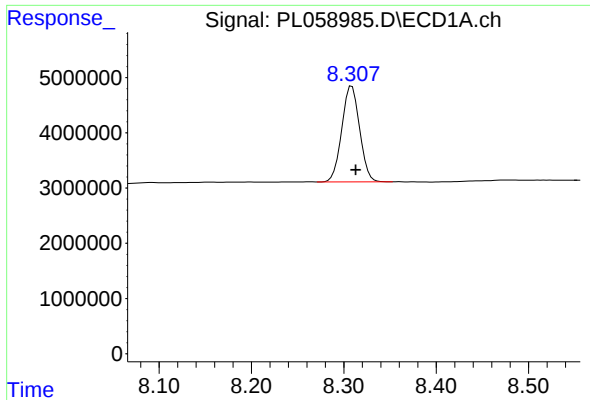

#28 Decachlorobiphenyl

R.T.: 8.309 min
Delta R.T.: -0.004 min
Response: 23267513
Conc: 13.77 ng/ml

Instrument :
ECD_L
ClientSampleId :

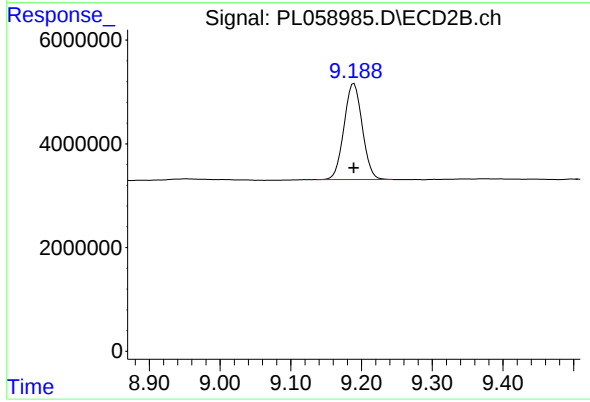

#28 Decachlorobiphenyl

R.T.: 9.189 min
Delta R.T.: 0.000 min
Response: 33203617
Conc: 12.60 ng/ml