

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052920\
 Data File : PL058999.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 May 2020 16:45
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 01 05:39:21 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052020.M
 Quant Title : GC Extractables
 QLast Update : Wed May 20 11:27:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.529	4.077	43763913	60699360	23.867	22.411
28)	SA Decachlor...	8.310	9.191	39197621	55295241	23.200	20.975
Target Compounds							
2)	A alpha-BHC	3.984	0.000	2103725	0	0.774	N.D. #
4)	MA Heptachlor	0.000	5.267	0	947435	N.D.	0.247 #
7)	B delta-BHC	0.000	5.119f	0	1904725	N.D.	0.522 #
8)	B Heptachlo...	0.000	5.958	0	1427961	N.D.	0.433 #
14)	MA Endrin	0.000	6.798	0	1456597	N.D.	0.584 #
15)	B Endosulfa...	0.000	7.012	0	1114183	N.D.	0.397 #
22)	Mirex	0.000	8.313f	0	327576	N.D.	0.149 #
23)	Chlordane-1	4.436f	0.000	735798	0	14.063	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052920\
Data File : PL058999.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 May 2020 16:45
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 01 05:39:21 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052020.M
Quant Title : GC Extractables
QLast Update : Wed May 20 11:27:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

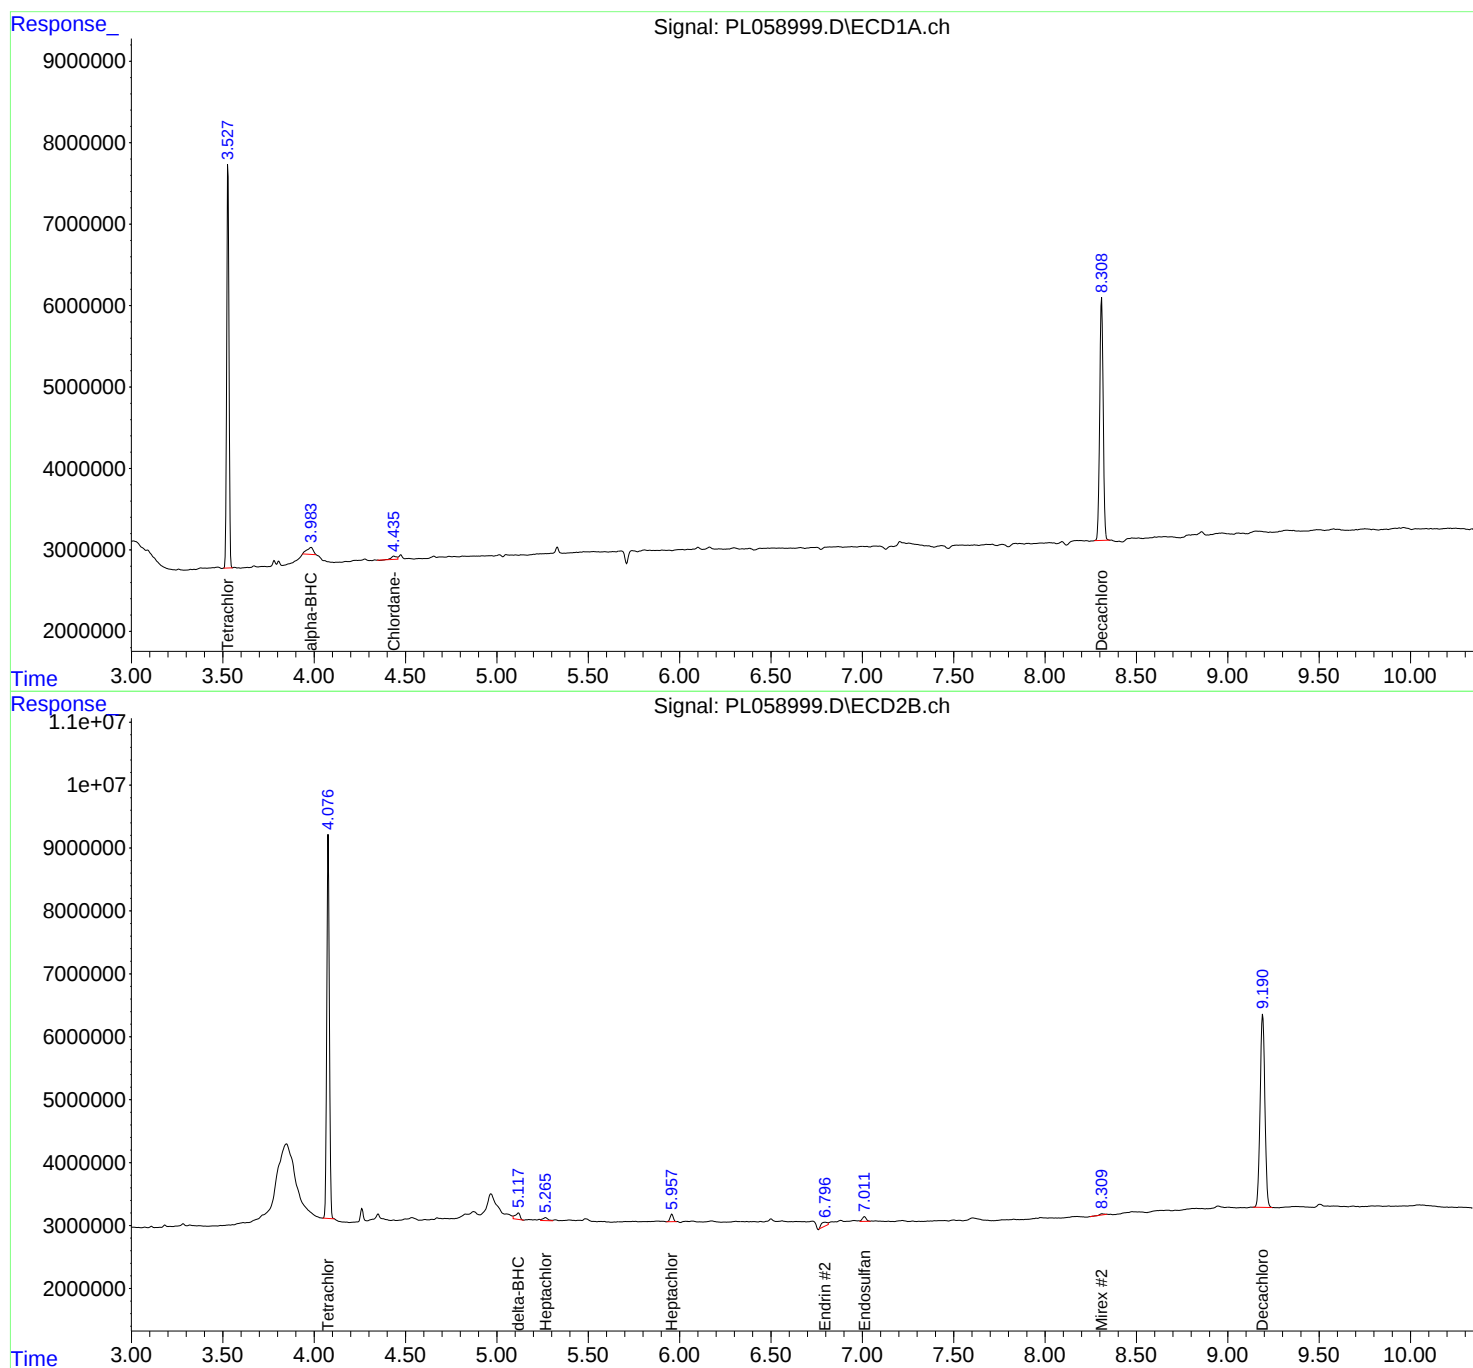


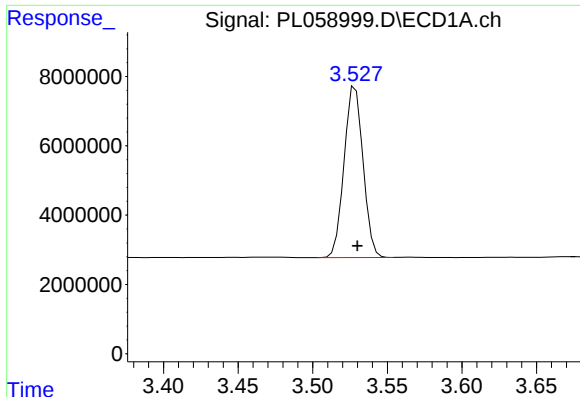

#1 Tetrachloro-m-xylene


R.T.: 3.529 min
Delta R.T.: -0.001 min
Response: 43763913
Conc: 23.87 ng/ml

Instrument :
ECD_L
ClientSampleId :

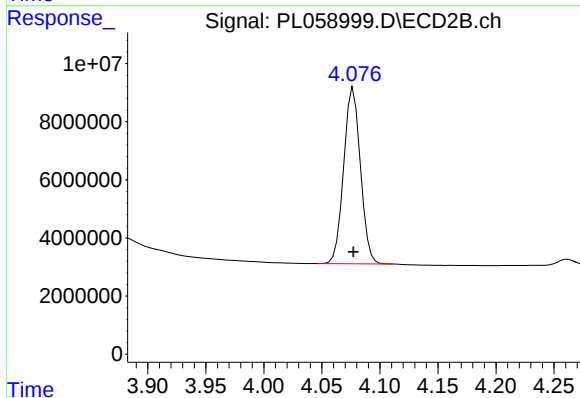


#1 Tetrachloro-m-xylene

R.T.: 4.077 min
Delta R.T.: 0.000 min
Response: 60699360
Conc: 22.41 ng/ml

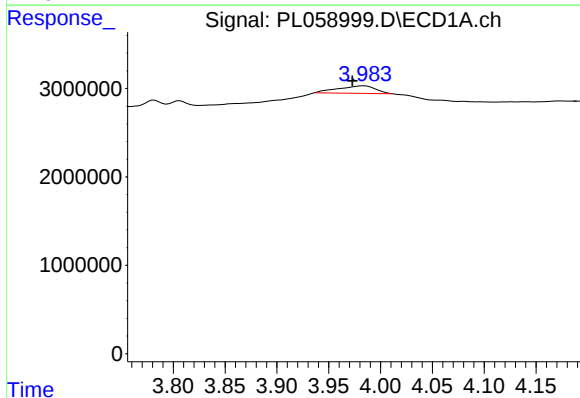


#2 alpha-BHC

R.T.: 3.984 min
Delta R.T.: 0.011 min
Response: 2103725
Conc: 0.77 ng/ml

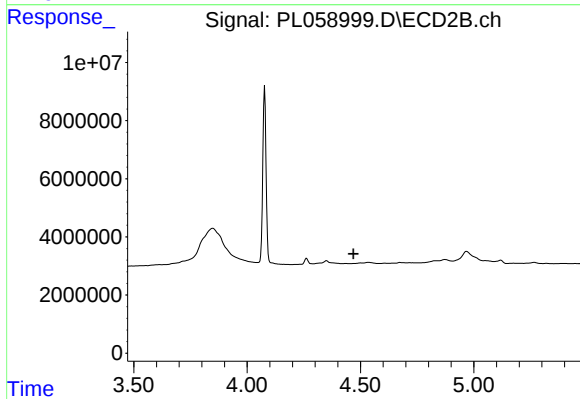

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.469 min
Response: 0
Conc: N.D.

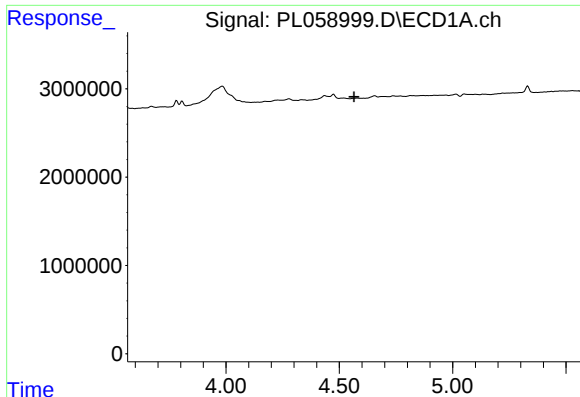

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 4.566 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

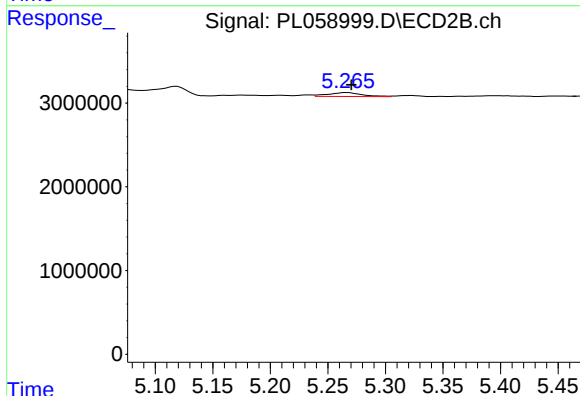


#4 Heptachlor

R.T.: 5.267 min
Delta R.T.: -0.004 min
Response: 947435
Conc: 0.25 ng/ml

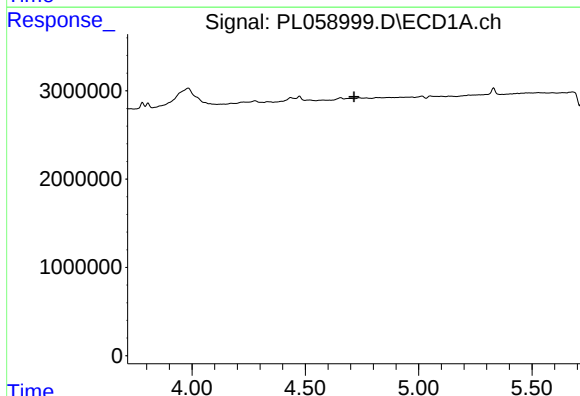


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.715 min
Response: 0
Conc: N.D.

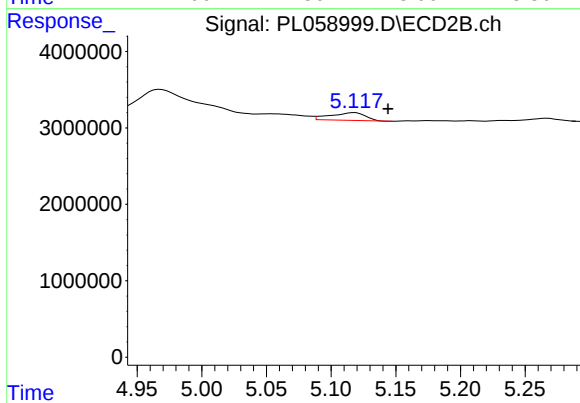

#7 delta-BHC


R.T.: 5.119 min
Delta R.T.: -0.025 min
Response: 1904725
Conc: 0.52 ng/ml

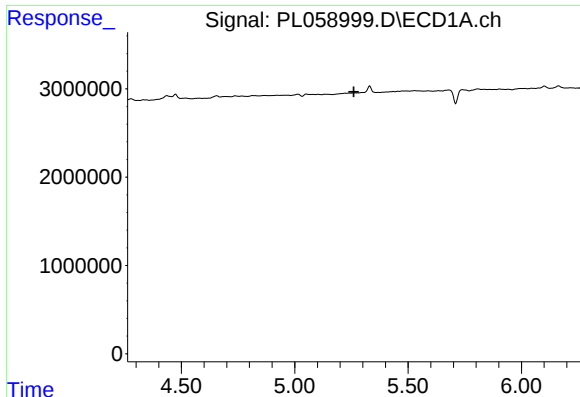

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 5.261 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

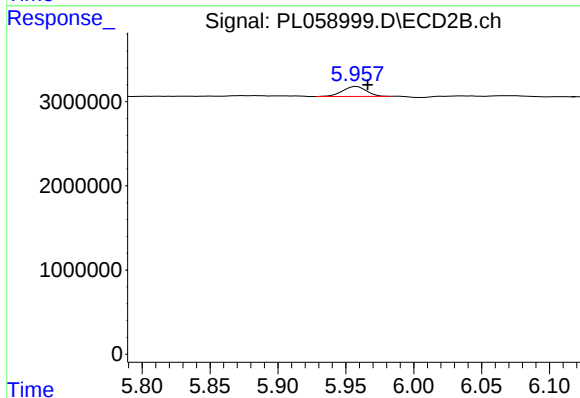


#8 Heptachlor epoxide

R.T.: 5.958 min
Delta R.T.: -0.008 min
Response: 1427961
Conc: 0.43 ng/ml

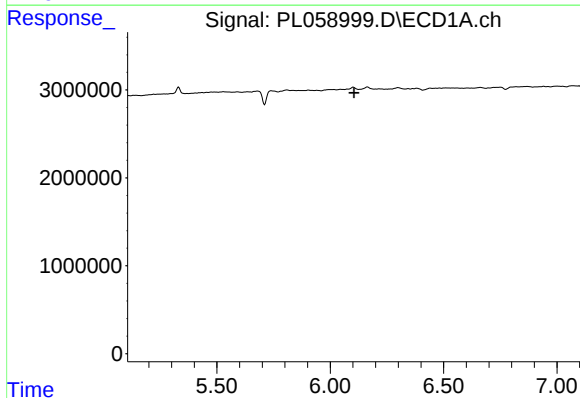


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.105 min
Response: 0
Conc: N.D.

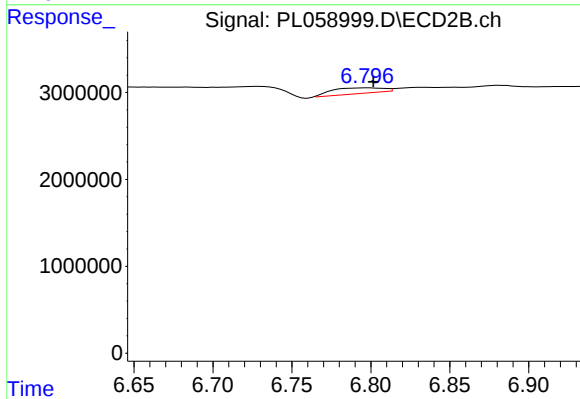

#14 Endrin


R.T.: 6.798 min
Delta R.T.: -0.004 min
Response: 1456597
Conc: 0.58 ng/ml

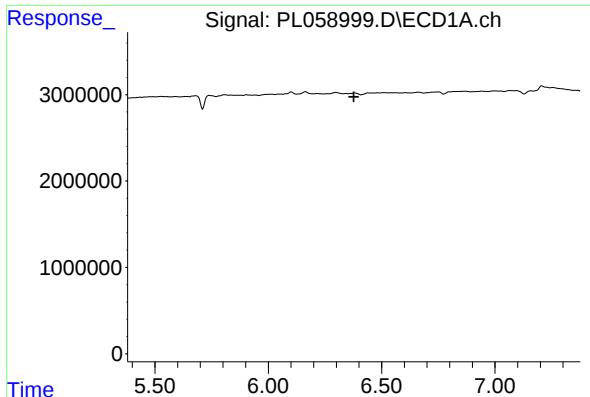

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.377 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

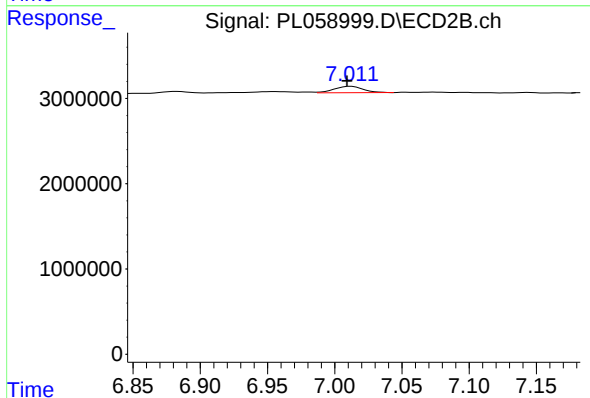


#15 Endosulfan II

R.T.: 7.012 min
Delta R.T.: 0.003 min
Response: 1114183
Conc: 0.40 ng/ml

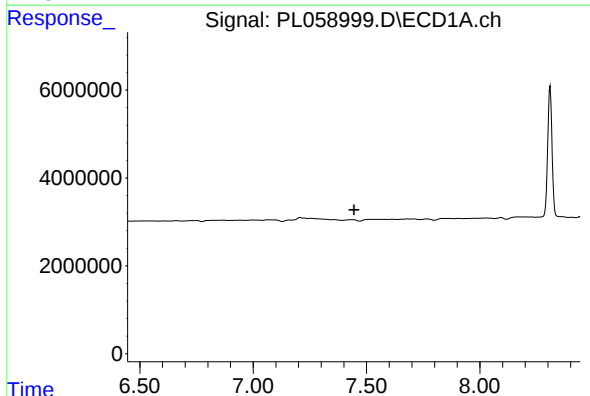


#22 Mirex

R.T.: 0.000 min
Exp R.T.: 7.446 min
Response: 0
Conc: N.D.

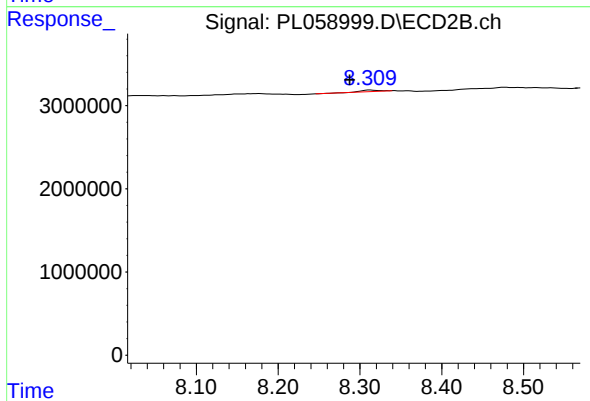

#22 Mirex


R.T.: 8.313 min
Delta R.T.: 0.025 min
Response: 327576
Conc: 0.15 ng/ml

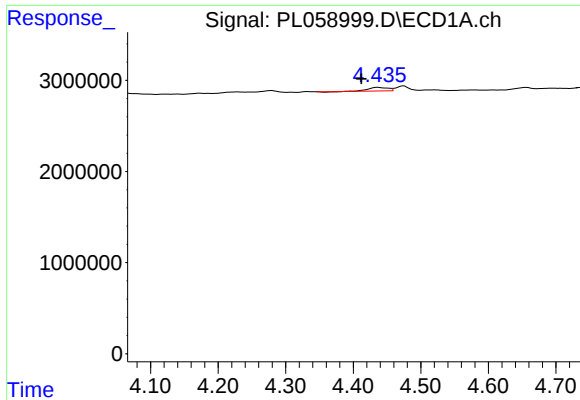

#23 Chlordane-1


R.T.: 4.436 min
Delta R.T.: 0.024 min
Response: 735798
Conc: 14.06 ng/ml

Instrument :
ECD_L
ClientSampleId :

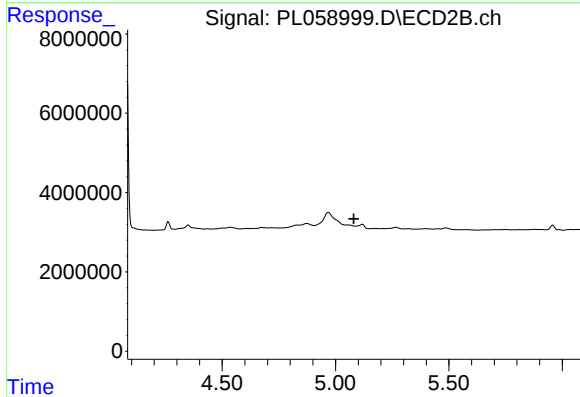


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.081 min
Response: 0
Conc: N.D.

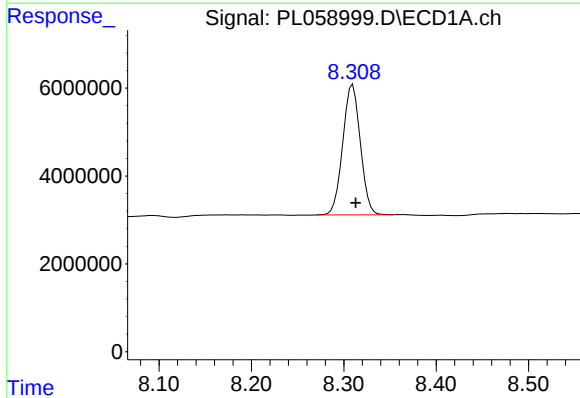

#28 Decachlorobiphenyl

R.T.: 8.310 min
Delta R.T.: -0.003 min
Response: 39197621
Conc: 23.20 ng/ml

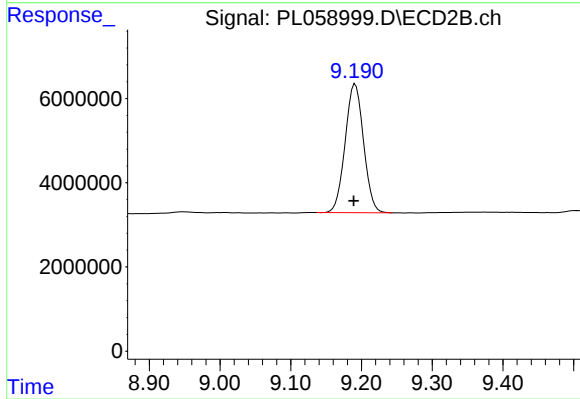

#28 Decachlorobiphenyl

R.T.: 9.191 min
Delta R.T.: 0.002 min
Response: 55295241
Conc: 20.98 ng/ml