

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052921\
 Data File : PL066954.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 May 2021 16:01
 Operator : AR\AJ
 Sample : M2491-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 31 06:10:43 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052721CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu May 27 02:30:58 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	4.482	5.530	5414127	8684596	10.145	9.821
27)	SA Decachlor...	10.226	11.431	13666462	18147480	20.381	19.877
Target Compounds							
4)	MA Heptachlor	0.000	7.202f	0	233904	N.D.	0.236
7)	B delta-BHC	0.000	7.004	0	1963071	N.D.	1.777
8)	B Heptachlo...	0.000	8.056f	0	212773	N.D.	0.231
10)	B trans-Chl...	0.000	8.250	0	502330	N.D.	0.544
12)	B 4,4'-DDE	0.000	8.537	0	82708	N.D.	<MDL
13)	MA Dieldrin	0.000	8.688	0	154701	N.D.	0.176
15)	B Endosulfa...	8.130f	9.177	3823134	304880	6.366	0.418 #
16)	A 4,4'-DDD	0.000	9.031f	0	2542411	N.D.	3.431
21)	B Endrin ke...	0.000	10.084f	0	381597	N.D.	0.463

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052921\
Data File : PL066954.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 May 2021 16:01
Operator : AR\AJ
Sample : M2491-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 31 06:10:43 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052721CLP.M
Quant Title : GC Extractables
QLast Update : Thu May 27 02:30:58 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

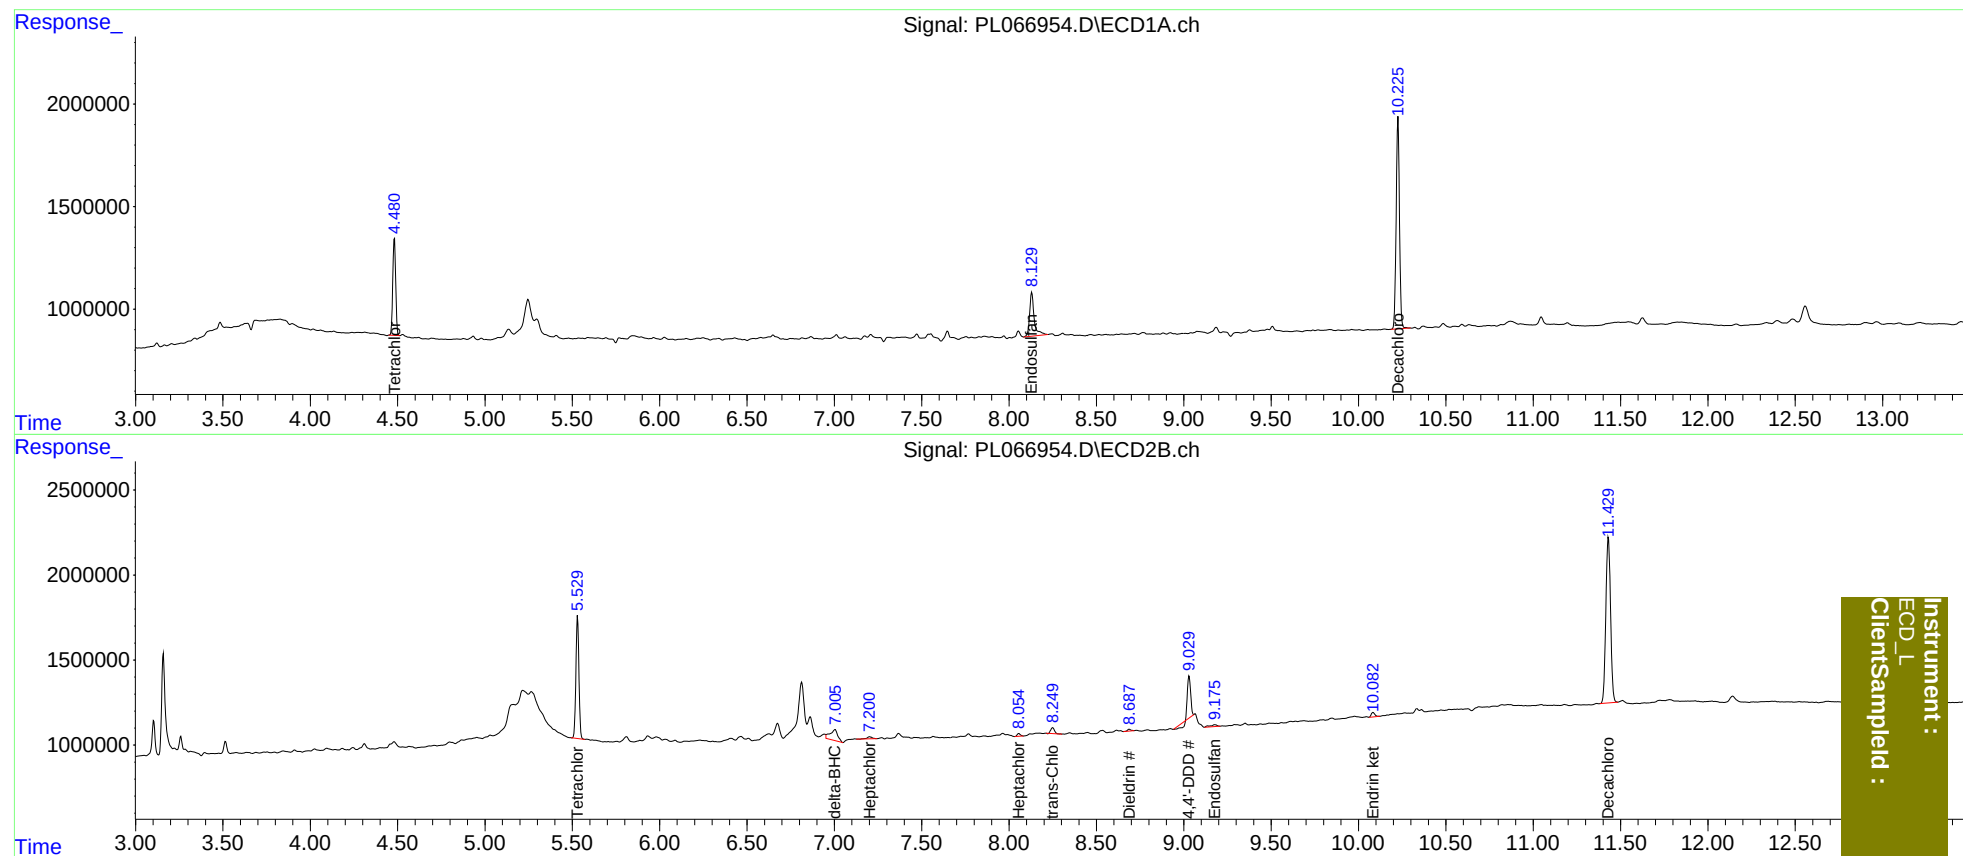


Instrument :
ECD_L
ClientSampled :
M2491-01

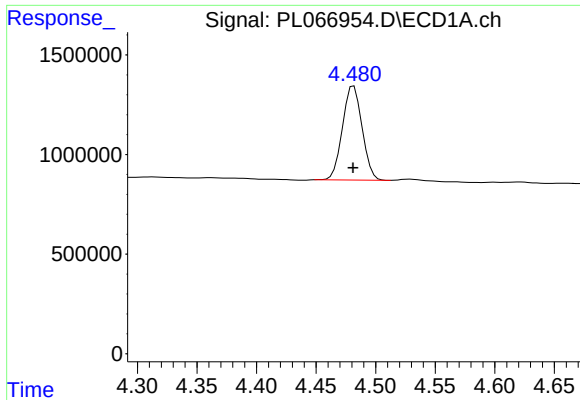

#1 Tetrachloro-m-xylene


R.T.: 4.482 min
Delta R.T.: 0.000 min
Response: 5414127
Conc: 10.15 ng/ml

Instrument :
ECD_L
ClientSampleId :

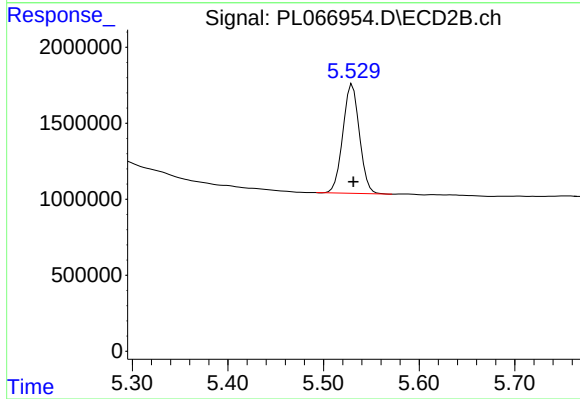


#1 Tetrachloro-m-xylene

R.T.: 5.530 min
Delta R.T.: -0.001 min
Response: 8684596
Conc: 9.82 ng/ml

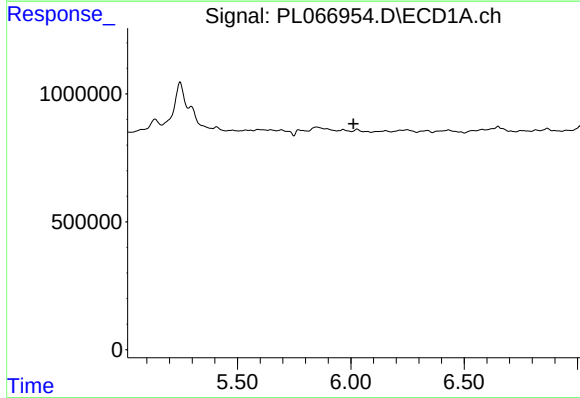


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 6.012 min
Response: 0
Conc: N.D.

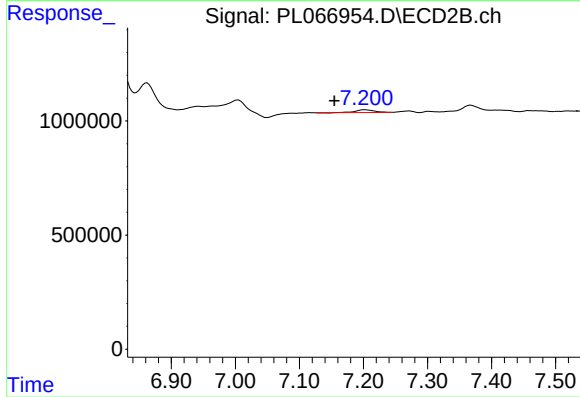

#4 Heptachlor


R.T.: 7.202 min
Delta R.T.: 0.047 min
Response: 233904
Conc: 0.24 ng/ml

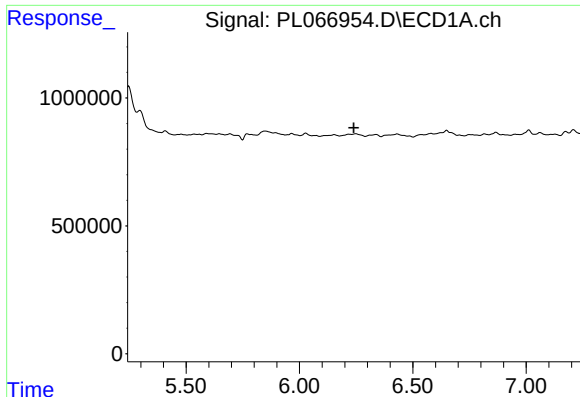

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 6.240 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

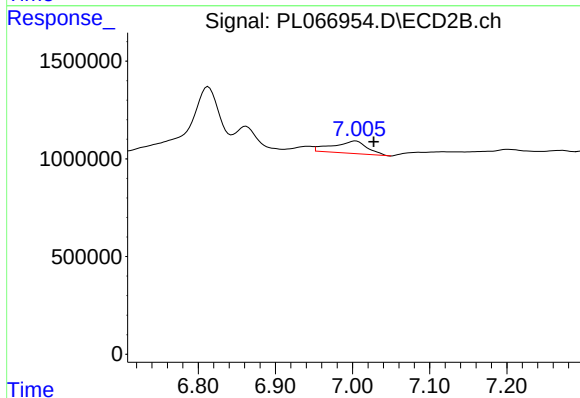


#7 delta-BHC

R.T.: 7.004 min
Delta R.T.: -0.023 min
Response: 1963071
Conc: 1.78 ng/ml

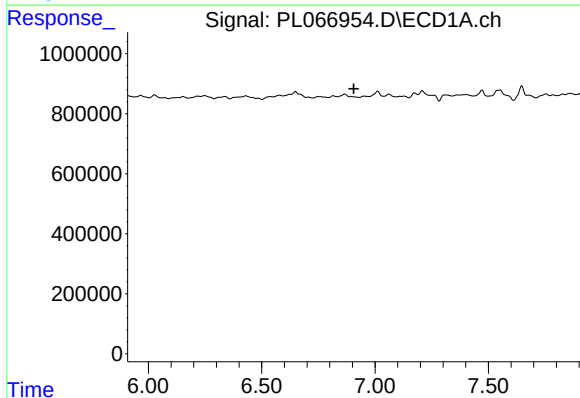


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 6.906 min
Response: 0
Conc: N.D.

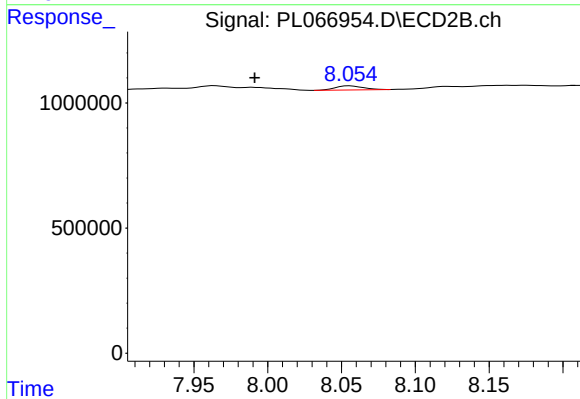

#8 Heptachlor epoxide


R.T.: 8.056 min
Delta R.T.: 0.065 min
Response: 212773
Conc: 0.23 ng/ml

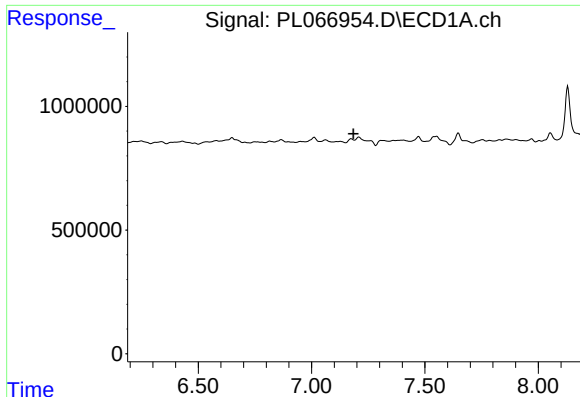

#10 trans-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.186 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

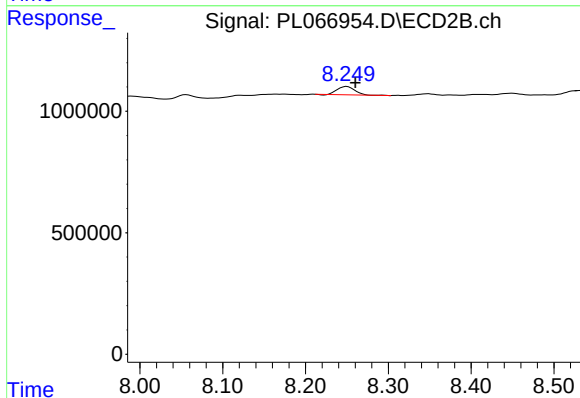


#10 trans-Chlordane

R.T.: 8.250 min
Delta R.T.: -0.010 min
Response: 502330
Conc: 0.54 ng/ml

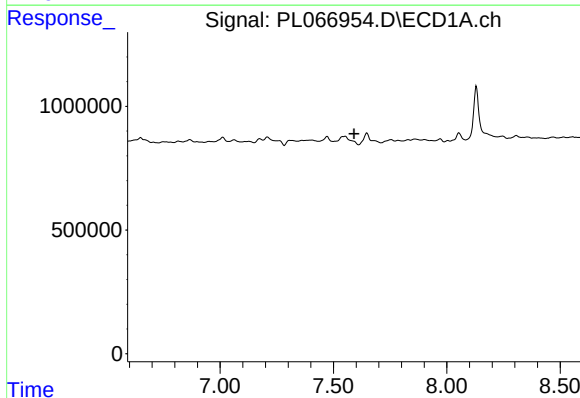


#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 7.591 min
Response: 0
Conc: N.D.

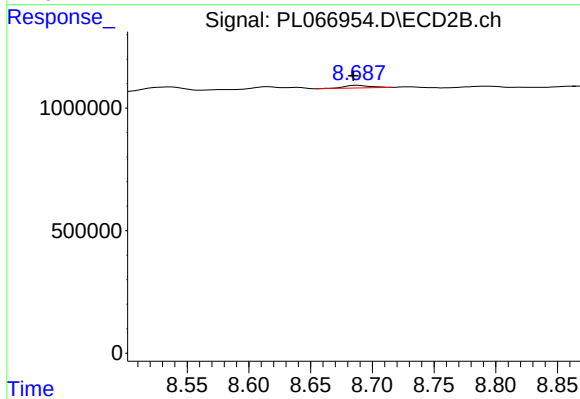

#13 Dieldrin


R.T.: 8.688 min
Delta R.T.: 0.004 min
Response: 154701
Conc: 0.18 ng/ml

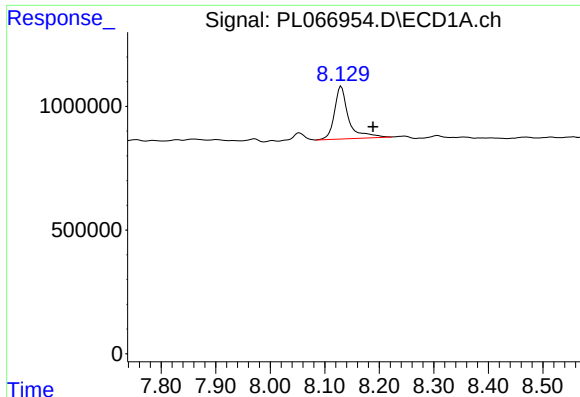

#15 Endosulfan II


R.T.: 8.130 min
Delta R.T.: -0.059 min
Response: 3823134
Conc: 6.37 ng/ml

Instrument :
ECD_L
ClientSampleId :

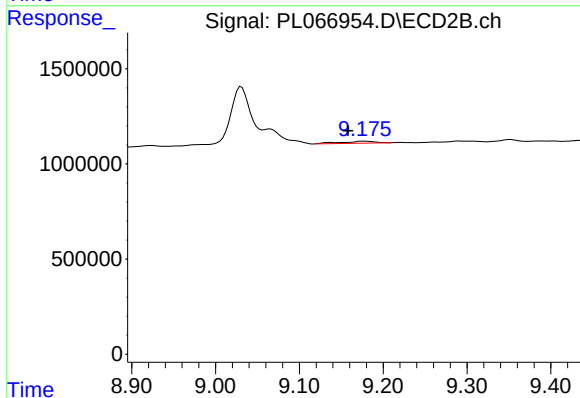


#15 Endosulfan II

R.T.: 9.177 min
Delta R.T.: 0.019 min
Response: 304880
Conc: 0.42 ng/ml

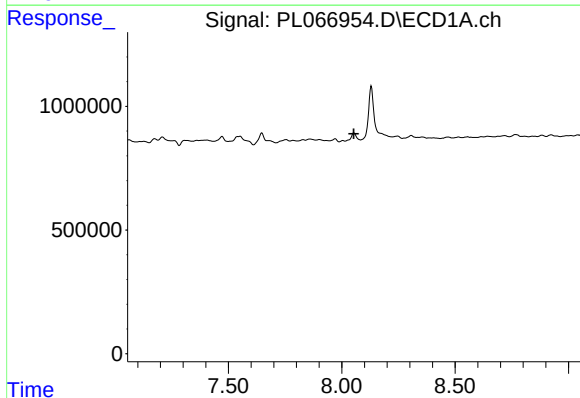


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 8.053 min
Response: 0
Conc: N.D.

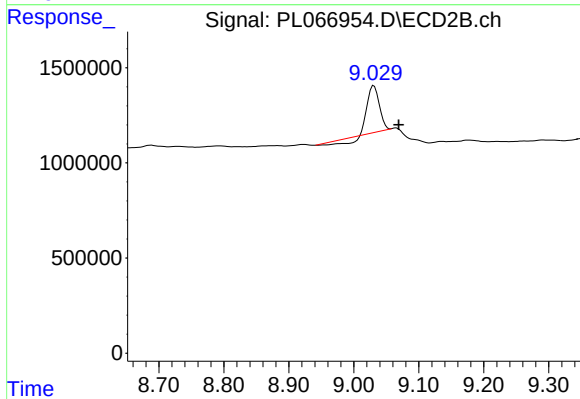

#16 4,4'-DDD


R.T.: 9.031 min
Delta R.T.: -0.038 min
Response: 2542411
Conc: 3.43 ng/ml

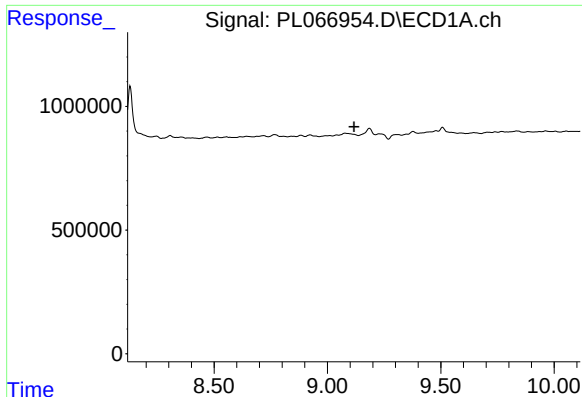

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 9.117 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

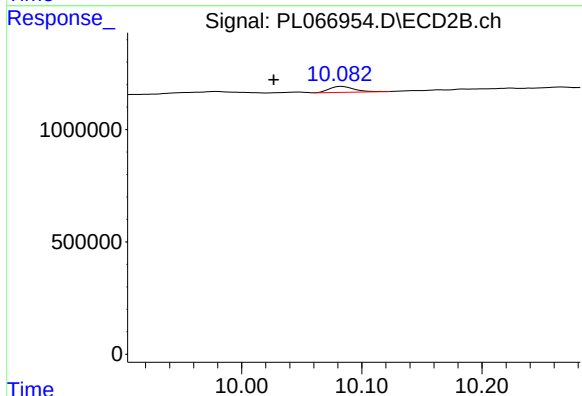


#21 Endrin ketone

R.T.: 10.084 min
Delta R.T.: 0.057 min
Response: 381597
Conc: 0.46 ng/ml

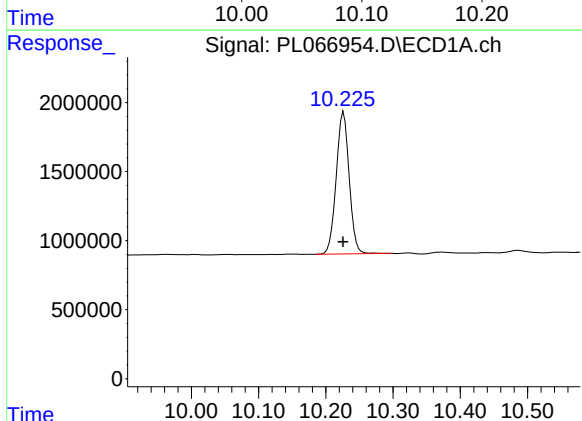

#27 Decachlorobiphenyl

R.T.: 10.226 min
Delta R.T.: 0.000 min
Response: 13666462
Conc: 20.38 ng/ml

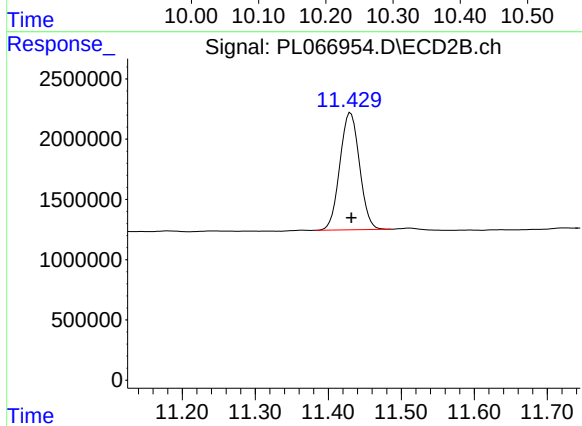

#27 Decachlorobiphenyl

R.T.: 11.431 min
Delta R.T.: 0.000 min
Response: 18147480
Conc: 19.88 ng/ml