

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052921\
 Data File : PL066943.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 May 2021 10:55
 Operator : AR\AJ
 Sample : M2250-02
 Misc : PEST MDL 1 PPB
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MDL-WATER-QT3-2021-06

Manual Integrations
 APPROVED

Ankita
 6/1/2021 1:43:49 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 31 06:07:50 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052721CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu May 27 02:30:58 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	4.483	5.533	10267550	16330467	19.240	18.468
27)	SA Decachlor...	10.228	11.433	26888068	35032222	40.099	38.372
Target Compounds							
2)	A alpha-BHC	5.180	6.113	587616	896323	0.726m	0.815
3)	MA gamma-BHC...	5.601	6.509	729305	895651	1.032m	0.841
4)	MA Heptachlor	6.014	7.157	692584	918554	1.026	0.926
5)	MB Aldrin	6.336	7.526	709826	874345	1.041	0.917m
6)	B beta-BHC	5.983	6.767	363515	1384670	0.988m	2.165 #
7)	B delta-BHC	6.242	7.029	745343	1145663	1.067	1.037
8)	B Heptachlo...	6.909	7.993	717130	1007492	1.105	1.095
9)	A Endosulfan I	7.309	8.398	696483	785942	1.103	0.955
10)	B trans-Chl...	7.188	8.262	736512	944012	1.075	1.022
11)	B cis-Chlor...	7.256	8.343	750500	915289	1.098	1.007
12)	B 4,4'-DDE	7.473	8.531	611362	669777	0.980m	0.797m
13)	MA Dieldrin	7.593	8.687	673939	798027	0.993	0.910
14)	MA Endrin	7.878	8.926	646287	638890	1.050m	0.881
15)	B Endosulfa...	8.189	9.159	825701	770199	1.375m	1.057
16)	A 4,4'-DDD	8.054	9.068	508921	841044	0.946m	1.135m
17)	MA 4,4'-DDT	8.314	9.387	387092	542812	0.743m	0.826
18)	B Endrin al...	8.377	9.293	547933	628510	1.079m	0.959m
19)	B Endosulfa...	8.609	9.532	675990	749796	1.183	1.019
20)	A Methoxychlor	8.909	9.875	302871	348782	1.026m	0.938
21)	B Endrin ke...	9.119	10.028	739052	856481	1.092	1.038

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052921\
Data File : PL066943.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 May 2021 10:55
Operator : AR\AJ
Sample : M2250-02
Misc : PEST MDL 1 PPB
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 31 06:07:50 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052721CLP.M
Quant Title : GC Extractables
QLast Update : Thu May 27 02:30:58 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

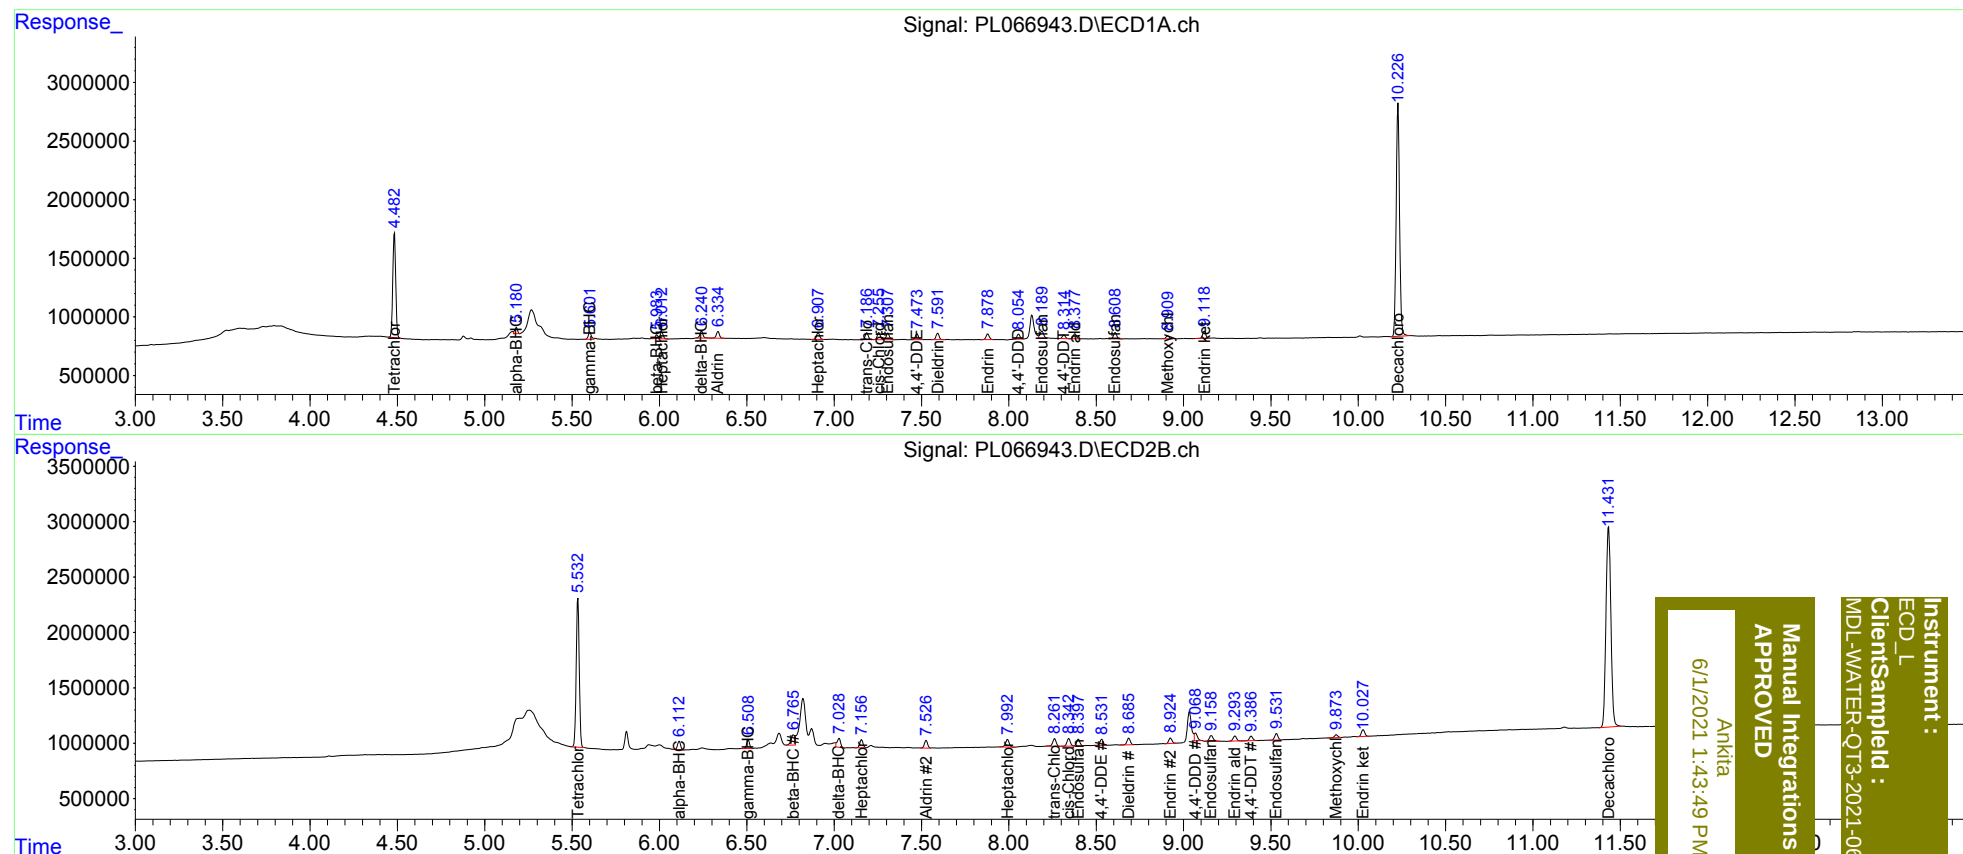

Manual Integrations
APPROVED

Ankita

6/1/2021 1:43:49 PM

Instrument :
ECD_L
Client Sample :
MDL-WATER-QT3-2021-06