

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL052925\  
 Data File : PL095819.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 29 May 2025 08:35  
 Operator : AR\AJ  
 Sample : HEXANE  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 ECD\_L  
 ClientSampleId :

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 30 00:51:53 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\PL052125.M  
 Quant Title : GC Extractables  
 QLast Update : Thu May 22 06:29:30 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

#### System Monitoring Compounds

| Target Compounds |              |       |       |         |          |       |          |
|------------------|--------------|-------|-------|---------|----------|-------|----------|
| 8) B             | Heptachlo... | 5.714 | 0.000 | 7985774 | 0        | 2.092 | N.D. #   |
| 14) MA           | Endrin       | 0.000 | 5.784 | 0       | 4370872  | N.D.  | 0.896 #  |
| 24)              | Chlordane-2  | 0.000 | 4.475 | 0       | 18534991 | N.D.  | 83.209 # |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL052925\  
Data File : PL095819.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 29 May 2025 08:35  
Operator : AR\AJ  
Sample : HEXANE  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
ECD\_L  
ClientSampleId :

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: May 30 00:51:53 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\PL052125.M  
Quant Title : GC Extractables  
QLast Update : Thu May 22 06:29:30 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

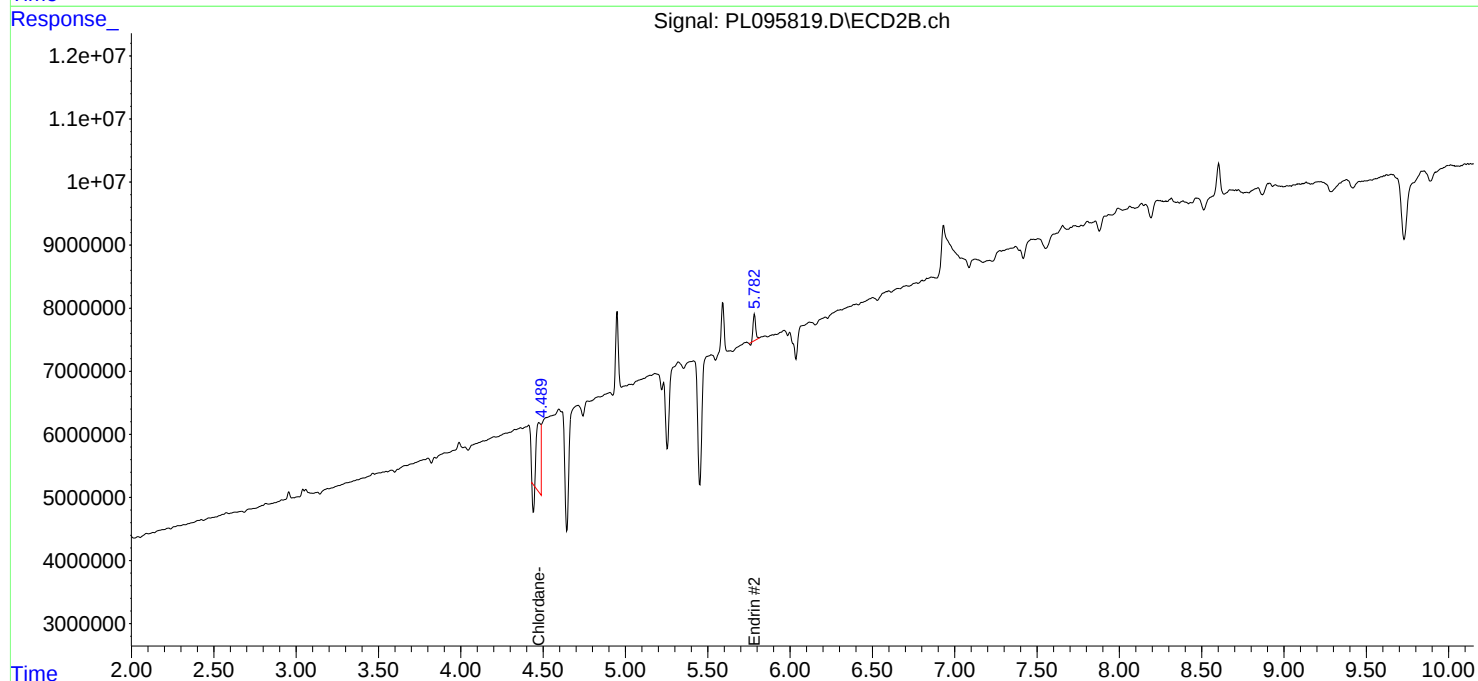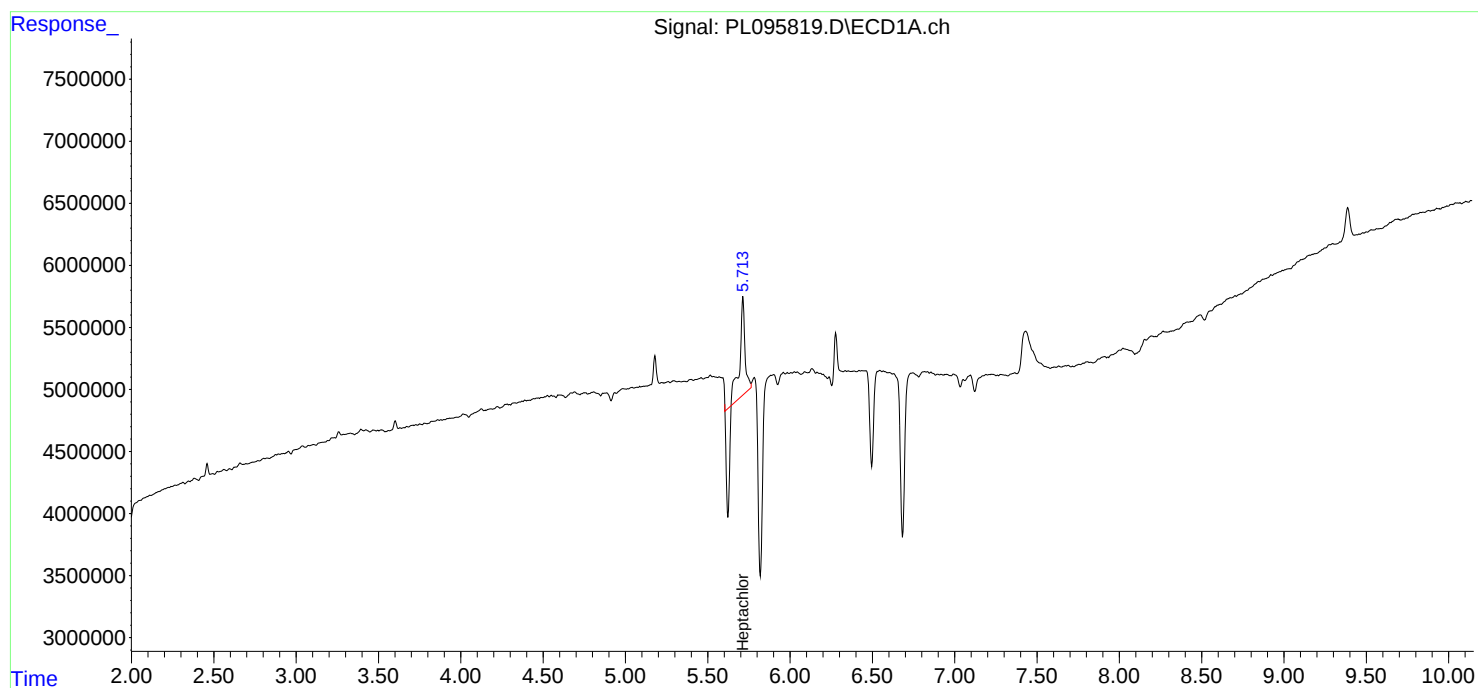


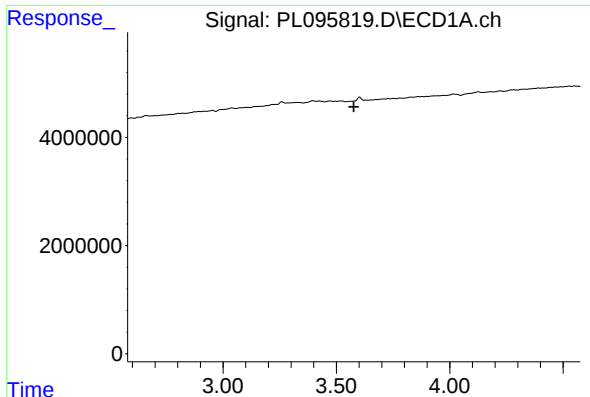

#1 Tetrachloro-m-xylene


R.T.: 0.000 min  
Exp R.T.: 3.577 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_L  
ClientSampleId :

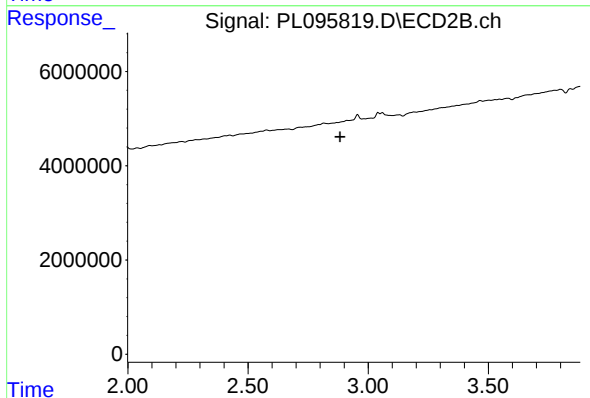


#1 Tetrachloro-m-xylene

R.T.: 0.000 min  
Exp R.T.: 2.883 min  
Response: 0  
Conc: N.D.

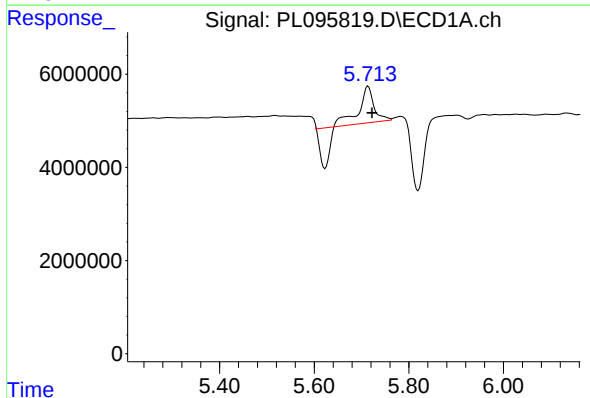


#8 Heptachlor epoxide

R.T.: 5.714 min  
Delta R.T.: -0.008 min  
Response: 7985774  
Conc: 2.09 ng/ml

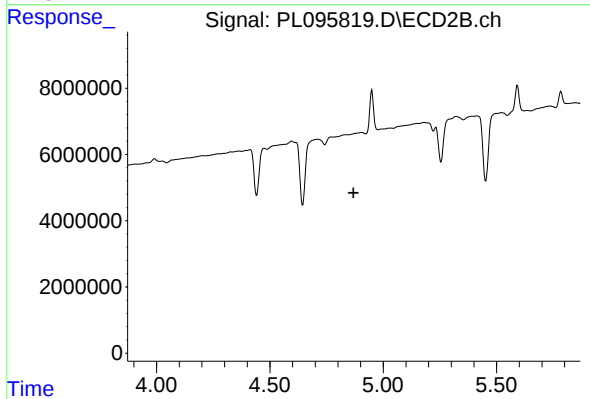

#8 Heptachlor epoxide


R.T.: 0.000 min  
Exp R.T.: 4.869 min  
Response: 0  
Conc: N.D.

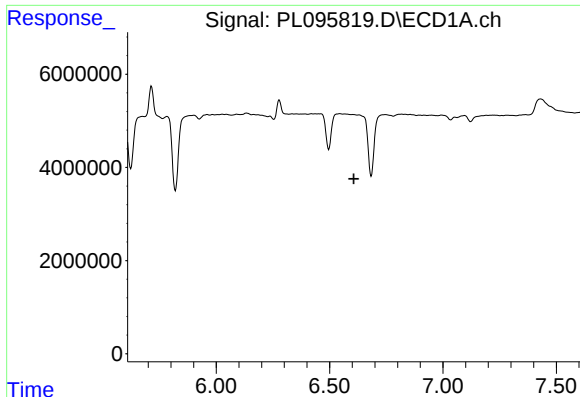

#14 Endrin


R.T.: 0.000 min  
Exp R.T.: 6.607 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_L  
ClientSampleId :

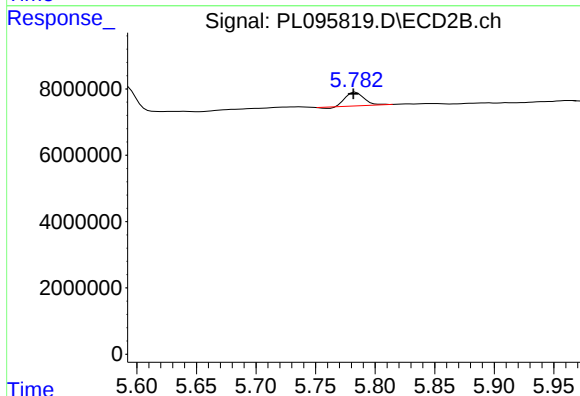


#14 Endrin

R.T.: 5.784 min  
Delta R.T.: 0.002 min  
Response: 4370872  
Conc: 0.90 ng/ml

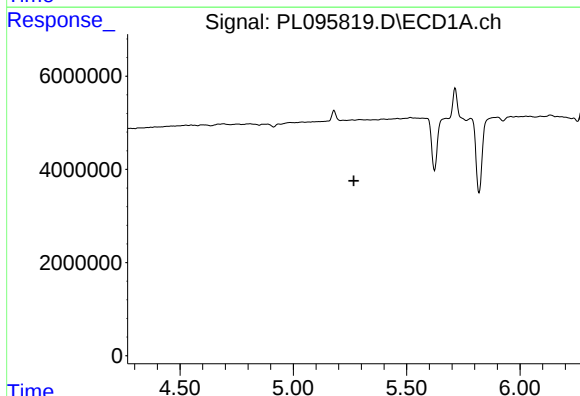


#24 Chlordane-2

R.T.: 0.000 min  
Exp R.T.: 5.267 min  
Response: 0  
Conc: N.D.

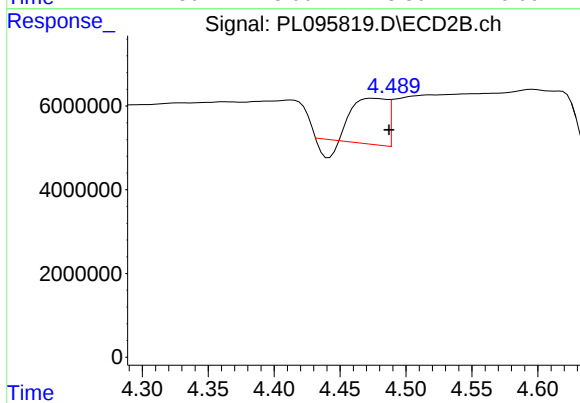

#24 Chlordane-2


R.T.: 4.475 min  
Delta R.T.: -0.012 min  
Response: 18534991  
Conc: 83.21 ng/ml

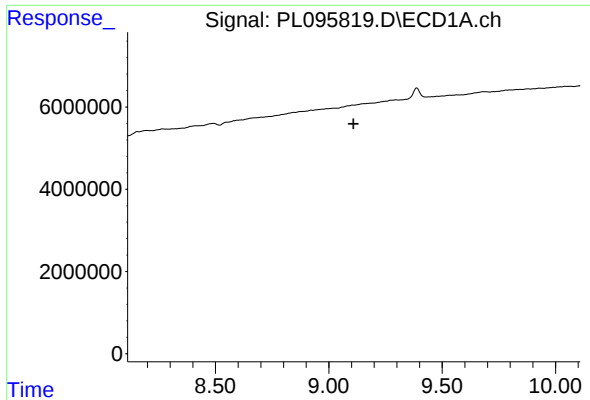

#28 Decachlorobiphenyl

R.T.: 0.000 min  
Exp R.T. : 9.109 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_L  
ClientSampleId :

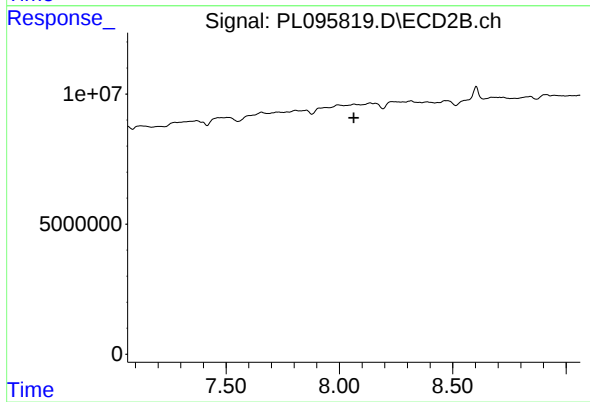

#28 Decachlorobiphenyl

R.T.: 0.000 min  
Exp R.T. : 8.064 min  
Response: 0  
Conc: N.D.