

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052925\
 Data File : PL095831.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 May 2025 15:22
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 30 00:53:47 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052125.M
 Quant Title : GC Extractables
 QLast Update : Thu May 22 06:29:30 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.572	2.885	63032627	84220143	19.977	21.518
28)	SA Decachlor...	9.100	8.061	41388120	80896708	17.565	18.493
Target Compounds							
24)	Chlordane-2	0.000	4.481	0	3532991	N.D.	15.861 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052925\
Data File : PL095831.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 May 2025 15:22
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 30 00:53:47 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052125.M
Quant Title : GC Extractables
QLast Update : Thu May 22 06:29:30 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

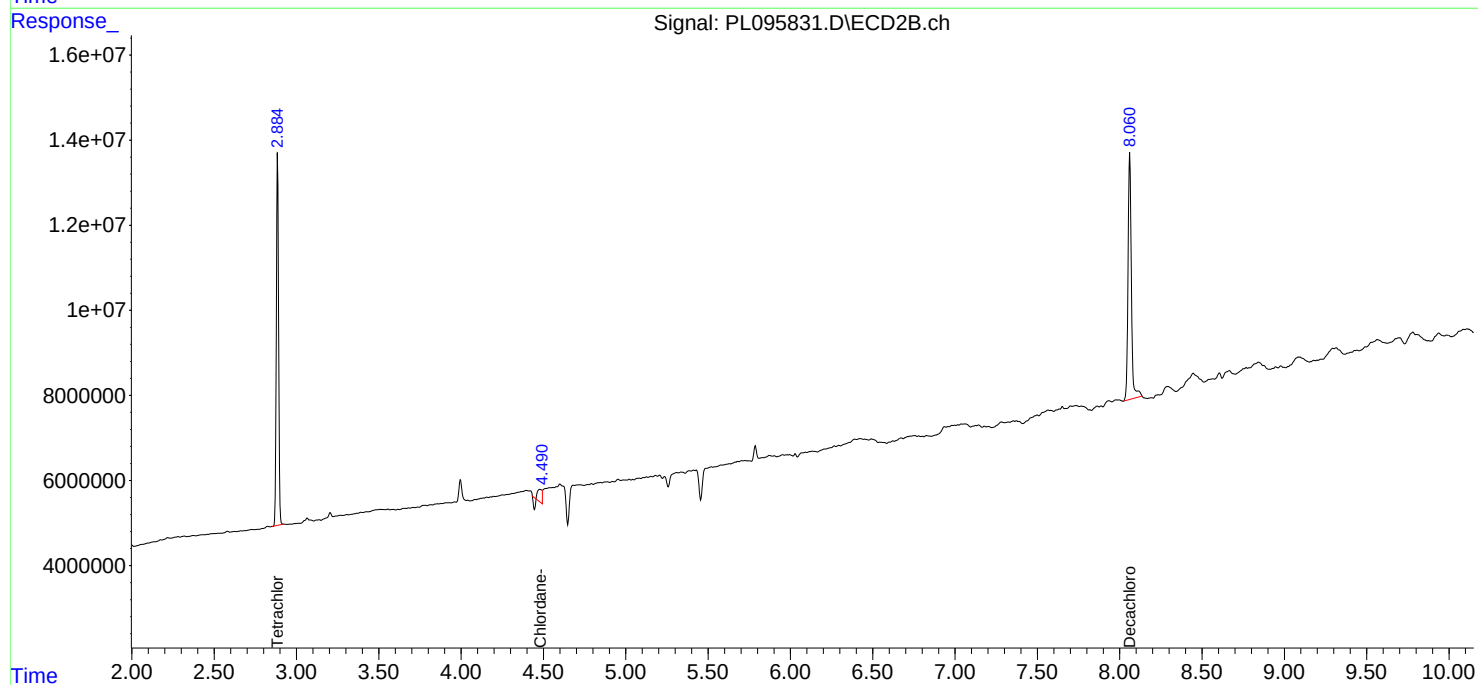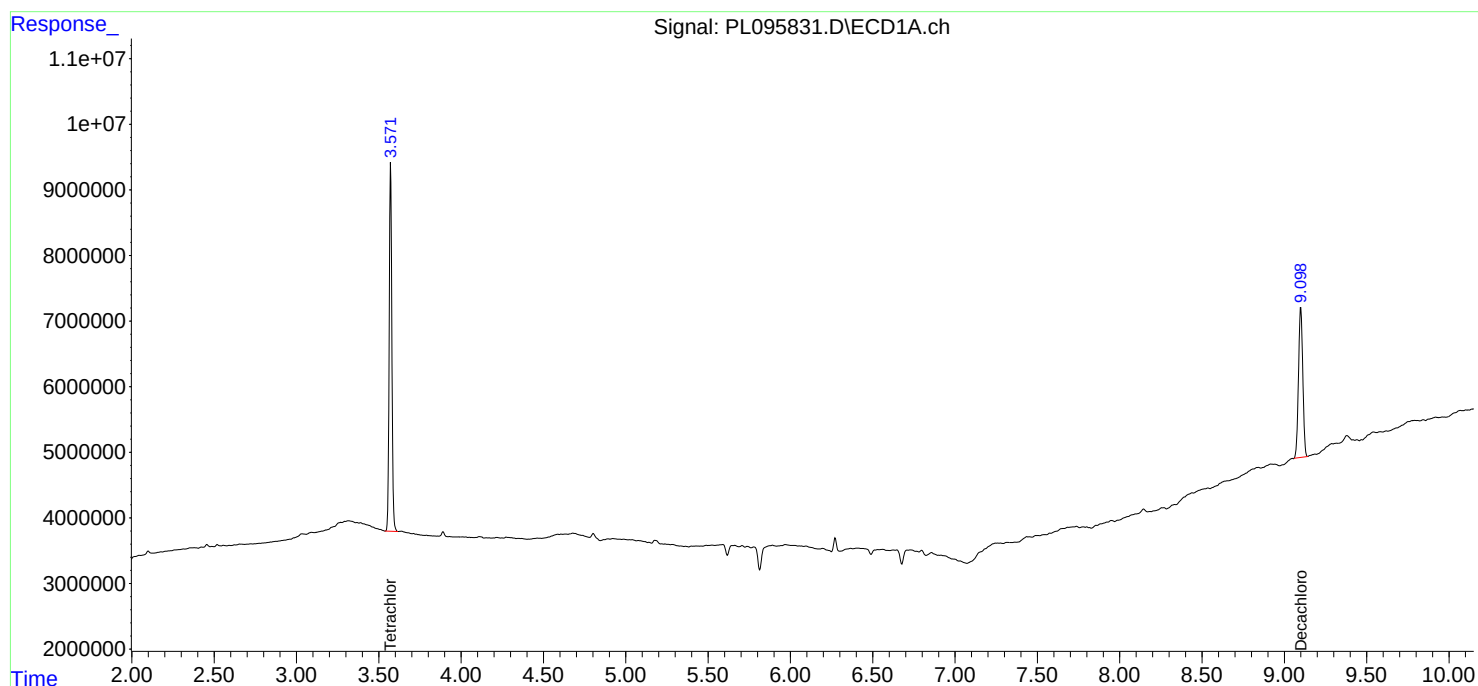


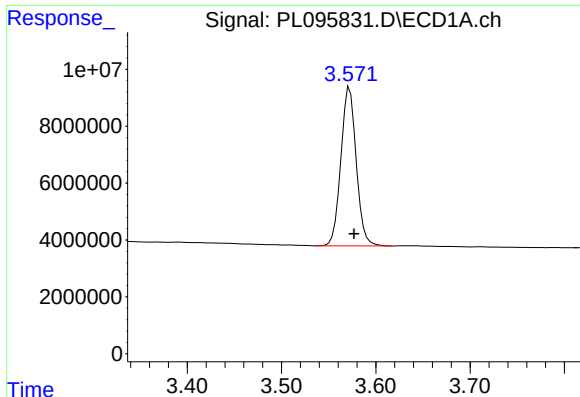

#1 Tetrachloro-m-xylene


R.T.: 3.572 min
Delta R.T.: -0.005 min
Response: 63032627
Conc: 19.98 ng/ml

Instrument :
ECD_L
ClientSampleId :

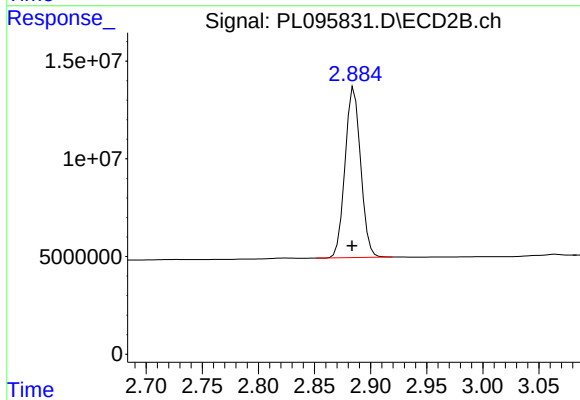


#1 Tetrachloro-m-xylene

R.T.: 2.885 min
Delta R.T.: 0.002 min
Response: 84220143
Conc: 21.52 ng/ml

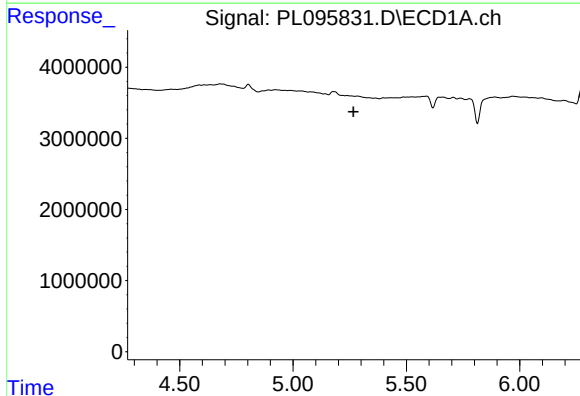


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.267 min
Response: 0
Conc: N.D.

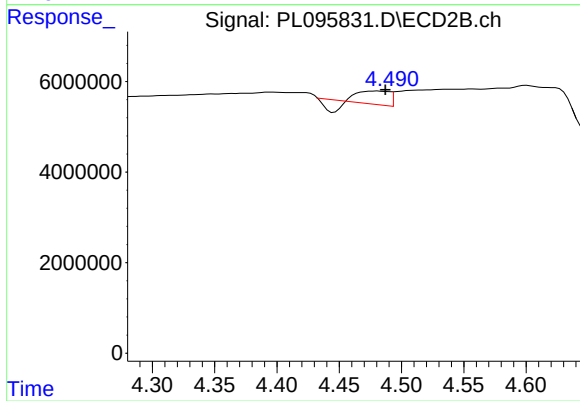

#24 Chlordane-2


R.T.: 4.481 min
Delta R.T.: -0.006 min
Response: 3532991
Conc: 15.86 ng/ml

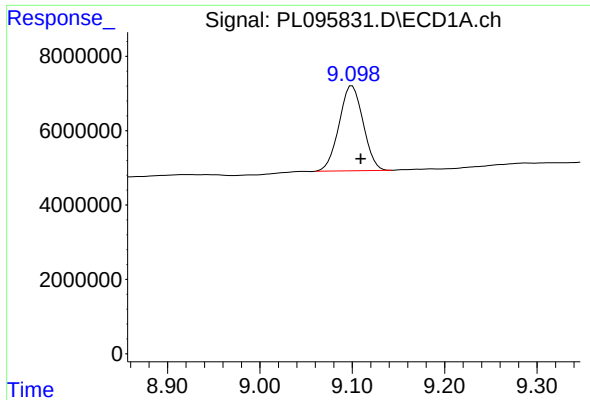

#28 Decachlorobiphenyl

R.T.: 9.100 min
Delta R.T.: -0.009 min
Response: 41388120
Conc: 17.56 ng/ml

Instrument :
ECD_L
ClientSampleId :

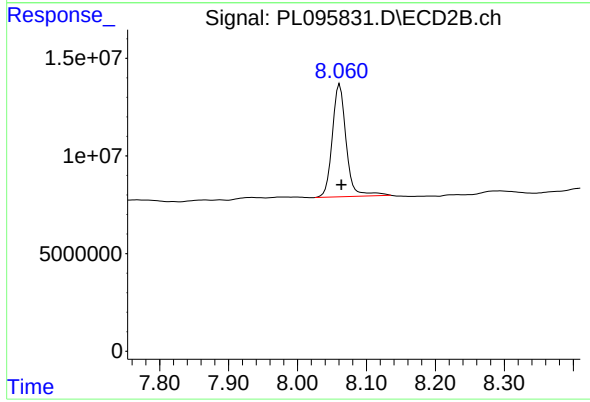

#28 Decachlorobiphenyl

R.T.: 8.061 min
Delta R.T.: -0.002 min
Response: 80896708
Conc: 18.49 ng/ml