

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL053019\
 Data File : PL049087.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 May 2019 12:35
 Operator : SM\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 31 01:29:39 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL053019.M
 Quant Title : GC Extractables
 QLast Update : Fri May 31 01:29:18 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.324	3.937	570.8E6	138.4E6	50.000	50.000
28)	SA Decachlor...	7.993	8.973	596.6E6	156.0E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.165	4.923	263.8E6	66174012	500.000	500.000
24)	Chlordane-2	4.655	5.391	289.0E6	70123177	500.000	500.000
25)	Chlordane-3	5.211	6.035	892.2E6	237.1E6	500.000	500.000
26)	Chlordane-4	5.266	6.108	820.6E6	283.3E6	500.000	500.000
27)	Chlordane-5	6.089	6.911	260.4E6	54791599	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL053019\
Data File : PL049087.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 May 2019 12:35
Operator : SM\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 31 01:29:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL053019.M
Quant Title : GC Extractables
QLast Update : Fri May 31 01:29:18 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

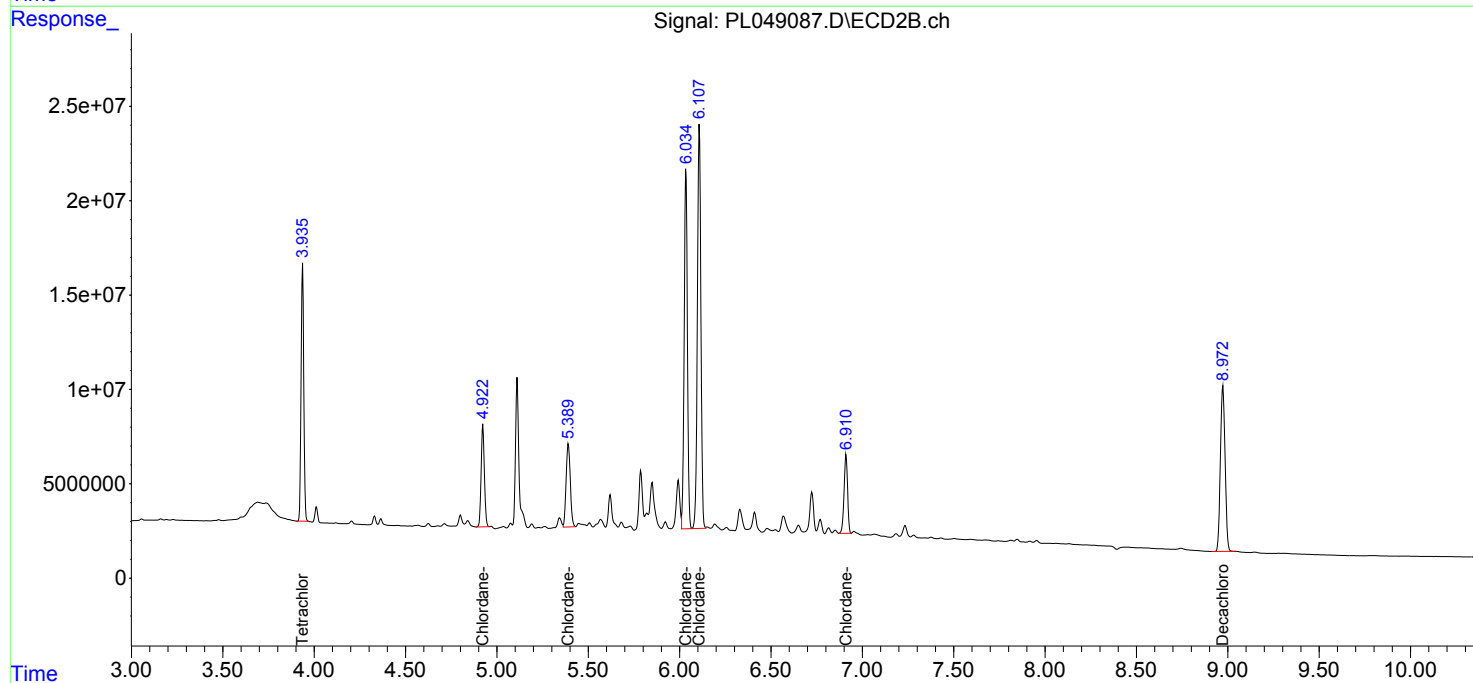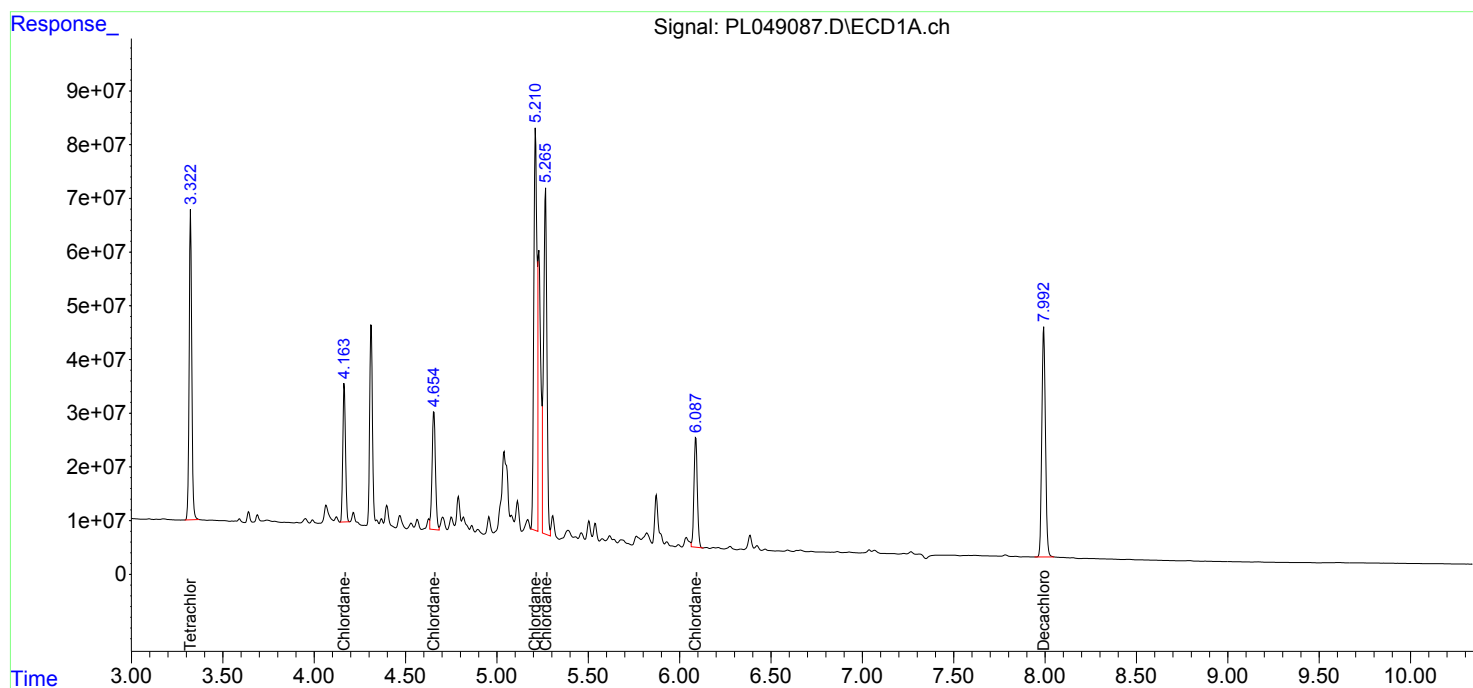


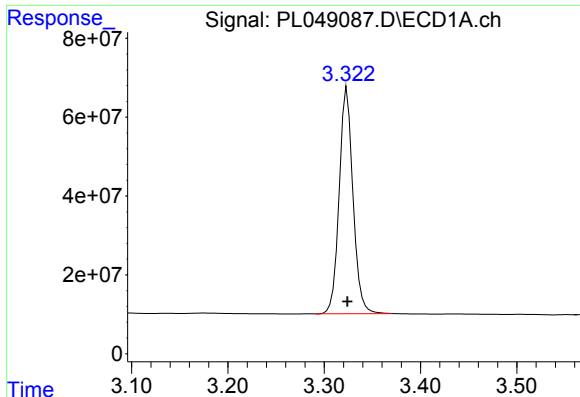

#1 Tetrachloro-m-xylene


R.T.: 3.324 min
Delta R.T.: 0.000 min
Response: 570835088
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

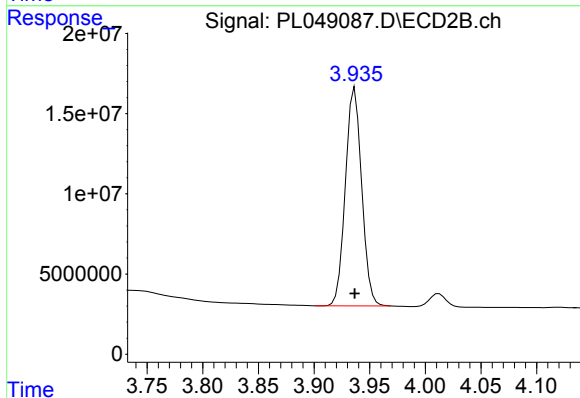


#1 Tetrachloro-m-xylene

R.T.: 3.937 min
Delta R.T.: 0.000 min
Response: 138424714
Conc: 50.00 ng/ml

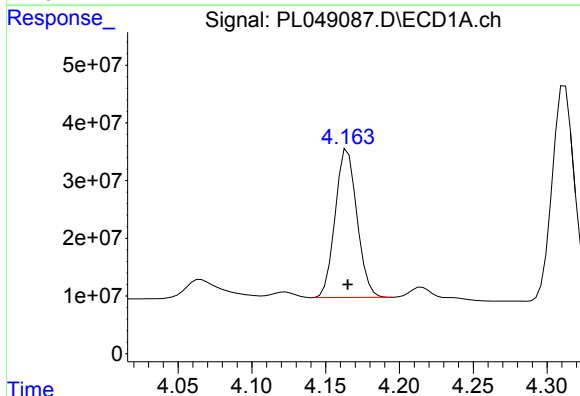


#23 Chlordane-1

R.T.: 4.165 min
Delta R.T.: 0.000 min
Response: 263836444
Conc: 500.00 ng/ml

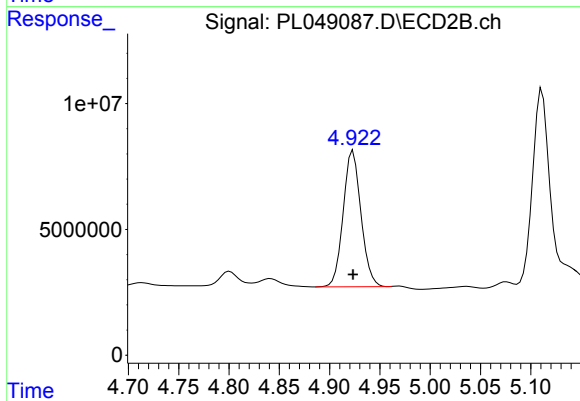

#23 Chlordane-1


R.T.: 4.923 min
Delta R.T.: 0.000 min
Response: 66174012
Conc: 500.00 ng/ml

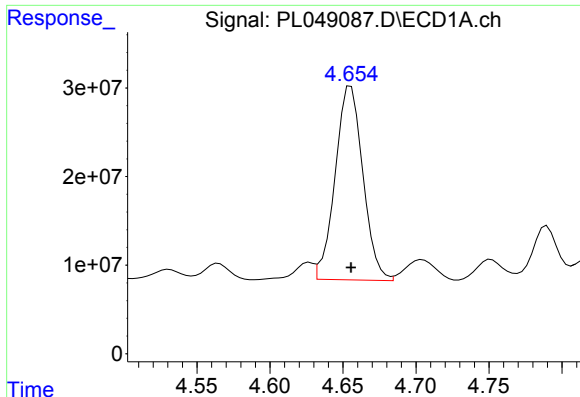

#24 Chlordane-2


R.T.: 4.655 min
Delta R.T.: 0.000 min
Response: 288998300
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

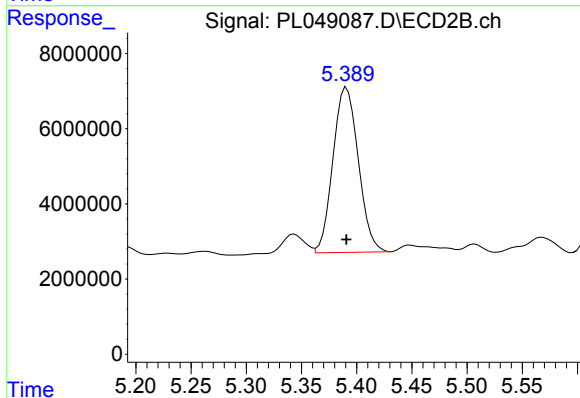


#24 Chlordane-2

R.T.: 5.391 min
Delta R.T.: 0.000 min
Response: 70123177
Conc: 500.00 ng/ml

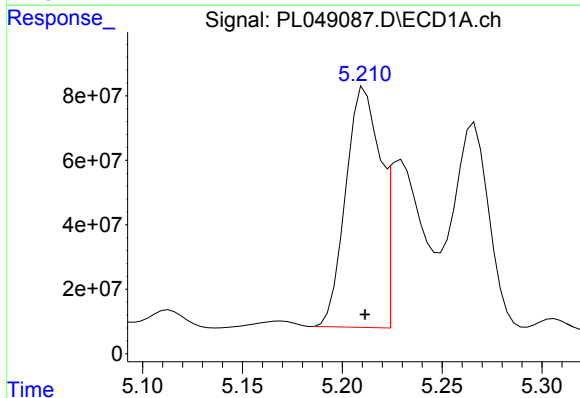


#25 Chlordane-3

R.T.: 5.211 min
Delta R.T.: 0.000 min
Response: 892238128
Conc: 500.00 ng/ml

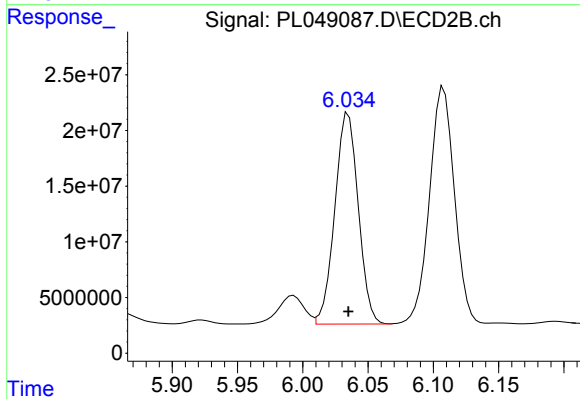

#25 Chlordane-3


R.T.: 6.035 min
Delta R.T.: 0.000 min
Response: 237143365
Conc: 500.00 ng/ml

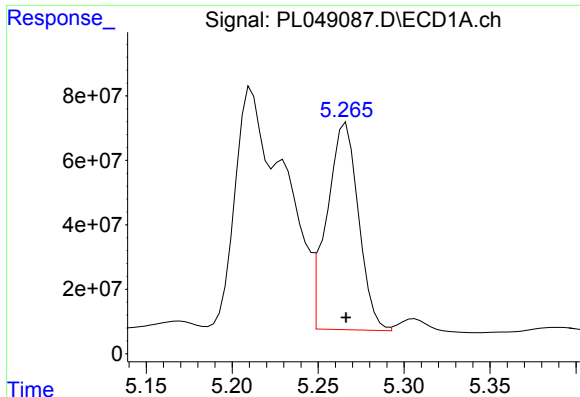

#26 Chlordane-4


R.T.: 5.266 min
Delta R.T.: 0.000 min
Response: 820562347
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

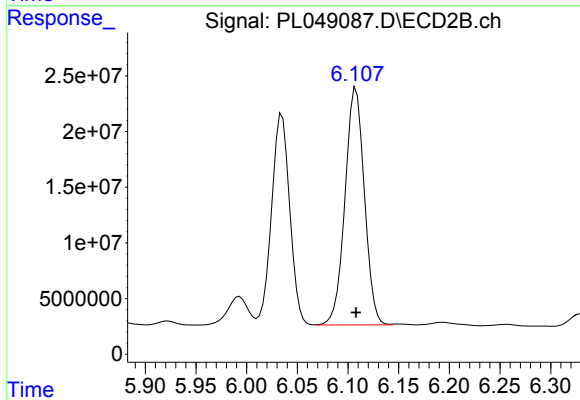


#26 Chlordane-4

R.T.: 6.108 min
Delta R.T.: 0.000 min
Response: 283321917
Conc: 500.00 ng/ml

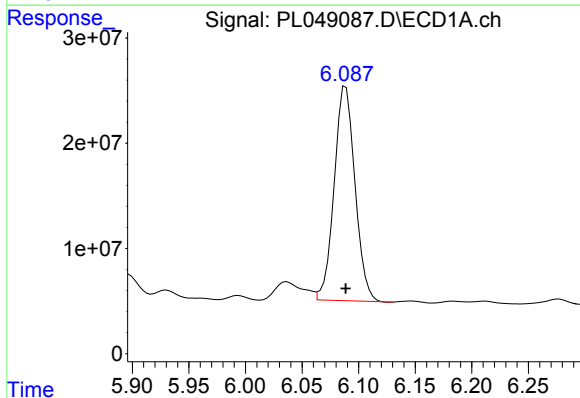


#27 Chlordane-5

R.T.: 6.089 min
Delta R.T.: 0.000 min
Response: 260371689
Conc: 500.00 ng/ml

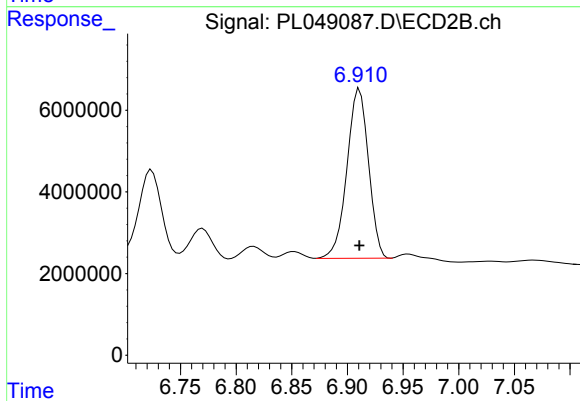

#27 Chlordane-5


R.T.: 6.911 min
Delta R.T.: 0.000 min
Response: 54791599
Conc: 500.00 ng/ml

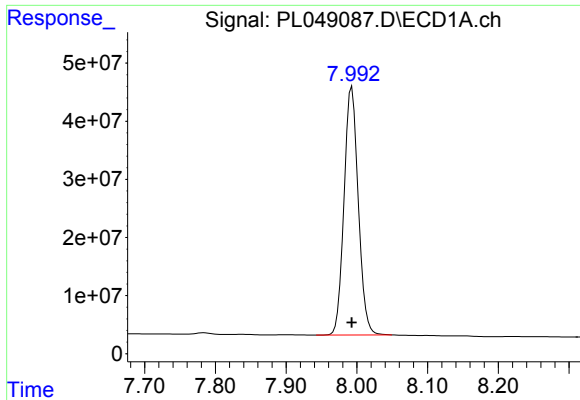

#28 Decachlorobiphenyl

R.T.: 7.993 min
Delta R.T.: 0.000 min
Response: 596578716
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

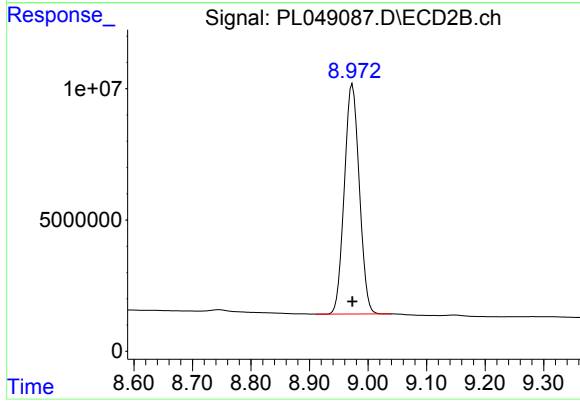

#28 Decachlorobiphenyl

R.T.: 8.973 min
Delta R.T.: 0.000 min
Response: 156008487
Conc: 50.00 ng/ml