

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL053019\
 Data File : PL049113.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 May 2019 19:11
 Operator : SM\AJ
 Sample : K3090-10
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-4-D

Manual Integrations
 APPROVED

Ankita
 5/31/2019 8:36:34 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 31 05:09:24 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL053019.M
 Quant Title : GC Extractables
 QLast Update : Fri May 31 01:35:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.325	3.937	194.2E6	53570056	17.627m	18.542
28)	SA Decachlor...	7.994	8.975	268.8E6	72385203	21.137	21.674

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL053019\
Data File : PL049113.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 May 2019 19:11
Operator : SM\AJ
Sample : K3090-10
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TP-4-D


Manual Integrations
APPROVED

Ankita
5/31/2019 8:36:34 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 31 05:09:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL053019.M
Quant Title : GC Extractables
QLast Update : Fri May 31 01:35:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

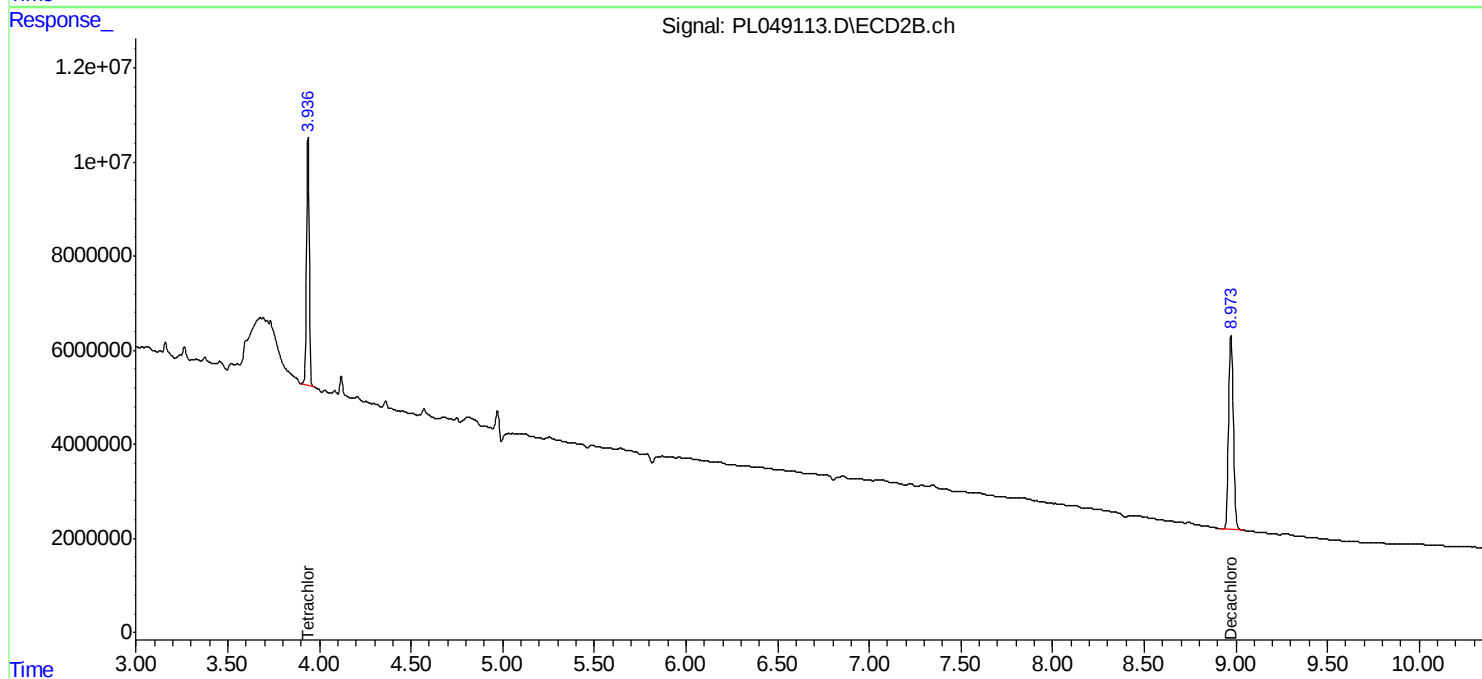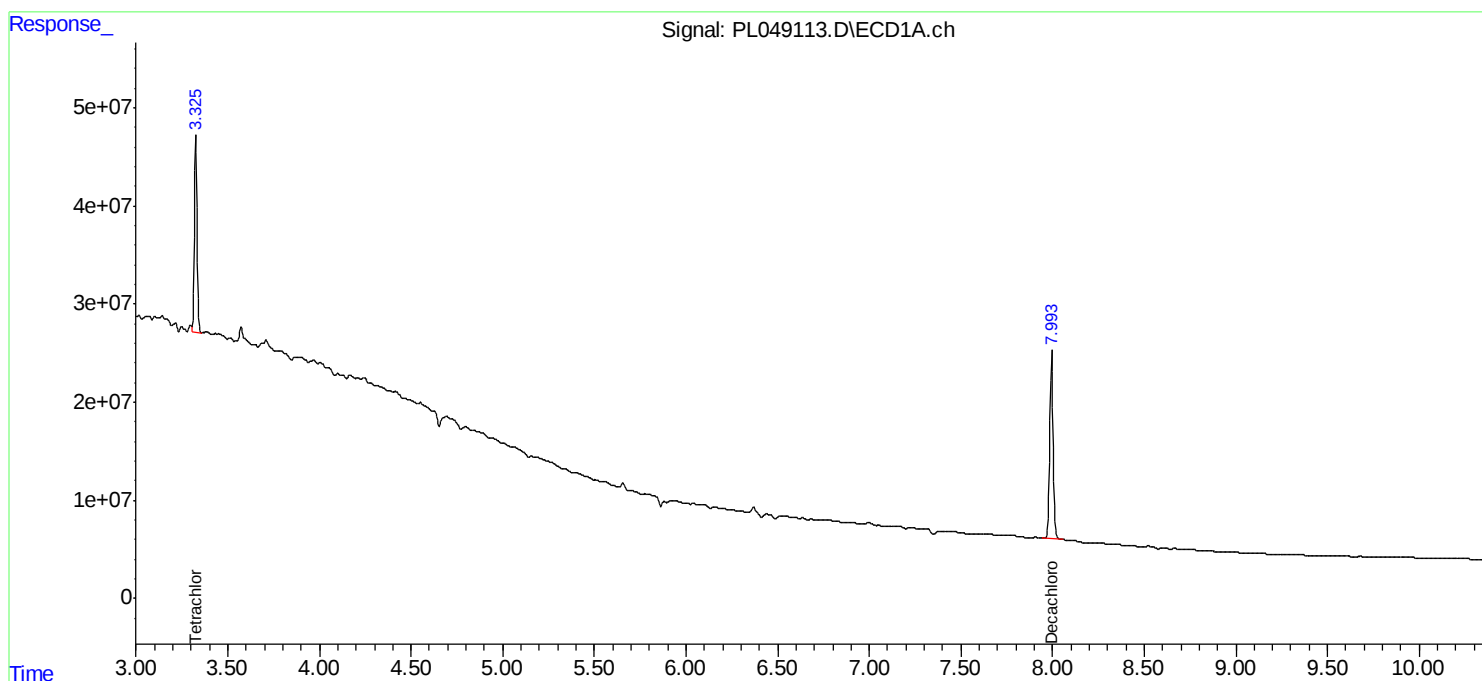

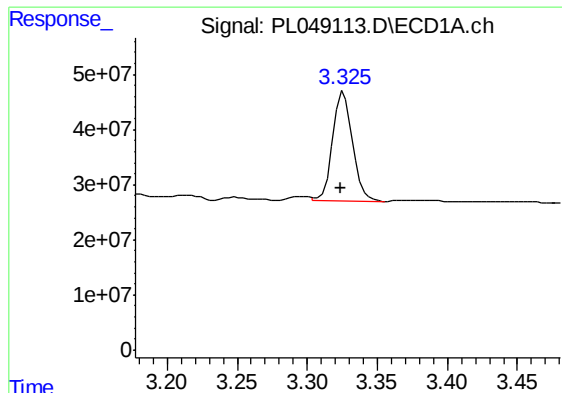


#1 Tetrachloro-m-xylene

R.T.: 3.325 min
Delta R.T.: 0.000 min
Response: 194224529
Conc: 17.63 ng/ml m

Instrument :
ECD_L
ClientSampleId :
TP-4-D


Manual Integrations
APPROVED

Ankita
5/31/2019 8:36:34 AM

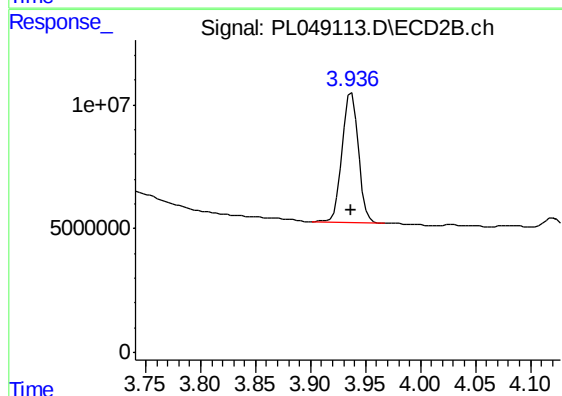


#1 Tetrachloro-m-xylene

R.T.: 3.937 min
Delta R.T.: 0.000 min
Response: 53570056
Conc: 18.54 ng/ml

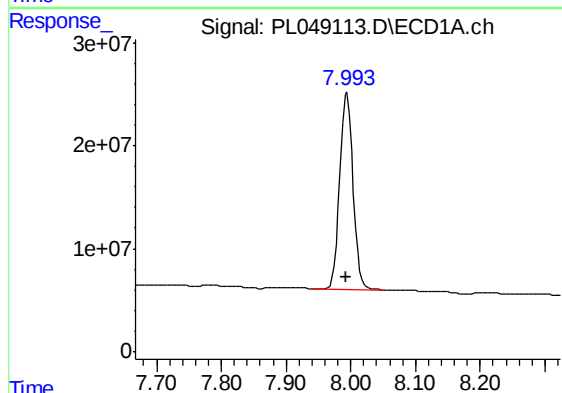

#28 Decachlorobiphenyl

R.T.: 7.994 min
Delta R.T.: 0.002 min
Response: 268763723
Conc: 21.14 ng/ml

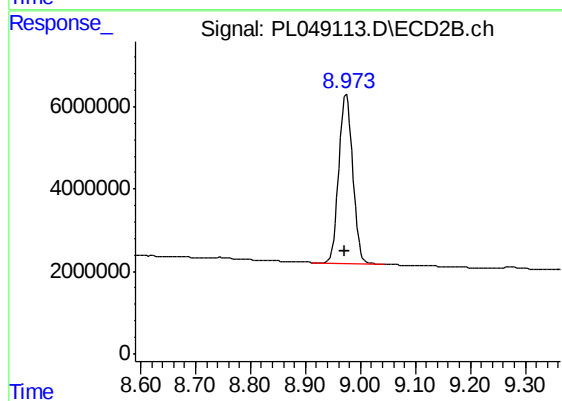

#28 Decachlorobiphenyl

R.T.: 8.975 min
Delta R.T.: 0.002 min
Response: 72385203
Conc: 21.67 ng/ml