

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL053023\
 Data File : PL083100.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 May 2023 16:59
 Operator : AR\AJ
 Sample : 02971-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SB16

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 30 21:09:42 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051923.M
 Quant Title : GC Extractables
 QLast Update : Sat May 20 04:58:53 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.317	2.637	60868340	53335692	20.710	20.545
28)	SA Decachlor...	8.736	7.742	44099988	50240825	21.027	20.205
Target Compounds							
11)	B alpha-Chl...	5.771	4.879	1680612	1878986	0.524	0.626



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL053023\
Data File : PL083100.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 May 2023 16:59
Operator : AR\AJ
Sample : 02971-01
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
SB16

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 30 21:09:42 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051923.M
Quant Title : GC Extractables
QLast Update : Sat May 20 04:58:53 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

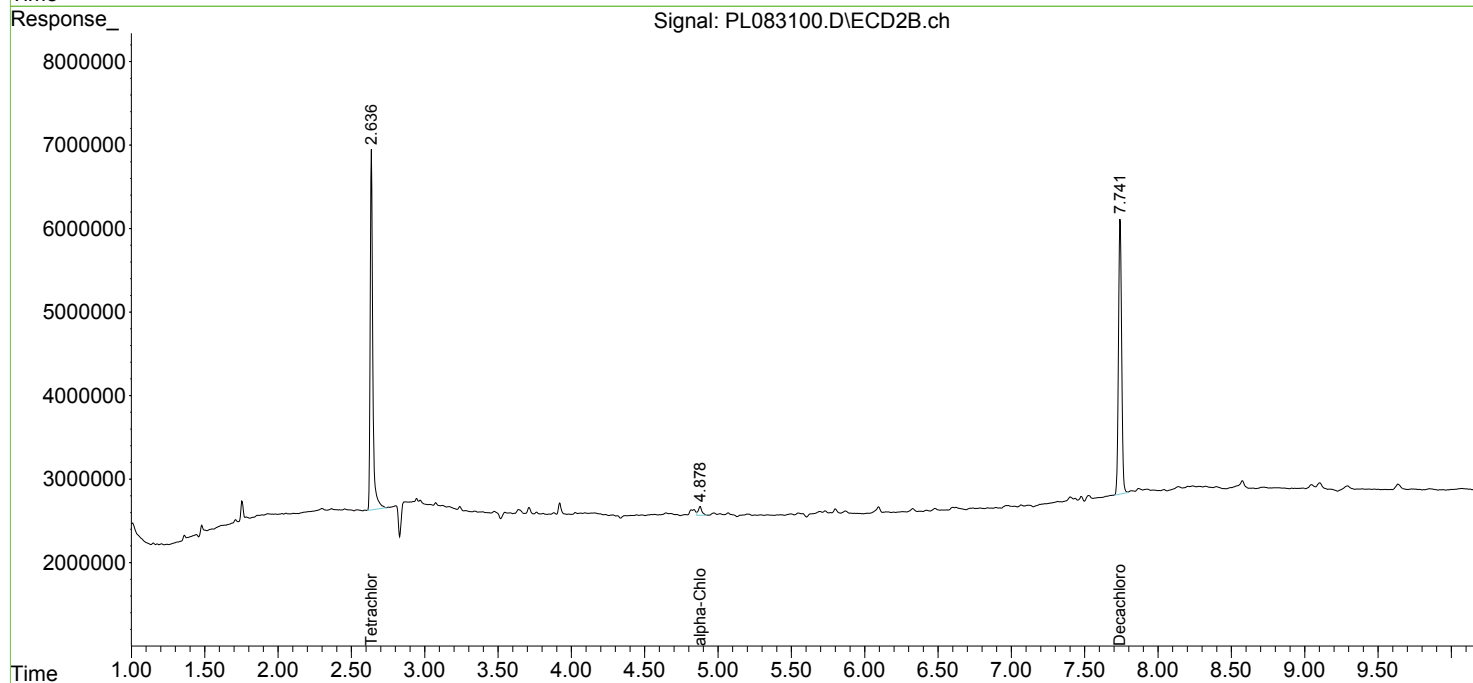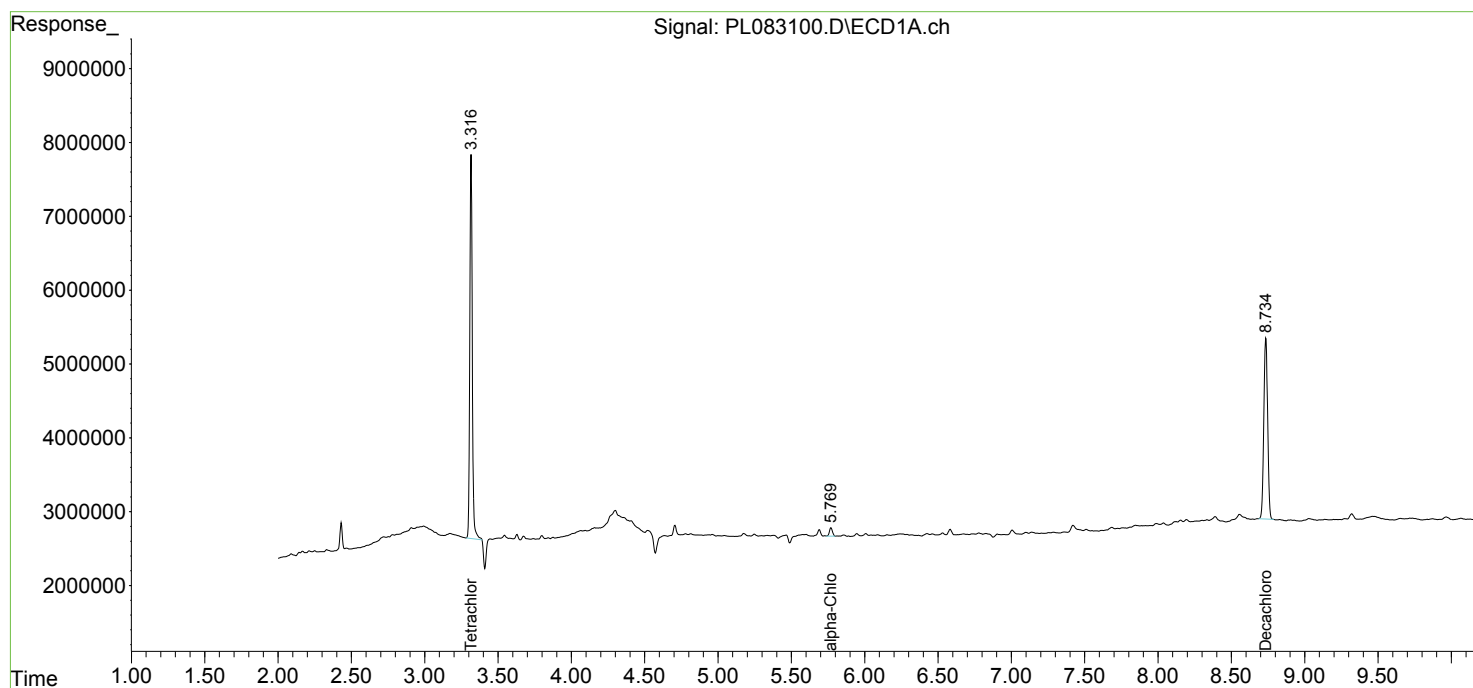


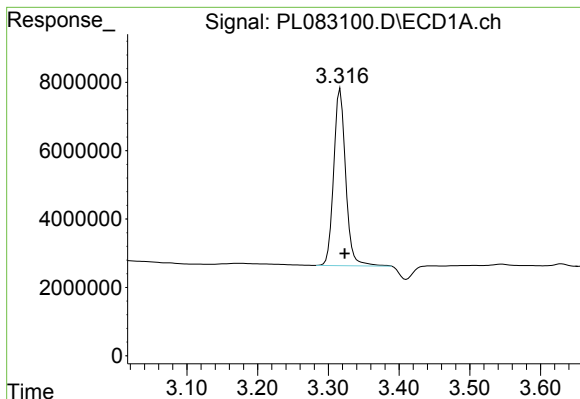

#1 Tetrachloro-m-xylene


R.T.: 3.317 min
Delta R.T.: -0.006 min
Response: 60868340
Conc: 20.71 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB16

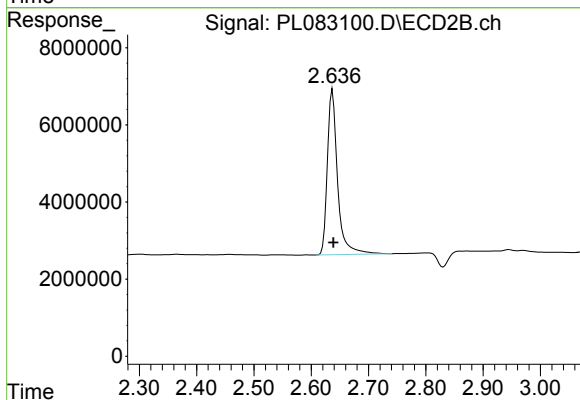


#1 Tetrachloro-m-xylene

R.T.: 2.637 min
Delta R.T.: -0.002 min
Response: 53335692
Conc: 20.54 ng/ml

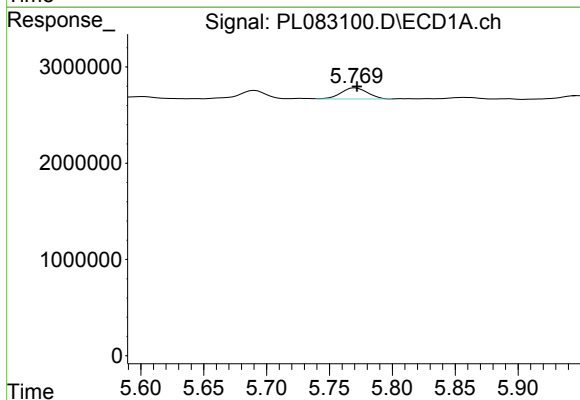


#11 alpha-Chlordane

R.T.: 5.771 min
Delta R.T.: -0.001 min
Response: 1680612
Conc: 0.52 ng/ml

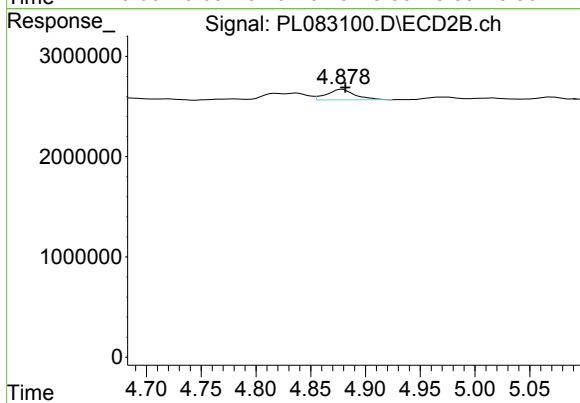

#11 alpha-Chlordane


R.T.: 4.879 min
Delta R.T.: -0.003 min
Response: 1878986
Conc: 0.63 ng/ml

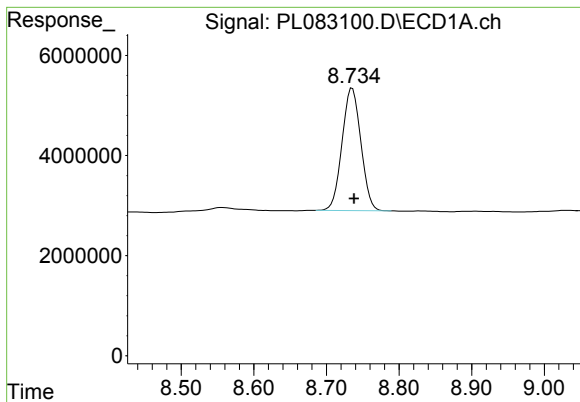

#28 Decachlorobiphenyl

R.T.: 8.736 min
Delta R.T.: -0.002 min
Response: 44099988
Conc: 21.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB16

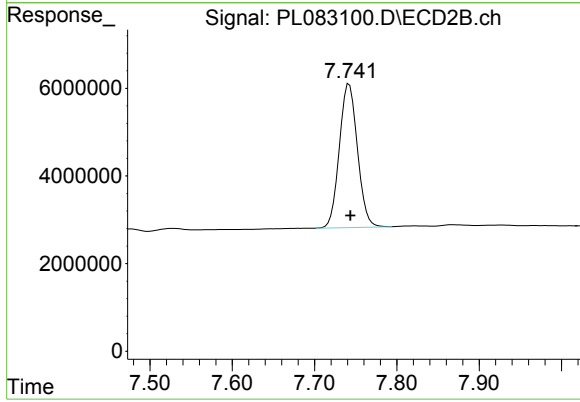

#28 Decachlorobiphenyl

R.T.: 7.742 min
Delta R.T.: -0.001 min
Response: 50240825
Conc: 20.21 ng/ml