

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL053025\
 Data File : PL095833.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 May 2025 08:16
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 30 22:49:41 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052125.M
 Quant Title : GC Extractables
 QLast Update : Thu May 22 06:29:30 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

8) B	Heptachlo...	5.715	0.000	4609616	0	1.208	N.D.	#
13) MA	Dieldrin	0.000	5.524f	0	18637277	N.D.	3.516	#
14) MA	Endrin	0.000	5.785	0	8515645	N.D.	1.746	#
16) A	4,4'-DDD	6.747	0.000	16754374	0	5.717	N.D.	#
24)	Chlordane-2	0.000	4.476	0	17983245	N.D.	80.732	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL053025\
Data File : PL095833.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 May 2025 08:16
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 30 22:49:41 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052125.M
Quant Title : GC Extractables
QLast Update : Thu May 22 06:29:30 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

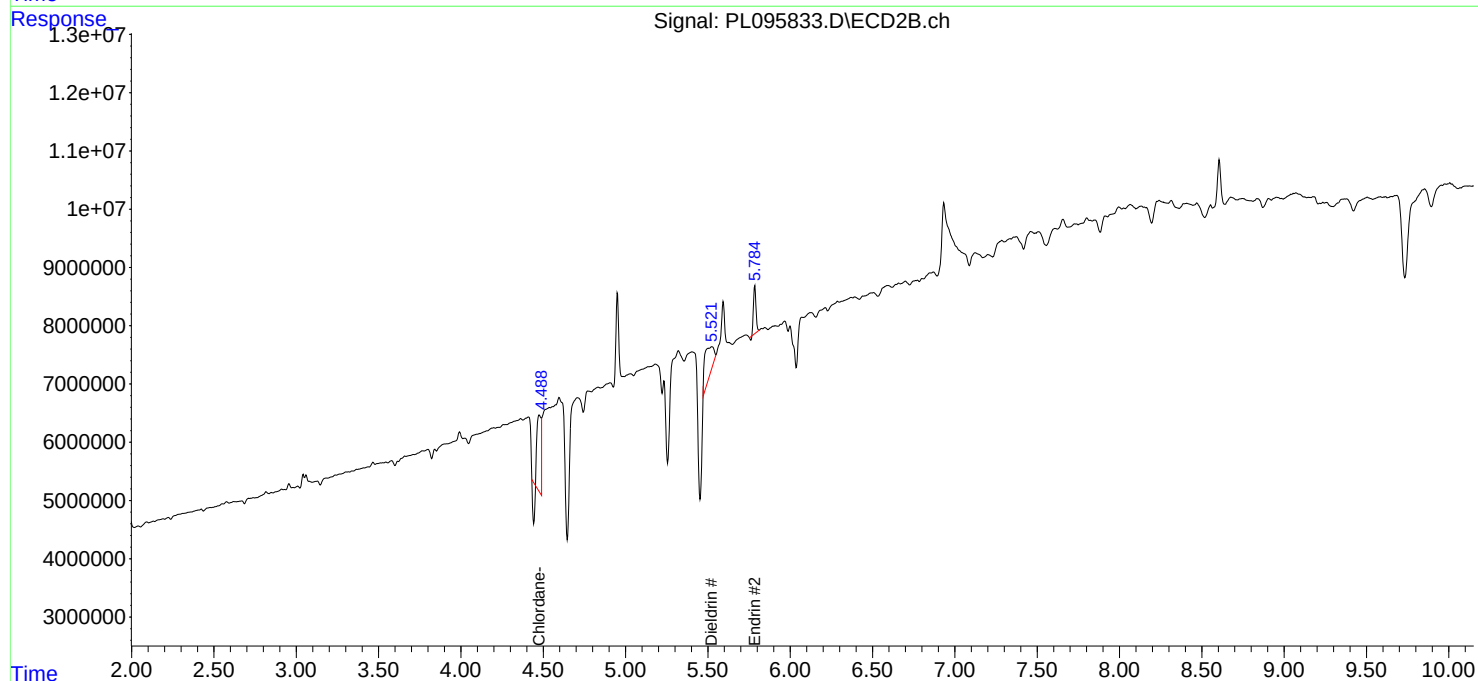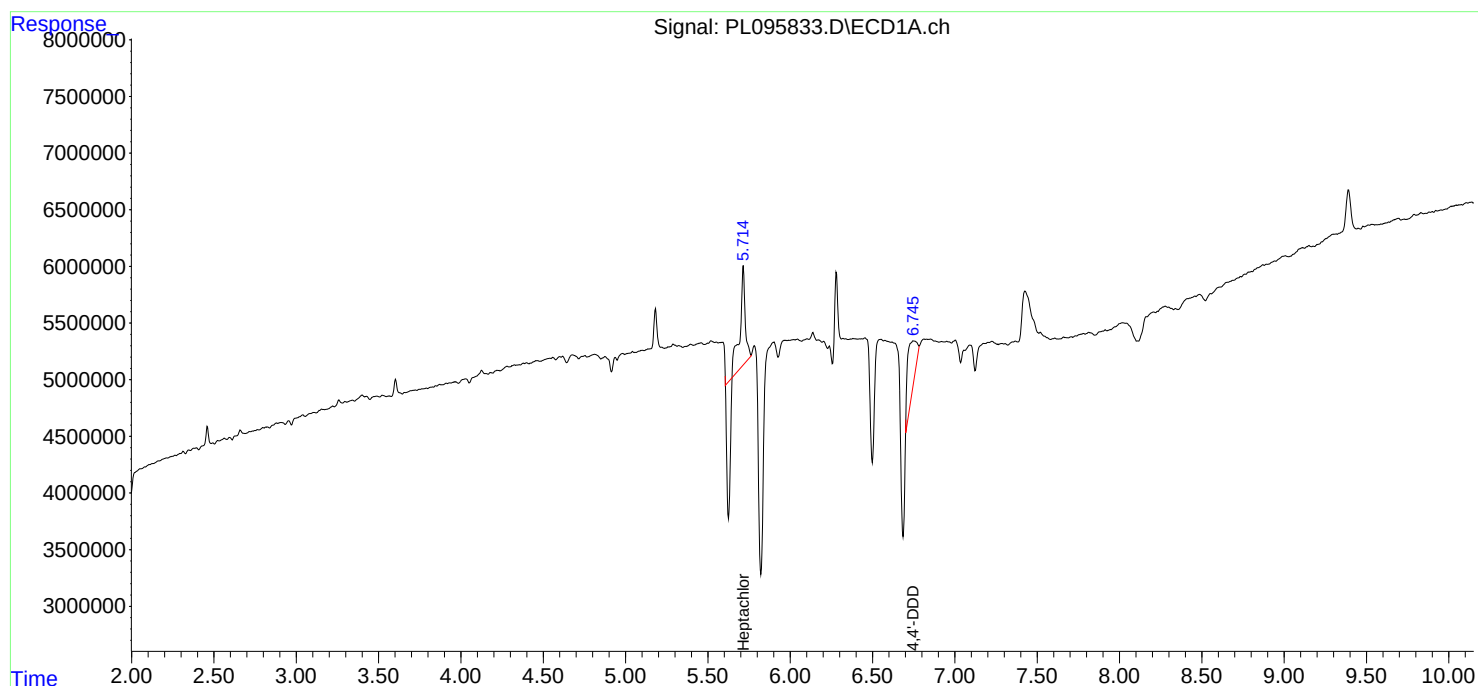


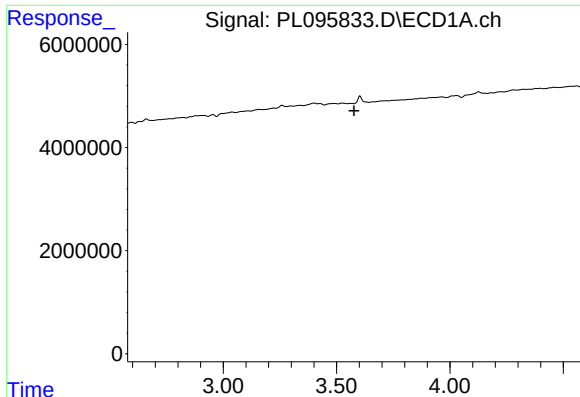

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.577 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

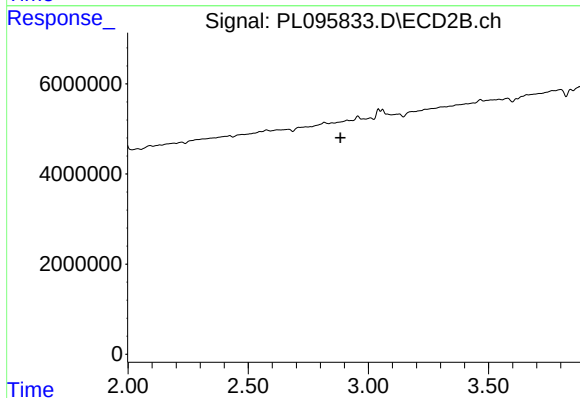


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 2.883 min
Response: 0
Conc: N.D.

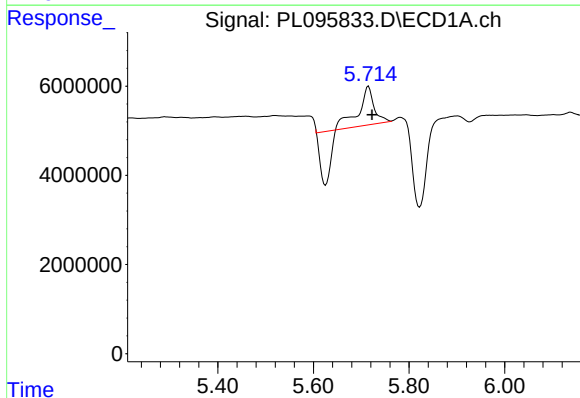


#8 Heptachlor epoxide

R.T.: 5.715 min
Delta R.T.: -0.007 min
Response: 4609616
Conc: 1.21 ng/ml

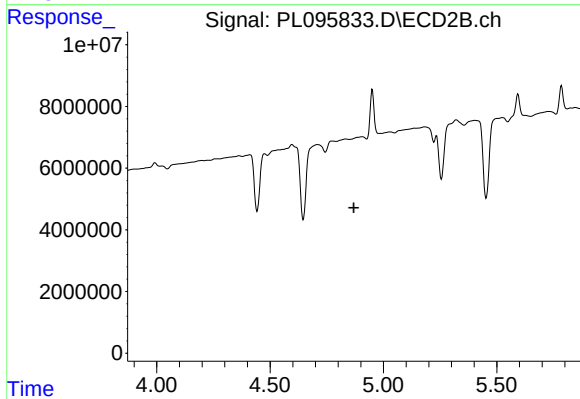

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.869 min
Response: 0
Conc: N.D.

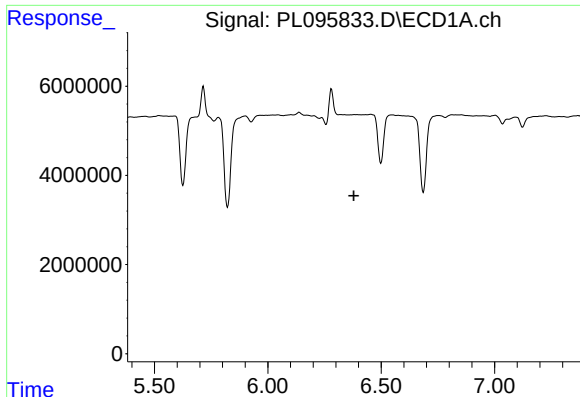

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 6.379 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

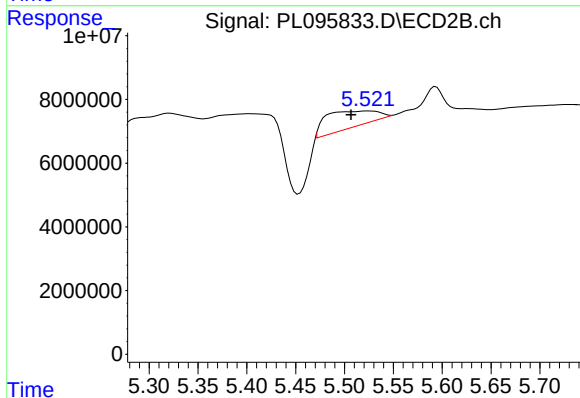


#13 Dieldrin

R.T.: 5.524 min
Delta R.T.: 0.017 min
Response: 18637277
Conc: 3.52 ng/ml

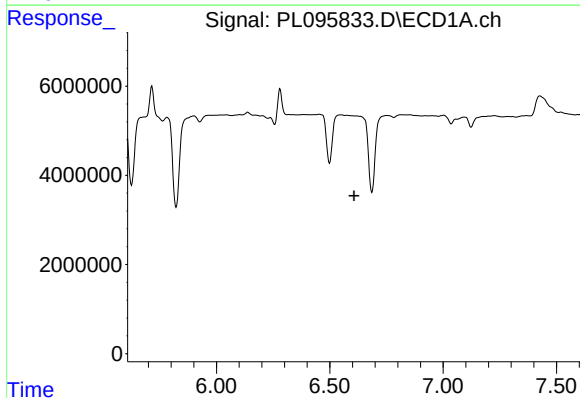


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.607 min
Response: 0
Conc: N.D.

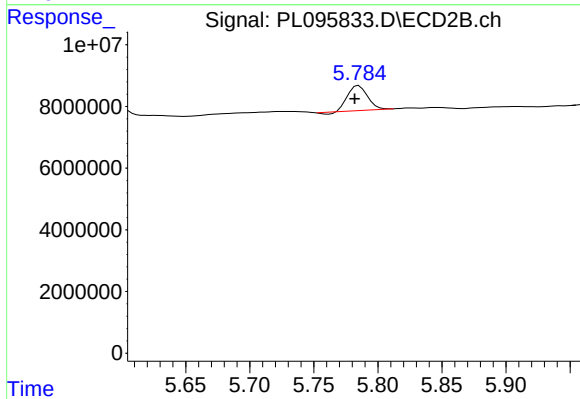

#14 Endrin


R.T.: 5.785 min
Delta R.T.: 0.003 min
Response: 8515645
Conc: 1.75 ng/ml

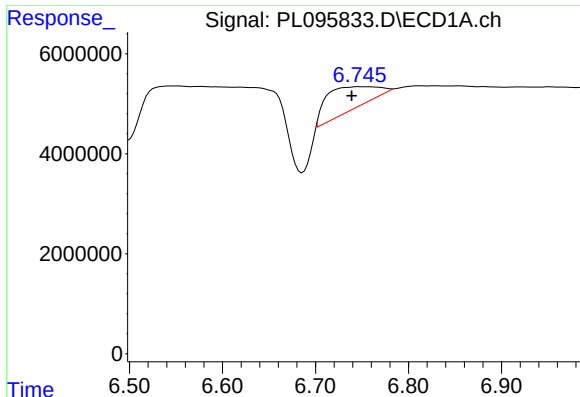

#16 4,4'-DDD


R.T.: 6.747 min
Delta R.T.: 0.008 min
Response: 16754374
Conc: 5.72 ng/ml

Instrument :
ECD_L
ClientSampleId :

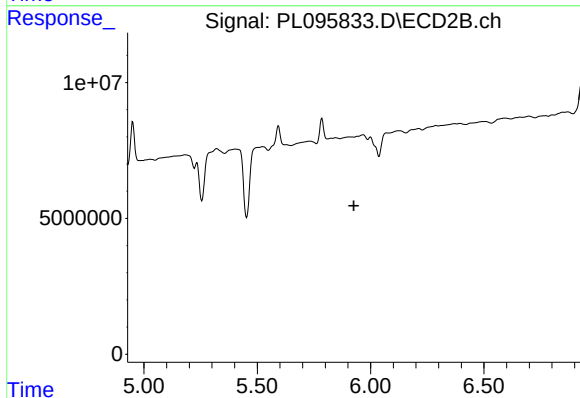


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.926 min
Response: 0
Conc: N.D.

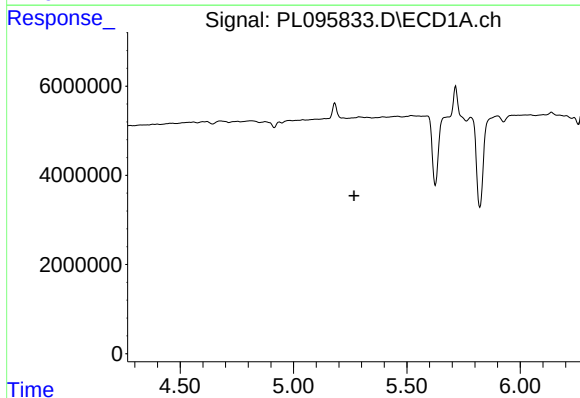


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.267 min
Response: 0
Conc: N.D.

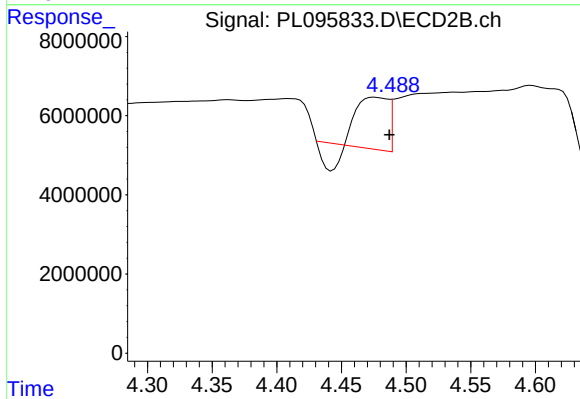

#24 Chlordane-2


R.T.: 4.476 min
Delta R.T.: -0.011 min
Response: 17983245
Conc: 80.73 ng/ml

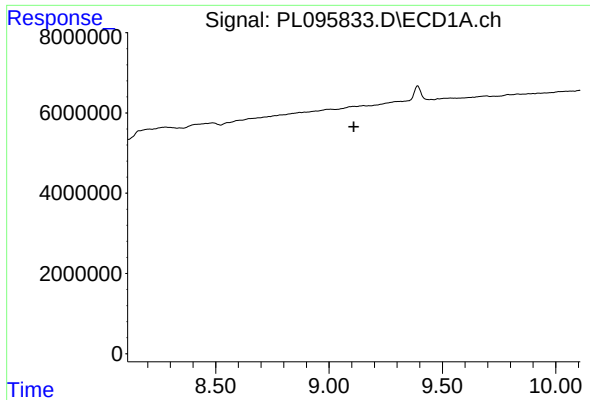

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.109 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

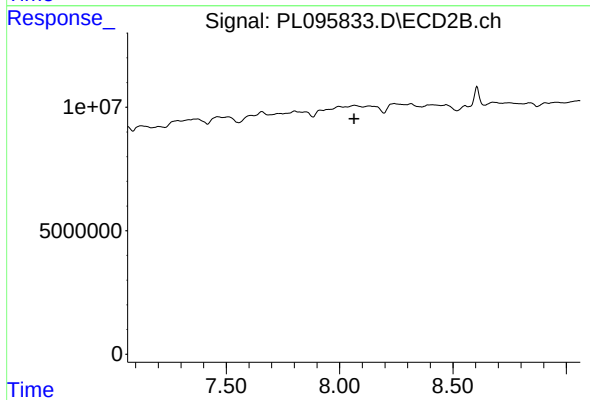

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.064 min
Response: 0
Conc: N.D.