

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL053119\
 Data File : PL049139.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 May 2019 14:04
 Operator : SM\AJ
 Sample : K3097-21
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 0441-PR-4(PASSAIC)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 31 23:11:18 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL053019.M
 Quant Title : GC Extractables
 QLast Update : Fri May 31 01:35:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.324	3.937	180.7E6	47783045	16.401	16.539
28) SA Decachlor...	7.993	8.973	90930336	33736766	7.151	10.102 #
Target Compounds						
6) B beta-BHC	0.000	4.765f	0	1236577	N.D.	0.718 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL053119\
Data File : PL049139.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 May 2019 14:04
Operator : SM\AJ
Sample : K3097-21
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
0441-PR-4(PASSAIC)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 31 23:11:18 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL053019.M
Quant Title : GC Extractables
QLast Update : Fri May 31 01:35:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

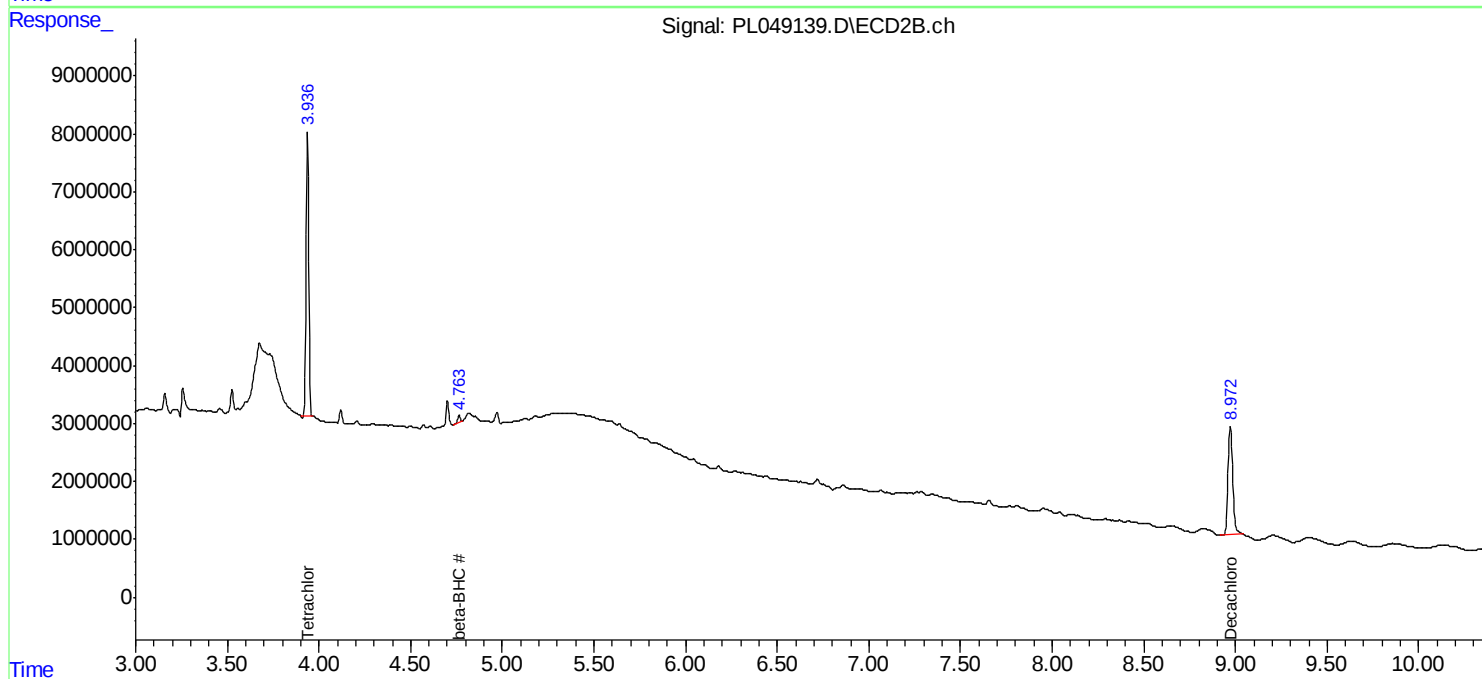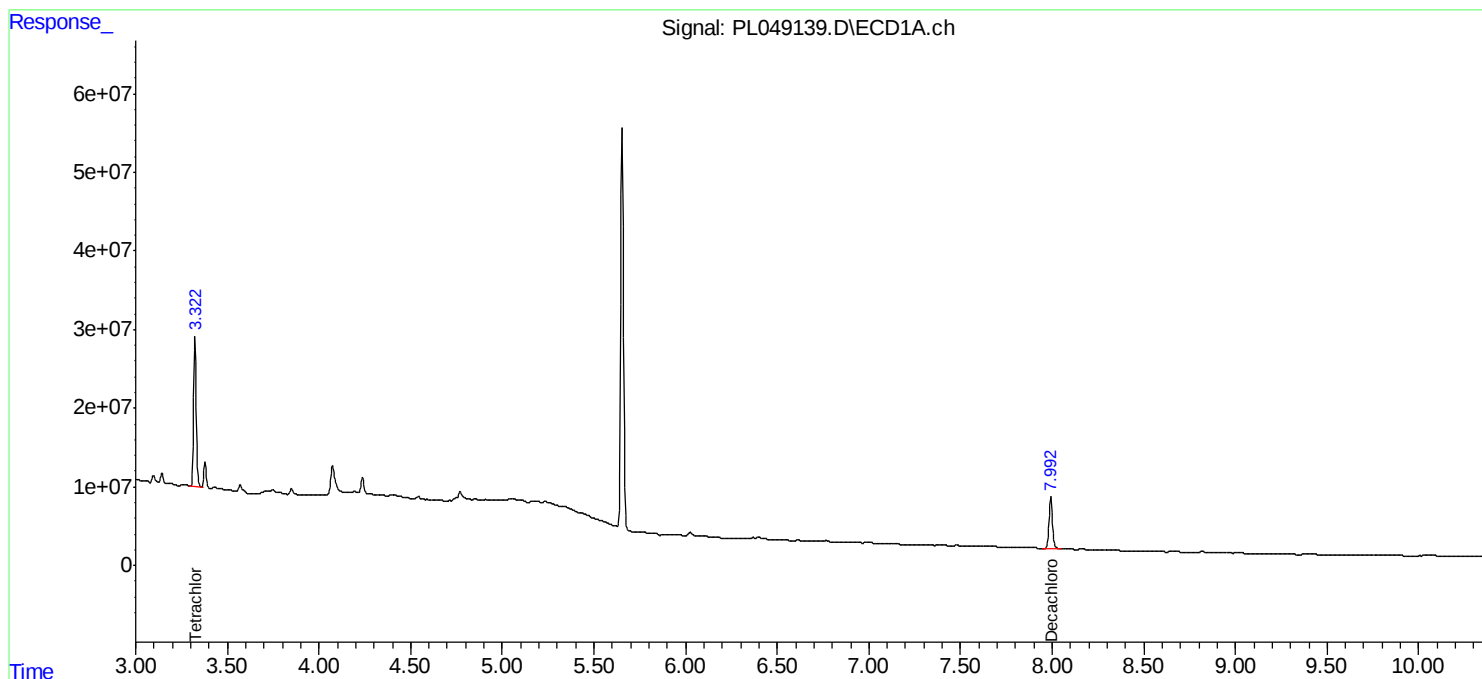


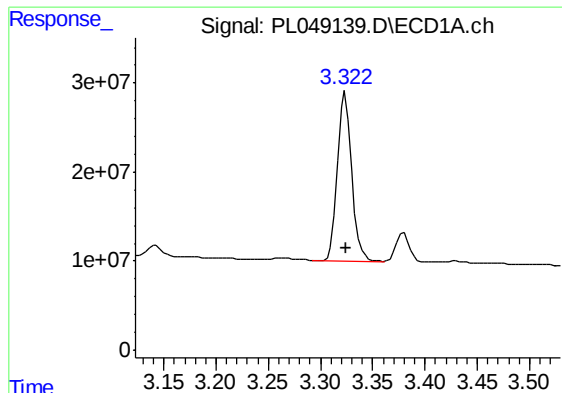

#1 Tetrachloro-m-xylene


R.T.: 3.324 min
Delta R.T.: 0.000 min
Response: 180716660
Conc: 16.40 ng/ml

Instrument :
ECD_L
ClientSampleId :
0441-PR-4(PASSAIC)

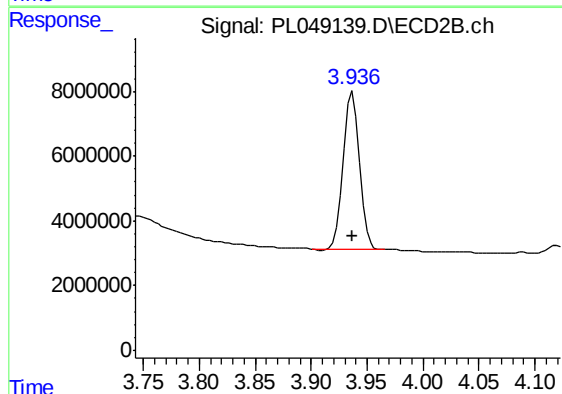


#1 Tetrachloro-m-xylene

R.T.: 3.937 min
Delta R.T.: 0.000 min
Response: 47783045
Conc: 16.54 ng/ml

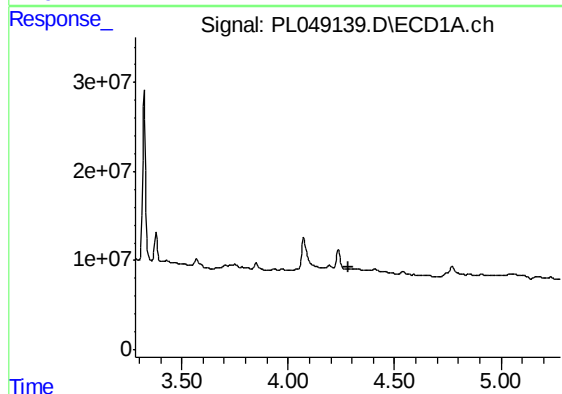


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.282 min
Response: 0
Conc: N.D.

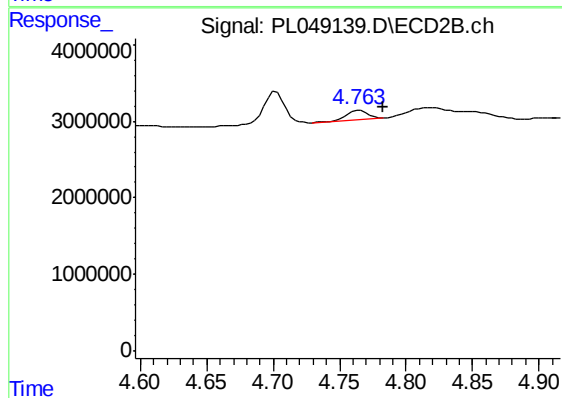

#6 beta-BHC


R.T.: 4.765 min
Delta R.T.: -0.018 min
Response: 1236577
Conc: 0.72 ng/ml

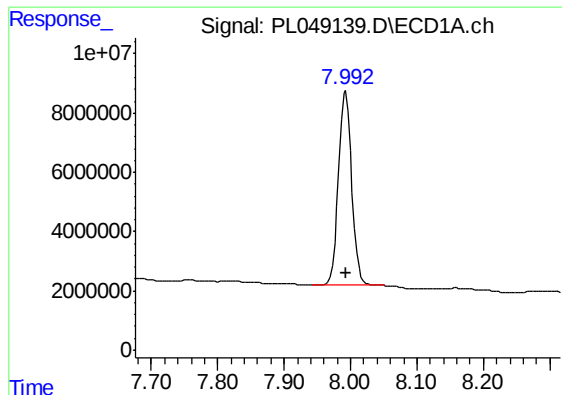

#28 Decachlorobiphenyl

R.T.: 7.993 min
Delta R.T.: 0.000 min
Response: 90930336
Conc: 7.15 ng/ml

Instrument :
ECD_L
ClientSampleId :
0441-PR-4(PASSAIC)

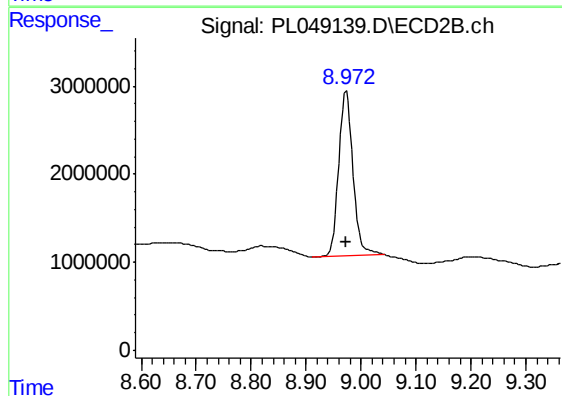

#28 Decachlorobiphenyl

R.T.: 8.973 min
Delta R.T.: 0.001 min
Response: 33736766
Conc: 10.10 ng/ml