

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL053119\
 Data File : PL049140.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 May 2019 14:18
 Operator : SM\AJ
 Sample : K3097-22
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 0442-PR-5(PASSAIC)

Manual Integrations
 APPROVED

Ankita
 6/3/2019 2:17:15 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 31 23:11:31 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL053019.M
 Quant Title : GC Extractables
 QLast Update : Fri May 31 01:35:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.324	3.935	90911068	24559415	8.251	8.501m
28)	SA Decachlor...	7.993	8.973	62067870	22552208	4.881	6.753 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL053119\
Data File : PL049140.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 May 2019 14:18
Operator : SM\AJ
Sample : K3097-22
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
0442-PR-5(PASSAIC)


Manual Integrations
APPROVED

Ankita
6/3/2019 2:17:15 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 31 23:11:31 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL053019.M
Quant Title : GC Extractables
QLast Update : Fri May 31 01:35:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

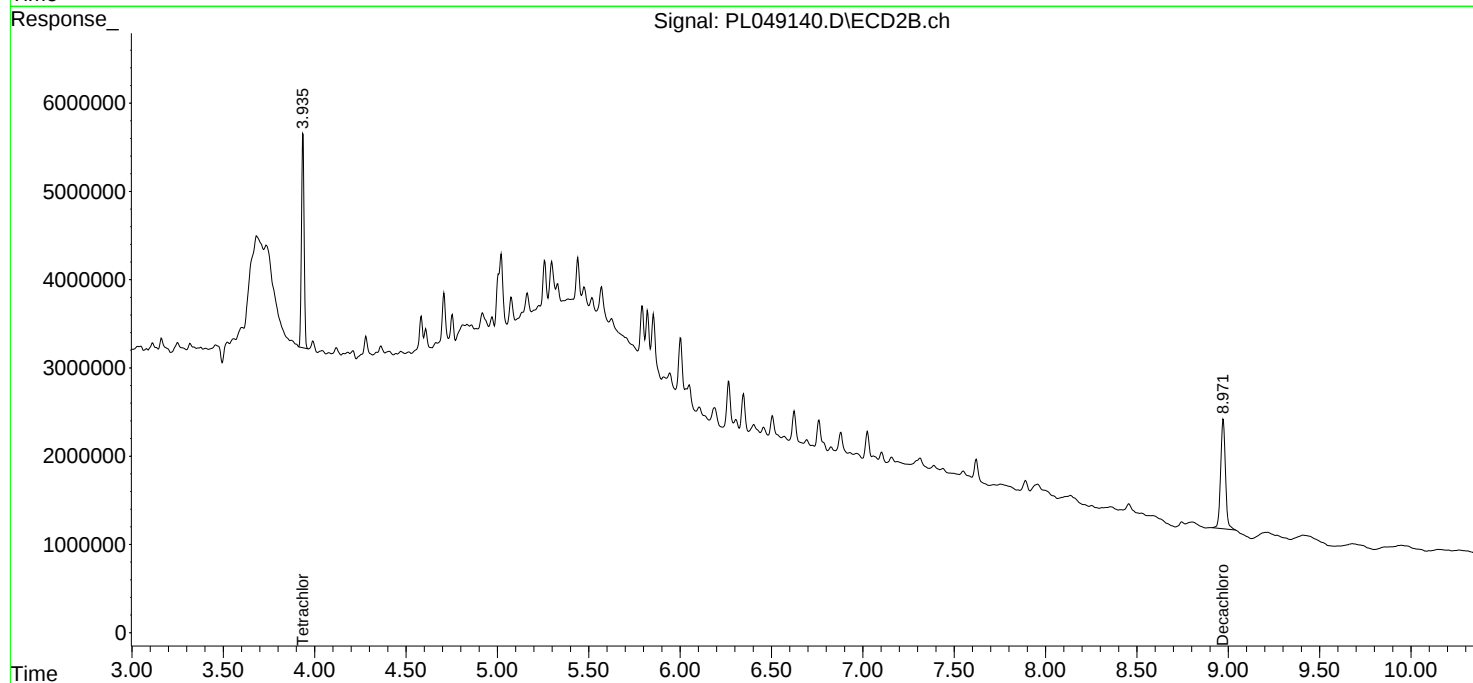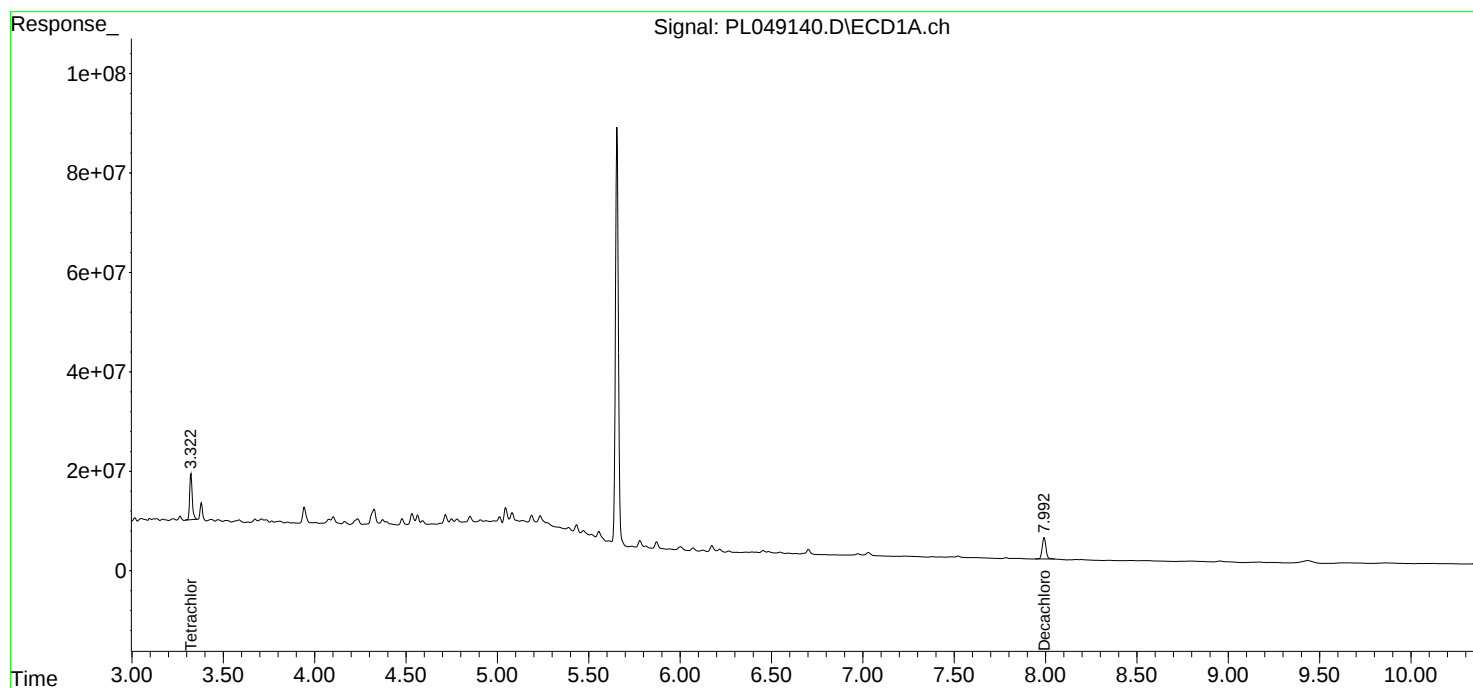

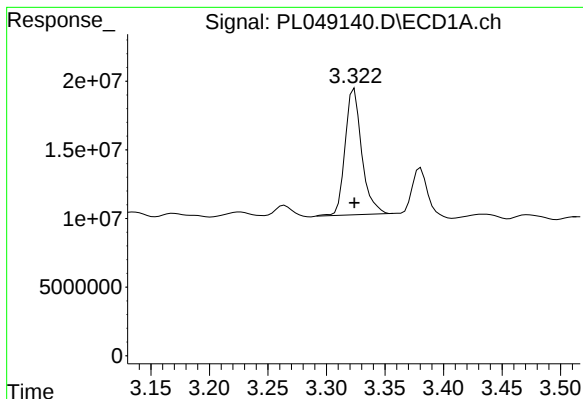


#1 Tetrachloro-m-xylene

R.T.: 3.324 min
Delta R.T.: 0.000 min
Response: 90911068
Conc: 8.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
0442-PR-5(PASSAIC)


Manual Integrations
APPROVED

Ankita
6/3/2019 2:17:15 PM

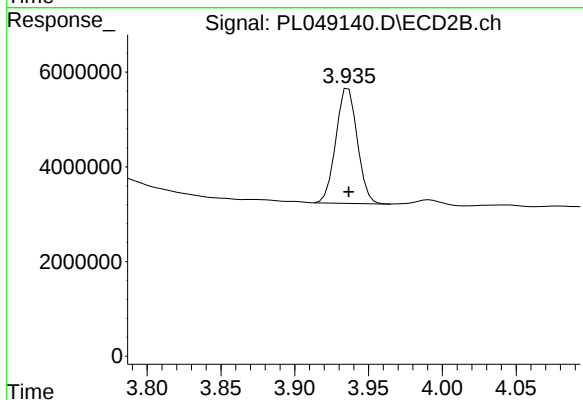


#1 Tetrachloro-m-xylene

R.T.: 3.935 min
Delta R.T.: -0.002 min
Response: 24559415
Conc: 8.50 ng/ml m

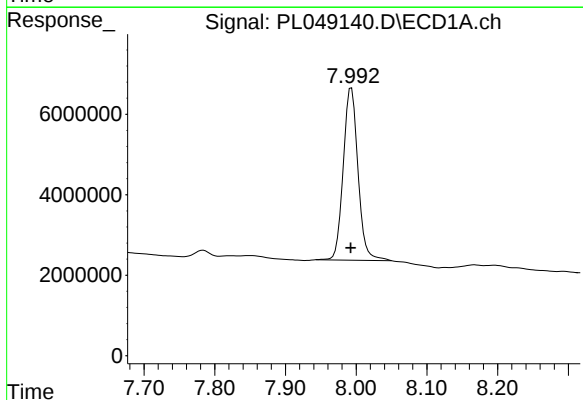

#28 Decachlorobiphenyl

R.T.: 7.993 min
Delta R.T.: 0.000 min
Response: 62067870
Conc: 4.88 ng/ml

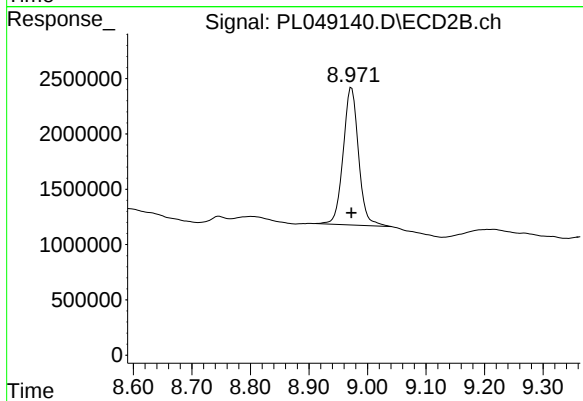

#28 Decachlorobiphenyl

R.T.: 8.973 min
Delta R.T.: 0.000 min
Response: 22552208
Conc: 6.75 ng/ml