

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL053119\
 Data File : PL049141.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 May 2019 14:33
 Operator : SM\AJ
 Sample : K3097-23
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 0443-PR-6(PASSAIC)

Manual Integrations
 APPROVED

Ankita
 6/3/2019 2:17:17 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 31 23:11:45 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL053019.M
 Quant Title : GC Extractables
 QLast Update : Fri May 31 01:35:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.322	3.935	83963691	23198819	7.620m	8.030m
28) SA Decachlor...	7.993	8.973	72280506	22602714	5.684	6.768

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL053119\
Data File : PL049141.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 May 2019 14:33
Operator : SM\AJ
Sample : K3097-23
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
0443-PR-6(PASSAIC)


Manual Integrations
APPROVED

Ankita
6/3/2019 2:17:17 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 31 23:11:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL053019.M
Quant Title : GC Extractables
QLast Update : Fri May 31 01:35:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

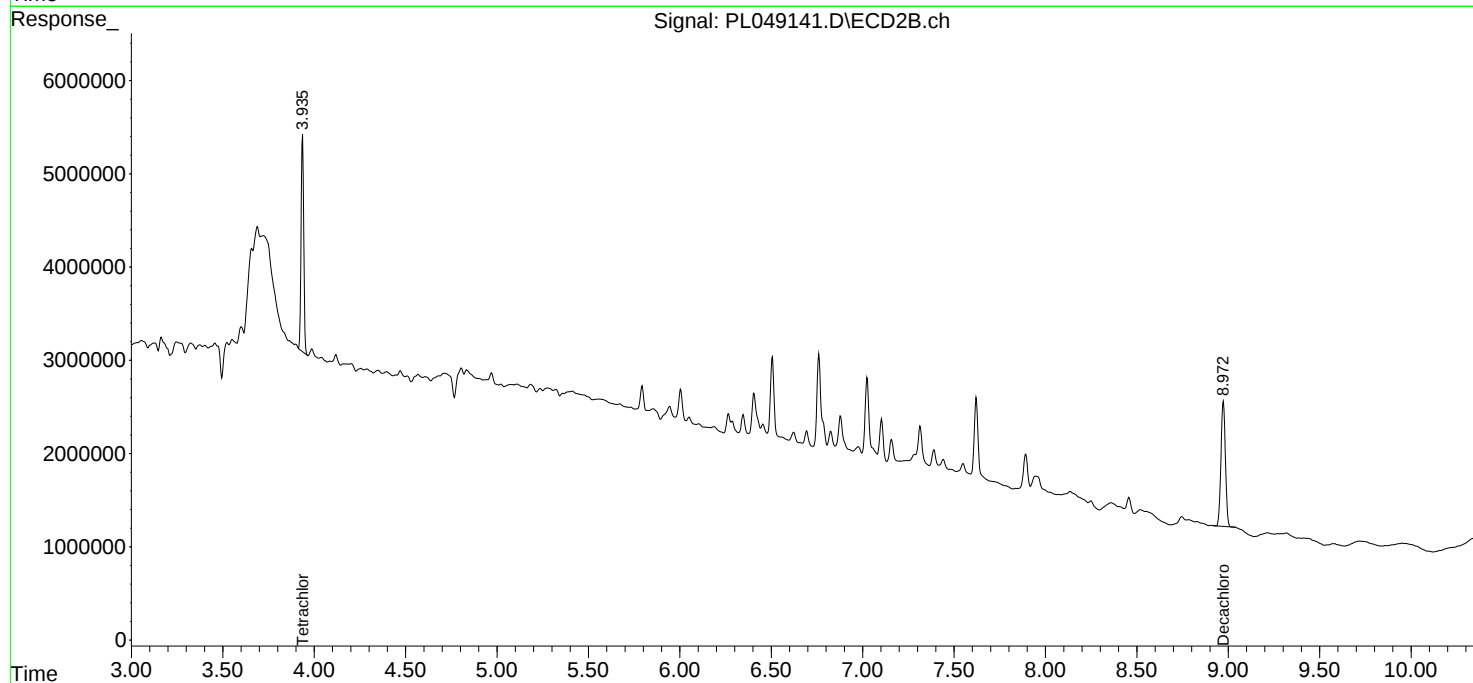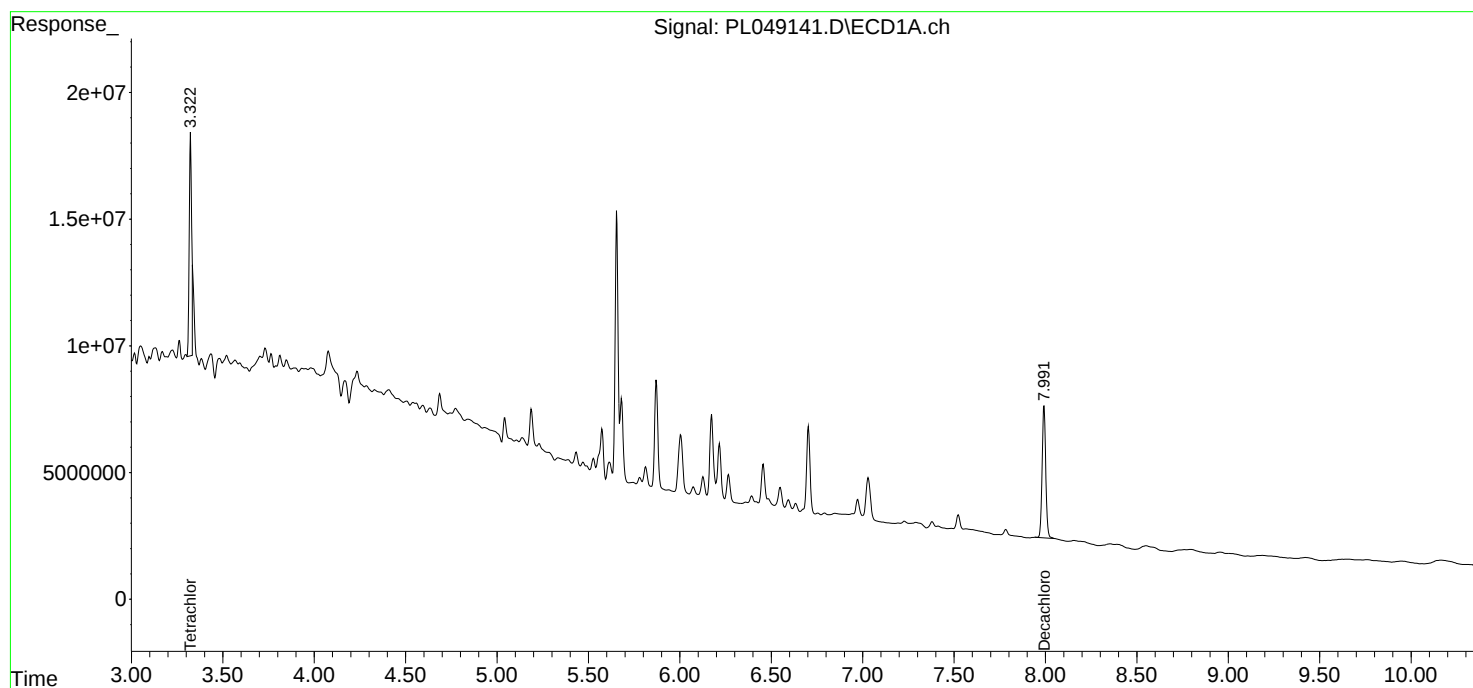

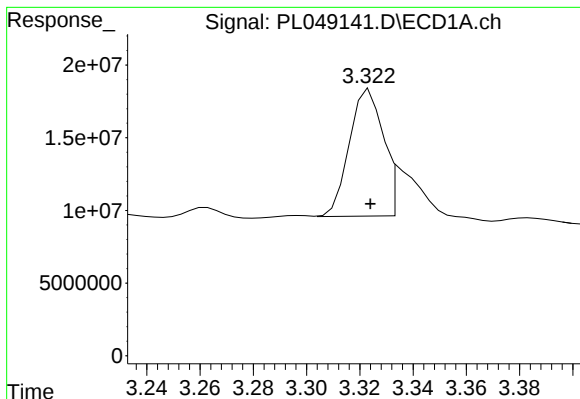


#1 Tetrachloro-m-xylene

R.T.: 3.322 min
Delta R.T.: -0.002 min
Response: 83963691
Conc: 7.62 ng/ml m

Instrument :
ECD_L
ClientSampleId :
0443-PR-6(PASSAIC)


Manual Integrations
APPROVED

Ankita
6/3/2019 2:17:17 PM

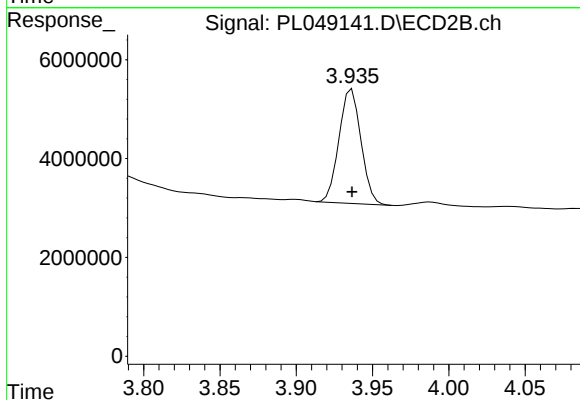


#1 Tetrachloro-m-xylene

R.T.: 3.935 min
Delta R.T.: -0.001 min
Response: 23198819
Conc: 8.03 ng/ml m

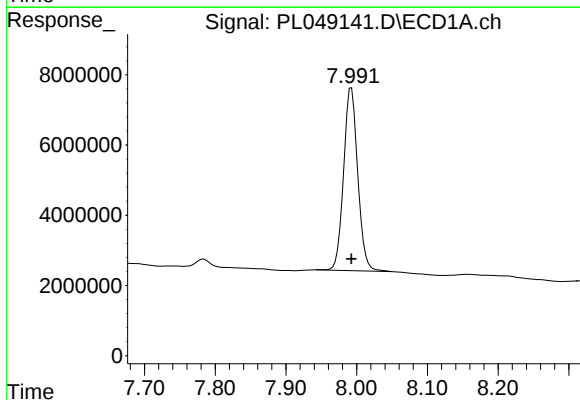

#28 Decachlorobiphenyl

R.T.: 7.993 min
Delta R.T.: 0.000 min
Response: 72280506
Conc: 5.68 ng/ml

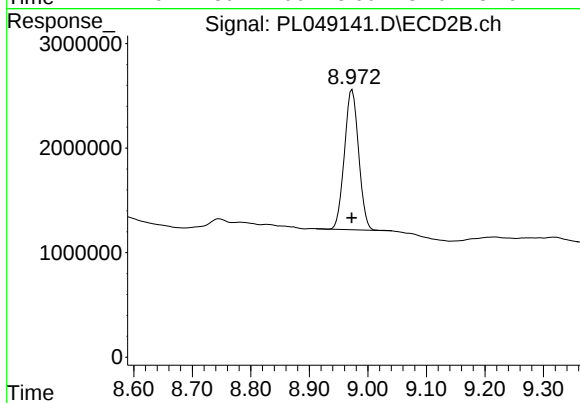

#28 Decachlorobiphenyl

R.T.: 8.973 min
Delta R.T.: 0.000 min
Response: 22602714
Conc: 6.77 ng/ml