

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL053122\
 Data File : PL075288.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 May 2022 15:17
 Operator : AR\AJ
 Sample : N3042-05
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 31 15:34:27 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
 Quant Title : GC Extractables
 QLast Update : Tue May 31 02:52:42 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.640	4.639	3250418	8742284	5.530	5.519
28)	SA Decachlor...	11.639	10.388	2262831	5235721	4.220	3.815
Target Compounds							
7)	B delta-BHC	0.000	6.401	0	135324	N.D.	0.063 #
11)	B alpha-Chl...	0.000	7.405	0	141343	N.D.	0.077 #
14)	MA Endrin	0.000	8.069f	0	447152	N.D.	0.287 #
15)	B Endosulfa...	9.305	0.000	108568	0	0.192	N.D. #
16)	A 4,4'-DDD	9.201	0.000	138303	0	0.280	N.D. #
17)	MA 4,4'-DDT	0.000	8.466	0	391592	N.D.	0.274 #
19)	B Endosulfa...	0.000	8.776	0	425059	N.D.	0.284 #
21)	B Endrin ke...	10.186f	0.000	237297	0	0.387	N.D. #
23)	Chlordane-1	0.000	5.954	0	78413	N.D.	1.376 #
26)	Chlordane-4	0.000	7.405	0	141343	N.D.	0.729 #
27)	Chlordane-5	0.000	8.128	0	363365	N.D.	7.053 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL053122\
Data File : PL075288.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 May 2022 15:17
Operator : AR\AJ
Sample : N3042-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 31 15:34:27 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
Quant Title : GC Extractables
QLast Update : Tue May 31 02:52:42 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

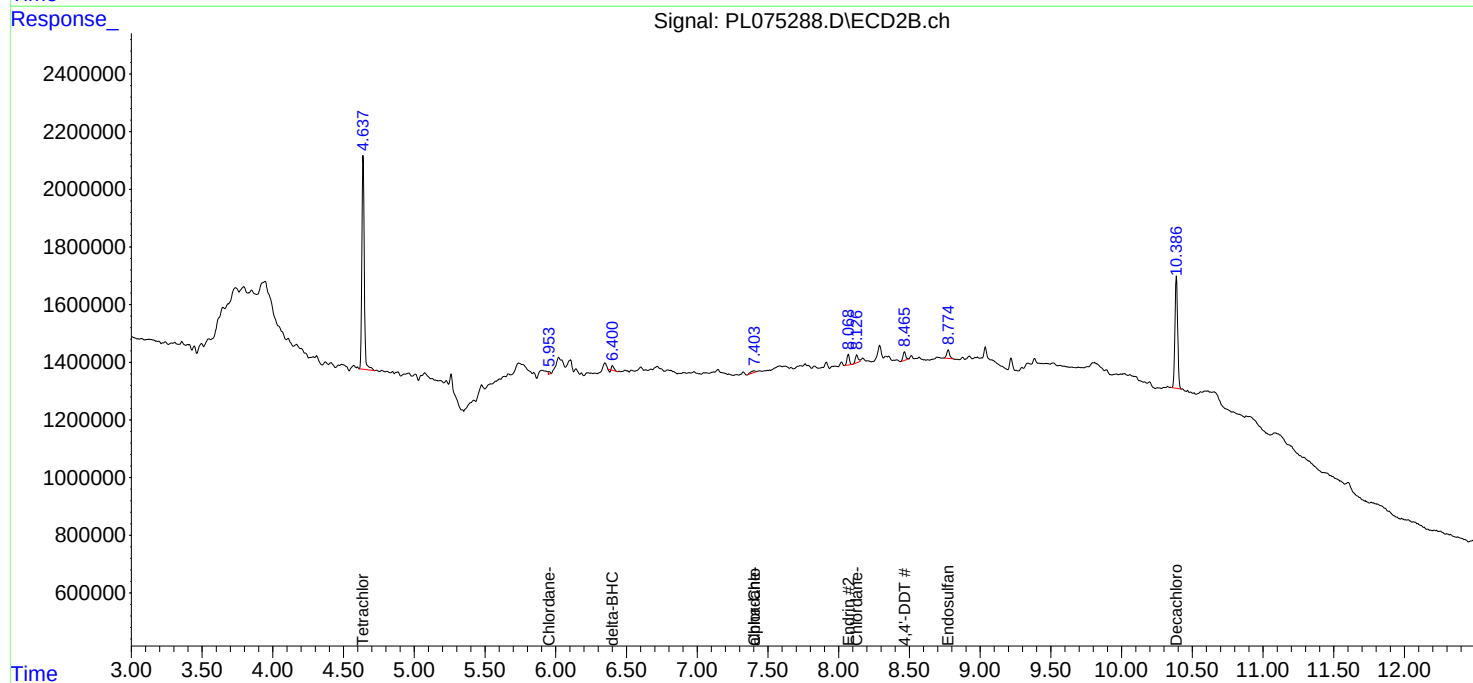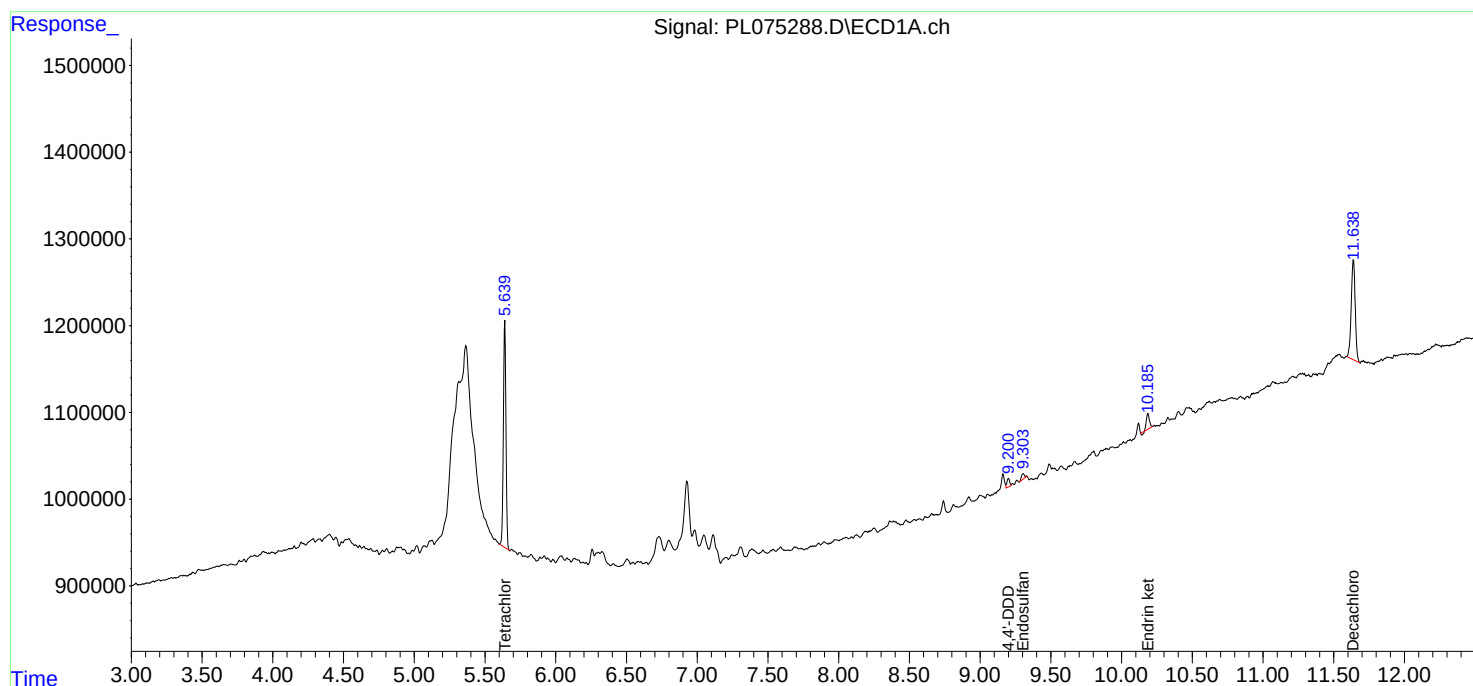


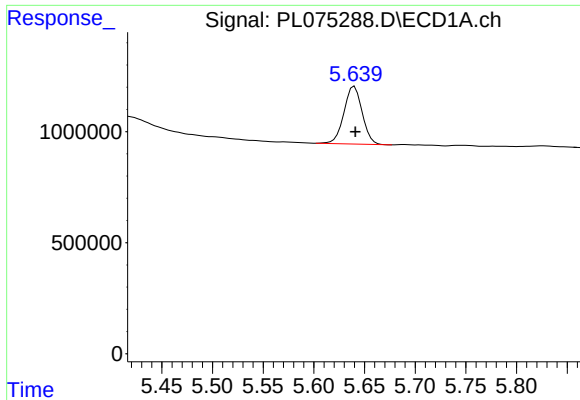

#1 Tetrachloro-m-xylene


R.T.: 5.640 min
Delta R.T.: 0.000 min
Response: 3250418
Conc: 5.53 ng/ml

Instrument :
ECD_L
ClientSampleId :

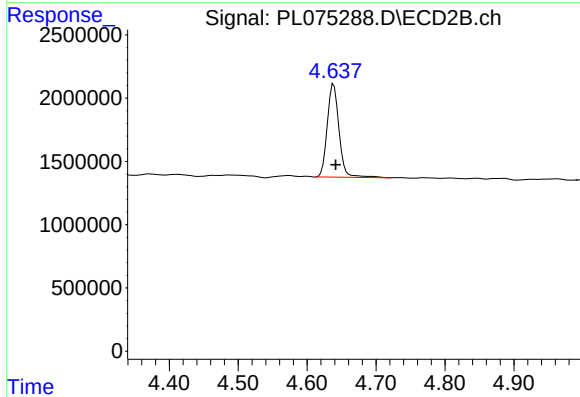


#1 Tetrachloro-m-xylene

R.T.: 4.639 min
Delta R.T.: -0.003 min
Response: 8742284
Conc: 5.52 ng/ml

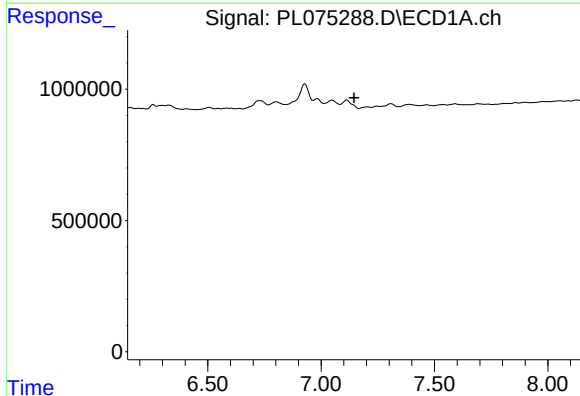


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 7.146 min
Response: 0
Conc: N.D.

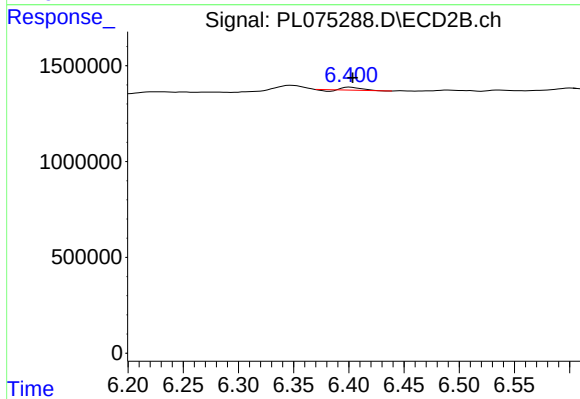

#7 delta-BHC


R.T.: 6.401 min
Delta R.T.: -0.002 min
Response: 135324
Conc: 0.06 ng/ml

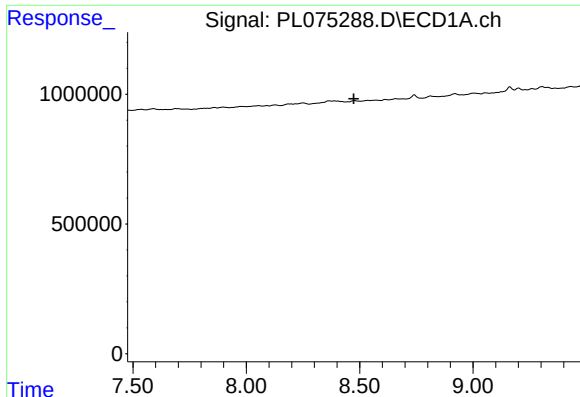

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 8.474 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

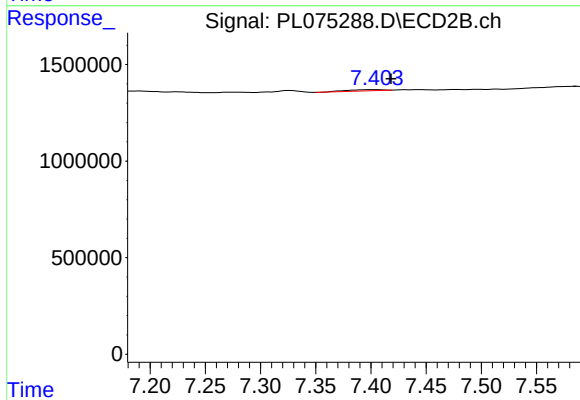


#11 alpha-Chlordane

R.T.: 7.405 min
Delta R.T.: -0.013 min
Response: 141343
Conc: 0.08 ng/ml

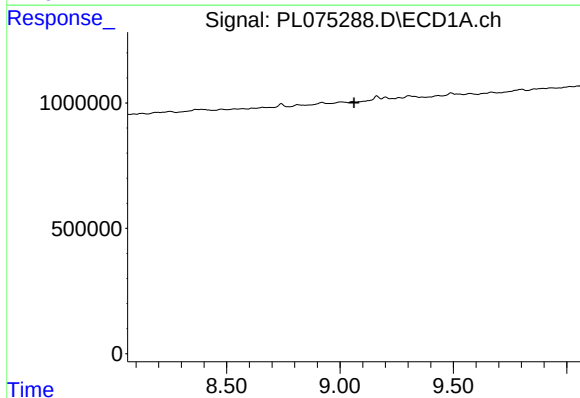


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 9.062 min
Response: 0
Conc: N.D.

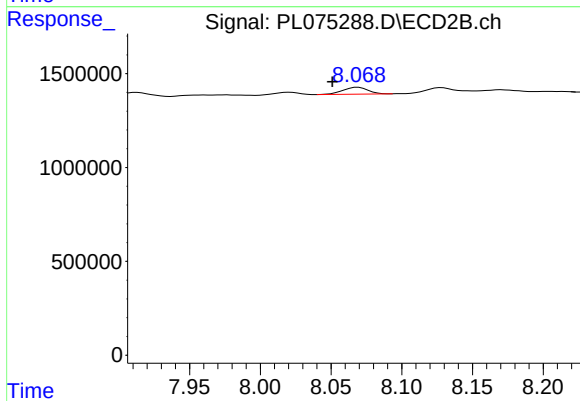

#14 Endrin


R.T.: 8.069 min
Delta R.T.: 0.018 min
Response: 447152
Conc: 0.29 ng/ml

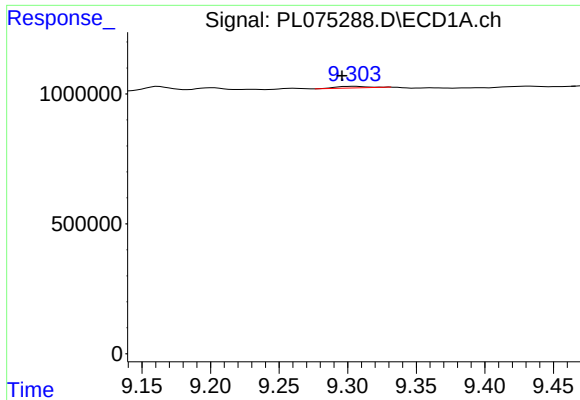

#15 Endosulfan II


R.T.: 9.305 min
Delta R.T.: 0.009 min
Response: 108568
Conc: 0.19 ng/ml

Instrument :
ECD_L
ClientSampleId :

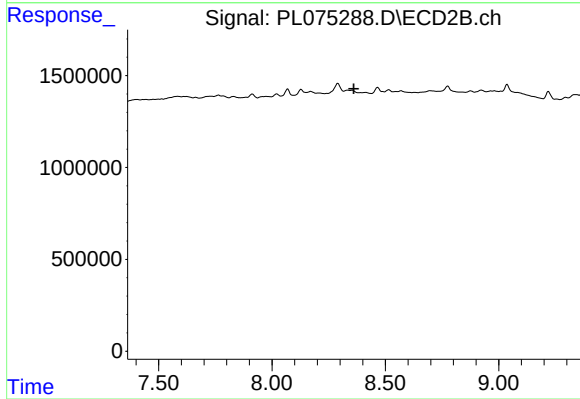


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.361 min
Response: 0
Conc: N.D.

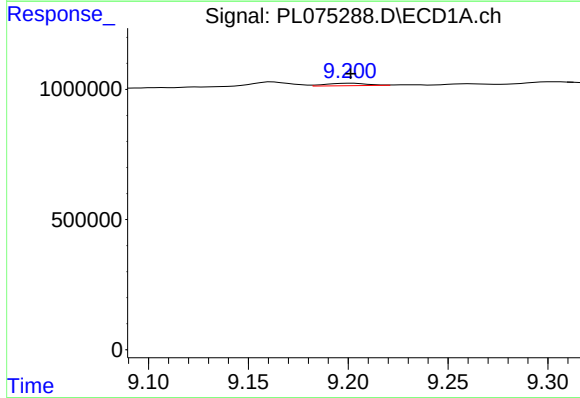


#16 4,4'-DDD

R.T.: 9.201 min
Delta R.T.: 0.000 min
Response: 138303
Conc: 0.28 ng/ml

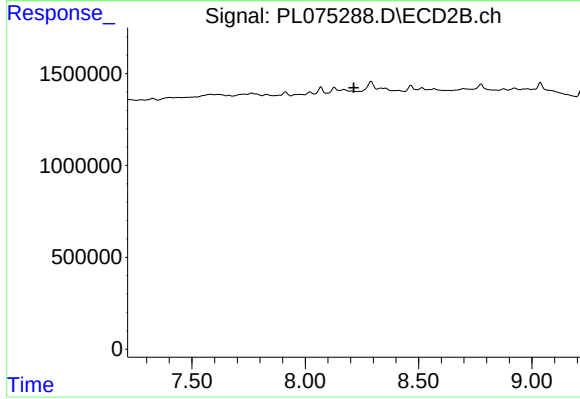

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 8.215 min
Response: 0
Conc: N.D.

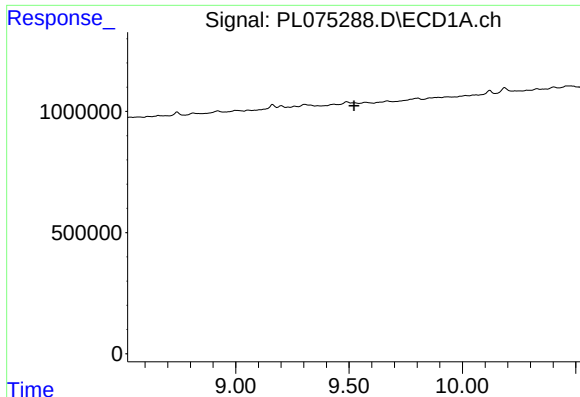

#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 9.522 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

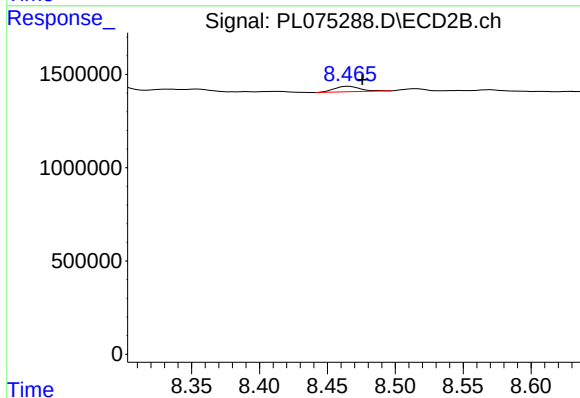

#17 4,4'-DDT


R.T.: 8.466 min
Delta R.T.: -0.010 min
Response: 391592
Conc: 0.27 ng/ml

#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 9.669 min
Response: 0
Conc: N.D.

#19 Endosulfan Sulfate


R.T.: 8.776 min
Delta R.T.: -0.003 min
Response: 425059
Conc: 0.28 ng/ml

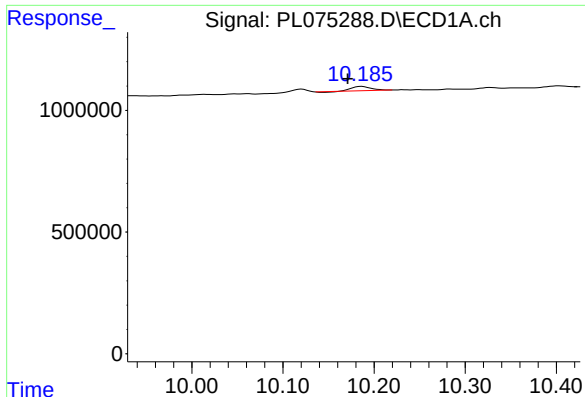

#21 Endrin ketone


R.T.: 10.186 min
Delta R.T.: 0.015 min
Response: 237297
Conc: 0.39 ng/ml

Instrument :
ECD_L
ClientSampleId :

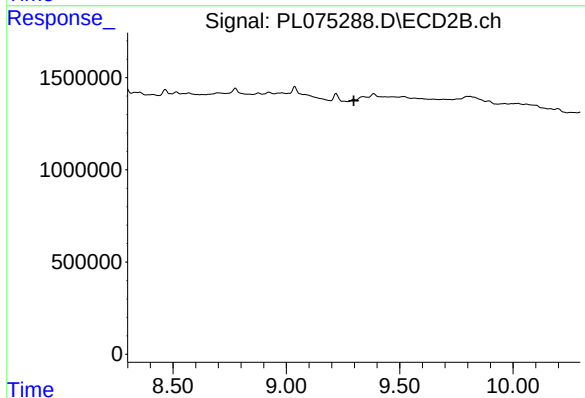


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.298 min
Response: 0
Conc: N.D.

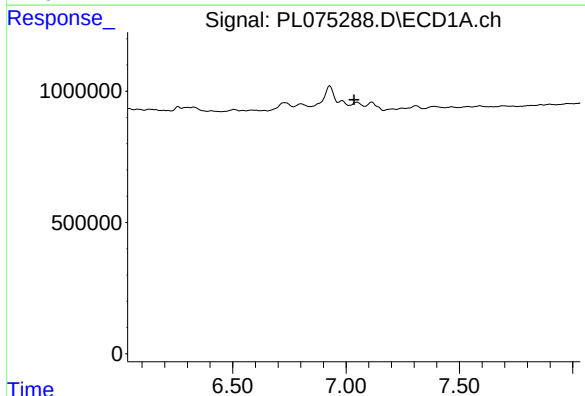


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 7.036 min
Response: 0
Conc: N.D.

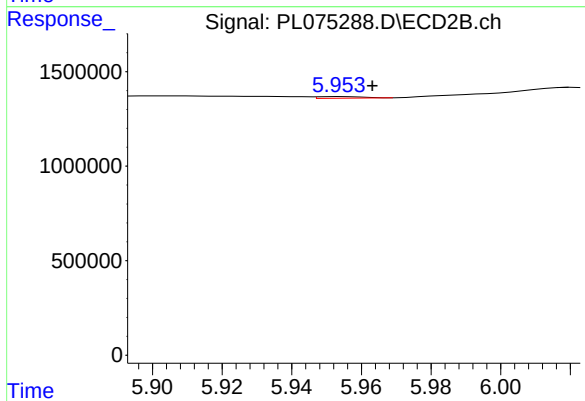

#23 Chlordane-1


R.T.: 5.954 min
Delta R.T.: -0.009 min
Response: 78413
Conc: 1.38 ng/ml

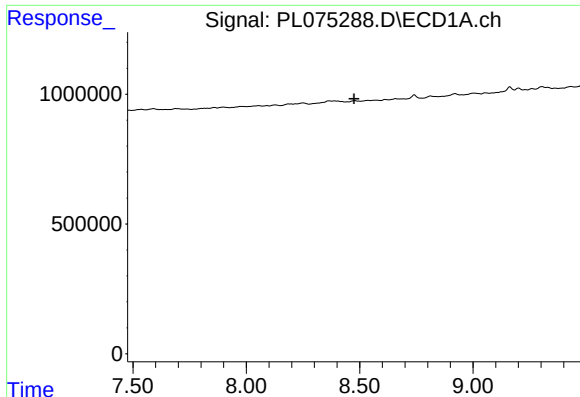

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 8.476 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

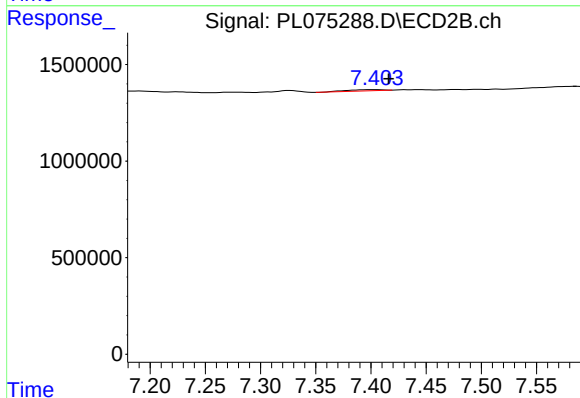


#26 Chlordane-4

R.T.: 7.405 min
Delta R.T.: -0.011 min
Response: 141343
Conc: 0.73 ng/ml

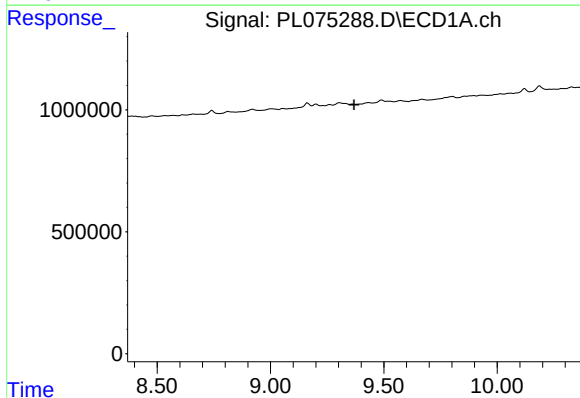


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 9.369 min
Response: 0
Conc: N.D.

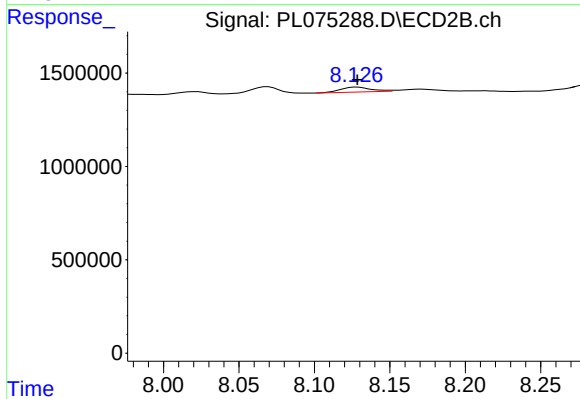

#27 Chlordane-5


R.T.: 8.128 min
Delta R.T.: 0.000 min
Response: 363365
Conc: 7.05 ng/ml

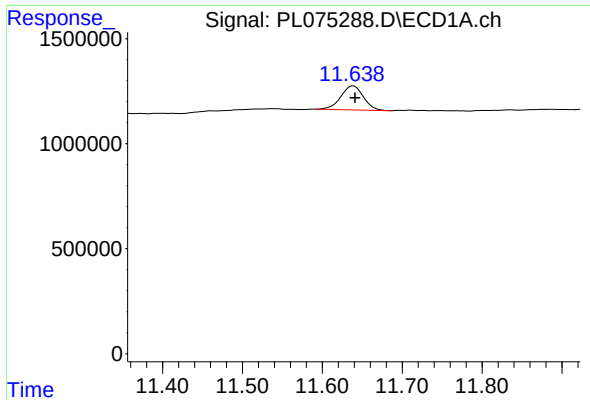

#28 Decachlorobiphenyl

R.T.: 11.639 min
Delta R.T.: -0.002 min
Response: 2262831
Conc: 4.22 ng/ml

Instrument :
ECD_L
ClientSampleId :

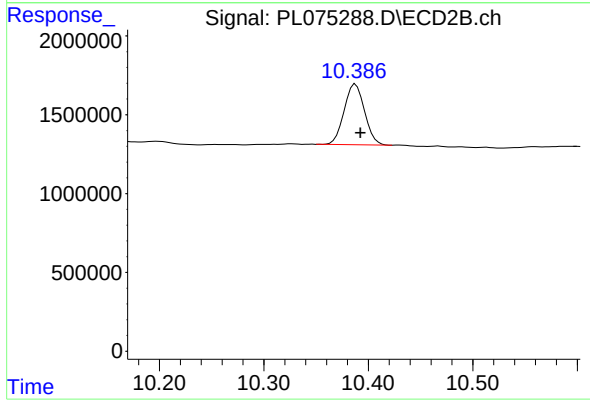

#28 Decachlorobiphenyl

R.T.: 10.388 min
Delta R.T.: -0.005 min
Response: 5235721
Conc: 3.82 ng/ml