

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL053122\
 Data File : PL075311.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 May 2022 23:24
 Operator : AR\AJ
 Sample : N2930-11
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 01 07:47:33 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
 Quant Title : GC Extractables
 QLast Update : Tue May 31 02:52:42 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.641	4.640	10566495	27901805	17.978	17.613
28)	SA Decachlor...	11.638	10.388	7835482	18119580	14.613	13.204
Target Compounds							
7)	B delta-BHC	0.000	6.403	0	60063	N.D.	0.028 #
10)	B gamma-Chl...	0.000	7.329f	0	309936	N.D.	0.169 #
12)	B 4,4'-DDE	8.658	7.628	292756	866186	0.503	0.532
13)	MA Dieldrin	8.812	7.766	633716	220942	1.000	0.127 #
14)	MA Endrin	0.000	8.064	0	1936363	N.D.	1.244 #
15)	B Endosulfa...	9.272f	8.355	517149	399741	0.916	0.254 #
16)	A 4,4'-DDD	9.202	0.000	2805935	0	5.673	N.D. #
17)	MA 4,4'-DDT	0.000	8.464	0	9584464	N.D.	6.702 #
19)	B Endosulfa...	0.000	8.776	0	5475461	N.D.	3.658 #
24)	Chlordane-2	0.000	6.638	0	1004469	N.D.	14.553 #
25)	Chlordane-3	0.000	7.329f	0	309936	N.D.	1.699 #
27)	Chlordane-5	0.000	8.128	0	7670109	N.D.	148.883 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL053122\
Data File : PL075311.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 May 2022 23:24
Operator : AR\AJ
Sample : N2930-11
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 01 07:47:33 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
Quant Title : GC Extractables
QLast Update : Tue May 31 02:52:42 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

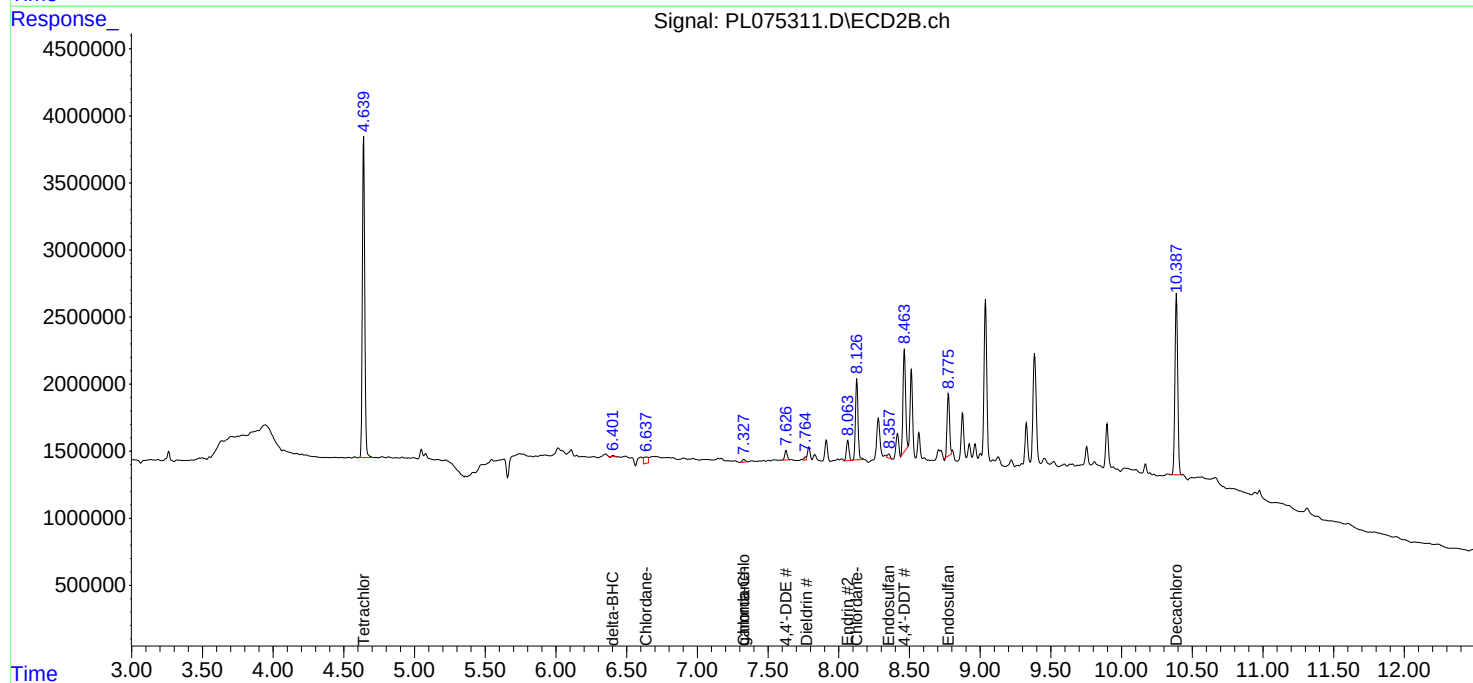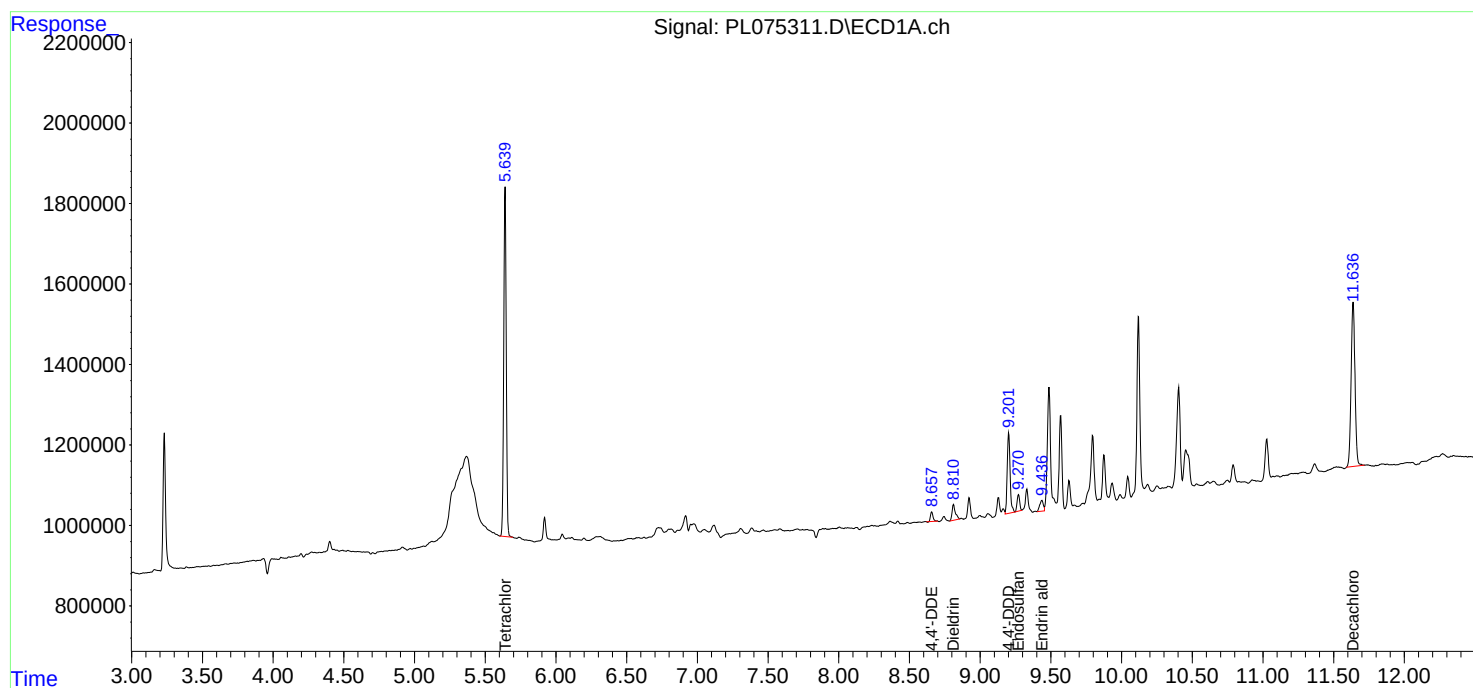


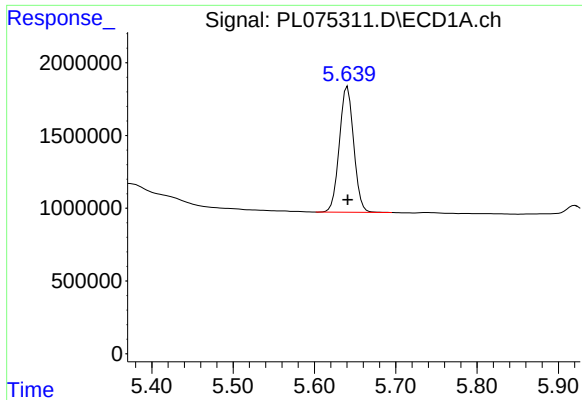

#1 Tetrachloro-m-xylene


R.T.: 5.641 min
Delta R.T.: 0.000 min
Response: 10566495
Conc: 17.98 ng/ml

Instrument :
ECD_L
ClientSampleId :

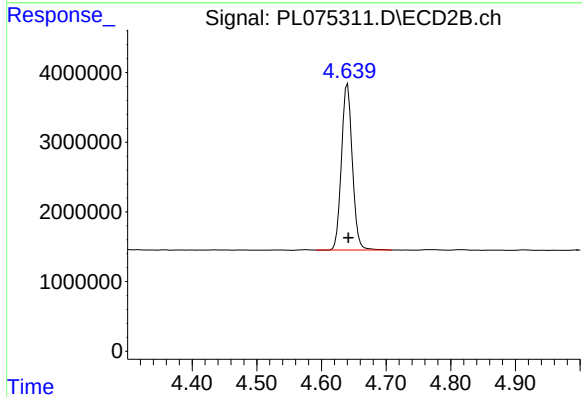


#1 Tetrachloro-m-xylene

R.T.: 4.640 min
Delta R.T.: -0.001 min
Response: 27901805
Conc: 17.61 ng/ml

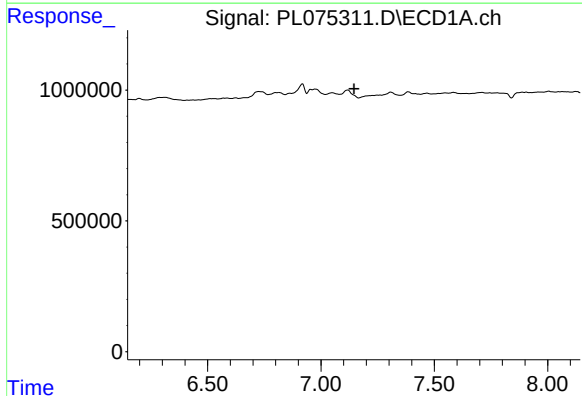


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 7.146 min
Response: 0
Conc: N.D.

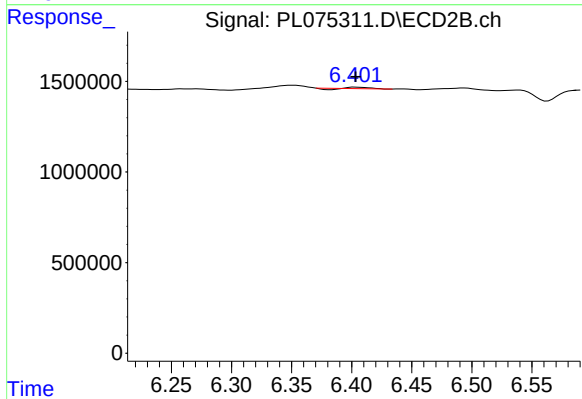

#7 delta-BHC


R.T.: 6.403 min
Delta R.T.: 0.000 min
Response: 60063
Conc: 0.03 ng/ml

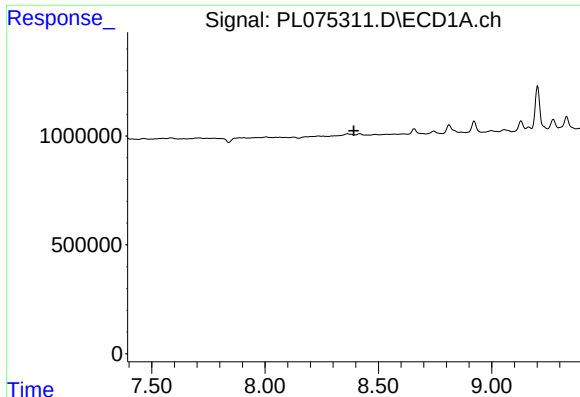

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 8.392 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

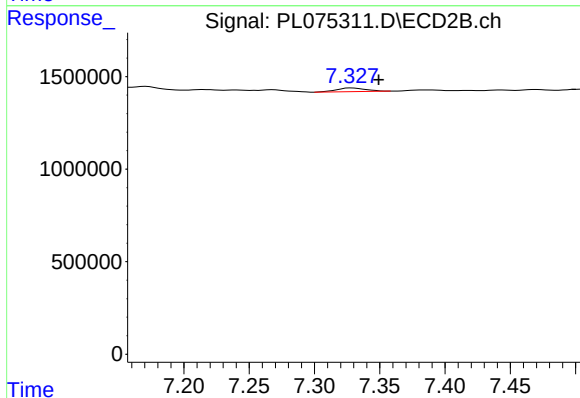


#10 gamma-Chlordane

R.T.: 7.329 min
Delta R.T.: -0.020 min
Response: 309936
Conc: 0.17 ng/ml

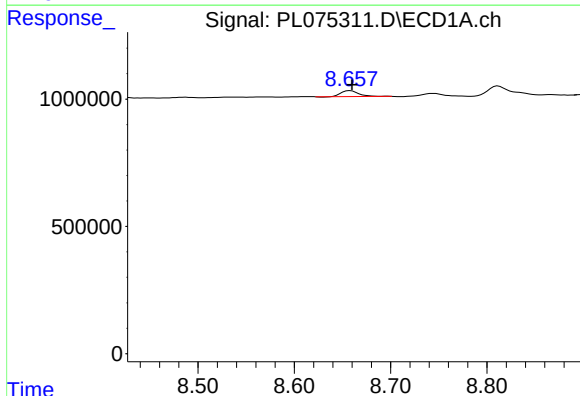


#12 4,4'-DDE

R.T.: 8.658 min
Delta R.T.: -0.002 min
Response: 292756
Conc: 0.50 ng/ml

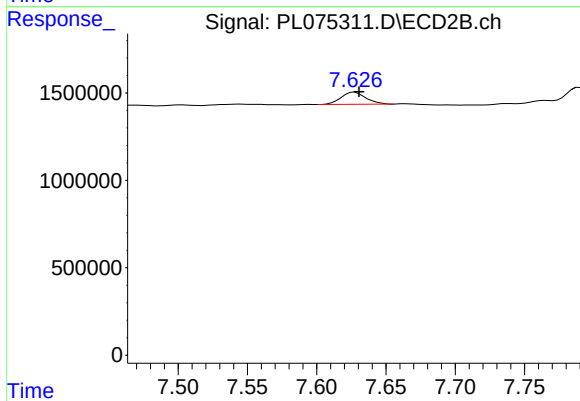

#12 4,4'-DDE


R.T.: 7.628 min
Delta R.T.: -0.003 min
Response: 866186
Conc: 0.53 ng/ml

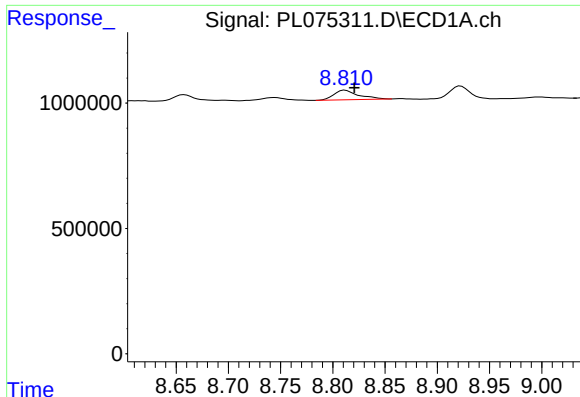

#13 Dieldrin


R.T.: 8.812 min
Delta R.T.: -0.009 min
Response: 633716
Conc: 1.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

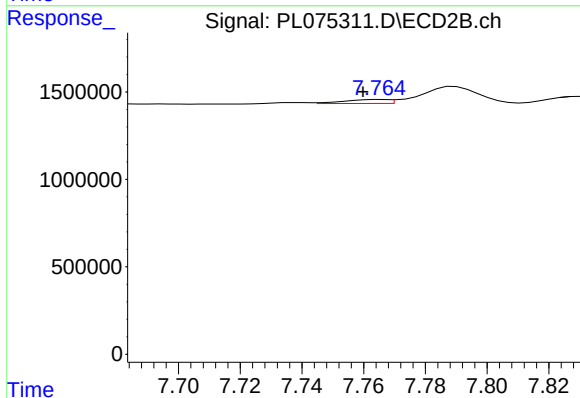


#13 Dieldrin

R.T.: 7.766 min
Delta R.T.: 0.006 min
Response: 220942
Conc: 0.13 ng/ml

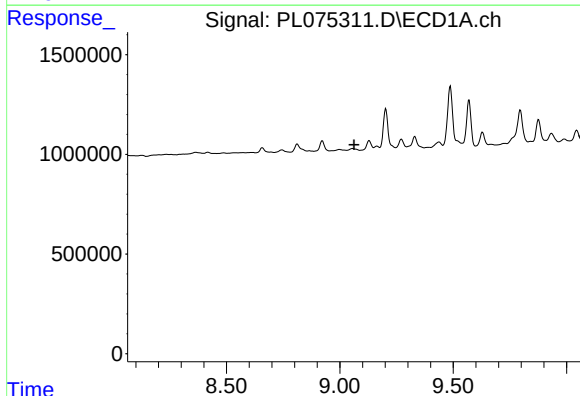


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 9.062 min
Response: 0
Conc: N.D.

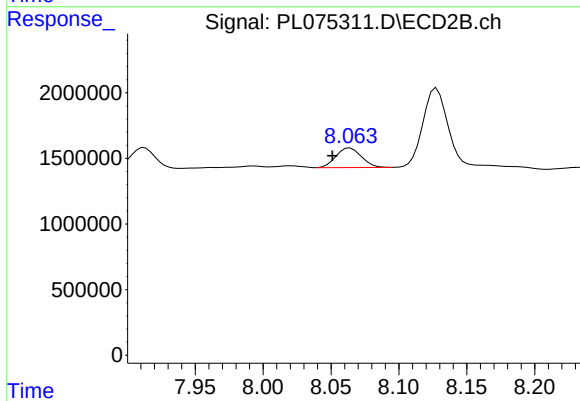

#14 Endrin


R.T.: 8.064 min
Delta R.T.: 0.013 min
Response: 1936363
Conc: 1.24 ng/ml

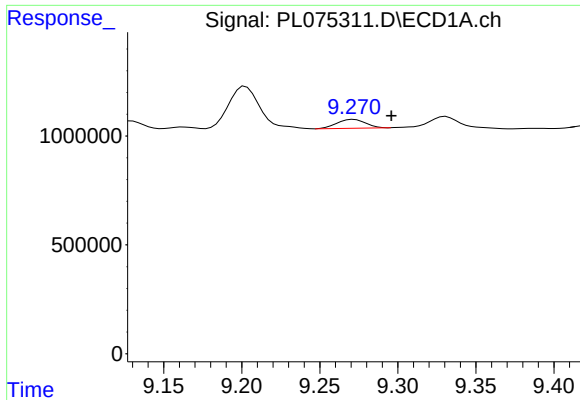

#15 Endosulfan II


R.T.: 9.272 min
Delta R.T.: -0.024 min
Response: 517149
Conc: 0.92 ng/ml

Instrument :
ECD_L
ClientSampleId :

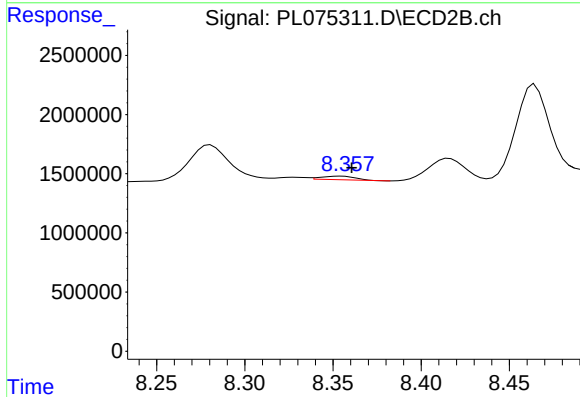


#15 Endosulfan II

R.T.: 8.355 min
Delta R.T.: -0.006 min
Response: 399741
Conc: 0.25 ng/ml

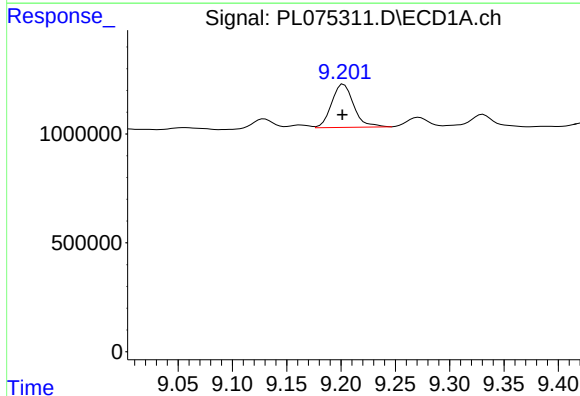


#16 4,4'-DDD

R.T.: 9.202 min
Delta R.T.: 0.001 min
Response: 2805935
Conc: 5.67 ng/ml

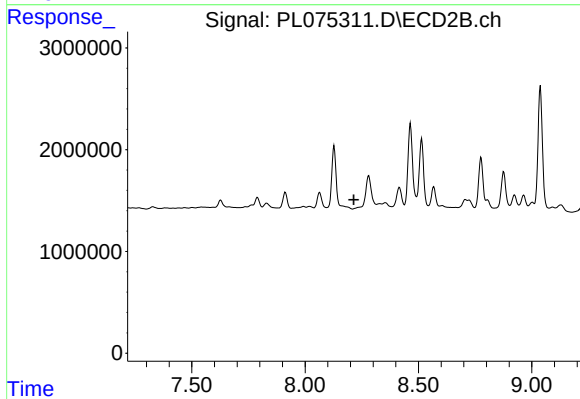

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 8.215 min
Response: 0
Conc: N.D.

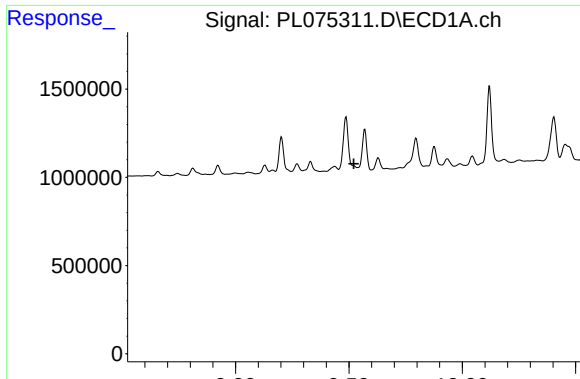

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 9.522 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

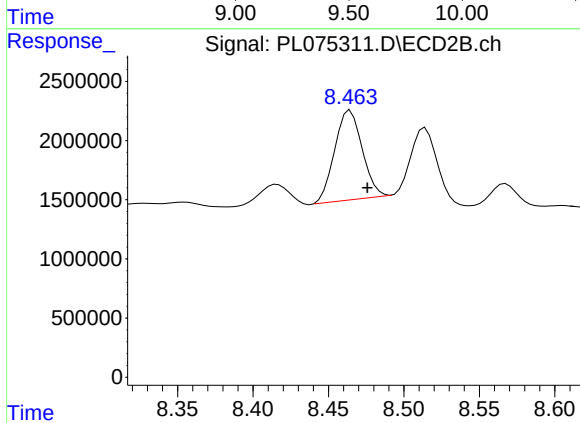


#17 4,4'-DDT

R.T.: 8.464 min
Delta R.T.: -0.011 min
Response: 9584464
Conc: 6.70 ng/ml

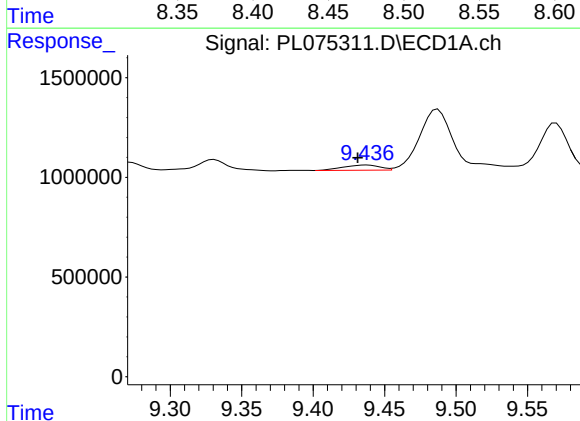


#18 Endrin aldehyde

R.T.: 9.437 min
Delta R.T.: 0.006 min
Response: 473716
Conc: 1.08 ng/ml

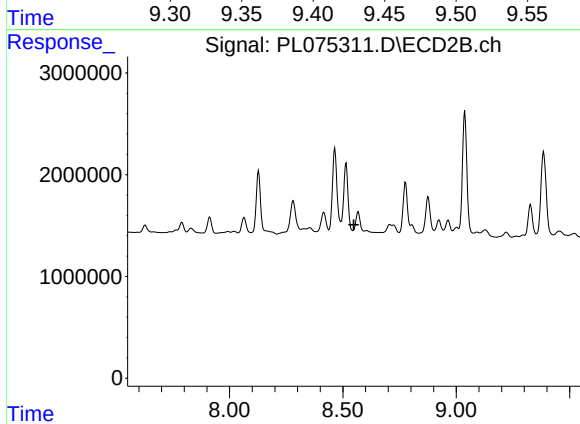

#18 Endrin aldehyde


R.T.: 8.567 min
Delta R.T.: 0.019 min
Response: -4219952
Conc: N.D.

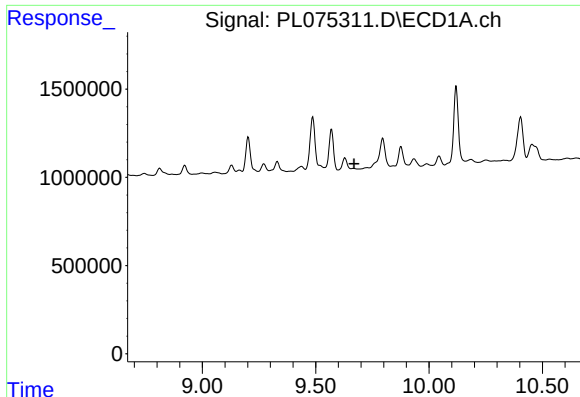

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 9.669 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

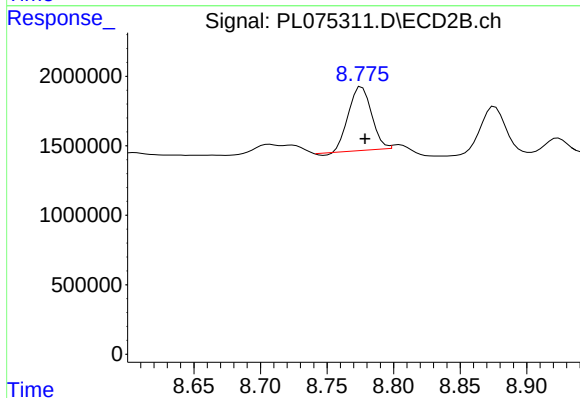


#19 Endosulfan Sulfate

R.T.: 8.776 min
Delta R.T.: -0.003 min
Response: 5475461
Conc: 3.66 ng/ml

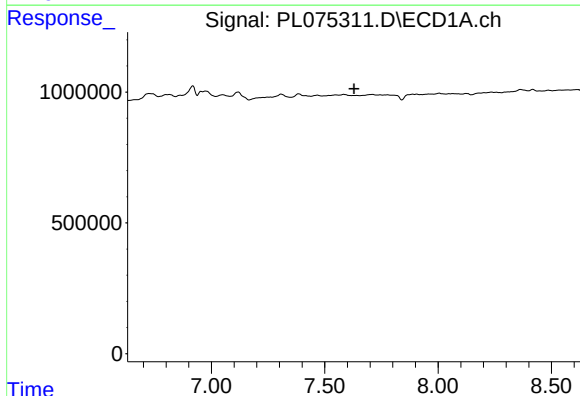


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T.: 7.630 min
Response: 0
Conc: N.D.

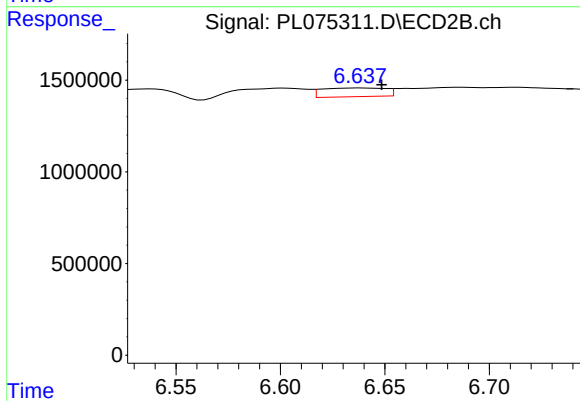

#24 Chlordane-2


R.T.: 6.638 min
Delta R.T.: -0.010 min
Response: 1004469
Conc: 14.55 ng/ml

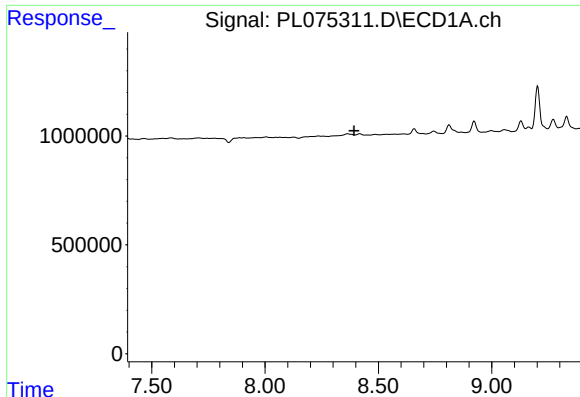

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 8.392 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

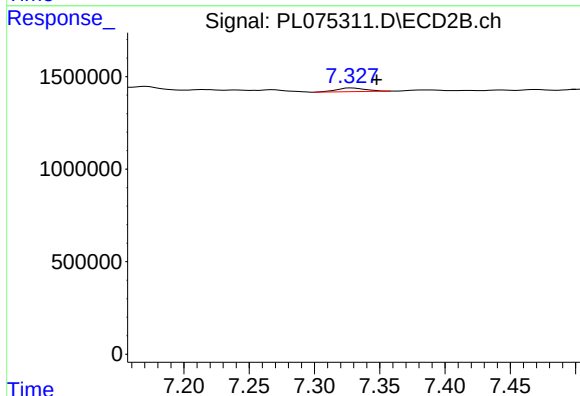


#25 Chlordane-3

R.T.: 7.329 min
Delta R.T.: -0.019 min
Response: 309936
Conc: 1.70 ng/ml

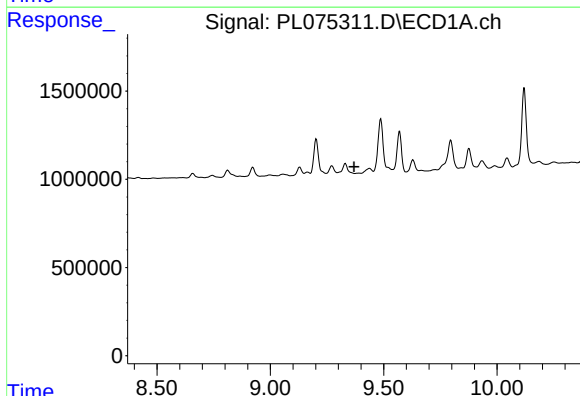


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 9.369 min
Response: 0
Conc: N.D.

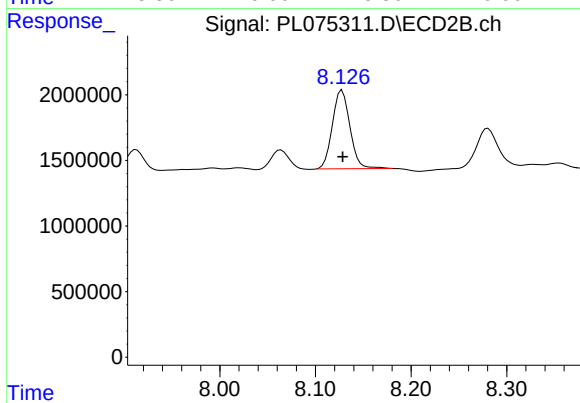

#27 Chlordane-5


R.T.: 8.128 min
Delta R.T.: 0.000 min
Response: 7670109
Conc: 148.88 ng/ml

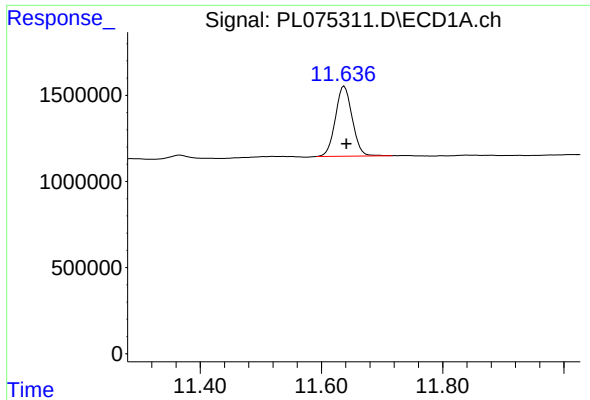

#28 Decachlorobiphenyl

R.T.: 11.638 min
Delta R.T.: -0.003 min
Response: 7835482
Conc: 14.61 ng/ml

Instrument :
ECD_L
ClientSampleId :

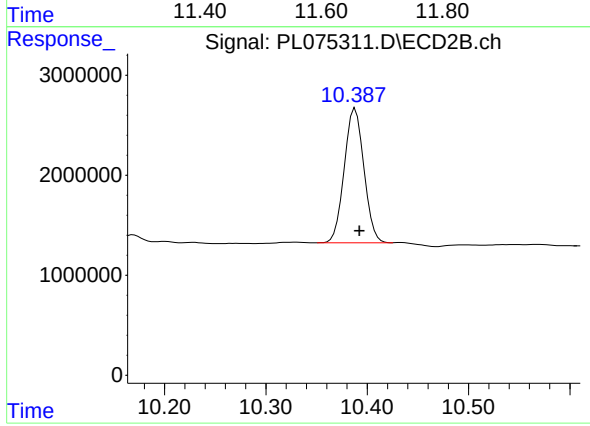

#28 Decachlorobiphenyl

R.T.: 10.388 min
Delta R.T.: -0.004 min
Response: 18119580
Conc: 13.20 ng/ml