

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL053122\
 Data File : PL075316.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Jun 2022 00:47
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 01 07:49:14 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
 Quant Title : GC Extractables
 QLast Update : Tue May 31 02:52:42 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.640	4.640	14696395	38515187	25.005	24.313
28)	SA Decachlor...	11.639	10.387	13889701	32298049	25.905	23.536
Target Compounds							
7)	B delta-BHC	0.000	6.403	0	347307	N.D.	0.162 #
8)	B Heptachlo...	8.124	0.000	2971229	0	4.352	N.D. #
13)	MA Dieldrin	0.000	7.758	0	3578514	N.D.	2.062 #
14)	MA Endrin	0.000	8.070f	0	1197101	N.D.	0.769 #
15)	B Endosulfa...	9.303	0.000	241502	0	0.428	N.D. #
19)	B Endosulfa...	0.000	8.775	0	319248	N.D.	0.213 #
21)	B Endrin ke...	10.186	0.000	310222	0	0.505	N.D. #
27)	Chlordane-5	0.000	8.156f	0	453829	N.D.	8.809 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL053122\
Data File : PL075316.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Jun 2022 00:47
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 01 07:49:14 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
Quant Title : GC Extractables
QLast Update : Tue May 31 02:52:42 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

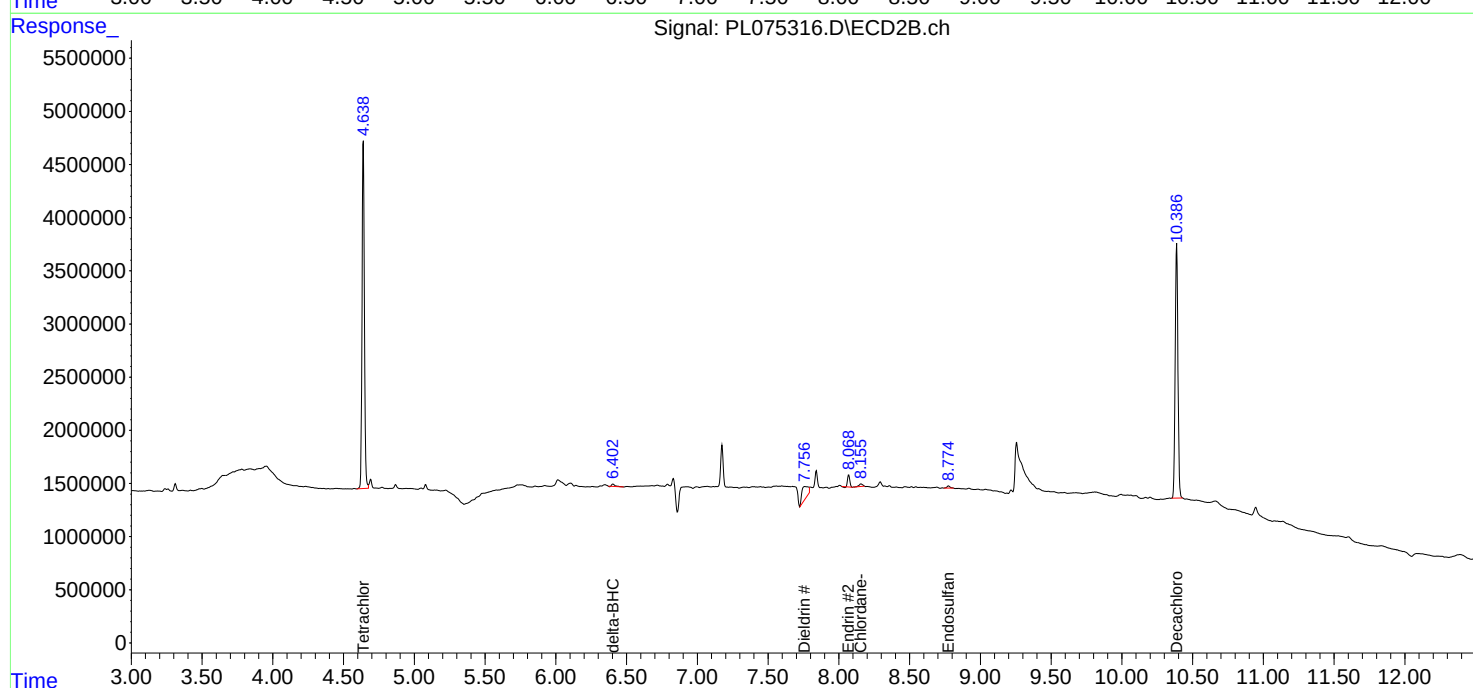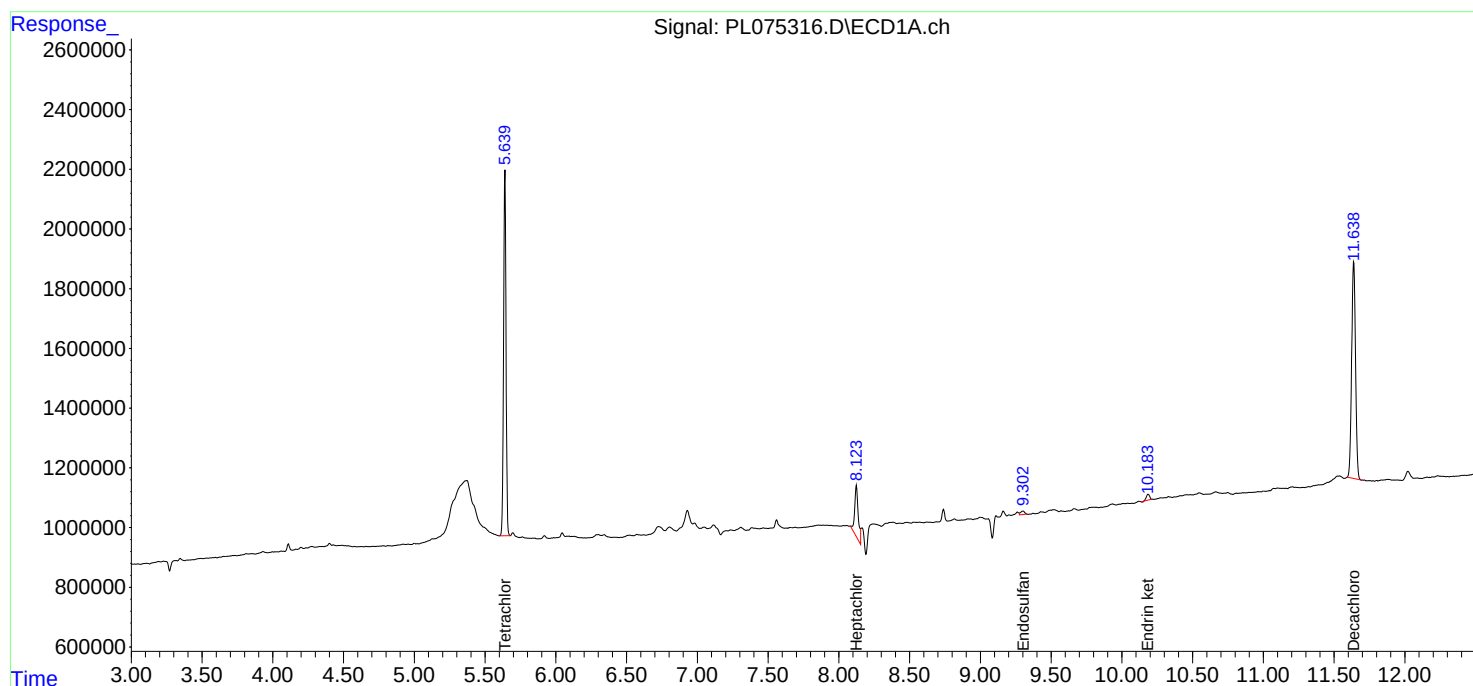


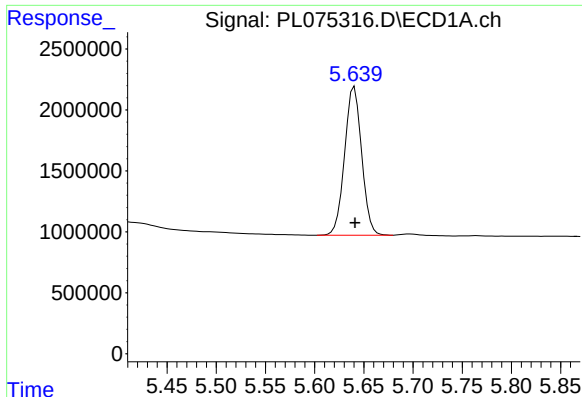

#1 Tetrachloro-m-xylene


R.T.: 5.640 min
Delta R.T.: 0.000 min
Response: 14696395
Conc: 25.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

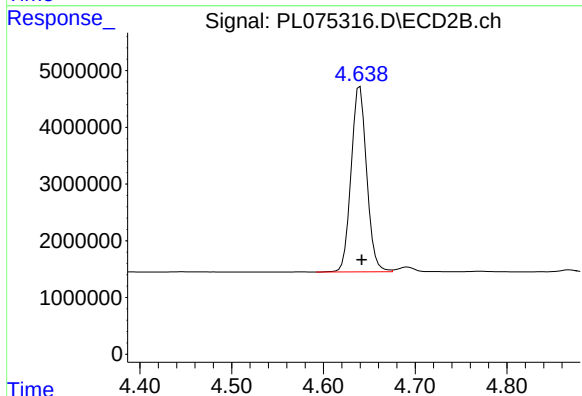


#1 Tetrachloro-m-xylene

R.T.: 4.640 min
Delta R.T.: -0.002 min
Response: 38515187
Conc: 24.31 ng/ml

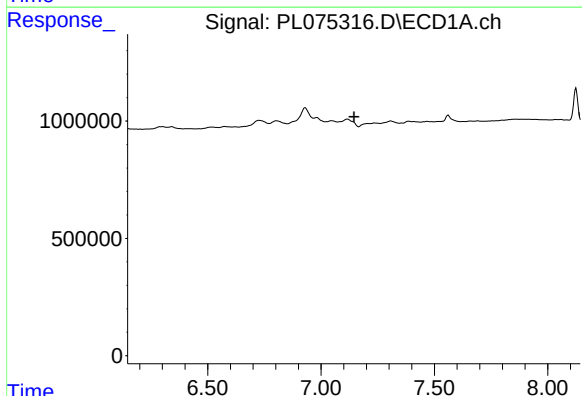


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 7.146 min
Response: 0
Conc: N.D.

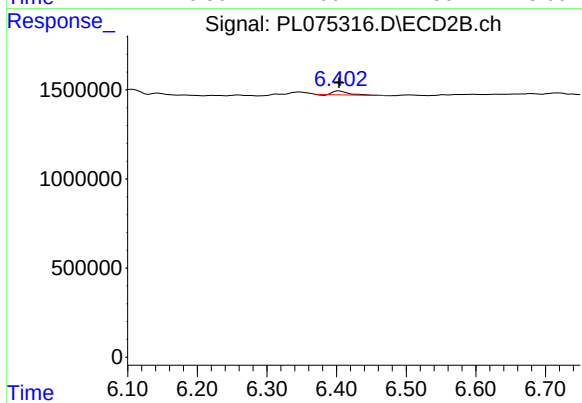

#7 delta-BHC


R.T.: 6.403 min
Delta R.T.: 0.000 min
Response: 347307
Conc: 0.16 ng/ml

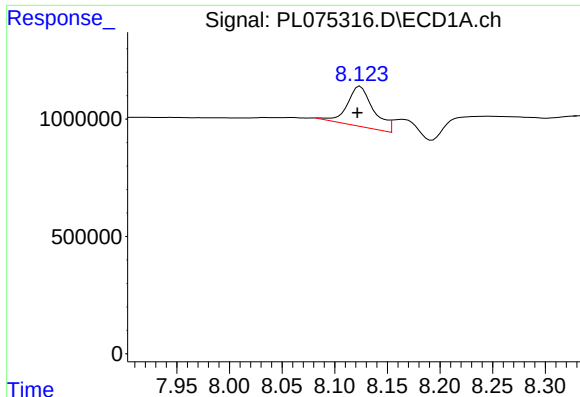

#8 Heptachlor epoxide


R.T.: 8.124 min
Delta R.T.: 0.003 min
Response: 2971229
Conc: 4.35 ng/ml

Instrument :
ECD_L
ClientSampleId :

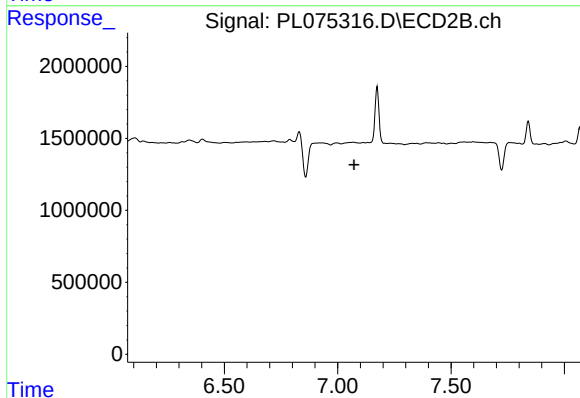


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 7.072 min
Response: 0
Conc: N.D.

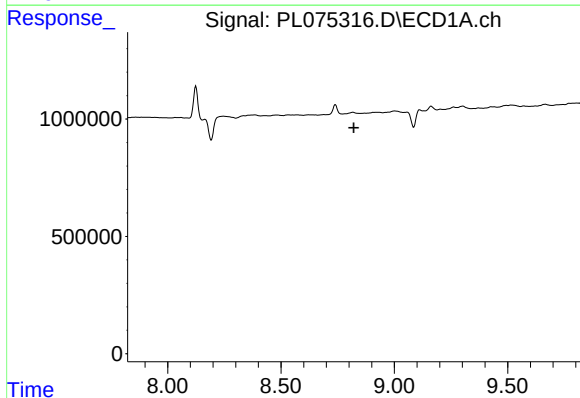


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 8.821 min
Response: 0
Conc: N.D.

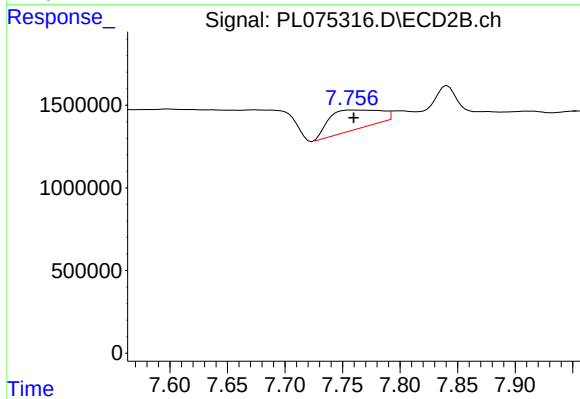

#13 Dieldrin


R.T.: 7.758 min
Delta R.T.: -0.002 min
Response: 3578514
Conc: 2.06 ng/ml

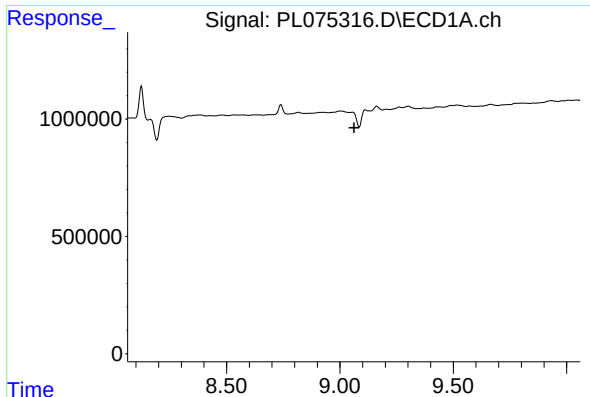

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 9.062 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

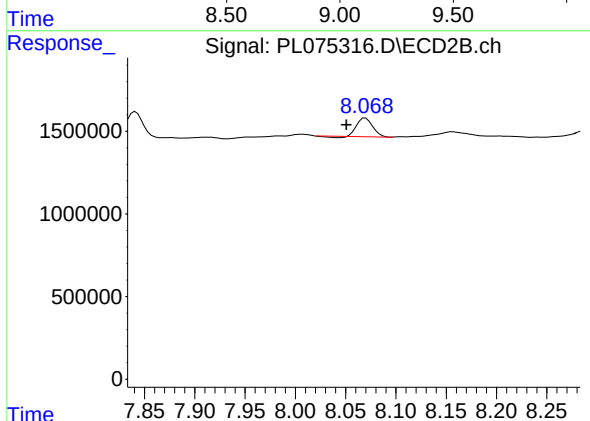


#14 Endrin

R.T.: 8.070 min
Delta R.T.: 0.019 min
Response: 1197101
Conc: 0.77 ng/ml

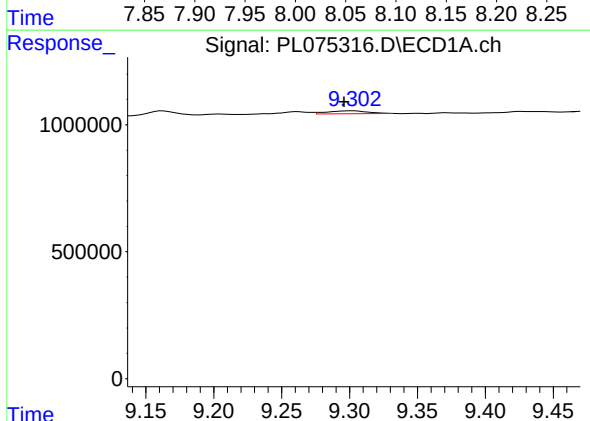


#15 Endosulfan II

R.T.: 9.303 min
Delta R.T.: 0.007 min
Response: 241502
Conc: 0.43 ng/ml

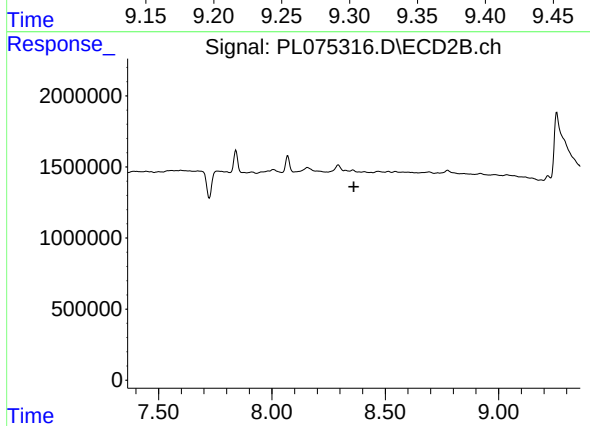

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.361 min
Response: 0
Conc: N.D.

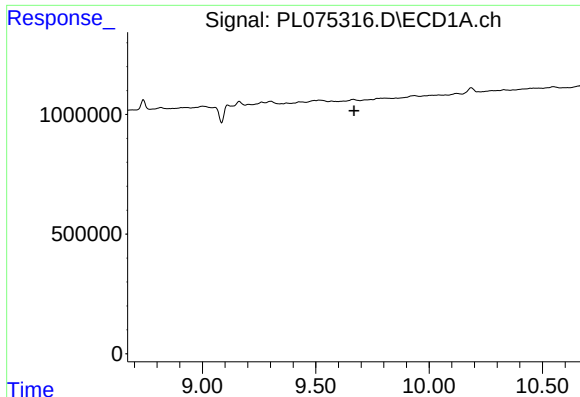

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 9.669 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

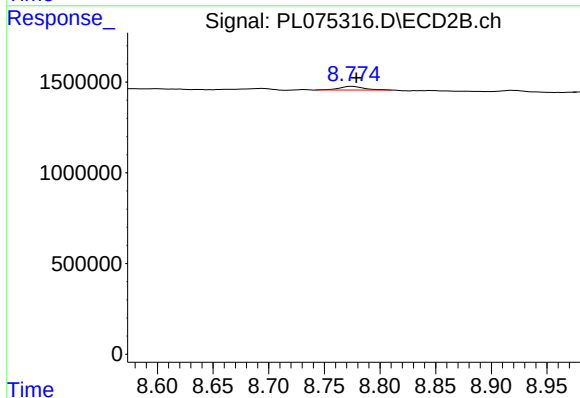


#19 Endosulfan Sulfate

R.T.: 8.775 min
Delta R.T.: -0.004 min
Response: 319248
Conc: 0.21 ng/ml

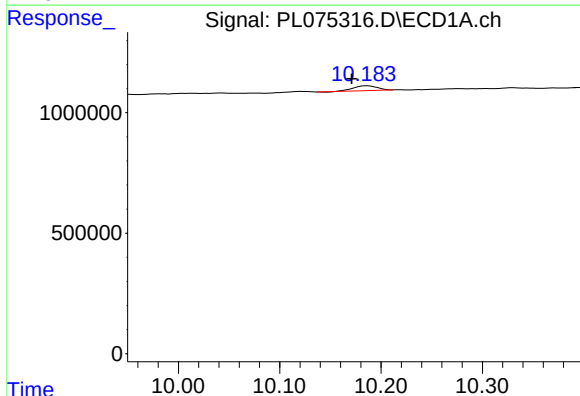


#21 Endrin ketone

R.T.: 10.186 min
Delta R.T.: 0.015 min
Response: 310222
Conc: 0.51 ng/ml

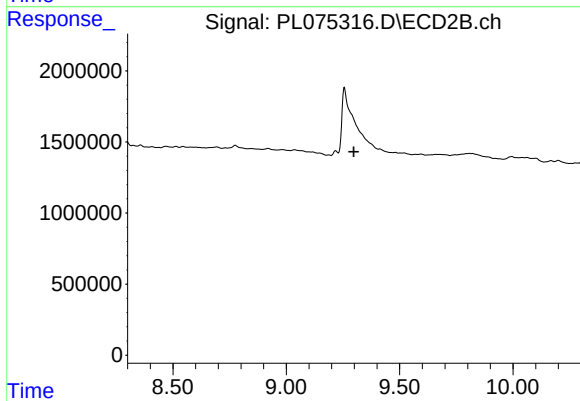

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 9.298 min
Response: 0
Conc: N.D.

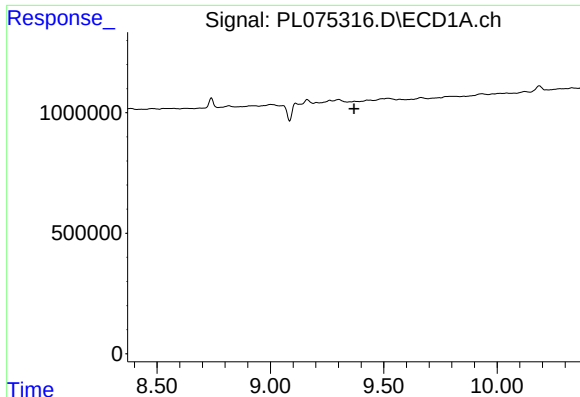

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 9.369 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

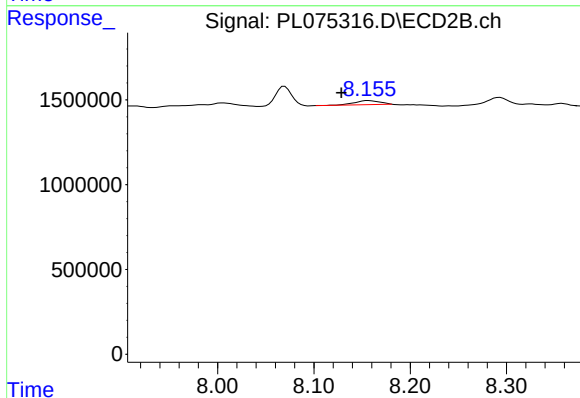


#27 Chlordane-5

R.T.: 8.156 min
Delta R.T.: 0.028 min
Response: 453829
Conc: 8.81 ng/ml

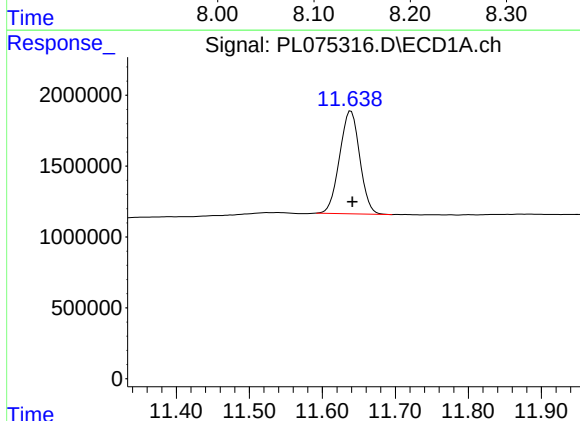

#28 Decachlorobiphenyl

R.T.: 11.639 min
Delta R.T.: -0.002 min
Response: 13889701
Conc: 25.90 ng/ml

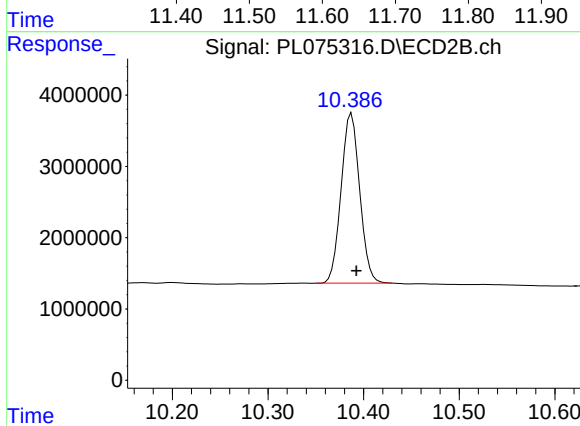

#28 Decachlorobiphenyl

R.T.: 10.387 min
Delta R.T.: -0.005 min
Response: 32298049
Conc: 23.54 ng/ml