

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL053122\
 Data File : PL075331.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Jun 2022 05:12
 Operator : AR\AJ
 Sample : N3042-05
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 01 07:54:28 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
 Quant Title : GC Extractables
 QLast Update : Tue May 31 02:52:42 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.640	4.640	3414012	8230301	5.809	5.195
28)	SA Decachlor...	11.639	10.389	2320314	5548463	4.327	4.043
Target Compounds							
11)	B alpha-Chl...	0.000	7.404	0	146504	N.D.	0.080 #
13)	MA Dieldrin	0.000	7.763	0	175621	N.D.	0.101 #
14)	MA Endrin	0.000	8.070f	0	273742	N.D.	0.176 #
15)	B Endosulfa...	9.302	0.000	100410	0	0.178	N.D. #
16)	A 4,4'-DDD	9.202	0.000	150543	0	0.304	N.D. #
17)	MA 4,4'-DDT	0.000	8.466	0	387232	N.D.	0.271 #
19)	B Endosulfa...	0.000	8.776	0	293482	N.D.	0.196 #
21)	B Endrin ke...	10.187f	0.000	291269	0	0.474	N.D. #
26)	Chlordane-4	0.000	7.404	0	146504	N.D.	0.756 #
27)	Chlordane-5	0.000	8.128	0	373988	N.D.	7.259 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL053122\
Data File : PL075331.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Jun 2022 05:12
Operator : AR\AJ
Sample : N3042-05
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 01 07:54:28 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
Quant Title : GC Extractables
QLast Update : Tue May 31 02:52:42 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

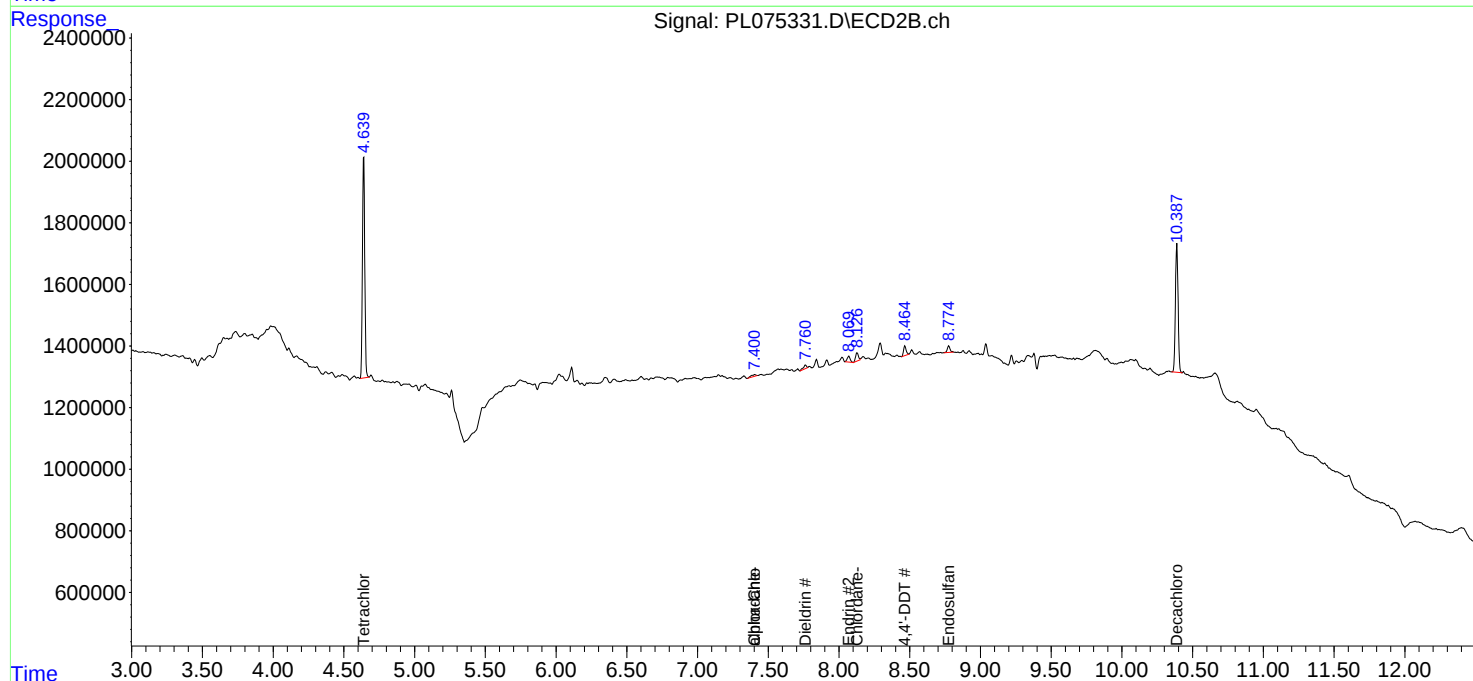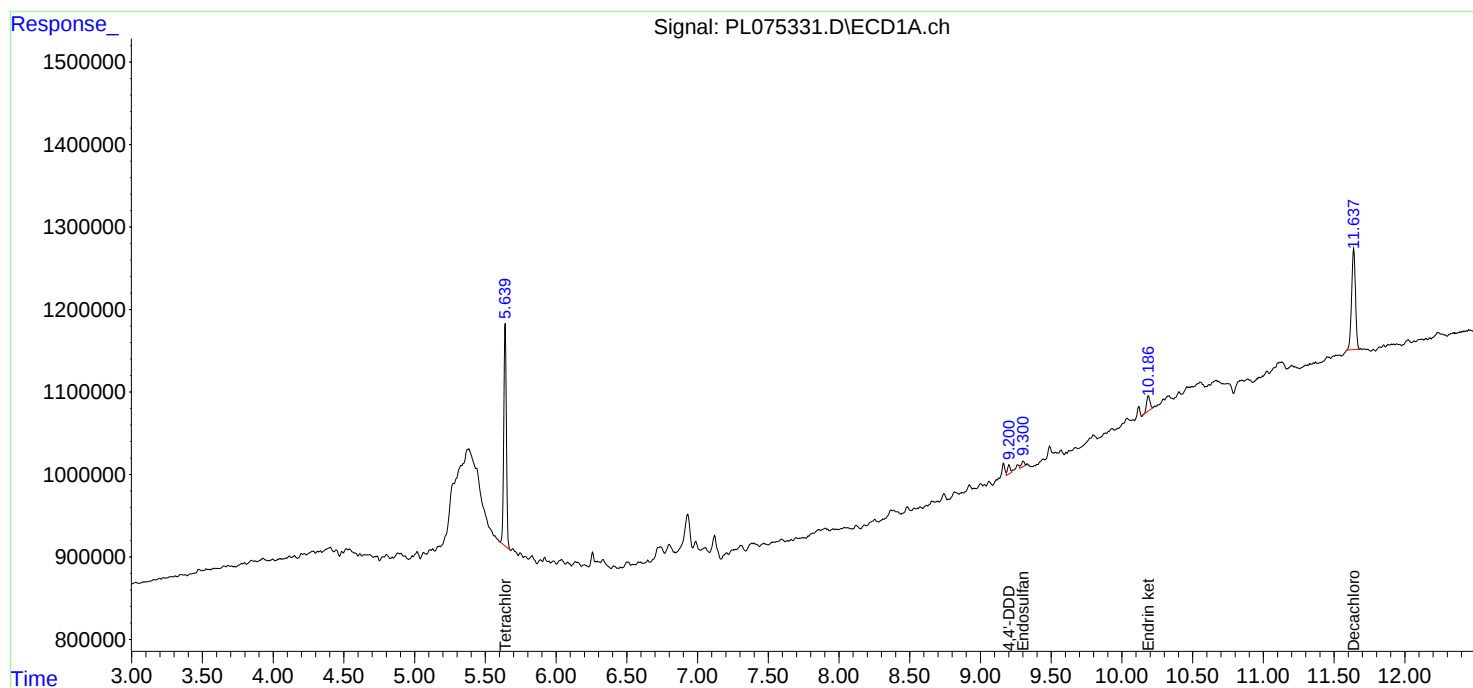


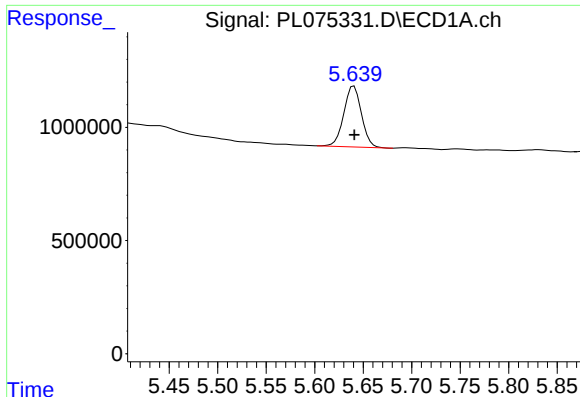

#1 Tetrachloro-m-xylene


R.T.: 5.640 min
Delta R.T.: 0.000 min
Response: 3414012
Conc: 5.81 ng/ml

Instrument :
ECD_L
ClientSampleId :

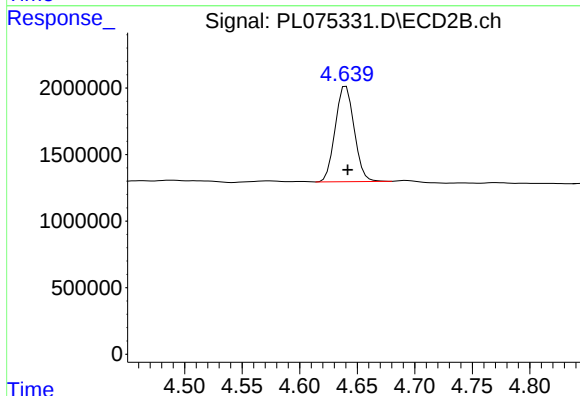


#1 Tetrachloro-m-xylene

R.T.: 4.640 min
Delta R.T.: -0.001 min
Response: 8230301
Conc: 5.20 ng/ml

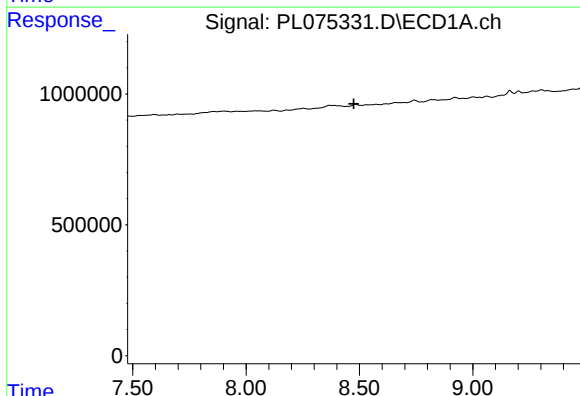


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 8.474 min
Response: 0
Conc: N.D.

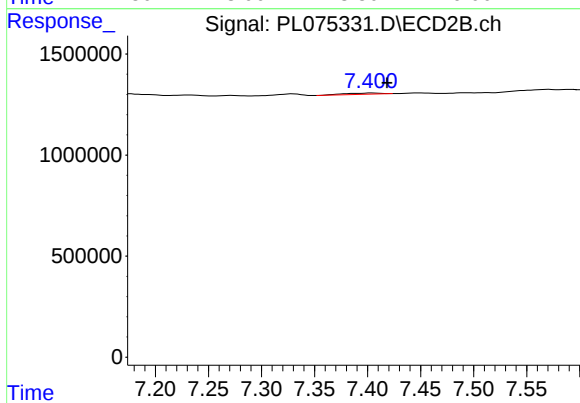

#11 alpha-Chlordane


R.T.: 7.404 min
Delta R.T.: -0.014 min
Response: 146504
Conc: 0.08 ng/ml

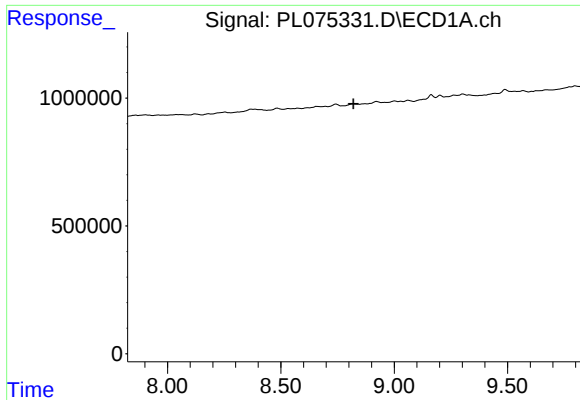

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 8.821 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

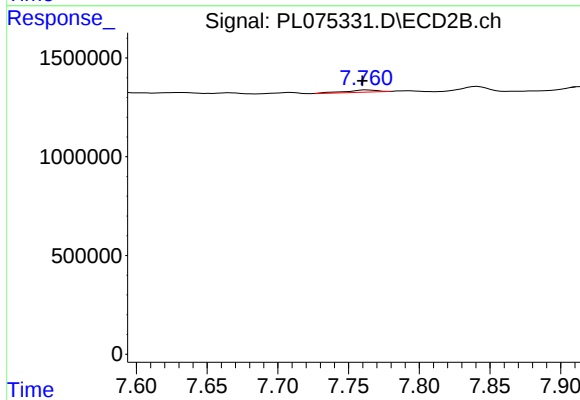


#13 Dieldrin

R.T.: 7.763 min
Delta R.T.: 0.003 min
Response: 175621
Conc: 0.10 ng/ml

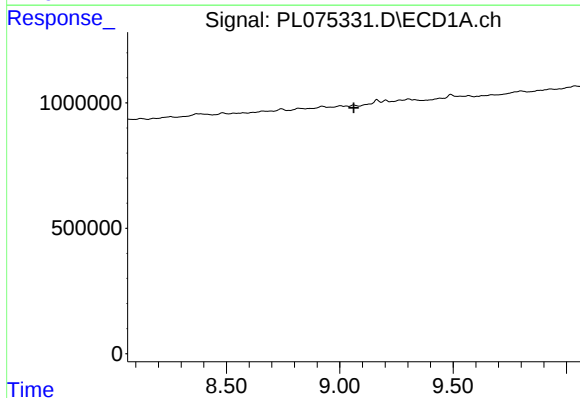


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 9.062 min
Response: 0
Conc: N.D.

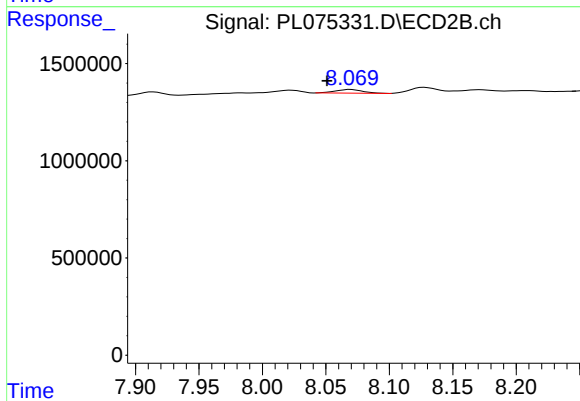

#14 Endrin


R.T.: 8.070 min
Delta R.T.: 0.019 min
Response: 273742
Conc: 0.18 ng/ml

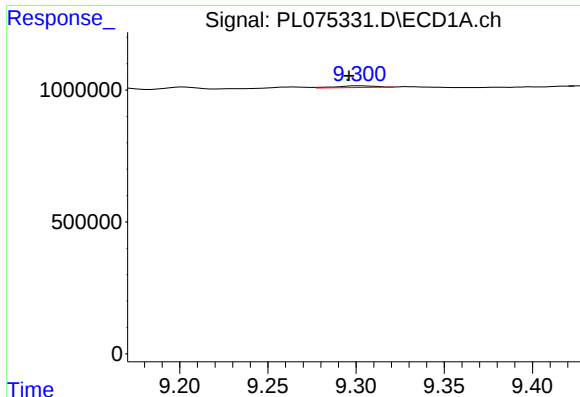

#15 Endosulfan II


R.T.: 9.302 min
Delta R.T.: 0.006 min
Response: 100410
Conc: 0.18 ng/ml

Instrument :
ECD_L
ClientSampleId :

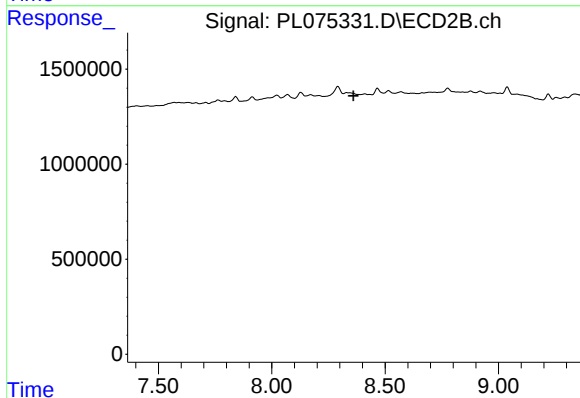


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.361 min
Response: 0
Conc: N.D.

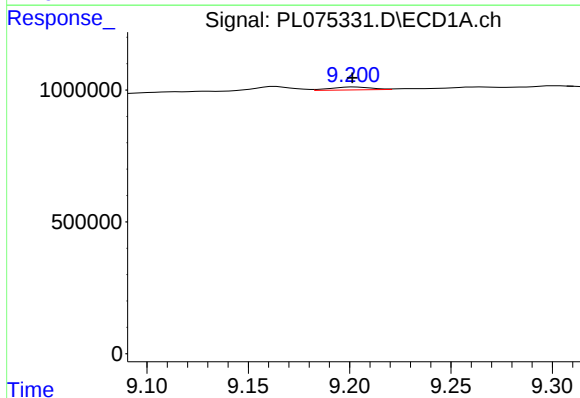


#16 4,4'-DDD

R.T.: 9.202 min
Delta R.T.: 0.000 min
Response: 150543
Conc: 0.30 ng/ml

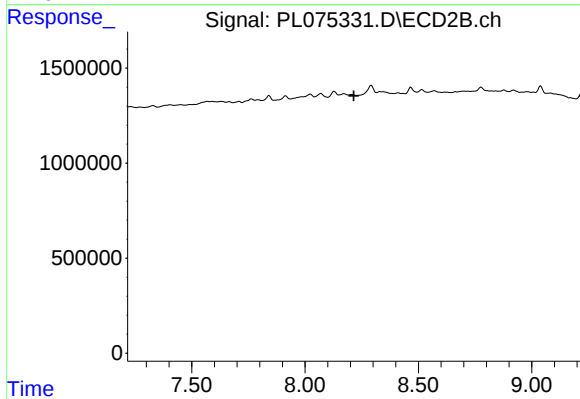

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 8.215 min
Response: 0
Conc: N.D.

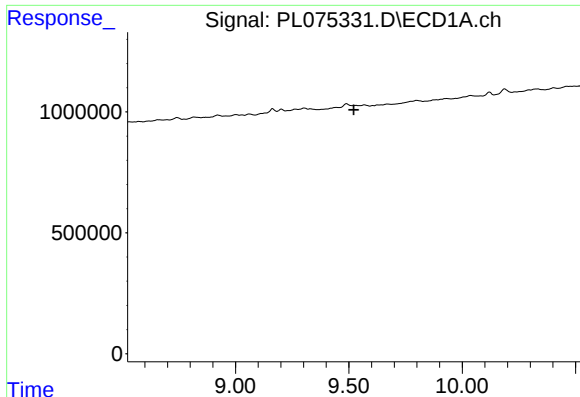

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 9.522 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

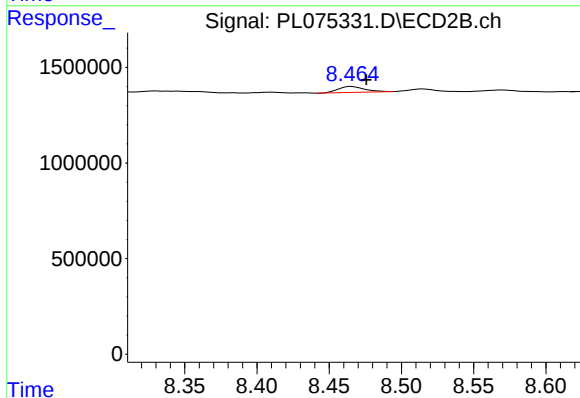


#17 4,4'-DDT

R.T.: 8.466 min
Delta R.T.: -0.010 min
Response: 387232
Conc: 0.27 ng/ml

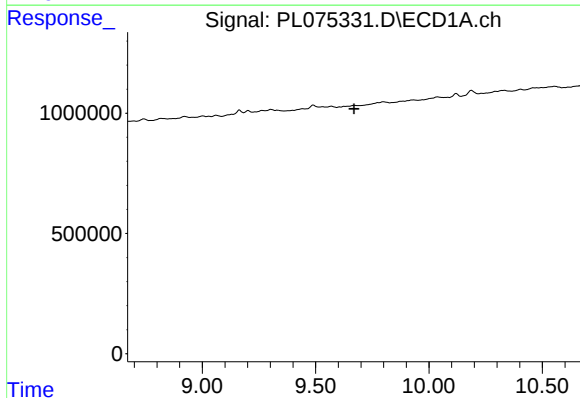


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 9.669 min
Response: 0
Conc: N.D.

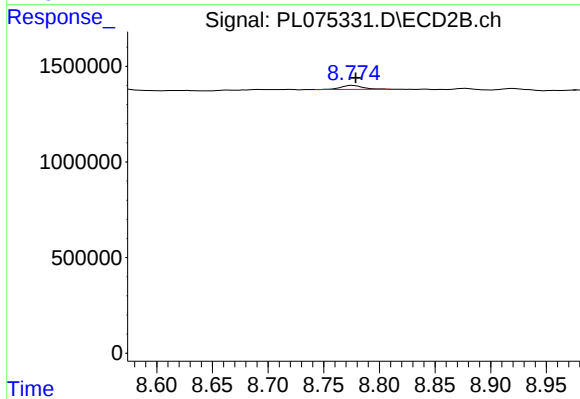

#19 Endosulfan Sulfate


R.T.: 8.776 min
Delta R.T.: -0.003 min
Response: 293482
Conc: 0.20 ng/ml

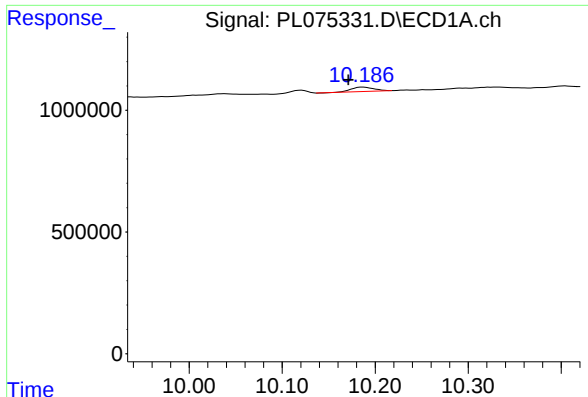

#21 Endrin ketone


R.T.: 10.187 min
Delta R.T.: 0.016 min
Response: 291269
Conc: 0.47 ng/ml

Instrument :
ECD_L
ClientSampleId :

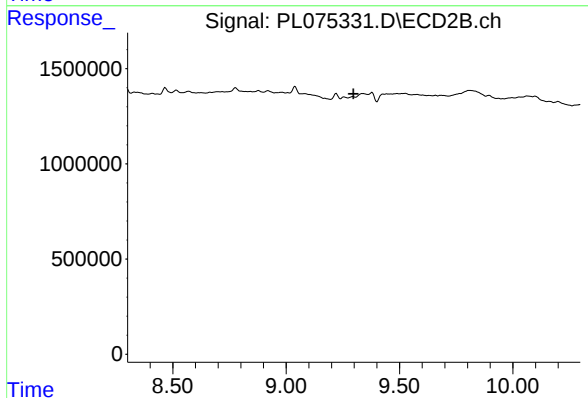


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.298 min
Response: 0
Conc: N.D.

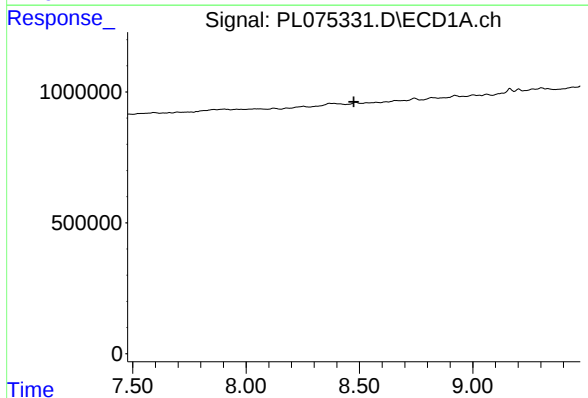


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 8.476 min
Response: 0
Conc: N.D.

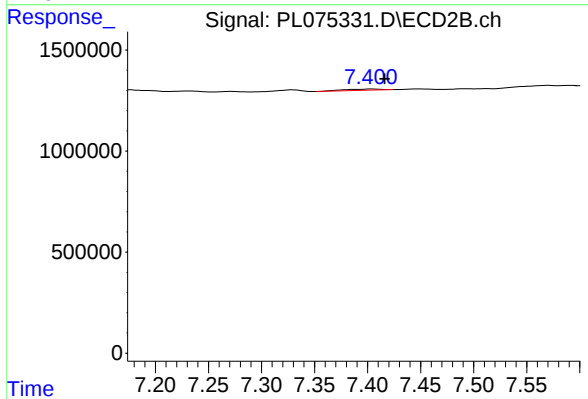

#26 Chlordane-4


R.T.: 7.404 min
Delta R.T.: -0.012 min
Response: 146504
Conc: 0.76 ng/ml

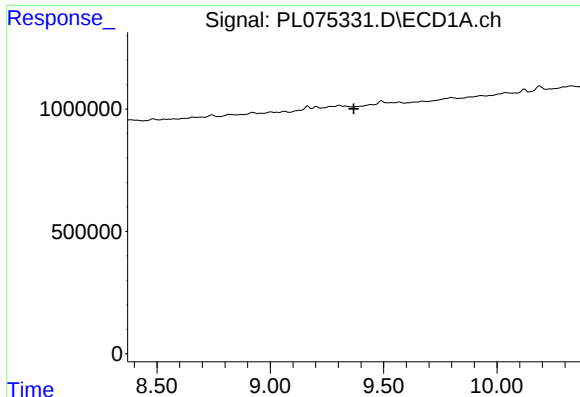

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 9.369 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

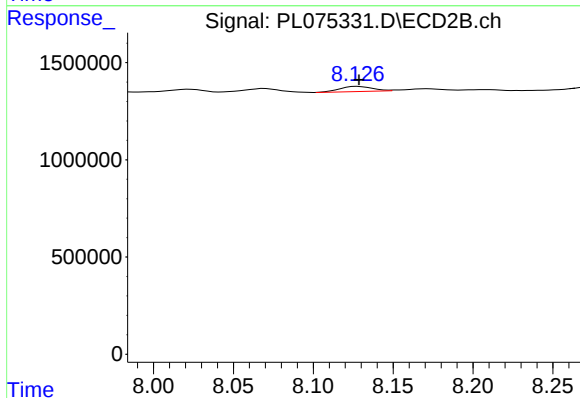


#27 Chlordane-5

R.T.: 8.128 min
Delta R.T.: 0.000 min
Response: 373988
Conc: 7.26 ng/ml

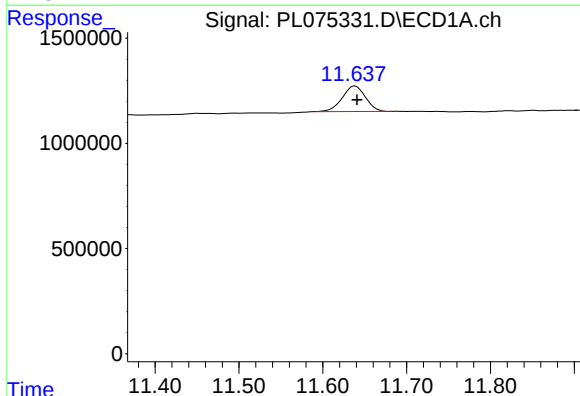

#28 Decachlorobiphenyl

R.T.: 11.639 min
Delta R.T.: -0.002 min
Response: 2320314
Conc: 4.33 ng/ml

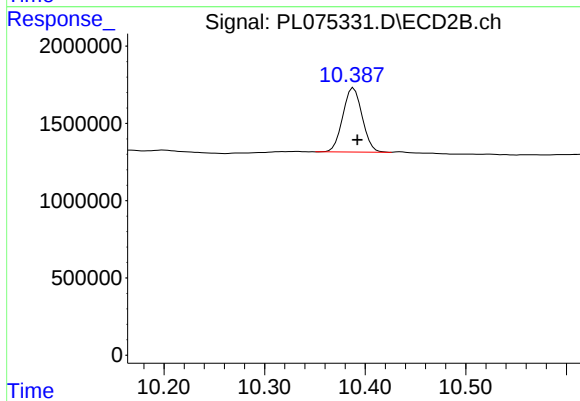

#28 Decachlorobiphenyl

R.T.: 10.389 min
Delta R.T.: -0.004 min
Response: 5548463
Conc: 4.04 ng/ml