

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL053122\
 Data File : PL075301.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 May 2022 20:38
 Operator : AR\AJ
 Sample : PB144972BS
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB144972BS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 06/01/2022
 Supervised By : Ankita Jodhani 06/01/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 01 07:43:56 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
 Quant Title : GC Extractables
 QLast Update : Tue May 31 02:52:42 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.651	4.644	118255	356103	0.201m	0.225m
28) SA Decachlor...	11.628	10.401	58387	28760	0.109m	0.021m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL053122\
Data File : PL075301.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 May 2022 20:38
Operator : AR\AJ
Sample : PB144972BS
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PB144972BS


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 06/01/2022
Supervised By : Ankita Jodhani 06/01/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 01 07:43:56 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
Quant Title : GC Extractables
QLast Update : Tue May 31 02:52:42 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

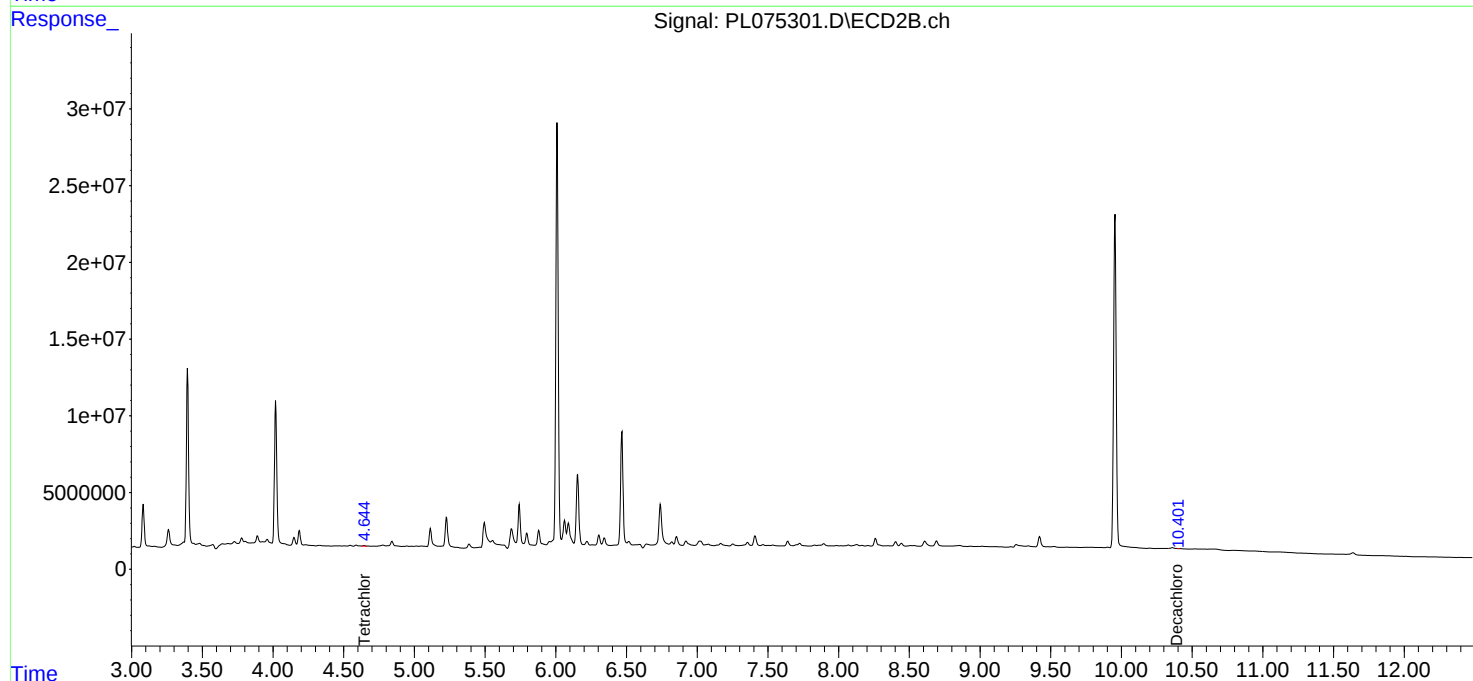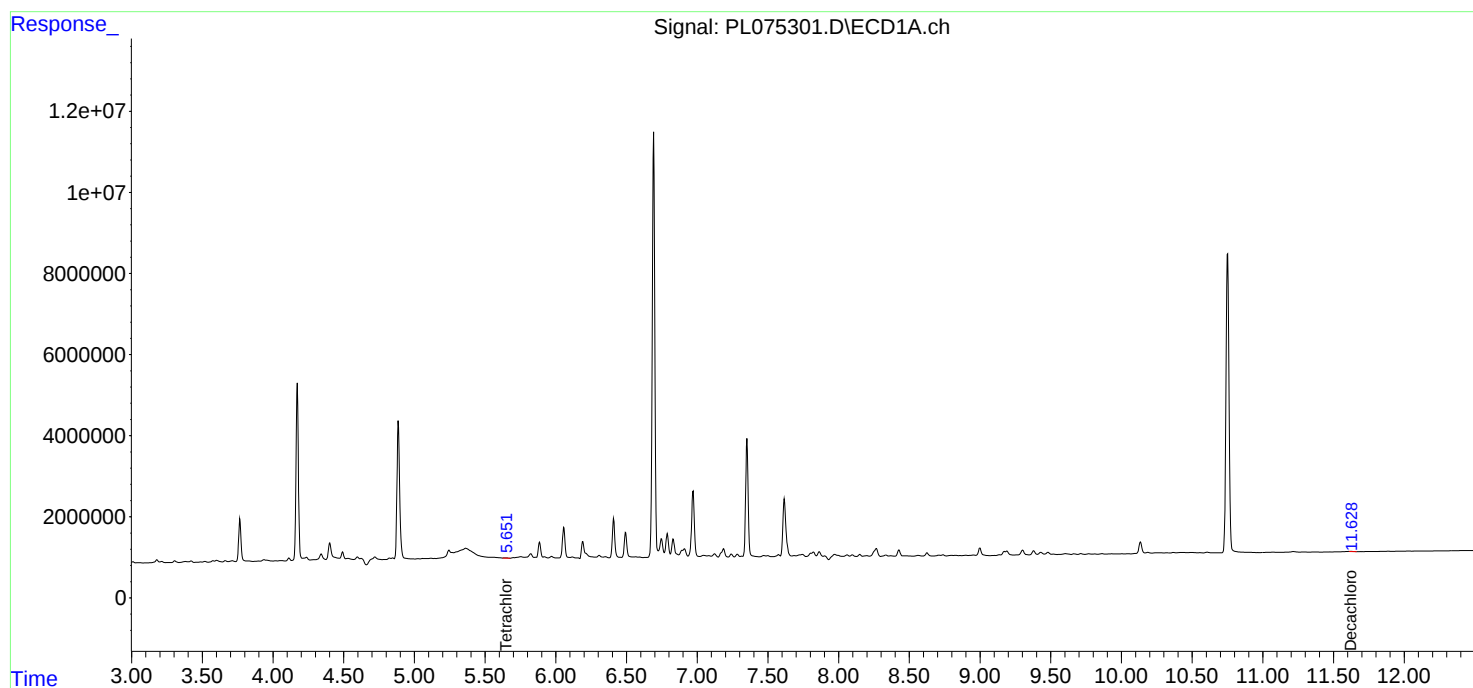

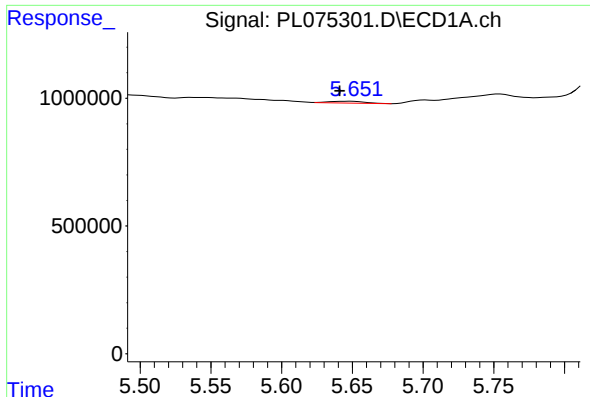

#1 Tetrachloro-m-xylene

R.T.: 5.651 min
Delta R.T.: 0.010 min
Response: 118255
Conc: 0.20 ng/ml

Instrument :

ECD_L

ClientSampleId :

PB144972BS

Manual Integrations

APPROVED

Reviewed By :Abdul Mirza 06/01/2022

Supervised By :Ankita Jodhani 06/01/2022

#1 Tetrachloro-m-xylene

R.T.: 4.644 min
Delta R.T.: 0.003 min
Response: 356103
Conc: 0.22 ng/ml m

#28 Decachlorobiphenyl

R.T.: 11.628 min
Delta R.T.: -0.013 min
Response: 58387
Conc: 0.11 ng/ml m

#28 Decachlorobiphenyl

R.T.: 10.401 min
Delta R.T.: 0.009 min
Response: 28760
Conc: 0.02 ng/ml m