

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL053123\
 Data File : PL083118.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 May 2023 14:52
 Operator : AR\AJ
 Sample : 02977-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 FOUNDATION-TEST-PIT

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 01 05:07:52 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051923.M
 Quant Title : GC Extractables
 QLast Update : Sat May 20 04:58:53 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.320	2.633	59733248	52670398	20.324	20.288
28)	SA Decachlor...	8.740	7.742	46435887	52591274	22.140	21.150
Target Compounds							
13)	MA Dieldrin	6.095	5.197	1798237	2015455	0.598	0.714



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL053123\
Data File : PL083118.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 May 2023 14:52
Operator : AR\AJ
Sample : 02977-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
FOUNDATION-TEST-PIT

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 01 05:07:52 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051923.M
Quant Title : GC Extractables
QLast Update : Sat May 20 04:58:53 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

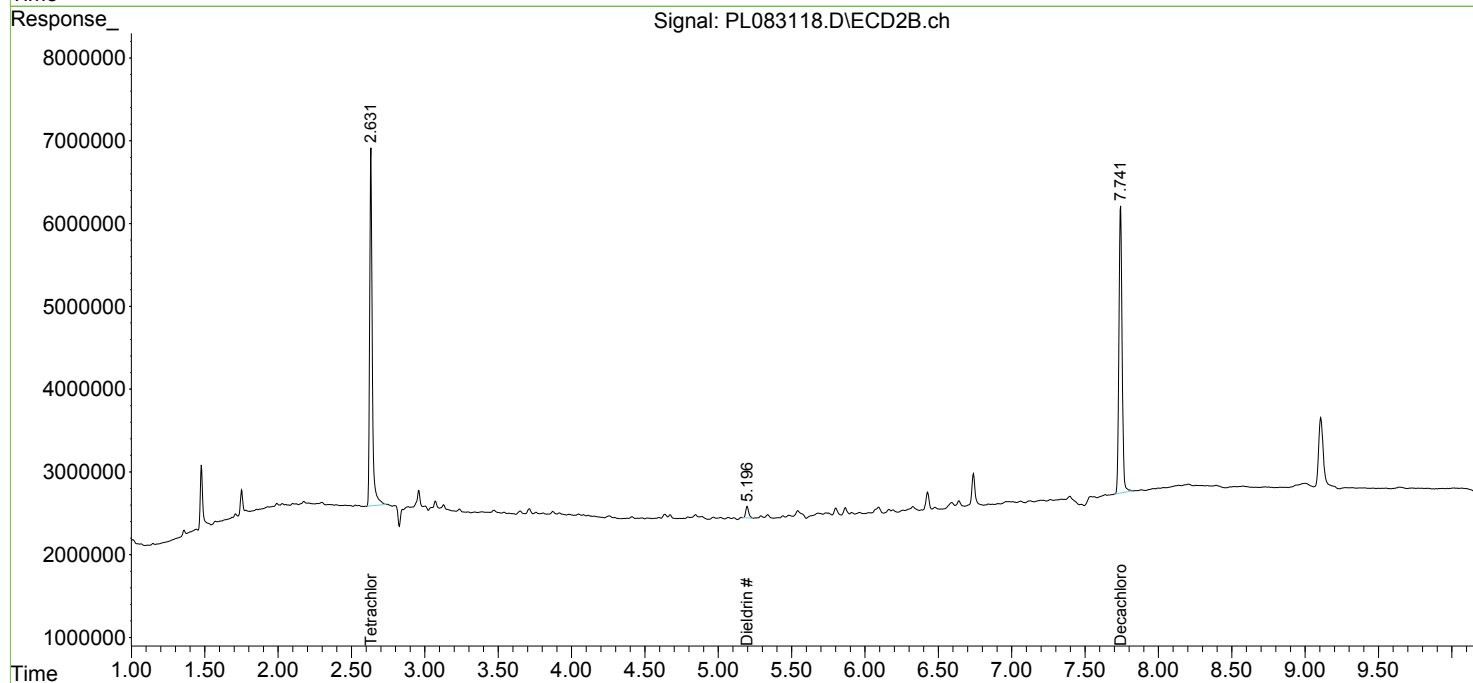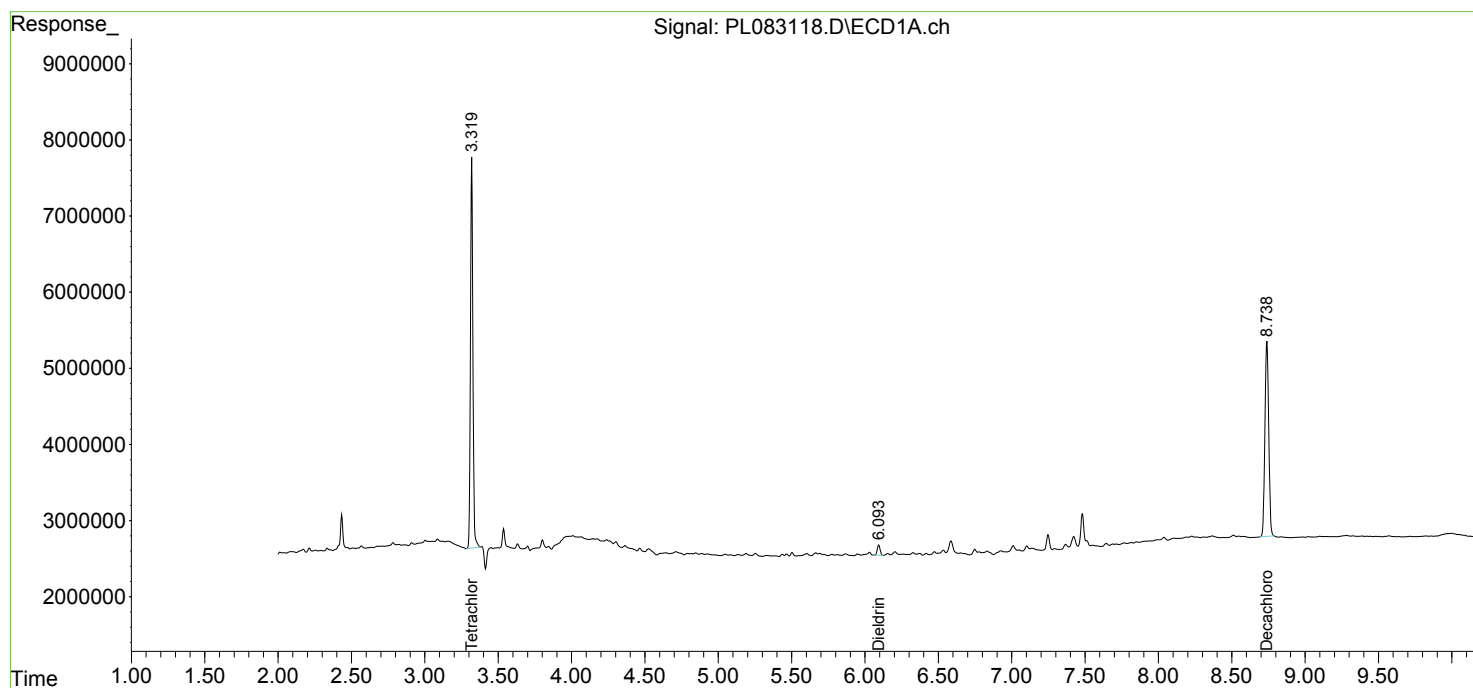


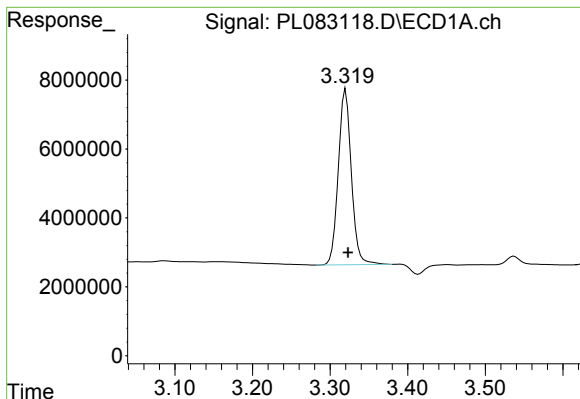

#1 Tetrachloro-m-xylene


R.T.: 3.320 min
Delta R.T.: -0.003 min
Response: 59733248
Conc: 20.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
FOUNDATION-TEST-PIT

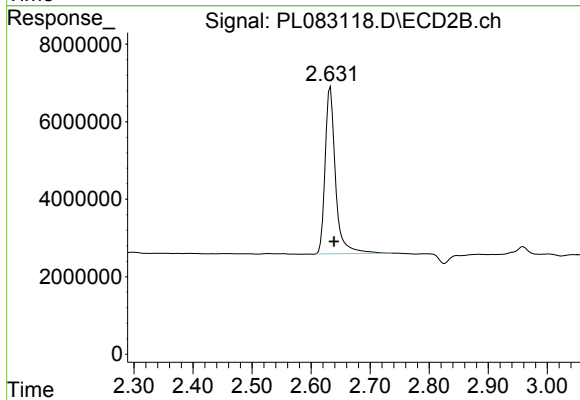


#1 Tetrachloro-m-xylene

R.T.: 2.633 min
Delta R.T.: -0.006 min
Response: 52670398
Conc: 20.29 ng/ml

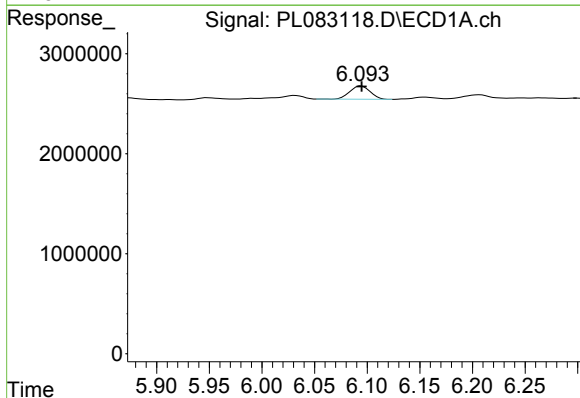


#13 Dieldrin

R.T.: 6.095 min
Delta R.T.: 0.000 min
Response: 1798237
Conc: 0.60 ng/ml

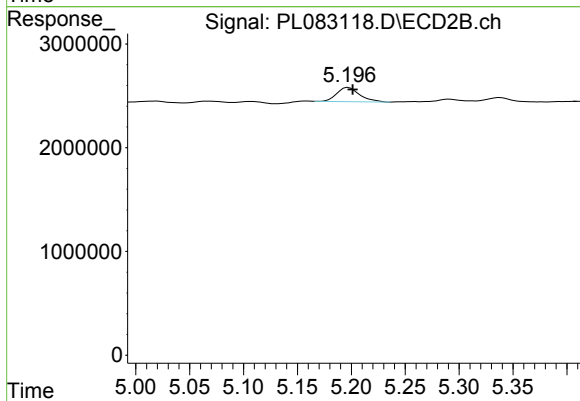

#13 Dieldrin


R.T.: 5.197 min
Delta R.T.: -0.004 min
Response: 2015455
Conc: 0.71 ng/ml

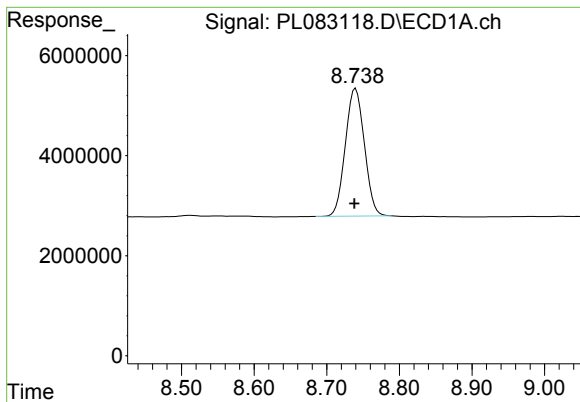

#28 Decachlorobiphenyl

R.T.: 8.740 min
Delta R.T.: 0.002 min
Response: 46435887
Conc: 22.14 ng/ml

Instrument :
ECD_L
ClientSampleId :
FOUNDATION-TEST-PIT

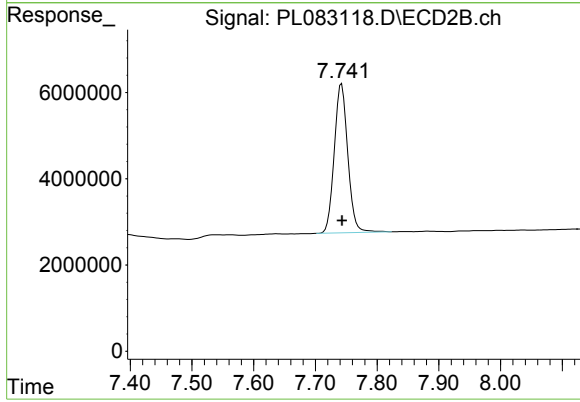

#28 Decachlorobiphenyl

R.T.: 7.742 min
Delta R.T.: -0.001 min
Response: 52591274
Conc: 21.15 ng/ml