

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060121\
 Data File : PL066969.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Jun 2021 16:52
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 02 02:30:58 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060121.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 02 02:30:26 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.479	5.530	43508343	68647250	103.577	102.979
28)	SA Decachlor...	10.225	11.432	61850418	80848392	94.396	95.506
Target Compounds							
23)	Chlordane-1	5.800	6.912	14646486	22448877	1030.199	1075.903
24)	Chlordane-2	6.486	7.503	19575078	27214706	972.635	980.890
25)	Chlordane-3	7.185	8.260	55750085	107.6E6	1010.808	1053.471
26)	Chlordane-4	7.251	8.342	61106283	129.4E6	1013.974	1037.397
27)	Chlordane-5	8.192	9.229	17838679	24164117	1001.920	1011.794



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060121\
Data File : PL066969.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Jun 2021 16:52
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 02 02:30:58 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060121.M
Quant Title : GC Extractables
QLast Update : Wed Jun 02 02:30:26 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

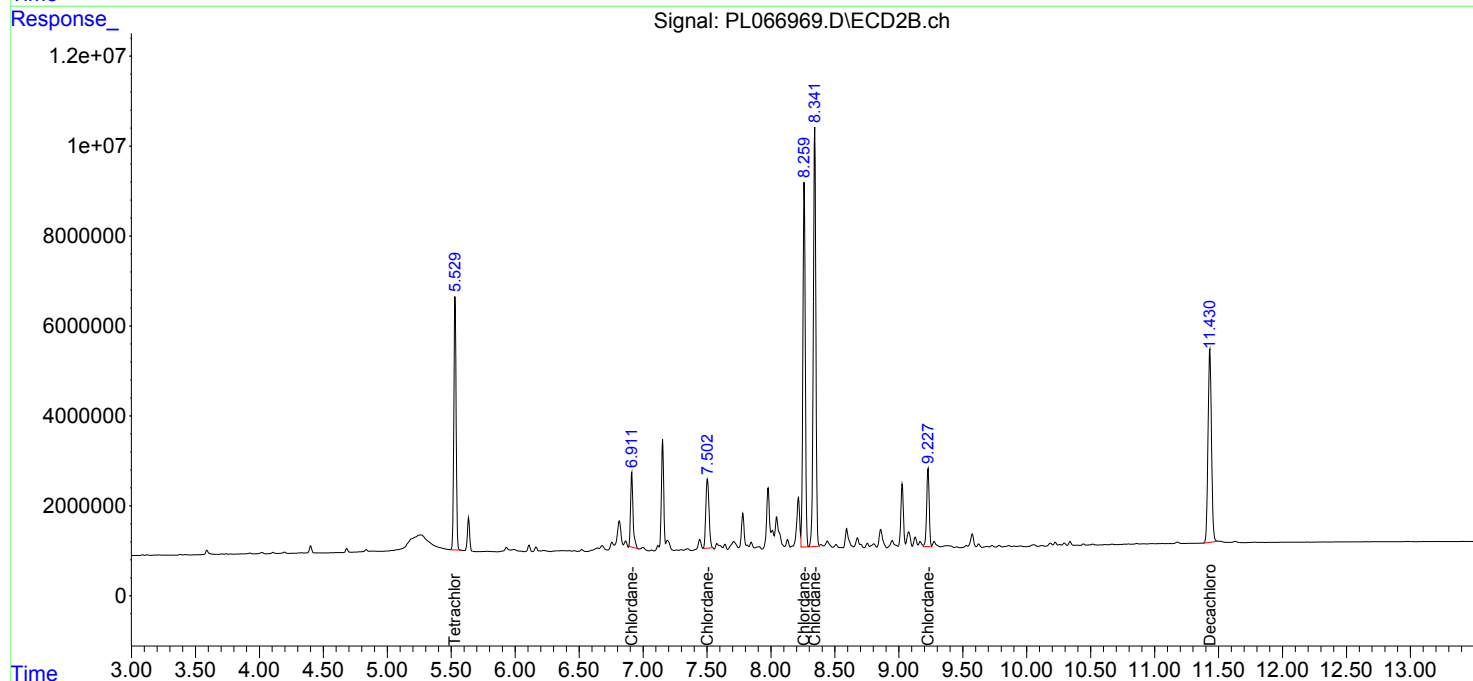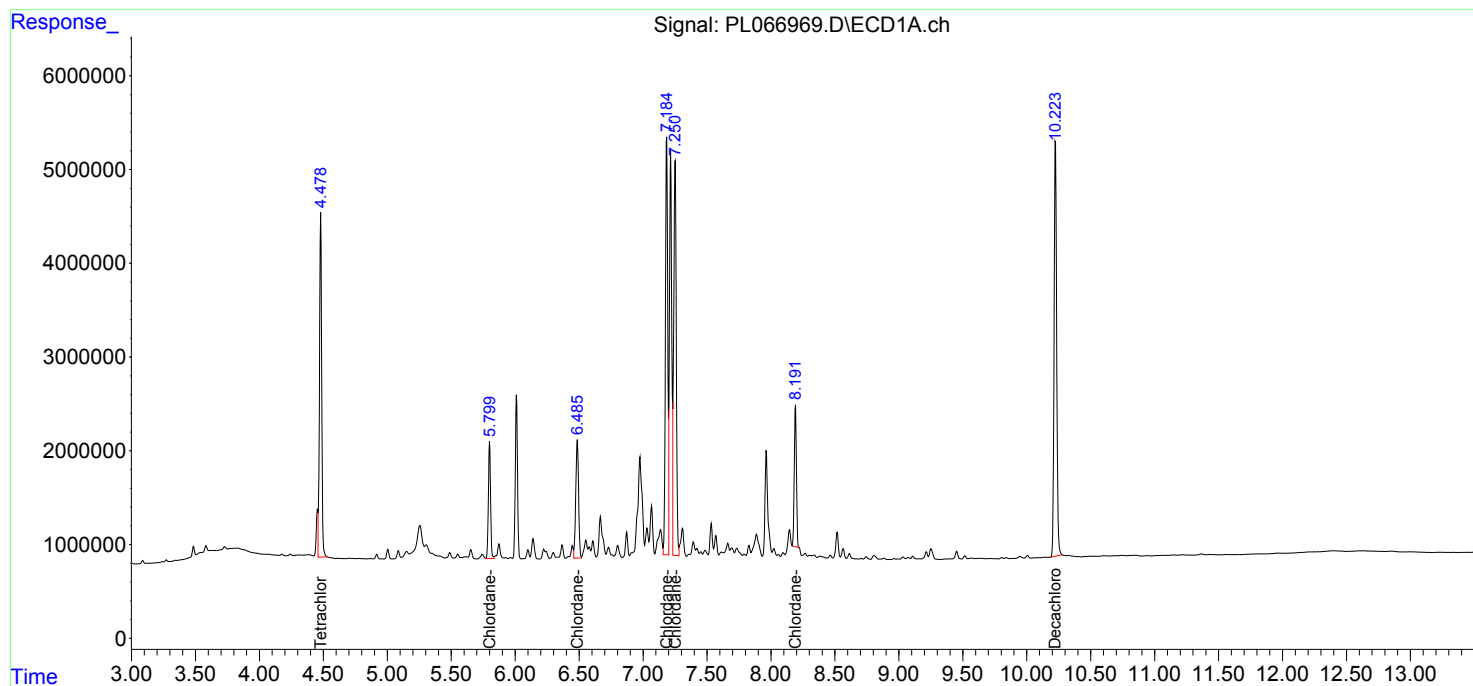


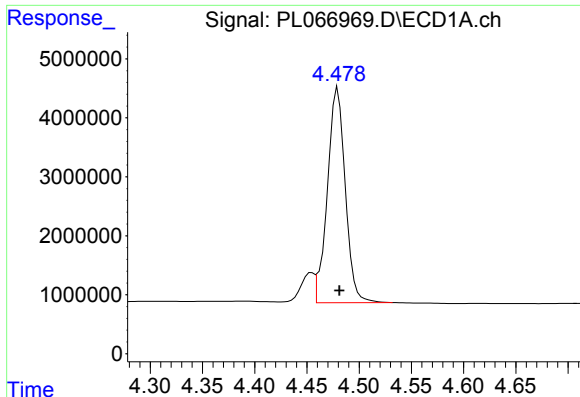

#1 Tetrachloro-m-xylene


R.T.: 4.479 min
Delta R.T.: -0.002 min
Response: 43508343
Conc: 103.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

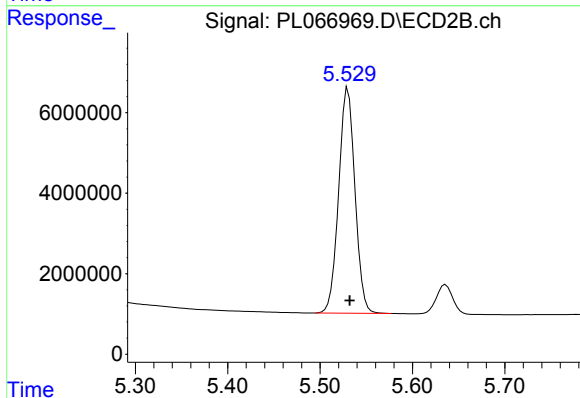


#1 Tetrachloro-m-xylene

R.T.: 5.530 min
Delta R.T.: -0.002 min
Response: 68647250
Conc: 102.98 ng/ml

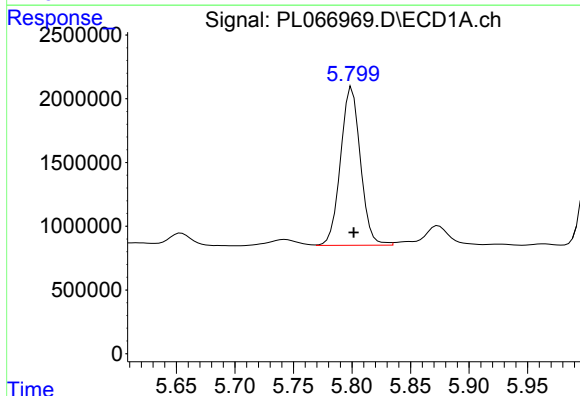


#23 Chlordane-1

R.T.: 5.800 min
Delta R.T.: -0.002 min
Response: 14646486
Conc: 1030.20 ng/ml

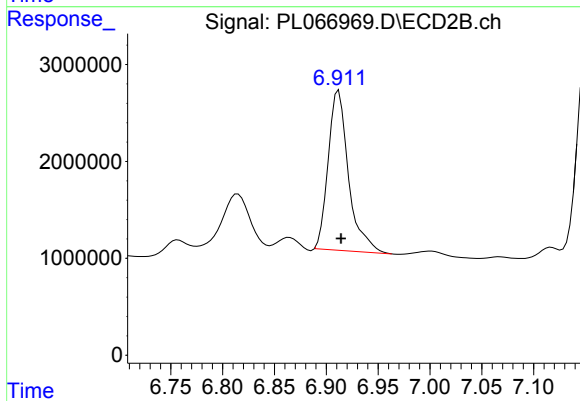

#23 Chlordane-1


R.T.: 6.912 min
Delta R.T.: -0.003 min
Response: 22448877
Conc: 1075.90 ng/ml

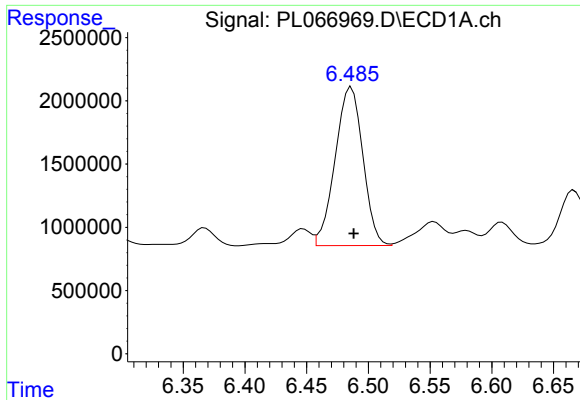

#24 Chlordane-2


R.T.: 6.486 min
Delta R.T.: -0.002 min
Response: 19575078
Conc: 972.64 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

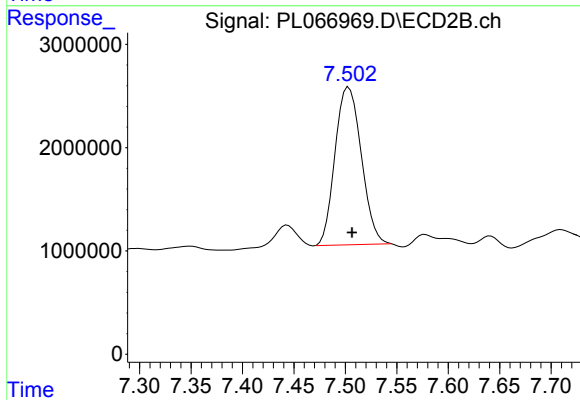


#24 Chlordane-2

R.T.: 7.503 min
Delta R.T.: -0.003 min
Response: 27214706
Conc: 980.89 ng/ml

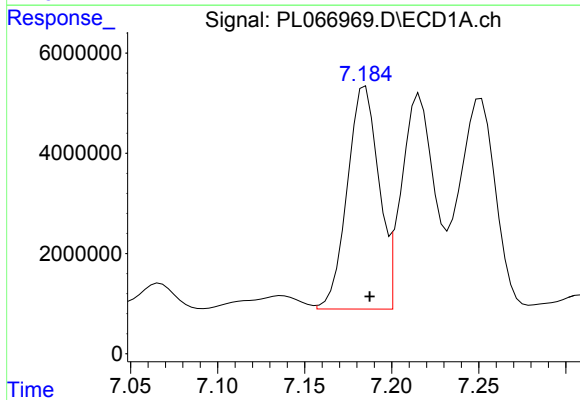


#25 Chlordane-3

R.T.: 7.185 min
Delta R.T.: -0.002 min
Response: 55750085
Conc: 1010.81 ng/ml

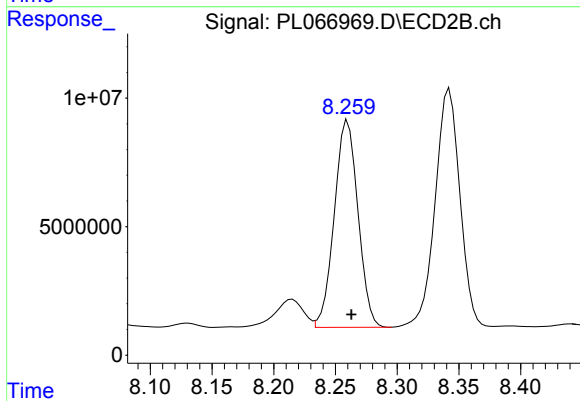

#25 Chlordane-3


R.T.: 8.260 min
Delta R.T.: -0.003 min
Response: 107639994
Conc: 1053.47 ng/ml

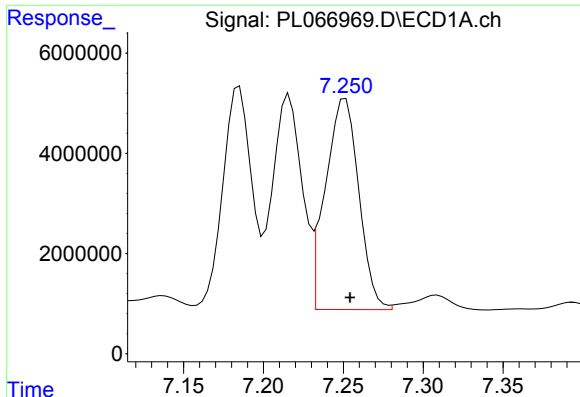

#26 Chlordane-4


R.T.: 7.251 min
Delta R.T.: -0.003 min
Response: 61106283
Conc: 1013.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

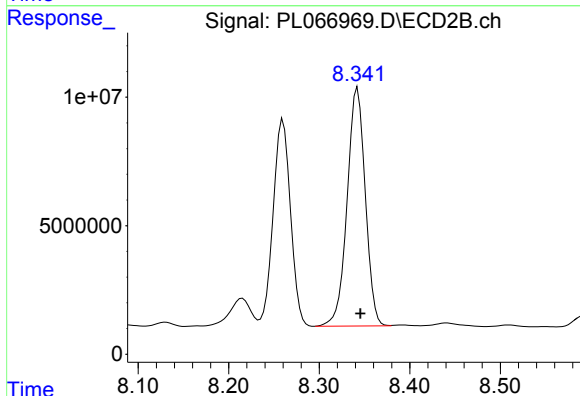


#26 Chlordane-4

R.T.: 8.342 min
Delta R.T.: -0.003 min
Response: 129437682
Conc: 1037.40 ng/ml

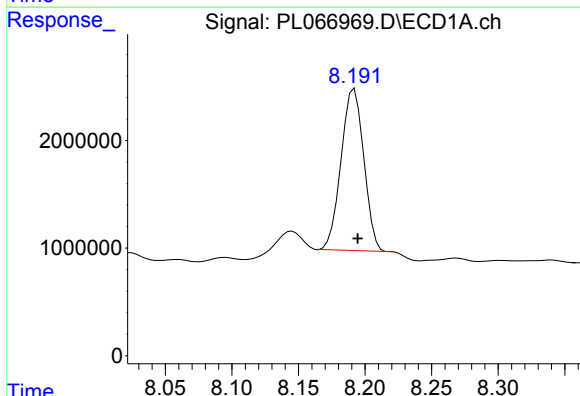


#27 Chlordane-5

R.T.: 8.192 min
Delta R.T.: -0.003 min
Response: 17838679
Conc: 1001.92 ng/ml

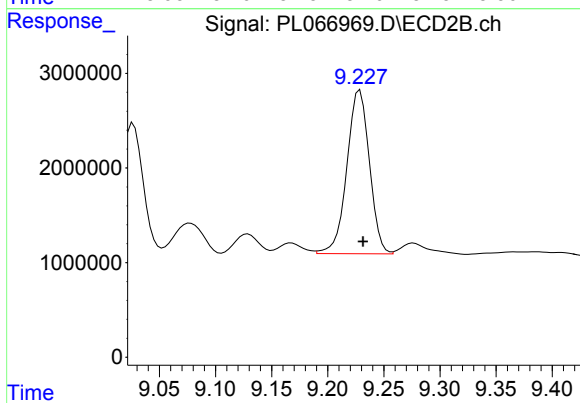

#27 Chlordane-5


R.T.: 9.229 min
Delta R.T.: -0.003 min
Response: 24164117
Conc: 1011.79 ng/ml

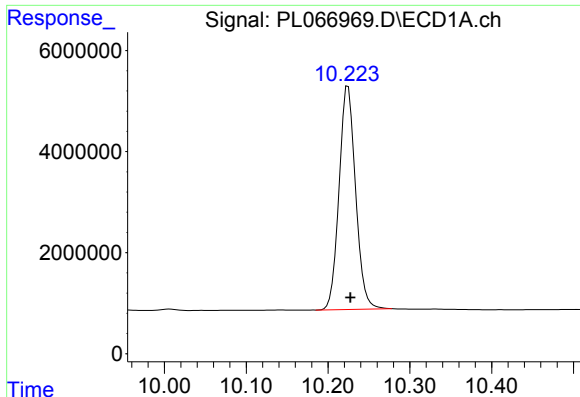

#28 Decachlorobiphenyl

R.T.: 10.225 min
Delta R.T.: -0.003 min
Response: 61850418
Conc: 94.40 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

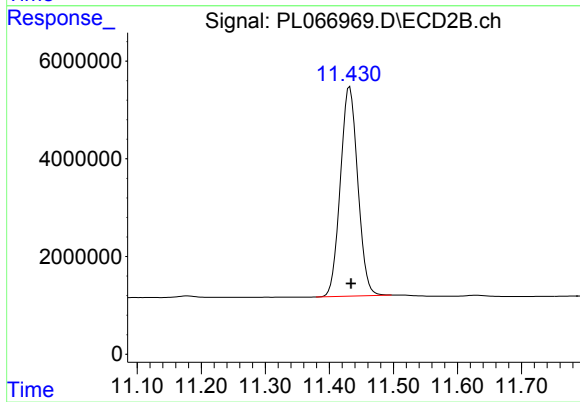

#28 Decachlorobiphenyl

R.T.: 11.432 min
Delta R.T.: -0.002 min
Response: 80848392
Conc: 95.51 ng/ml