

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060121\
 Data File : PL066970.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Jun 2021 17:11
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 02 02:31:06 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060121.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 02 02:30:26 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.480	5.532	33858143	53398460	80.603	80.104
28)	SA Decachlor...	10.227	11.434	48816339	63070086	74.503	74.504
Target Compounds							
23)	Chlordane-1	5.802	6.914	11747425	17275357	826.286	827.953
24)	Chlordane-2	6.488	7.506	15876176	21308388	788.846	768.011
25)	Chlordane-3	7.186	8.263	44836534	82696841	812.934	809.353
26)	Chlordane-4	7.253	8.345	48762794	99893452	809.151	800.611
27)	Chlordane-5	8.194	9.231	14143313	18704438	794.368	783.188



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060121\
Data File : PL066970.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Jun 2021 17:11
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 02 02:31:06 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060121.M
Quant Title : GC Extractables
QLast Update : Wed Jun 02 02:30:26 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

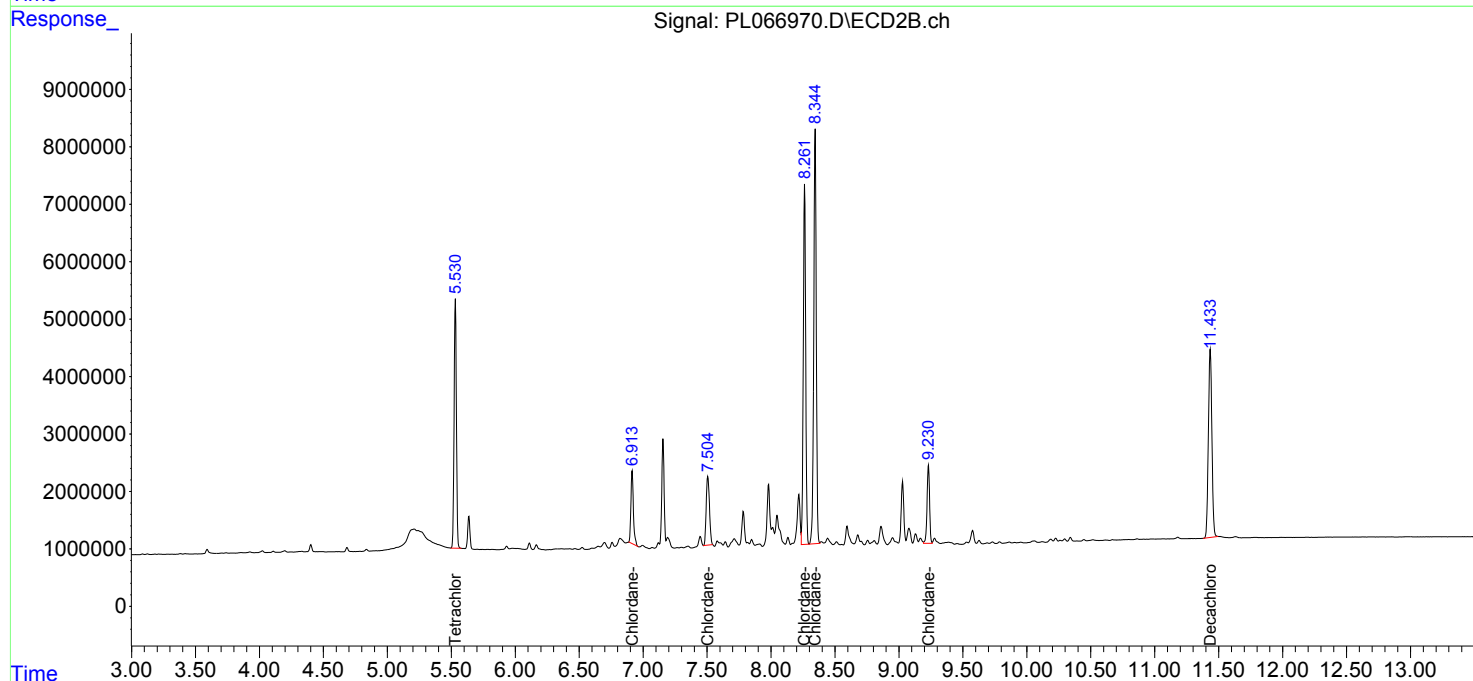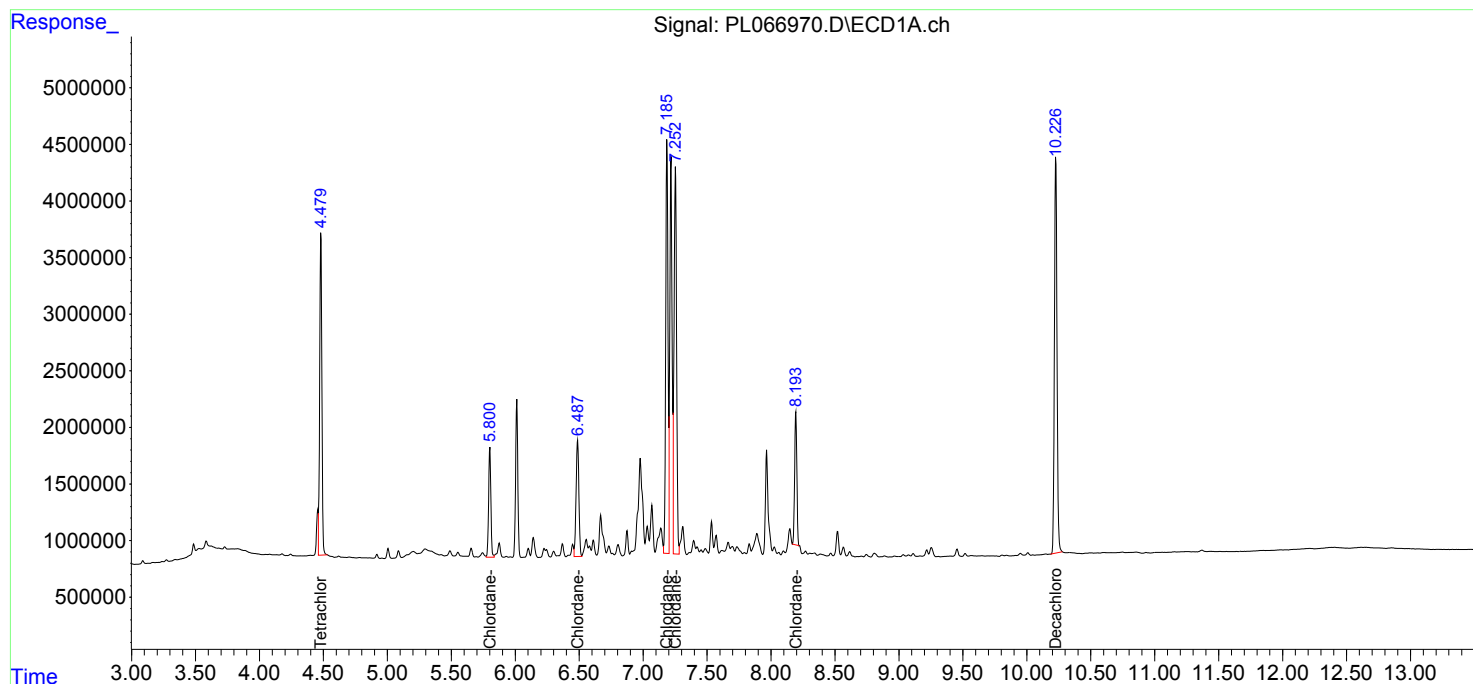


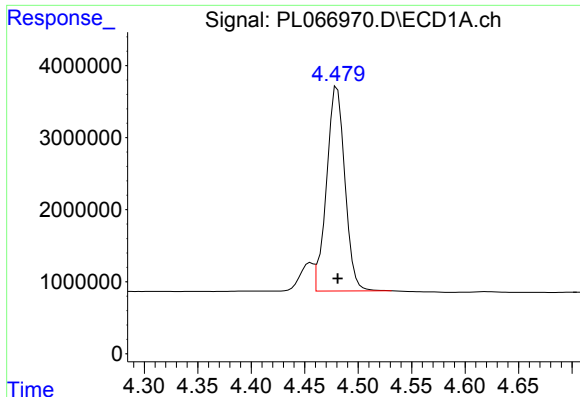

#1 Tetrachloro-m-xylene


R.T.: 4.480 min
Delta R.T.: 0.000 min
Response: 33858143
Conc: 80.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

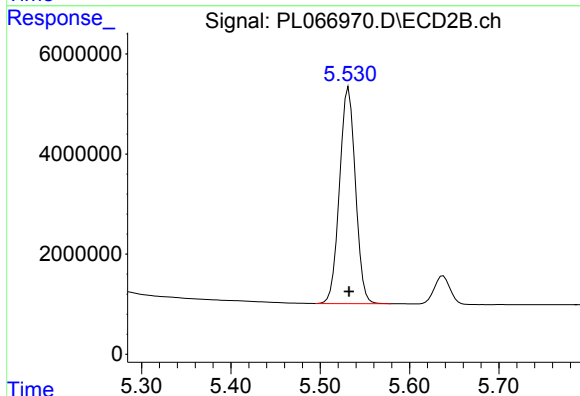


#1 Tetrachloro-m-xylene

R.T.: 5.532 min
Delta R.T.: 0.000 min
Response: 53398460
Conc: 80.10 ng/ml

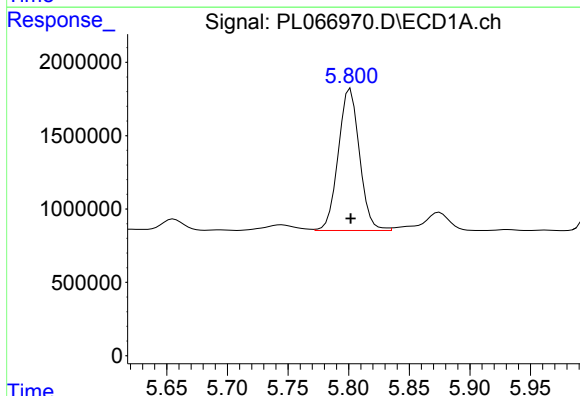


#23 Chlordane-1

R.T.: 5.802 min
Delta R.T.: 0.000 min
Response: 11747425
Conc: 826.29 ng/ml

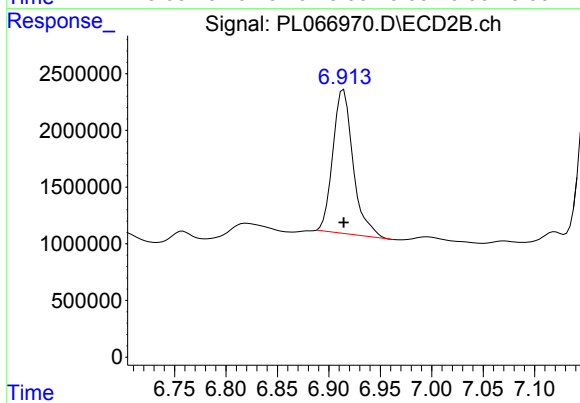

#23 Chlordane-1


R.T.: 6.914 min
Delta R.T.: 0.000 min
Response: 17275357
Conc: 827.95 ng/ml

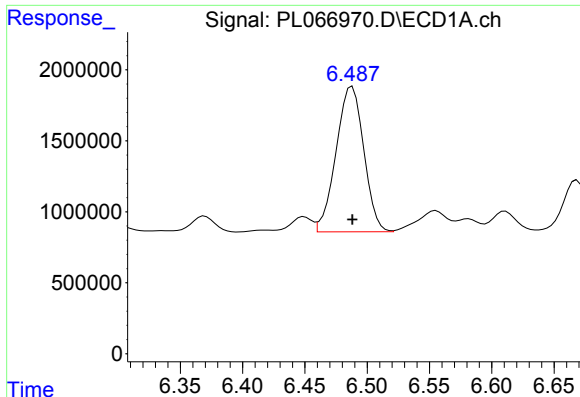

#24 Chlordane-2


R.T.: 6.488 min
Delta R.T.: 0.000 min
Response: 15876176
Conc: 788.85 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

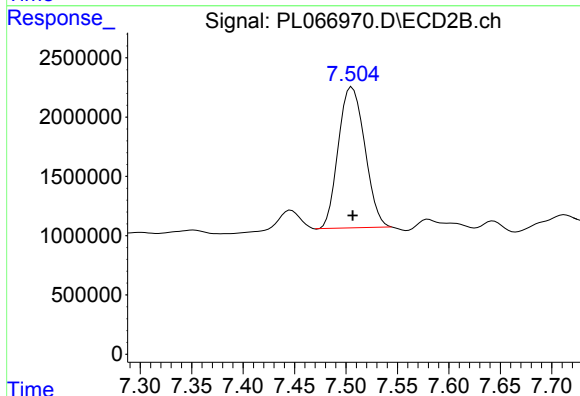


#24 Chlordane-2

R.T.: 7.506 min
Delta R.T.: 0.000 min
Response: 21308388
Conc: 768.01 ng/ml

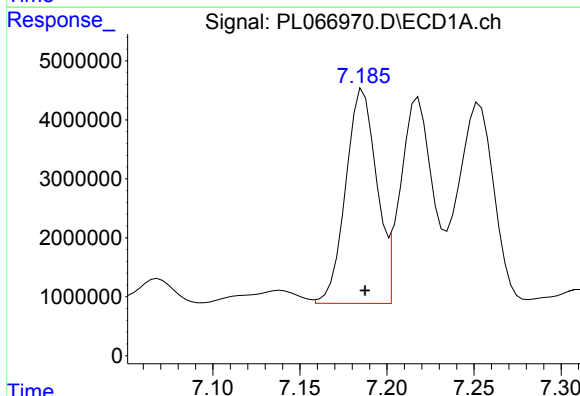


#25 Chlordane-3

R.T.: 7.186 min
Delta R.T.: 0.000 min
Response: 44836534
Conc: 812.93 ng/ml

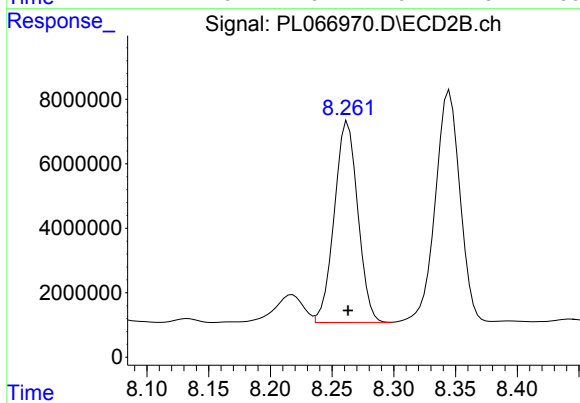

#25 Chlordane-3


R.T.: 8.263 min
Delta R.T.: 0.000 min
Response: 82696841
Conc: 809.35 ng/ml

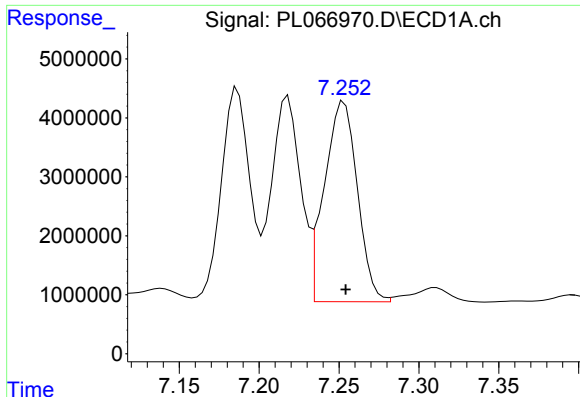

#26 Chlordane-4


R.T.: 7.253 min
Delta R.T.: 0.000 min
Response: 48762794
Conc: 809.15 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

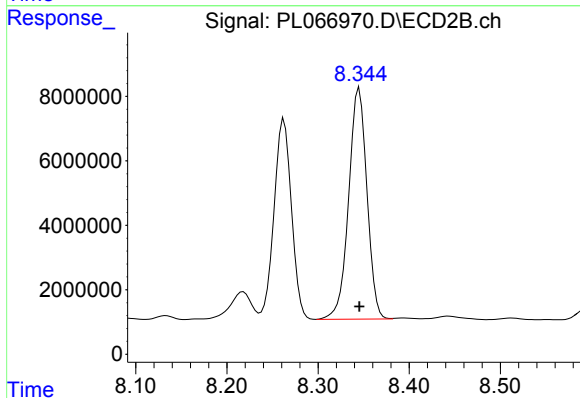


#26 Chlordane-4

R.T.: 8.345 min
Delta R.T.: 0.000 min
Response: 99893452
Conc: 800.61 ng/ml

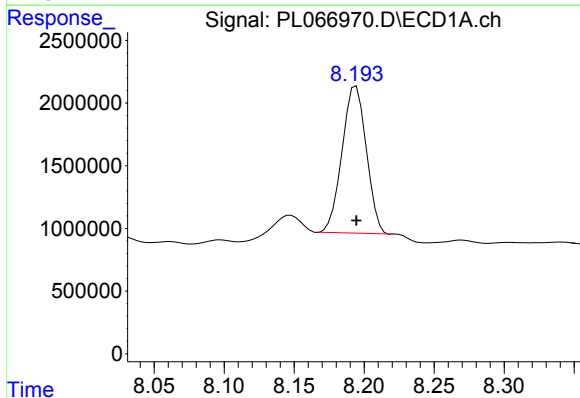


#27 Chlordane-5

R.T.: 8.194 min
Delta R.T.: 0.000 min
Response: 14143313
Conc: 794.37 ng/ml

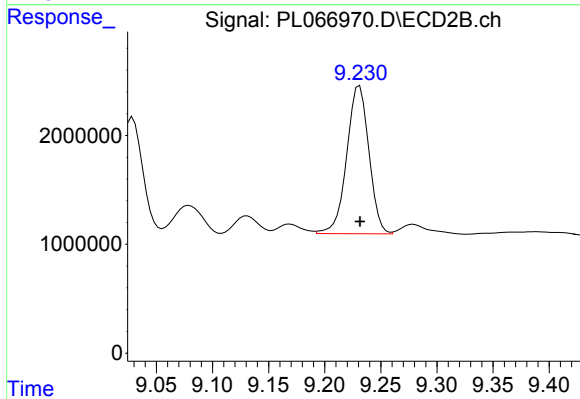

#27 Chlordane-5


R.T.: 9.231 min
Delta R.T.: 0.000 min
Response: 18704438
Conc: 783.19 ng/ml

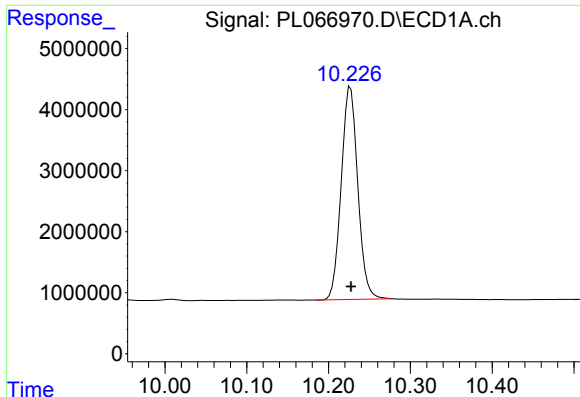

#28 Decachlorobiphenyl

R.T.: 10.227 min
Delta R.T.: 0.000 min
Response: 48816339
Conc: 74.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

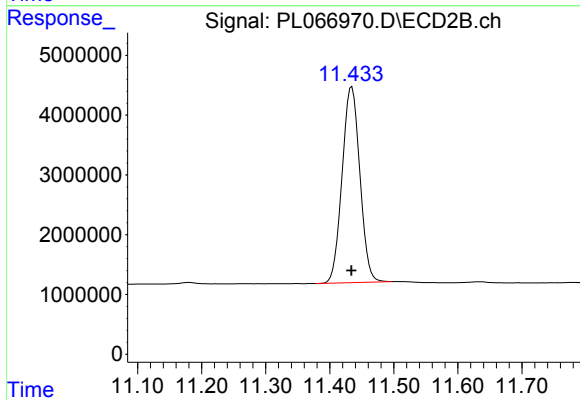

#28 Decachlorobiphenyl

R.T.: 11.434 min
Delta R.T.: 0.000 min
Response: 63070086
Conc: 74.50 ng/ml