

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060122\
 Data File : PL075341.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Jun 2022 09:18
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 02 05:59:01 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 01 10:19:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.643	4.641	12209413	31573519	20.774	19.931
28)	SA Decachlor...	11.641	10.389	11432456	24245087	21.322	17.668
Target Compounds							
7)	B delta-BHC	0.000	6.404	0	213600	N.D.	0.100 #
11)	B alpha-Chl...	0.000	7.397f	0	83053	N.D.	0.045 #
14)	MA Endrin	0.000	8.071f	0	668368	N.D.	0.429 #
17)	MA 4,4'-DDT	9.528	0.000	166248	0	0.285	N.D. #
19)	B Endosulfa...	9.668	0.000	69543	0	0.125	N.D. #
21)	B Endrin ke...	10.188f	0.000	301775	0	0.492	N.D. #
26)	Chlordane-4	0.000	7.397f	0	83053	N.D.	0.440 #
27)	Chlordane-5	0.000	8.159f	0	340408	N.D.	6.822 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060122\
Data File : PL075341.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Jun 2022 09:18
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 02 05:59:01 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
Quant Title : GC Extractables
QLast Update : Wed Jun 01 10:19:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

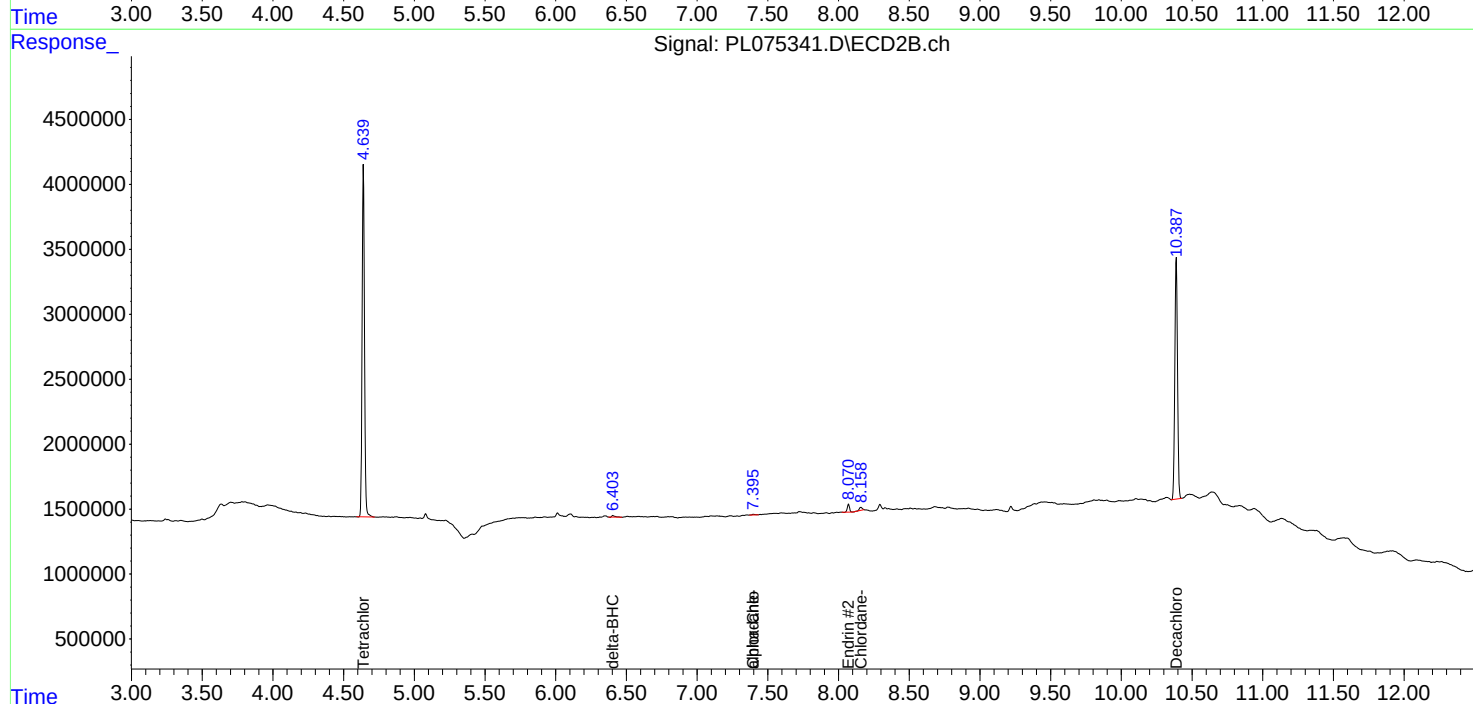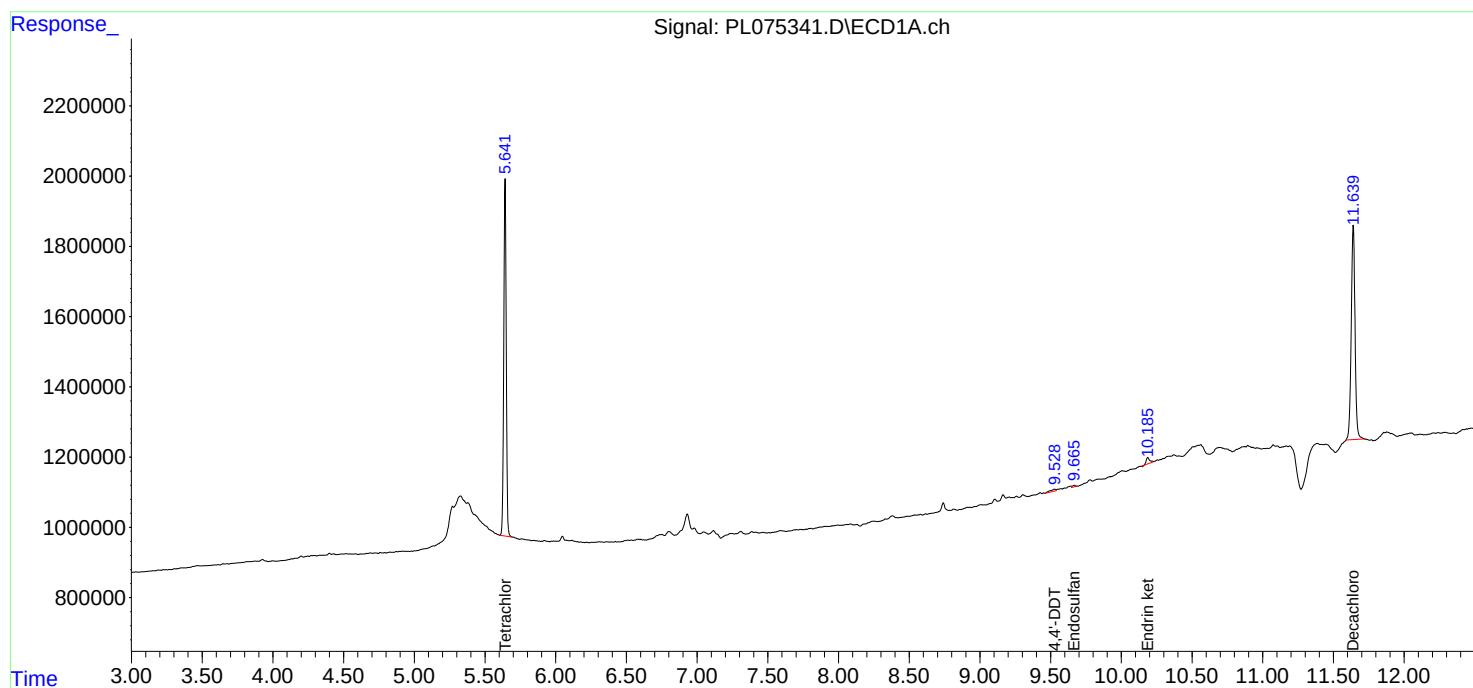


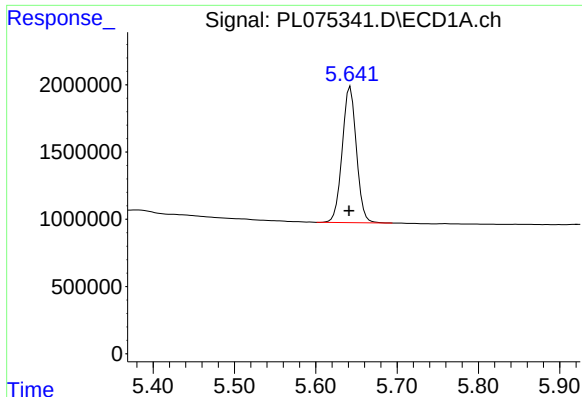

#1 Tetrachloro-m-xylene


R.T.: 5.643 min
Delta R.T.: 0.002 min
Response: 12209413
Conc: 20.77 ng/ml

Instrument :
ECD_L
ClientSampleId :

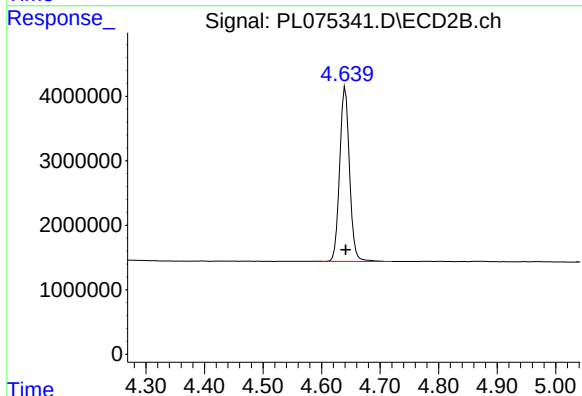


#1 Tetrachloro-m-xylene

R.T.: 4.641 min
Delta R.T.: -0.001 min
Response: 31573519
Conc: 19.93 ng/ml

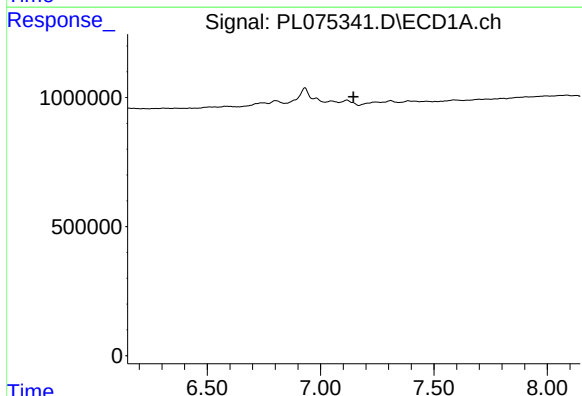


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 7.146 min
Response: 0
Conc: N.D.

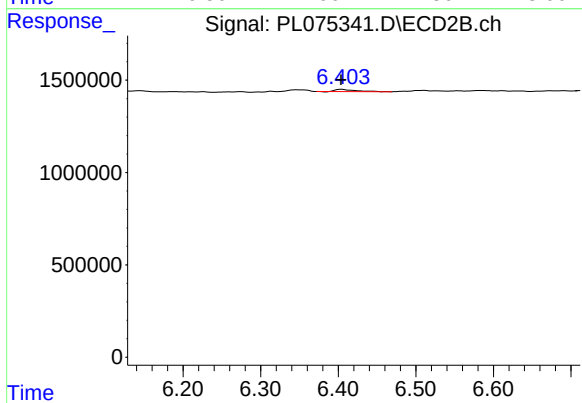

#7 delta-BHC


R.T.: 6.404 min
Delta R.T.: 0.001 min
Response: 213600
Conc: 0.10 ng/ml

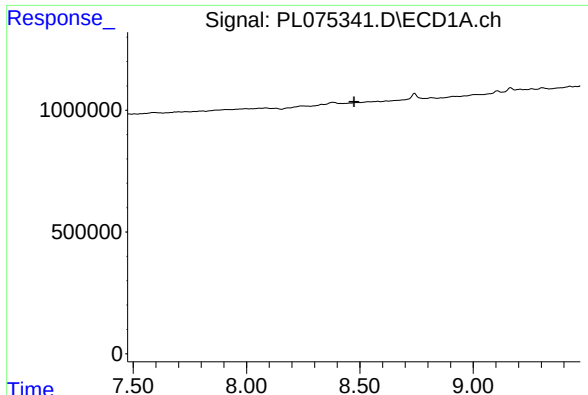

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 8.474 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

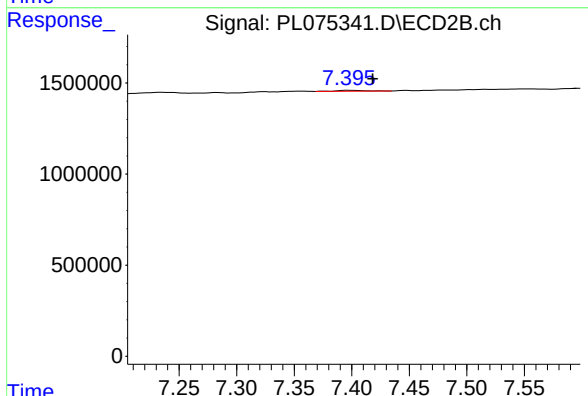


#11 alpha-Chlordane

R.T.: 7.397 min
Delta R.T.: -0.021 min
Response: 83053
Conc: 0.05 ng/ml

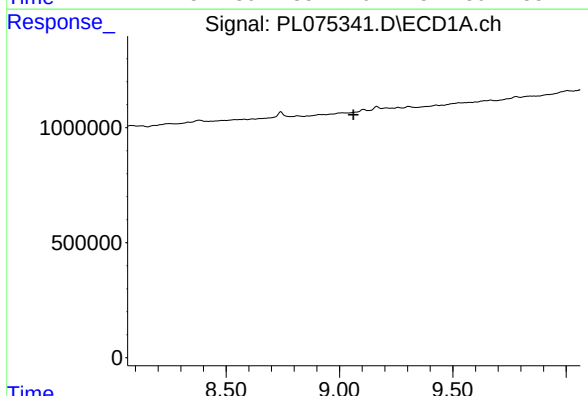


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 9.062 min
Response: 0
Conc: N.D.

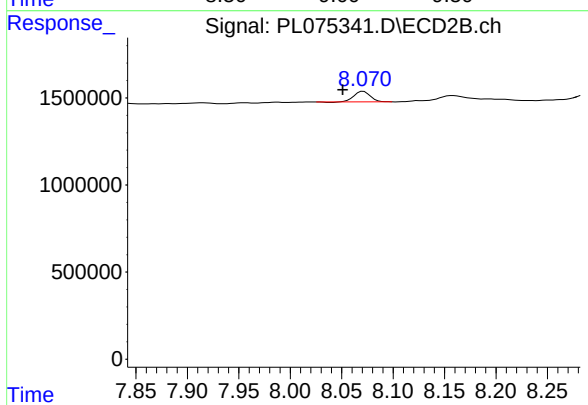

#14 Endrin


R.T.: 8.071 min
Delta R.T.: 0.020 min
Response: 668368
Conc: 0.43 ng/ml

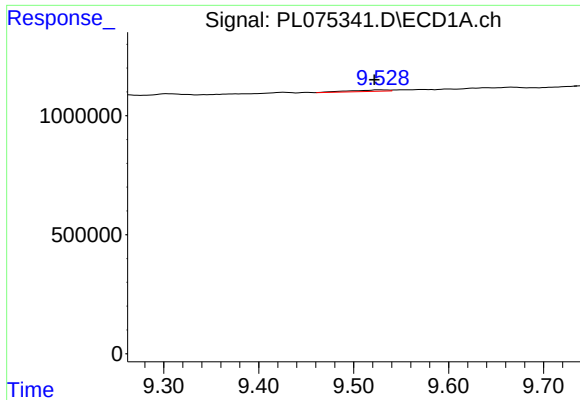

#17 4,4'-DDT


R.T.: 9.528 min
Delta R.T.: 0.006 min
Response: 166248
Conc: 0.29 ng/ml

Instrument :
ECD_L
ClientSampleId :

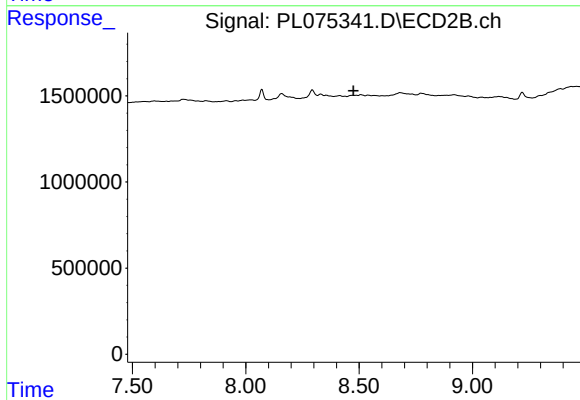


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 8.476 min
Response: 0
Conc: N.D.

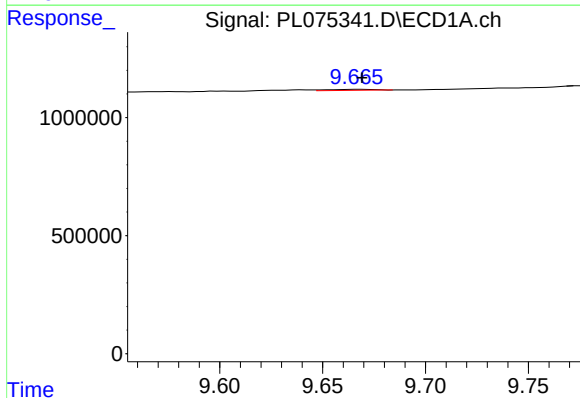


#19 Endosulfan Sulfate

R.T.: 9.668 min
Delta R.T.: -0.002 min
Response: 69543
Conc: 0.13 ng/ml

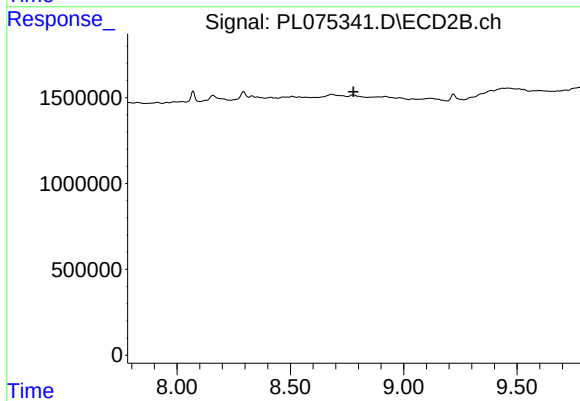

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 8.779 min
Response: 0
Conc: N.D.

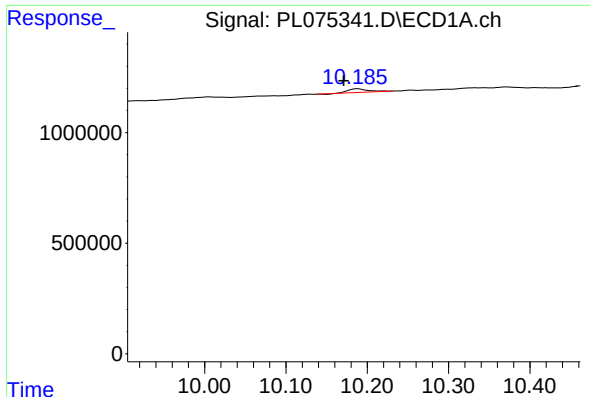

#21 Endrin ketone


R.T.: 10.188 min
Delta R.T.: 0.017 min
Response: 301775
Conc: 0.49 ng/ml

Instrument :
ECD_L
ClientSampleId :

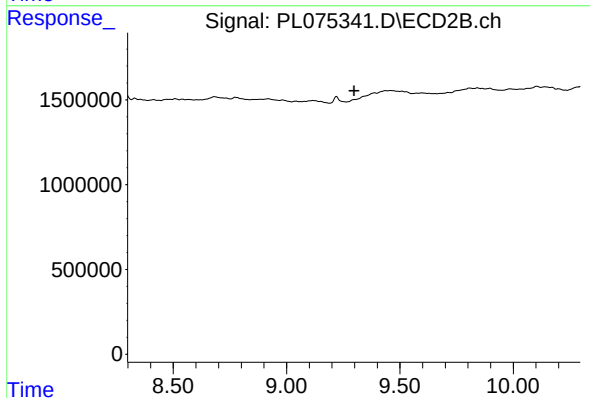


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.298 min
Response: 0
Conc: N.D.

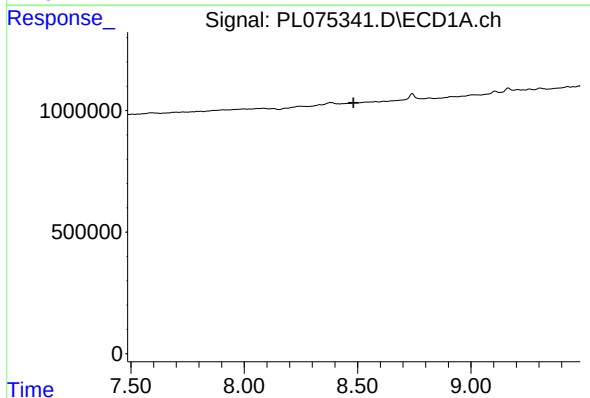


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 8.482 min
Response: 0
Conc: N.D.

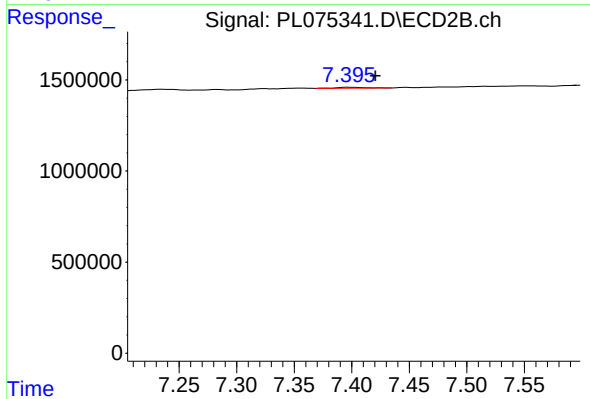

#26 Chlordane-4


R.T.: 7.397 min
Delta R.T.: -0.023 min
Response: 83053
Conc: 0.44 ng/ml

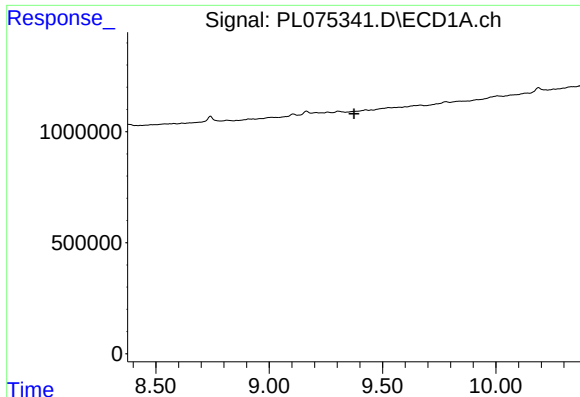

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 9.375 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

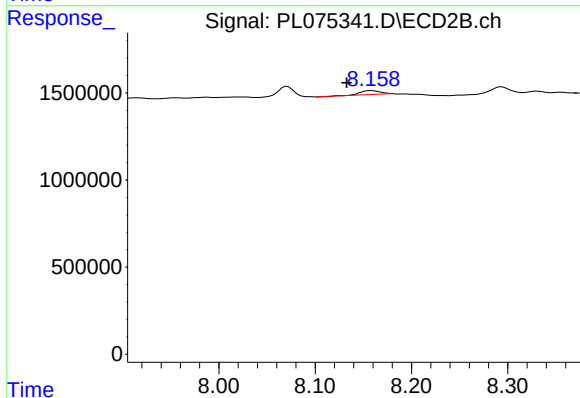


#27 Chlordane-5

R.T.: 8.159 min
Delta R.T.: 0.026 min
Response: 340408
Conc: 6.82 ng/ml

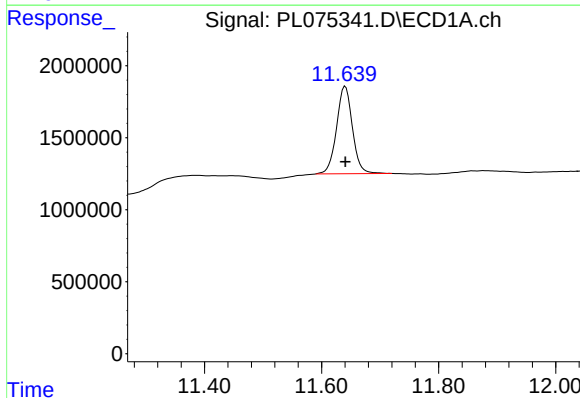

#28 Decachlorobiphenyl

R.T.: 11.641 min
Delta R.T.: 0.000 min
Response: 11432456
Conc: 21.32 ng/ml

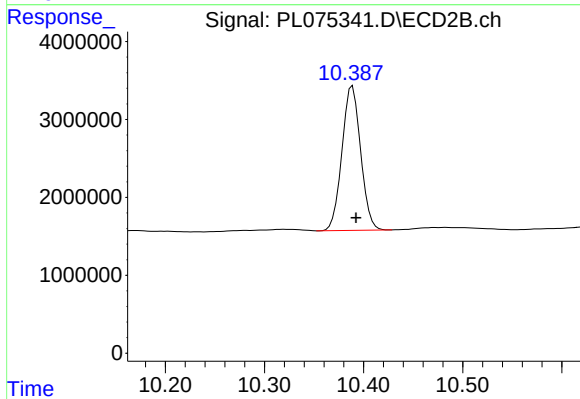

#28 Decachlorobiphenyl

R.T.: 10.389 min
Delta R.T.: -0.004 min
Response: 24245087
Conc: 17.67 ng/ml