

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060122\
 Data File : PL075344.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Jun 2022 10:53
 Operator : AR\AJ
 Sample : N3080-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 02 05:59:40 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 01 10:19:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.650	4.643	6264977	16643822	10.659	10.507
28)	SA Decachlor...	11.646	10.391	6452128	14523954	12.033	10.584
Target Compounds							
3)	MA gamma-BHC...	6.648f	0.000	395342	0	0.505	N.D. #
9)	A Endosulfan I	0.000	7.489	0	112742	N.D.	0.067 #
10)	B gamma-Chl...	0.000	7.343	0	311562	N.D.	0.169 #
12)	B 4,4'-DDE	0.000	7.631	0	328619	N.D.	0.202 #
14)	MA Endrin	0.000	8.073f	0	493460	N.D.	0.317 #
15)	B Endosulfa...	9.302	0.000	311988	0	0.553	N.D. #
17)	MA 4,4'-DDT	9.524	8.470	52082	418073	0.089	0.292 #
21)	B Endrin ke...	10.184	0.000	952469	0	1.551	N.D. #
23)	Chlordane-1	0.000	5.969	0	912755	N.D.	16.393 #
25)	Chlordane-3	0.000	7.343	0	311562	N.D.	1.765 #
27)	Chlordane-5	0.000	8.132	0	533114	N.D.	10.683 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060122\
Data File : PL075344.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Jun 2022 10:53
Operator : AR\AJ
Sample : N3080-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 02 05:59:40 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
Quant Title : GC Extractables
QLast Update : Wed Jun 01 10:19:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

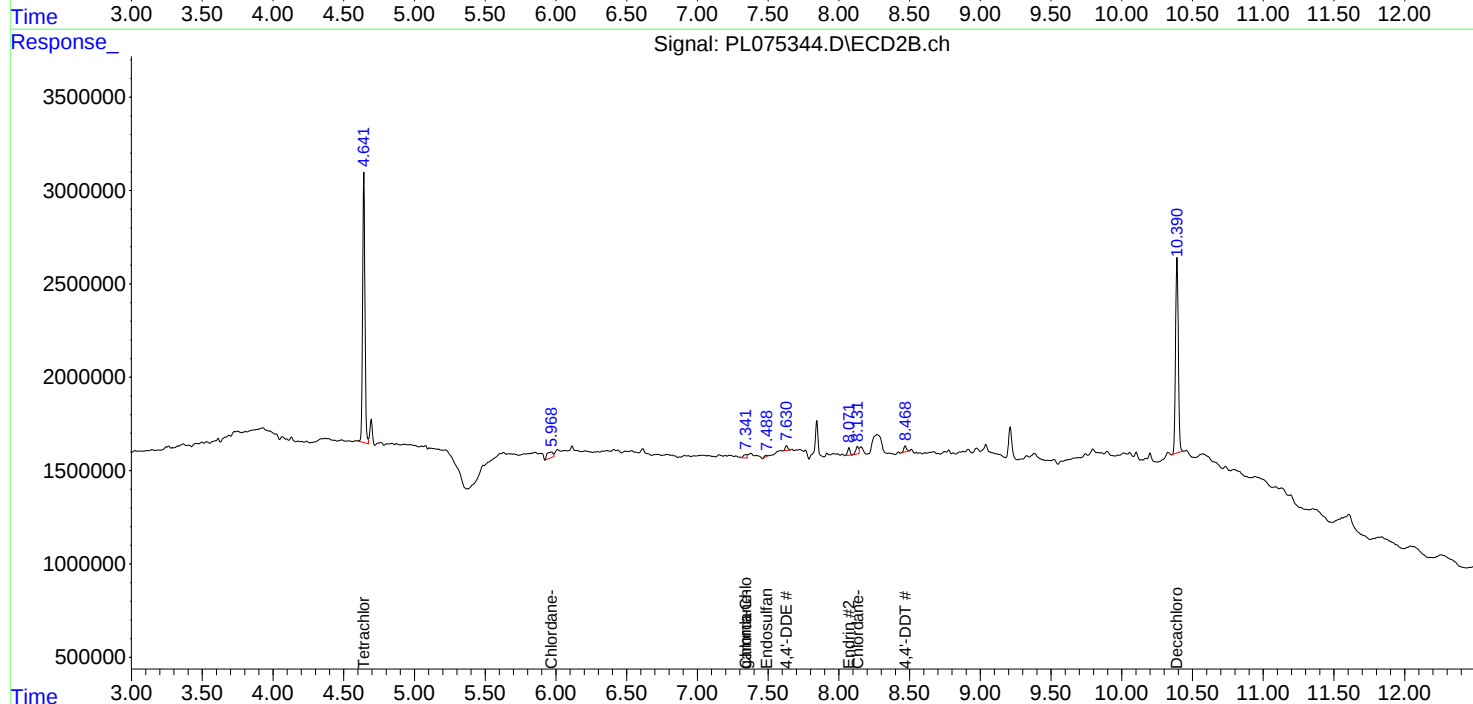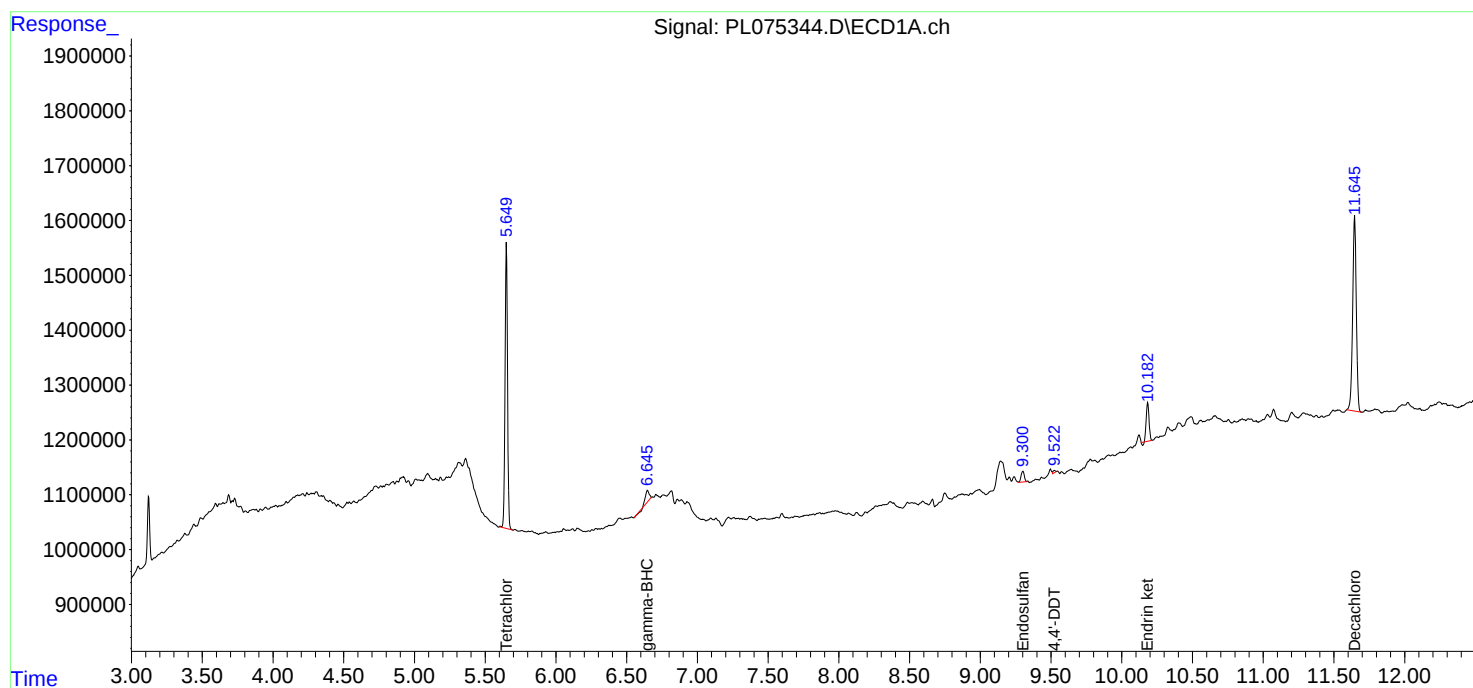


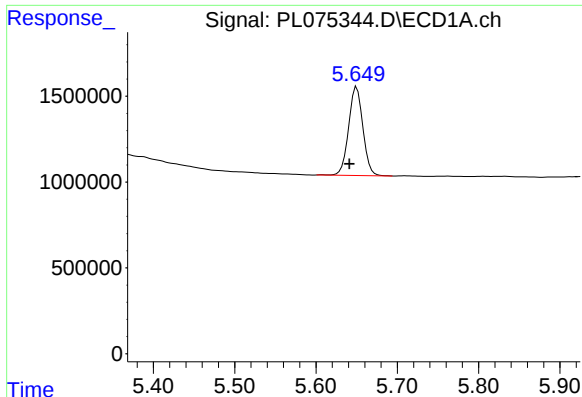

#1 Tetrachloro-m-xylene


R.T.: 5.650 min
Delta R.T.: 0.009 min
Response: 6264977
Conc: 10.66 ng/ml

Instrument :
ECD_L
ClientSampleId :

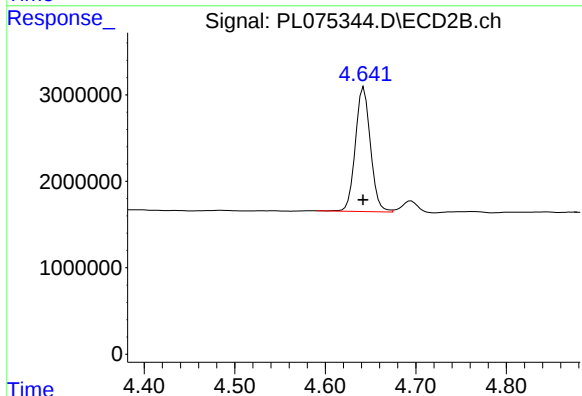


#1 Tetrachloro-m-xylene

R.T.: 4.643 min
Delta R.T.: 0.001 min
Response: 16643822
Conc: 10.51 ng/ml

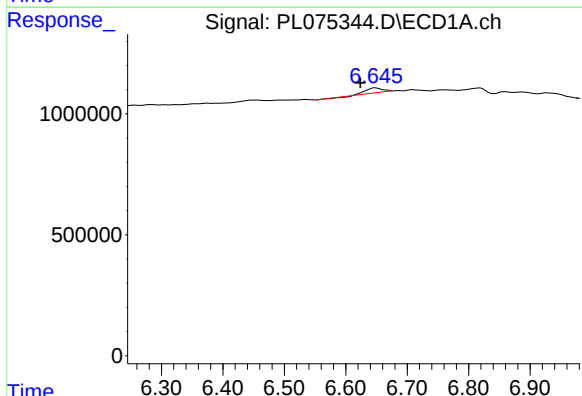


#3 gamma-BHC (Lindane)

R.T.: 6.648 min
Delta R.T.: 0.024 min
Response: 395342
Conc: 0.51 ng/ml

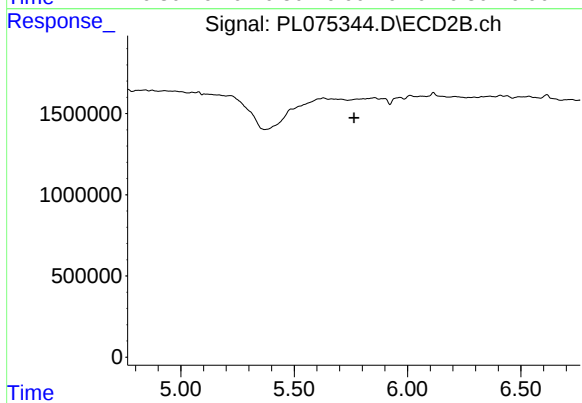

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 5.765 min
Response: 0
Conc: N.D.

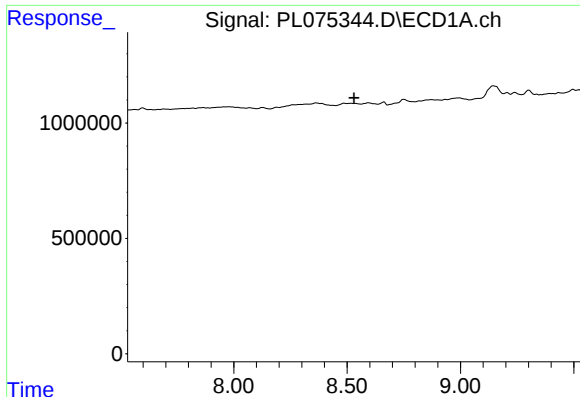

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 8.530 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

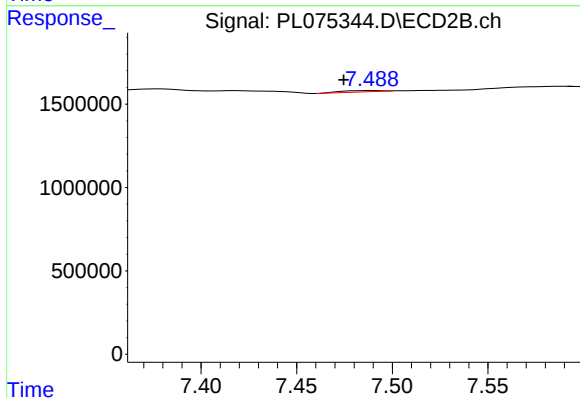


#9 Endosulfan I

R.T.: 7.489 min
Delta R.T.: 0.015 min
Response: 112742
Conc: 0.07 ng/ml

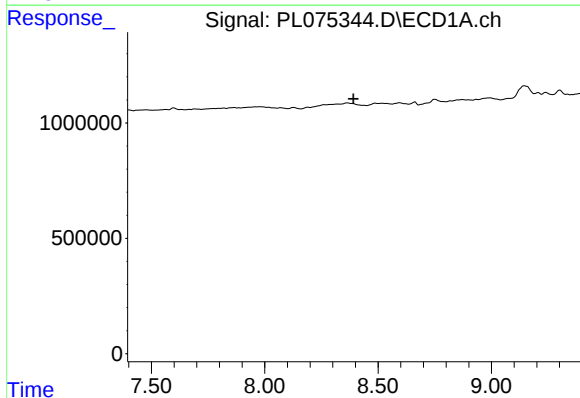


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 8.392 min
Response: 0
Conc: N.D.

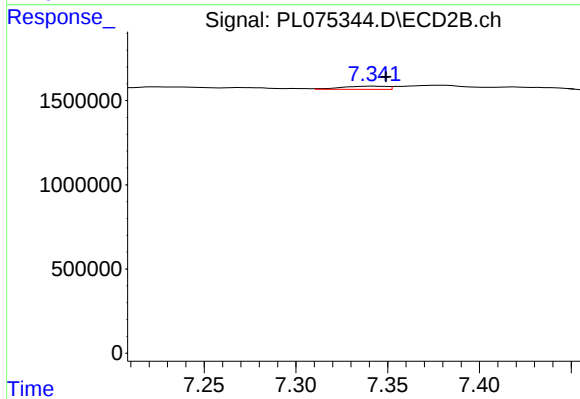

#10 gamma-Chlordane


R.T.: 7.343 min
Delta R.T.: -0.006 min
Response: 311562
Conc: 0.17 ng/ml

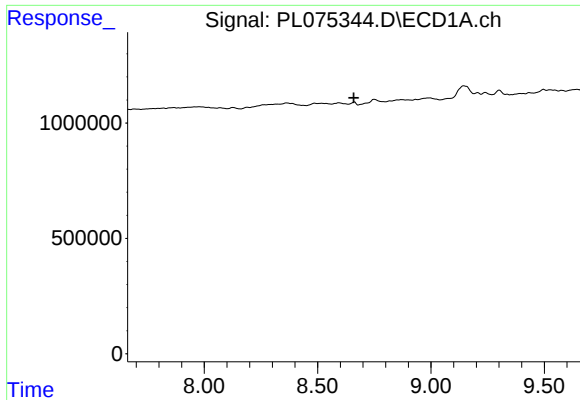

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 8.660 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

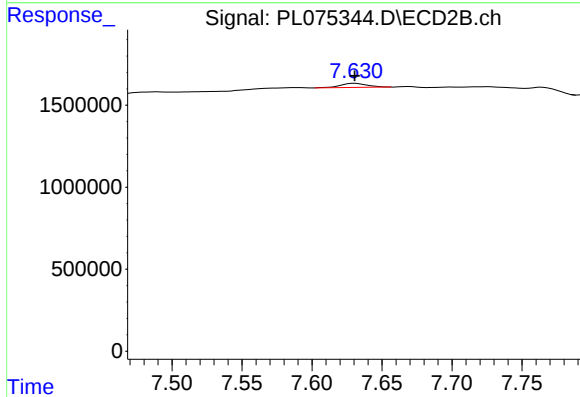


#12 4,4'-DDE

R.T.: 7.631 min
Delta R.T.: 0.000 min
Response: 328619
Conc: 0.20 ng/ml

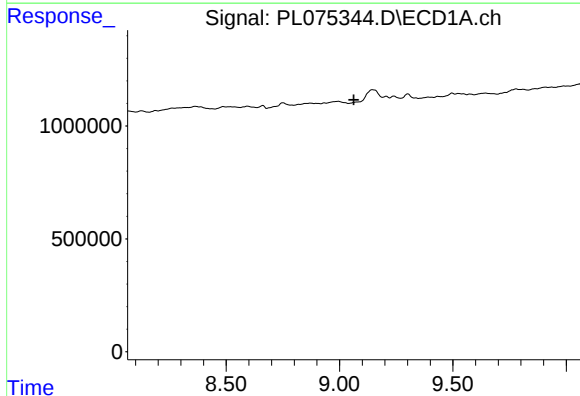


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 9.062 min
Response: 0
Conc: N.D.

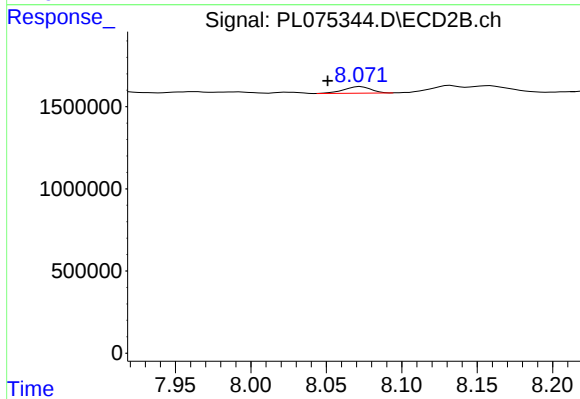

#14 Endrin


R.T.: 8.073 min
Delta R.T.: 0.022 min
Response: 493460
Conc: 0.32 ng/ml

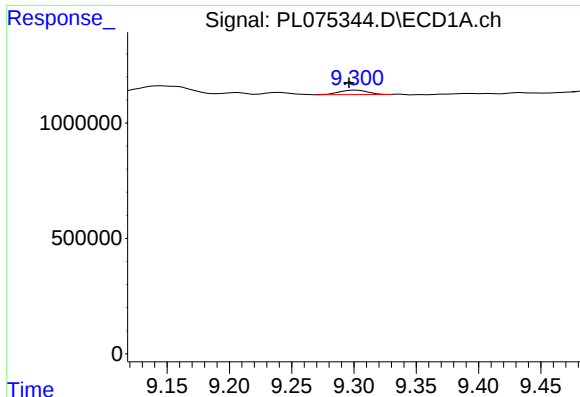

#15 Endosulfan II


R.T.: 9.302 min
Delta R.T.: 0.006 min
Response: 311988
Conc: 0.55 ng/ml

Instrument :
ECD_L
ClientSampleId :

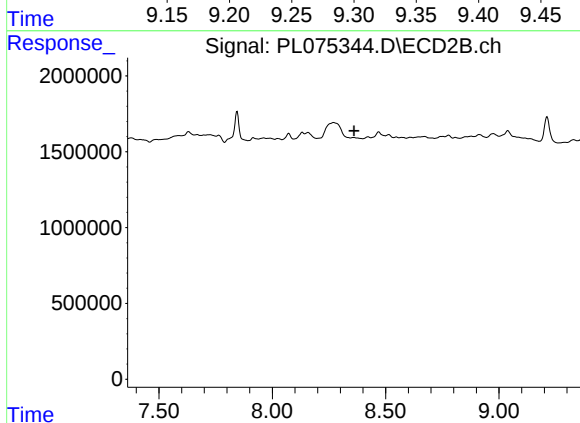


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.361 min
Response: 0
Conc: N.D.

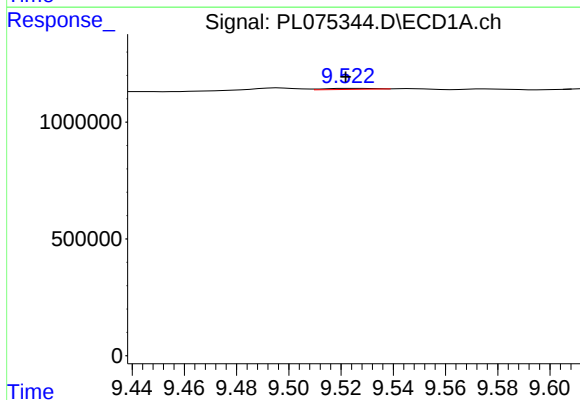


#17 4,4'-DDT

R.T.: 9.524 min
Delta R.T.: 0.002 min
Response: 52082
Conc: 0.09 ng/ml

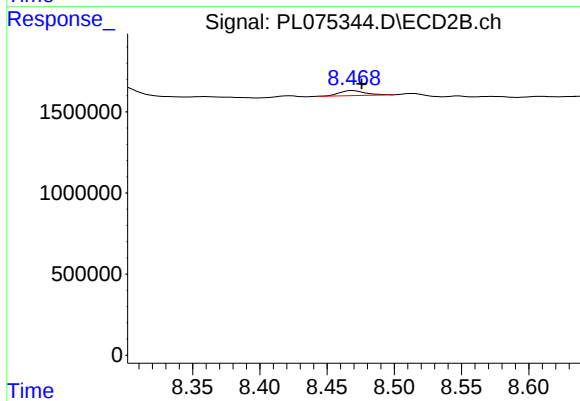

#17 4,4'-DDT


R.T.: 8.470 min
Delta R.T.: -0.006 min
Response: 418073
Conc: 0.29 ng/ml

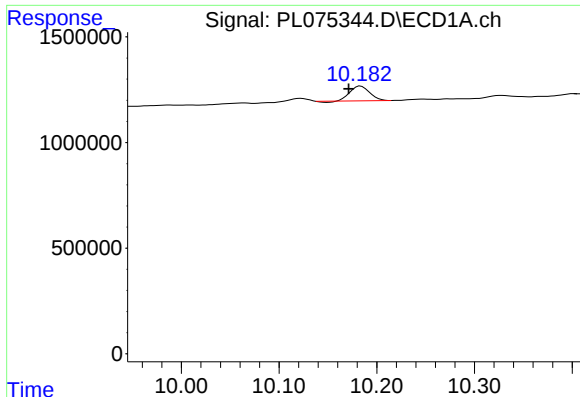

#21 Endrin ketone


R.T.: 10.184 min
Delta R.T.: 0.012 min
Response: 952469
Conc: 1.55 ng/ml

Instrument :
ECD_L
ClientSampleId :

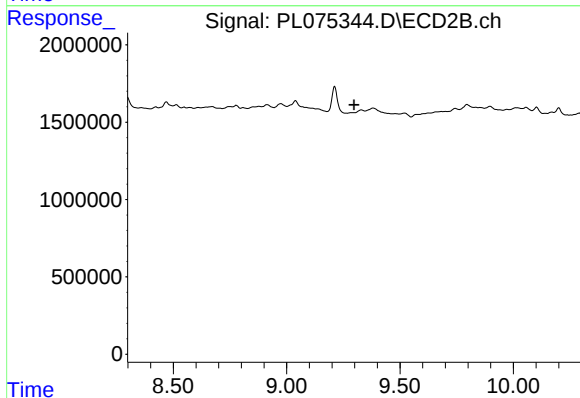


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.298 min
Response: 0
Conc: N.D.

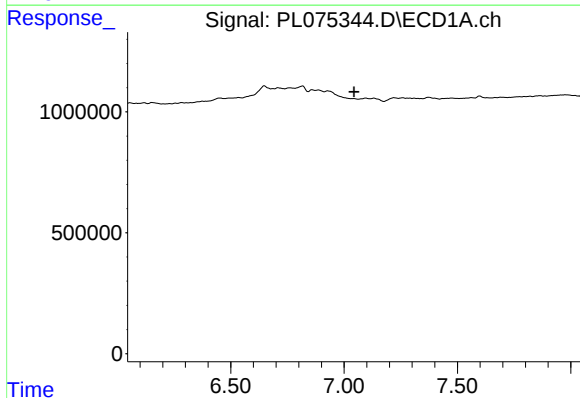


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 7.044 min
Response: 0
Conc: N.D.

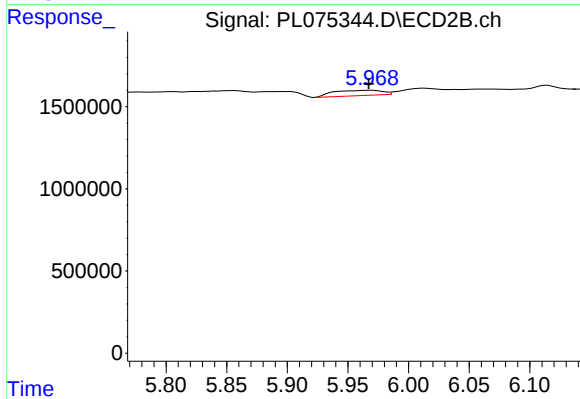

#23 Chlordane-1


R.T.: 5.969 min
Delta R.T.: 0.001 min
Response: 912755
Conc: 16.39 ng/ml

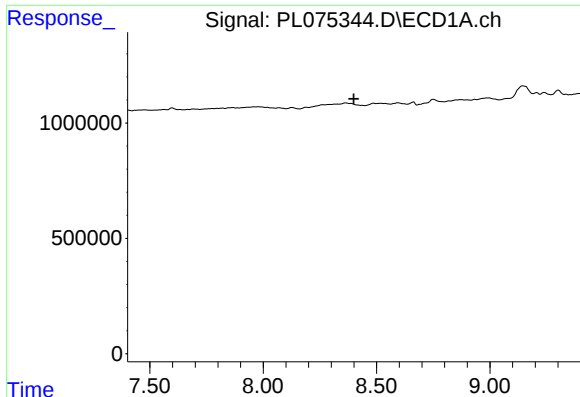

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 8.399 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

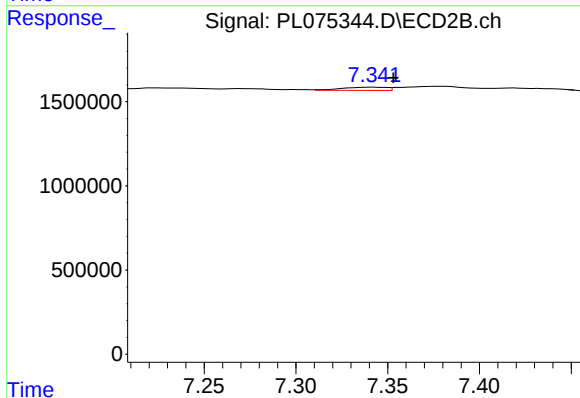


#25 Chlordane-3

R.T.: 7.343 min
Delta R.T.: -0.010 min
Response: 311562
Conc: 1.77 ng/ml

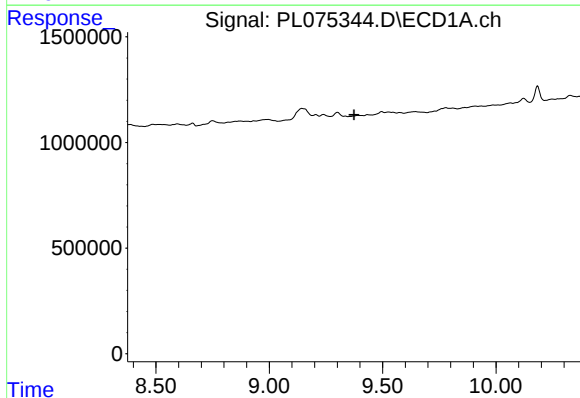


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 9.375 min
Response: 0
Conc: N.D.

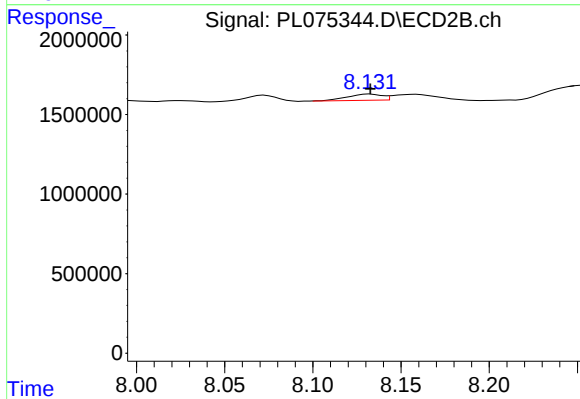

#27 Chlordane-5


R.T.: 8.132 min
Delta R.T.: 0.000 min
Response: 533114
Conc: 10.68 ng/ml

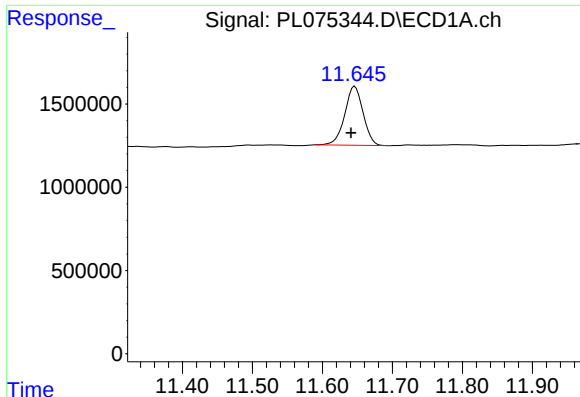

#28 Decachlorobiphenyl

R.T.: 11.646 min
Delta R.T.: 0.005 min
Response: 6452128
Conc: 12.03 ng/ml

Instrument :
ECD_L
ClientSampleId :

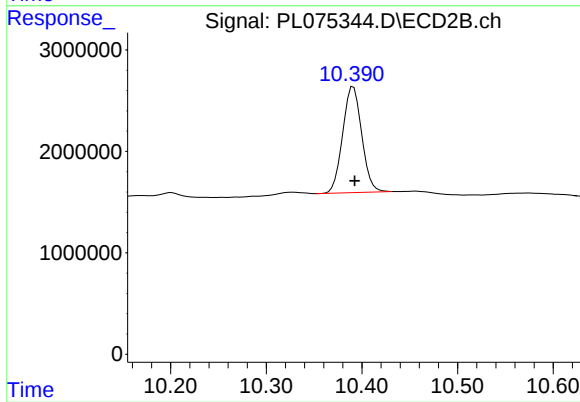

#28 Decachlorobiphenyl

R.T.: 10.391 min
Delta R.T.: -0.001 min
Response: 14523954
Conc: 10.58 ng/ml