

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060122\
 Data File : PL075364.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Jun 2022 19:27
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 02 09:21:39 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 01 10:19:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.643	4.641	12369716	33595295	21.046	21.207
28)	SA Decachlor...	11.639	10.388	10764974	26892393	20.077	19.597
Target Compounds							
7)	B delta-BHC	0.000	6.412	0	497563	N.D.	0.232 #
11)	B alpha-Chl...	0.000	7.396f	0	315617	N.D.	0.173 #
13)	MA Dieldrin	0.000	7.747	0	306826	N.D.	0.177 #
14)	MA Endrin	0.000	8.071f	0	69022	N.D.	0.044 #
15)	B Endosulfa...	9.303	0.000	325188	0	0.576	N.D. #
17)	MA 4,4'-DDT	9.495f	0.000	95042	0	0.163	N.D. #
18)	B Endrin al...	0.000	8.574f	0	486920	N.D.	0.404 #
21)	B Endrin ke...	10.186f	0.000	340170	0	0.554	N.D. #
26)	Chlordane-4	0.000	7.396f	0	315617	N.D.	1.671 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060122\
Data File : PL075364.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Jun 2022 19:27
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 02 09:21:39 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
Quant Title : GC Extractables
QLast Update : Wed Jun 01 10:19:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

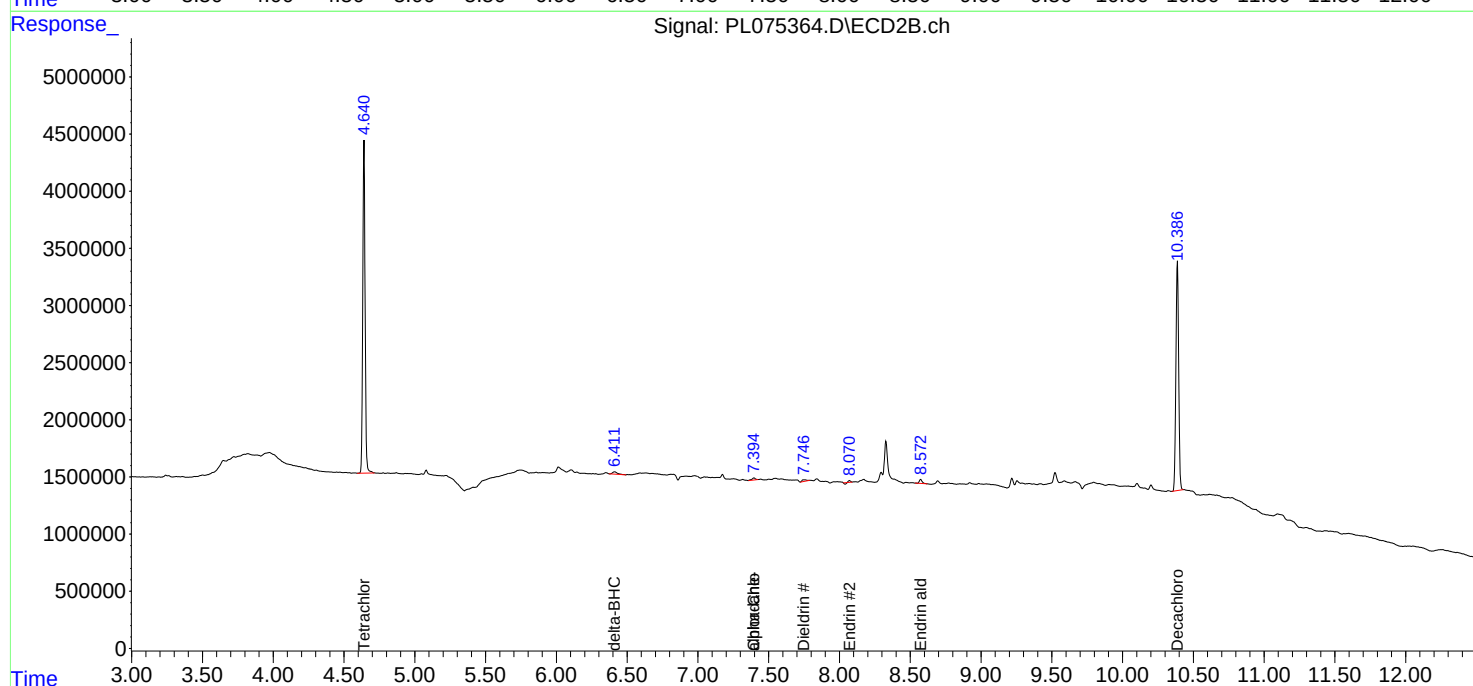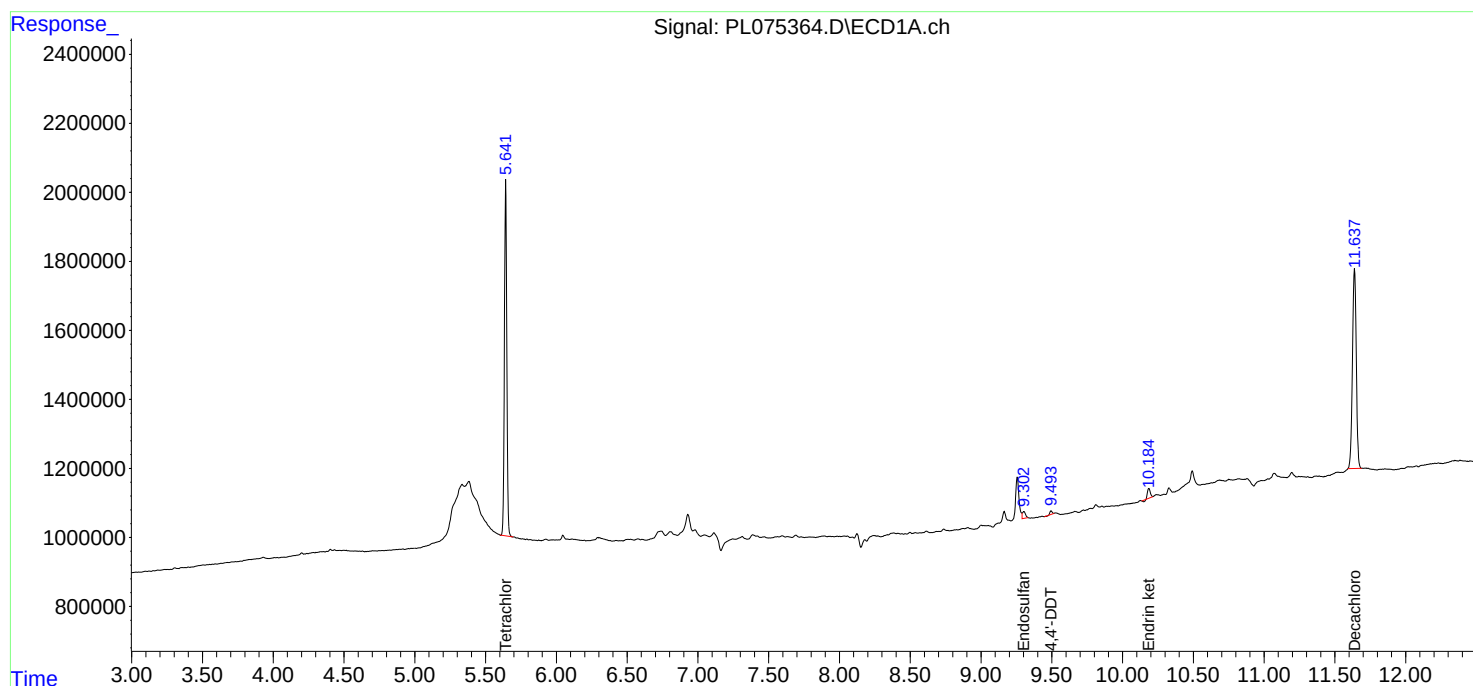


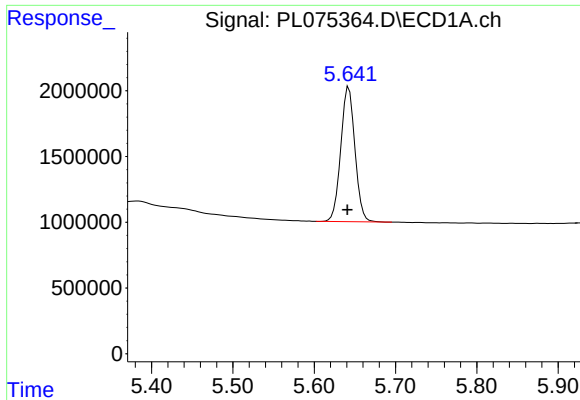

#1 Tetrachloro-m-xylene


R.T.: 5.643 min
Delta R.T.: 0.002 min
Response: 12369716
Conc: 21.05 ng/ml

Instrument :
ECD_L
ClientSampleId :

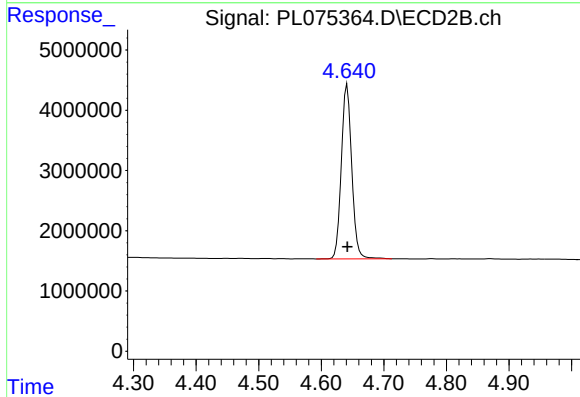


#1 Tetrachloro-m-xylene

R.T.: 4.641 min
Delta R.T.: 0.000 min
Response: 33595295
Conc: 21.21 ng/ml

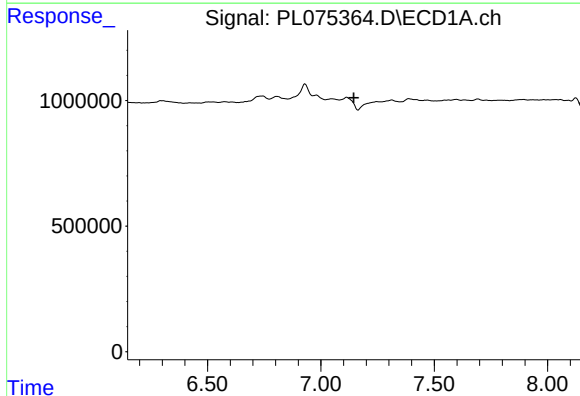


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 7.146 min
Response: 0
Conc: N.D.

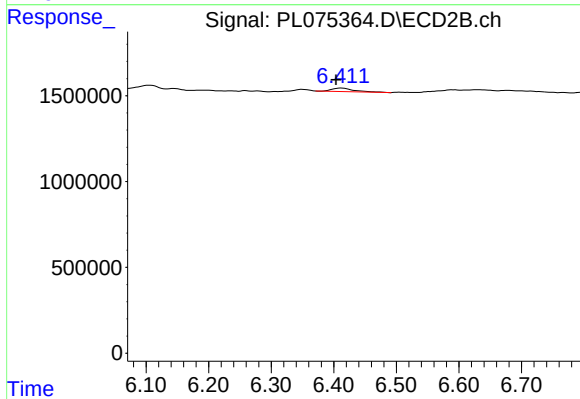

#7 delta-BHC


R.T.: 6.412 min
Delta R.T.: 0.009 min
Response: 497563
Conc: 0.23 ng/ml

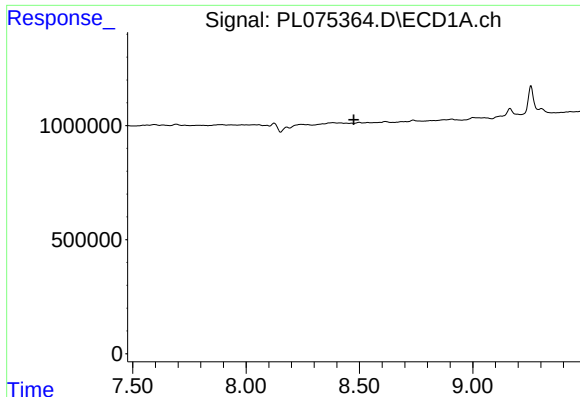

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 8.474 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

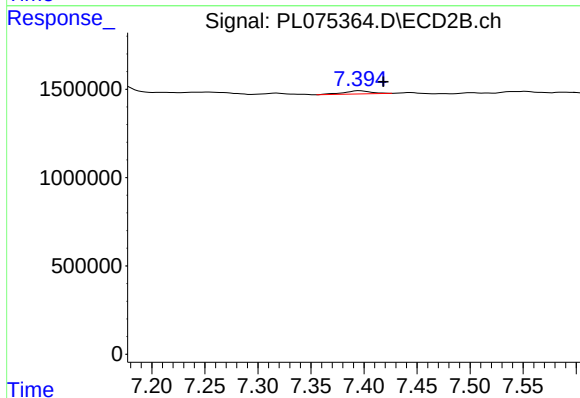


#11 alpha-Chlordane

R.T.: 7.396 min
Delta R.T.: -0.022 min
Response: 315617
Conc: 0.17 ng/ml

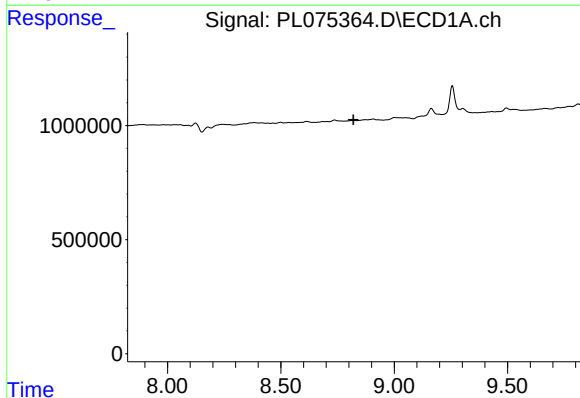


#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 8.821 min
Response: 0
Conc: N.D.

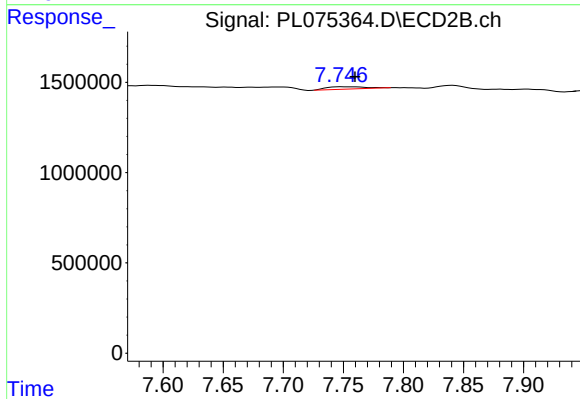

#13 Dieldrin


R.T.: 7.747 min
Delta R.T.: -0.012 min
Response: 306826
Conc: 0.18 ng/ml

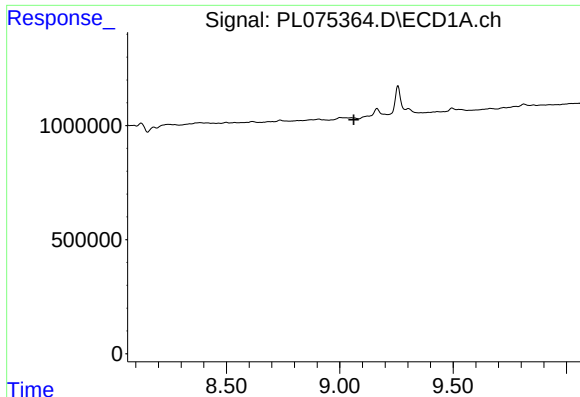

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 9.062 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

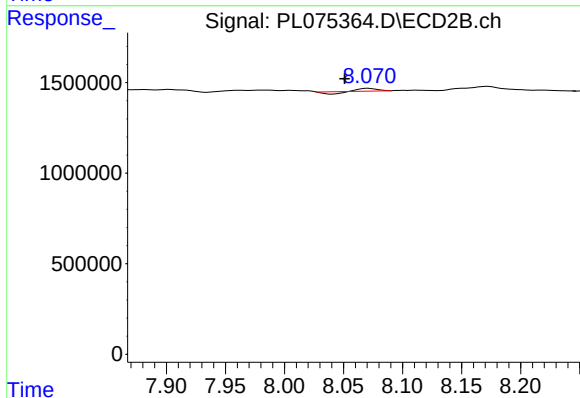


#14 Endrin

R.T.: 8.071 min
Delta R.T.: 0.020 min
Response: 69022
Conc: 0.04 ng/ml

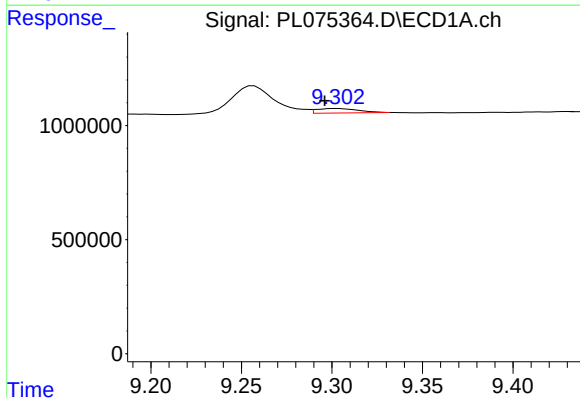


#15 Endosulfan II

R.T.: 9.303 min
Delta R.T.: 0.007 min
Response: 325188
Conc: 0.58 ng/ml

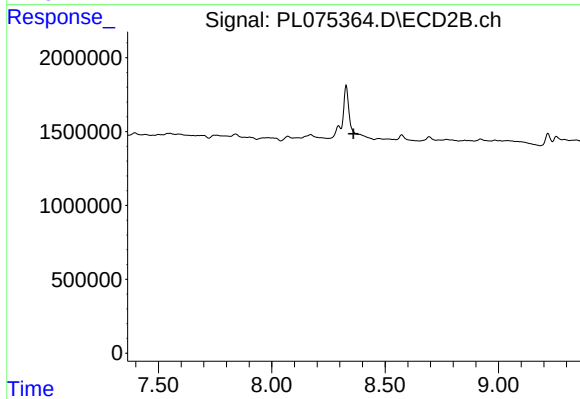

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.361 min
Response: 0
Conc: N.D.

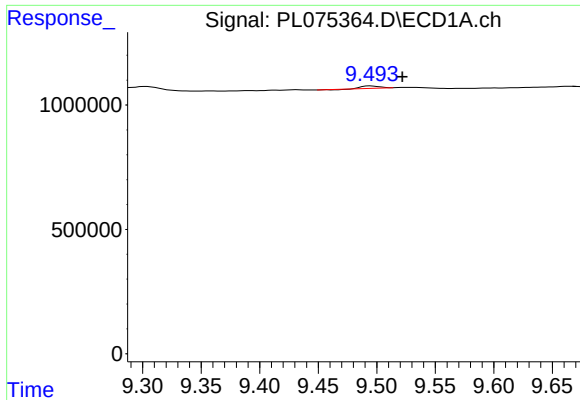

#17 4,4'-DDT


R.T.: 9.495 min
Delta R.T.: -0.027 min
Response: 95042
Conc: 0.16 ng/ml

Instrument :
ECD_L
ClientSampleId :

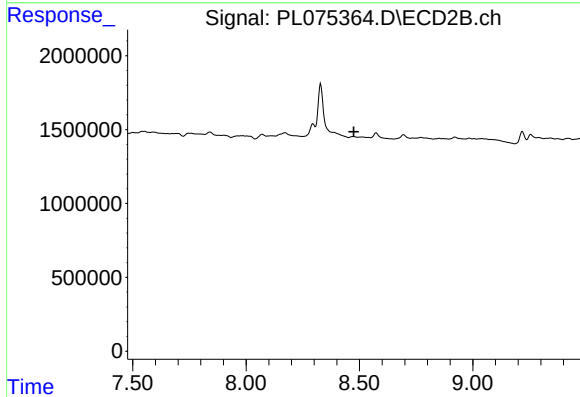


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 8.476 min
Response: 0
Conc: N.D.

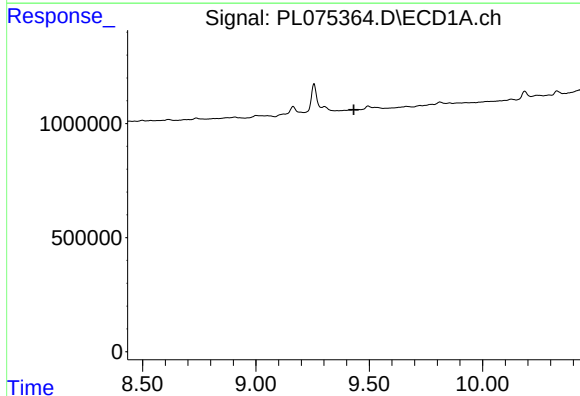


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 9.431 min
Response: 0
Conc: N.D.

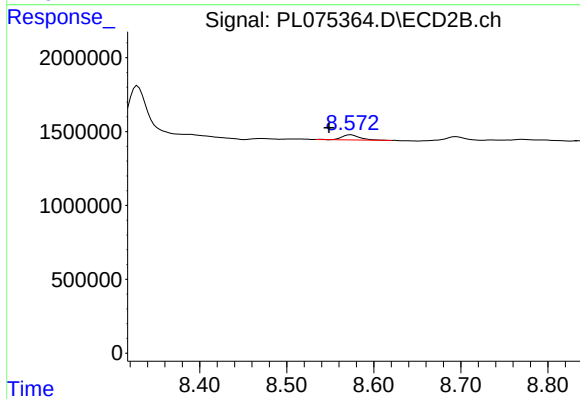

#18 Endrin aldehyde


R.T.: 8.574 min
Delta R.T.: 0.025 min
Response: 486920
Conc: 0.40 ng/ml

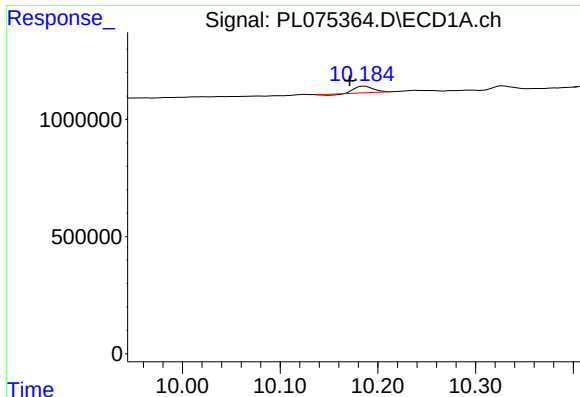

#21 Endrin ketone


R.T.: 10.186 min
Delta R.T.: 0.015 min
Response: 340170
Conc: 0.55 ng/ml

Instrument :
ECD_L
ClientSampleId :

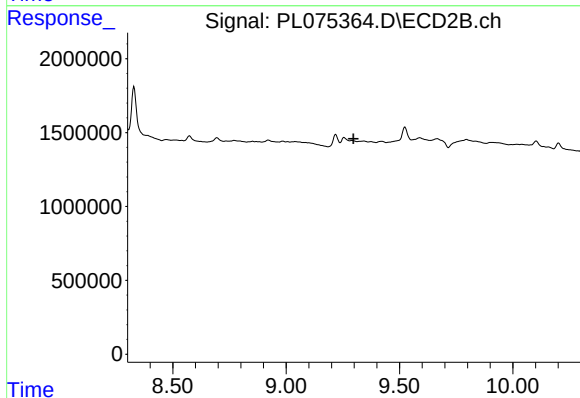


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.298 min
Response: 0
Conc: N.D.

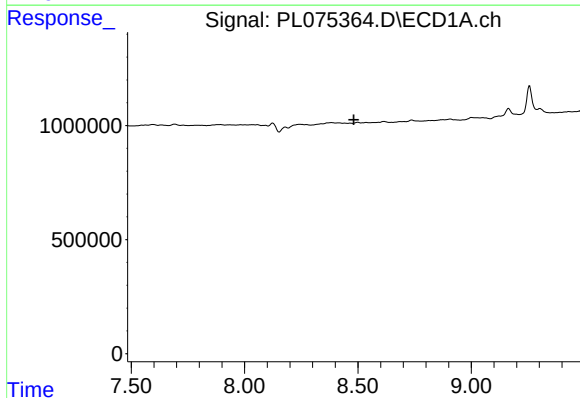


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 8.482 min
Response: 0
Conc: N.D.

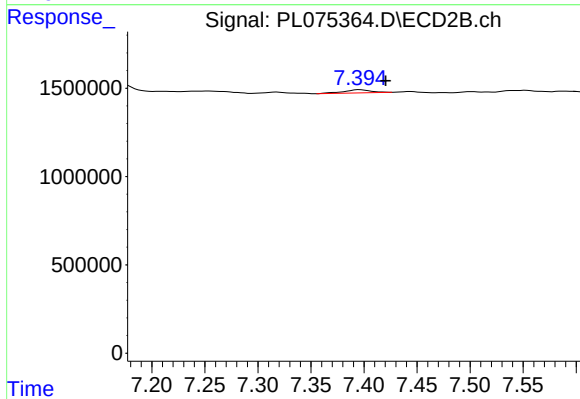

#26 Chlordane-4


R.T.: 7.396 min
Delta R.T.: -0.025 min
Response: 315617
Conc: 1.67 ng/ml

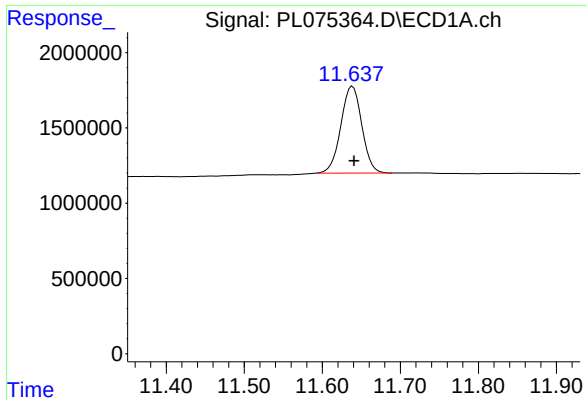

#28 Decachlorobiphenyl

R.T.: 11.639 min
Delta R.T.: -0.002 min
Response: 10764974
Conc: 20.08 ng/ml

Instrument :
ECD_L
ClientSampleId :

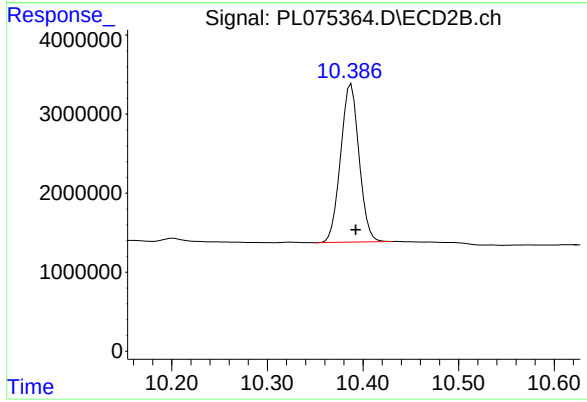

#28 Decachlorobiphenyl

R.T.: 10.388 min
Delta R.T.: -0.005 min
Response: 26892393
Conc: 19.60 ng/ml