

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060123\
 Data File : PL083147.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Jun 2023 14:57
 Operator : AR\AJ
 Sample : 02983-06
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SB24B

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 06/02/2023
 Supervised By : Ankita Jodhani 06/02/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 01 21:08:16 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051923.M
 Quant Title : GC Extractables
 QLast Update : Sat May 20 04:58:53 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.316	2.635	52101601	45678972	17.728	17.595
2)	SA Decachlor...	8.735	7.741	30170923	31141580	14.385	12.524
Target Compounds							
12)	B 4,4'-DDE	5.946	5.066	887659	904069	0.322	0.372m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060123\
Data File : PL083147.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Jun 2023 14:57
Operator : AR\AJ
Sample : 02983-06
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SB24B


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 06/02/2023
Supervised By : Ankita Jodhani 06/02/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 01 21:08:16 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051923.M
Quant Title : GC Extractables
QLast Update : Sat May 20 04:58:53 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

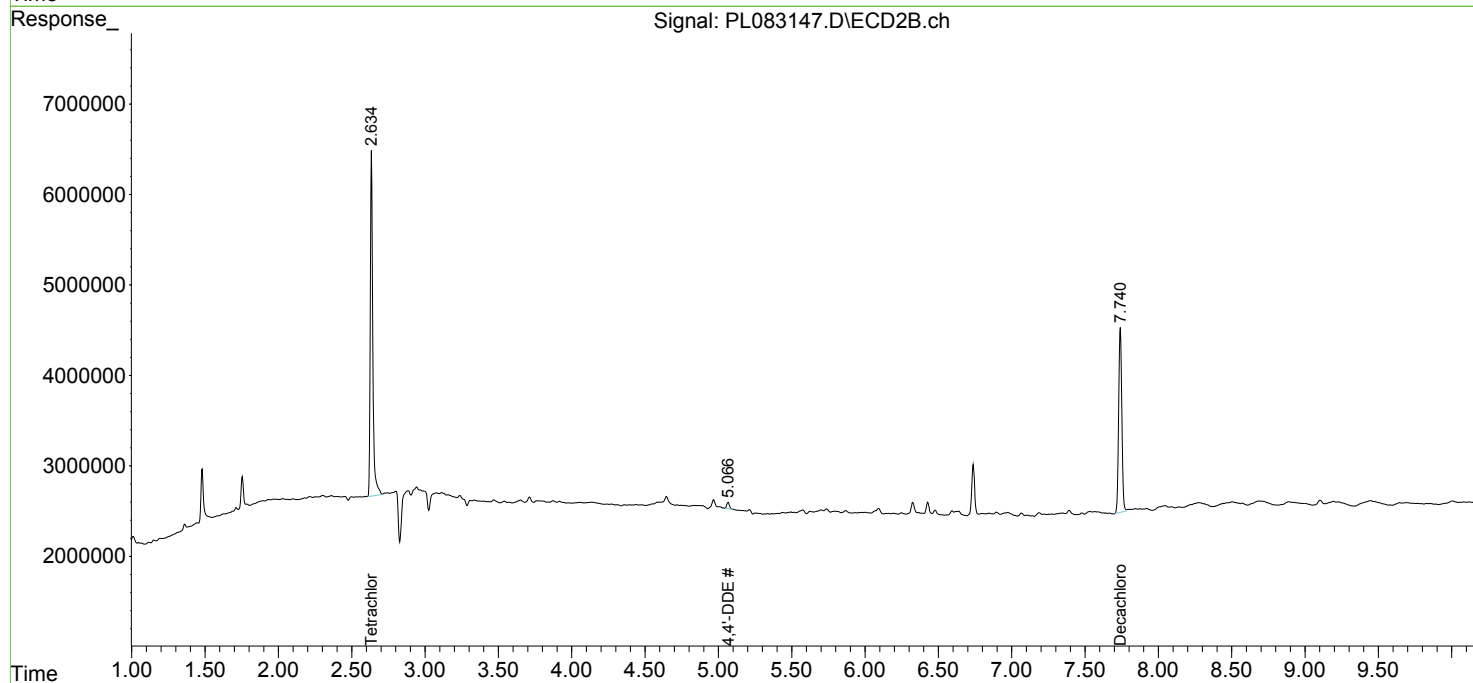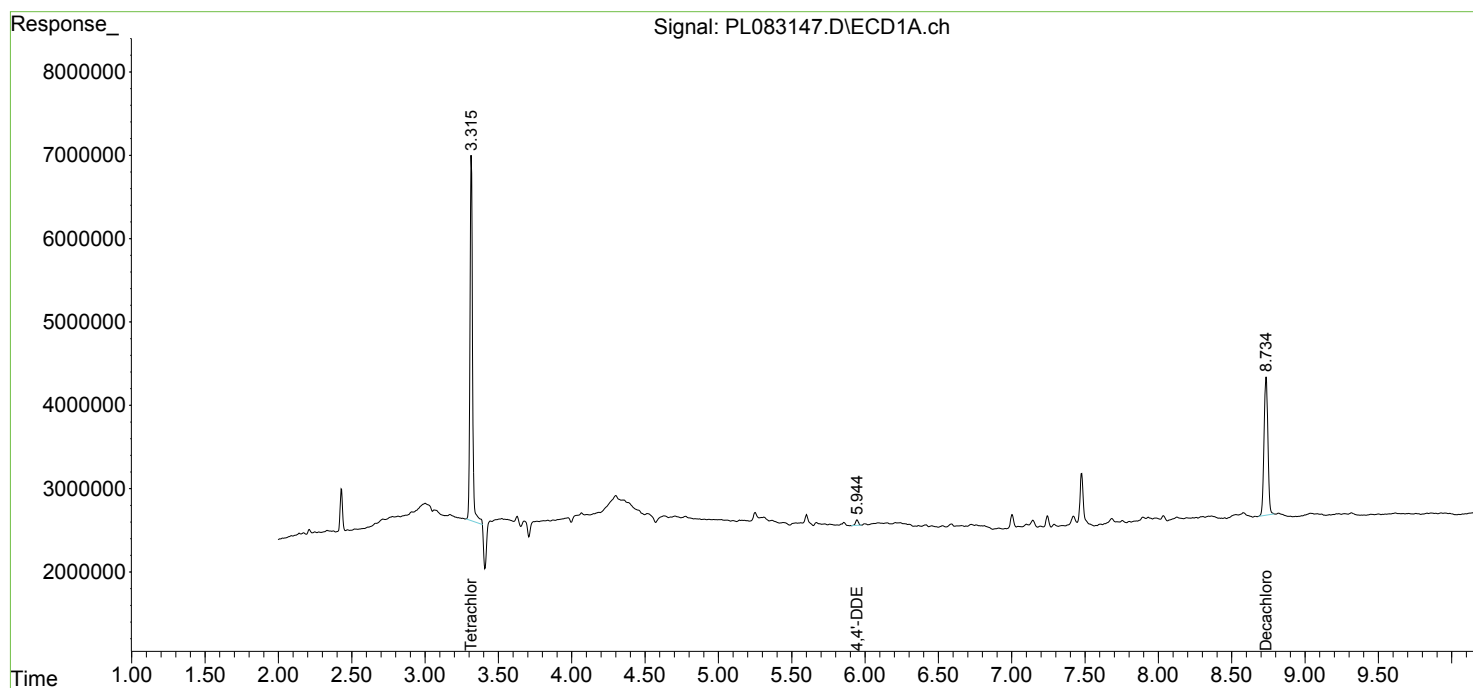

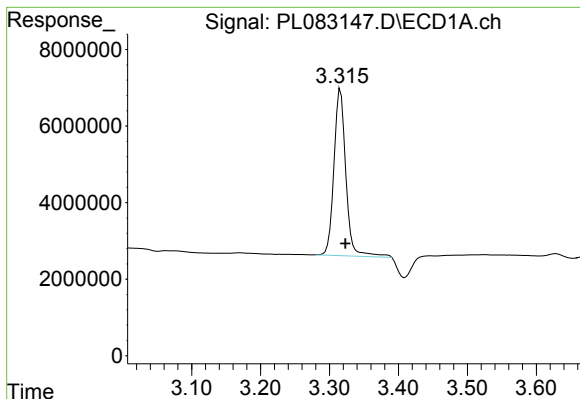


#1 Tetrachloro-m-xylene

R.T.: 3.316 min
Delta R.T.: -0.007 min
Response: 52101601
Conc: 17.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB24B


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/02/2023
Supervised By :Ankita Jodhani 06/02/2023

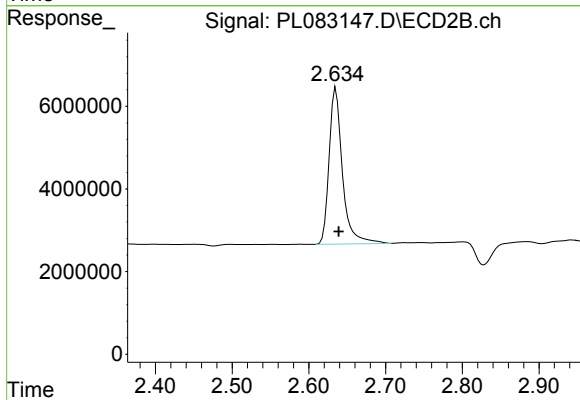


#1 Tetrachloro-m-xylene

R.T.: 2.635 min
Delta R.T.: -0.004 min
Response: 45678972
Conc: 17.60 ng/ml

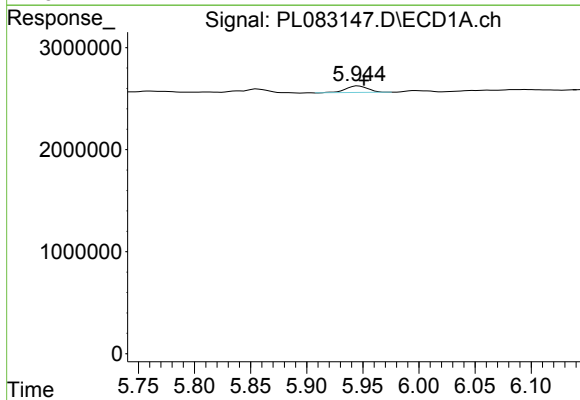


#12 4,4'-DDE

R.T.: 5.946 min
Delta R.T.: -0.005 min
Response: 887659
Conc: 0.32 ng/ml

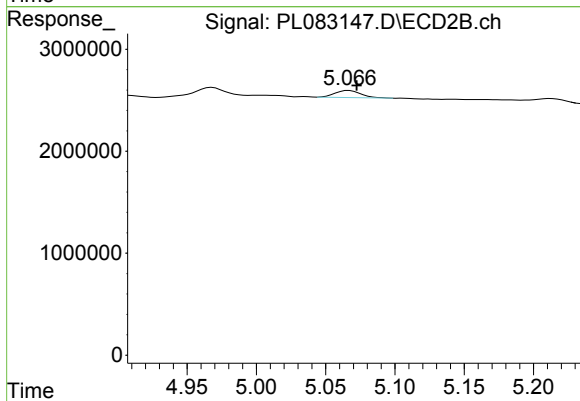

#12 4,4'-DDE

R.T.: 5.066 min
Delta R.T.: -0.007 min
Response: 904069
Conc: 0.37 ng/ml m

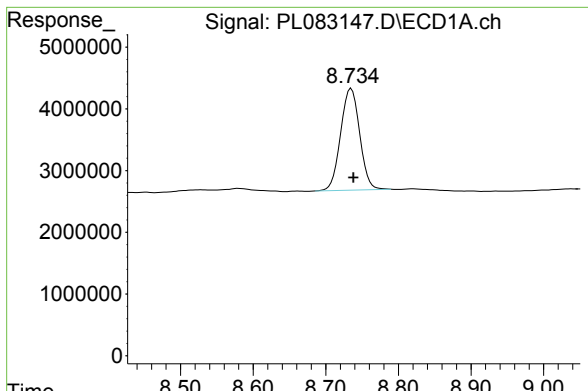


#28 Decachlorobiphenyl

R.T.: 8.735 min
Delta R.T.: -0.003 min
Response: 30170923
Conc: 14.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB24B

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/02/2023
Supervised By :Ankita Jodhani 06/02/2023

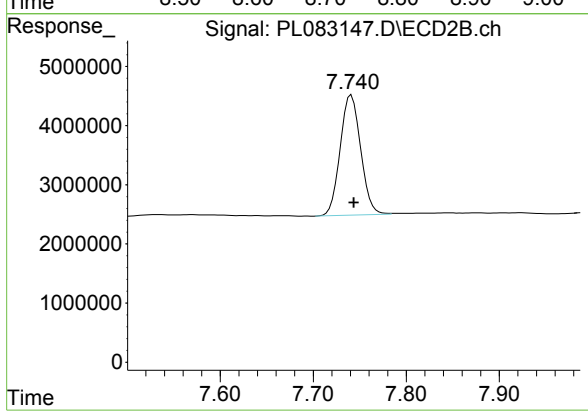

#28 Decachlorobiphenyl

R.T.: 7.741 min
Delta R.T.: -0.003 min
Response: 31141580
Conc: 12.52 ng/ml