

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060220\
 Data File : PL059061.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jun 2020 16:11
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 02 17:30:06 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052020.M
 Quant Title : GC Extractables
 QLast Update : Wed May 20 11:27:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.528	4.076	38595346	54130197	21.049	19.986
28)	SA Decachlor...	8.307	9.190	32819125	44552677	19.425	16.900
Target Compounds							
4)	MA Heptachlor	0.000	5.263	0	8058468	N.D.	2.104 #
8)	B Heptachlo...	0.000	5.952	0	2943647	N.D.	0.892 #
9)	A Endosulfan I	0.000	6.314	0	1899844	N.D.	0.646 #
10)	B gamma-Chl...	0.000	6.206	0	1320129	N.D.	0.399 #
15)	B Endosulfa...	0.000	7.012	0	1653015	N.D.	0.590 #
17)	MA 4,4'-DDT	0.000	7.232	0	16445	N.D.	0.007 #
20)	A Methoxychlor	0.000	7.657f	0	10968678	N.D.	7.865 #
25)	Chlordane-3	0.000	6.206	0	1320129	N.D.	3.468 #
27)	Chlordane-5	0.000	7.079	0	292157	N.D.	3.688 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060220\
Data File : PL059061.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jun 2020 16:11
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 02 17:30:06 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052020.M
Quant Title : GC Extractables
QLast Update : Wed May 20 11:27:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

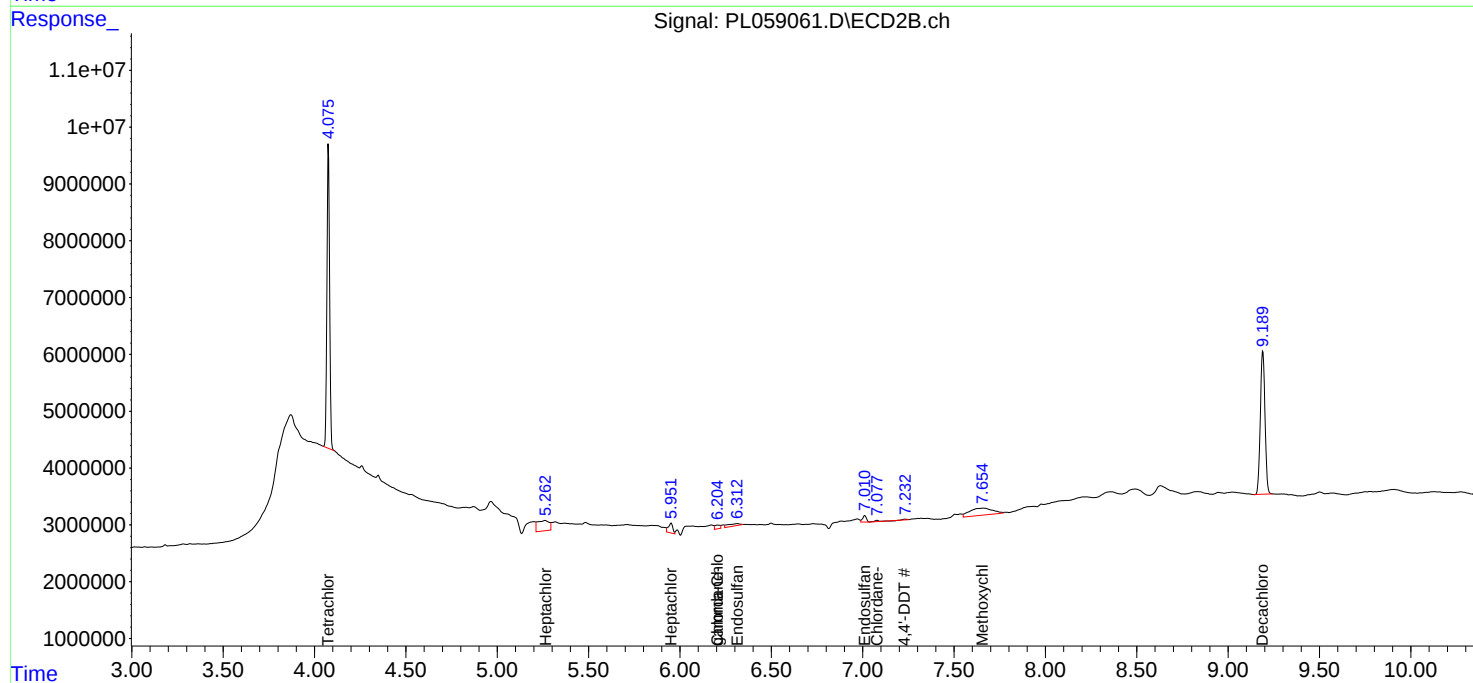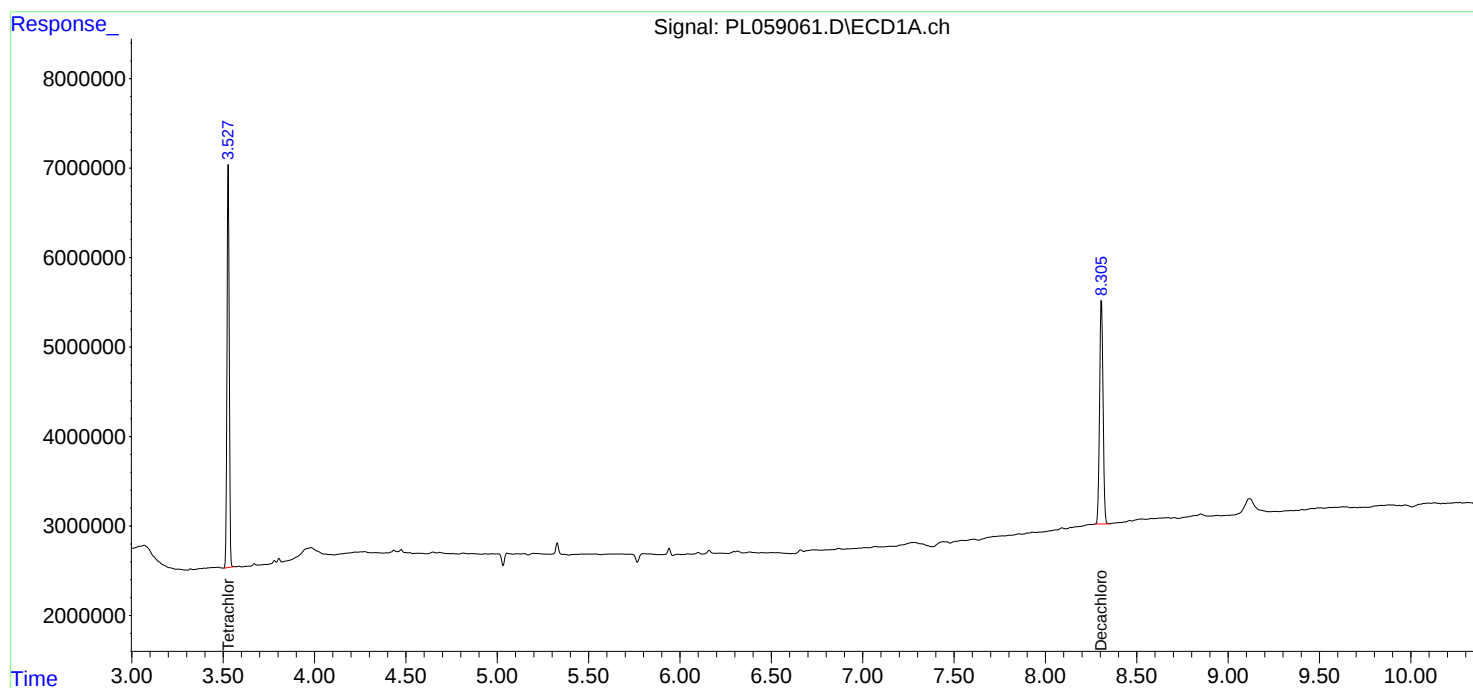


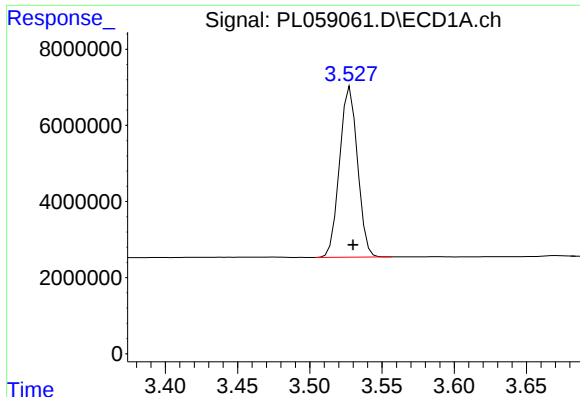

#1 Tetrachloro-m-xylene


R.T.: 3.528 min
Delta R.T.: -0.002 min
Response: 38595346
Conc: 21.05 ng/ml

Instrument :
ECD_L
ClientSampleId :

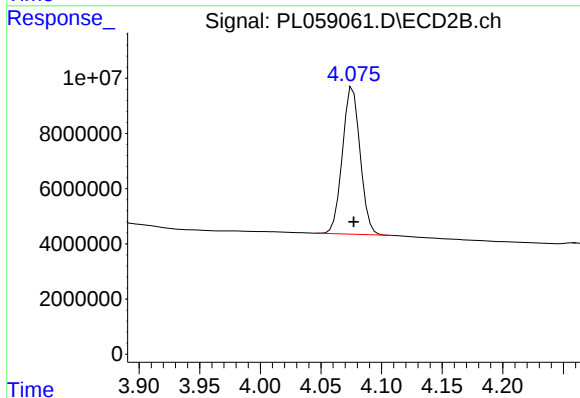


#1 Tetrachloro-m-xylene

R.T.: 4.076 min
Delta R.T.: 0.000 min
Response: 54130197
Conc: 19.99 ng/ml

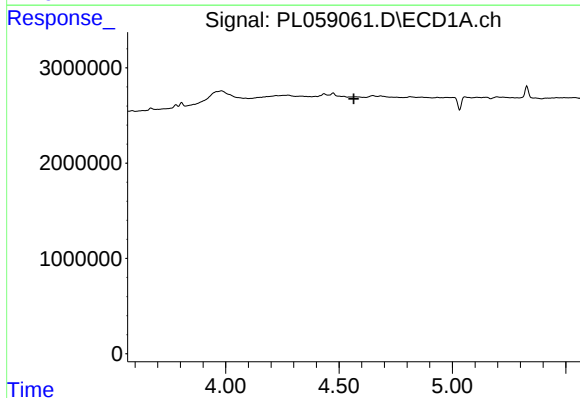


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.566 min
Response: 0
Conc: N.D.

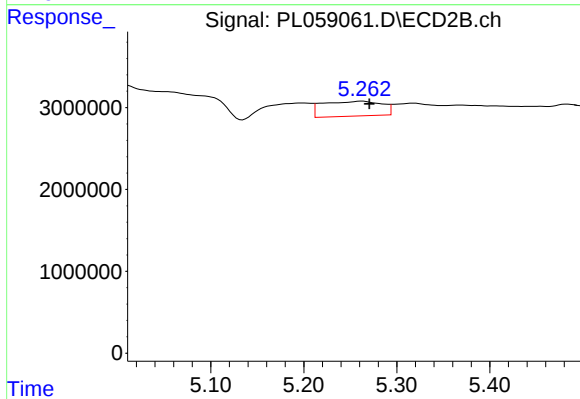

#4 Heptachlor


R.T.: 5.263 min
Delta R.T.: -0.008 min
Response: 8058468
Conc: 2.10 ng/ml

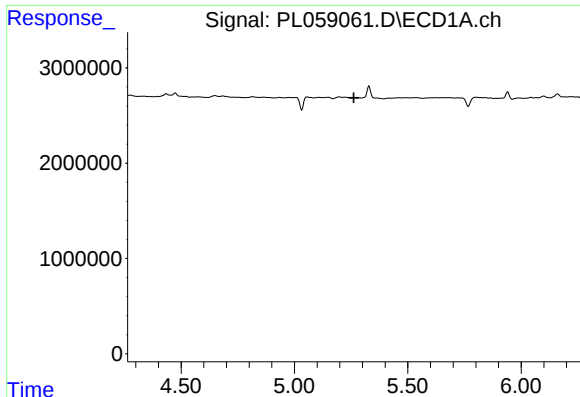

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.261 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

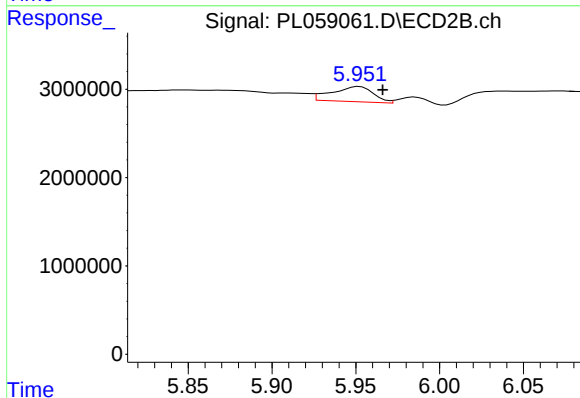


#8 Heptachlor epoxide

R.T.: 5.952 min
Delta R.T.: -0.014 min
Response: 2943647
Conc: 0.89 ng/ml

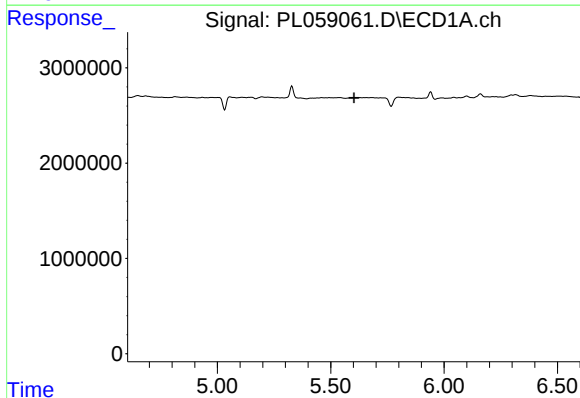


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.603 min
Response: 0
Conc: N.D.

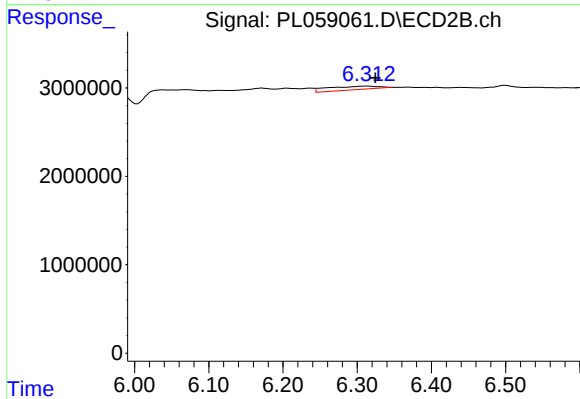

#9 Endosulfan I


R.T.: 6.314 min
Delta R.T.: -0.011 min
Response: 1899844
Conc: 0.65 ng/ml

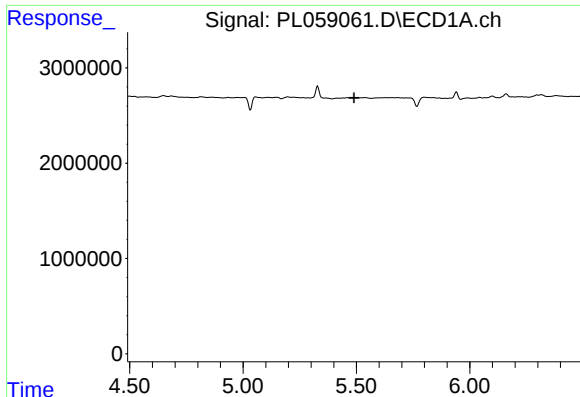

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.490 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

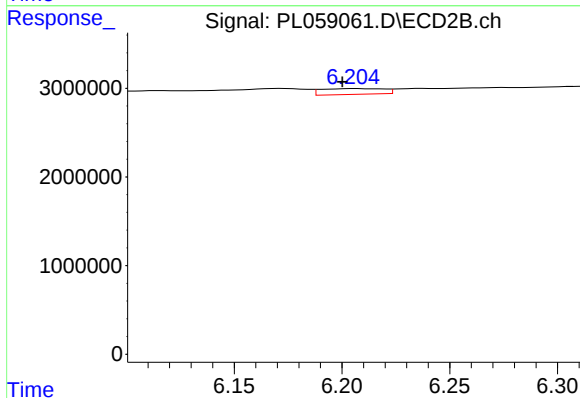


#10 gamma-Chlordane

R.T.: 6.206 min
Delta R.T.: 0.005 min
Response: 1320129
Conc: 0.40 ng/ml

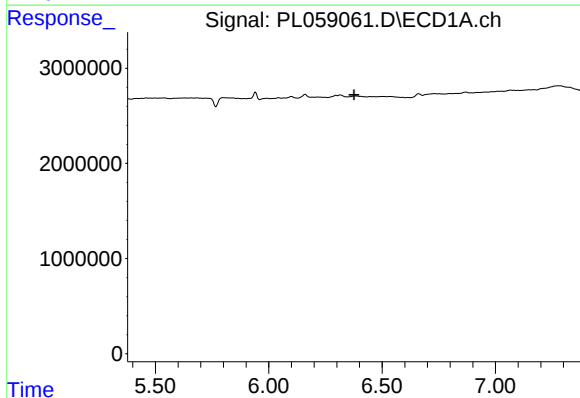


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.377 min
Response: 0
Conc: N.D.

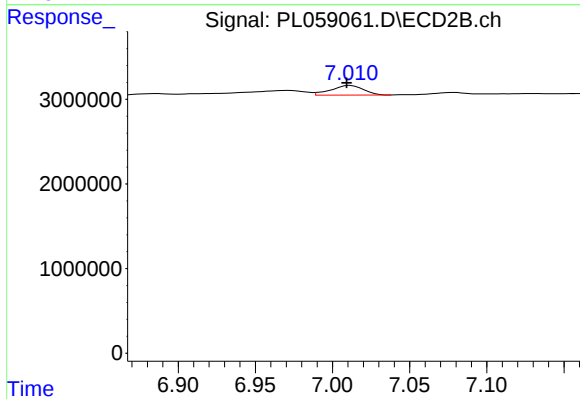

#15 Endosulfan II


R.T.: 7.012 min
Delta R.T.: 0.003 min
Response: 1653015
Conc: 0.59 ng/ml

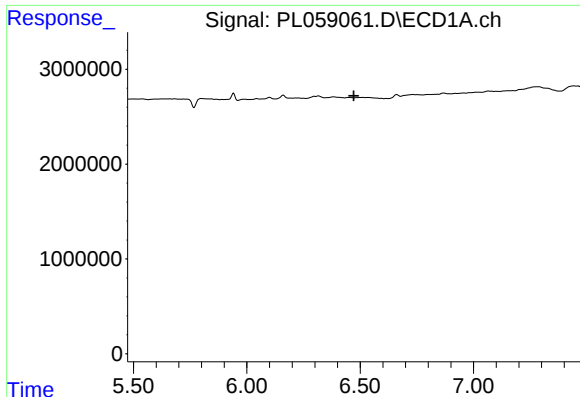

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.471 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

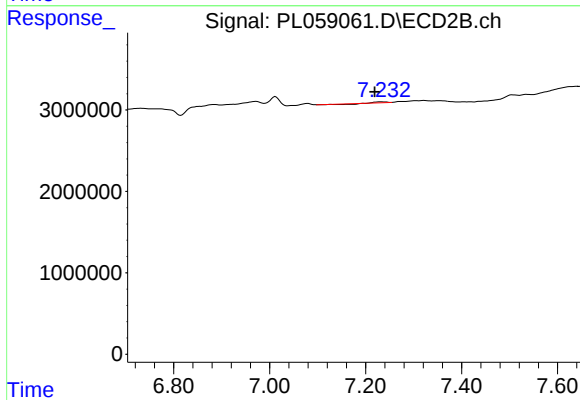


#17 4,4'-DDT

R.T.: 7.232 min
Delta R.T.: 0.013 min
Response: 16445
Conc: 0.01 ng/ml

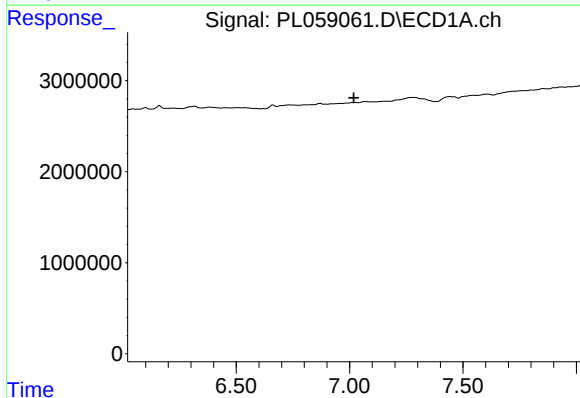


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 7.018 min
Response: 0
Conc: N.D.

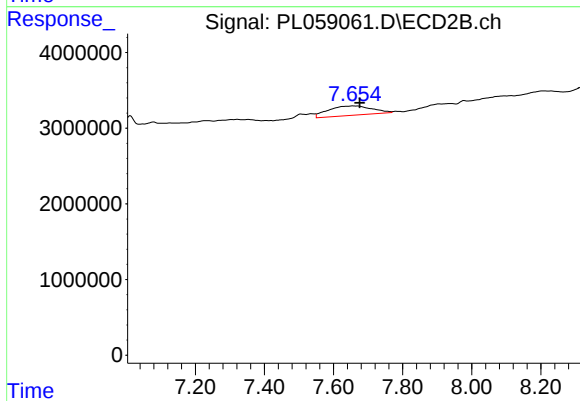

#20 Methoxychlor


R.T.: 7.657 min
Delta R.T.: -0.019 min
Response: 10968678
Conc: 7.86 ng/ml

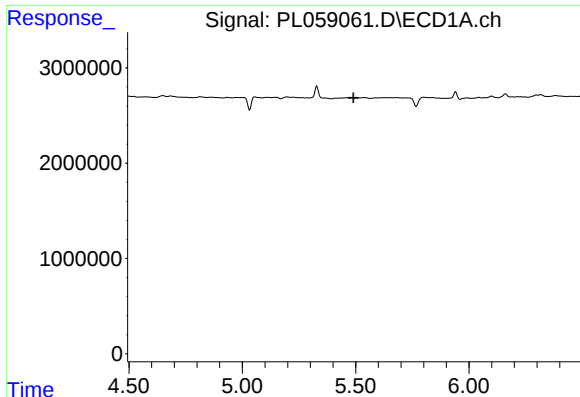

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.491 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

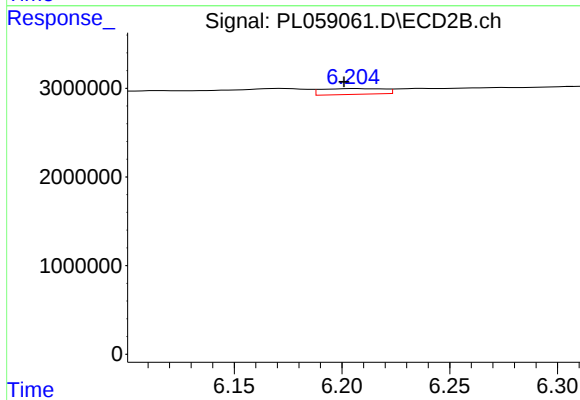


#25 Chlordane-3

R.T.: 6.206 min
Delta R.T.: 0.005 min
Response: 1320129
Conc: 3.47 ng/ml

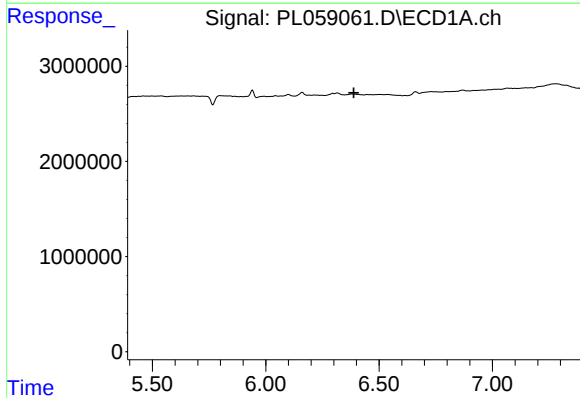


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.389 min
Response: 0
Conc: N.D.

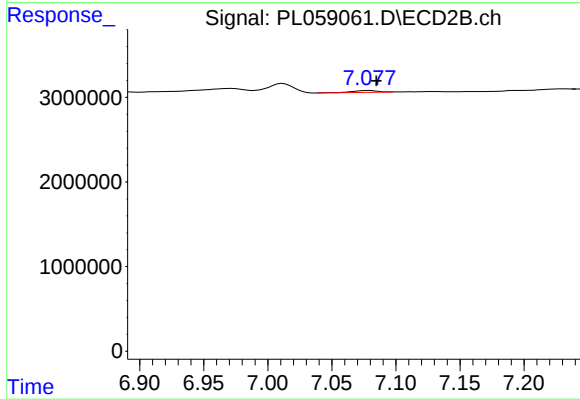

#27 Chlordane-5


R.T.: 7.079 min
Delta R.T.: -0.005 min
Response: 292157
Conc: 3.69 ng/ml

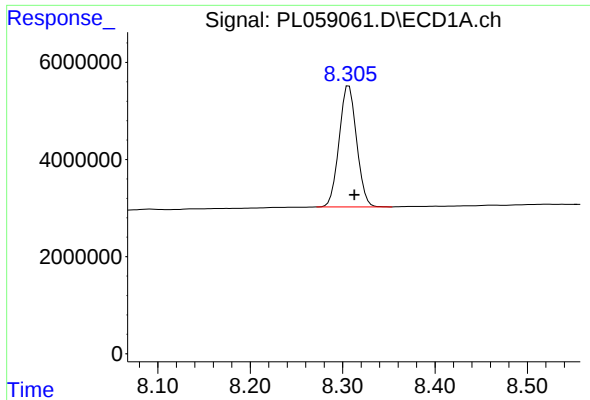

#28 Decachlorobiphenyl

R.T.: 8.307 min
Delta R.T.: -0.006 min
Response: 32819125
Conc: 19.42 ng/ml

Instrument :
ECD_L
ClientSampleId :

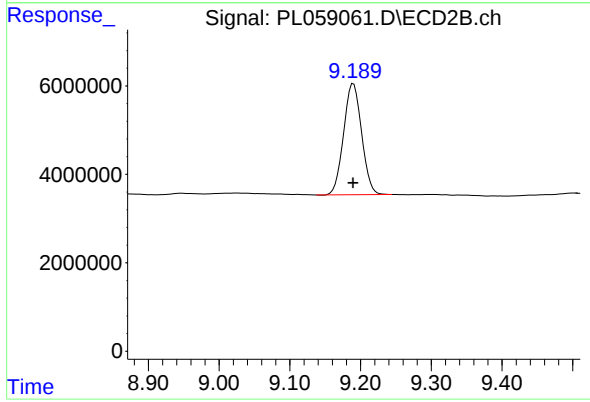

#28 Decachlorobiphenyl

R.T.: 9.190 min
Delta R.T.: 0.000 min
Response: 44552677
Conc: 16.90 ng/ml