

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060220\
 Data File : PL059053.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jun 2020 12:31
 Operator : AJ\MA
 Sample : L2822-02 5X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 C0AP7

Manual Integrations
 APPROVED

mohammad
 6/3/2020 1:15:18 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 02 15:51:27 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052020.M
 Quant Title : GC Extractables
 QLast Update : Wed May 20 11:27:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.513f	4.077	40493736	3957046	22.084m	1.461m#
28) SA Decachlor...	8.307	9.192	8403053	10555362	4.973	4.004

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060220\
Data File : PL059053.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jun 2020 12:31
Operator : AJ\MA
Sample : L2822-02 5X
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
C0AP7


Manual Integrations
APPROVED

mohammad
6/3/2020 1:15:18 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 02 15:51:27 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052020.M
Quant Title : GC Extractables
QLast Update : Wed May 20 11:27:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

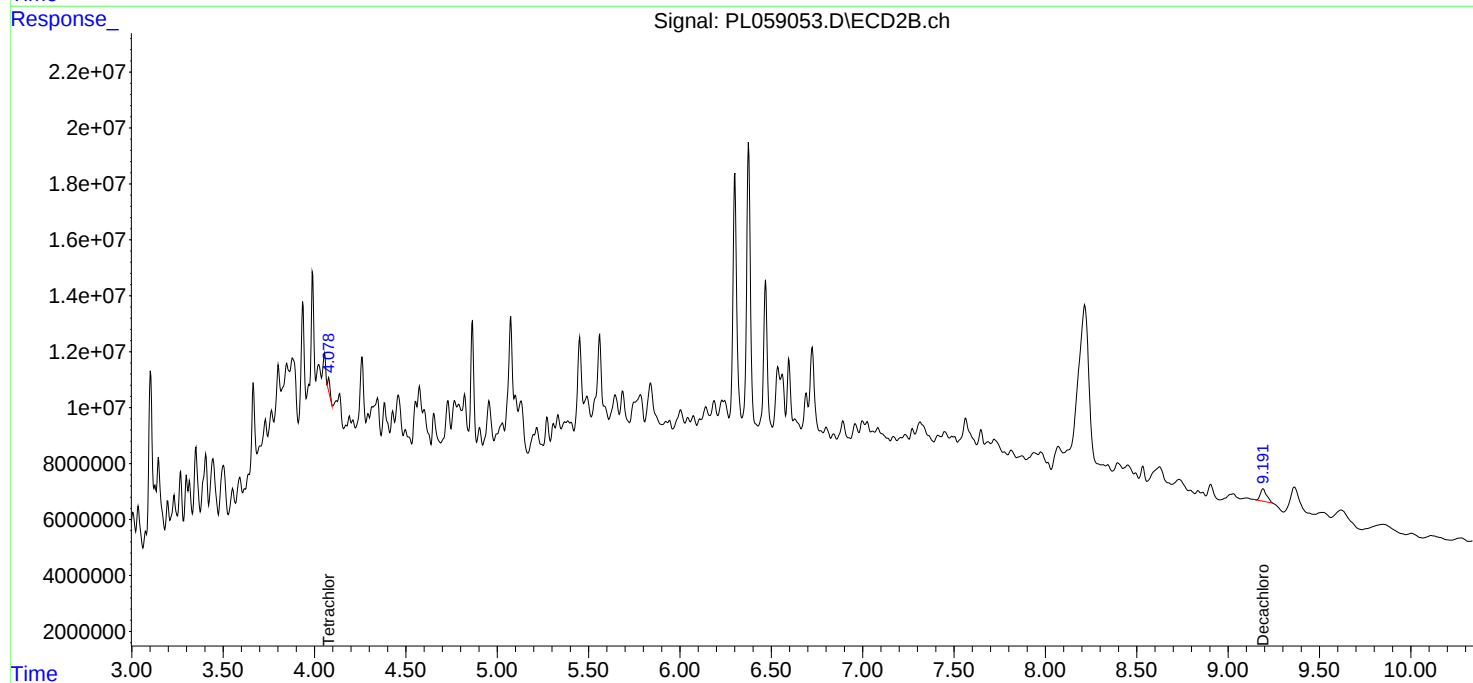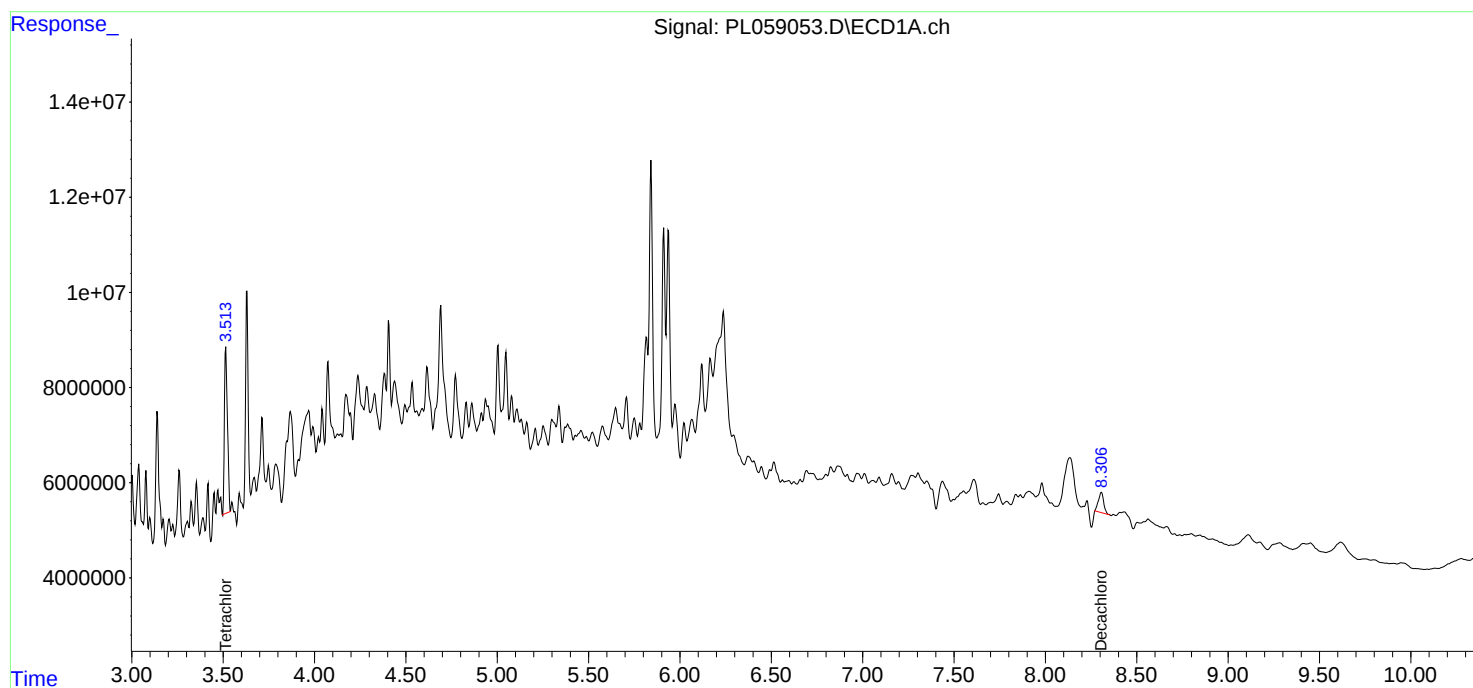

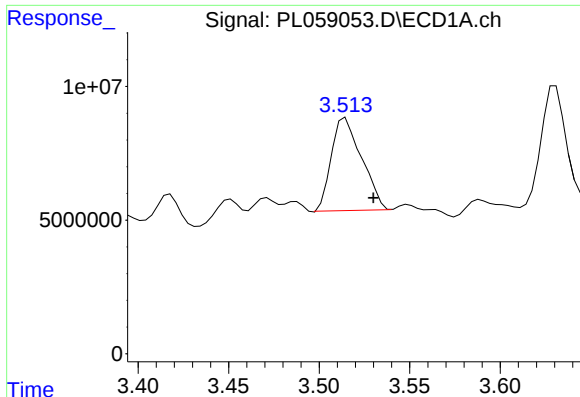

#1 Tetrachloro-m-xylene

R.T.: 3.513 min

Delta R.T.: -0.017 min


Response: 40493736

Conc: 22.08 ng/ml m

Instrument :
ECD_L
ClientSampleId :
C0AP7

Manual Integrations
APPROVED

mohammad
6/3/2020 1:15:18 PM

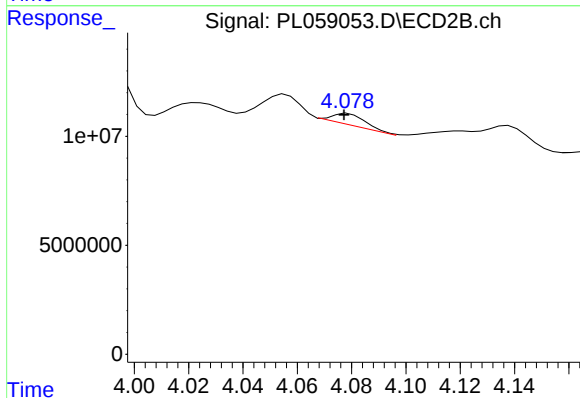

#1 Tetrachloro-m-xylene

R.T.: 4.077 min

Delta R.T.: 0.000 min

Response: 3957046

Conc: 1.46 ng/ml m


#28 Decachlorobiphenyl

R.T.: 8.307 min

Delta R.T.: -0.006 min

Response: 8403053

Conc: 4.97 ng/ml

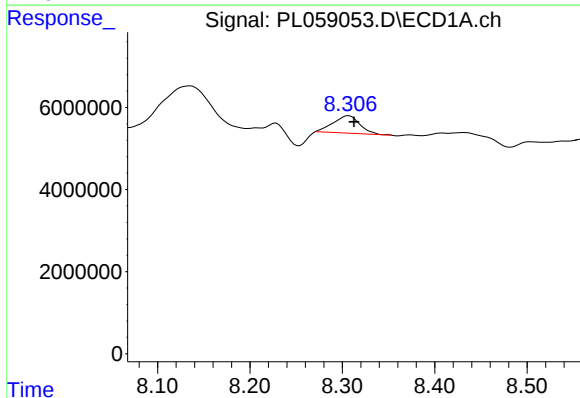

#28 Decachlorobiphenyl

R.T.: 9.192 min

Delta R.T.: 0.002 min

Response: 10555362

Conc: 4.00 ng/ml