

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060221\
 Data File : PL066992.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jun 2021 12:00
 Operator : AR\AJ
 Sample : M2551-06
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 02 14:41:59 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060121.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 02 14:20:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.481	5.532	10504129	16777384	25.651	25.935
28)	SA Decachlor...	10.227	11.433	16479406	22031750	25.485	26.406
Target Compounds							
6)	B beta-BHC	5.966f	0.000	450858	0	1.693	N.D. #
7)	B delta-BHC	0.000	7.009f	0	2258077	N.D.	2.974 #
10)	B gamma-Chl...	0.000	8.240f	0	1524889	N.D.	2.147 #
14)	MA Endrin	7.898f	0.000	452970	0	0.875	N.D. #
15)	B Endosulfa...	8.179	9.182f	511249	587393	0.987	0.952
17)	MA 4,4'-DDT	8.341f	0.000	233955	0	0.508	N.D. #
18)	B Endrin al...	8.376	0.000	191896	0	0.417	N.D. #
23)	Chlordane-1	5.784f	0.000	248271	0	16.281	N.D. #
25)	Chlordane-3	0.000	8.240f	0	1524889	N.D.	14.567 #
27)	Chlordane-5	8.179	0.000	511249	0	27.095	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060221\
Data File : PL066992.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jun 2021 12:00
Operator : AR\AJ
Sample : M2551-06
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 02 14:41:59 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060121.M
Quant Title : GC Extractables
QLast Update : Wed Jun 02 14:20:39 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

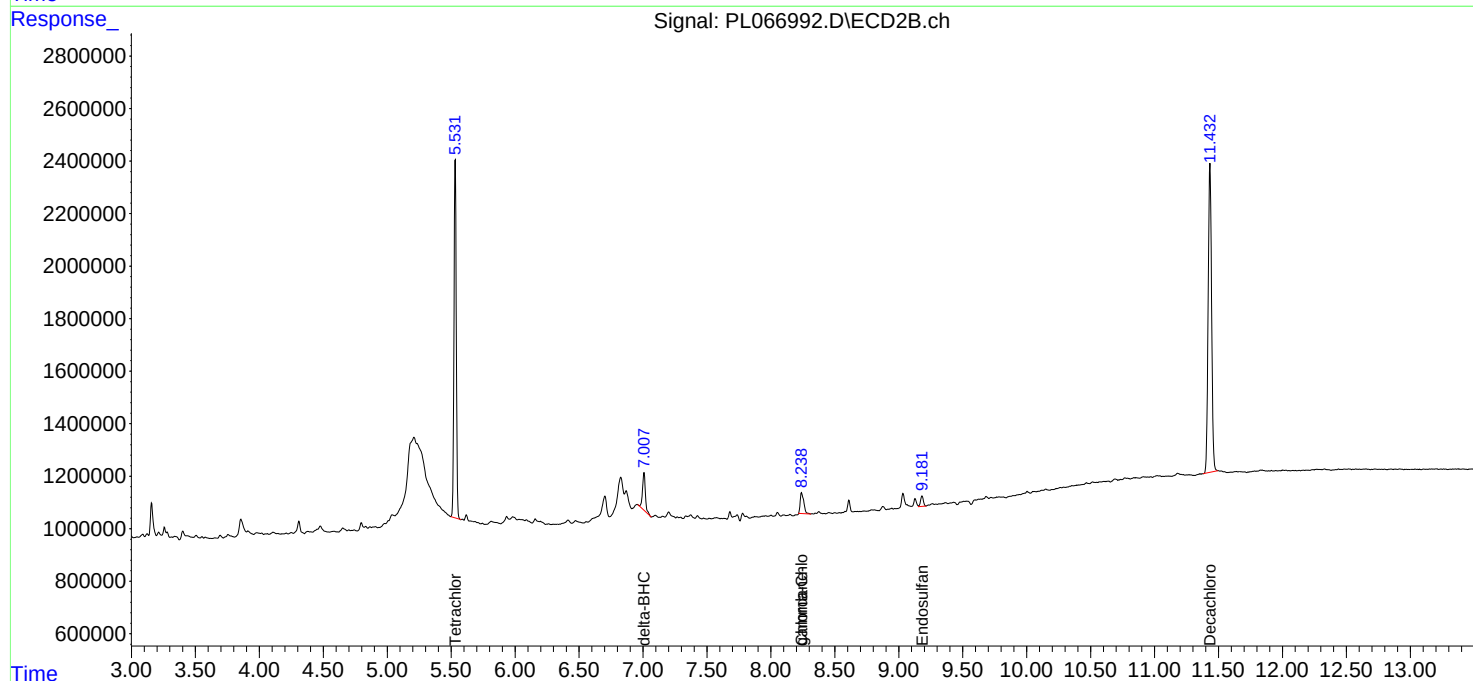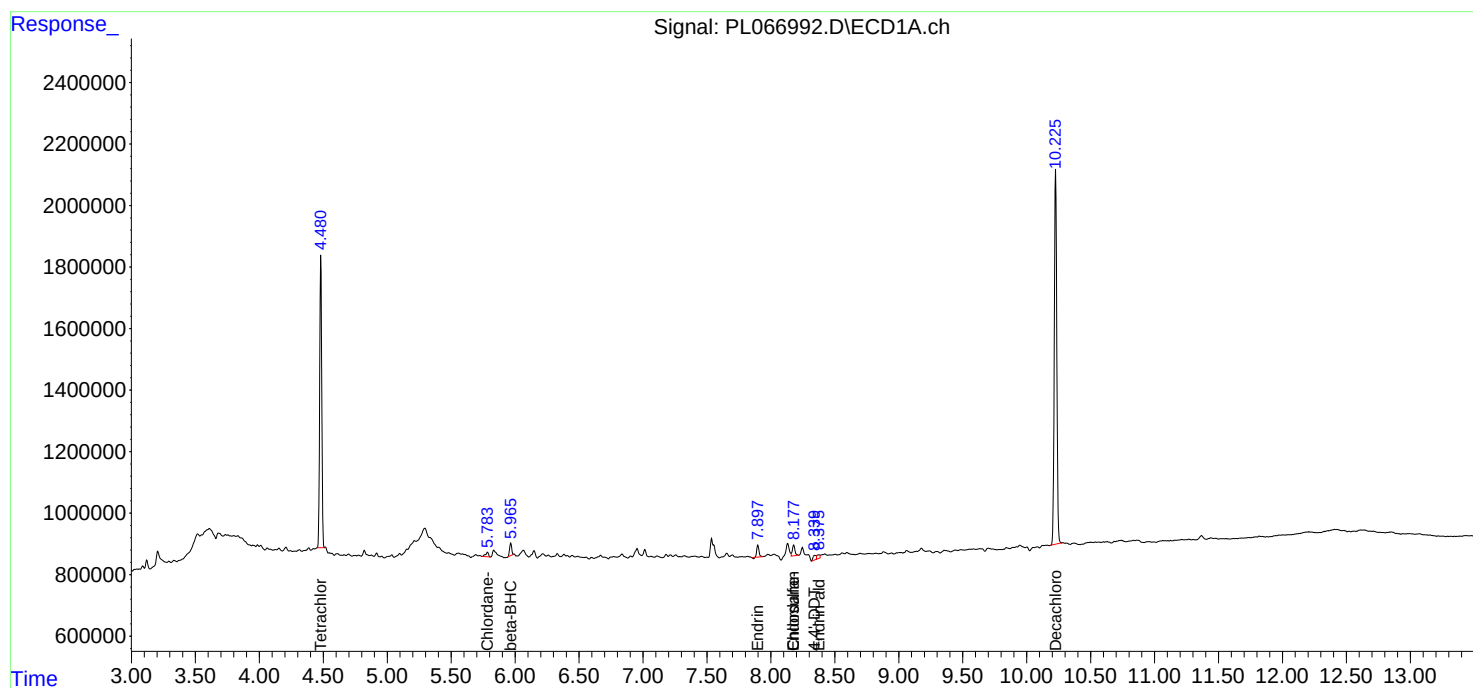


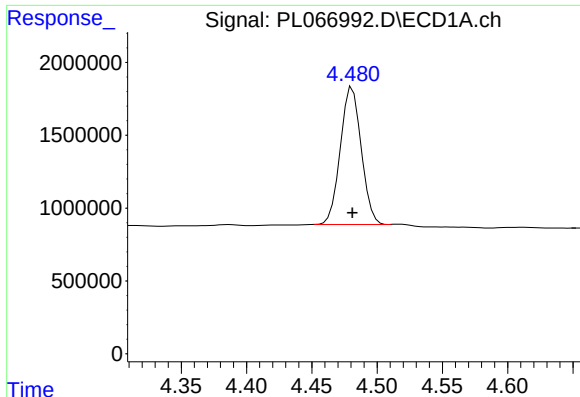

#1 Tetrachloro-m-xylene


R.T.: 4.481 min
Delta R.T.: 0.000 min
Response: 10504129
Conc: 25.65 ng/ml

Instrument :
ECD_L
ClientSampleId :

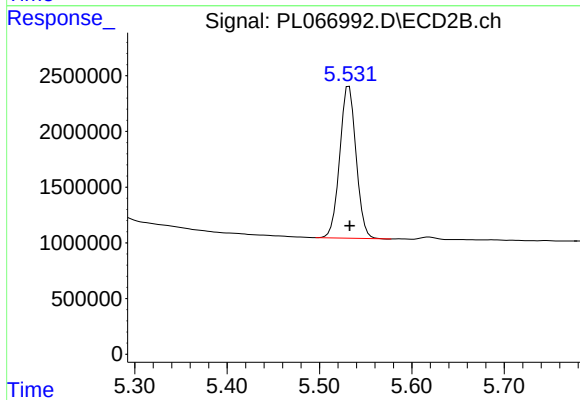


#1 Tetrachloro-m-xylene

R.T.: 5.532 min
Delta R.T.: 0.000 min
Response: 16777384
Conc: 25.94 ng/ml

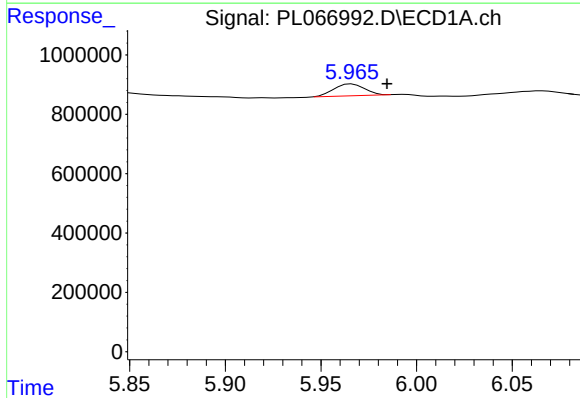


#6 beta-BHC

R.T.: 5.966 min
Delta R.T.: -0.018 min
Response: 450858
Conc: 1.69 ng/ml

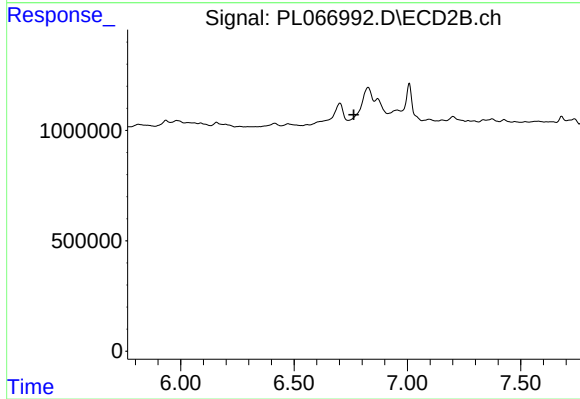

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 6.763 min
Response: 0
Conc: N.D.

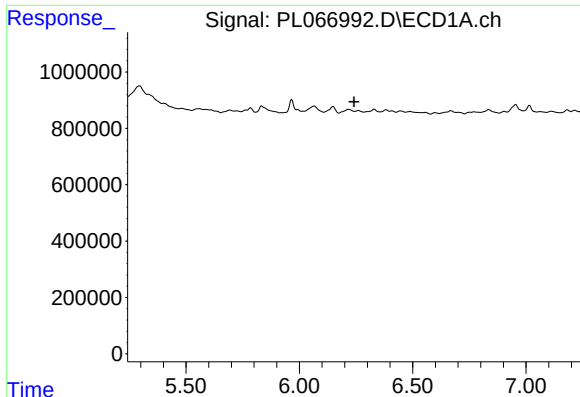

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 6.241 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

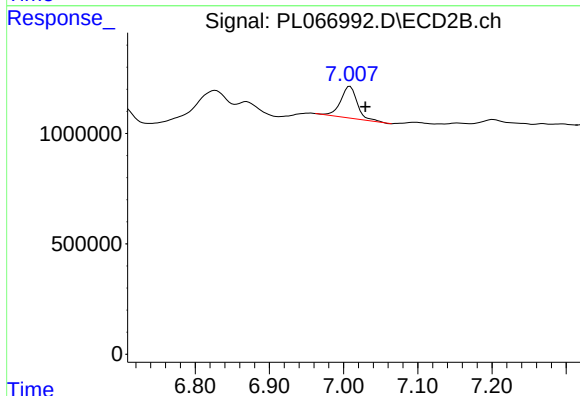


#7 delta-BHC

R.T.: 7.009 min
Delta R.T.: -0.021 min
Response: 2258077
Conc: 2.97 ng/ml

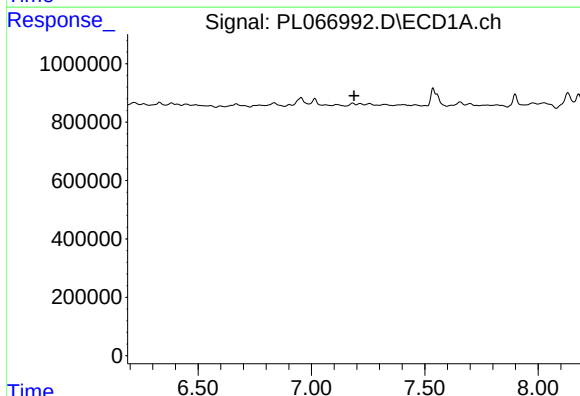


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.188 min
Response: 0
Conc: N.D.

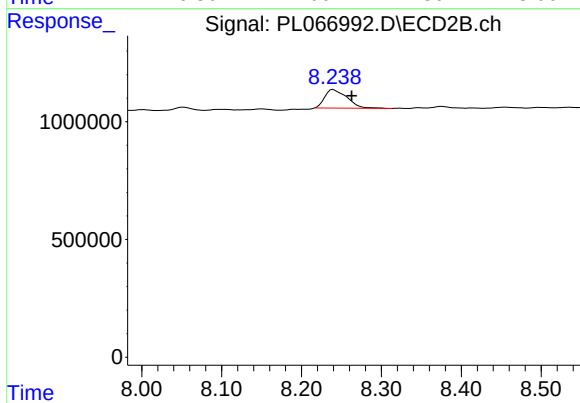

#10 gamma-Chlordane


R.T.: 8.240 min
Delta R.T.: -0.023 min
Response: 1524889
Conc: 2.15 ng/ml

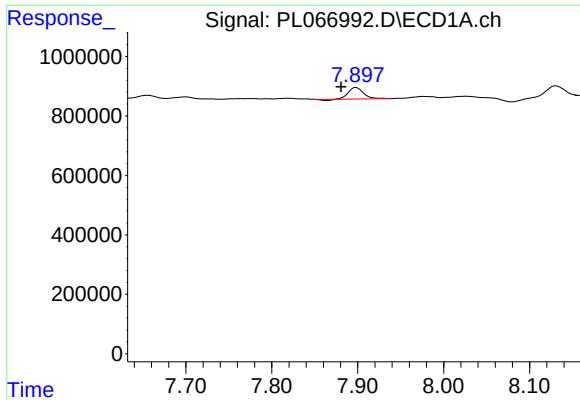

#14 Endrin


R.T.: 7.898 min
Delta R.T.: 0.018 min
Response: 452970
Conc: 0.87 ng/ml

Instrument :
ECD_L
ClientSampleId :

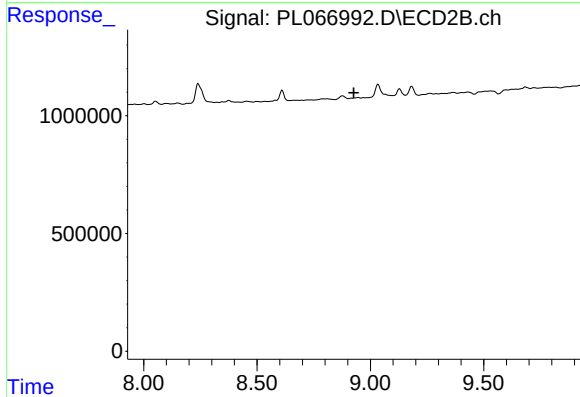


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 8.927 min
Response: 0
Conc: N.D.

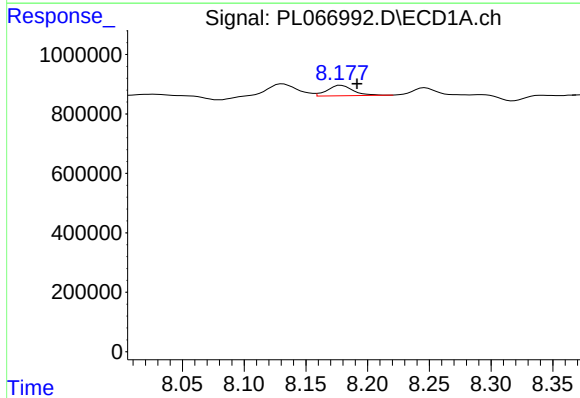


#15 Endosulfan II

R.T.: 8.179 min
Delta R.T.: -0.013 min
Response: 511249
Conc: 0.99 ng/ml

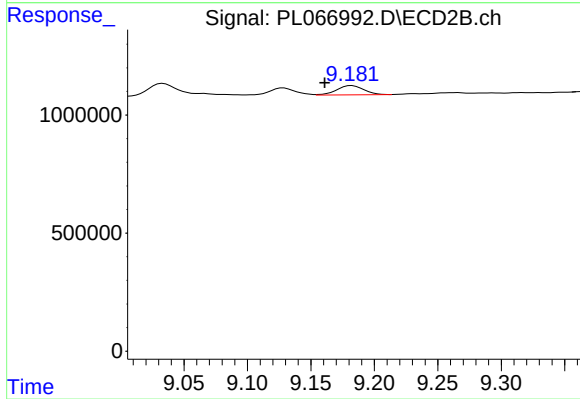

#15 Endosulfan II


R.T.: 9.182 min
Delta R.T.: 0.021 min
Response: 587393
Conc: 0.95 ng/ml

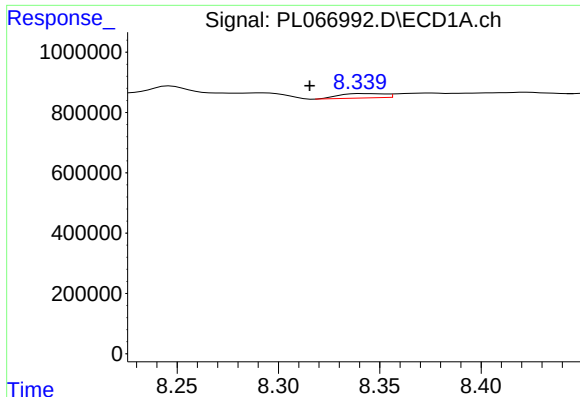

#17 4,4'-DDT


R.T.: 8.341 min
Delta R.T.: 0.026 min
Response: 233955
Conc: 0.51 ng/ml

Instrument :
ECD_L
ClientSampleId :

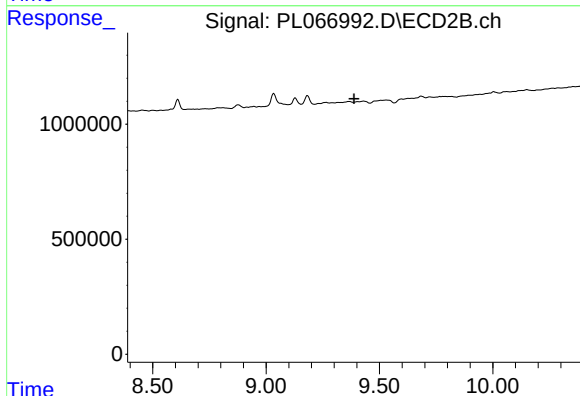


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 9.389 min
Response: 0
Conc: N.D.

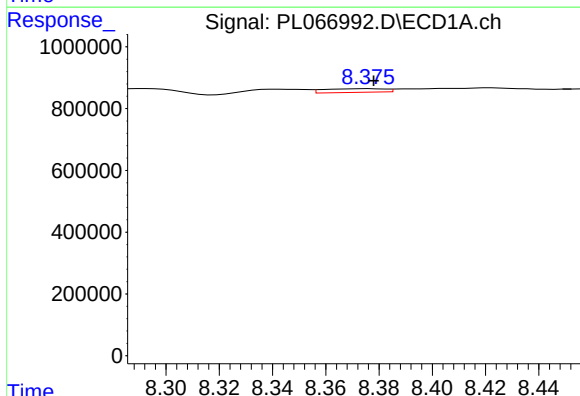


#18 Endrin aldehyde

R.T.: 8.376 min
Delta R.T.: -0.002 min
Response: 191896
Conc: 0.42 ng/ml

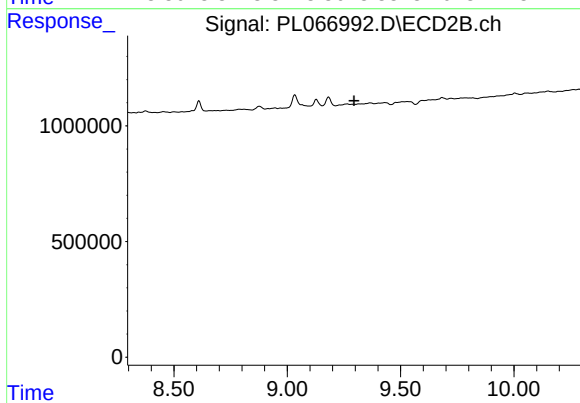

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 9.295 min
Response: 0
Conc: N.D.

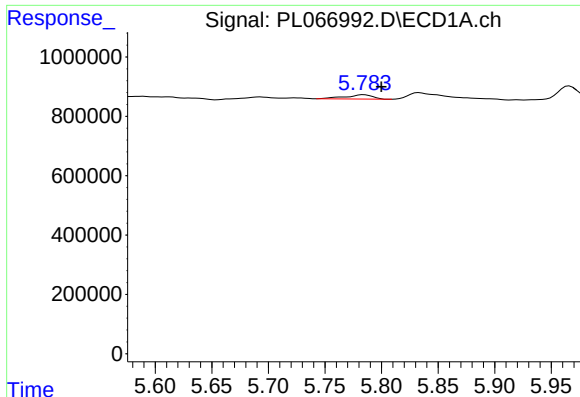

#23 Chlordane-1


R.T.: 5.784 min
Delta R.T.: -0.016 min
Response: 248271
Conc: 16.28 ng/ml

Instrument :
ECD_L
ClientSampleId :

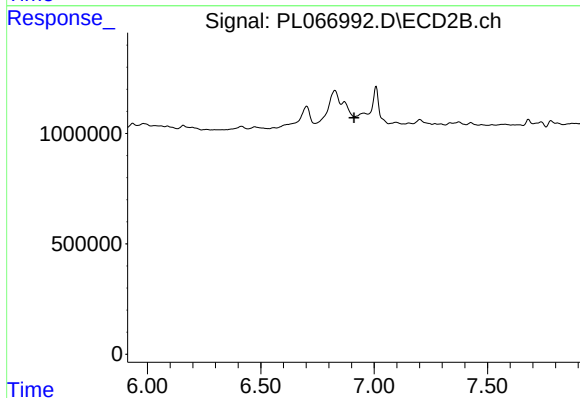


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 6.912 min
Response: 0
Conc: N.D.

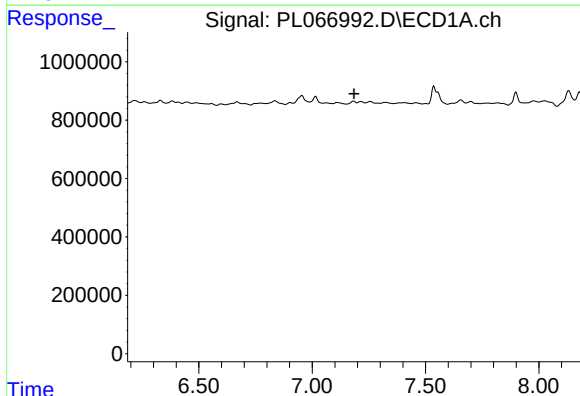


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 7.185 min
Response: 0
Conc: N.D.

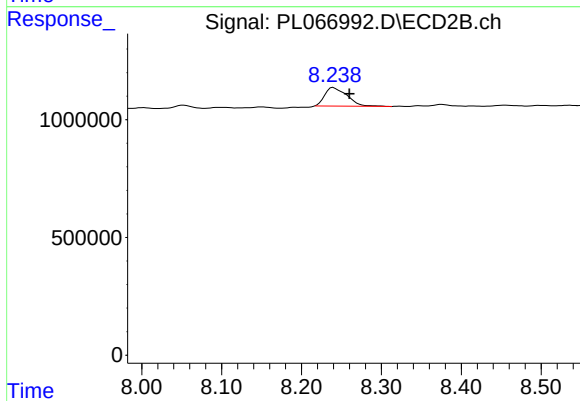

#25 Chlordane-3


R.T.: 8.240 min
Delta R.T.: -0.020 min
Response: 1524889
Conc: 14.57 ng/ml

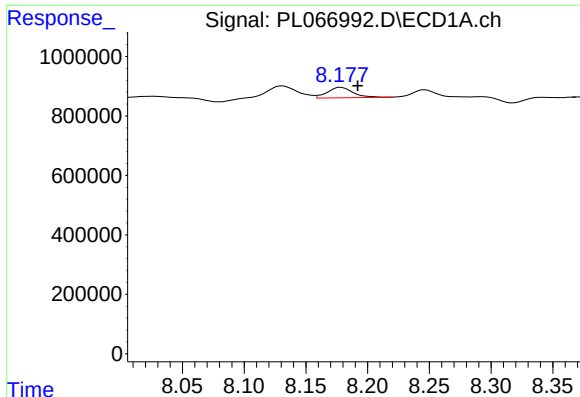

#27 Chlordane-5


R.T.: 8.179 min
Delta R.T.: -0.013 min
Response: 511249
Conc: 27.09 ng/ml

Instrument :
ECD_L
ClientSampleId :

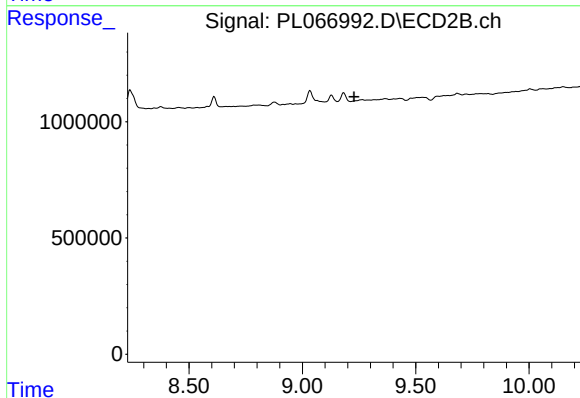


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 9.229 min
Response: 0
Conc: N.D.

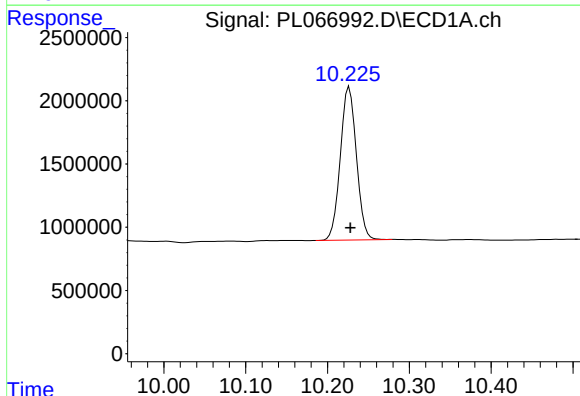

#28 Decachlorobiphenyl

R.T.: 10.227 min
Delta R.T.: -0.001 min
Response: 16479406
Conc: 25.49 ng/ml

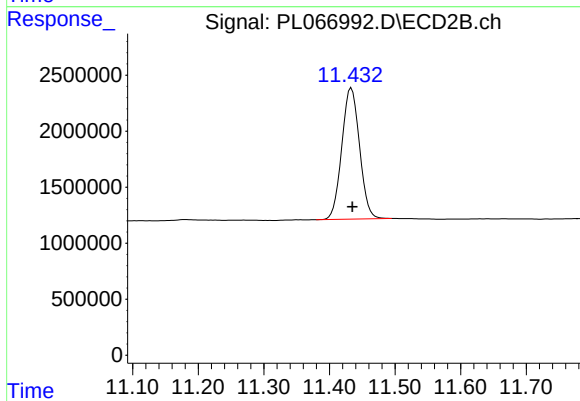

#28 Decachlorobiphenyl

R.T.: 11.433 min
Delta R.T.: -0.002 min
Response: 22031750
Conc: 26.41 ng/ml