

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060221\
 Data File : PL066993.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jun 2021 12:20
 Operator : AR\AJ
 Sample : M2551-10
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 02 14:42:07 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060121.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 02 14:20:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.480	5.532	9719795	15484542	23.736	23.937
28)	SA Decachlor...	10.226	11.433	15122577	20394073	23.387	24.443
Target Compounds							
6)	B beta-BHC	5.966f	0.000	516727	0	1.940	N.D. #
7)	B delta-BHC	0.000	7.009f	0	2173357	N.D.	2.862 #
10)	B gamma-Chl...	0.000	8.241f	0	945637	N.D.	1.332 #
14)	MA Endrin	7.899f	0.000	698780	0	1.349	N.D. #
15)	B Endosulfa...	8.178	9.183f	239030	562577	0.461	0.912 #
18)	B Endrin al...	8.360f	0.000	218163	0	0.474	N.D. #
23)	Chlordane-1	5.785	0.000	265760	0	17.428	N.D. #
25)	Chlordane-3	0.000	8.241f	0	945637	N.D.	9.033 #
27)	Chlordane-5	8.178	0.000	239030	0	12.668	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060221\
Data File : PL066993.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jun 2021 12:20
Operator : AR\AJ
Sample : M2551-10
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 02 14:42:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060121.M
Quant Title : GC Extractables
QLast Update : Wed Jun 02 14:20:39 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

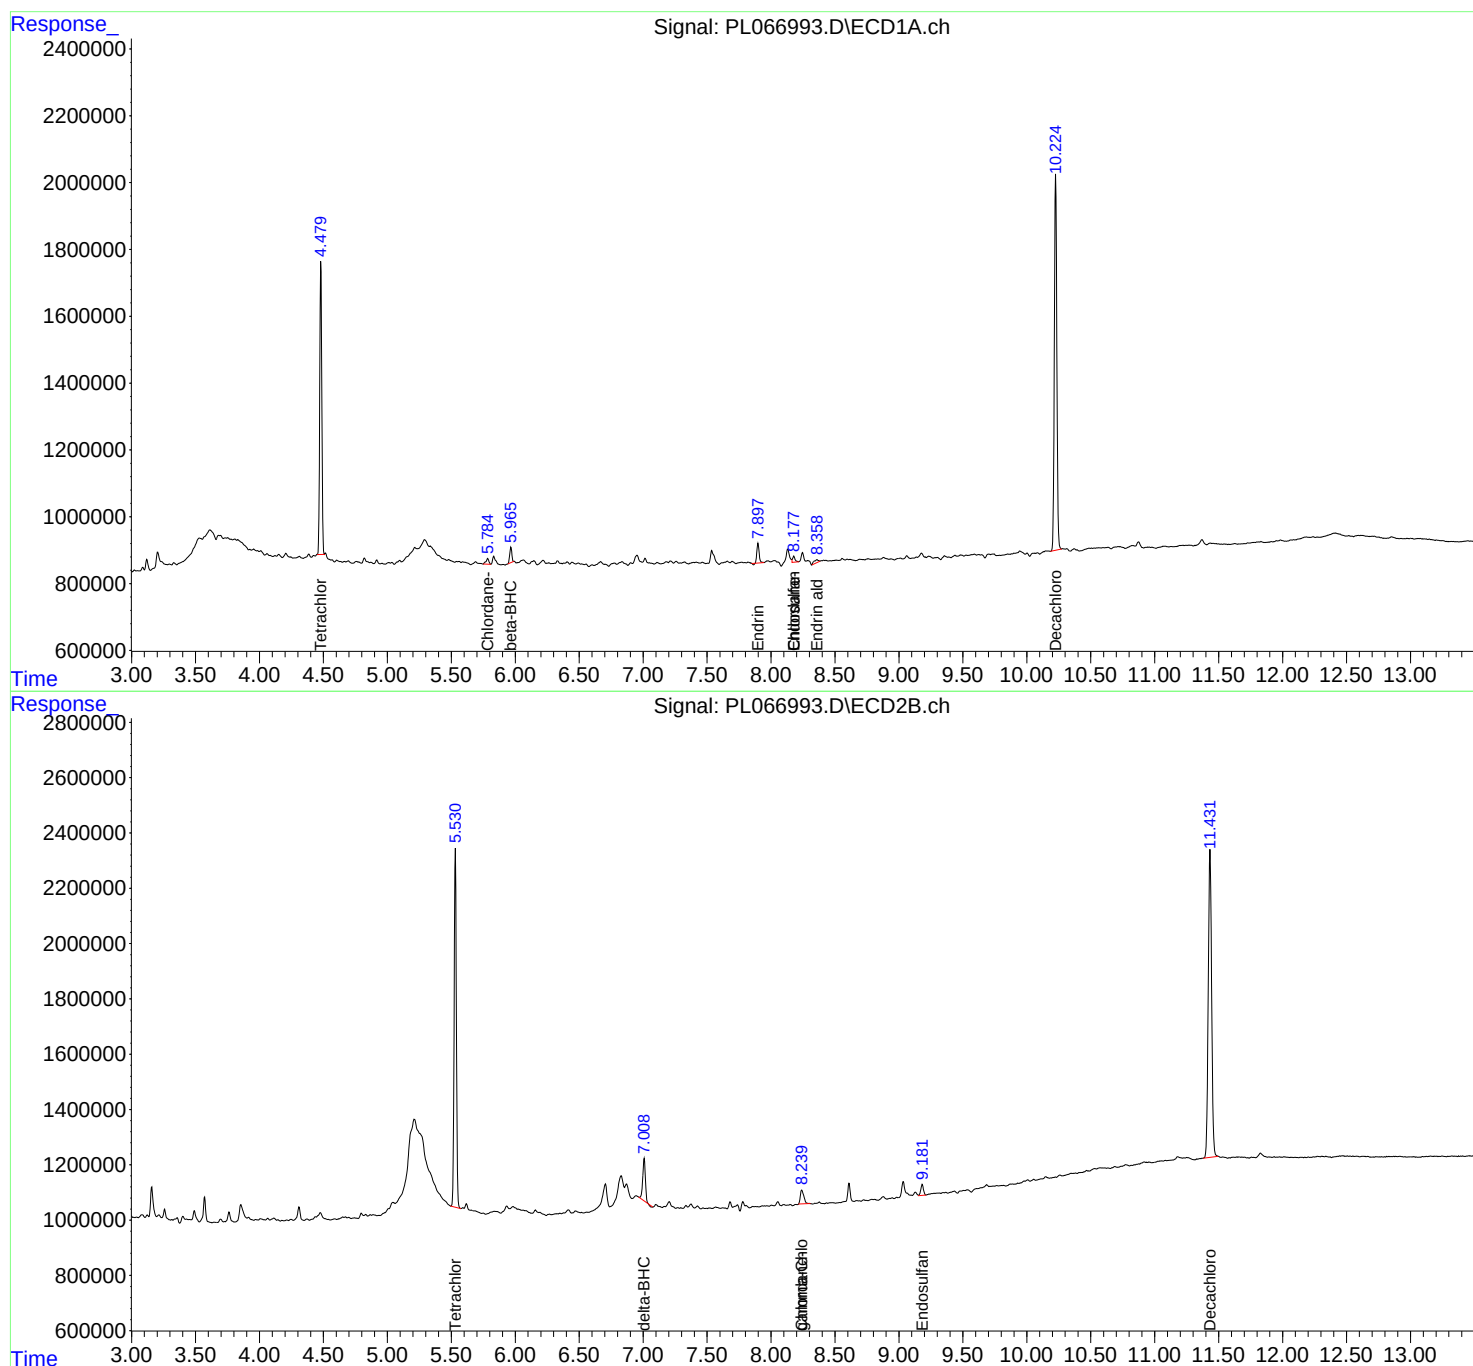


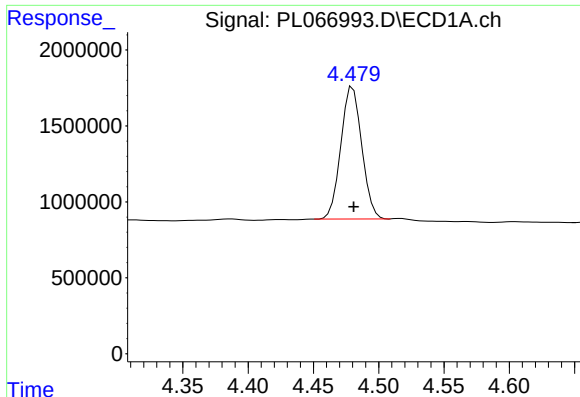

#1 Tetrachloro-m-xylene


R.T.: 4.480 min
Delta R.T.: 0.000 min
Response: 9719795
Conc: 23.74 ng/ml

Instrument :
ECD_L
ClientSampleId :

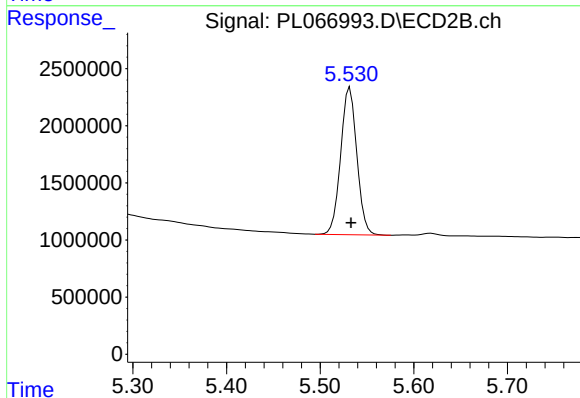


#1 Tetrachloro-m-xylene

R.T.: 5.532 min
Delta R.T.: -0.001 min
Response: 15484542
Conc: 23.94 ng/ml

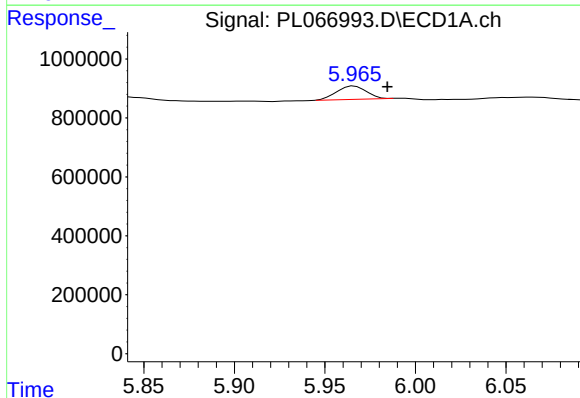


#6 beta-BHC

R.T.: 5.966 min
Delta R.T.: -0.018 min
Response: 516727
Conc: 1.94 ng/ml

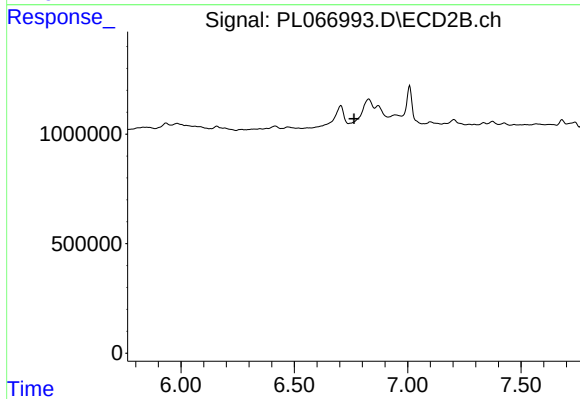

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 6.763 min
Response: 0
Conc: N.D.

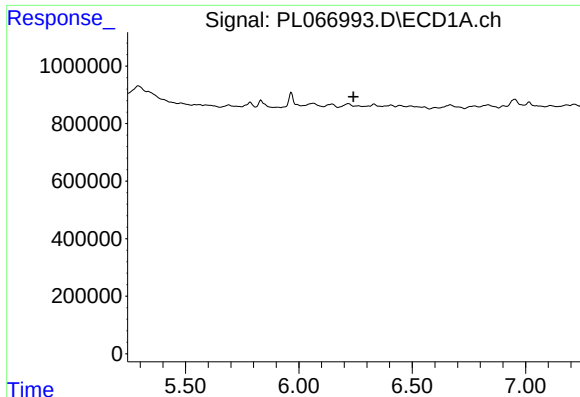

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 6.241 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

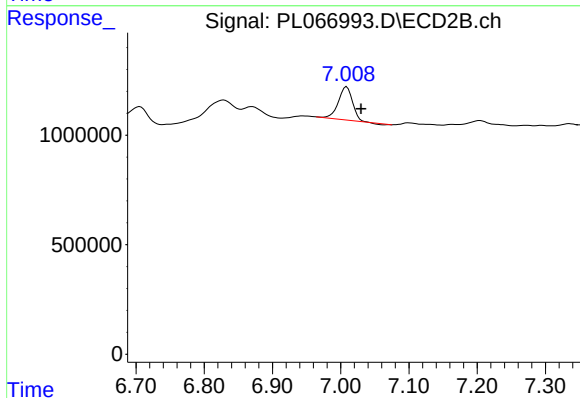


#7 delta-BHC

R.T.: 7.009 min
Delta R.T.: -0.021 min
Response: 2173357
Conc: 2.86 ng/ml

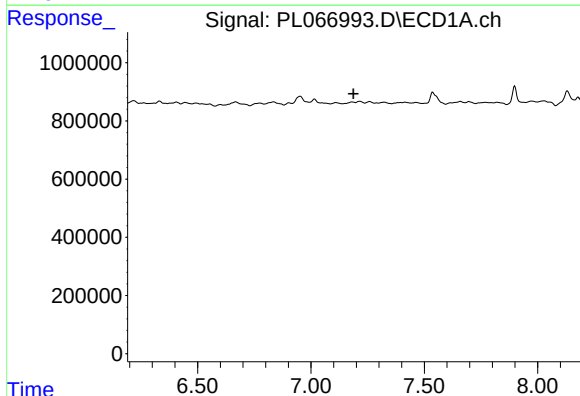


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.188 min
Response: 0
Conc: N.D.

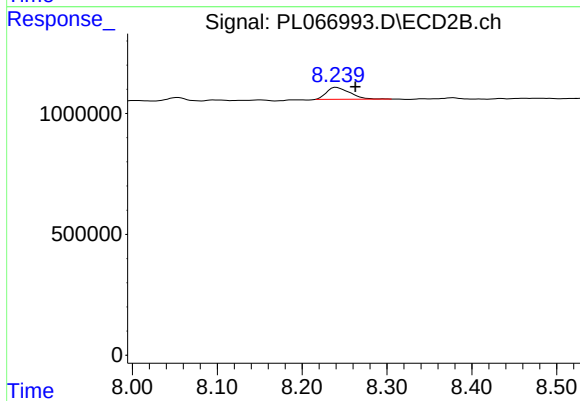

#10 gamma-Chlordane


R.T.: 8.241 min
Delta R.T.: -0.022 min
Response: 945637
Conc: 1.33 ng/ml

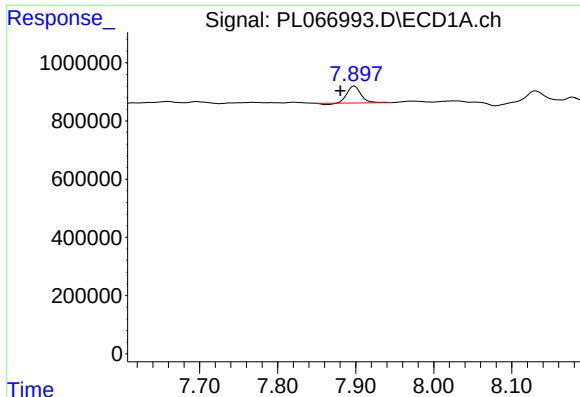

#14 Endrin


R.T.: 7.899 min
Delta R.T.: 0.018 min
Response: 698780
Conc: 1.35 ng/ml

Instrument :
ECD_L
ClientSampleId :

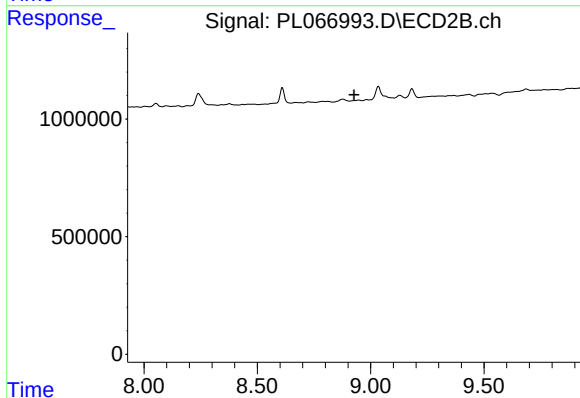


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 8.927 min
Response: 0
Conc: N.D.

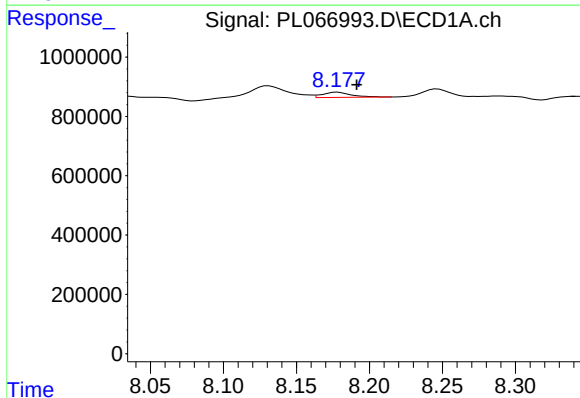


#15 Endosulfan II

R.T.: 8.178 min
Delta R.T.: -0.013 min
Response: 239030
Conc: 0.46 ng/ml

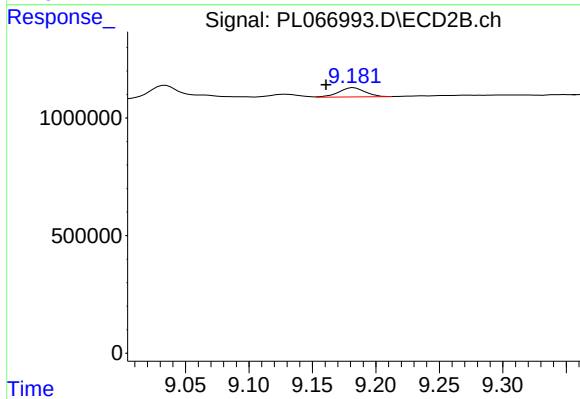

#15 Endosulfan II


R.T.: 9.183 min
Delta R.T.: 0.022 min
Response: 562577
Conc: 0.91 ng/ml

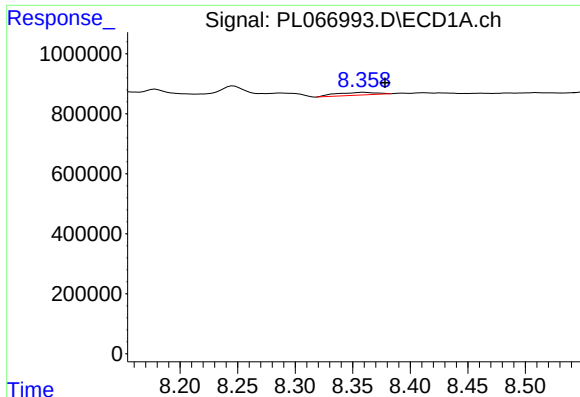

#18 Endrin aldehyde


R.T.: 8.360 min
Delta R.T.: -0.018 min
Response: 218163
Conc: 0.47 ng/ml

Instrument :
ECD_L
ClientSampleId :

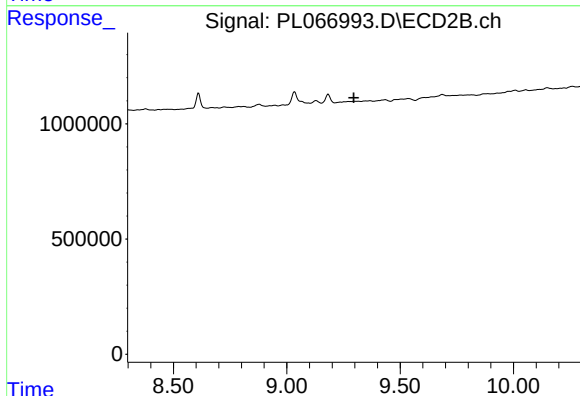


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 9.295 min
Response: 0
Conc: N.D.

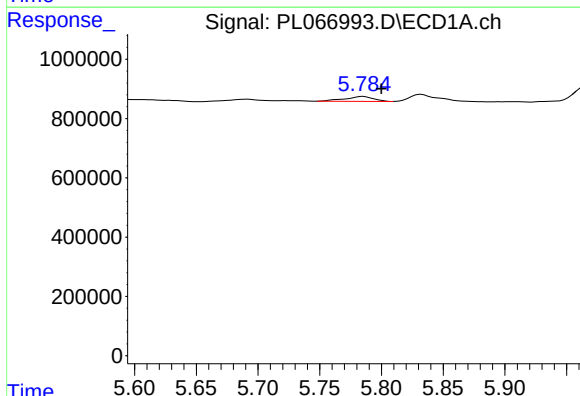


#23 Chlordane-1

R.T.: 5.785 min
Delta R.T.: -0.015 min
Response: 265760
Conc: 17.43 ng/ml

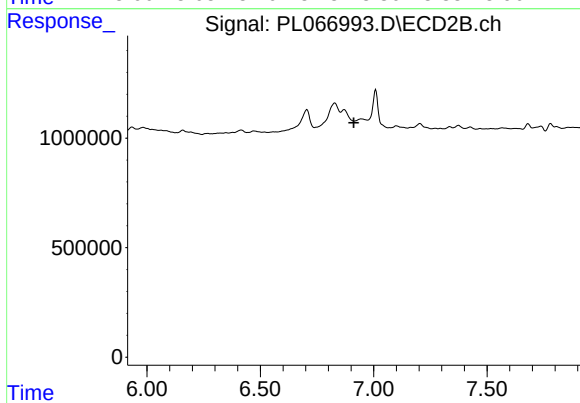

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 6.912 min
Response: 0
Conc: N.D.

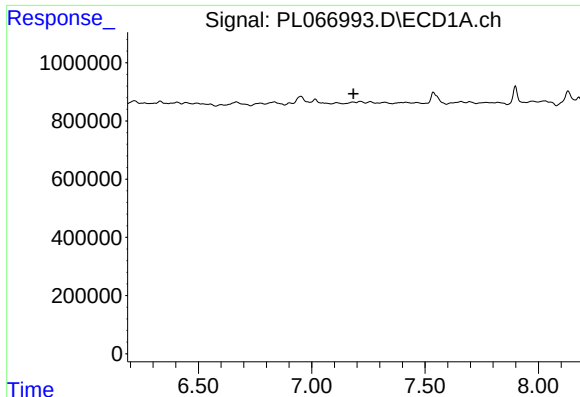

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.185 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

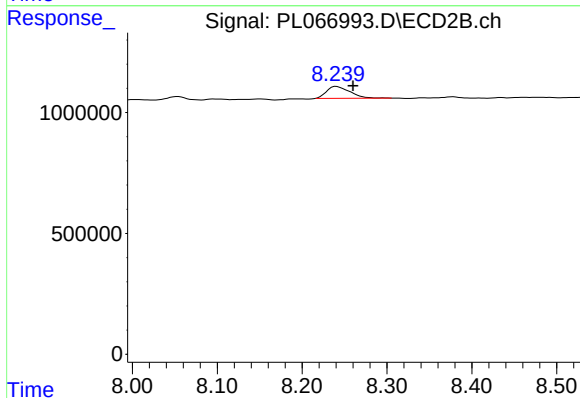


#25 Chlordane-3

R.T.: 8.241 min
Delta R.T.: -0.019 min
Response: 945637
Conc: 9.03 ng/ml

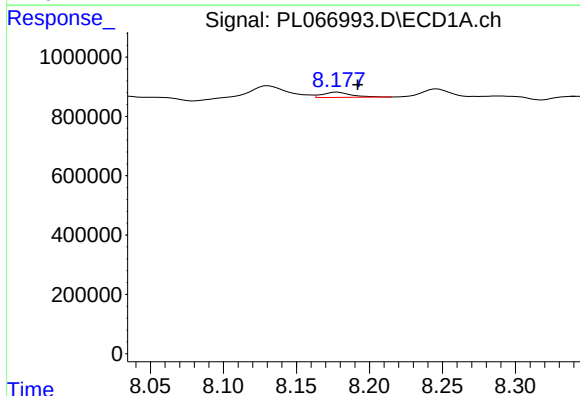


#27 Chlordane-5

R.T.: 8.178 min
Delta R.T.: -0.013 min
Response: 239030
Conc: 12.67 ng/ml

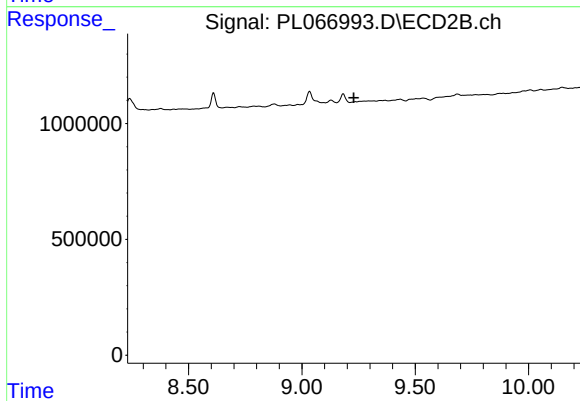

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 9.229 min
Response: 0
Conc: N.D.

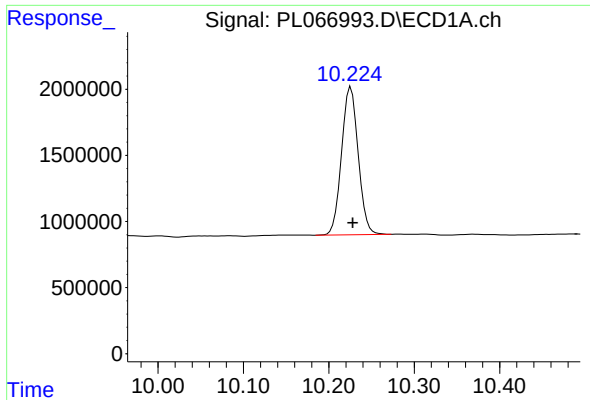

#28 Decachlorobiphenyl

R.T.: 10.226 min
Delta R.T.: -0.002 min
Response: 15122577
Conc: 23.39 ng/ml

Instrument :
ECD_L
ClientSampleId :

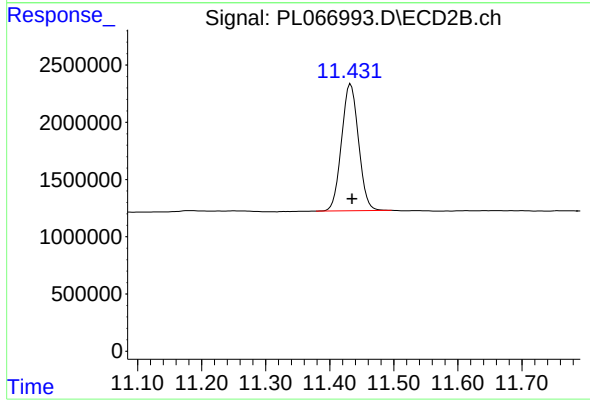

#28 Decachlorobiphenyl

R.T.: 11.433 min
Delta R.T.: -0.002 min
Response: 20394073
Conc: 24.44 ng/ml