

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060221\
 Data File : PL066994.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jun 2021 12:39
 Operator : AR\AJ
 Sample : M2560-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 02 14:42:15 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060121.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 02 14:20:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.481	5.532	10491813	16116152	25.621	24.913
28)	SA Decachlor...	10.227	11.433	12492642	16863242	19.320	20.211
Target Compounds							
4)	MA Heptachlor	5.991f	0.000	291556	0	0.555	N.D. #
6)	B beta-BHC	5.991	0.000	291556	0	1.095	N.D. #
7)	B delta-BHC	0.000	7.008f	0	2870072	N.D.	3.780 #
11)	B alpha-Chl...	7.256	0.000	217247	0	0.378	N.D. #
14)	MA Endrin	7.899f	0.000	458080	0	0.885	N.D. #
15)	B Endosulfa...	8.181	9.183f	259186	500256	0.500	0.811 #
17)	MA 4,4'-DDT	8.340f	0.000	45421	0	0.099	N.D. #
26)	Chlordane-4	7.256	0.000	217247	0	3.403	N.D. #
27)	Chlordane-5	8.181	0.000	259186	0	13.736	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060221\
Data File : PL066994.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jun 2021 12:39
Operator : AR\AJ
Sample : M2560-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 02 14:42:15 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060121.M
Quant Title : GC Extractables
QLast Update : Wed Jun 02 14:20:39 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

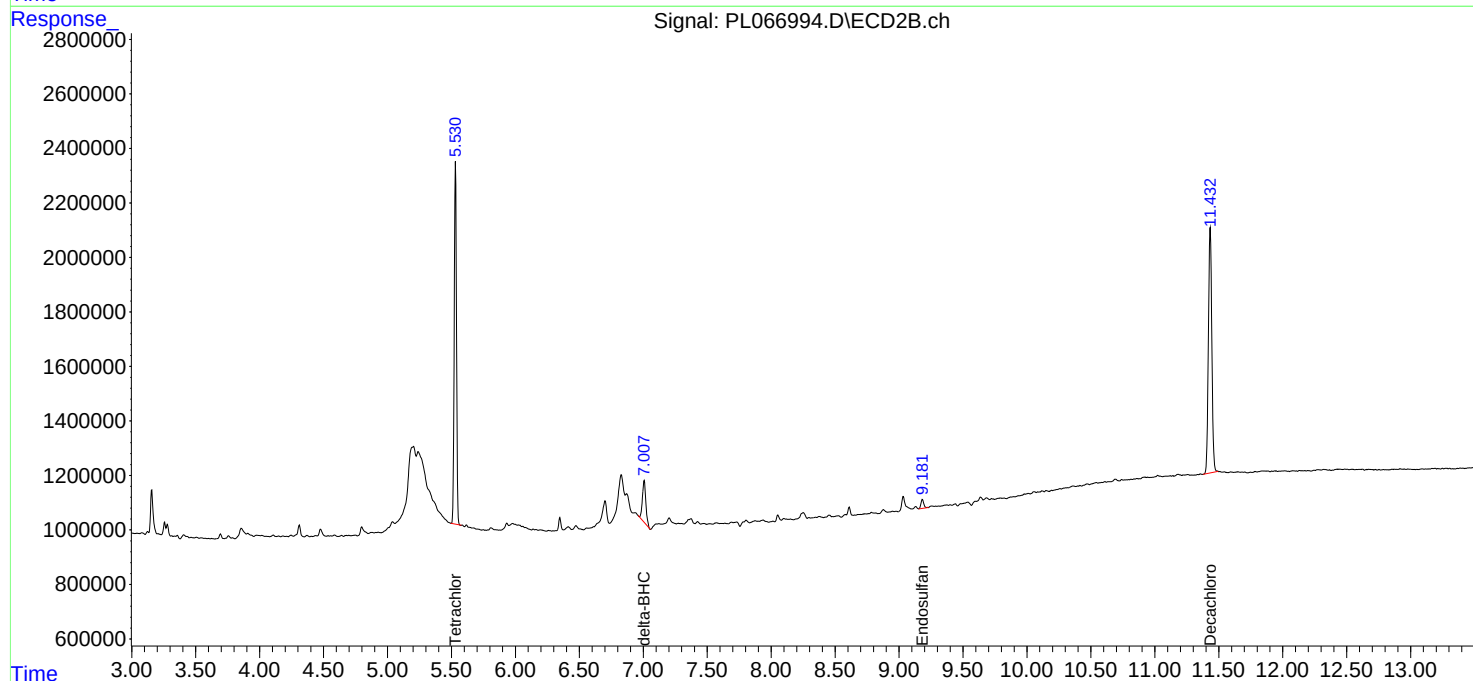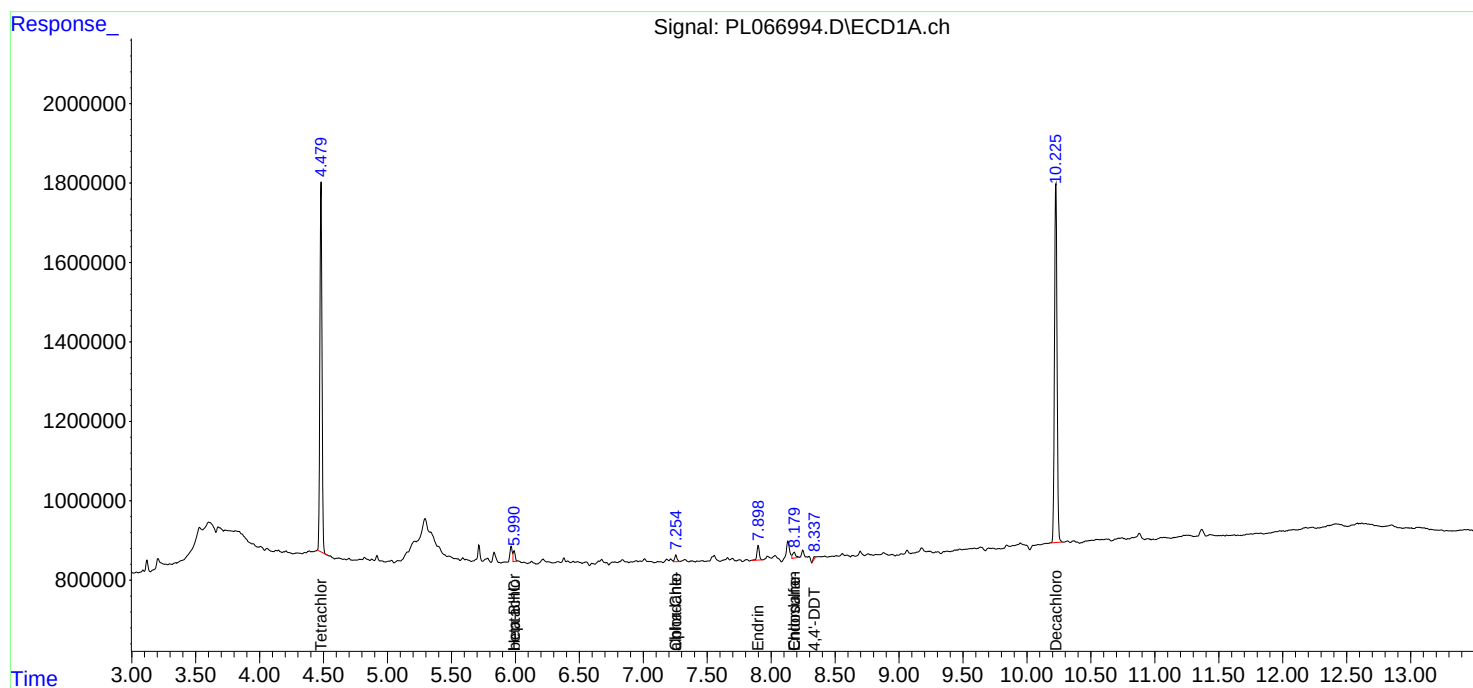


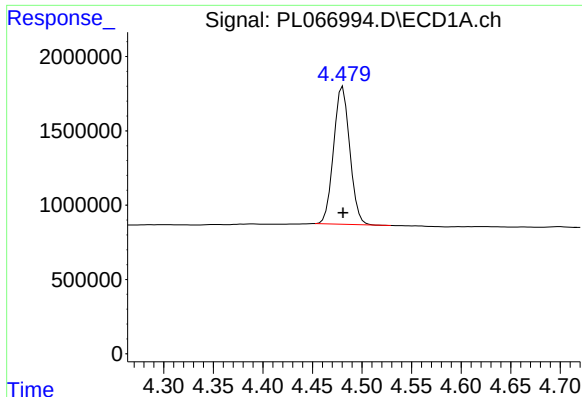

#1 Tetrachloro-m-xylene


R.T.: 4.481 min
Delta R.T.: 0.000 min
Response: 10491813
Conc: 25.62 ng/ml

Instrument :
ECD_L
ClientSampleId :

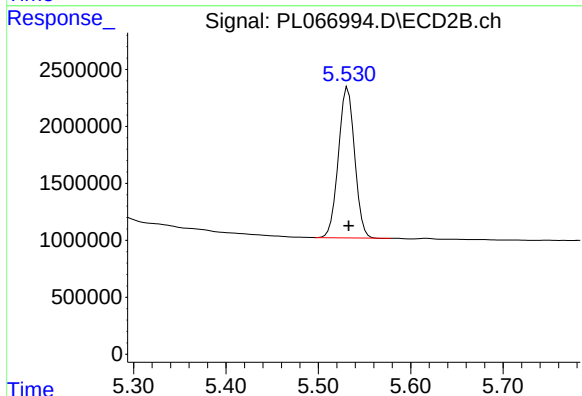


#1 Tetrachloro-m-xylene

R.T.: 5.532 min
Delta R.T.: 0.000 min
Response: 16116152
Conc: 24.91 ng/ml

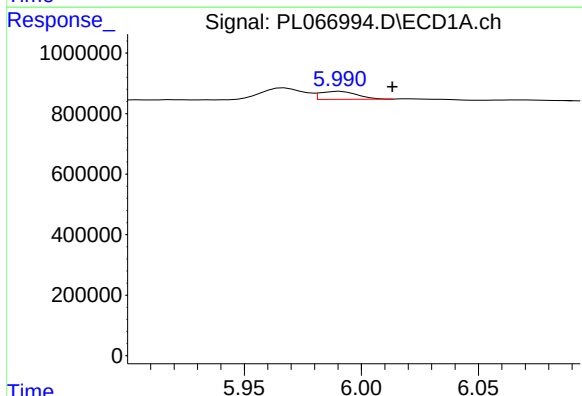


#4 Heptachlor

R.T.: 5.991 min
Delta R.T.: -0.022 min
Response: 291556
Conc: 0.56 ng/ml

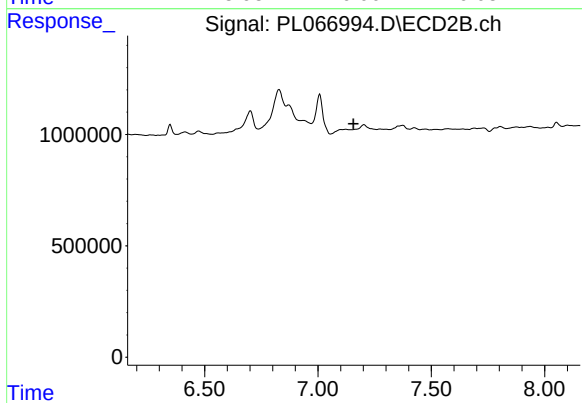

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 7.157 min
Response: 0
Conc: N.D.

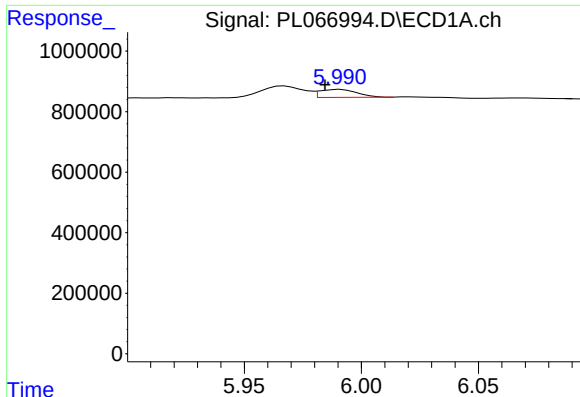

#6 beta-BHC


R.T.: 5.991 min
Delta R.T.: 0.006 min
Response: 291556
Conc: 1.09 ng/ml

Instrument :
ECD_L
ClientSampleId :

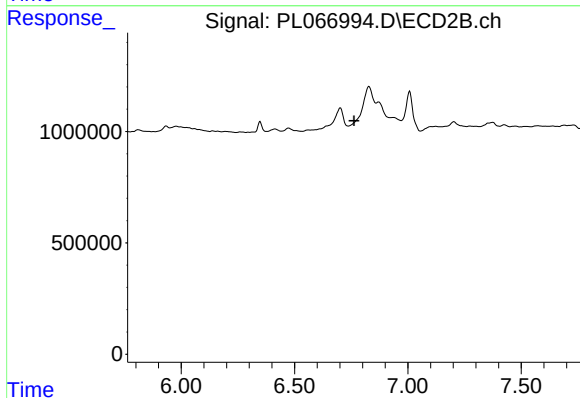


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.763 min
Response: 0
Conc: N.D.

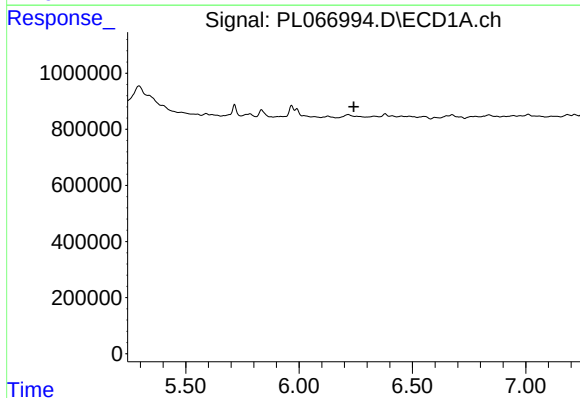


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.241 min
Response: 0
Conc: N.D.

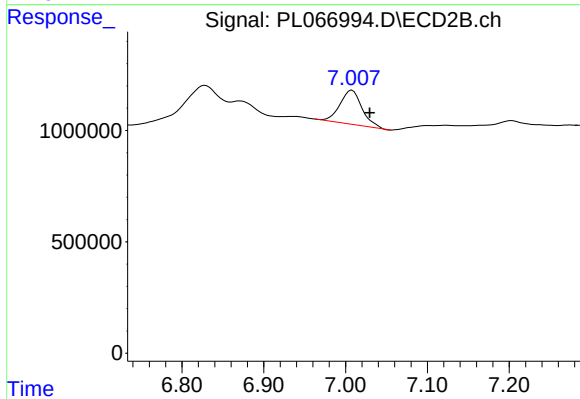

#7 delta-BHC


R.T.: 7.008 min
Delta R.T.: -0.022 min
Response: 2870072
Conc: 3.78 ng/ml

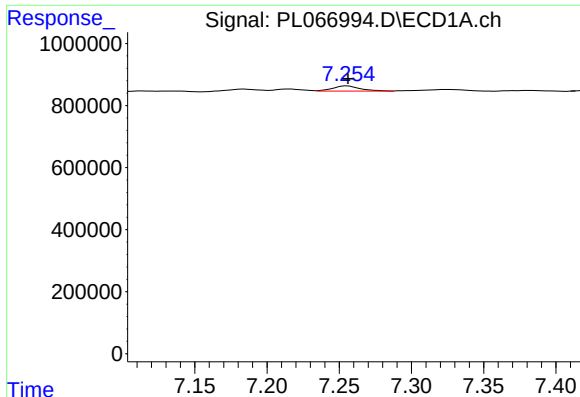

#11 alpha-Chlordane


R.T.: 7.256 min
Delta R.T.: 0.000 min
Response: 217247
Conc: 0.38 ng/ml

Instrument :
ECD_L
ClientSampleId :

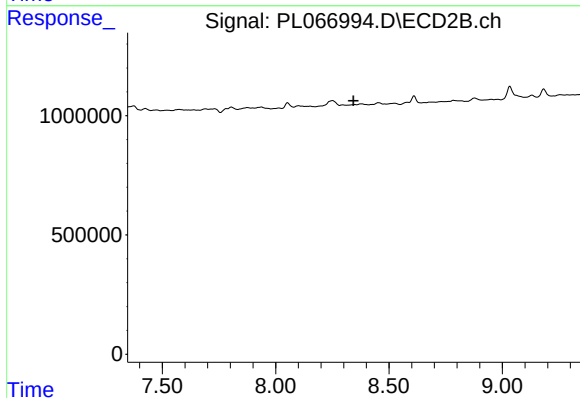


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 8.344 min
Response: 0
Conc: N.D.

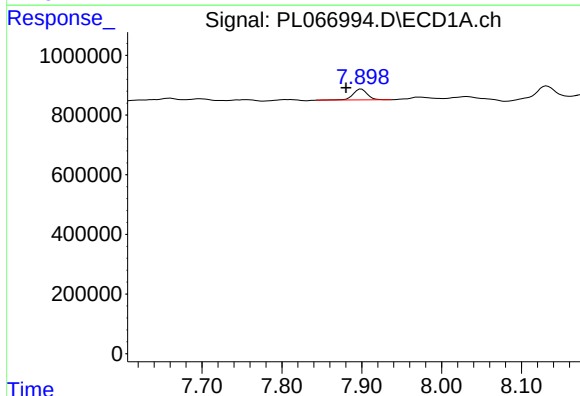


#14 Endrin

R.T.: 7.899 min
Delta R.T.: 0.019 min
Response: 458080
Conc: 0.88 ng/ml

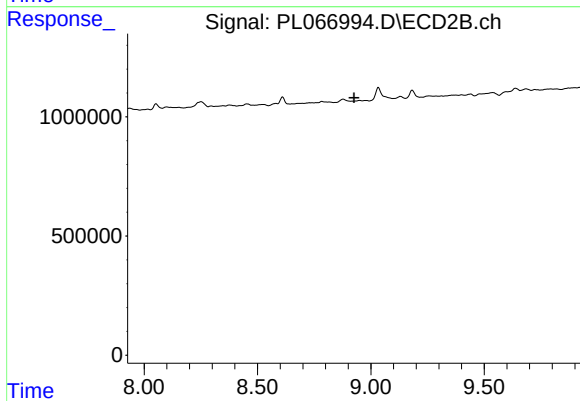

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 8.927 min
Response: 0
Conc: N.D.

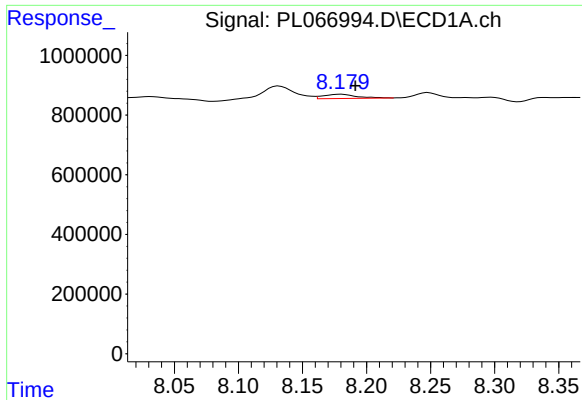

#15 Endosulfan II


R.T.: 8.181 min
Delta R.T.: -0.011 min
Response: 259186
Conc: 0.50 ng/ml

Instrument :
ECD_L
ClientSampleId :

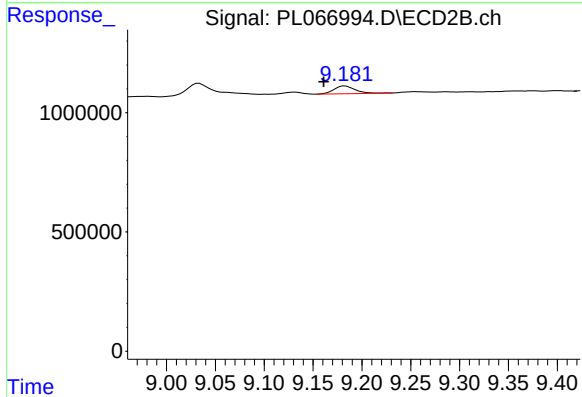


#15 Endosulfan II

R.T.: 9.183 min
Delta R.T.: 0.022 min
Response: 500256
Conc: 0.81 ng/ml

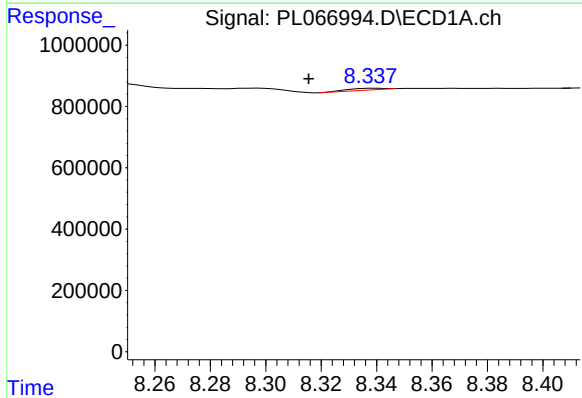


#17 4,4'-DDT

R.T.: 8.340 min
Delta R.T.: 0.024 min
Response: 45421
Conc: 0.10 ng/ml

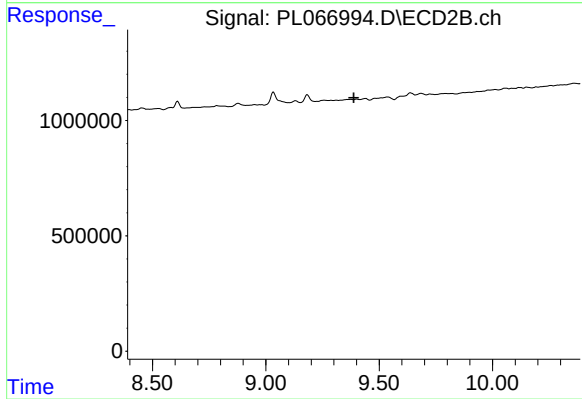

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 9.389 min
Response: 0
Conc: N.D.

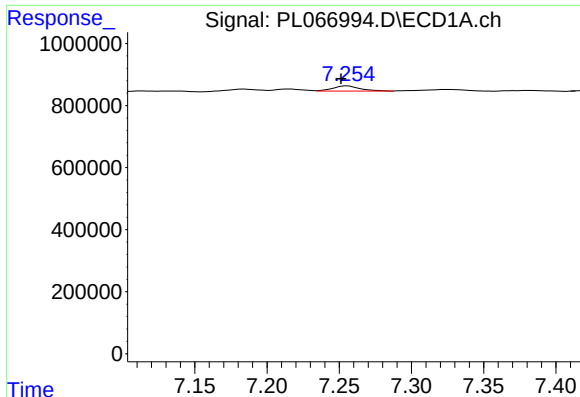

#26 Chlordane-4


R.T.: 7.256 min
Delta R.T.: 0.004 min
Response: 217247
Conc: 3.40 ng/ml

Instrument :
ECD_L
ClientSampleId :

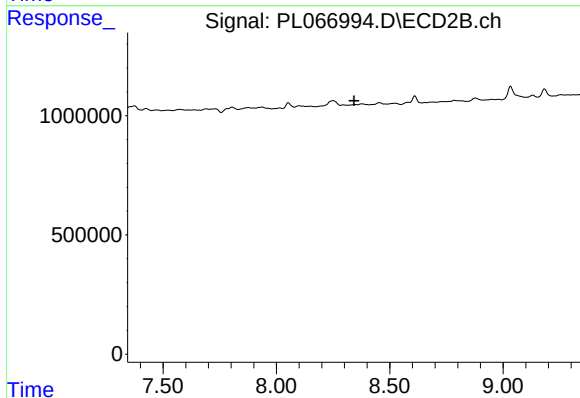


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 8.342 min
Response: 0
Conc: N.D.

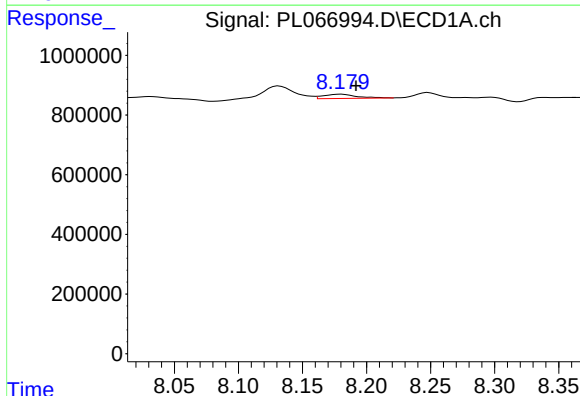


#27 Chlordane-5

R.T.: 8.181 min
Delta R.T.: -0.011 min
Response: 259186
Conc: 13.74 ng/ml

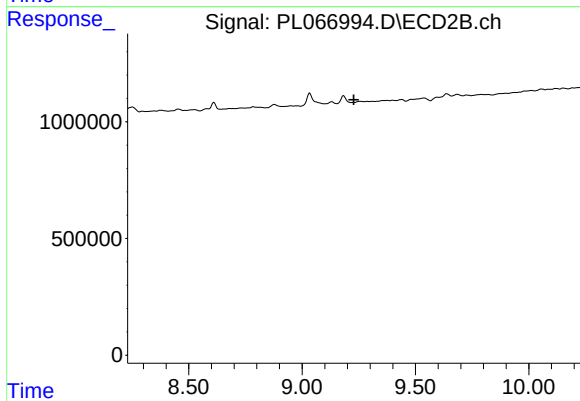

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T. : 9.229 min
Response: 0
Conc: N.D.

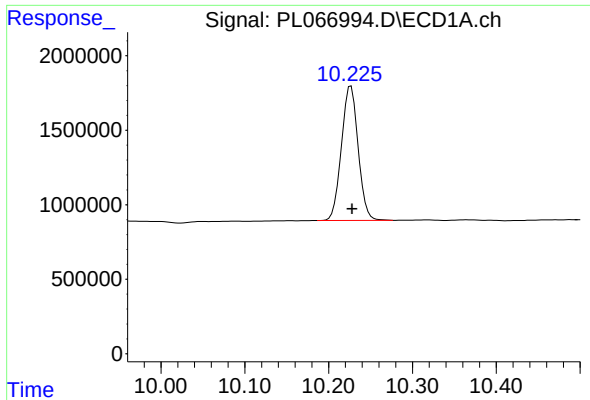

#28 Decachlorobiphenyl

R.T.: 10.227 min
Delta R.T.: -0.001 min
Response: 12492642
Conc: 19.32 ng/ml

Instrument :
ECD_L
ClientSampleId :

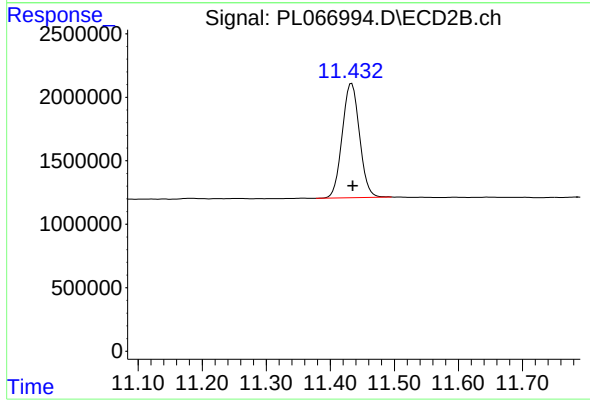

#28 Decachlorobiphenyl

R.T.: 11.433 min
Delta R.T.: -0.002 min
Response: 16863242
Conc: 20.21 ng/ml