

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060221\
 Data File : PL067008.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jun 2021 18:25
 Operator : AR\AJ
 Sample : M2574-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 NB-07-060121

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 03 04:57:32 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060121.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 02 14:20:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.480	5.529	5672843	9116048	13.853	14.092
28)	SA Decachlor...	10.225	11.429	8609424	11907665	13.314	14.272
Target Compounds							
2)	A alpha-BHC	5.181	0.000	750438	0	1.419	N.D. #
9)	A Endosulfan I	7.318	0.000	704397	0	1.340	N.D. #
10)	B gamma-Chl...	7.185	8.260	924582	357815	1.614	0.504 #
11)	B alpha-Chl...	7.253	8.342	1396231	1512024	2.428	2.128
15)	B Endosulfa...	8.180	0.000	521588	0	1.007	N.D. #
25)	Chlordane-3	7.185	8.260	924582	357815	15.871	3.418 #
26)	Chlordane-4	7.253	8.342	1396231	1512024	21.874	11.862 #
27)	Chlordane-5	8.180	0.000	521588	0	27.643	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060221\
Data File : PL067008.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jun 2021 18:25
Operator : AR\AJ
Sample : M2574-01
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
NB-07-060121

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 03 04:57:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060121.M
Quant Title : GC Extractables
QLast Update : Wed Jun 02 14:20:39 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

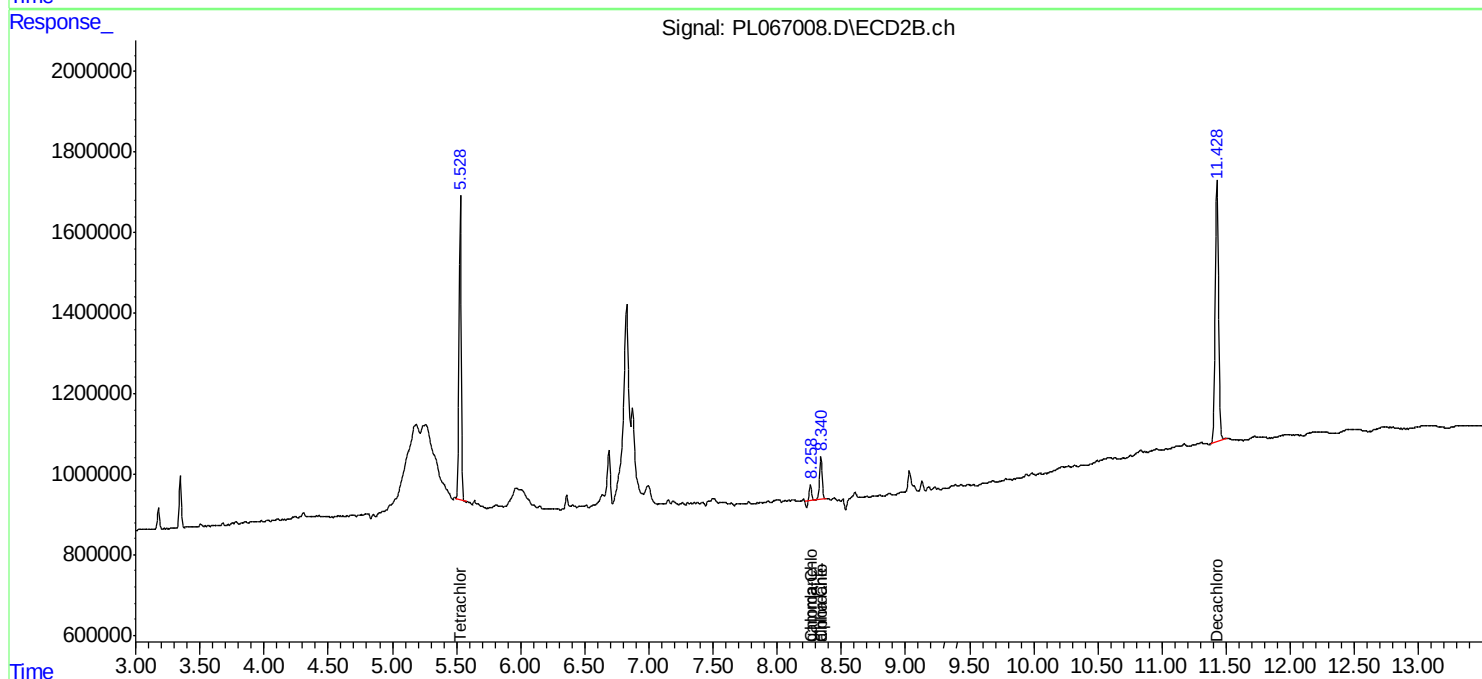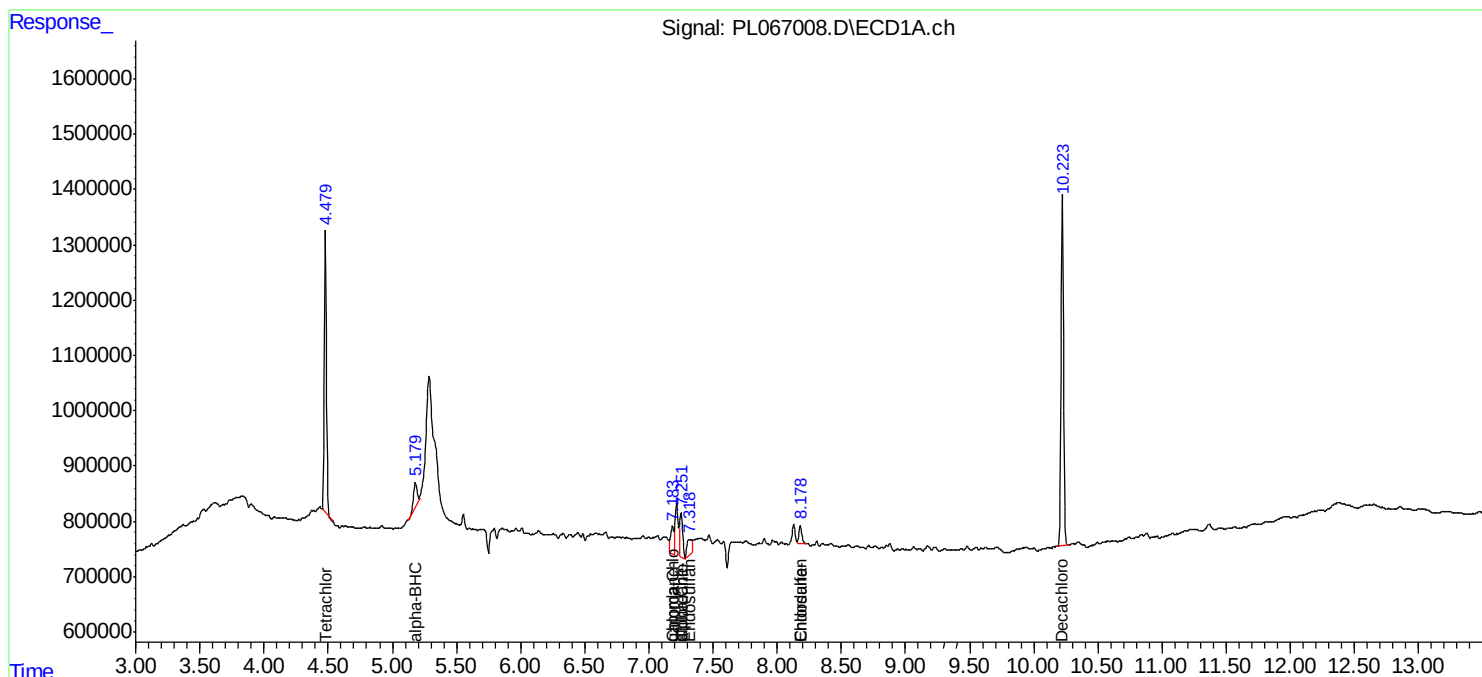


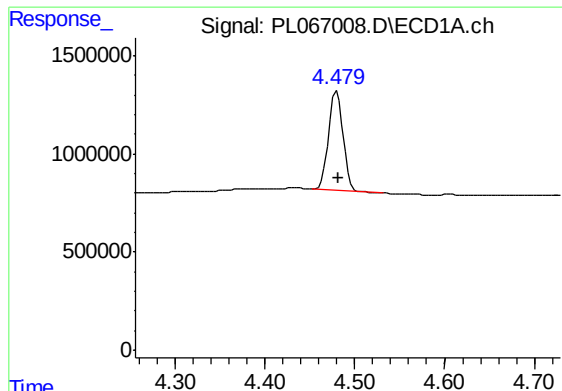

#1 Tetrachloro-m-xylene


R.T.: 4.480 min
Delta R.T.: 0.000 min
Response: 5672843
Conc: 13.85 ng/ml

Instrument :
ECD_L
ClientSampleId :
NB-07-060121

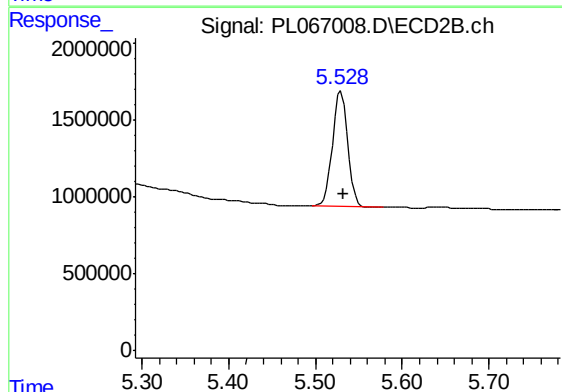


#1 Tetrachloro-m-xylene

R.T.: 5.529 min
Delta R.T.: -0.003 min
Response: 9116048
Conc: 14.09 ng/ml

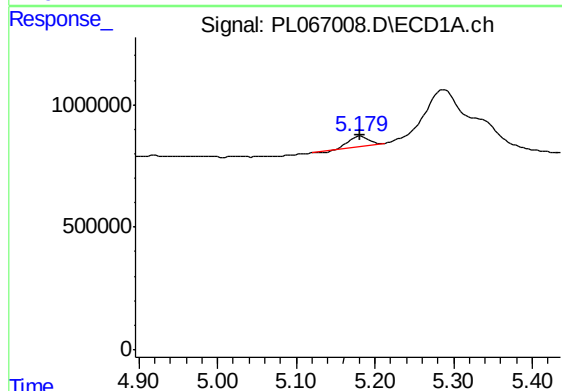


#2 alpha-BHC

R.T.: 5.181 min
Delta R.T.: 0.000 min
Response: 750438
Conc: 1.42 ng/ml

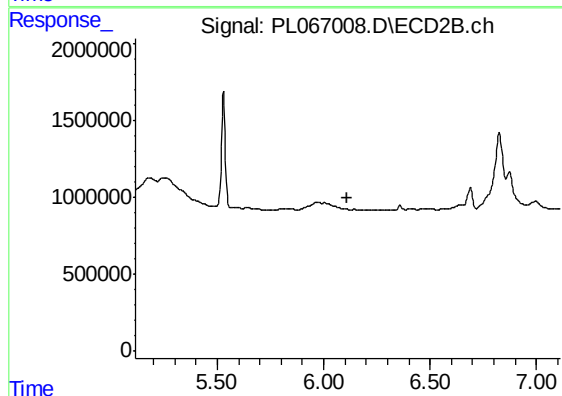

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 6.113 min
Response: 0
Conc: N.D.

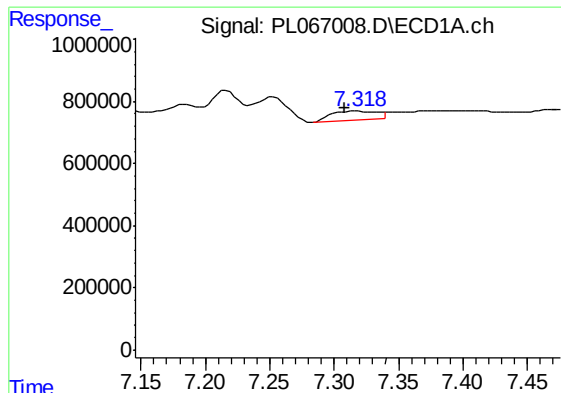

#9 Endosulfan I


R.T.: 7.318 min
Delta R.T.: 0.010 min
Response: 704397
Conc: 1.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
NB-07-060121

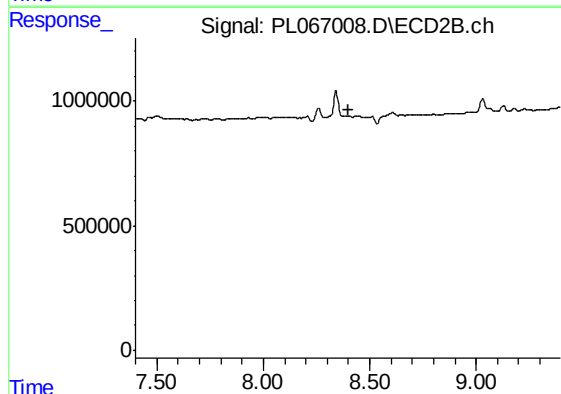


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 8.399 min
Response: 0
Conc: N.D.

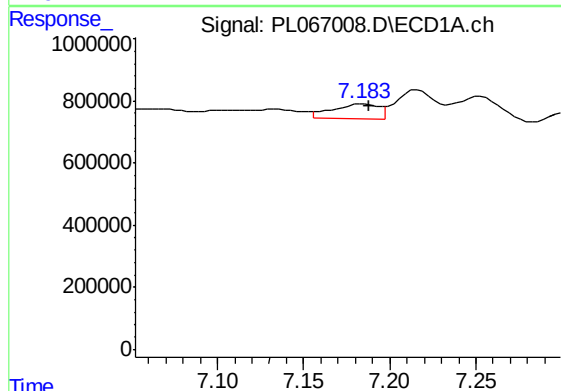


#10 gamma-Chlordane

R.T.: 7.185 min
Delta R.T.: -0.003 min
Response: 924582
Conc: 1.61 ng/ml

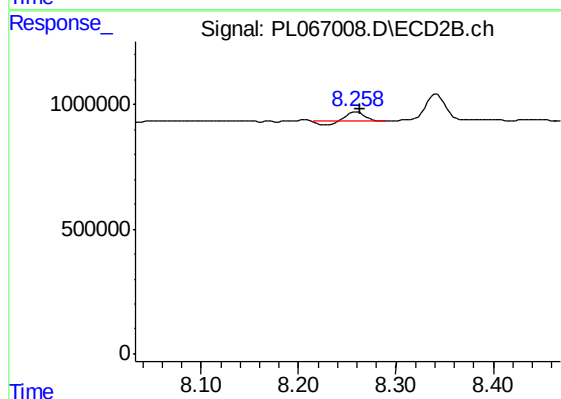

#10 gamma-Chlordane


R.T.: 8.260 min
Delta R.T.: -0.003 min
Response: 357815
Conc: 0.50 ng/ml

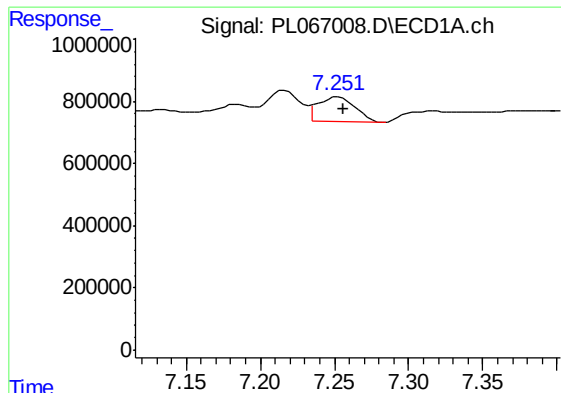

#11 alpha-Chlordane


R.T.: 7.253 min
Delta R.T.: -0.004 min
Response: 1396231
Conc: 2.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
NB-07-060121

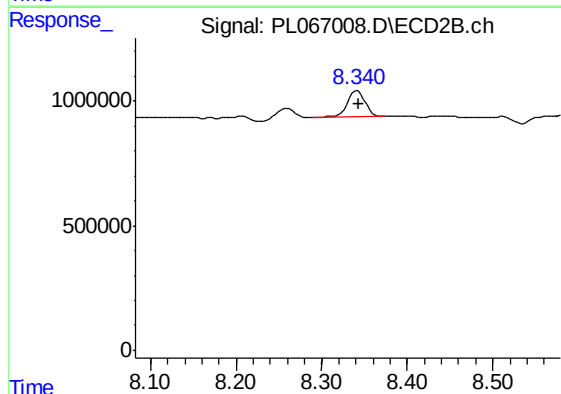


#11 alpha-Chlordane

R.T.: 8.342 min
Delta R.T.: -0.002 min
Response: 1512024
Conc: 2.13 ng/ml

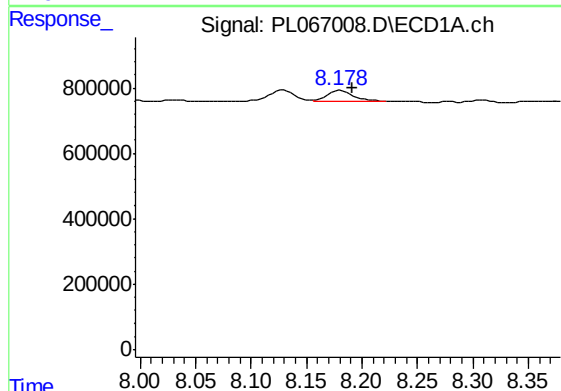


#15 Endosulfan II

R.T.: 8.180 min
Delta R.T.: -0.011 min
Response: 521588
Conc: 1.01 ng/ml

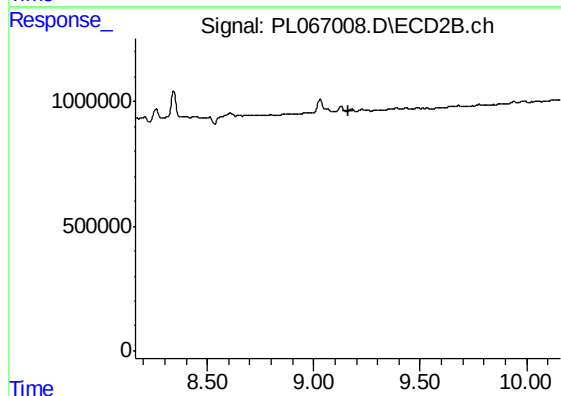

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 9.161 min
Response: 0
Conc: N.D.

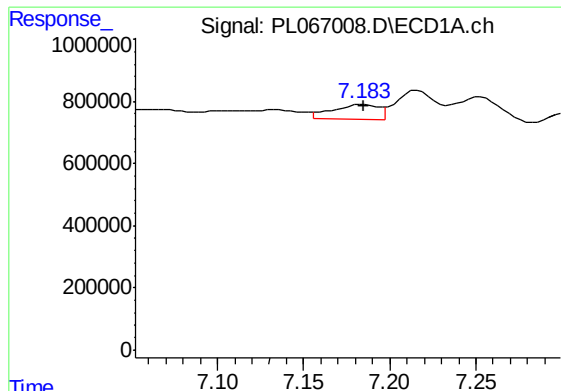

#25 Chlordane-3


R.T.: 7.185 min
Delta R.T.: 0.000 min
Response: 924582
Conc: 15.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
NB-07-060121

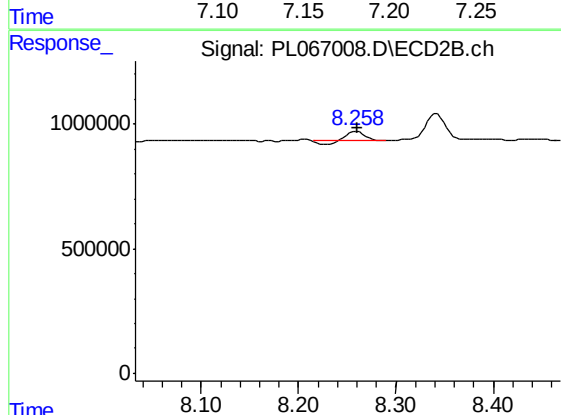


#25 Chlordane-3

R.T.: 8.260 min
Delta R.T.: 0.000 min
Response: 357815
Conc: 3.42 ng/ml

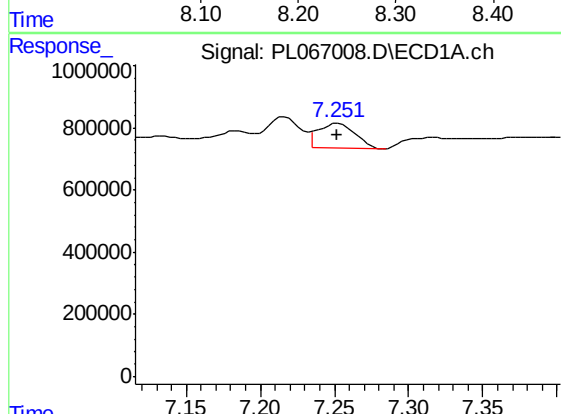


#26 Chlordane-4

R.T.: 7.253 min
Delta R.T.: 0.001 min
Response: 1396231
Conc: 21.87 ng/ml

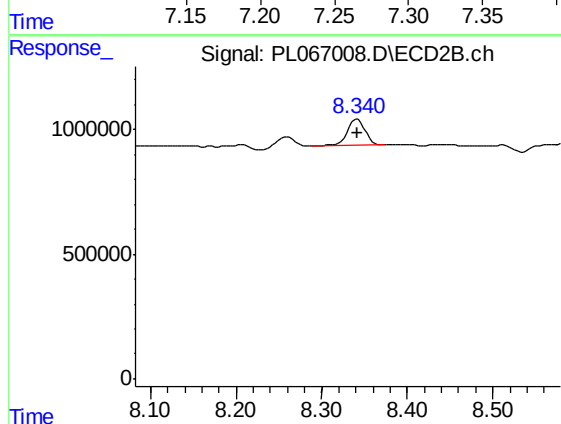

#26 Chlordane-4


R.T.: 8.342 min
Delta R.T.: 0.000 min
Response: 1512024
Conc: 11.86 ng/ml

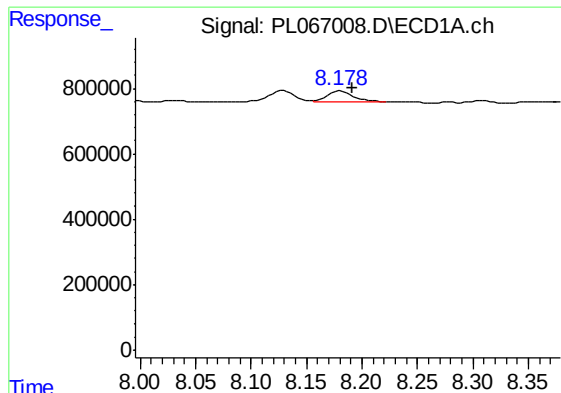

#27 Chlordane-5


R.T.: 8.180 min
Delta R.T.: -0.012 min
Response: 521588
Conc: 27.64 ng/ml

Instrument :
ECD_L
ClientSampleId :
NB-07-060121

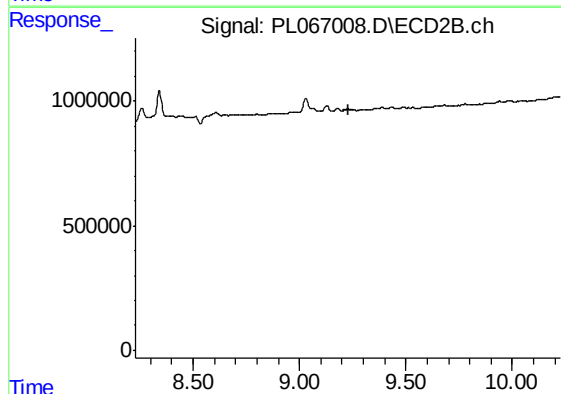


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 9.229 min
Response: 0
Conc: N.D.

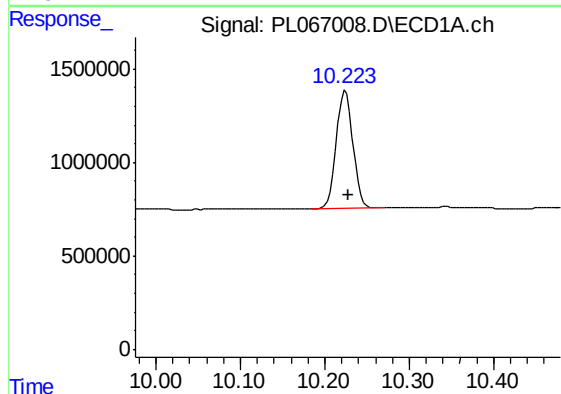

#28 Decachlorobiphenyl

R.T.: 10.225 min
Delta R.T.: -0.003 min
Response: 8609424
Conc: 13.31 ng/ml

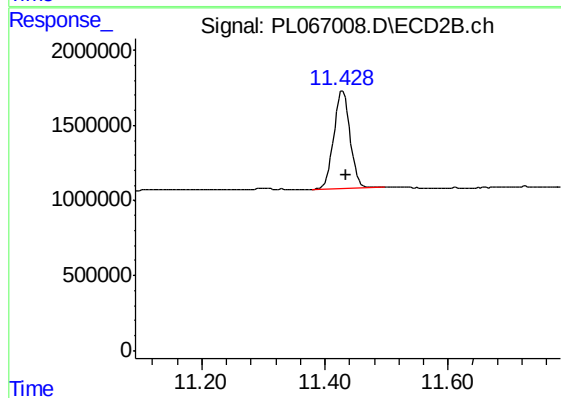

#28 Decachlorobiphenyl

R.T.: 11.429 min
Delta R.T.: -0.006 min
Response: 11907665
Conc: 14.27 ng/ml