

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060221\
 Data File : PL066995.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jun 2021 12:58
 Operator : AR\AJ
 Sample : M2565-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CL-02-052821

Manual Integrations
 APPROVED

Ankita
 6/3/2021 12:10:27 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 02 14:42:23 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060121.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 02 14:20:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.480	5.532	5864761	9214757	14.322	14.245
28) SA Decachlor...	10.227	11.433	8948284	12793484	13.838	15.333
Target Compounds						
10) B gamma-Chl...	7.183	8.259	278976	363209	0.487m	0.511m
11) B alpha-Chl...	7.252	8.344	334128	463934	0.581m	0.653

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060221\
Data File : PL066995.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jun 2021 12:58
Operator : AR\AJ
Sample : M2565-01
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
CL-02-052821


Manual Integrations
APPROVED

Ankita
6/3/2021 12:10:27 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 02 14:42:23 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060121.M
Quant Title : GC Extractables
QLast Update : Wed Jun 02 14:20:39 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

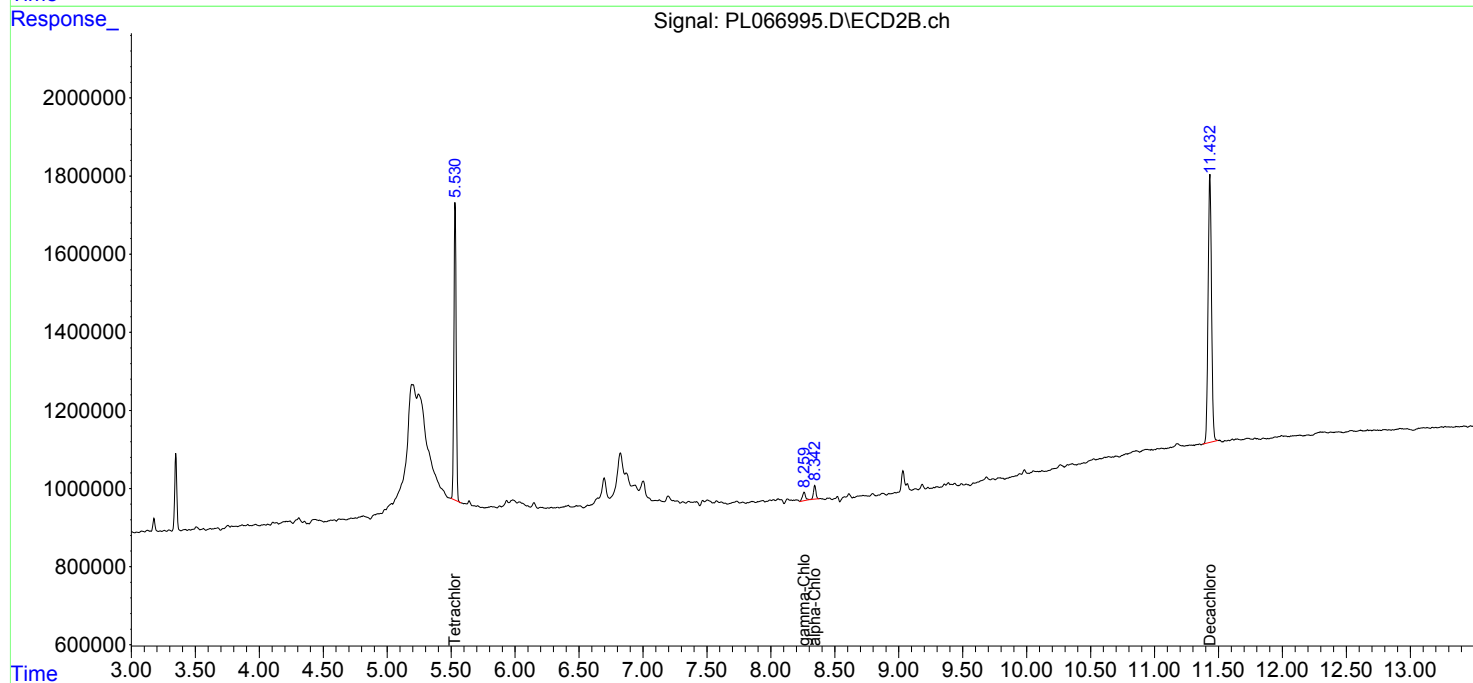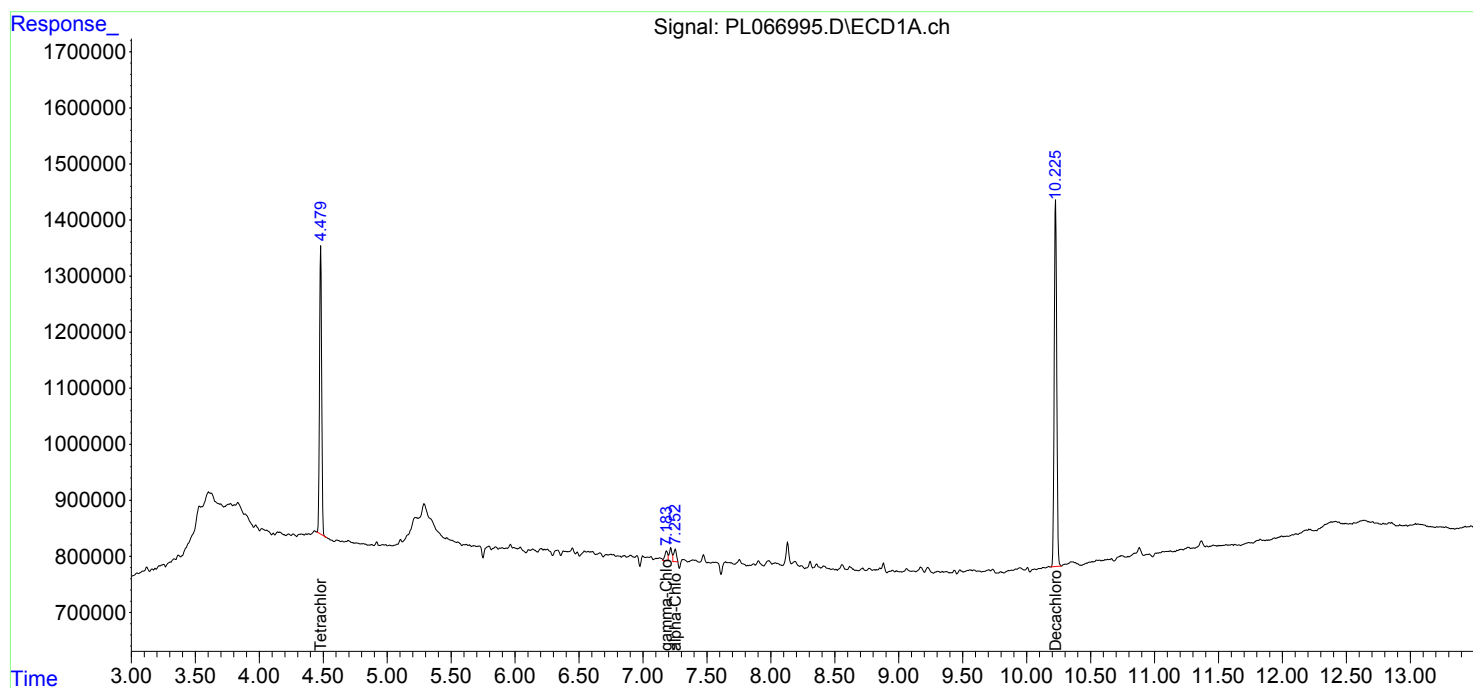

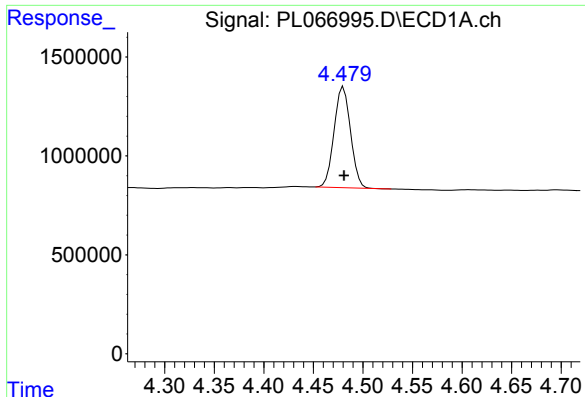


#1 Tetrachloro-m-xylene

R.T.: 4.480 min
Delta R.T.: 0.000 min
Response: 5864761
Conc: 14.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-02-052821


Manual Integrations
APPROVED

Ankita
6/3/2021 12:10:27 PM

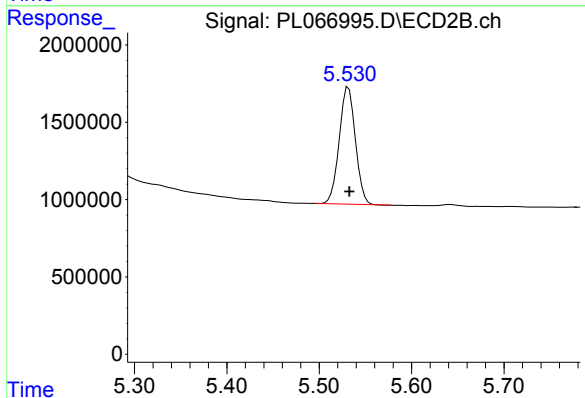


#1 Tetrachloro-m-xylene

R.T.: 5.532 min
Delta R.T.: -0.001 min
Response: 9214757
Conc: 14.24 ng/ml

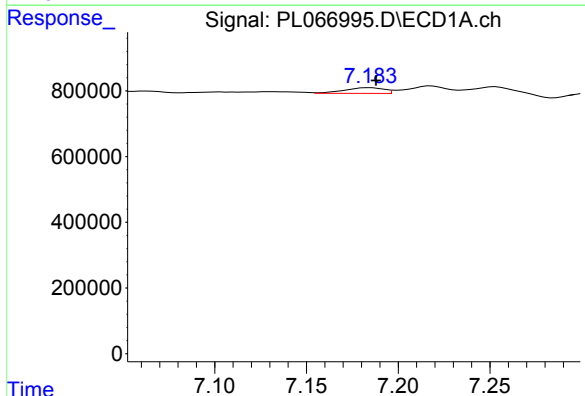


#10 gamma-Chlordane

R.T.: 7.183 min
Delta R.T.: -0.005 min
Response: 278976
Conc: 0.49 ng/ml m

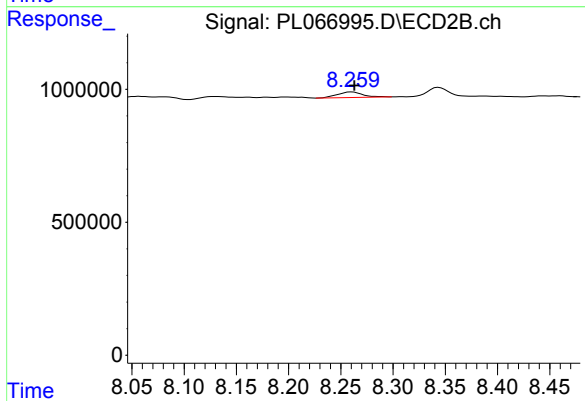

#10 gamma-Chlordane

R.T.: 8.259 min
Delta R.T.: -0.004 min
Response: 363209
Conc: 0.51 ng/ml m

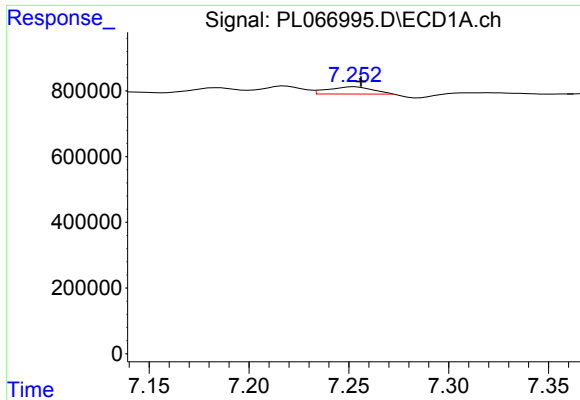


#11 alpha-Chlordane

R.T.: 7.252 min
Delta R.T.: -0.004 min
Response: 334128
Conc: 0.58 ng/ml m

Instrument :
ECD_L
ClientSampleId :
CL-02-052821


Manual Integrations
APPROVED

Ankita
6/3/2021 12:10:27 PM

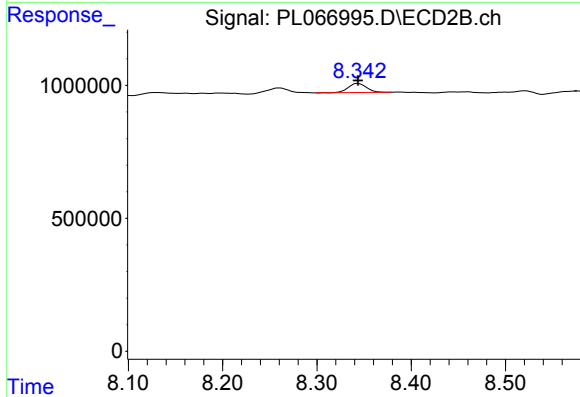


#11 alpha-Chlordane

R.T.: 8.344 min
Delta R.T.: 0.000 min
Response: 463934
Conc: 0.65 ng/ml

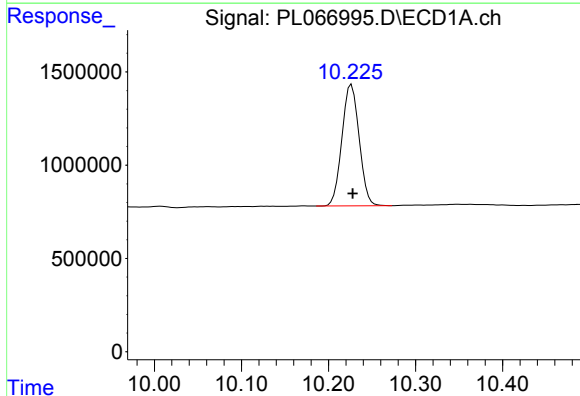

#28 Decachlorobiphenyl

R.T.: 10.227 min
Delta R.T.: -0.001 min
Response: 8948284
Conc: 13.84 ng/ml

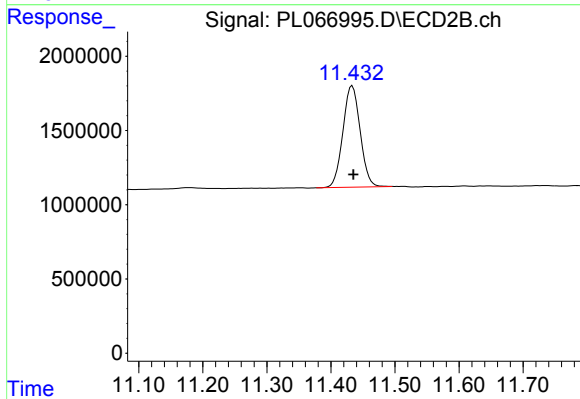

#28 Decachlorobiphenyl

R.T.: 11.433 min
Delta R.T.: -0.002 min
Response: 12793484
Conc: 15.33 ng/ml