

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060221\
 Data File : PL067008.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jun 2021 18:25
 Operator : AR\AJ
 Sample : M2574-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 NB-07-060121

Manual Integrations
 APPROVED

Ankita
 6/3/2021 12:11:17 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 03 04:57:32 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060121.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 02 14:20:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.480	5.529	5672843	9116048	13.853	14.092
28)	SA Decachlor...	10.225	11.429	8609424	11907665	13.314	14.272
Target Compounds							
10)	B gamma-Chl...	7.183	8.258	389155	504552	0.679m	0.710m
11)	B alpha-Chl...	7.251	8.342	604179	1512024	1.051m	2.128 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060221\
Data File : PL067008.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jun 2021 18:25
Operator : AR\AJ
Sample : M2574-01
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
NB-07-060121


Manual Integrations
APPROVED

Ankita
6/3/2021 12:11:17 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 03 04:57:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060121.M
Quant Title : GC Extractables
QLast Update : Wed Jun 02 14:20:39 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

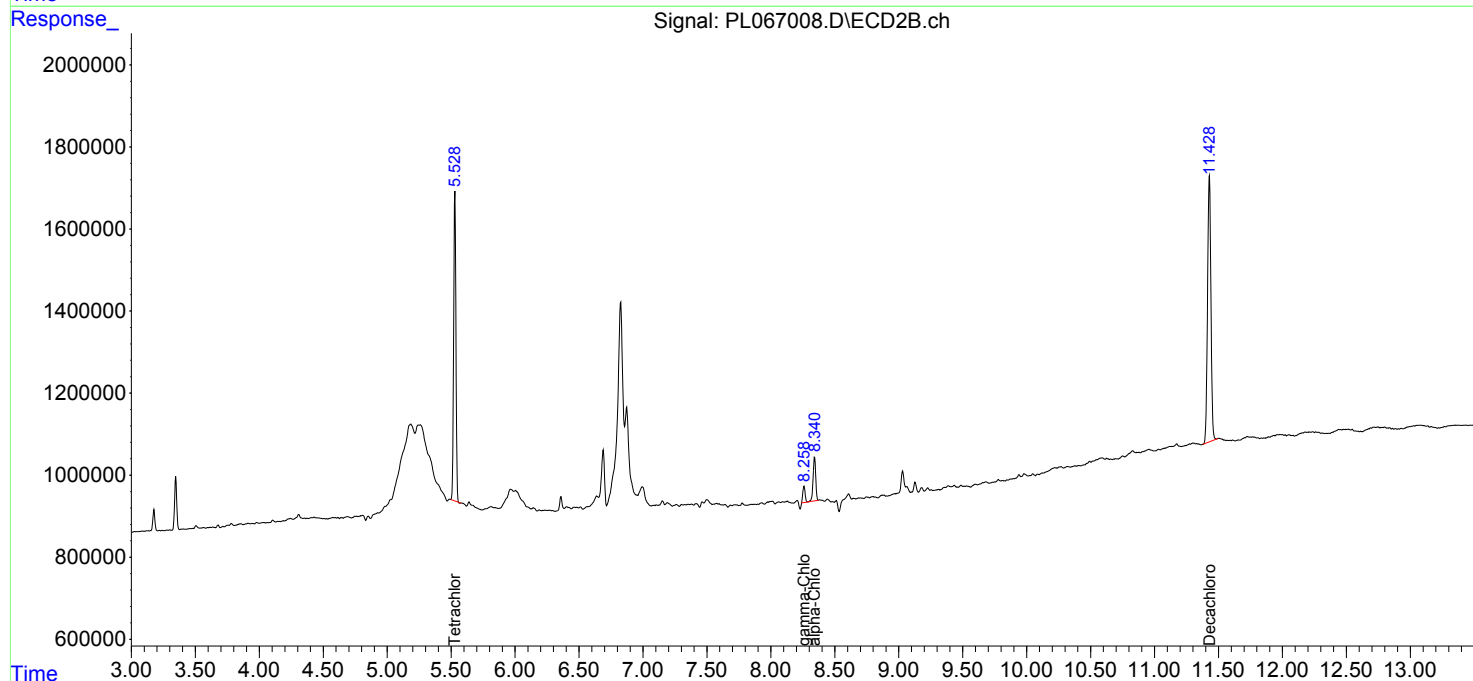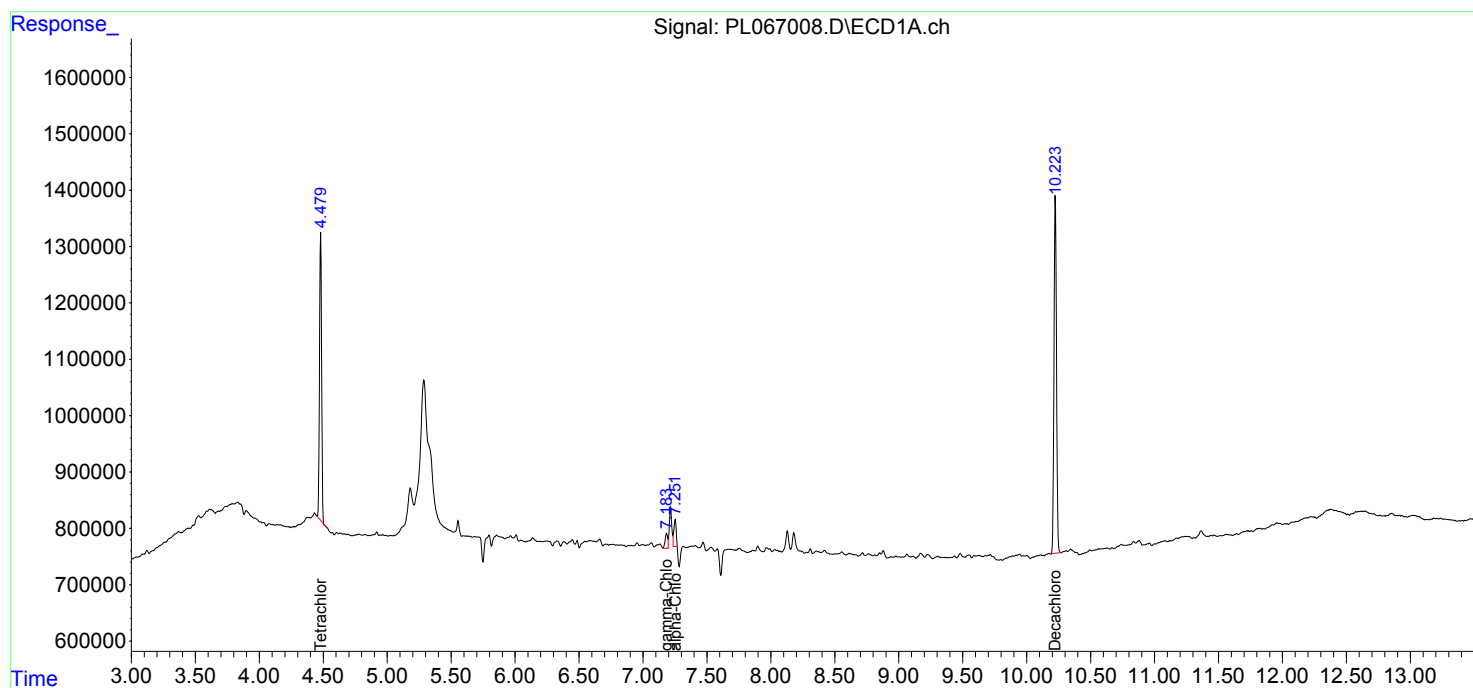

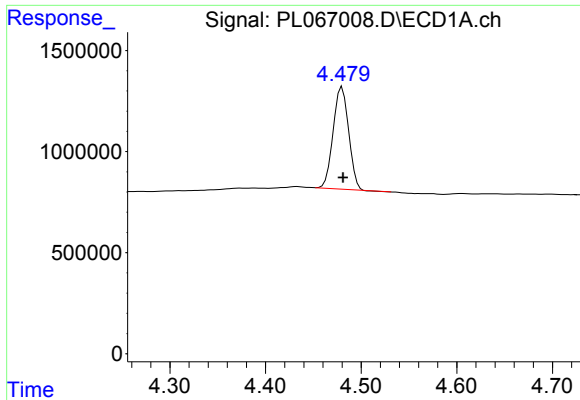


#1 Tetrachloro-m-xylene

R.T.: 4.480 min
Delta R.T.: 0.000 min
Response: 5672843
Conc: 13.85 ng/ml

Instrument :
ECD_L
ClientSampleId :
NB-07-060121


Manual Integrations
APPROVED

Ankita
6/3/2021 12:11:17 PM

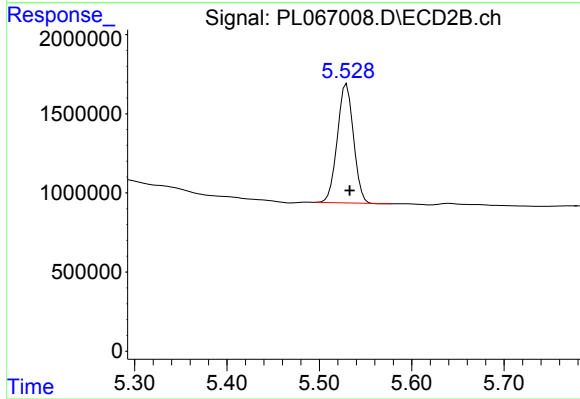


#1 Tetrachloro-m-xylene

R.T.: 5.529 min
Delta R.T.: -0.003 min
Response: 9116048
Conc: 14.09 ng/ml

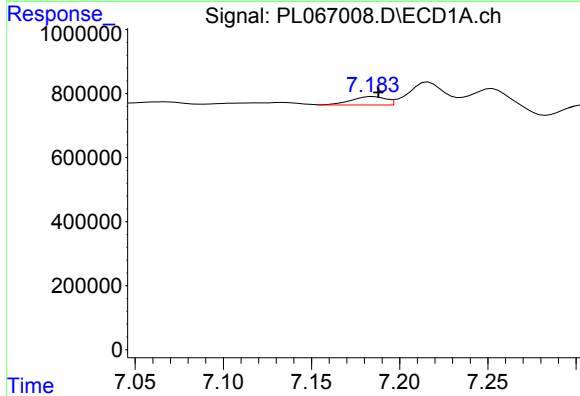


#10 gamma-Chlordane

R.T.: 7.183 min
Delta R.T.: -0.005 min
Response: 389155
Conc: 0.68 ng/ml m

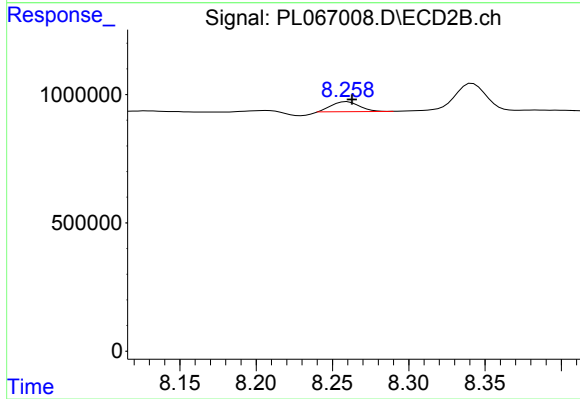

#10 gamma-Chlordane

R.T.: 8.258 min
Delta R.T.: -0.005 min
Response: 504552
Conc: 0.71 ng/ml m

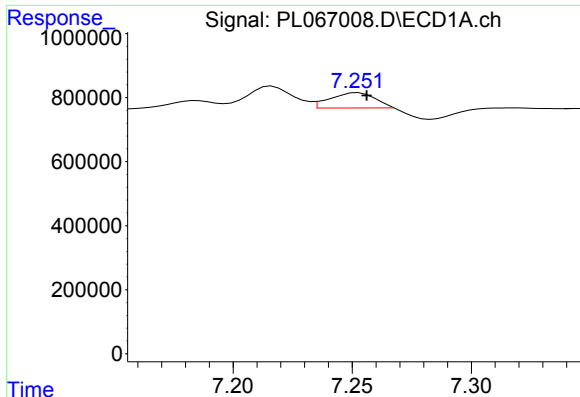


#11 alpha-Chlordane

R.T.: 7.251 min
Delta R.T.: -0.005 min
Response: 604179
Conc: 1.05 ng/ml m

Instrument :
ECD_L
ClientSampleId :
NB-07-060121


Manual Integrations
APPROVED

Ankita
6/3/2021 12:11:17 PM

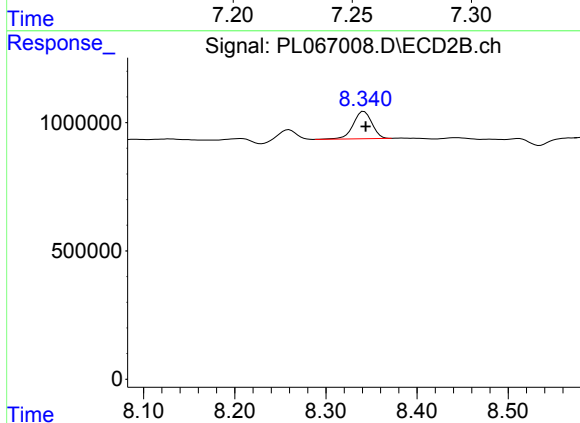


#11 alpha-Chlordane

R.T.: 8.342 min
Delta R.T.: -0.002 min
Response: 1512024
Conc: 2.13 ng/ml

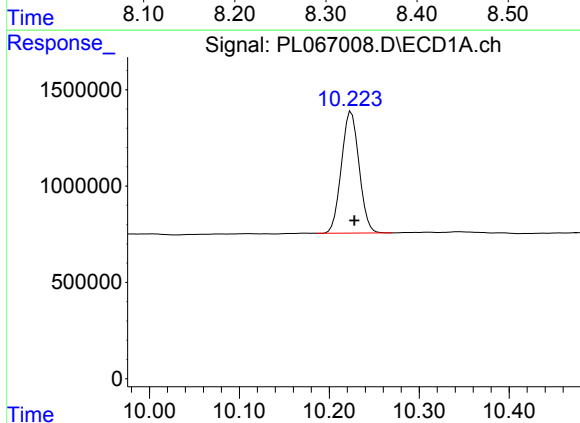

#28 Decachlorobiphenyl

R.T.: 10.225 min
Delta R.T.: -0.003 min
Response: 8609424
Conc: 13.31 ng/ml

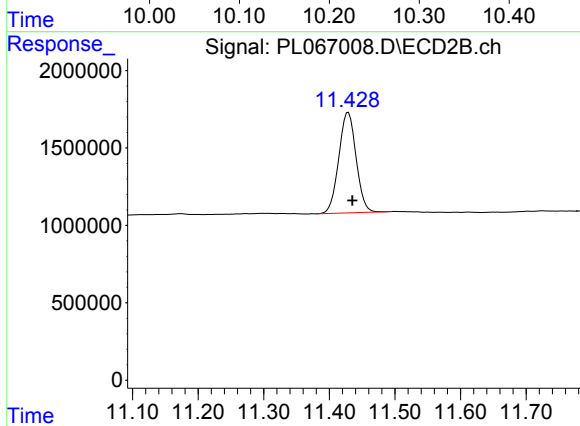

#28 Decachlorobiphenyl

R.T.: 11.429 min
Delta R.T.: -0.006 min
Response: 11907665
Conc: 14.27 ng/ml