

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060221\
 Data File : PL067027.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jun 2021 02:33
 Operator : AR\AJ
 Sample : M2580-07 10X
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 18-B3(0-2)

Manual Integrations
 APPROVED

Ankita
 6/3/2021 12:10:58 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 03 05:05:30 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060121.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 02 14:20:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.478	5.529	923112	1170896	2.254	1.810
28) SA Decachlor...	10.222	11.428	1274466	1617444	1.971	1.939
Target Compounds						
11) B alpha-Chl...	7.243	8.341	909225	862251	1.581m	1.214
12) B 4,4'-DDE	7.469	8.525	1486636	2882707	2.784	4.410 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060221\
Data File : PL067027.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jun 2021 02:33
Operator : AR\AJ
Sample : M2580-07 10X
Misc :
ALS Vial : 36 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
18-B3(0-2)


Manual Integrations
APPROVED

Ankita
6/3/2021 12:10:58 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 03 05:05:30 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060121.M
Quant Title : GC Extractables
QLast Update : Wed Jun 02 14:20:39 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

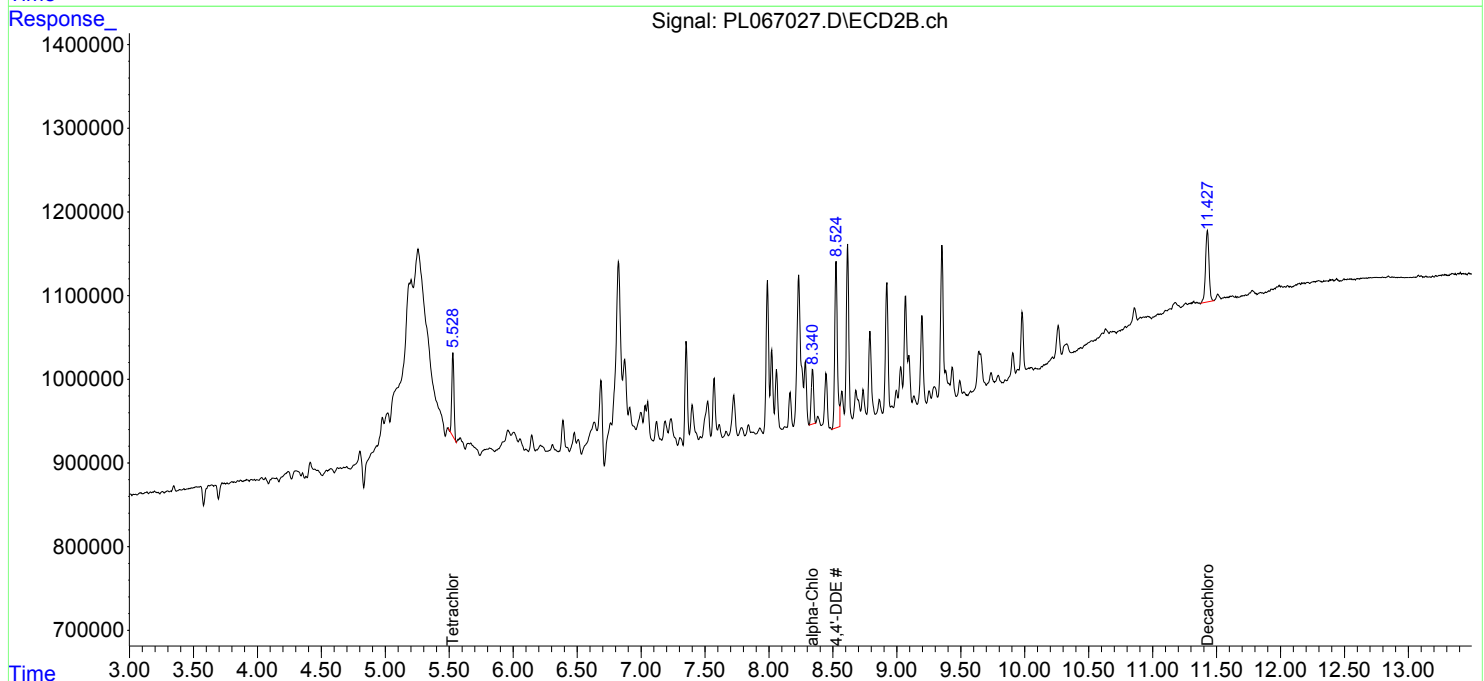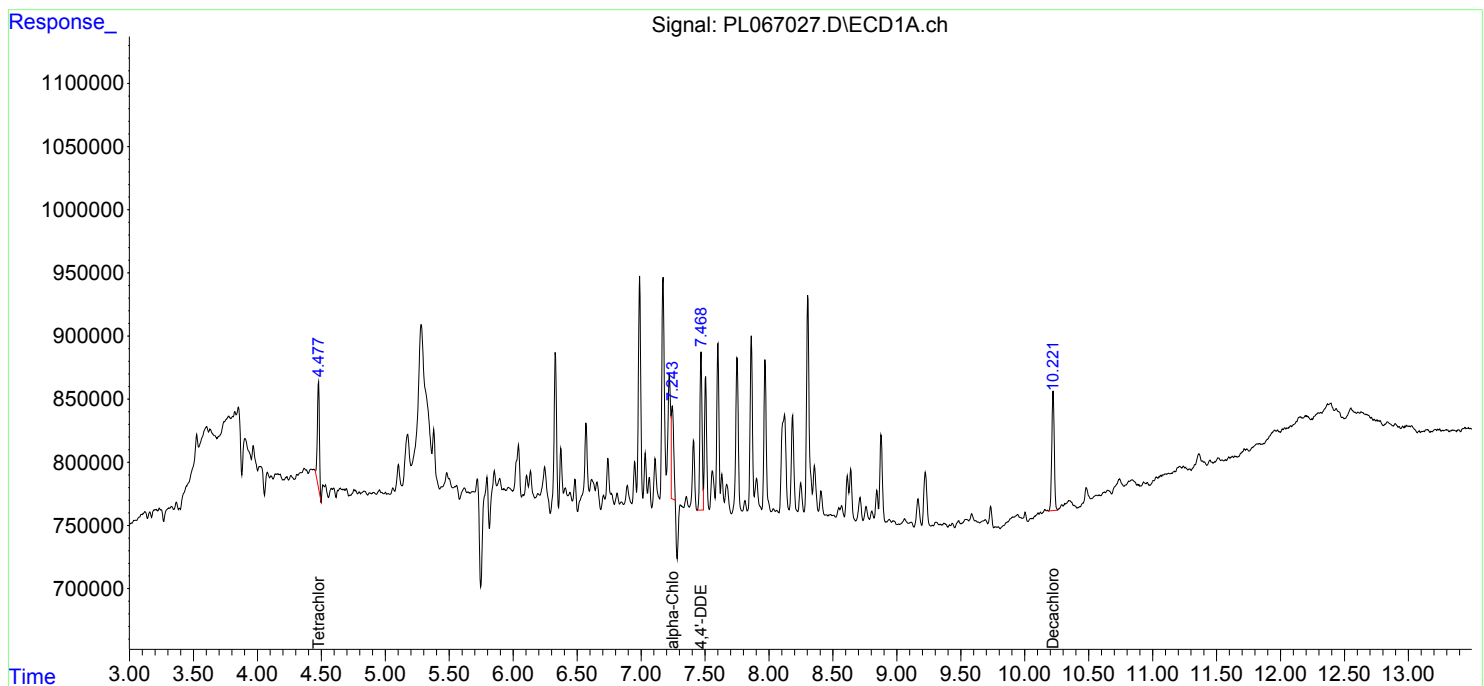

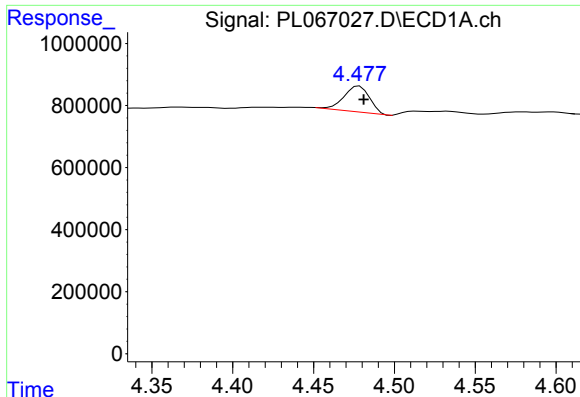


#1 Tetrachloro-m-xylene

R.T.: 4.478 min
Delta R.T.: -0.003 min
Response: 923112
Conc: 2.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
18-B3(0-2)


Manual Integrations
APPROVED

Ankita
6/3/2021 12:10:58 PM

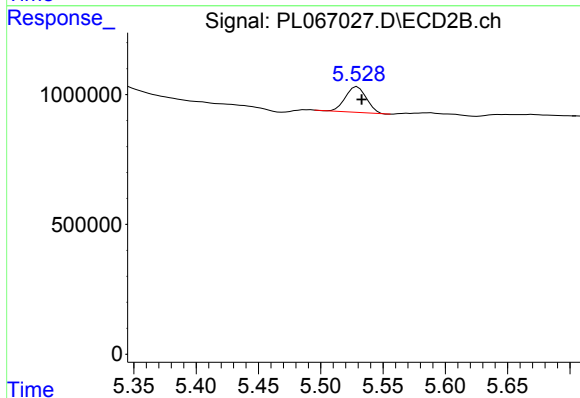


#1 Tetrachloro-m-xylene

R.T.: 5.529 min
Delta R.T.: -0.004 min
Response: 1170896
Conc: 1.81 ng/ml

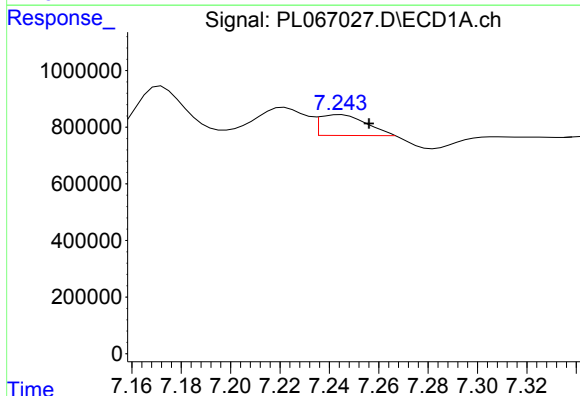


#11 alpha-Chlordane

R.T.: 7.243 min
Delta R.T.: -0.013 min
Response: 909225
Conc: 1.58 ng/ml m

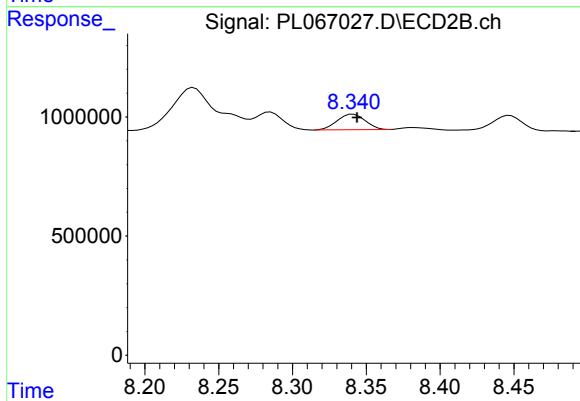

#11 alpha-Chlordane

R.T.: 8.341 min
Delta R.T.: -0.003 min
Response: 862251
Conc: 1.21 ng/ml

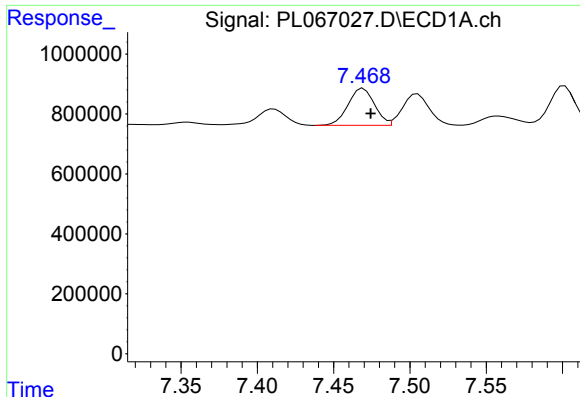


#12 4,4'-DDE

R.T.: 7.469 min
Delta R.T.: -0.005 min
Response: 1486636
Conc: 2.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
18-B3(0-2)


Manual Integrations
APPROVED

Ankita
6/3/2021 12:10:58 PM

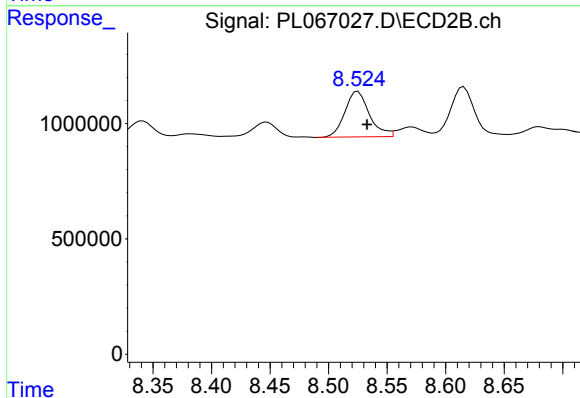


#12 4,4'-DDE

R.T.: 8.525 min
Delta R.T.: -0.008 min
Response: 2882707
Conc: 4.41 ng/ml

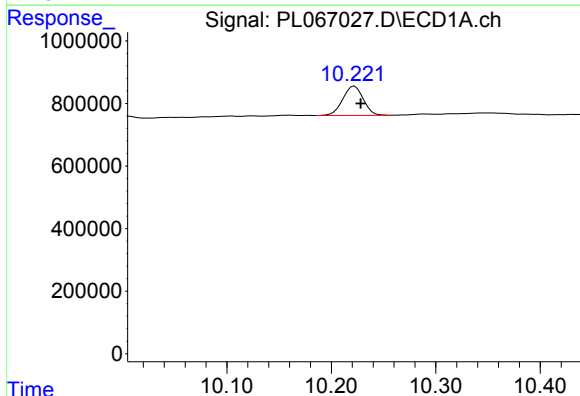

#28 Decachlorobiphenyl

R.T.: 10.222 min
Delta R.T.: -0.006 min
Response: 1274466
Conc: 1.97 ng/ml

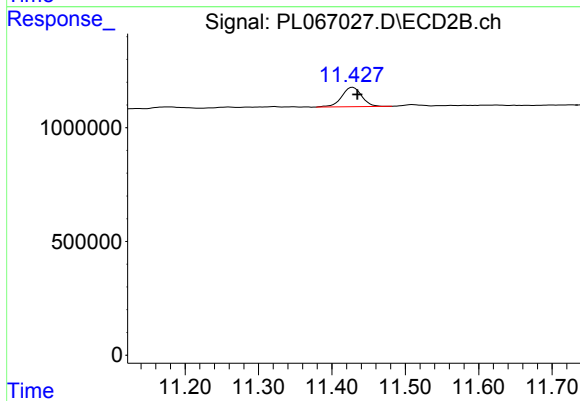

#28 Decachlorobiphenyl

R.T.: 11.428 min
Delta R.T.: -0.007 min
Response: 1617444
Conc: 1.94 ng/ml