

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060222\
 Data File : PL075371.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jun 2022 10:44
 Operator : AR\AJ
 Sample : N3099-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 03 06:01:04 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 01 10:19:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	5.649	4.644	9922779	23268257	16.883	14.688
28)	SA Decachlor...	11.645	10.392	7621346	16811547	14.214	12.251
Target Compounds							
2)	A alpha-BHC	6.211	0.000	89295	0	0.108	N.D. #
5)	MB Aldrin	7.682f	6.499	55426944	723936	76.009	0.375 #
7)	B delta-BHC	7.158	0.000	195041	0	0.254	N.D. #
9)	A Endosulfan I	0.000	7.474	0	1416685	N.D.	0.838 #
10)	B gamma-Chl...	0.000	7.354	0	6053203	N.D.	3.291 #
11)	B alpha-Chl...	0.000	7.414	0	2082123	N.D.	1.139 #
15)	B Endosulfa...	9.309	0.000	464220	0	0.822	N.D. #
17)	MA 4,4'-DDT	0.000	8.470	0	130573	N.D.	0.091 #
21)	B Endrin ke...	10.189f	0.000	840511	0	1.369	N.D. #
23)	Chlordane-1	0.000	5.966	0	342409	N.D.	6.150 #
25)	Chlordane-3	0.000	7.354	0	6053203	N.D.	34.294 #
26)	Chlordane-4	0.000	7.414	0	2082123	N.D.	11.022 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060222\
Data File : PL075371.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jun 2022 10:44
Operator : AR\AJ
Sample : N3099-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 03 06:01:04 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
Quant Title : GC Extractables
QLast Update : Wed Jun 01 10:19:11 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

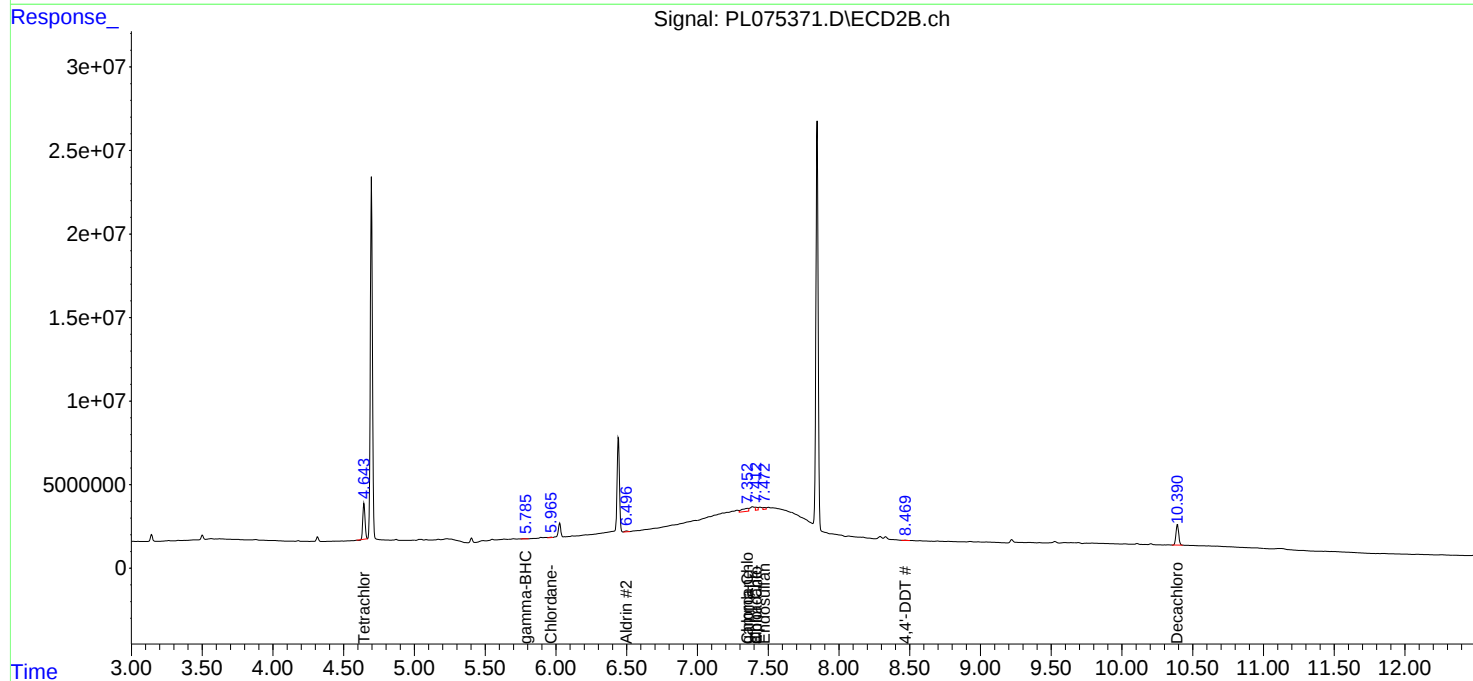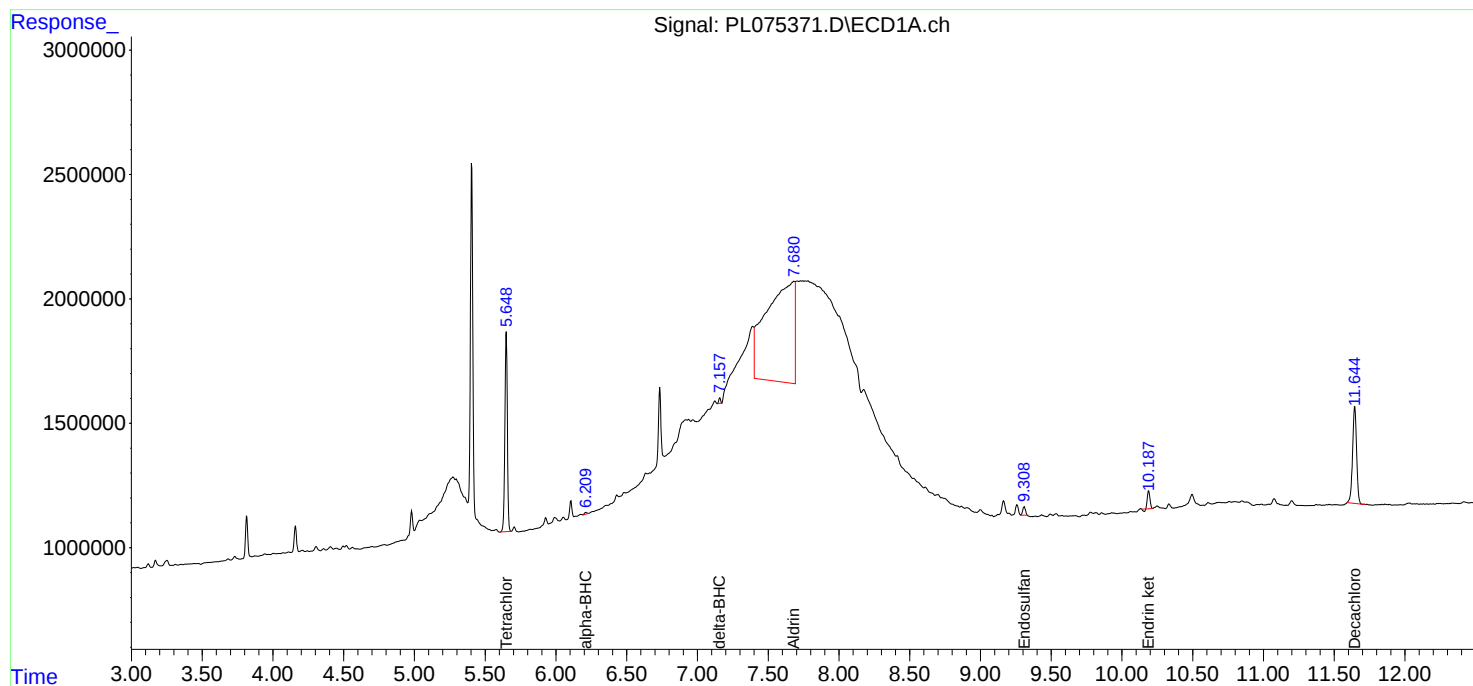

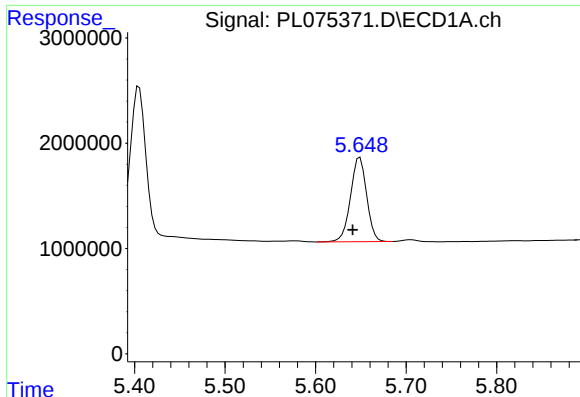


#1 Tetrachloro-m-xylene

R.T.: 5.649 min
Delta R.T.: 0.008 min
Response: 9922779
Conc: 16.88 ng/ml

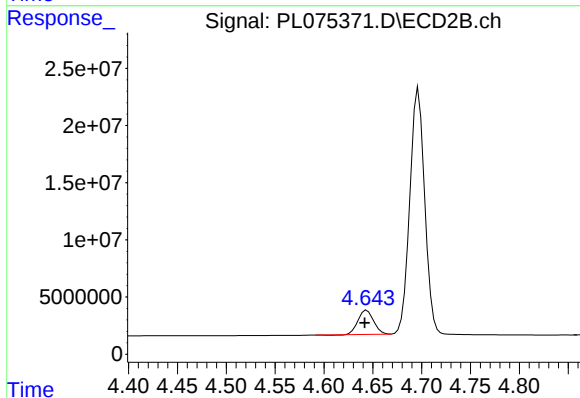


#1 Tetrachloro-m-xylene

R.T.: 4.644 min
Delta R.T.: 0.002 min
Response: 23268257
Conc: 14.69 ng/ml

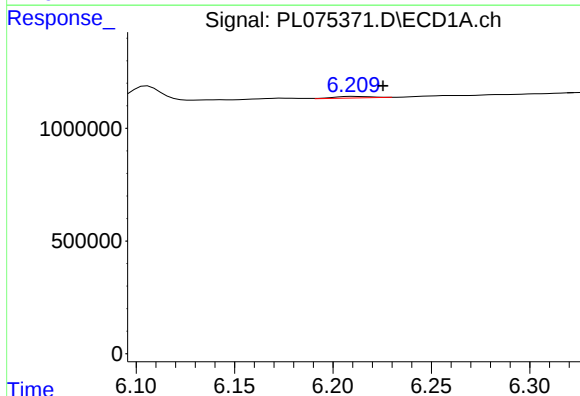


#2 alpha-BHC

R.T.: 6.211 min
Delta R.T.: -0.015 min
Response: 89295
Conc: 0.11 ng/ml

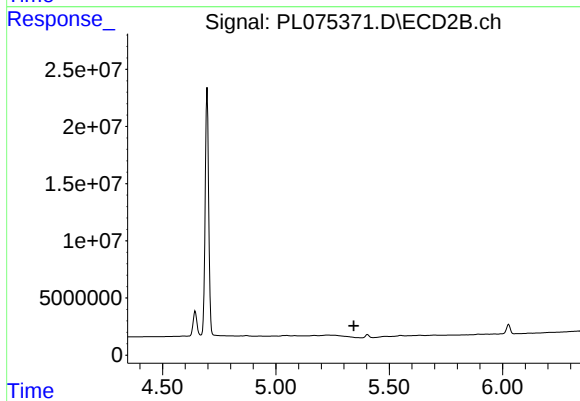


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T.: 5.344 min
Response: 0
Conc: N.D.

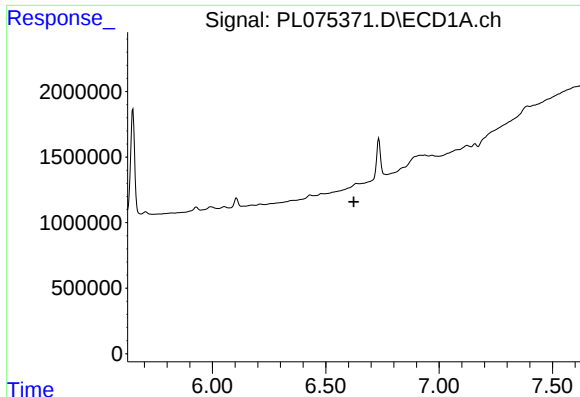


#3 gamma-BHC (Lindane)

R.T.: 6.635 min
Delta R.T.: 0.012 min
Response: -509676
Conc: N.D.

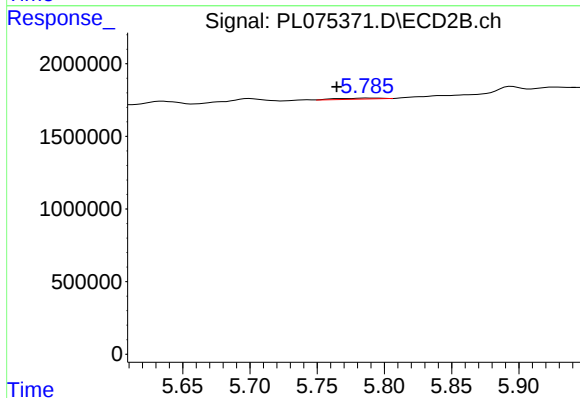


#3 gamma-BHC (Lindane)

R.T.: 5.787 min
Delta R.T.: 0.022 min
Response: 158388
Conc: 0.08 ng/ml

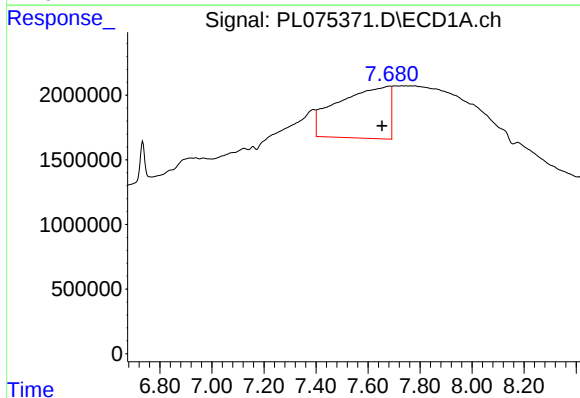


#5 Aldrin

R.T.: 7.682 min
Delta R.T.: 0.028 min
Response: 55426944
Conc: 76.01 ng/ml

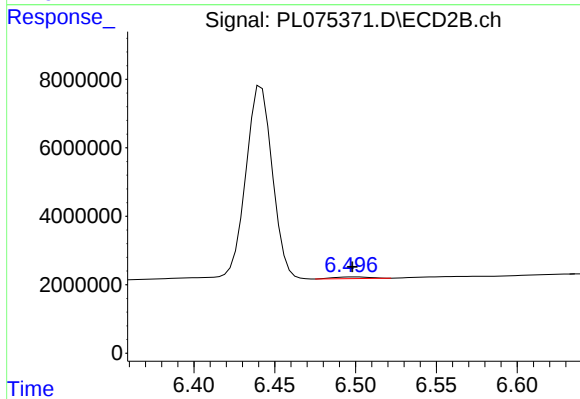


#5 Aldrin

R.T.: 6.499 min
Delta R.T.: 0.000 min
Response: 723936
Conc: 0.38 ng/ml

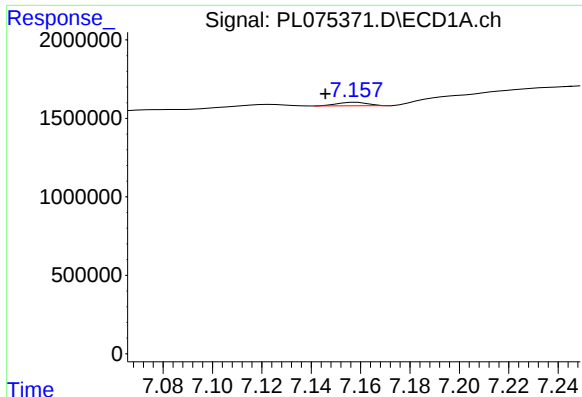


#7 delta-BHC

R.T.: 7.158 min
Delta R.T.: 0.013 min
Response: 195041
Conc: 0.25 ng/ml

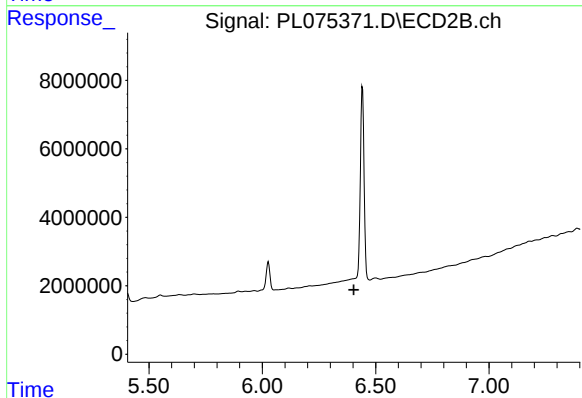


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.403 min
Response: 0
Conc: N.D.

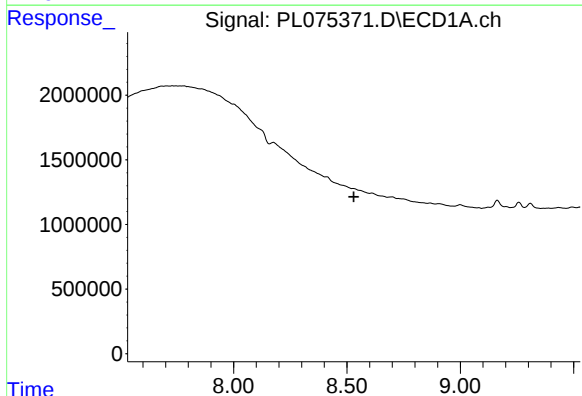


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 8.530 min
Response: 0
Conc: N.D.

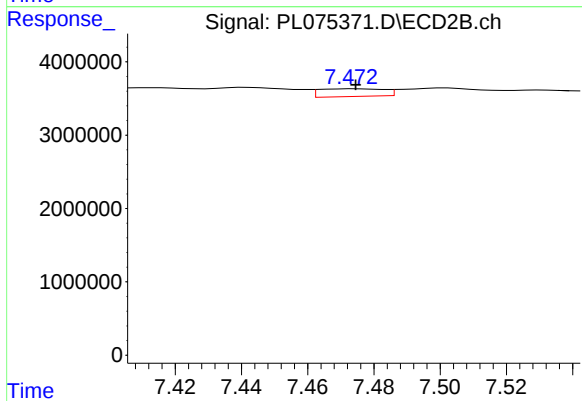


#9 Endosulfan I

R.T.: 7.474 min
Delta R.T.: 0.000 min
Response: 1416685
Conc: 0.84 ng/ml

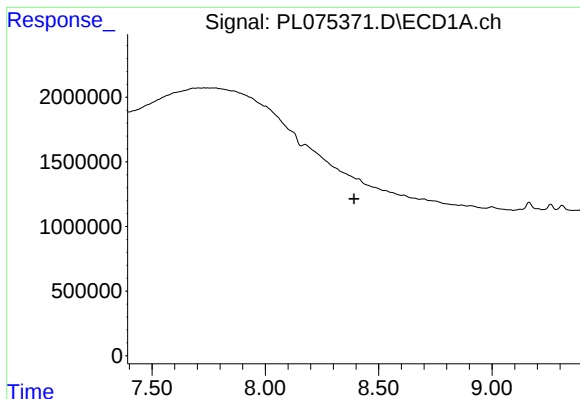


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 8.392 min
Response: 0
Conc: N.D.

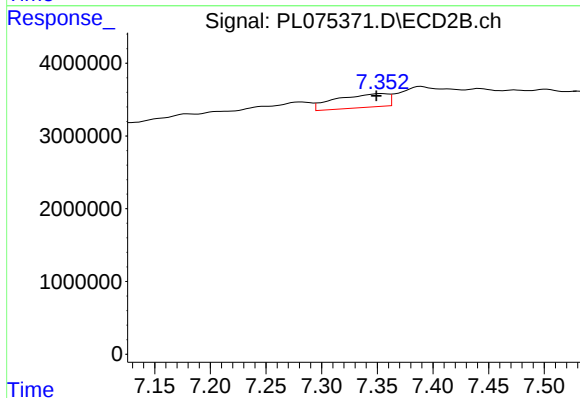


#10 gamma-Chlordane

R.T.: 7.354 min
Delta R.T.: 0.005 min
Response: 6053203
Conc: 3.29 ng/ml

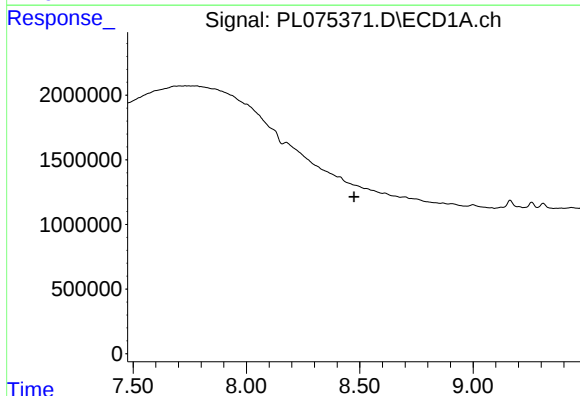


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 8.474 min
Response: 0
Conc: N.D.

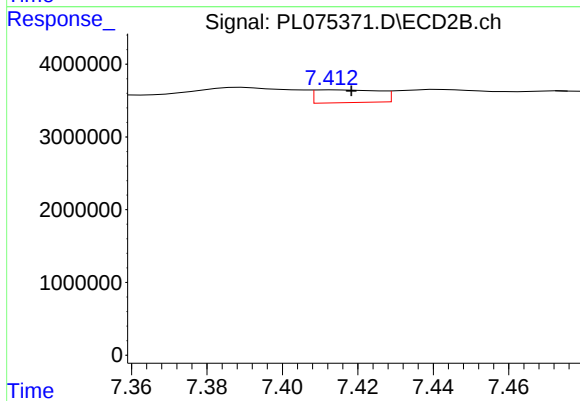


#11 alpha-Chlordane

R.T.: 7.414 min
Delta R.T.: -0.005 min
Response: 2082123
Conc: 1.14 ng/ml

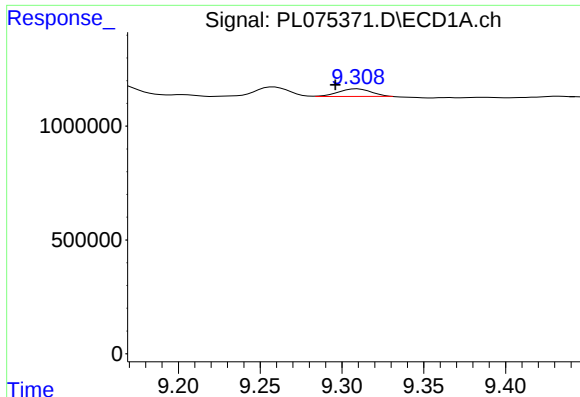


#15 Endosulfan II

R.T.: 9.309 min
Delta R.T.: 0.013 min
Response: 464220
Conc: 0.82 ng/ml

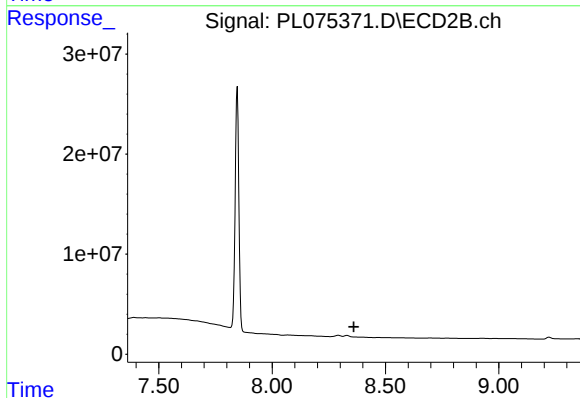


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.361 min
Response: 0
Conc: N.D.

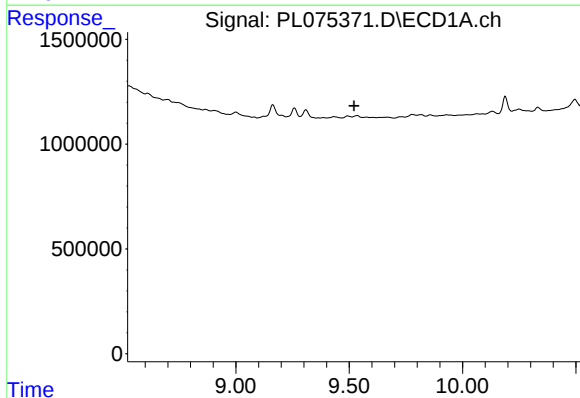


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 9.522 min
Response: 0
Conc: N.D.

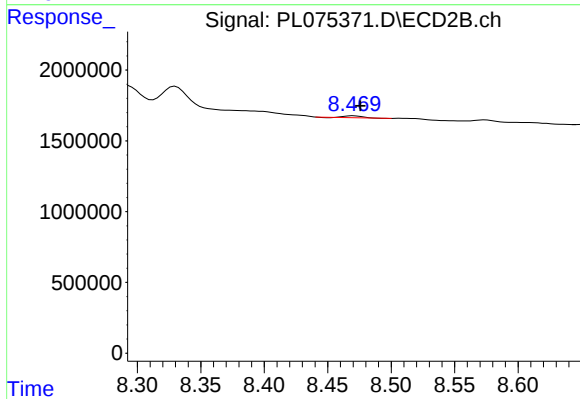


#17 4,4'-DDT

R.T.: 8.470 min
Delta R.T.: -0.005 min
Response: 130573
Conc: 0.09 ng/ml

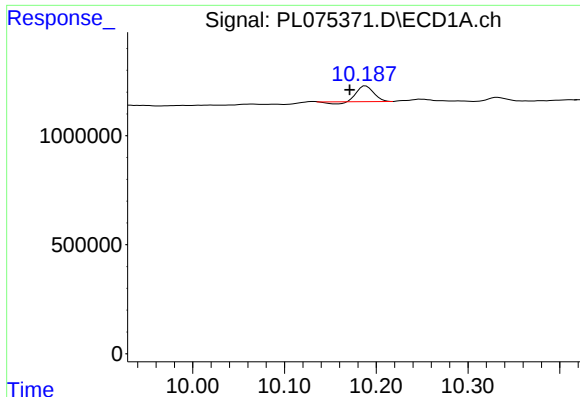


#21 Endrin ketone

R.T.: 10.189 min
Delta R.T.: 0.017 min
Response: 840511
Conc: 1.37 ng/ml

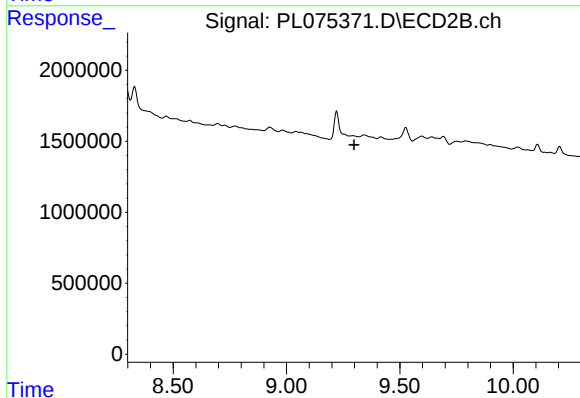


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.298 min
Response: 0
Conc: N.D.

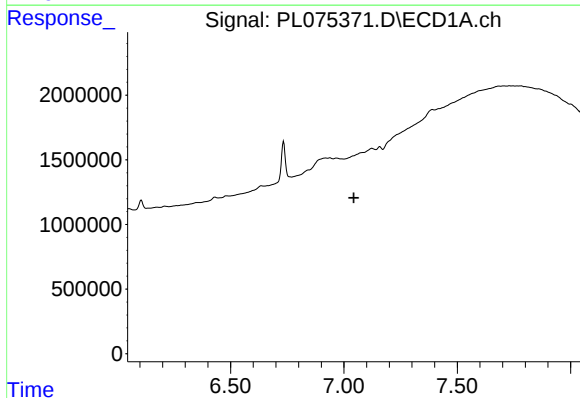


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 7.044 min
Response: 0
Conc: N.D.

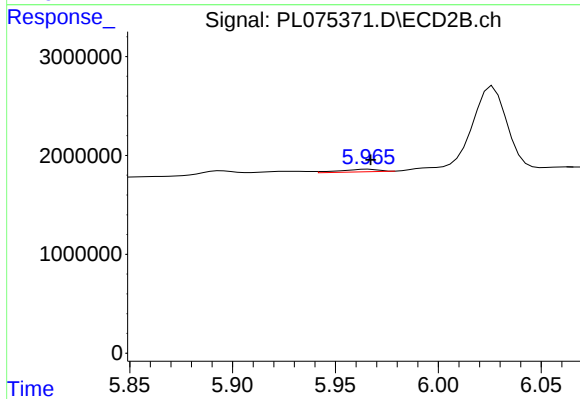


#23 Chlordane-1

R.T.: 5.966 min
Delta R.T.: -0.001 min
Response: 342409
Conc: 6.15 ng/ml

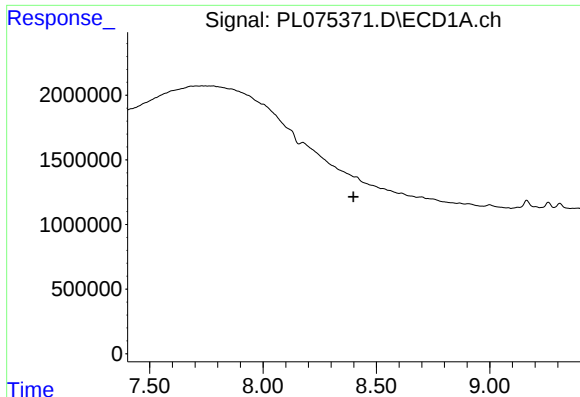


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 8.399 min
Response: 0
Conc: N.D.

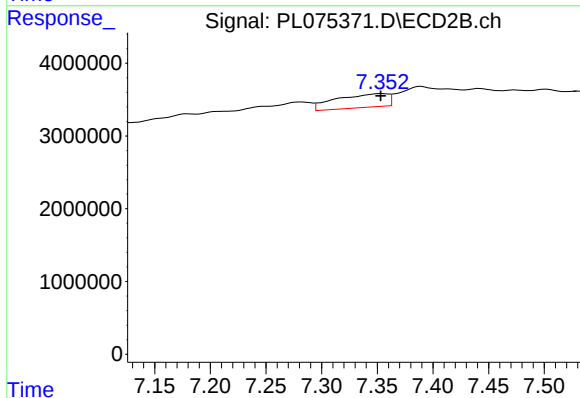


#25 Chlordane-3

R.T.: 7.354 min
Delta R.T.: 0.001 min
Response: 6053203
Conc: 34.29 ng/ml

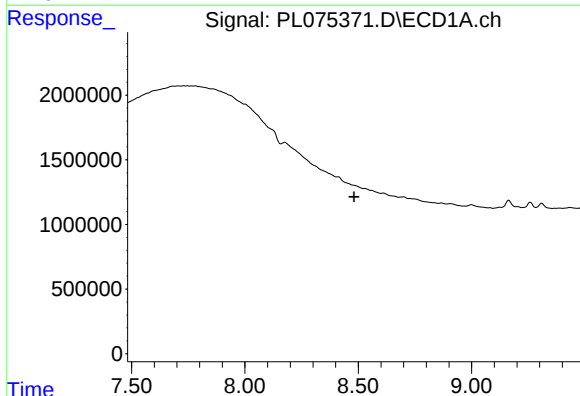


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 8.482 min
Response: 0
Conc: N.D.

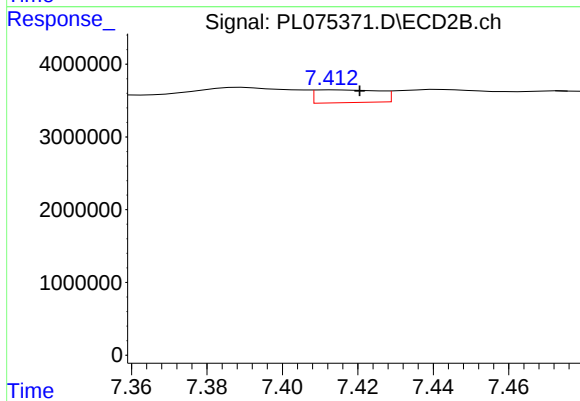


#26 Chlordane-4

R.T.: 7.414 min
Delta R.T.: -0.007 min
Response: 2082123
Conc: 11.02 ng/ml

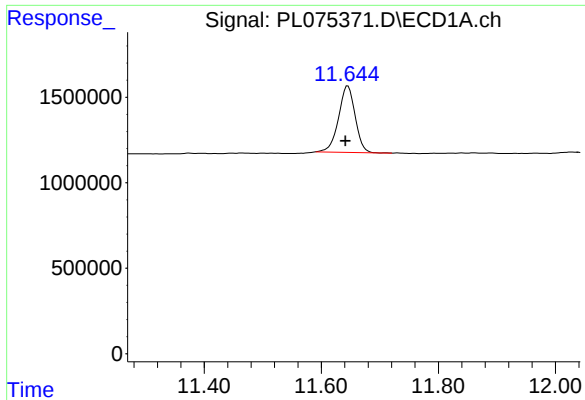

#28 Decachlorobiphenyl

R.T.: 11.645 min
Delta R.T.: 0.004 min
Response: 7621346
Conc: 14.21 ng/ml

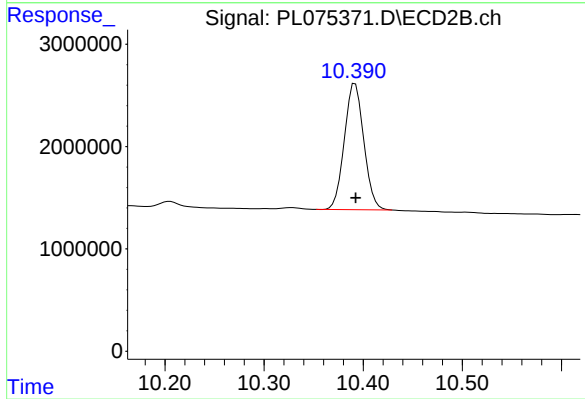

#28 Decachlorobiphenyl

R.T.: 10.392 min
Delta R.T.: 0.000 min
Response: 16811547
Conc: 12.25 ng/ml