

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060222\
 Data File : PL075372.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jun 2022 11:01
 Operator : AR\AJ
 Sample : N3099-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 03 06:01:18 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 01 10:19:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	5.644	4.644	9376631	23005330	15.954	14.522
28)	SA Decachlor...	11.642	10.389	6506313	14862881	12.135	10.831
Target Compounds							
2)	A alpha-BHC	6.205f	0.000	108189	0	0.131	N.D. #
3)	MA gamma-BHC...	6.627	0.000	61588	0	0.079	N.D. #
5)	MB Aldrin	0.000	6.496	0	629827	N.D.	0.326 #
9)	A Endosulfan I	0.000	7.475	0	761600	N.D.	0.451 #
11)	B alpha-Chl...	0.000	7.412	0	1079429	N.D.	0.591 #
15)	B Endosulfa...	9.309	8.331f	327455	1099329	0.580	0.698
16)	A 4,4'-DDD	9.200	0.000	170141	0	0.344	N.D. #
21)	B Endrin ke...	10.188f	0.000	472275	0	0.769	N.D. #
23)	Chlordane-1	7.071f	5.965	-87202	231769	N.D.	4.163
24)	Chlordane-2	0.000	6.643	0	238857	N.D.	3.496 #
26)	Chlordane-4	0.000	7.412	0	1079429	N.D.	5.714 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060222\
Data File : PL075372.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jun 2022 11:01
Operator : AR\AJ
Sample : N3099-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 03 06:01:18 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
Quant Title : GC Extractables
QLast Update : Wed Jun 01 10:19:11 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

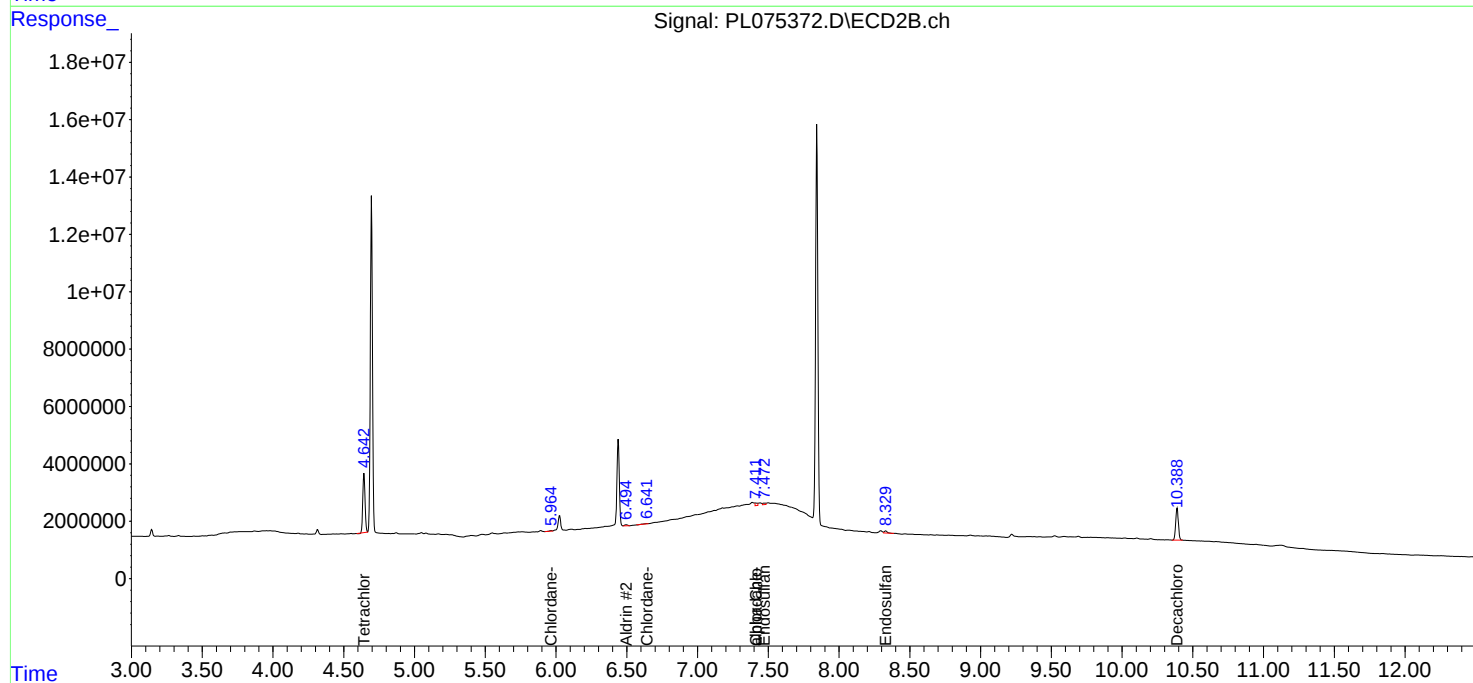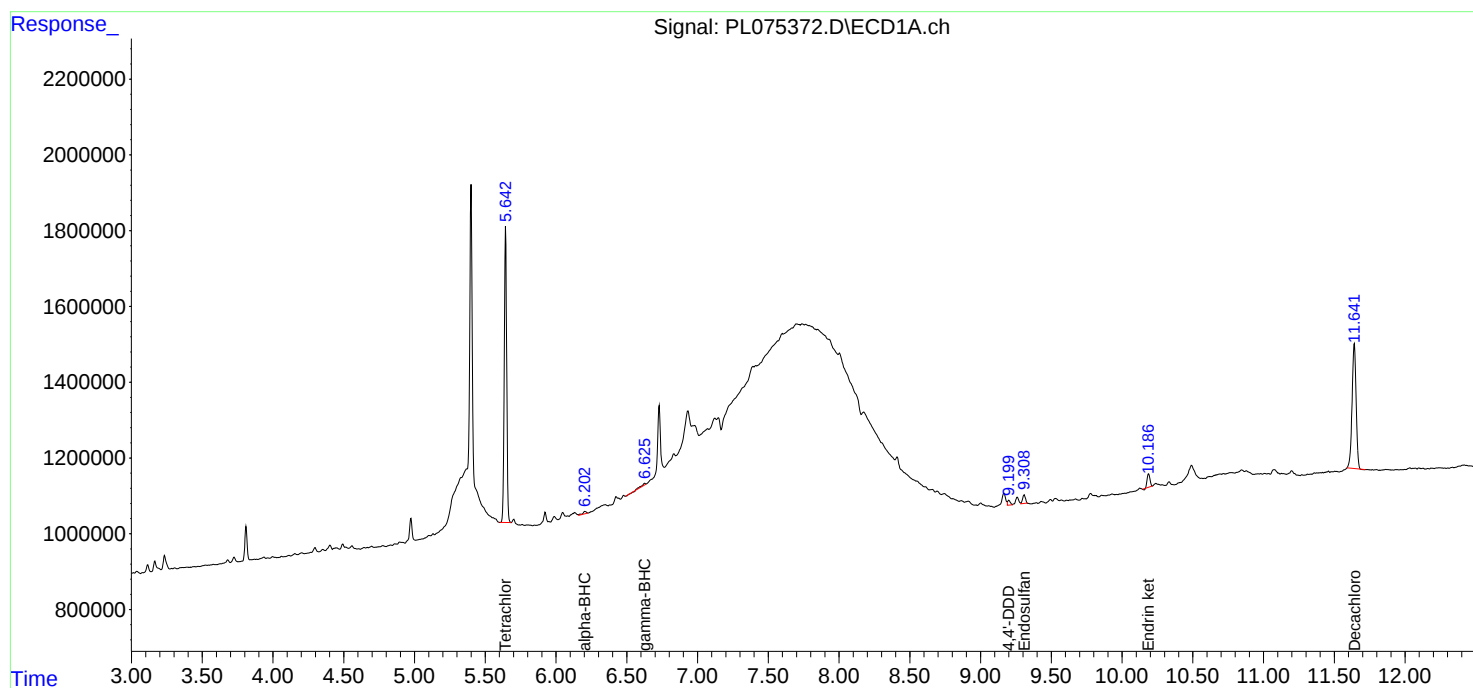

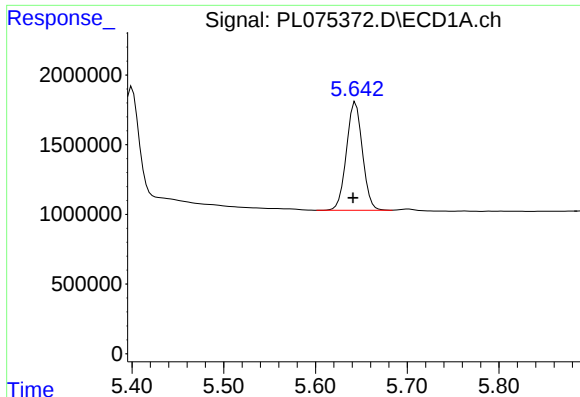


#1 Tetrachloro-m-xylene

R.T.: 5.644 min
Delta R.T.: 0.003 min
Response: 9376631
Conc: 15.95 ng/ml

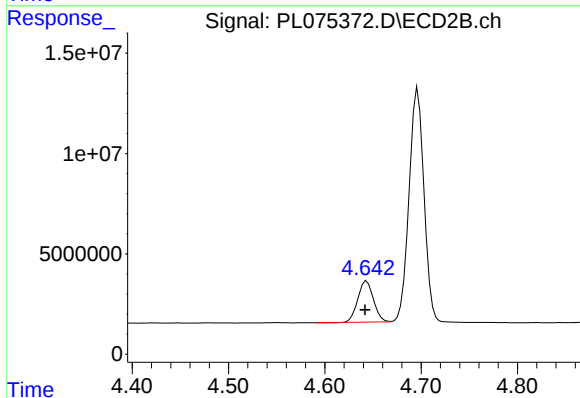


#1 Tetrachloro-m-xylene

R.T.: 4.644 min
Delta R.T.: 0.002 min
Response: 23005330
Conc: 14.52 ng/ml

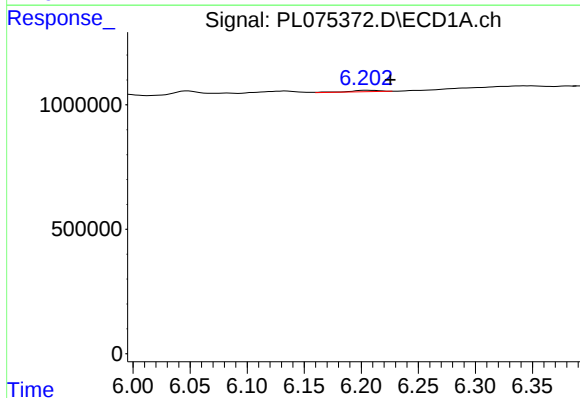


#2 alpha-BHC

R.T.: 6.205 min
Delta R.T.: -0.021 min
Response: 108189
Conc: 0.13 ng/ml

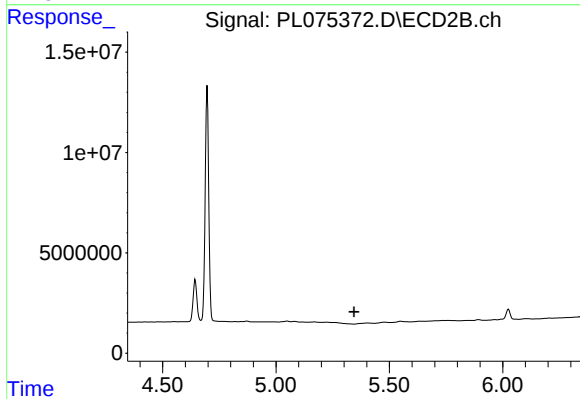


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T.: 5.344 min
Response: 0
Conc: N.D.

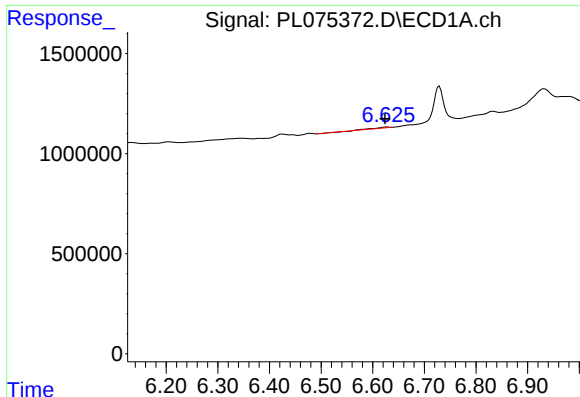


#3 gamma-BHC (Lindane)

R.T.: 6.627 min
Delta R.T.: 0.004 min
Response: 61588
Conc: 0.08 ng/ml

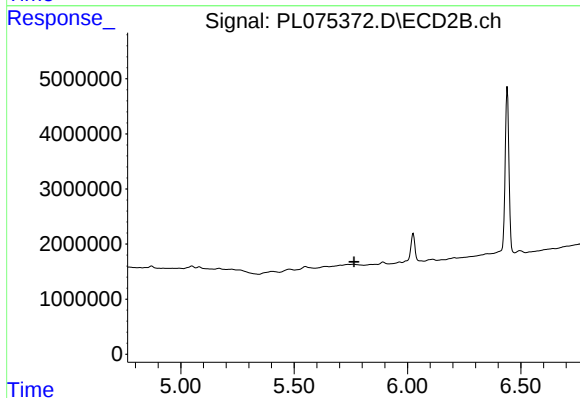


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T.: 5.765 min
Response: 0
Conc: N.D.

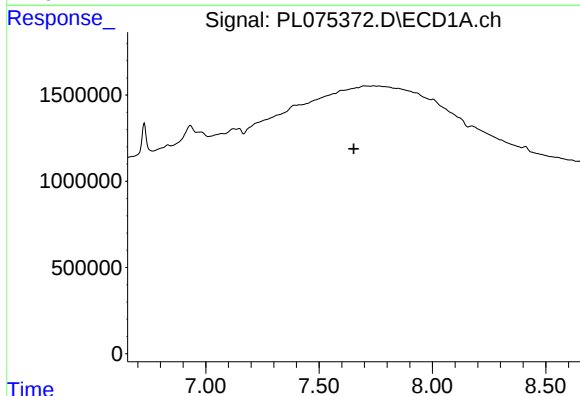


#5 Aldrin

R.T.: 0.000 min
Exp R.T.: 7.654 min
Response: 0
Conc: N.D.

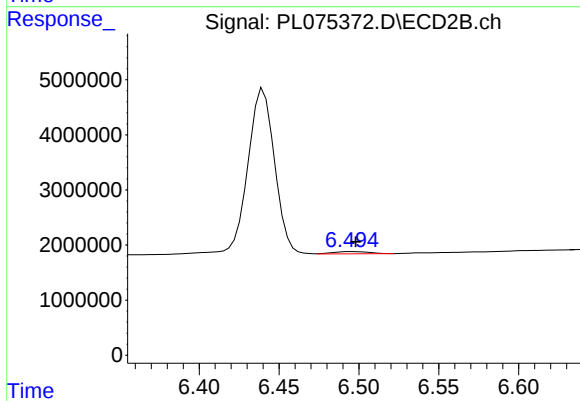


#5 Aldrin

R.T.: 6.496 min
Delta R.T.: -0.002 min
Response: 629827
Conc: 0.33 ng/ml

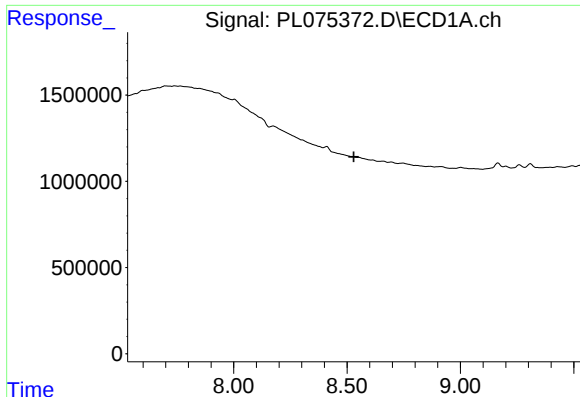


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 8.530 min
Response: 0
Conc: N.D.

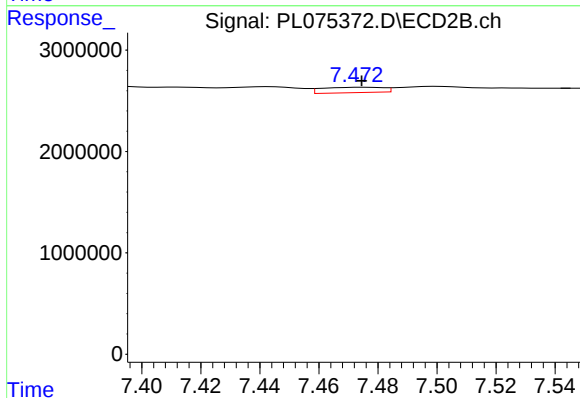


#9 Endosulfan I

R.T.: 7.475 min
Delta R.T.: 0.000 min
Response: 761600
Conc: 0.45 ng/ml

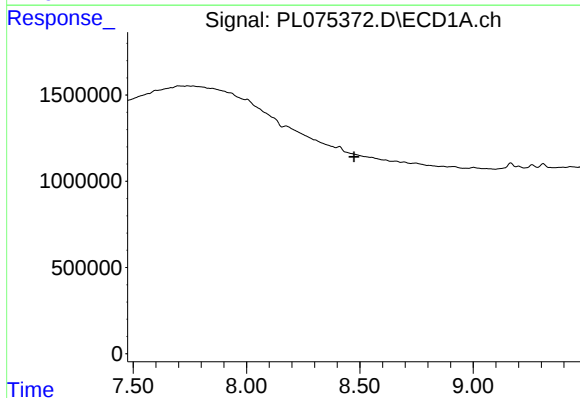


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 8.474 min
Response: 0
Conc: N.D.

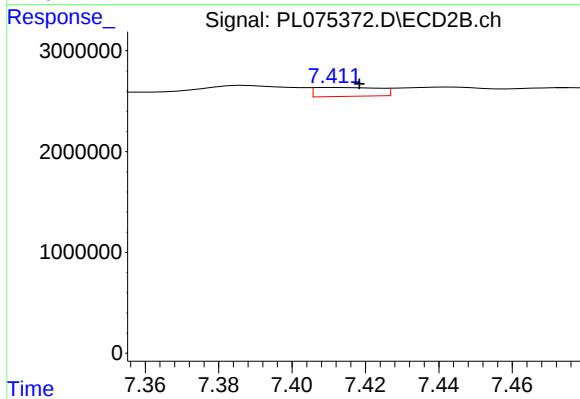


#11 alpha-Chlordane

R.T.: 7.412 min
Delta R.T.: -0.006 min
Response: 1079429
Conc: 0.59 ng/ml

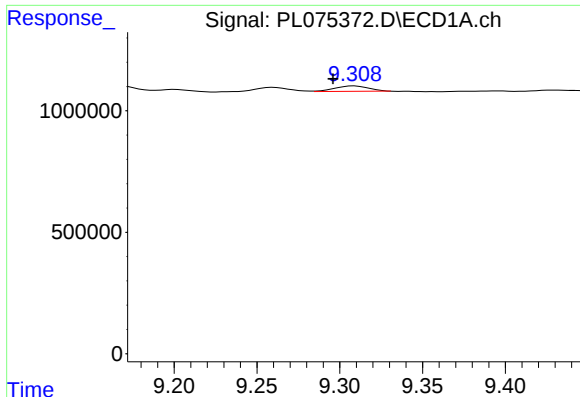


#15 Endosulfan II

R.T.: 9.309 min
Delta R.T.: 0.013 min
Response: 327455
Conc: 0.58 ng/ml

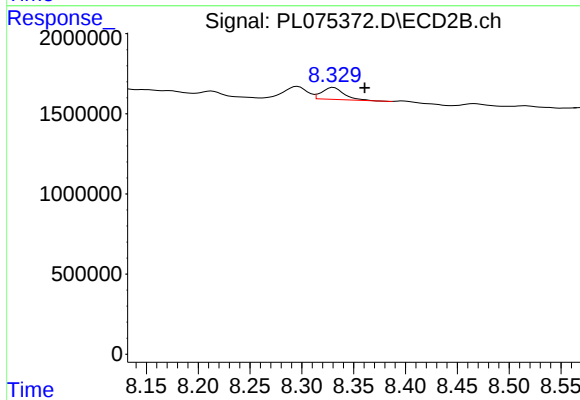


#15 Endosulfan II

R.T.: 8.331 min
Delta R.T.: -0.030 min
Response: 1099329
Conc: 0.70 ng/ml

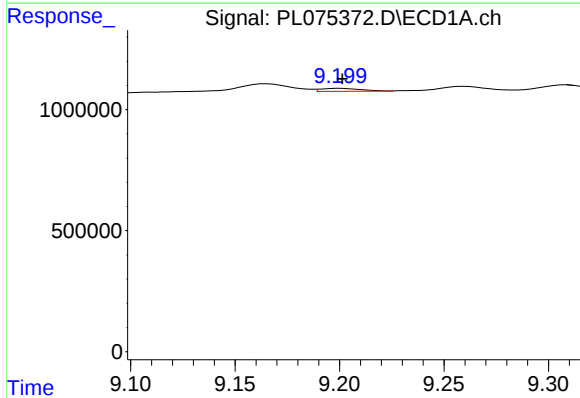


#16 4,4'-DDD

R.T.: 9.200 min
Delta R.T.: 0.000 min
Response: 170141
Conc: 0.34 ng/ml

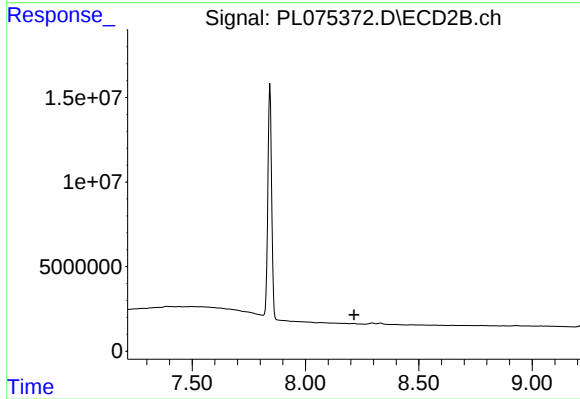


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 8.215 min
Response: 0
Conc: N.D.

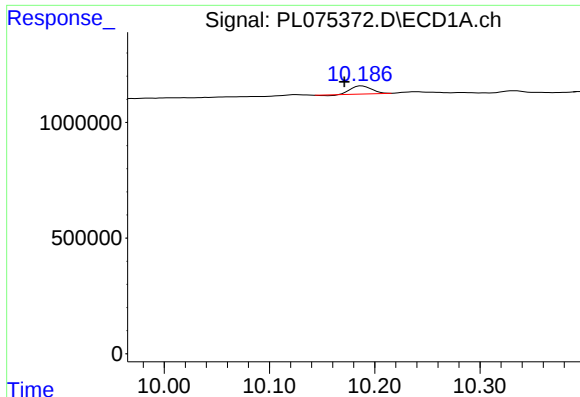


#21 Endrin ketone

R.T.: 10.188 min
Delta R.T.: 0.017 min
Response: 472275
Conc: 0.77 ng/ml

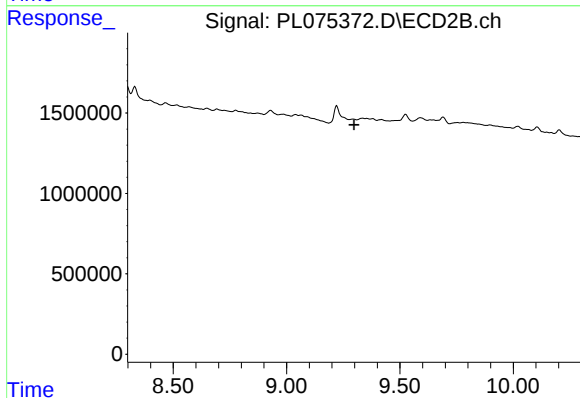


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 9.298 min
Response: 0
Conc: N.D.

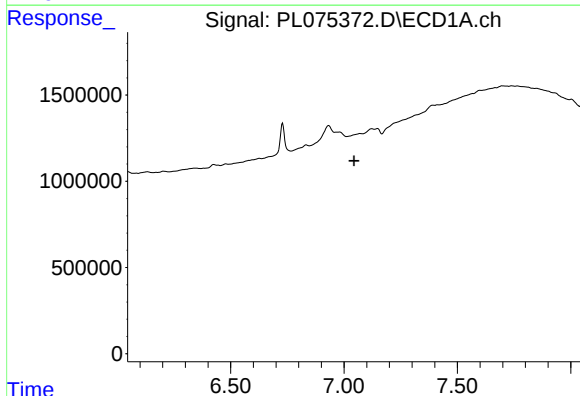


#23 Chlordane-1

R.T.: 7.071 min
Delta R.T.: 0.027 min
Response: -87202
Conc: N.D.

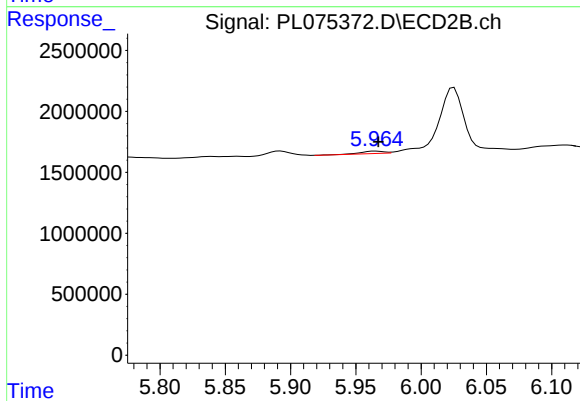


#23 Chlordane-1

R.T.: 5.965 min
Delta R.T.: -0.002 min
Response: 231769
Conc: 4.16 ng/ml

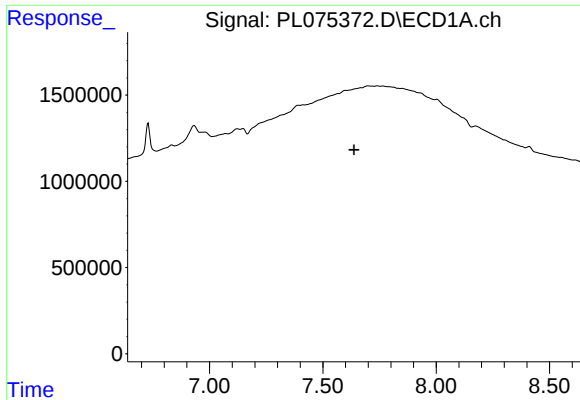


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T.: 7.638 min
Response: 0
Conc: N.D.

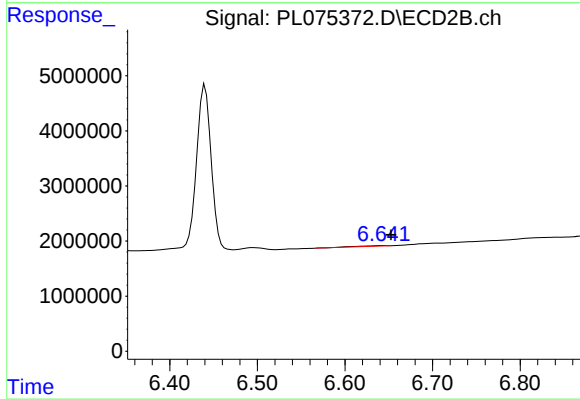


#24 Chlordane-2

R.T.: 6.643 min
Delta R.T.: -0.010 min
Response: 238857
Conc: 3.50 ng/ml

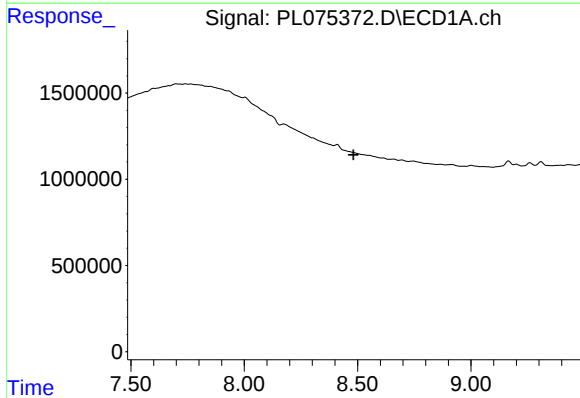


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 8.482 min
Response: 0
Conc: N.D.

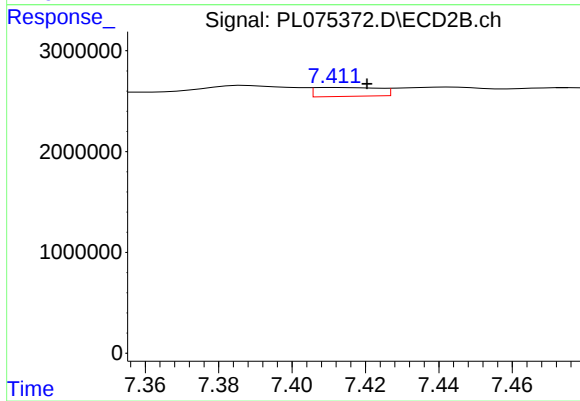


#26 Chlordane-4

R.T.: 7.412 min
Delta R.T.: -0.008 min
Response: 1079429
Conc: 5.71 ng/ml

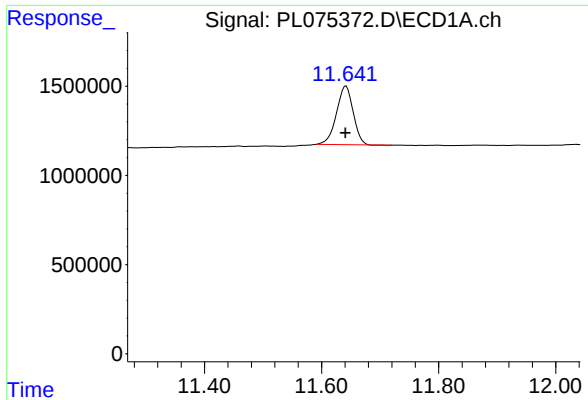

#28 Decachlorobiphenyl

R.T.: 11.642 min
Delta R.T.: 0.000 min
Response: 6506313
Conc: 12.13 ng/ml

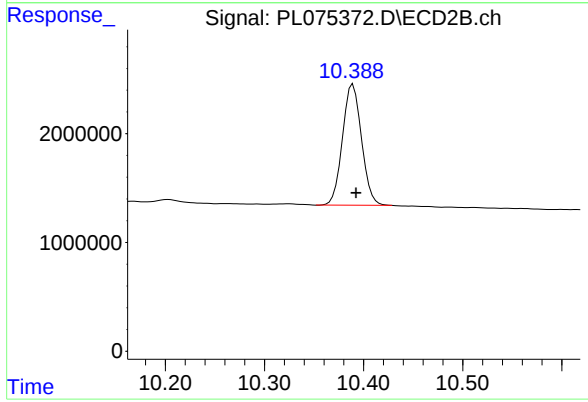

#28 Decachlorobiphenyl

R.T.: 10.389 min
Delta R.T.: -0.003 min
Response: 14862881
Conc: 10.83 ng/ml