

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060222\
 Data File : PL075382.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jun 2022 13:46
 Operator : AR\AJ
 Sample : N2932-03
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 03 06:03:24 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 01 10:19:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	5.644	4.642	15055387	40488997	25.616	25.559
28)	SA Decachlor...	11.640	10.388	9104961	23202613	16.981	16.908
Target Compounds							
5)	MB Aldrin	0.000	6.495	0	776209	N.D.	0.402 #
7)	B delta-BHC	0.000	6.411	0	321166	N.D.	0.150 #
11)	B alpha-Chl...	0.000	7.394f	0	359366	N.D.	0.197 #
14)	MA Endrin	0.000	8.069f	0	225385	N.D.	0.145 #
15)	B Endosulfa...	9.306	0.000	298677	0	0.529	N.D. #
17)	MA 4,4'-DDT	0.000	8.465	0	457254	N.D.	0.320 #
19)	B Endosulfa...	9.664	8.774	282436	141461	0.508	0.095 #
21)	B Endrin ke...	10.187f	0.000	159865	0	0.260	N.D. #
26)	Chlordane-4	0.000	7.394f	0	359366	N.D.	1.902 #
27)	Chlordane-5	0.000	8.127	0	228749	N.D.	4.584 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060222\
Data File : PL075382.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jun 2022 13:46
Operator : AR\AJ
Sample : N2932-03
Misc :
ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 03 06:03:24 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
Quant Title : GC Extractables
QLast Update : Wed Jun 01 10:19:11 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

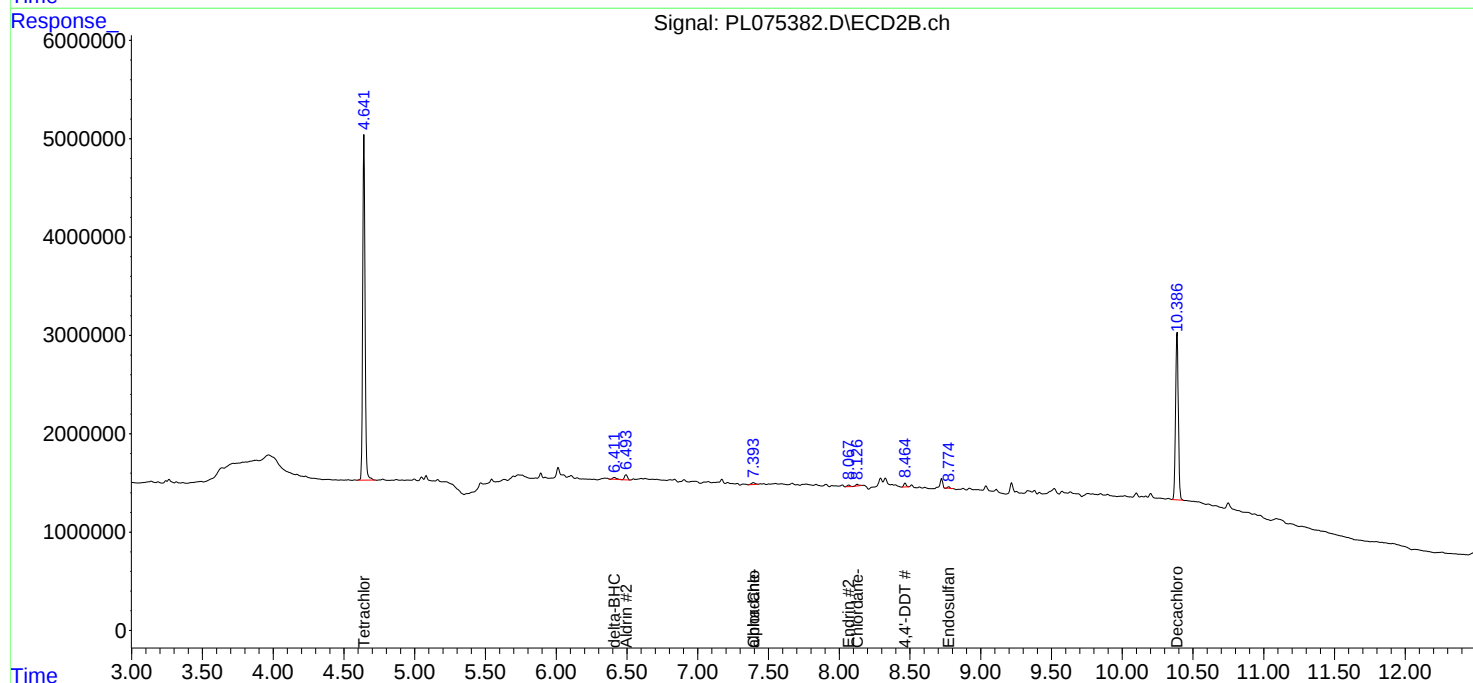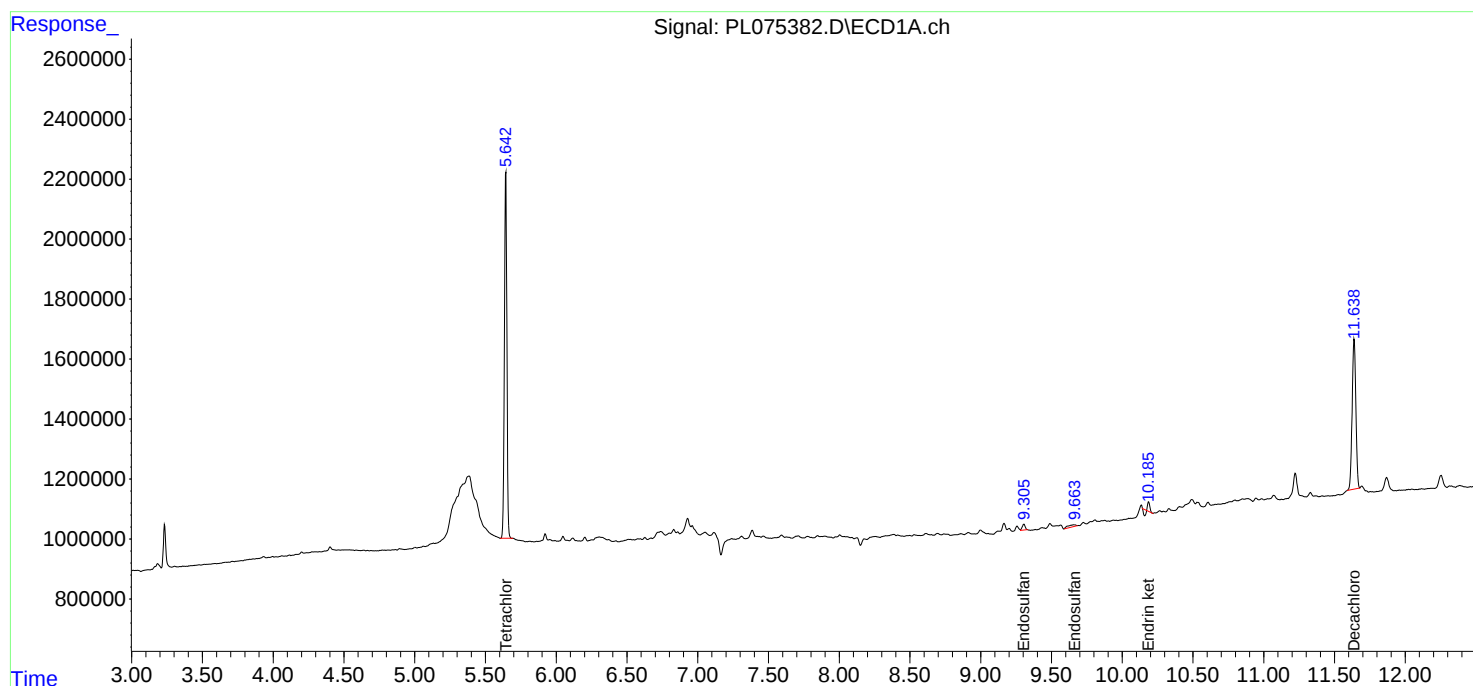

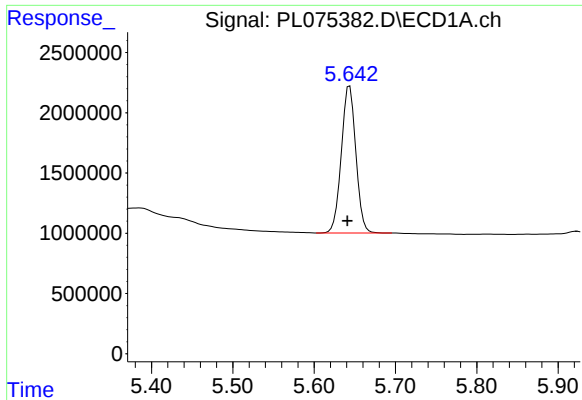


#1 Tetrachloro-m-xylene

R.T.: 5.644 min
Delta R.T.: 0.003 min
Response: 15055387
Conc: 25.62 ng/ml

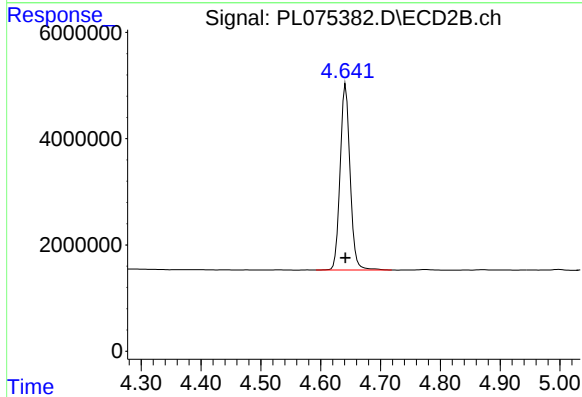


#1 Tetrachloro-m-xylene

R.T.: 4.642 min
Delta R.T.: 0.000 min
Response: 40488997
Conc: 25.56 ng/ml

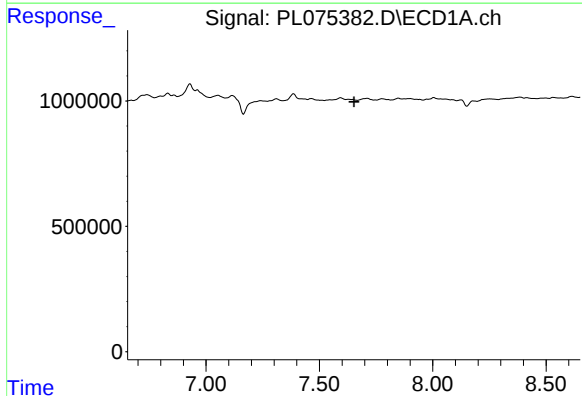


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 7.654 min
Response: 0
Conc: N.D.

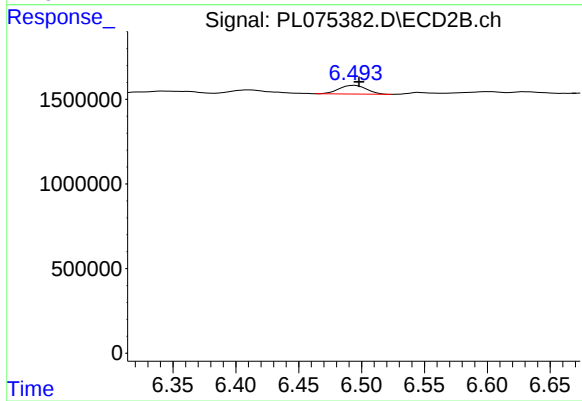


#5 Aldrin

R.T.: 6.495 min
Delta R.T.: -0.003 min
Response: 776209
Conc: 0.40 ng/ml

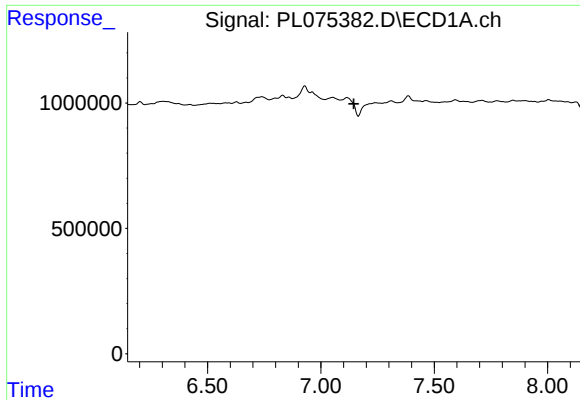


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 7.146 min
Response: 0
Conc: N.D.

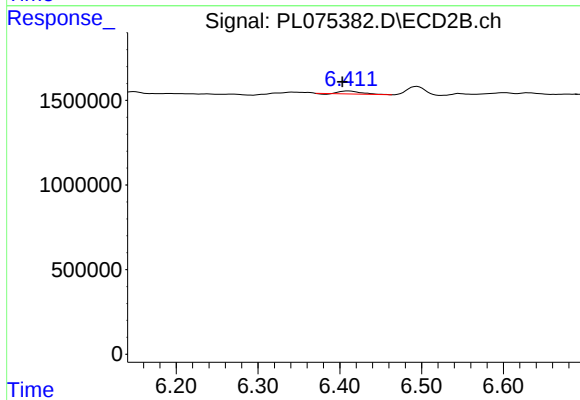


#7 delta-BHC

R.T.: 6.411 min
Delta R.T.: 0.007 min
Response: 321166
Conc: 0.15 ng/ml

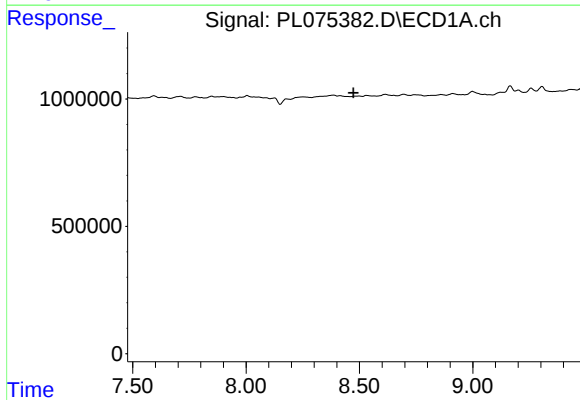


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 8.474 min
Response: 0
Conc: N.D.

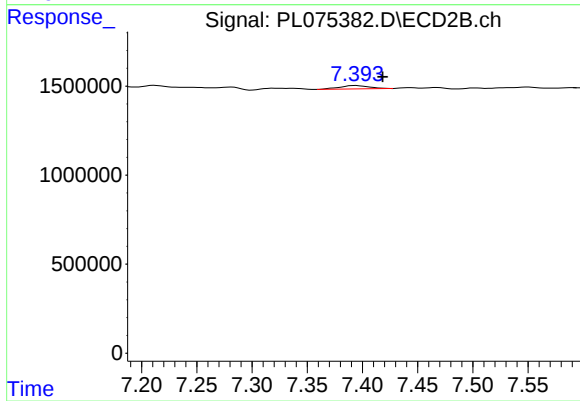


#11 alpha-Chlordane

R.T.: 7.394 min
Delta R.T.: -0.024 min
Response: 359366
Conc: 0.20 ng/ml

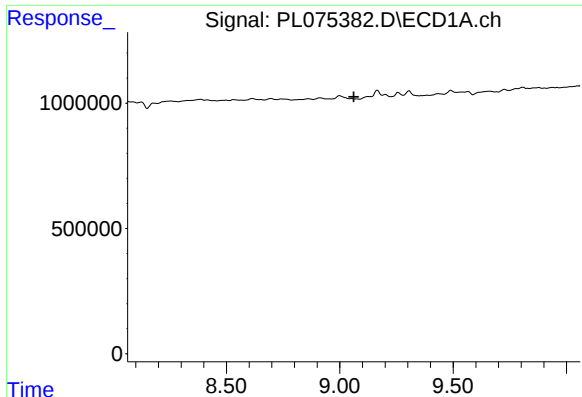


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 9.062 min
Response: 0
Conc: N.D.

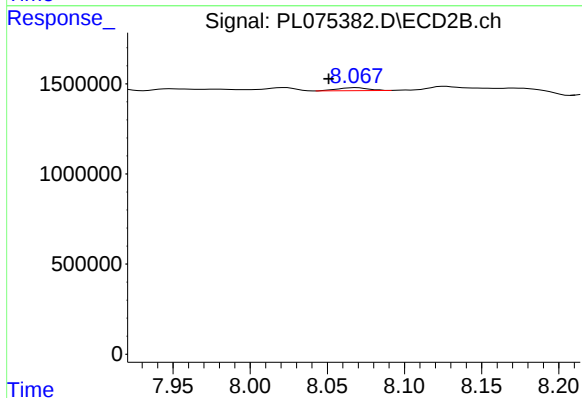


#14 Endrin

R.T.: 8.069 min
Delta R.T.: 0.018 min
Response: 225385
Conc: 0.14 ng/ml

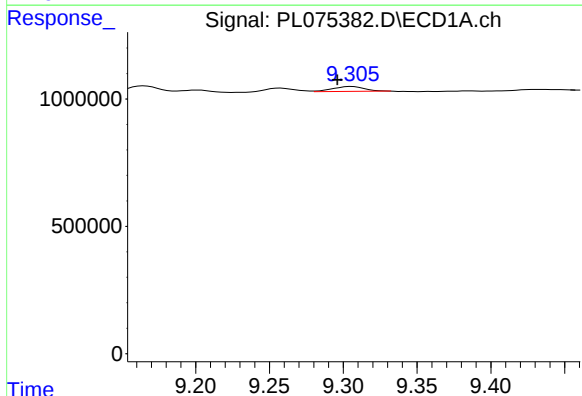


#15 Endosulfan II

R.T.: 9.306 min
Delta R.T.: 0.010 min
Response: 298677
Conc: 0.53 ng/ml

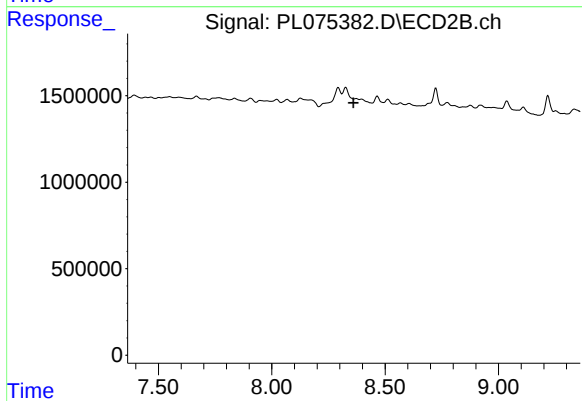


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 8.361 min
Response: 0
Conc: N.D.

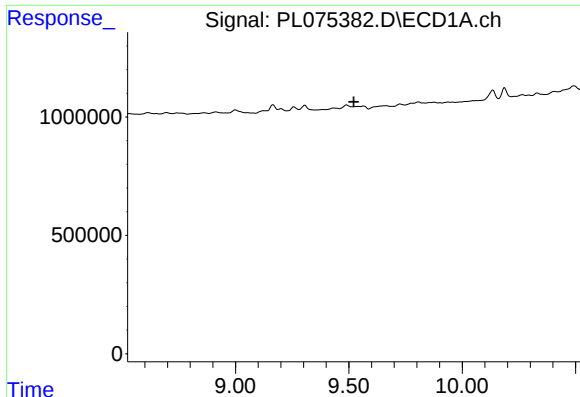


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 9.522 min
Response: 0
Conc: N.D.

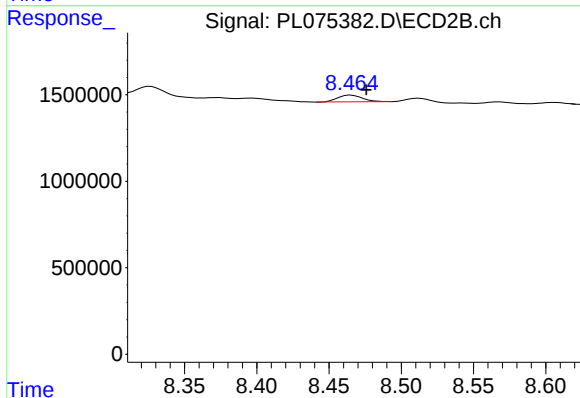


#17 4,4'-DDT

R.T.: 8.465 min
Delta R.T.: -0.010 min
Response: 457254
Conc: 0.32 ng/ml

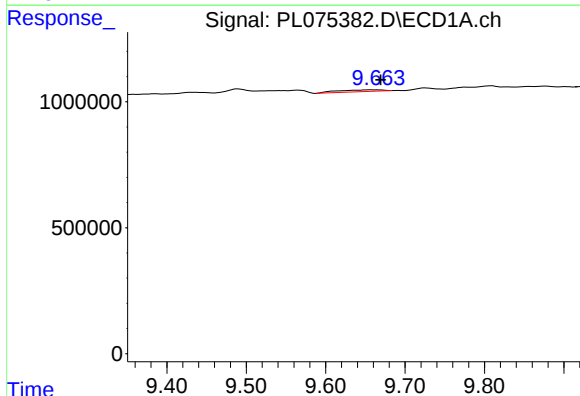


#19 Endosulfan Sulfate

R.T.: 9.664 min
Delta R.T.: -0.005 min
Response: 282436
Conc: 0.51 ng/ml

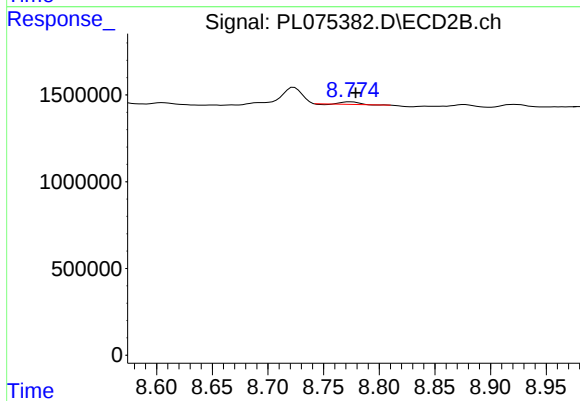


#19 Endosulfan Sulfate

R.T.: 8.774 min
Delta R.T.: -0.004 min
Response: 141461
Conc: 0.09 ng/ml

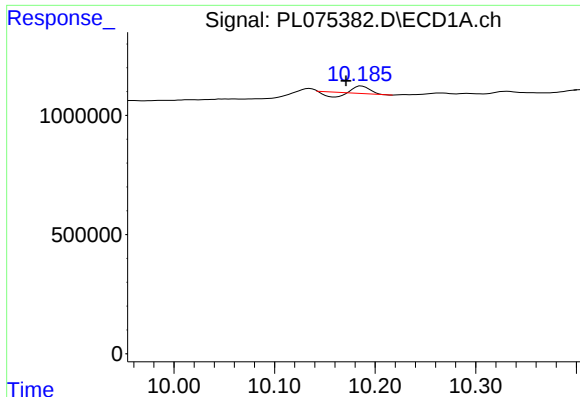


#21 Endrin ketone

R.T.: 10.187 min
Delta R.T.: 0.015 min
Response: 159865
Conc: 0.26 ng/ml

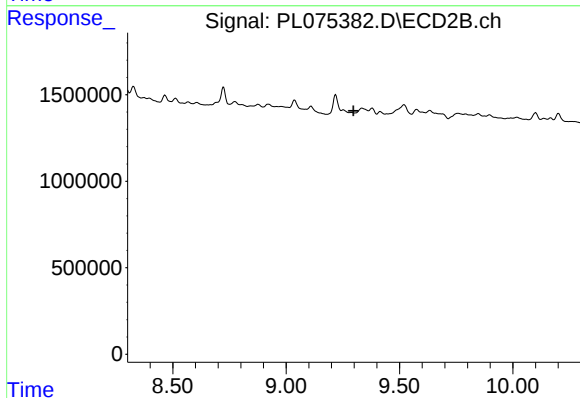


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.298 min
Response: 0
Conc: N.D.

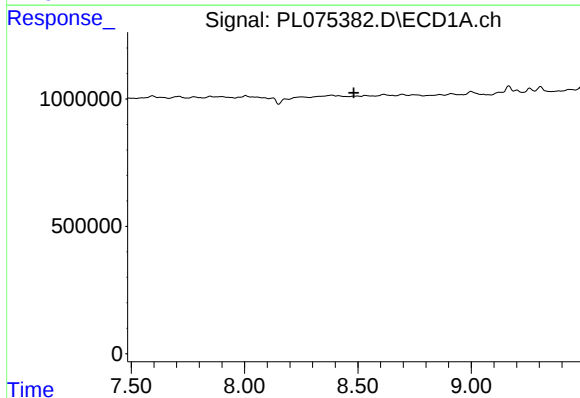


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 8.482 min
Response: 0
Conc: N.D.

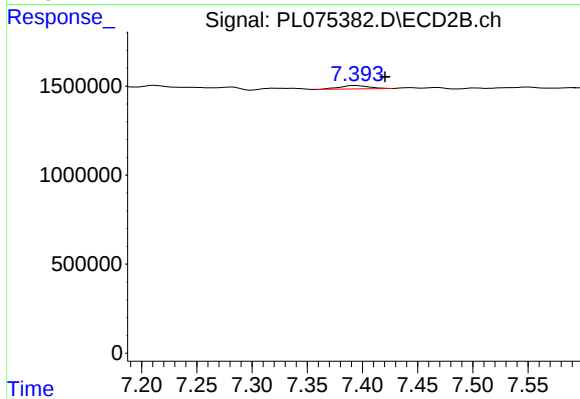


#26 Chlordane-4

R.T.: 7.394 min
Delta R.T.: -0.027 min
Response: 359366
Conc: 1.90 ng/ml

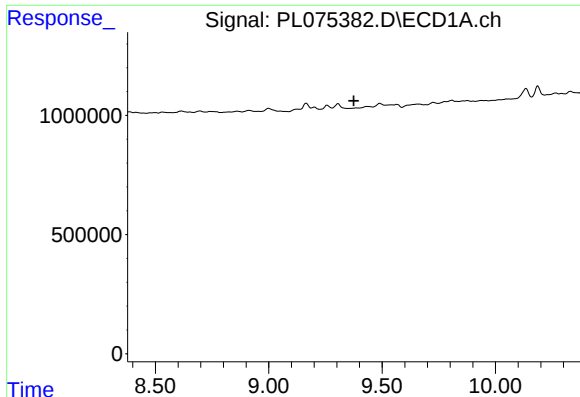


#27 Chlorine-5

R.T.: 0.000 min
Exp R.T.: 9.375 min
Response: 0
Conc: N.D.

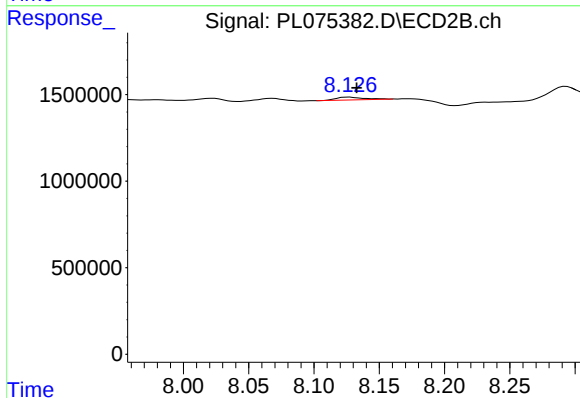


#27 Chlorine-5

R.T.: 8.127 min
Delta R.T.: -0.006 min
Response: 228749
Conc: 4.58 ng/ml

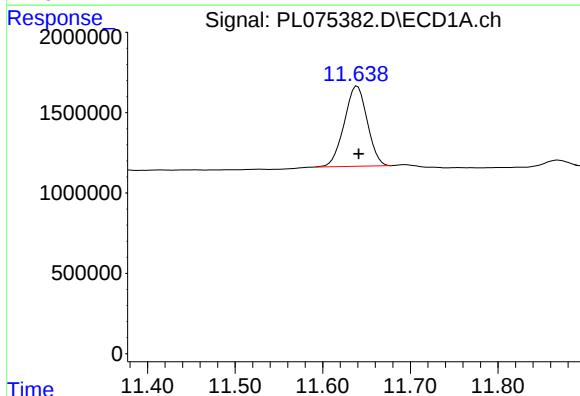

#28 Decachlorobiphenyl

R.T.: 11.640 min
Delta R.T.: -0.001 min
Response: 9104961
Conc: 16.98 ng/ml

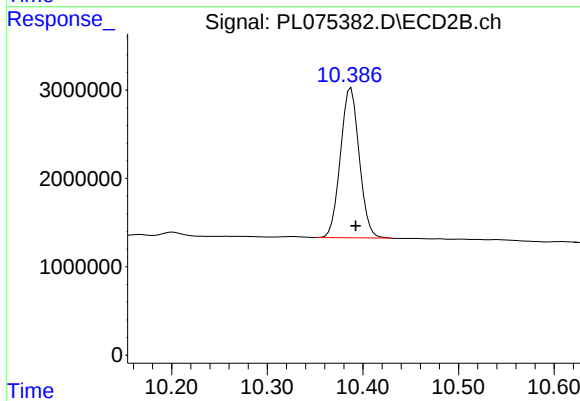

#28 Decachlorobiphenyl

R.T.: 10.388 min
Delta R.T.: -0.005 min
Response: 23202613
Conc: 16.91 ng/ml