

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060222\
 Data File : PL075391.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jun 2022 16:15
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 03 06:05:22 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 01 10:19:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	5.643	4.641	12124636	33138155	20.629	20.919
28)	SA Decachlor...	11.640	10.388	11470410	28013155	21.393	20.414
Target Compounds							
7)	B delta-BHC	0.000	6.411	0	409419	N.D.	0.191 #
8)	B Heptachlo...	8.125	0.000	1596322	0	2.338	N.D. #
11)	B alpha-Chl...	0.000	7.394f	0	263885	N.D.	0.144 #
13)	MA Dieldrin	0.000	7.760	0	1583814	N.D.	0.913 #
14)	MA Endrin	0.000	8.070f	0	112642	N.D.	0.072 #
15)	B Endosulfa...	9.303	0.000	224952	0	0.399	N.D. #
17)	MA 4,4'-DDT	9.534	8.489	176449	284637	0.303	0.199 #
19)	B Endosulfa...	9.677	0.000	131688	0	0.237	N.D. #
21)	B Endrin ke...	10.188f	0.000	731760	0	1.192	N.D. #
26)	Chlordane-4	0.000	7.394f	0	263885	N.D.	1.397 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060222\
Data File : PL075391.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jun 2022 16:15
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 03 06:05:22 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
Quant Title : GC Extractables
QLast Update : Wed Jun 01 10:19:11 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

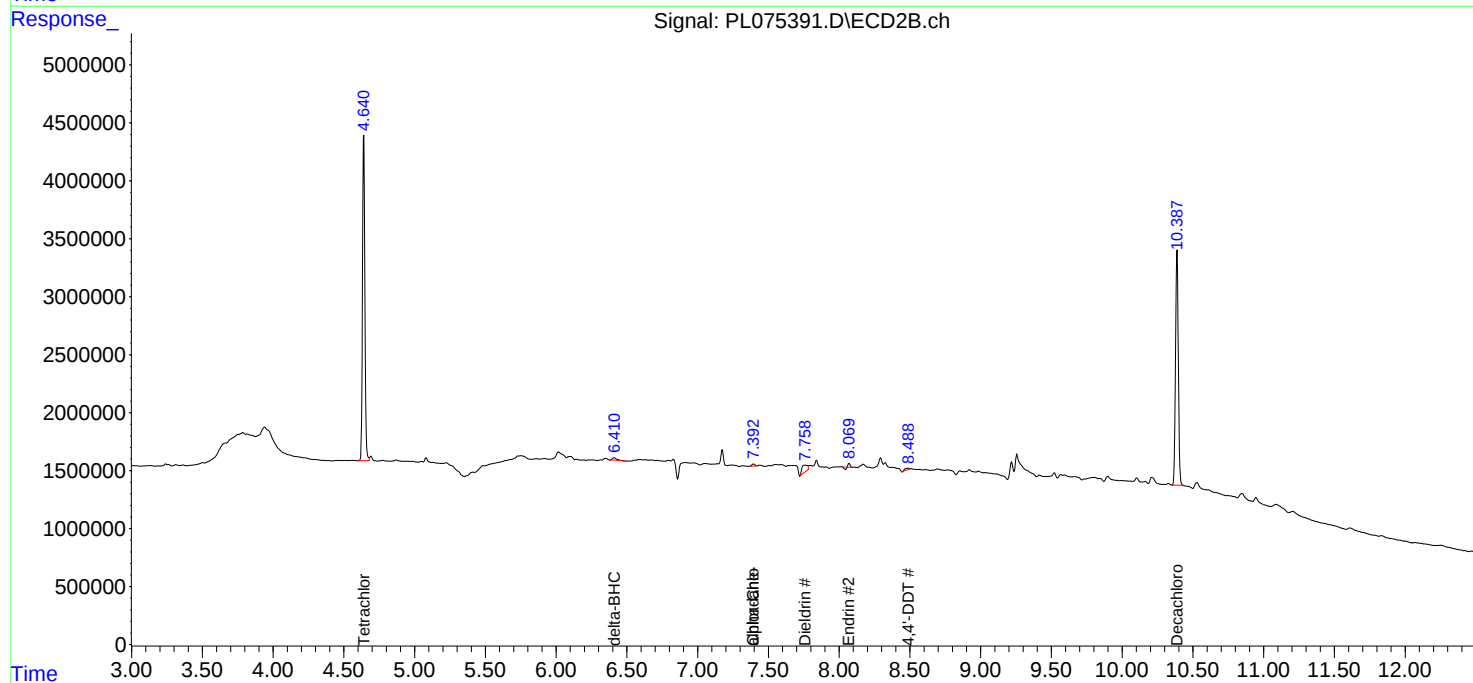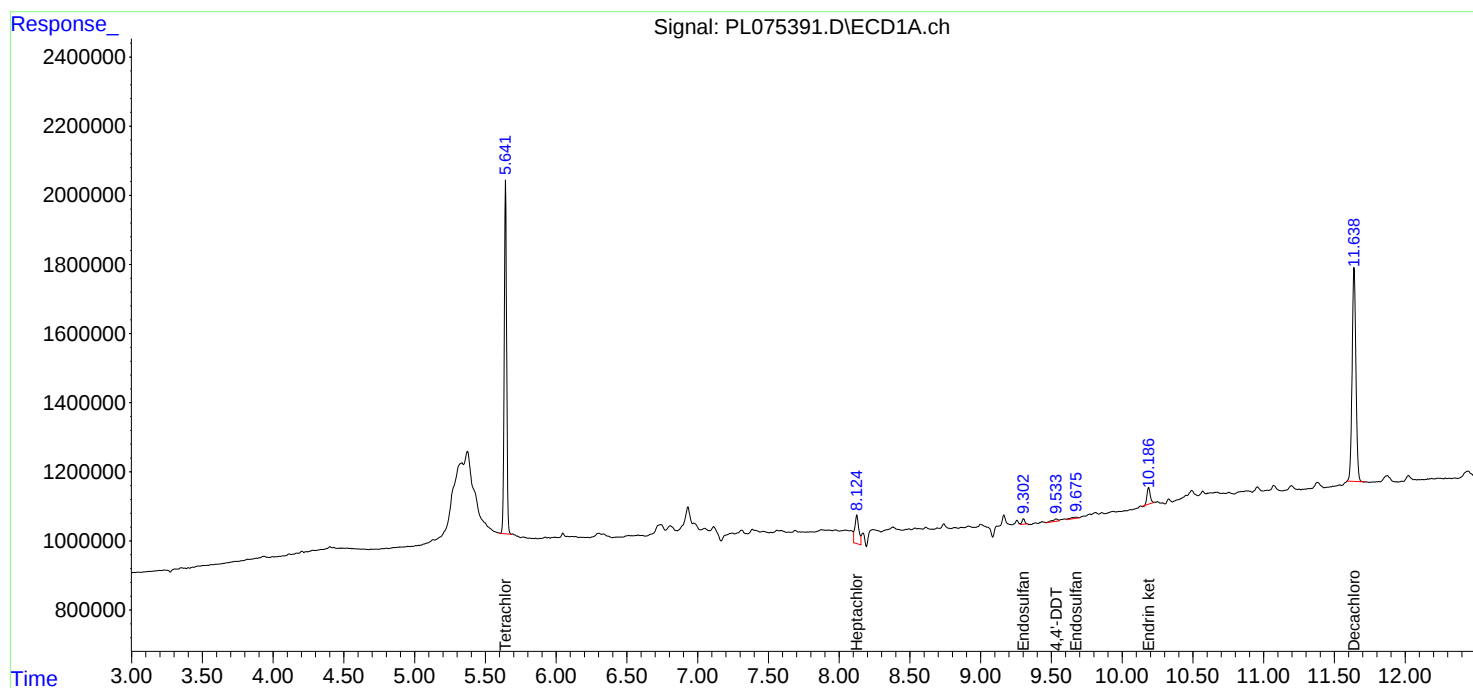

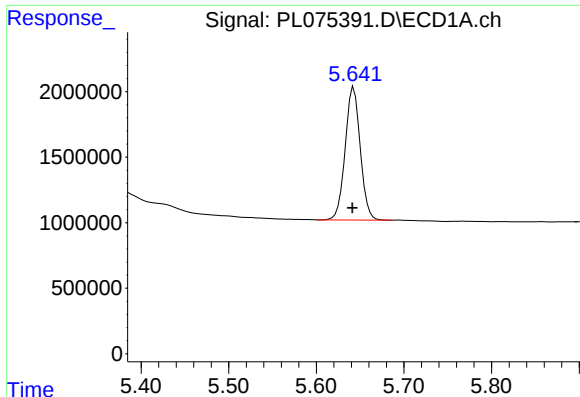


#1 Tetrachloro-m-xylene

R.T.: 5.643 min
Delta R.T.: 0.002 min
Response: 12124636
Conc: 20.63 ng/ml

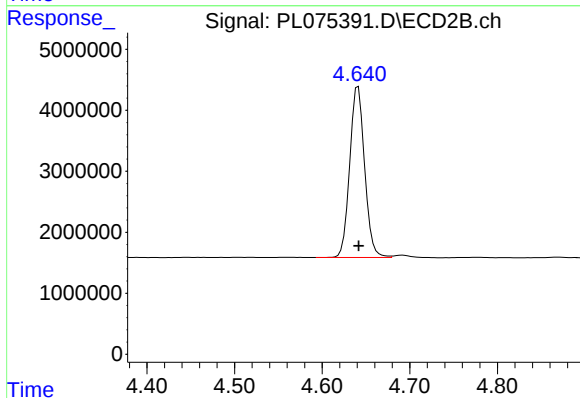


#1 Tetrachloro-m-xylene

R.T.: 4.641 min
Delta R.T.: 0.000 min
Response: 33138155
Conc: 20.92 ng/ml

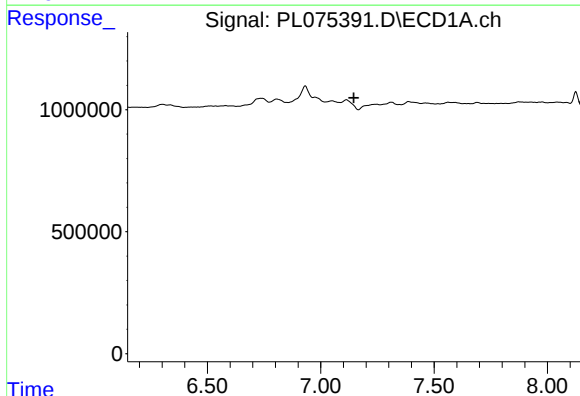


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 7.146 min
Response: 0
Conc: N.D.

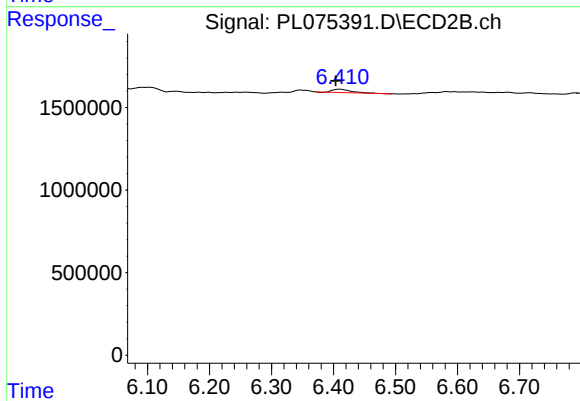


#7 delta-BHC

R.T.: 6.411 min
Delta R.T.: 0.008 min
Response: 409419
Conc: 0.19 ng/ml

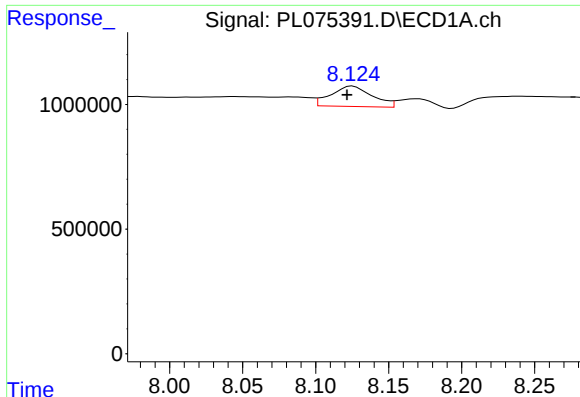


#8 Heptachlor epoxide

R.T.: 8.125 min
Delta R.T.: 0.004 min
Response: 1596322
Conc: 2.34 ng/ml

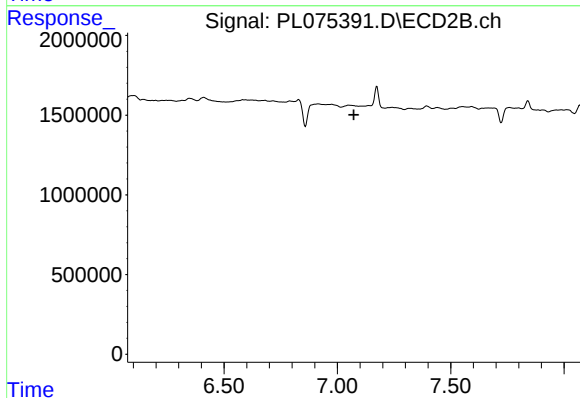


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 7.072 min
Response: 0
Conc: N.D.

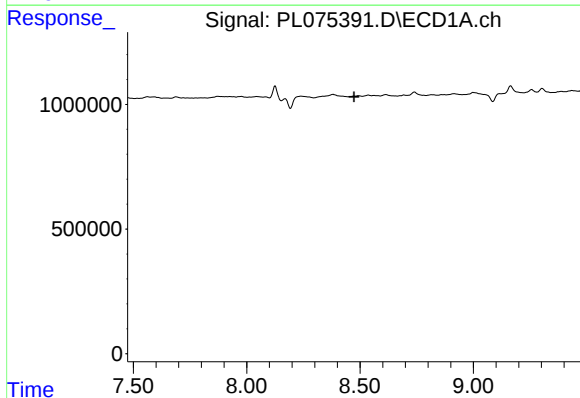


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 8.474 min
Response: 0
Conc: N.D.

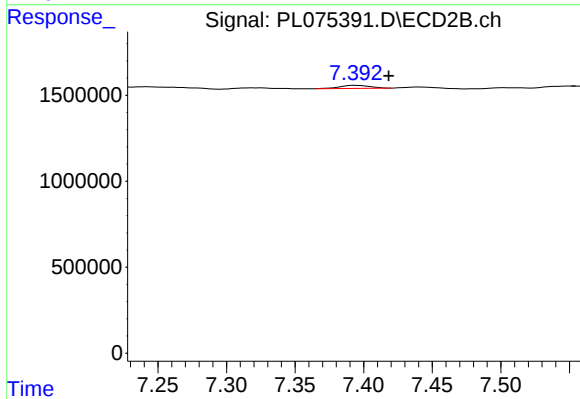


#11 alpha-Chlordane

R.T.: 7.394 min
Delta R.T.: -0.024 min
Response: 263885
Conc: 0.14 ng/ml

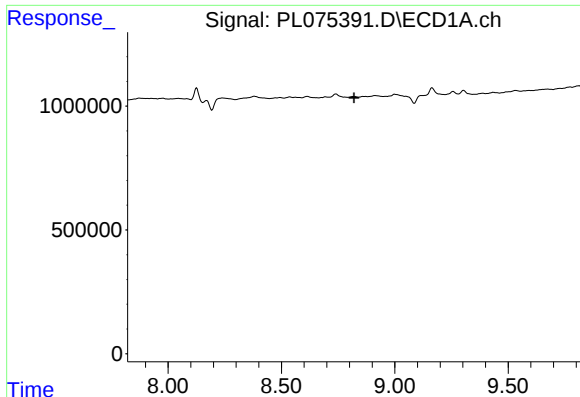


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 8.821 min
Response: 0
Conc: N.D.

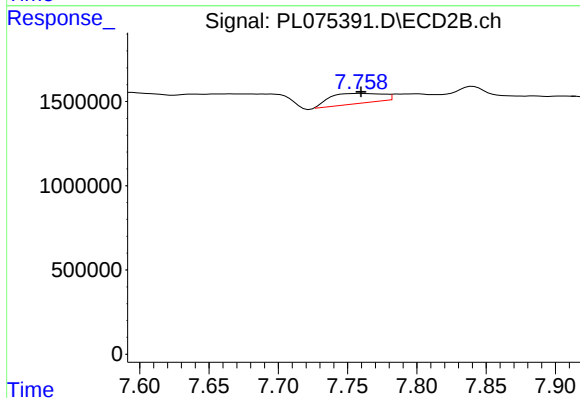


#13 Dieldrin

R.T.: 7.760 min
Delta R.T.: 0.000 min
Response: 1583814
Conc: 0.91 ng/ml

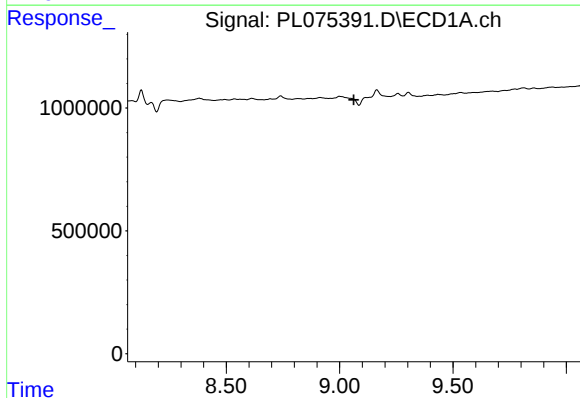


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 9.062 min
Response: 0
Conc: N.D.

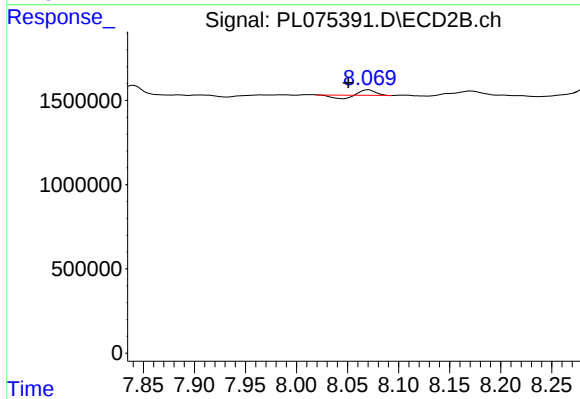


#14 Endrin

R.T.: 8.070 min
Delta R.T.: 0.020 min
Response: 112642
Conc: 0.07 ng/ml

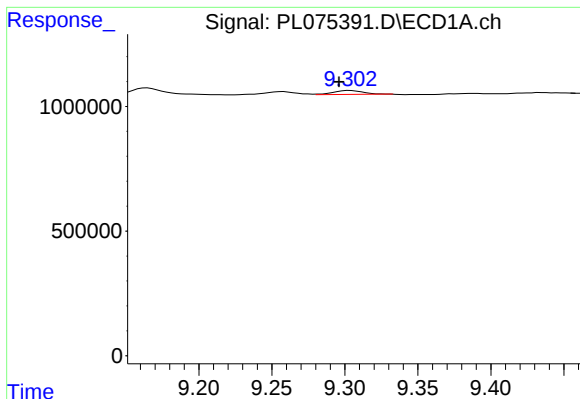


#15 Endosulfan II

R.T.: 9.303 min
Delta R.T.: 0.007 min
Response: 224952
Conc: 0.40 ng/ml

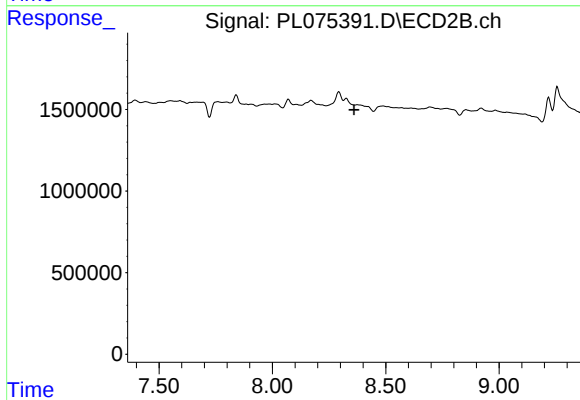


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 8.361 min
Response: 0
Conc: N.D.

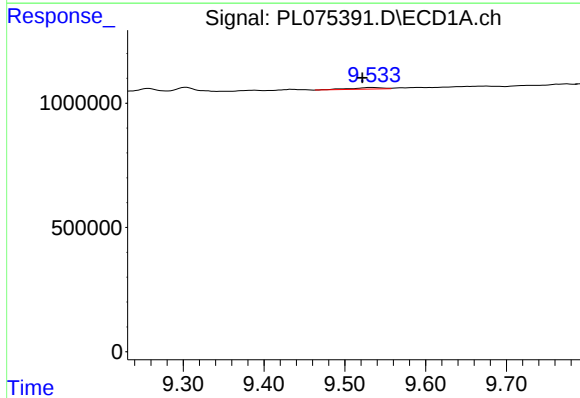


#17 4,4'-DDT

R.T.: 9.534 min
Delta R.T.: 0.012 min
Response: 176449
Conc: 0.30 ng/ml

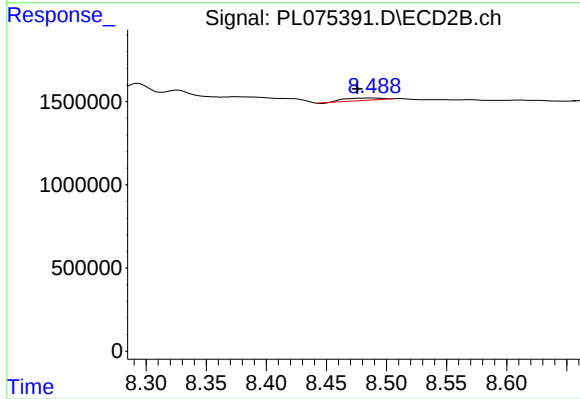


#17 4,4'-DDT

R.T.: 8.489 min
Delta R.T.: 0.013 min
Response: 284637
Conc: 0.20 ng/ml

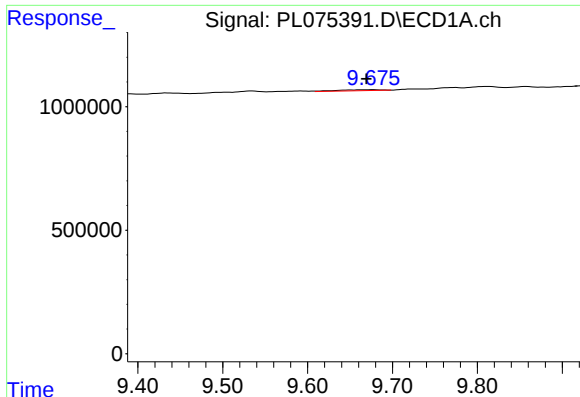


#19 Endosulfan Sulfate

R.T.: 9.677 min
Delta R.T.: 0.007 min
Response: 131688
Conc: 0.24 ng/ml

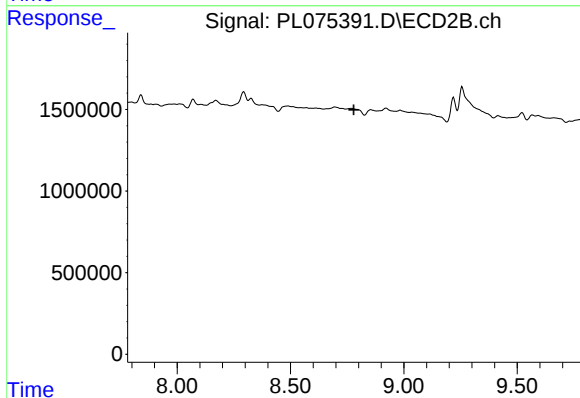


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 8.779 min
Response: 0
Conc: N.D.

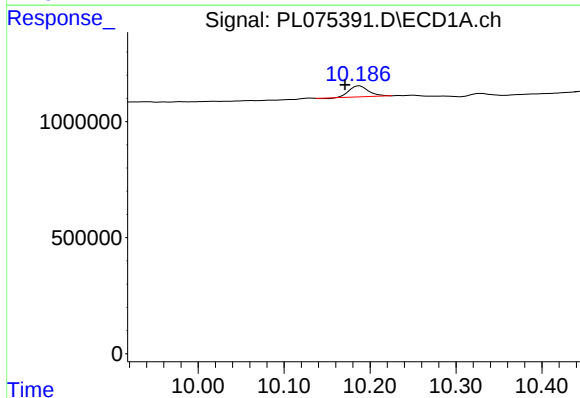


#21 Endrin ketone

R.T.: 10.188 min
Delta R.T.: 0.016 min
Response: 731760
Conc: 1.19 ng/ml

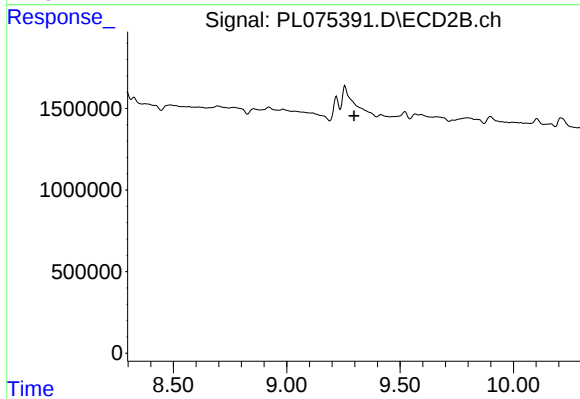


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 9.298 min
Response: 0
Conc: N.D.

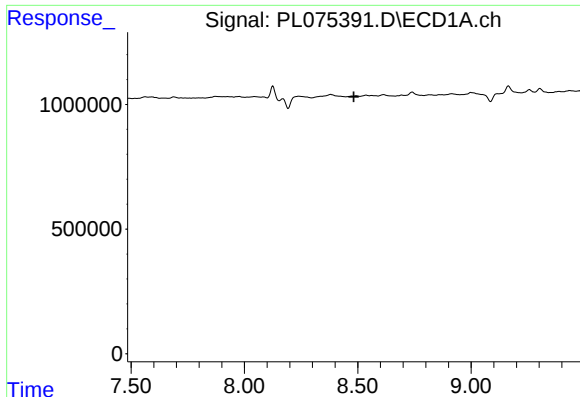


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 8.482 min
Response: 0
Conc: N.D.

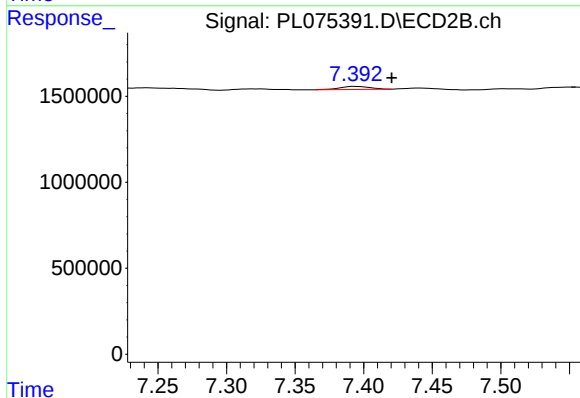


#26 Chlordane-4

R.T.: 7.394 min
Delta R.T.: -0.027 min
Response: 263885
Conc: 1.40 ng/ml

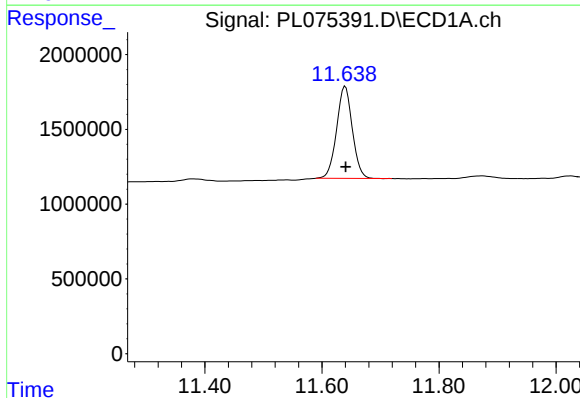

#28 Decachlorobiphenyl

R.T.: 11.640 min
Delta R.T.: -0.001 min
Response: 11470410
Conc: 21.39 ng/ml

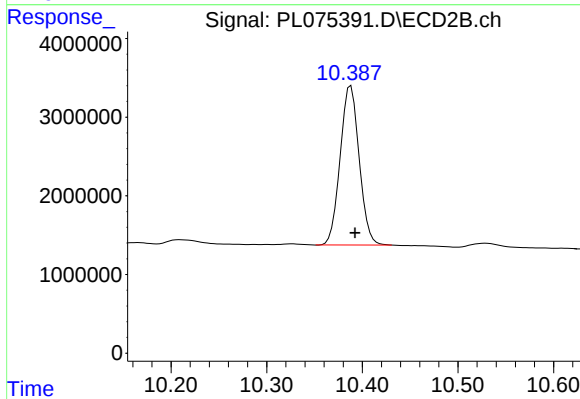

#28 Decachlorobiphenyl

R.T.: 10.388 min
Delta R.T.: -0.004 min
Response: 28013155
Conc: 20.41 ng/ml