

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060222\
 Data File : PL075397.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jun 2022 17:56
 Operator : AR\AJ
 Sample : PB144874TB
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 03 06:06:44 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 01 10:19:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	5.643	4.641	11343678	31325970	19.301	19.775
28)	SA Decachlor...	11.638	10.386	10571312	26113634	19.716	19.030
Target Compounds							
7)	B delta-BHC	0.000	6.412	0	294895	N.D.	0.137 #
9)	A Endosulfan I	0.000	7.501f	0	58127	N.D.	0.034 #
11)	B alpha-Chl...	0.000	7.396f	0	312713	N.D.	0.171 #
14)	MA Endrin	0.000	8.071f	0	85060	N.D.	0.055 #
15)	B Endosulfa...	9.304	0.000	216439	0	0.383	N.D. #
17)	MA 4,4'-DDT	9.533	0.000	269902	0	0.463	N.D. #
19)	B Endosulfa...	9.676	0.000	126464	0	0.227	N.D. #
21)	B Endrin ke...	10.187f	0.000	1148125	0	1.870	N.D. #
26)	Chlordane-4	0.000	7.442f	0	158732	N.D.	0.840 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060222\
Data File : PL075397.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jun 2022 17:56
Operator : AR\AJ
Sample : PB144874TB
Misc :
ALS Vial : 28 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 03 06:06:44 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
Quant Title : GC Extractables
QLast Update : Wed Jun 01 10:19:11 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

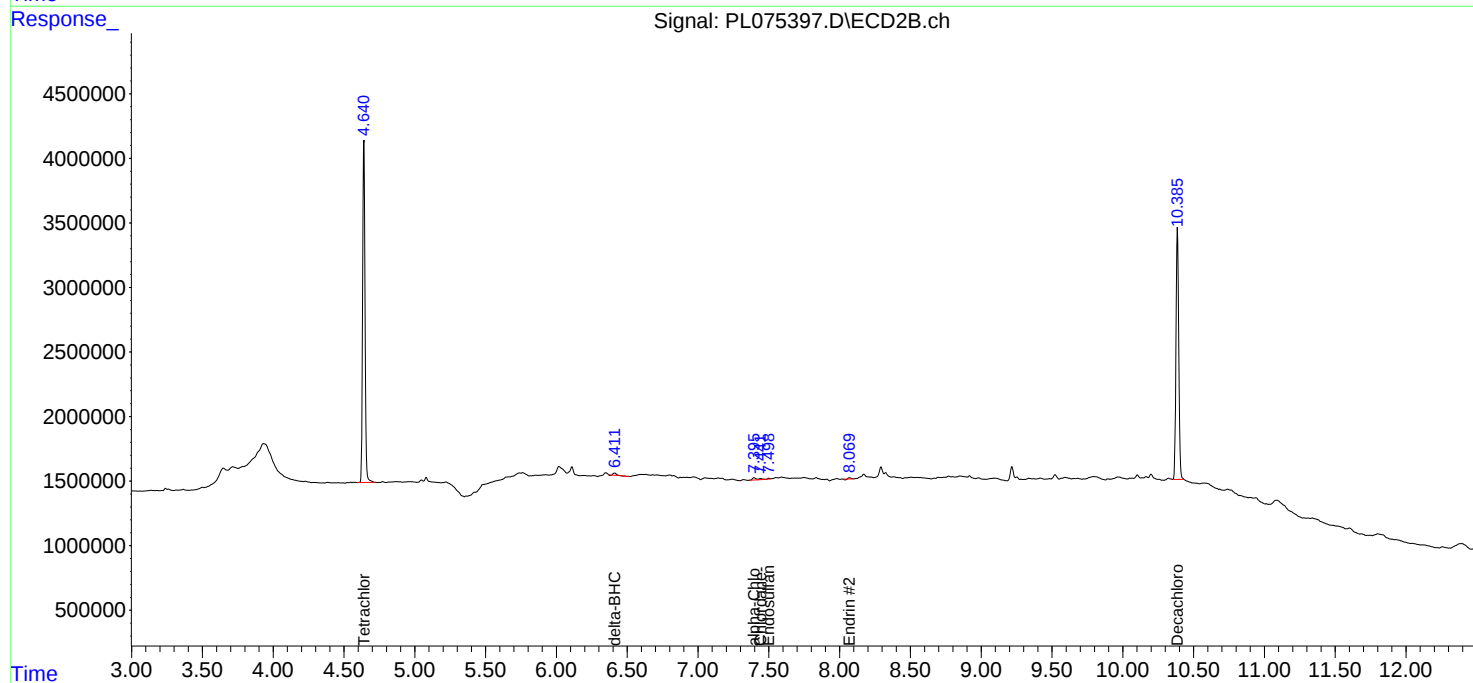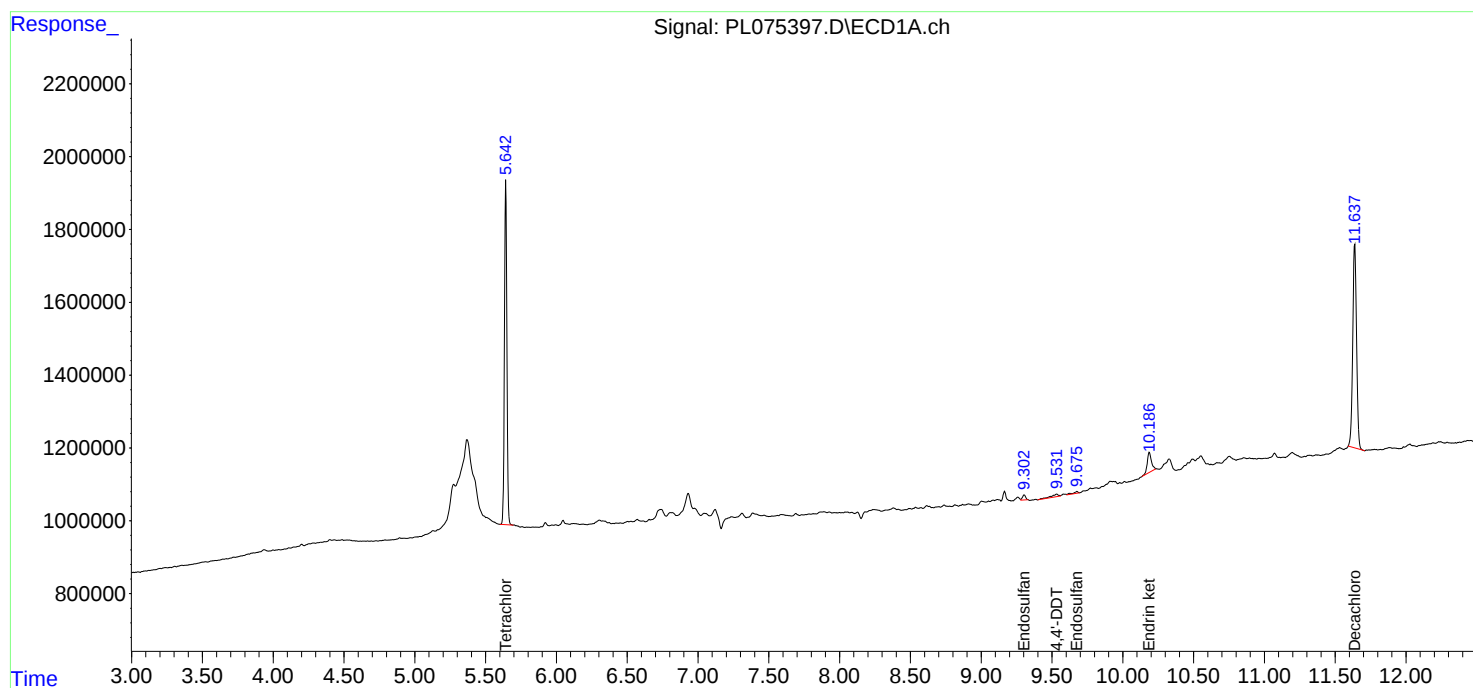

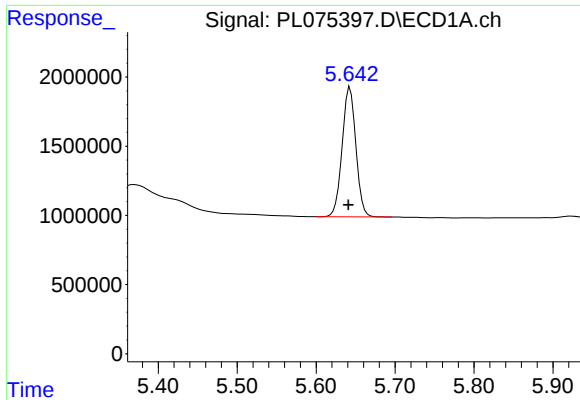


#1 Tetrachloro-m-xylene

R.T.: 5.643 min
Delta R.T.: 0.002 min
Response: 11343678
Conc: 19.30 ng/ml

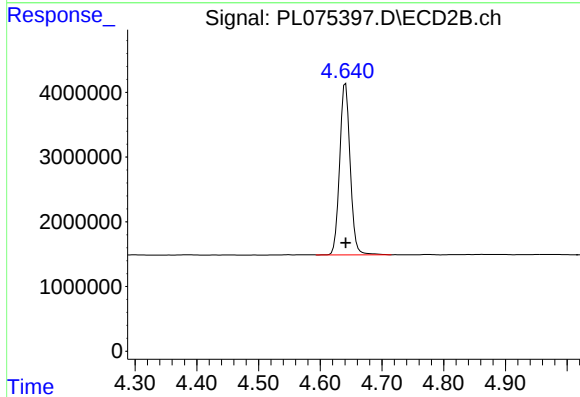


#1 Tetrachloro-m-xylene

R.T.: 4.641 min
Delta R.T.: 0.000 min
Response: 31325970
Conc: 19.77 ng/ml

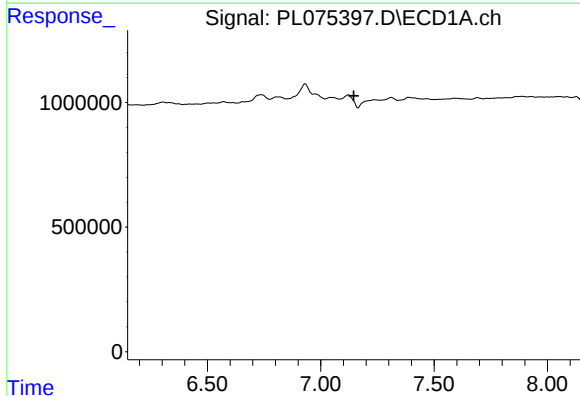


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 7.146 min
Response: 0
Conc: N.D.

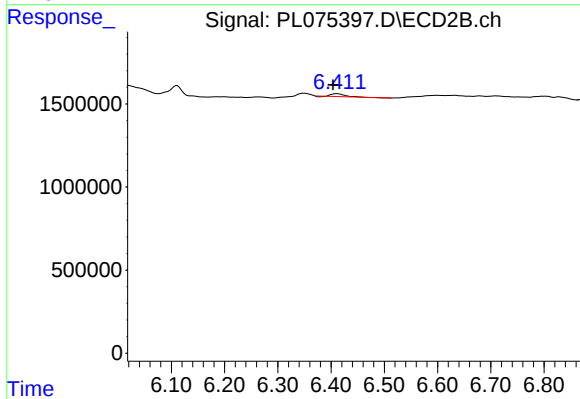


#7 delta-BHC

R.T.: 6.412 min
Delta R.T.: 0.009 min
Response: 294895
Conc: 0.14 ng/ml

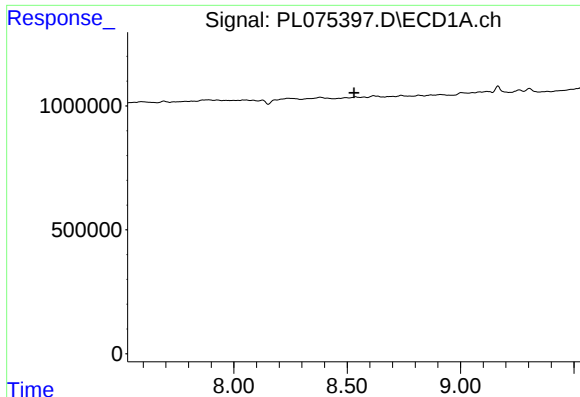


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 8.530 min
Response: 0
Conc: N.D.

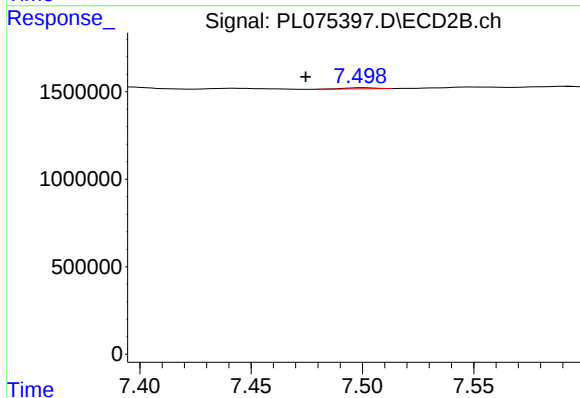


#9 Endosulfan I

R.T.: 7.501 min
Delta R.T.: 0.026 min
Response: 58127
Conc: 0.03 ng/ml

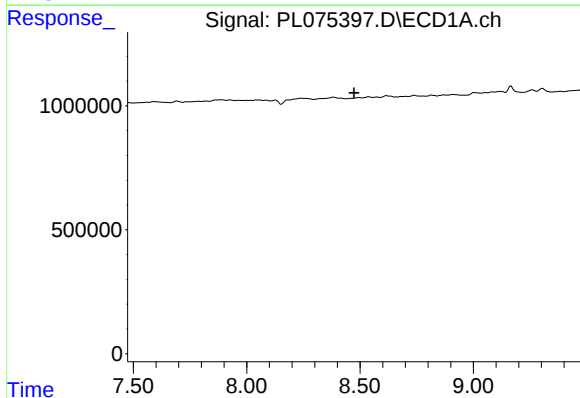


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 8.474 min
Response: 0
Conc: N.D.

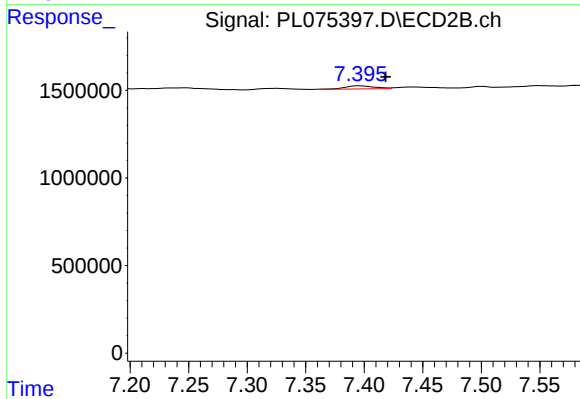


#11 alpha-Chlordane

R.T.: 7.396 min
Delta R.T.: -0.022 min
Response: 312713
Conc: 0.17 ng/ml

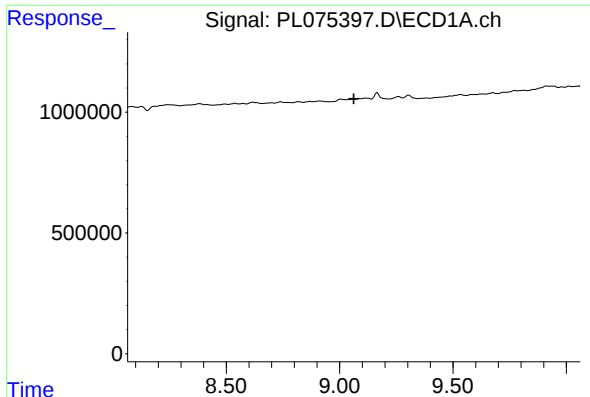


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 9.062 min
Response: 0
Conc: N.D.

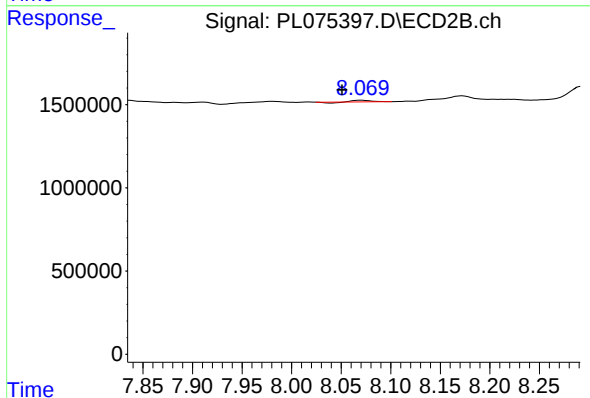


#14 Endrin

R.T.: 8.071 min
Delta R.T.: 0.020 min
Response: 85060
Conc: 0.05 ng/ml

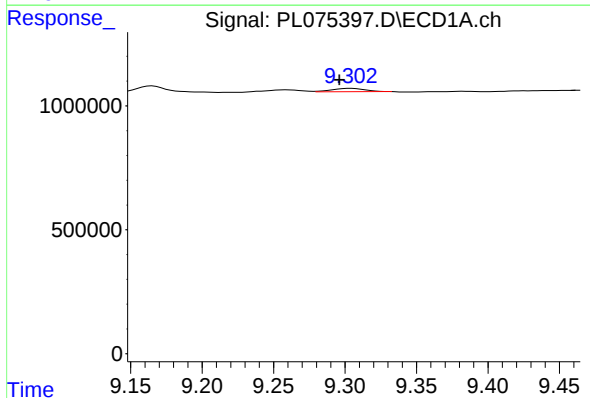


#15 Endosulfan II

R.T.: 9.304 min
Delta R.T.: 0.008 min
Response: 216439
Conc: 0.38 ng/ml

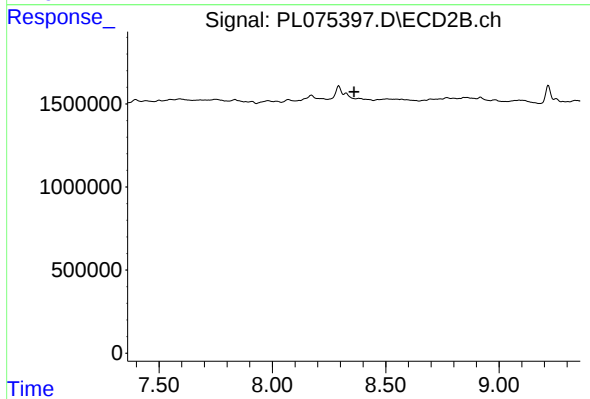


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 8.361 min
Response: 0
Conc: N.D.

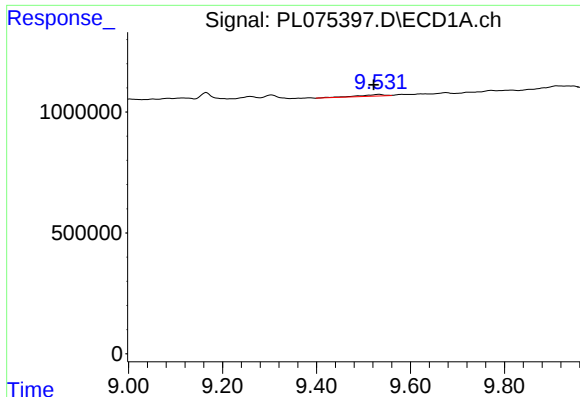


#17 4,4'-DDT

R.T.: 9.533 min
Delta R.T.: 0.011 min
Response: 269902
Conc: 0.46 ng/ml

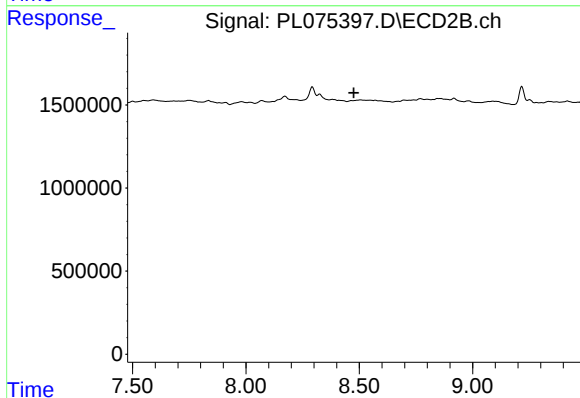


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 8.476 min
Response: 0
Conc: N.D.

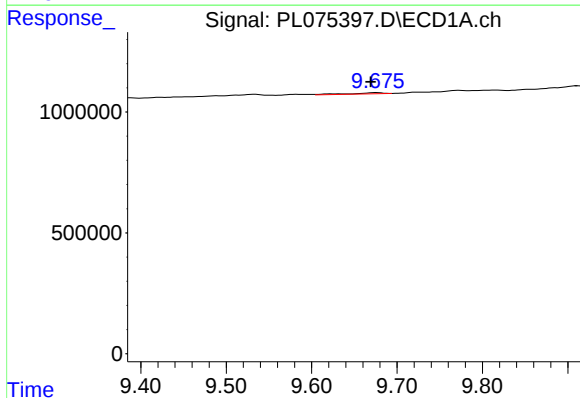


#19 Endosulfan Sulfate

R.T.: 9.676 min
Delta R.T.: 0.007 min
Response: 126464
Conc: 0.23 ng/ml

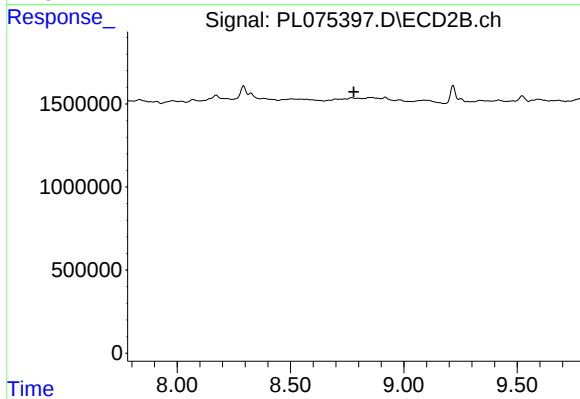


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 8.779 min
Response: 0
Conc: N.D.

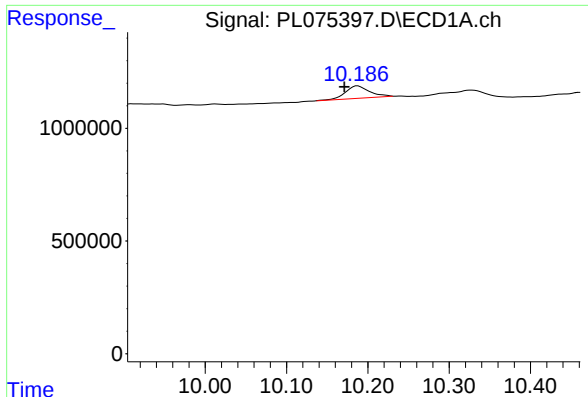


#21 Endrin ketone

R.T.: 10.187 min
Delta R.T.: 0.016 min
Response: 1148125
Conc: 1.87 ng/ml

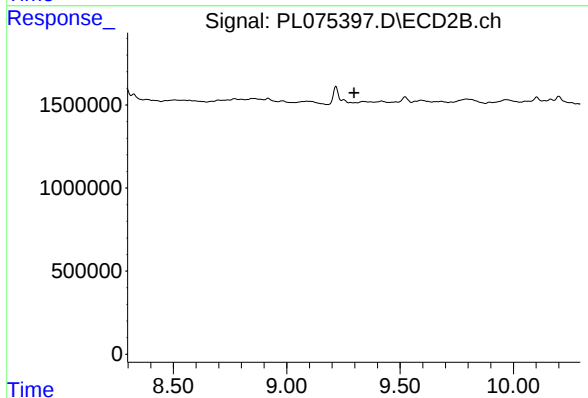


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.298 min
Response: 0
Conc: N.D.

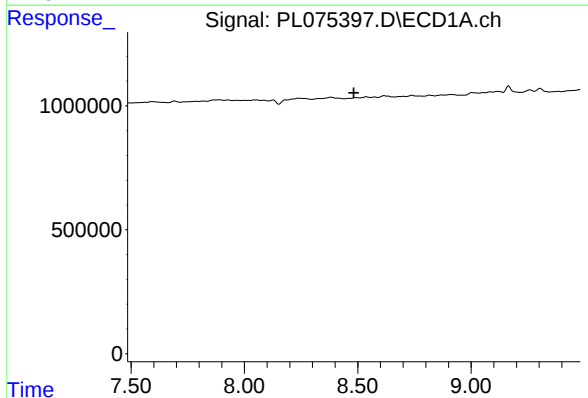


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 8.482 min
Response: 0
Conc: N.D.

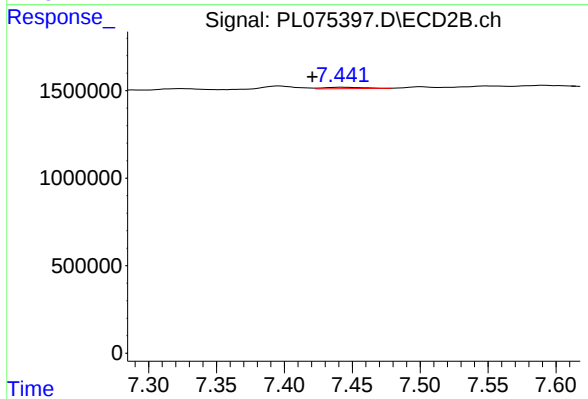


#26 Chlordane-4

R.T.: 7.442 min
Delta R.T.: 0.022 min
Response: 158732
Conc: 0.84 ng/ml

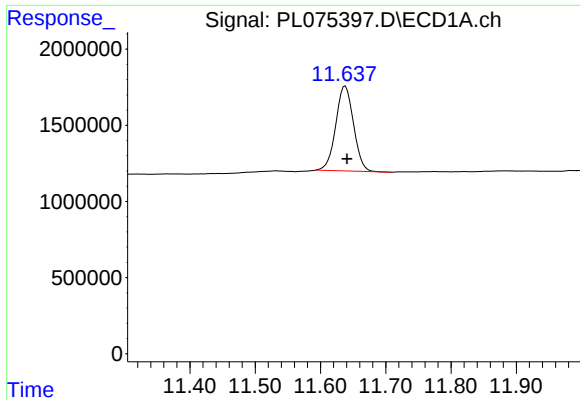

#28 Decachlorobiphenyl

R.T.: 11.638 min
Delta R.T.: -0.003 min
Response: 10571312
Conc: 19.72 ng/ml

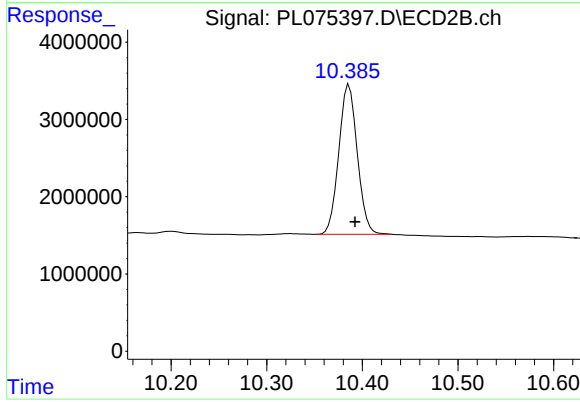

#28 Decachlorobiphenyl

R.T.: 10.386 min
Delta R.T.: -0.006 min
Response: 26113634
Conc: 19.03 ng/ml