

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060222\
 Data File : PL075410.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jun 2022 21:32
 Operator : AR\AJ
 Sample : N2951-06
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 03 06:10:07 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 01 10:19:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	5.643	4.642	10783461	29848980	18.347	18.842
28)	SA Decachlor...	11.640	10.388	7611533	18704051	14.196	13.630
Target Compounds							
7)	B delta-BHC	0.000	6.407	0	240073	N.D.	0.112 #
11)	B alpha-Chl...	0.000	7.393f	0	294311	N.D.	0.161 #
14)	MA Endrin	0.000	8.070f	0	380647	N.D.	0.245 #
15)	B Endosulfa...	9.305	0.000	234289	0	0.415	N.D. #
17)	MA 4,4'-DDT	0.000	8.466	0	268446	N.D.	0.188 #
26)	Chlordane-4	0.000	7.393f	0	294311	N.D.	1.558 #
27)	Chlordane-5	0.000	8.127	0	79706	N.D.	1.597 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060222\
Data File : PL075410.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jun 2022 21:32
Operator : AR\AJ
Sample : N2951-06
Misc :
ALS Vial : 41 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 03 06:10:07 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
Quant Title : GC Extractables
QLast Update : Wed Jun 01 10:19:11 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

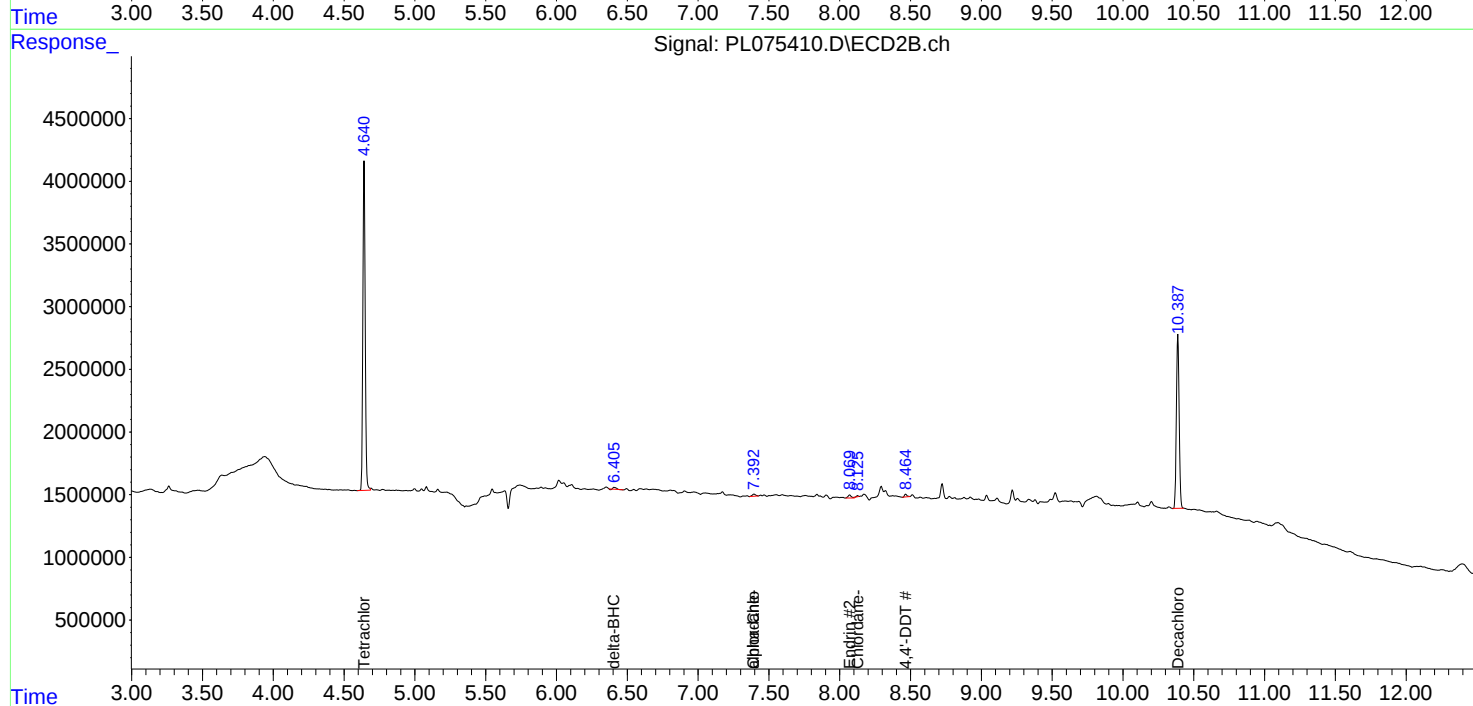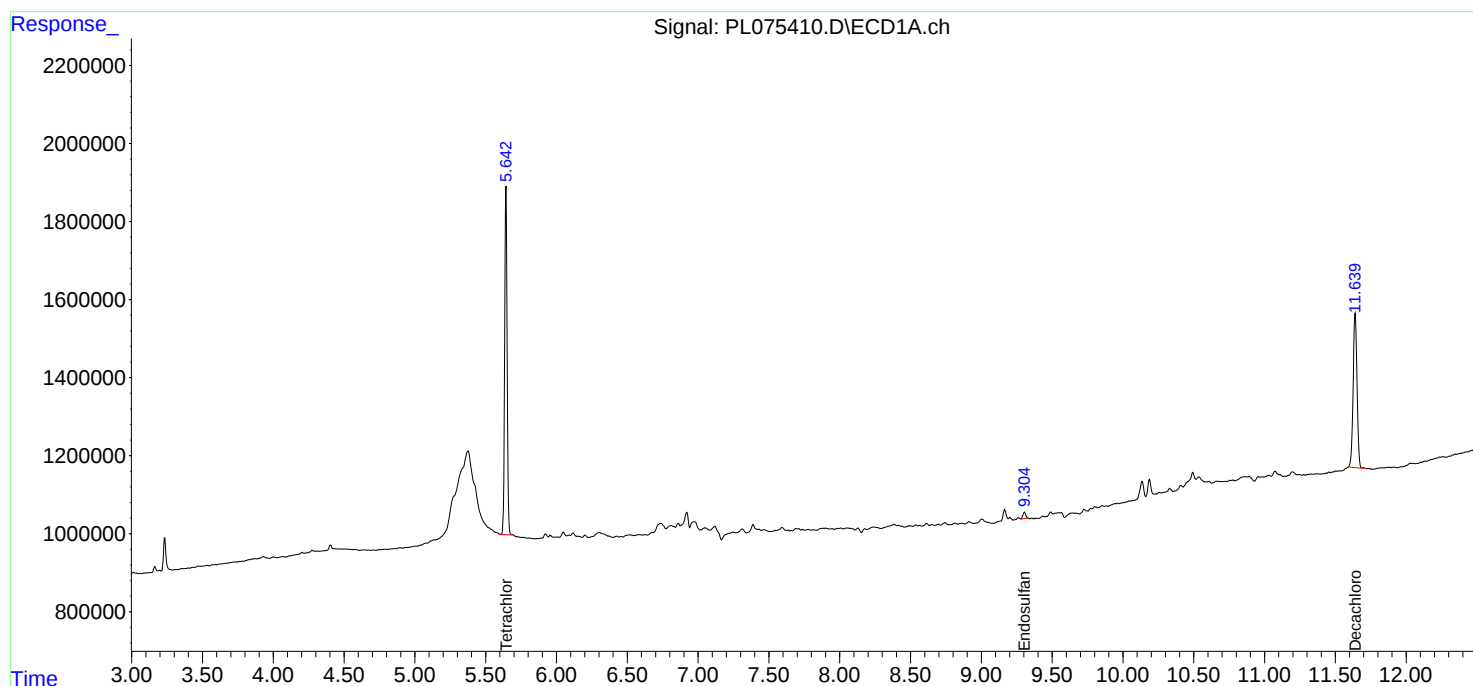

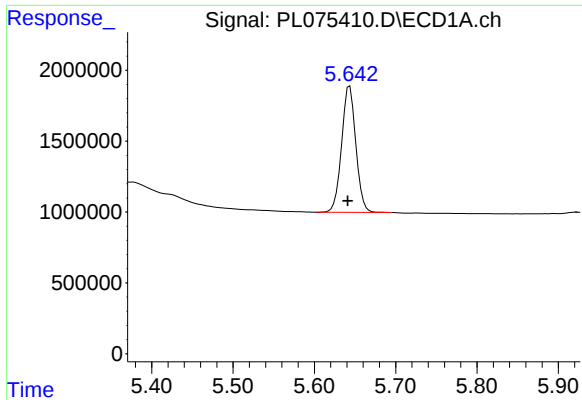


#1 Tetrachloro-m-xylene

R.T.: 5.643 min
Delta R.T.: 0.002 min
Response: 10783461
Conc: 18.35 ng/ml

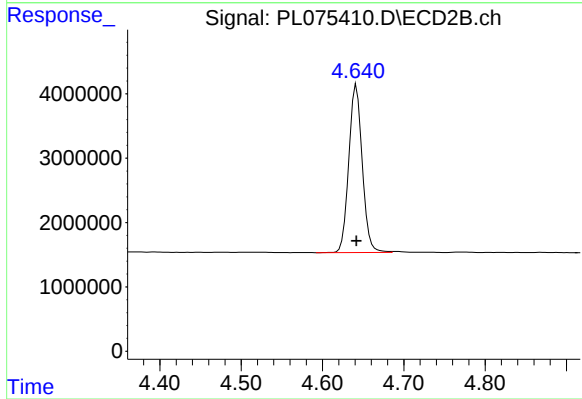


#1 Tetrachloro-m-xylene

R.T.: 4.642 min
Delta R.T.: 0.000 min
Response: 29848980
Conc: 18.84 ng/ml

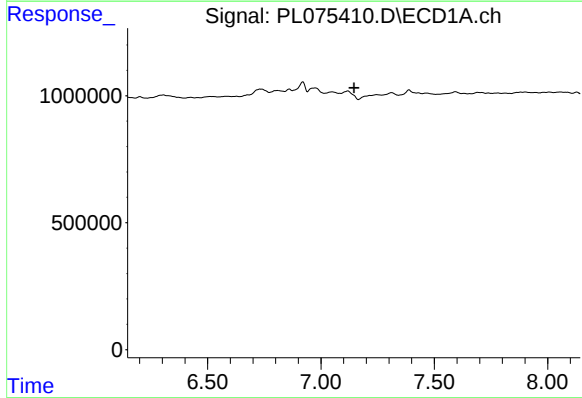


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 7.146 min
Response: 0
Conc: N.D.

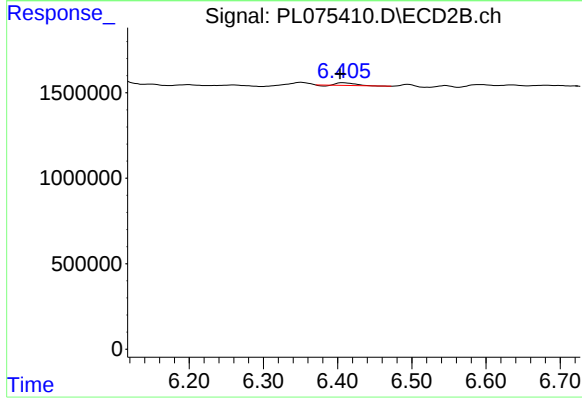


#7 delta-BHC

R.T.: 6.407 min
Delta R.T.: 0.004 min
Response: 240073
Conc: 0.11 ng/ml

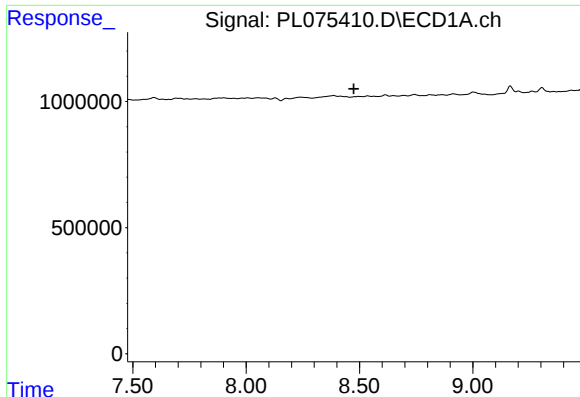


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 8.474 min
Response: 0
Conc: N.D.

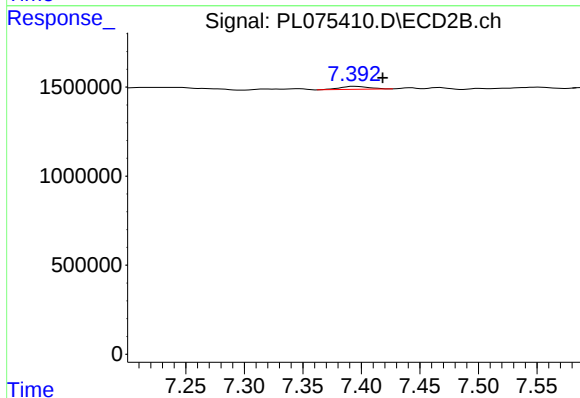


#11 alpha-Chlordane

R.T.: 7.393 min
Delta R.T.: -0.025 min
Response: 294311
Conc: 0.16 ng/ml

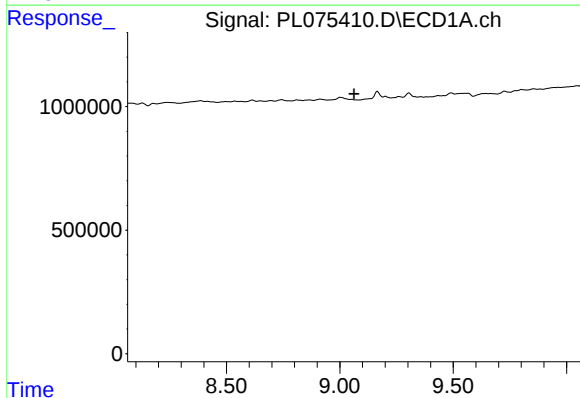


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 9.062 min
Response: 0
Conc: N.D.

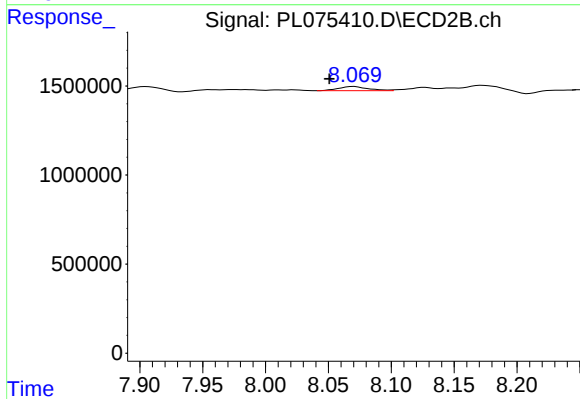


#14 Endrin

R.T.: 8.070 min
Delta R.T.: 0.019 min
Response: 380647
Conc: 0.24 ng/ml

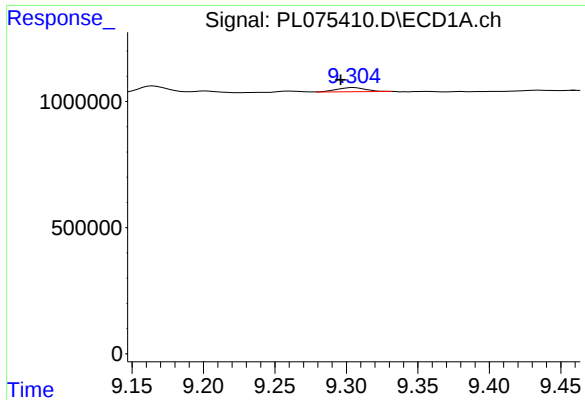


#15 Endosulfan II

R.T.: 9.305 min
Delta R.T.: 0.009 min
Response: 234289
Conc: 0.42 ng/ml

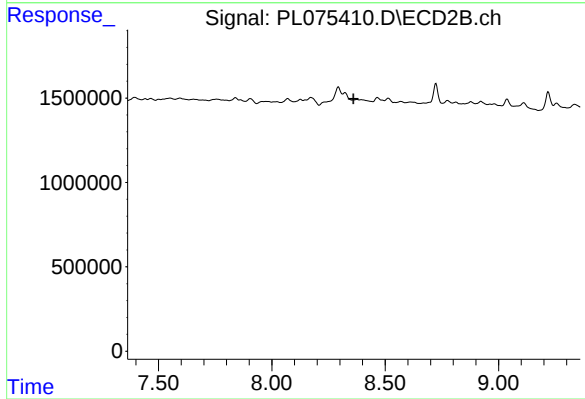


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.361 min
Response: 0
Conc: N.D.

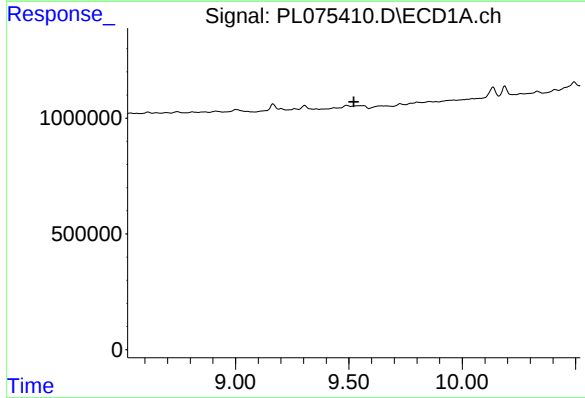


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 9.522 min
Response: 0
Conc: N.D.

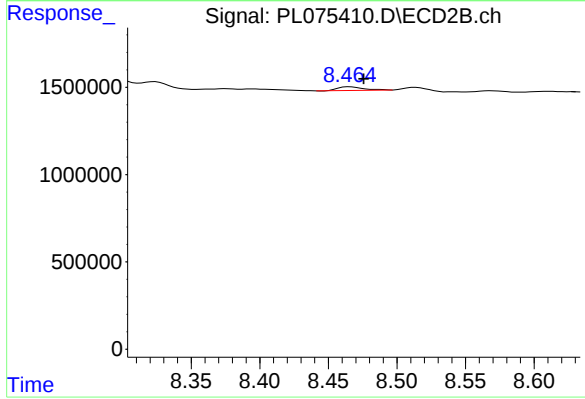


#17 4,4'-DDT

R.T.: 8.466 min
Delta R.T.: -0.010 min
Response: 268446
Conc: 0.19 ng/ml

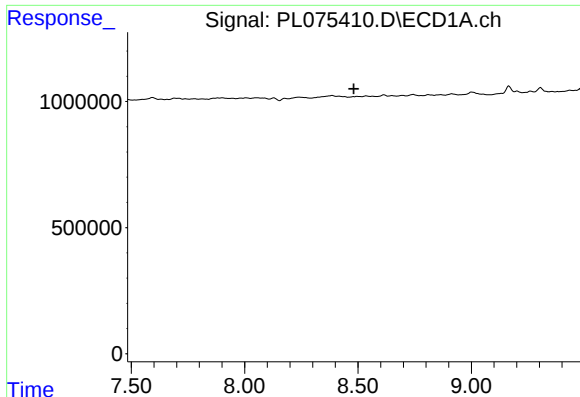


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 8.482 min
Response: 0
Conc: N.D.

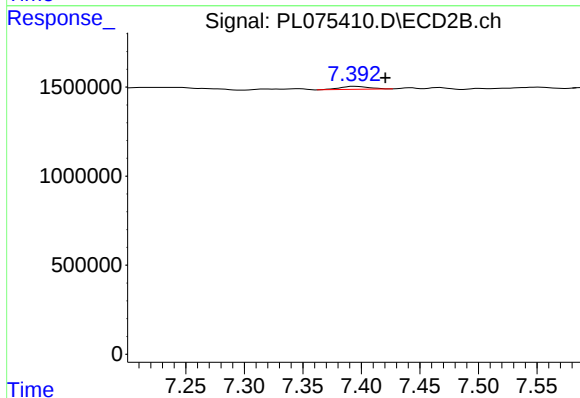


#26 Chlordane-4

R.T.: 7.393 min
Delta R.T.: -0.027 min
Response: 294311
Conc: 1.56 ng/ml

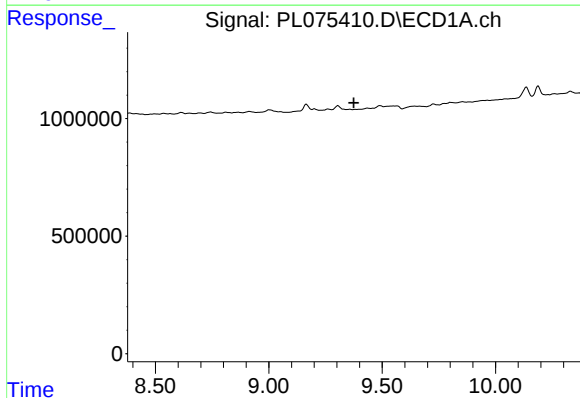


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 9.375 min
Response: 0
Conc: N.D.

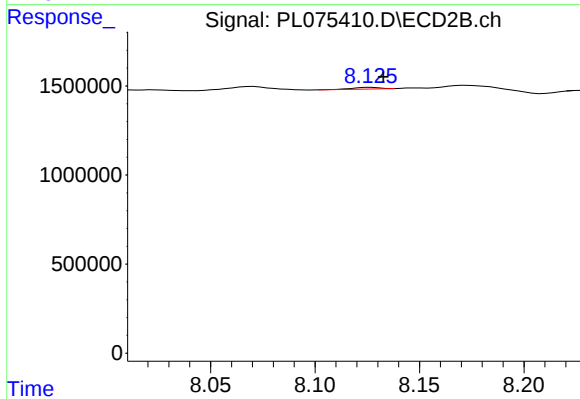


#27 Chlordane-5

R.T.: 8.127 min
Delta R.T.: -0.006 min
Response: 79706
Conc: 1.60 ng/ml

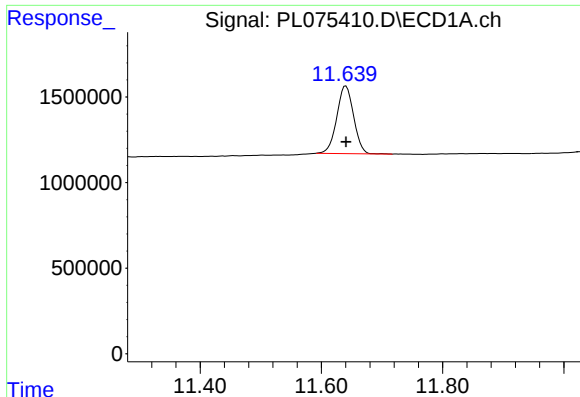

#28 Decachlorobiphenyl

R.T.: 11.640 min
Delta R.T.: 0.000 min
Response: 7611533
Conc: 14.20 ng/ml

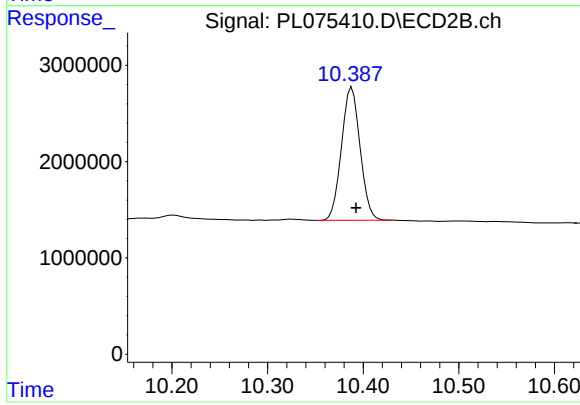

#28 Decachlorobiphenyl

R.T.: 10.388 min
Delta R.T.: -0.004 min
Response: 18704051
Conc: 13.63 ng/ml